

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM051921\
 Data File : BM030079.D
 Acq On : 19 May 2021 10:39
 Operator : CG/JU
 Sample : PB136510BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK510

Integration Parameters: LSCINT.P

Integrator: RTE

Smoother: OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0.1 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM050721.M
 Title : SVOA CALIBRATION

Signal : TIC: BM030079.D

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.034	22	25	35	rVB	46422	73005	1.18%	0.138%
2	3.446	94	95	131	rBV	352730	982884	15.93%	1.851%
3	6.704	643	649	666	rBV	727319	1306853	21.18%	2.462%
4	6.863	671	676	698	rVV	572437	1015340	16.46%	1.913%
5	7.051	702	708	726	rVV	810744	1401861	22.72%	2.641%
6	7.516	781	787	803	rBV	456895	799074	12.95%	1.505%
7	8.234	903	909	935	rBV	876165	1652052	26.78%	3.112%
8	8.669	975	983	1004	rBV	708398	1358638	22.02%	2.559%
9	9.386	1099	1105	1119	rBV	626437	1137239	18.43%	2.142%
10	9.922	1189	1196	1217	rBV	816795	1625281	26.34%	3.062%
11	10.286	1251	1258	1269	rBV	737946	1247821	20.22%	2.351%
12	10.439	1277	1284	1312	rBV	737276	1721226	27.90%	3.242%
13	11.933	1529	1538	1542	rBV7	6818	16674	0.27%	0.031%
14	13.592	1813	1820	1839	rBV	1906000	2895714	46.93%	5.455%
15	13.857	1858	1865	1879	rBV	2255078	3310119	53.65%	6.235%
16	14.168	1911	1918	1938	rVB	1234711	1828327	29.63%	3.444%
17	14.404	1953	1958	1982	rBV	394692	1040383	16.86%	1.960%
18	15.168	2081	2088	2106	rBV	2938177	4210226	68.24%	7.931%
19	15.310	2106	2112	2126	rVV	867406	1388358	22.50%	2.615%
20	15.410	2126	2129	2141	rVB2	38800	75593	1.23%	0.142%
21	15.957	2216	2222	2228	rVB6	9433	16070	0.26%	0.030%
22	16.715	2346	2351	2358	rBV4	3973	8328	0.13%	0.016%
23	16.915	2379	2385	2395	rBV	1541272	2179676	35.33%	4.106%
24	17.015	2396	2402	2417	rVV	3179477	4555394	73.83%	8.581%
25	17.851	2539	2544	2545	rBV4	6295	6680	0.11%	0.013%
26	18.956	2727	2732	2739	rBV	28149	44789	0.73%	0.084%
27	19.133	2758	2762	2764	rBV5	4766	7410	0.12%	0.014%
28	19.203	2770	2774	2778	rBV	23901	30862	0.50%	0.058%
29	19.315	2787	2793	2808	rBV	3945954	5452733	88.37%	10.271%
30	21.109	3093	3098	3109	rBV	1793759	2525155	40.93%	4.757%
31	22.615	3351	3354	3361	rVB2	77545	118178	1.92%	0.223%
32	23.121	3433	3440	3455	rBV	3470265	6170040	100.00%	11.623%
33	23.250	3456	3462	3472	rVV2	1447414	2701478	43.78%	5.089%
34	23.756	3545	3548	3554	rVB	114785	183219	2.97%	0.345%

Sum of corrected areas: 53086680




Instrument :

BNA_M

ClientSampleId :

SBLK510

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

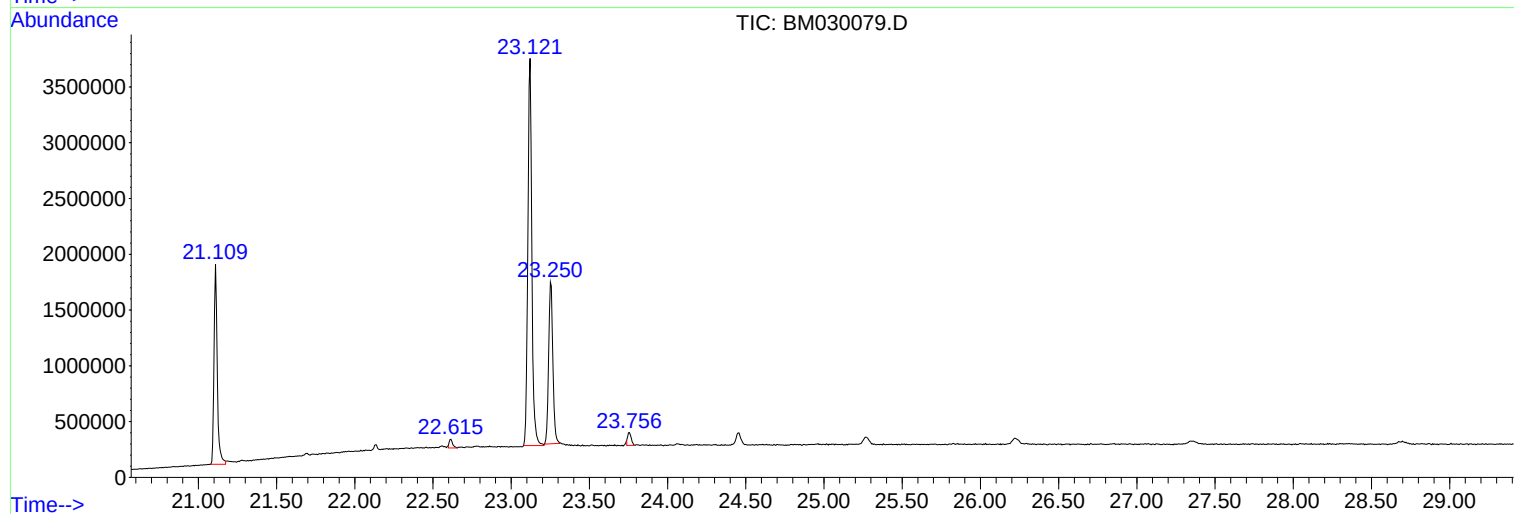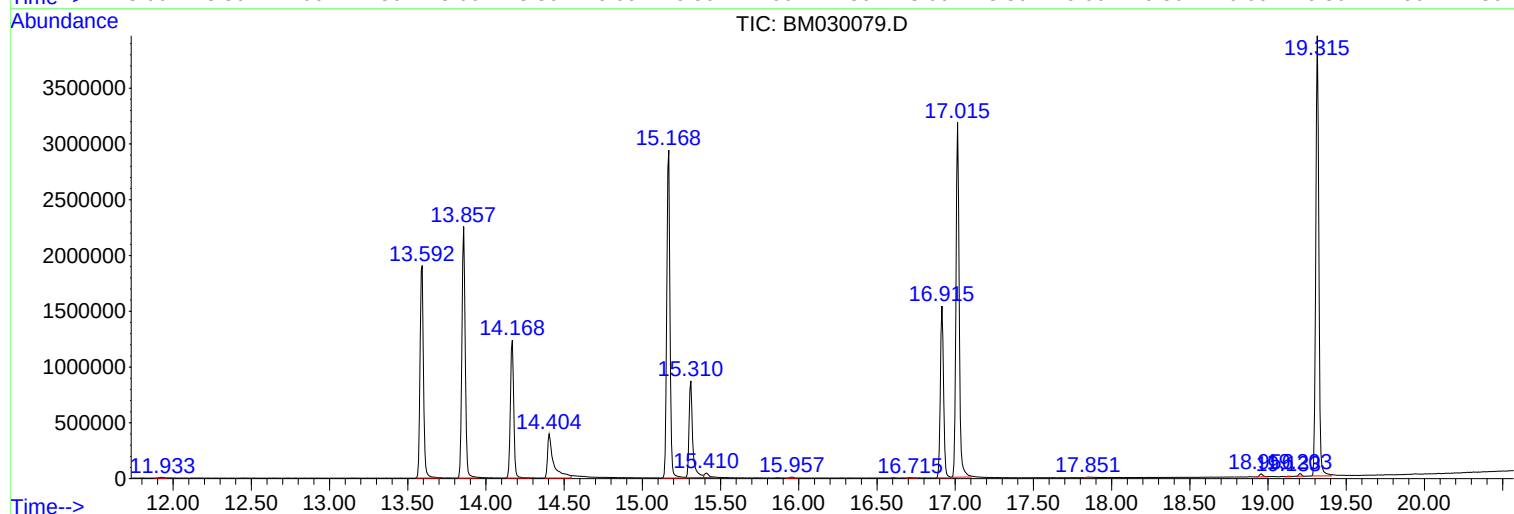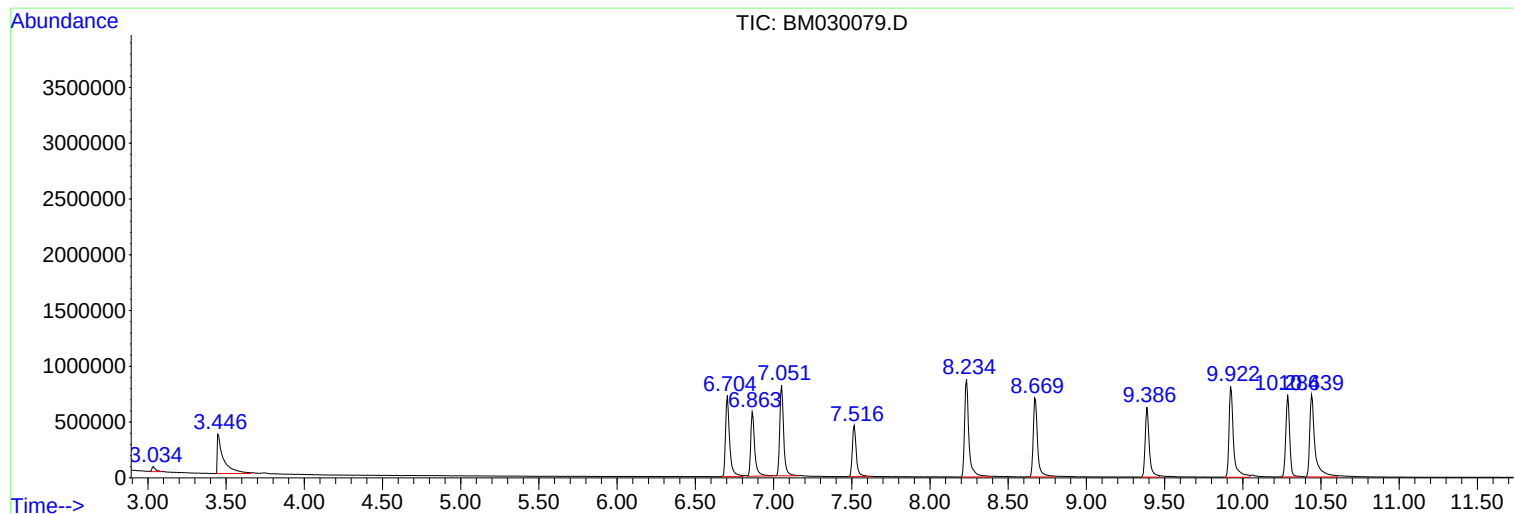

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM051921\
Data File : BM030079.D
Acq On : 19 May 2021 10:39
Operator : CG/JU
Sample : PB136510BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK510

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM050721.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM051921\
Data File : BM030079.D
Acq On : 19 May 2021 10:39
Operator : CG/JU
Sample : PB136510BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK510

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM050721.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
