
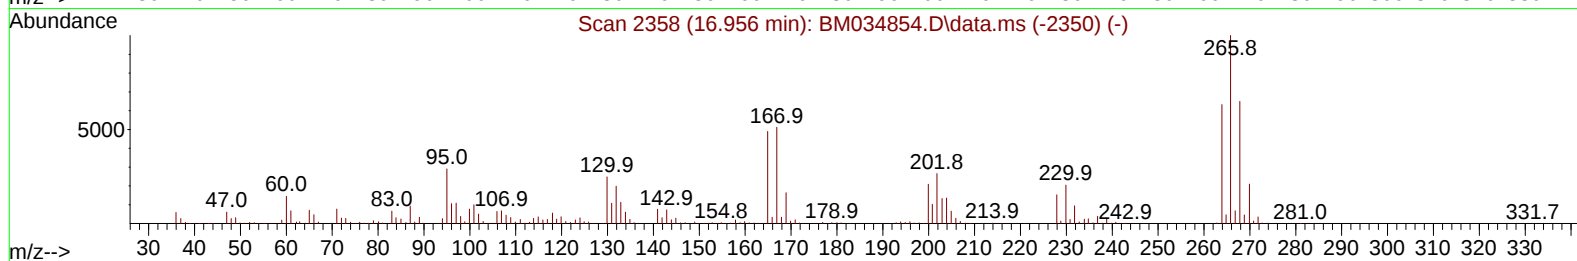
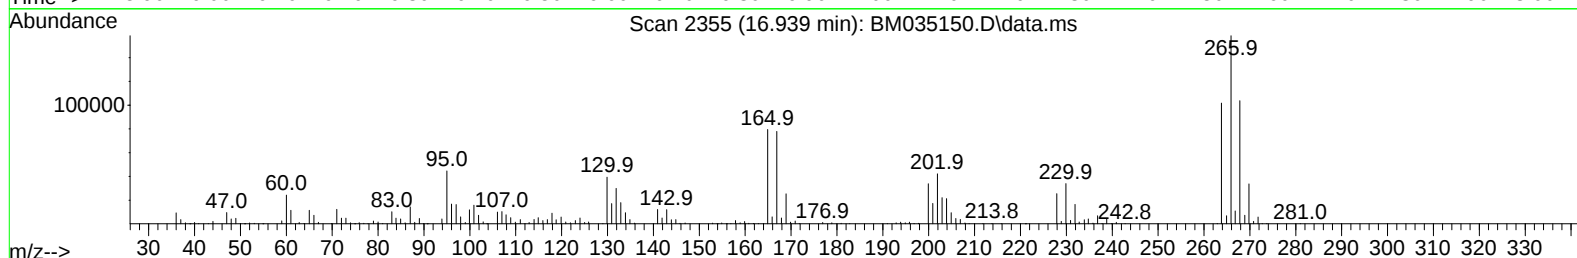


Data Path : Z:\svoasrv\HPCHEM1\BNA\_M\Data\BM051922\  
 Data File : BM035150.D  
 Acq On : 19 May 2022 13:12  
 Operator : CG/JU  
 Sample : DFTPP  
 Misc :  
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 20 07:34:51 2022  
 Quant Method : Z:\svoasrv\HPCHEM1\BNA\_M\Methods\8270-BM042722.M  
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 QLast Update : Fri May 20 04:53:59 2022  
 Response via : Initial Calibration

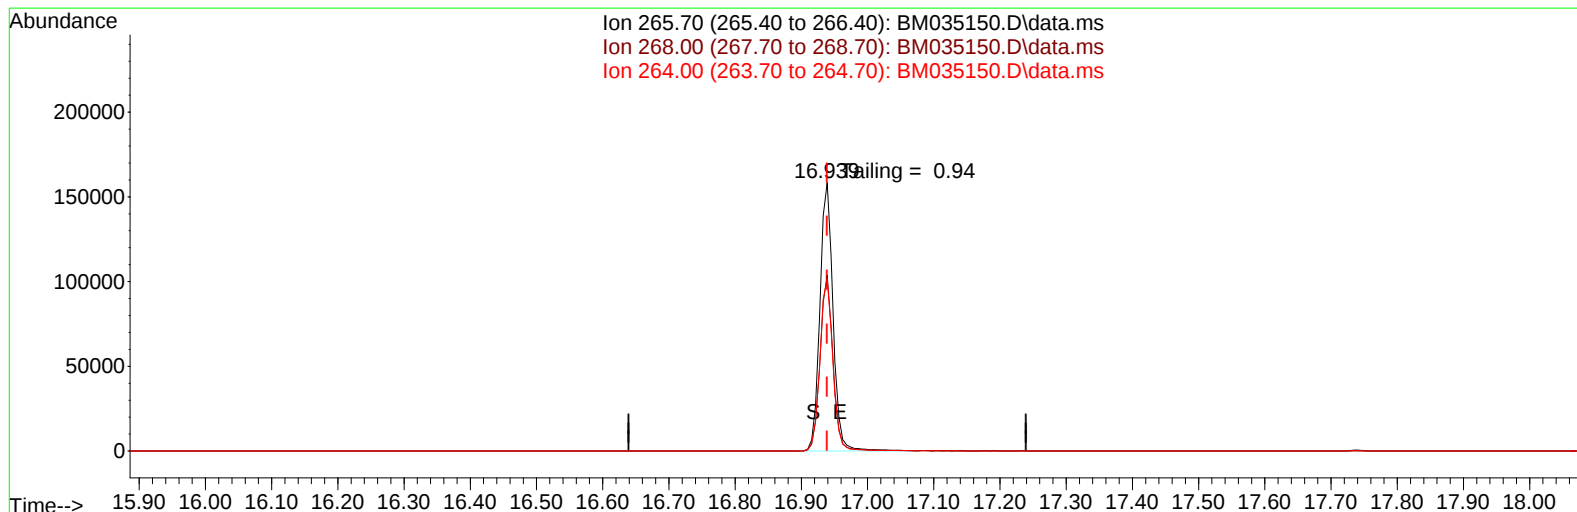

TIC: BM035150.D\data.ms

**(70) Pentachlorophenol (C)**




16.939min (+ 0.000) 173128.99 ng

response 219102

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 265.70 | 100.00 | 100.00 |
| 268.00 | 64.90  | 65.46  |
| 264.00 | 63.30  | 64.19  |
| 0.00   | 0.00   | 0.00   |

Data Path : Z:\svoasrv\HPCHEM1\BNA\_M\Data\BM051922\  
 Data File : BM035150.D  
 Acq On : 19 May 2022 13:12  
 Operator : CG/JU  
 Sample : DFTPP  
 Misc :  
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 20 07:34:51 2022  
 Quant Method : Z:\svoasrv\HPCHEM1\BNA\_M\Methods\8270-BM042722.M  
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 QLast Update : Fri May 20 04:53:59 2022  
 Response via : Initial Calibration

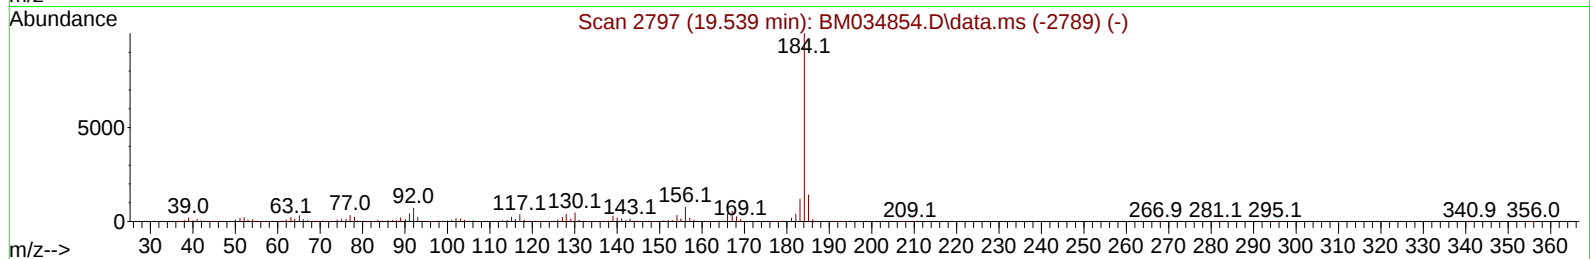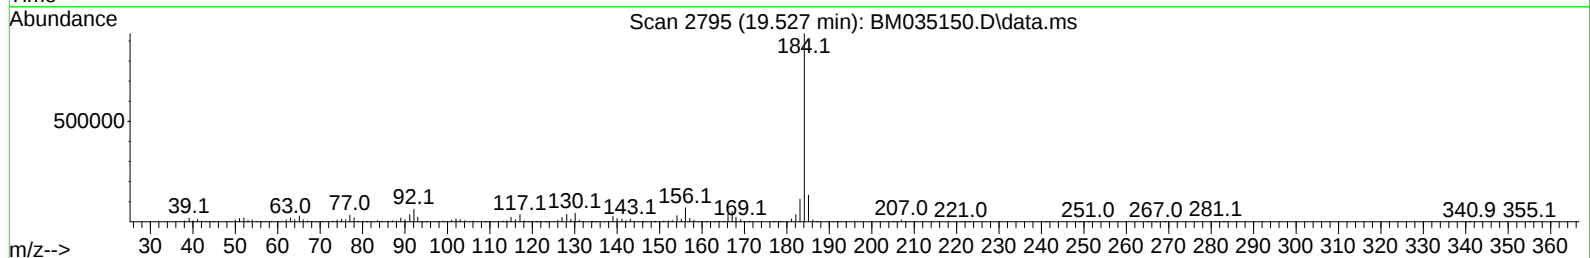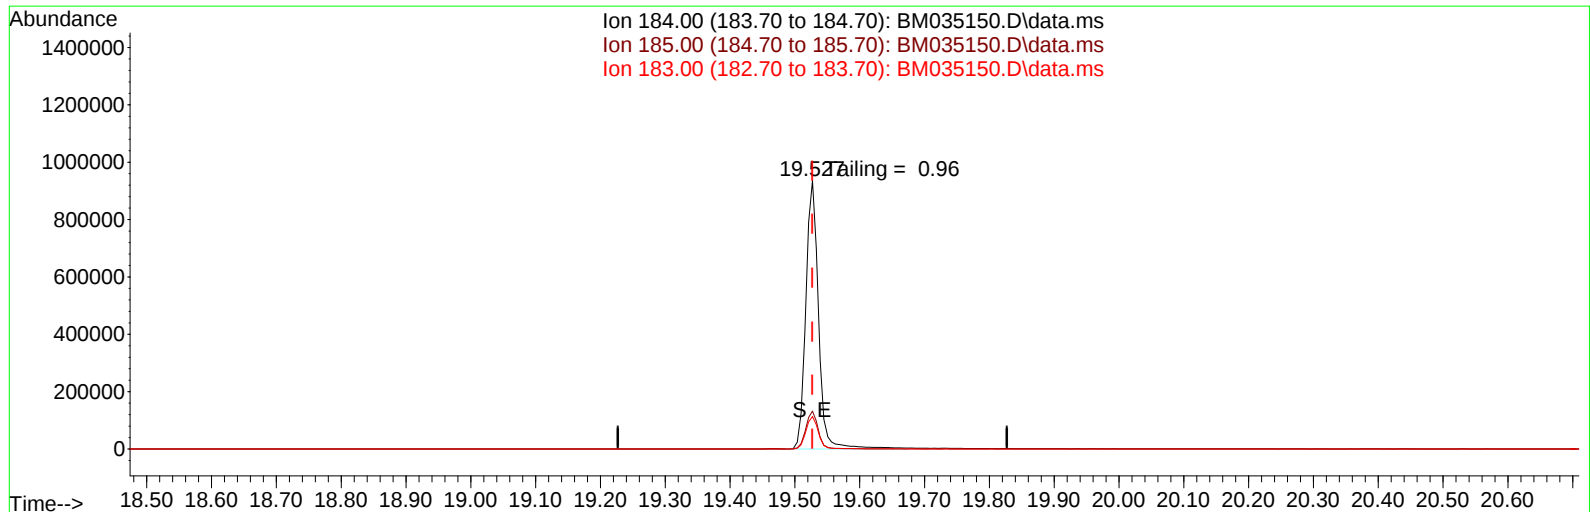

TIC: BM035150.D\data.ms

**(77) Benzidine****19.527min (+ 0.000) 72174.03 ng****response 1281029**

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 184.00 | 100.00 | 100.00 |
| 185.00 | 14.10  | 14.12  |
| 183.00 | 11.90  | 12.12  |
| 0.00   | 0.00   | 0.00   |