


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM051922\
 Data File : BM035150.D
 Acq On : 19 May 2022 13:12
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM042722.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri May 20 04:53:59 2022

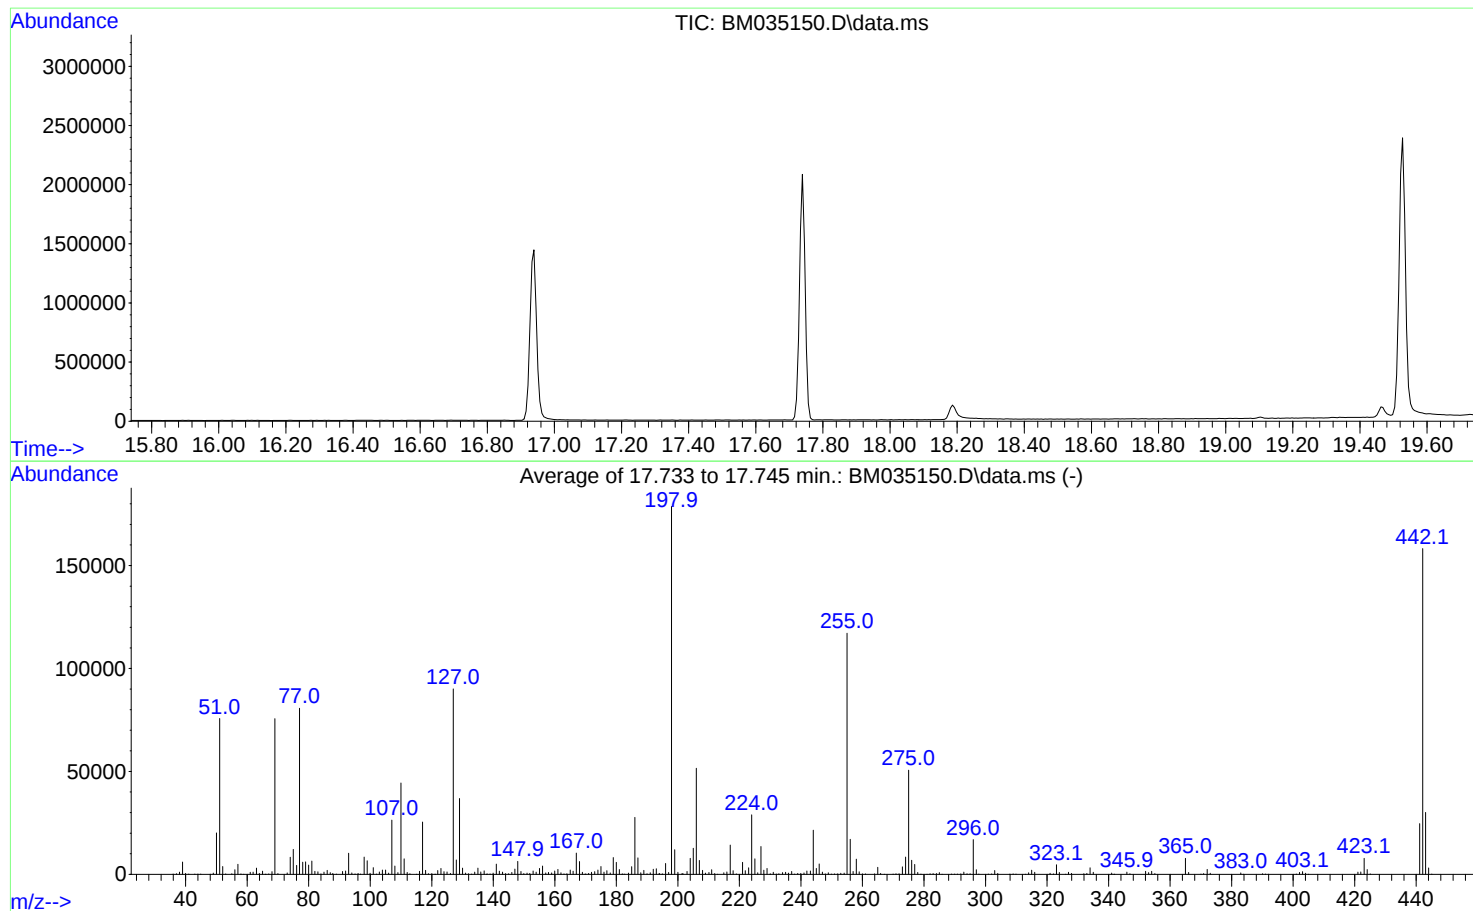




AutoFind: Scans 2490, 2491, 2492; Background Corrected with Scan 2484

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	42.4	75704	PASS
68	69	0.00	2	1.8	1344	PASS
69	198	0.00	100	42.3	75611	PASS
70	69	0.00	2	0.5	401	PASS
127	198	10	80	50.4	90059	PASS
197	198	0.00	2	0.5	962	PASS
198	198	100	100	100.0	178667	PASS
199	198	5	9	6.7	11946	PASS
275	198	10	60	28.3	50563	PASS
365	198	1	100	4.4	7782	PASS
441	198	0.01	100	13.8	24605	PASS
442	442	50	100	100.0	158227	PASS
443	442	15	24	19.0	30088	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM051922\
 Data File : BM035150.D
 Acq On : 19 May 2022 13:12
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Quant Time: May 20 07:34:51 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM042722.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri May 20 04:53:59 2022
 Response via : Initial Calibration

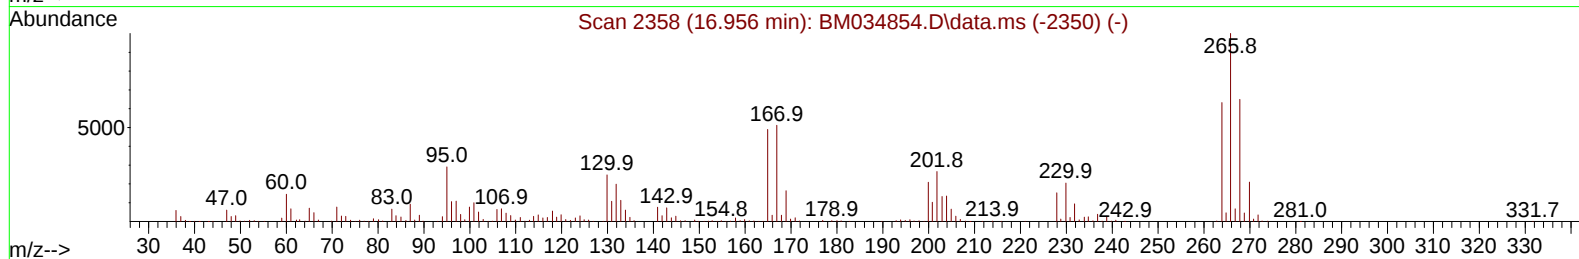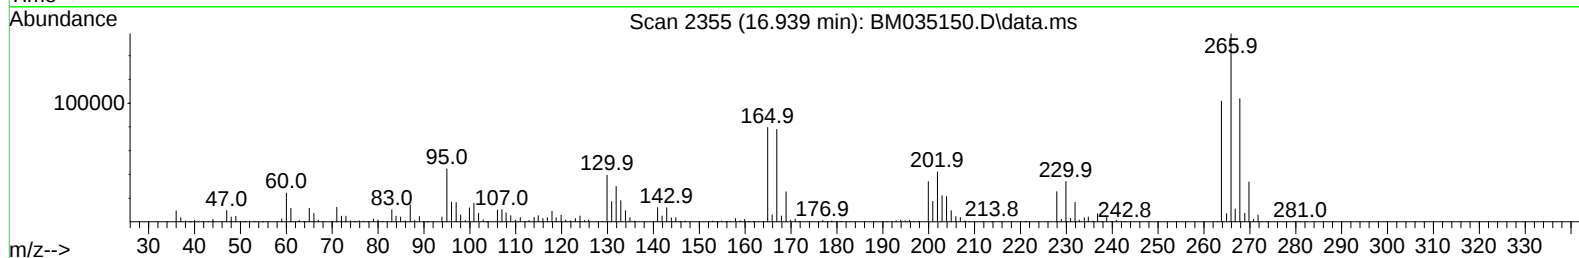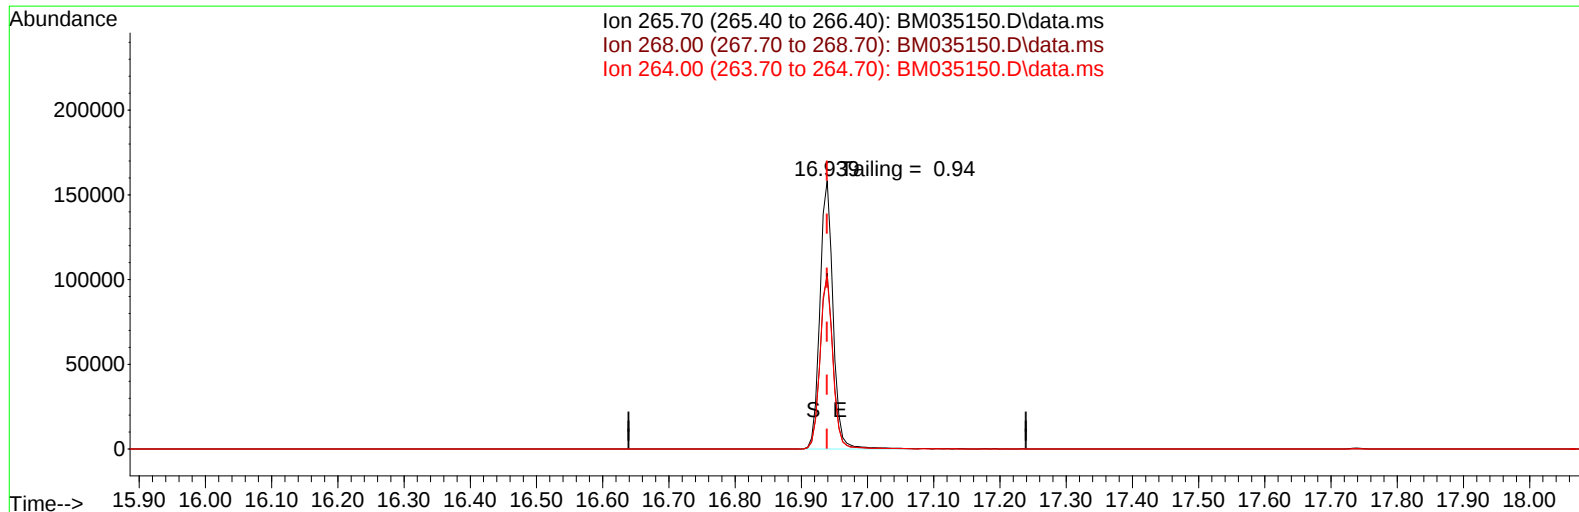

TIC: BM035150.D\data.ms

(70) Pentachlorophenol (C)

16.939min (+ 0.000) 173128.99 ng




response 219102

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.90	65.46
264.00	63.30	64.19
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM051922\
 Data File : BM035150.D
 Acq On : 19 May 2022 13:12
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Quant Time: May 20 07:34:51 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM042722.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri May 20 04:53:59 2022
 Response via : Initial Calibration

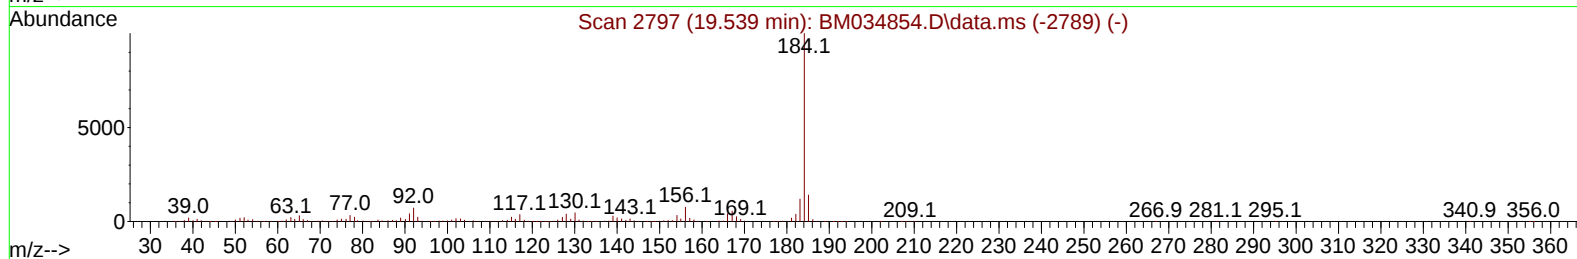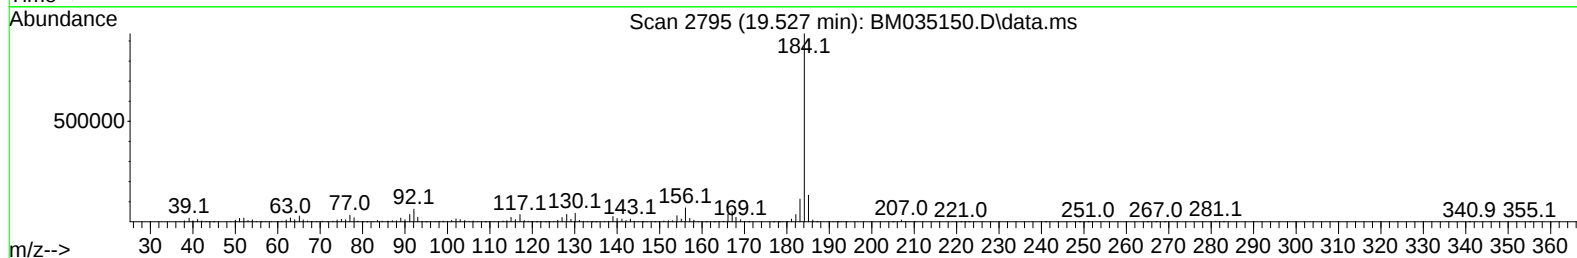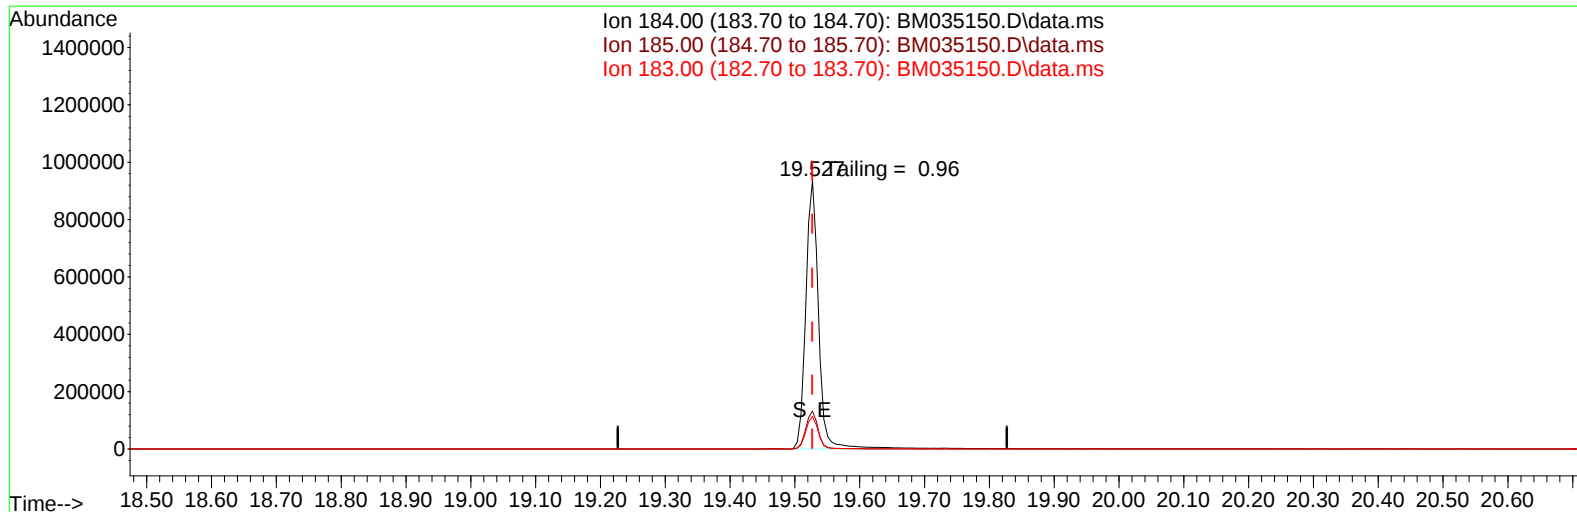

TIC: BM035150.D\data.ms

(77) Benzidine

19.527min (+ 0.000) 72174.03 ng

response 1281029

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.10	14.12
183.00	11.90	12.12
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
5/19/2022	BNA_M	<u>BM035150.D</u>
Compound Name	Response	Retention Time
DDT	661067	20.768
DDD	5208	20.38
DDE	273	19.821
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
5481	666548	0.82

Instrument :
BNA_M
ClientSampleId :
DFTPP