


Data Path : Z:\HPCHEM1\BNA_M\DATA\BM052015\
 Data File : BM001345.D
 Acq On : 21 May 2015 05:02
 Operator : TP/IZ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF043015.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed May 20 05:08:22 2015

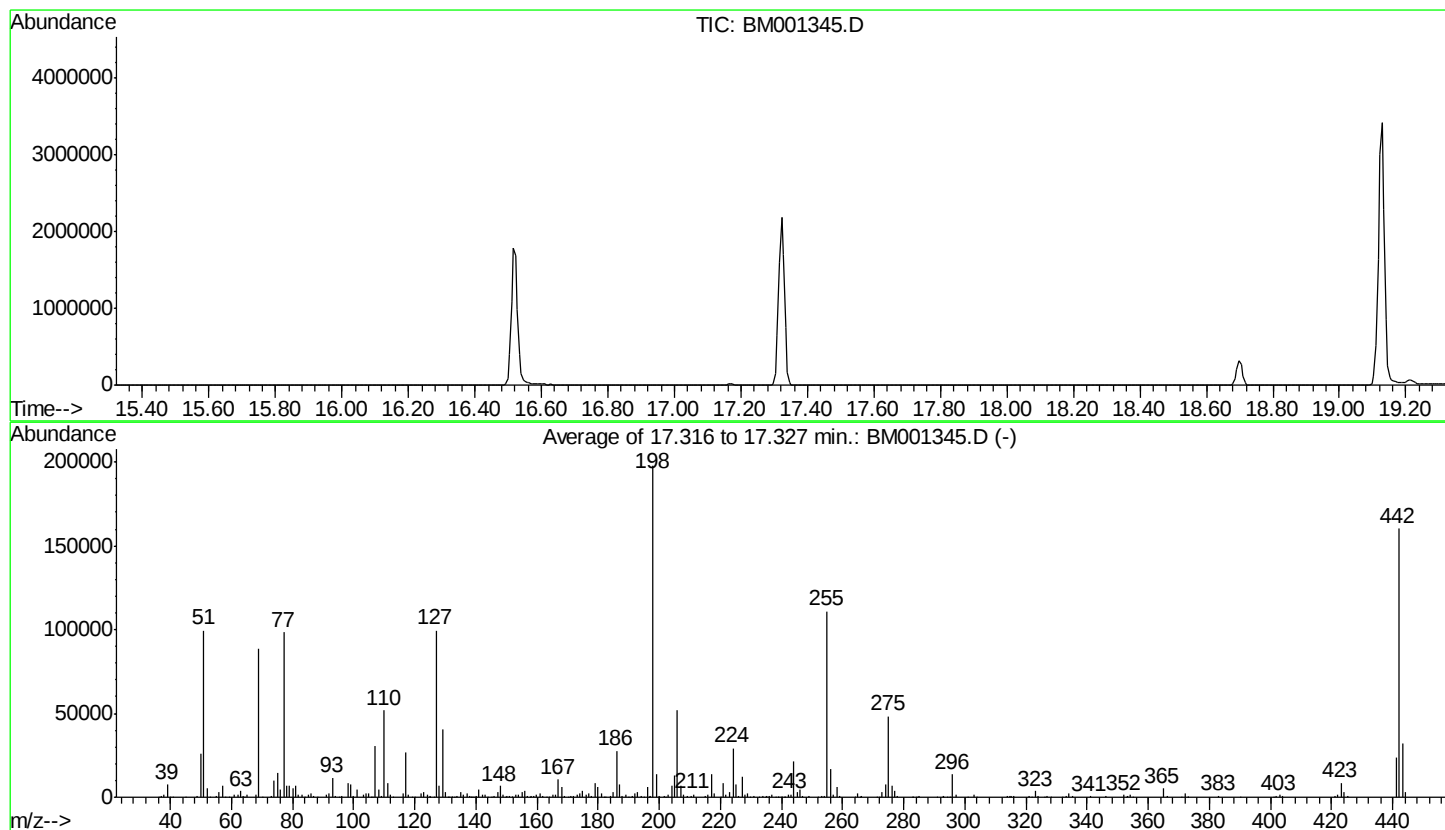

AutoFind: Scans 2487, 2488, 2489; Background Corrected with Scan 2480

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	50.4	99637	PASS
68	69	0.00	2	1.5	1353	PASS
69	198	0.00	100	44.7	88354	PASS
70	69	0.00	2	0.4	395	PASS
127	198	10	80	50.3	99514	PASS
197	198	0.00	2	0.4	713	PASS
198	198	100	100	100.0	197824	PASS
199	198	5	9	7.1	14071	PASS
275	198	10	60	24.4	48354	PASS
365	198	1	100	2.6	5210	PASS
441	442	0.01	24	14.8	23738	PASS
442	198	50	100	81.0	160181	PASS
443	442	15	24	19.9	31797	PASS