

Data Path : Z:\HPCHEM1\BNA M\DATA\BM052015\
 Data File : BM001353.D
 Acq On : 21 May 2015 09:47
 Operator : TP/IZ
 Sample : SSTDICC010
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SSTDICC010

Manual Integrations
 APPROVED

apatel
 5/21/2015 8:53:24 PM

Quant Time: May 21 11:06:12 2015
 Quant Method : Z:\HPCHEM1\BNA M\METHODS\SIMPAH-BM052015.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu May 21 08:43:35 2015
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.43	152	12220	5.00	ng	0.00
6) Naphthalene-d8	10.20	136	51026	5.00	ng	0.00
12) Acenaphthene-d10	14.11	164	31939	5.00	ng	0.00
18) Phenanthrene-d10	16.85	188	65118	5.00	ng	0.00
25) Chrysene-d12	21.07	240	70981	5.00	ng	0.00
32) Perylene-d12	23.17	264	67208	5.00	ng	0.00
System Monitoring Compounds						
4) 2-Fluorophenol	5.02	112	23083	9.75	ng	0.00
5) Phenol-d6	6.61	99	31823	10.46	ng	0.00
7) Nitrobenzene-d5	8.59	82	31960	10.79	ng	0.00
13) 2,4,6-Tribromophenol	15.59	330	13282	13.47	ng	0.00
14) 2-Fluorobiphenyl	12.72	172	90807	9.73	ng	0.00
27) Terphenyl-d14	19.50	244	91751	10.13	ng	0.00
Target Compounds						Qvalue
2) 1,4-Dioxane	2.89	88	8854	7.98	ng	# 82
3) n-Nitrosodimethylamine	3.21	42	14487	9.82	ng	# 89
8) Nitrobenzene	8.63	77	34406	11.07	ng	97
9) Naphthalene	10.25	128	104933	9.90	ng	99
10) Hexachlorobutadiene	10.54	225	19647	9.71	ng	99
11) 2-Methylnaphthalene	11.89	142	76307	10.15	ng	96
15) Acenaphthylene	13.82	152	144693	10.52	ng	100
16) Acenaphthene	14.17	154	82470	10.03	ng	98
17) Fluorene	15.15	166	61079	7.58	ng	# 96
19) 4-Bromophenyl-phenylether	16.04	248	34645	14.64	ng	99
20) Hexachlorobenzene	16.17	284	47655	11.13	ng	# 98
21) Pentachlorophenol	16.51	266	27616	17.99	ng	96
22) Phenanthrene	16.89	178	235664m	10.49	ng	
23) Anthracene	16.99	178	82390m	10.22	ng	
24) Fluoranthene	18.92	202	205735	12.29	ng	100
26) Pyrene	19.29	202	217447	10.41	ng	100
28) Benzo(a)anthracene	21.04	228	200681	10.39	ng	100
29) Chrysene	21.10	228	184672	9.93	ng	99
30) Bis(2-ethylhexyl)phthalate	20.99	149	128957	11.82	ng	99
31) Indeno(1,2,3-cd)pyrene	25.25	276	214225	10.29	ng	99
33) Benzo(b)fluoranthene	22.54	252	200918	10.26	ng	98
34) Benzo(k)fluoranthene	22.58	252	187527	10.02	ng	97
35) Benzo(a)pyrene	23.07	252	181849	10.43	ng	97
36) Dibenzo(a,h)anthracene	25.26	278	167145	10.23	ng	98
37) Benzo(g,h,i)perylene	25.88	276	173121	10.00	ng	96

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\HPCHEM1\BNA M\DATA\BM052015\
Data File : BM001353.D
Acq On : 21 May 2015 09:47
Operator : TP/IZ
Sample : SSTDIC010
Misc :
ALS Vial : 9 Sample Multiplier: 1


Instrument :
BNA_M
ClientSampleId :
SSTDIC010

Manual Integrations
APPROVED

apatel
5/21/2015 8:53:24 PM

Quant Time: May 21 11:06:12 2015
Quant Method : Z:\HPCHEM1\BNA M\METHODS\SIMPAH-BM052015.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu May 21 08:43:35 2015
Response via : Initial Calibration

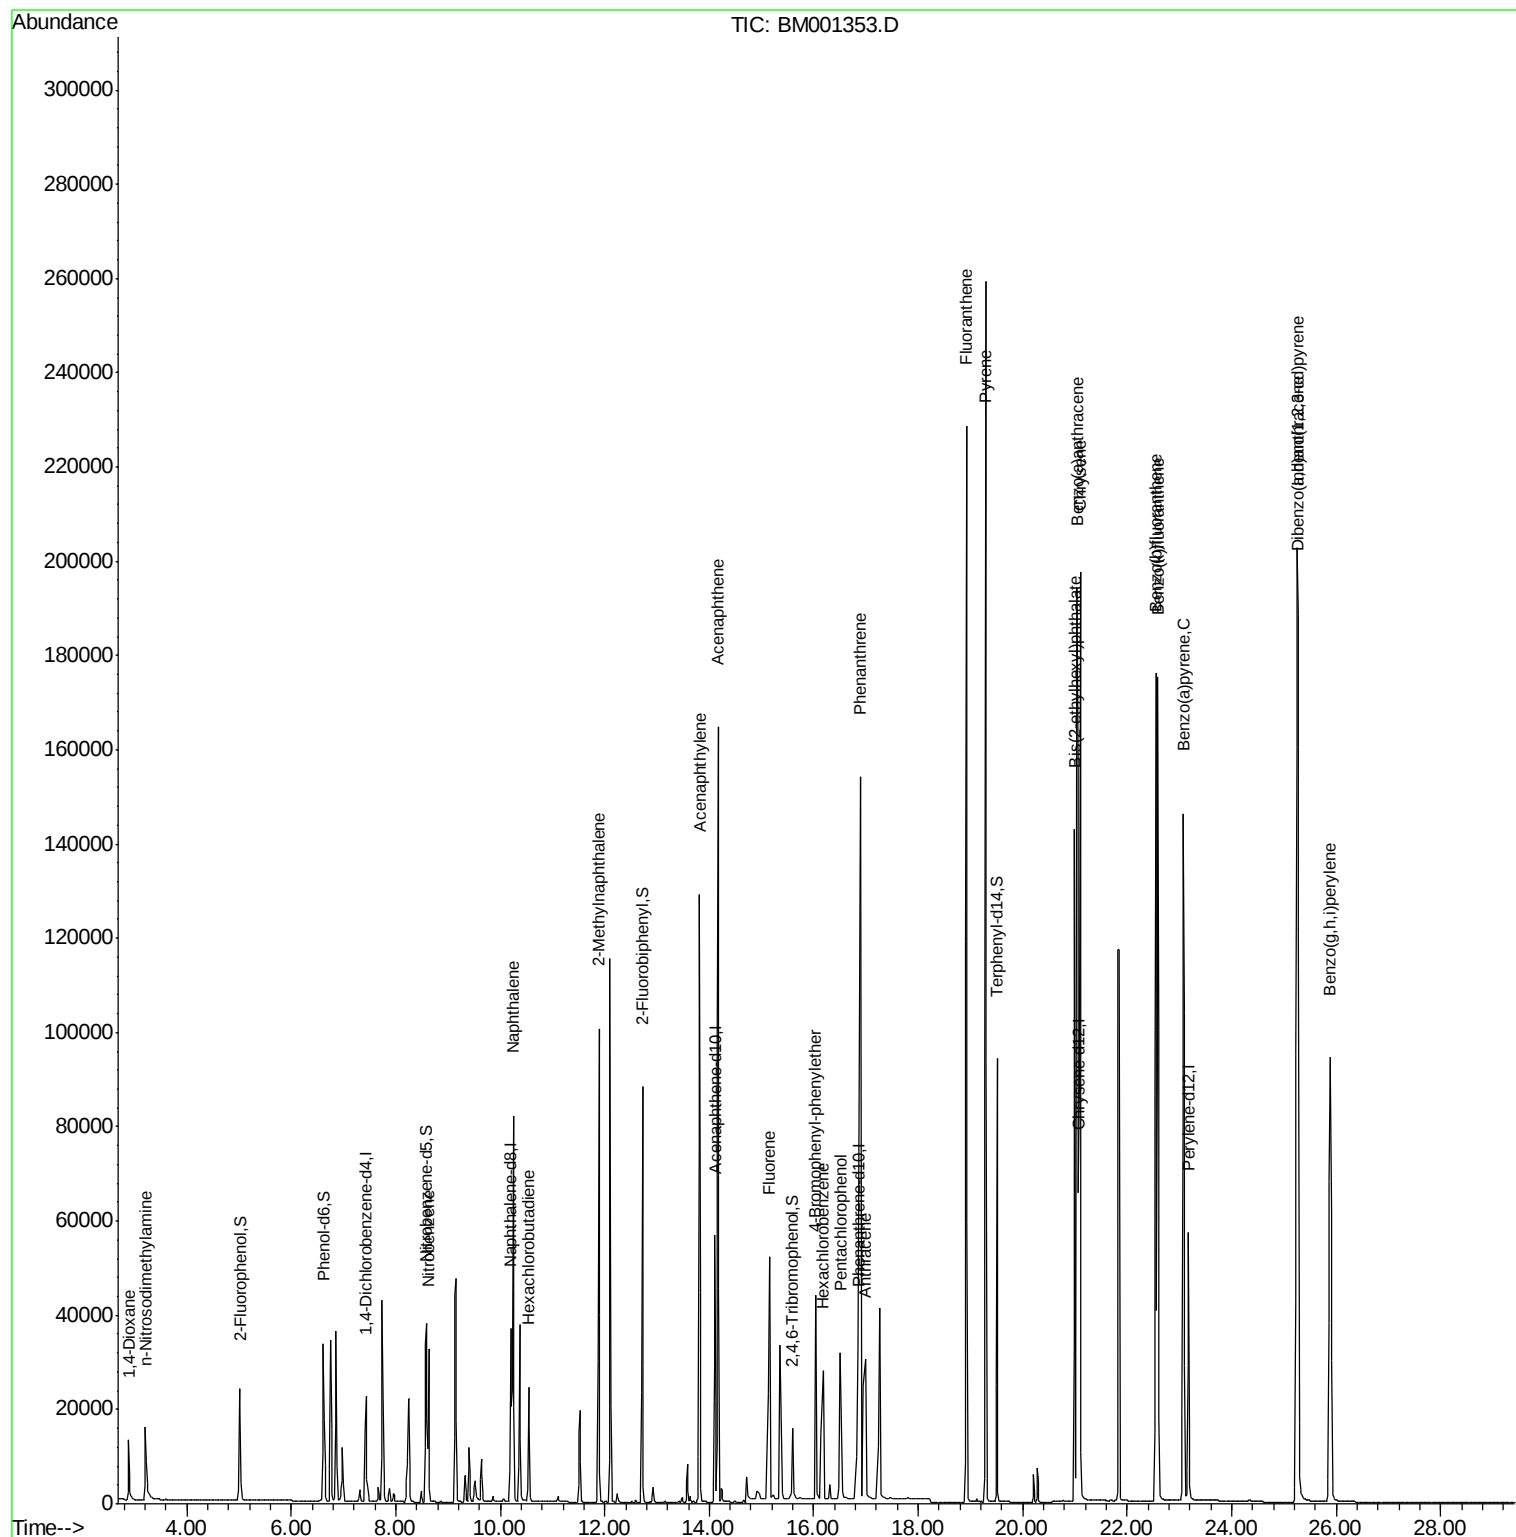

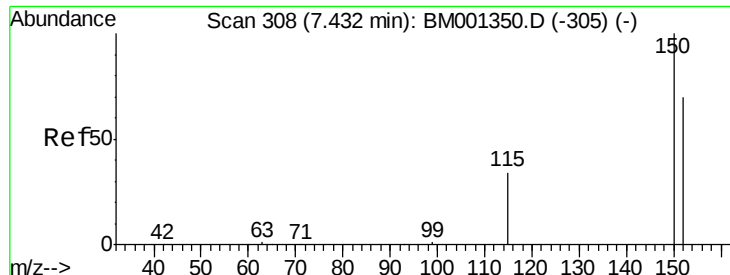

#1

1,4-Dichlorobenzene-d4

Concen: 5.00 ng

RT: 7.43 min Scan# 308

Delta R.T. 0.00 min

Lab File: BM001353.D

Acq: 21 May 2015 09:47

Instrument :

BNA_M


ClientSampleId :

SSTDIC010




Tot Ion:	152	Resp:	12220
Ion Ratio	Lower	Upper	
152	100		
150	142.8	114.1	171.1
115	48.2	39.2	58.8

Manual Integrations
APPROVED

apatel
5/21/2015 8:53:24 PM

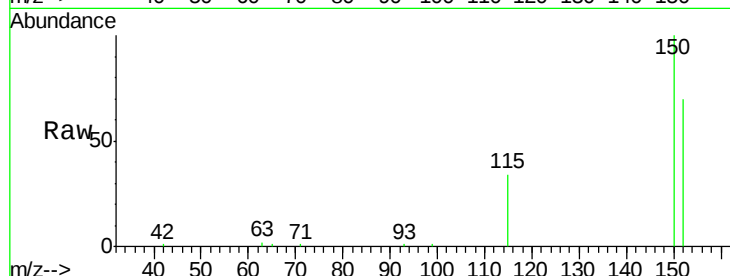

Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

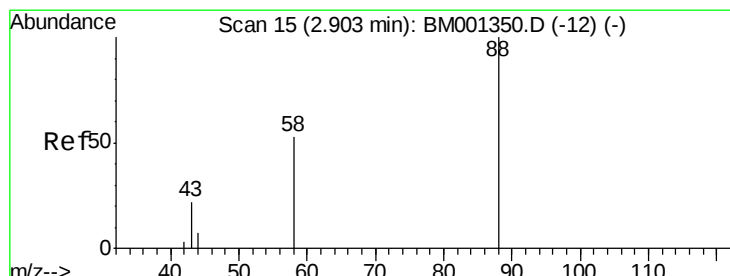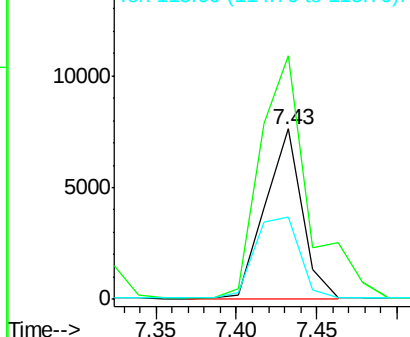

#2

1,4-Dioxane

Concen: 7.98 ng


RT: 2.89 min Scan# 14

Delta R.T. -0.02 min



Lab File: BM001353.D


Acq: 21 May 2015 09:47

Tgt Ion:	88	Resp:	8854
Ion Ratio	Lower	Upper	
88	100		
58	85.2	53.1	79.7#
43	38.3	27.8	41.8

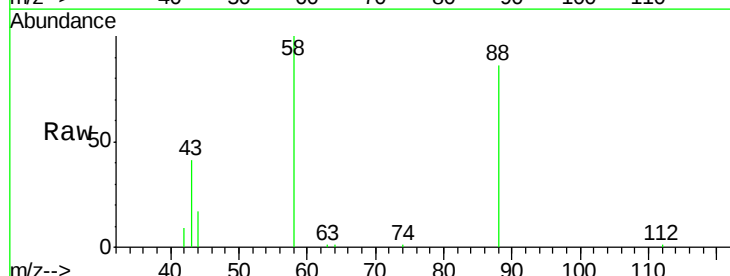

Abundance Ion 88.00 (87.70 to 88.70): BM0
Ion 58.00 (57.70 to 58.70): BM0
Ion 43.00 (42.70 to 43.70): BM0

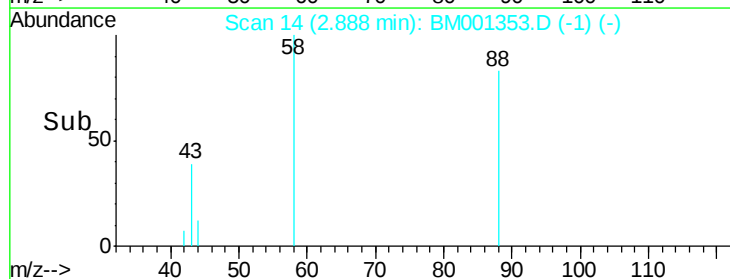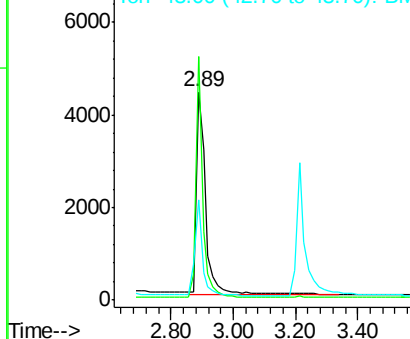



#3





n-Nitrosodimethylamine
 Concen: 9.82 ng
 RT: 3.21 min Scan# 35
 Delta R.T. -0.02 min
 Lab File: BM001353.D
 Acq: 21 May 2015 09:47

Instrument :
 BNA_M
 ClientSampleId :
 SSTDICC010

Tot Ion	Ratio	Lower	Upper
42	100		
74	97.7	70.0	105.0
44	6.1	3.6	5.4

Manual Integrations
 APPROVED




apatel
 5/21/2015 8:53:24 PM

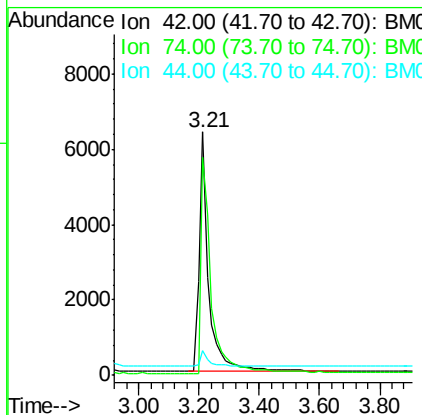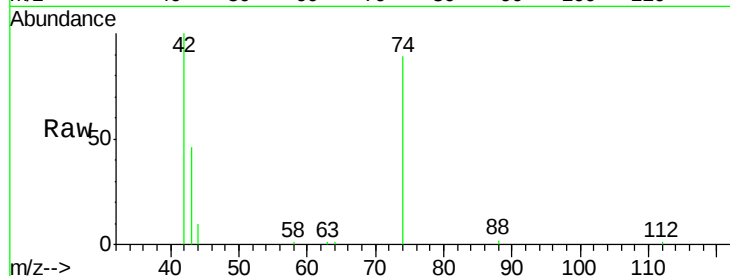


#4

2-Fluorophenol
 Concen: 9.75 ng
 RT: 5.02 min Scan# 152
 Delta R.T. 0.00 min
 Lab File: BM001353.D
 Acq: 21 May 2015 09:47

Tgt Ion	Ratio	Lower	Upper
112	100		
64	64.0	52.9	79.3
63	36.1	29.6	44.4

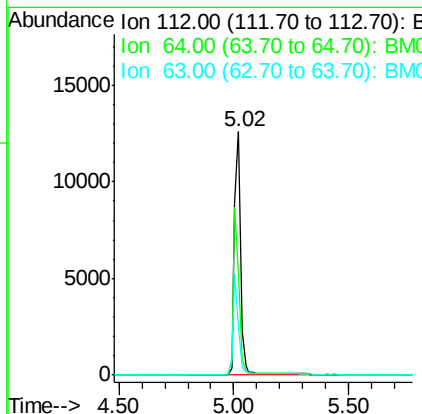



#5

Phenol-d6

Concen: 10.46 ng

RT: 6.61 min Scan# 255

Delta R.T. 0.00 min

Lab File: BM001353.D

Acq: 21 May 2015 09:47

Instrument :

BNA_M





ClientSampleId :

SSTDIC010

Tot Ion:	99	Resp:	31823
Ion Ratio	Lower	Upper	
99	100		
42	25.9	21.4	32.2
71	35.9	29.0	43.4

Manual Integrations
APPROVED

apatel
5/21/2015 8:53:24 PM

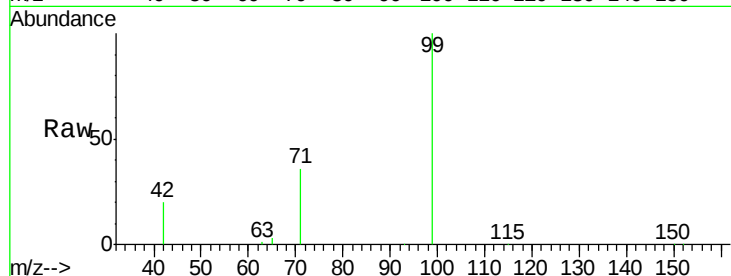

#6

Naphthalene-d8

Concen: 5.00 ng




RT: 10.20 min Scan# 536


Delta R.T. 0.00 min

Lab File: BM001353.D

Acq: 21 May 2015 09:47

Tgt Ion:	136	Resp:	51026
Ion Ratio	Lower	Upper	
136	100		
137	10.3	8.2	12.4
54	12.0	9.4	14.0
68	6.7	5.2	7.8

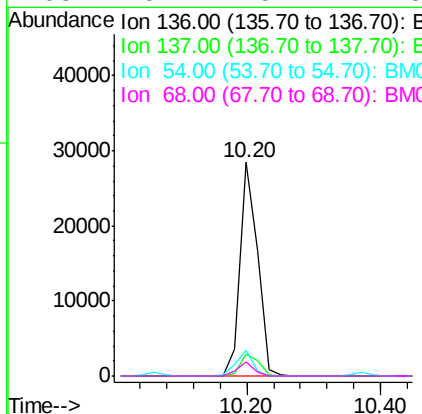



#7

Nitrobenzene-d5

Concen: 10.79 ng

RT: 8.59 min Scan# 396

Delta R.T. 0.00 min

Lab File: BM001353.D

Acq: 21 May 2015 09:47

Instrument :

BNA_M


ClientSampled :

SSTDICC010




Tot Ion:	82	Resp:	31960
Ion Ratio	Lower	Upper	
82	100		
128	44.8	33.5	50.3
54	49.9	45.1	67.7

Manual Integrations
APPROVED

apatel
5/21/2015 8:53:24 PM

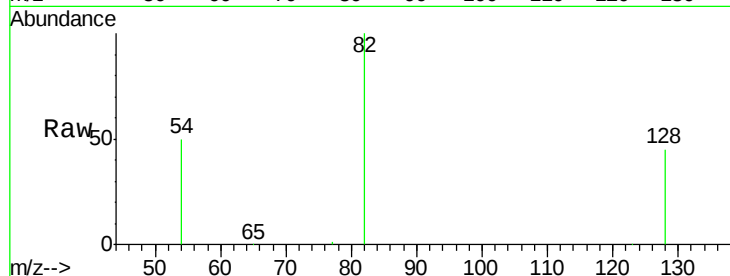

Abundance Ion 82.00 (81.70 to 82.70): BM001353.D (-392) (-)

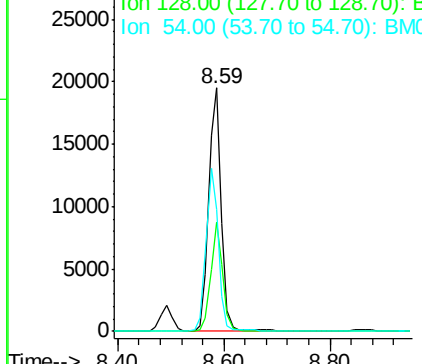

#8

Nitrobenzene

Concen: 11.07 ng


RT: 8.63 min Scan# 400

Delta R.T. 0.00 min



Lab File: BM001353.D


Acq: 21 May 2015 09:47

Tgt Ion:	77	Resp:	34406
Ion Ratio	Lower	Upper	
77	100		
123	44.1	33.6	50.4
65	14.6	11.3	16.9



Abundance Ion 77.00 (76.70 to 77.70): BM001353.D (-395) (-)

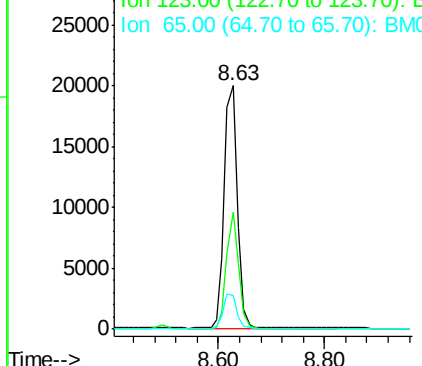



#9

Naphthalene

Concen: 9.90 ng

RT: 10.25 min Scan# 539

Delta R.T. 0.00 min

Lab File: BM001353.D

Acq: 21 May 2015 09:47

Instrument :

BNA_M





ClientSampleId :

SSTDIC010

Tot Ion:	128	Resp:	104933
Ion Ratio	Lower	Upper	
128	100		
129	10.9	9.1	13.7
127	12.5	10.4	15.6

Manual Integrations
APPROVED

apatel
5/21/2015 8:53:24 PM

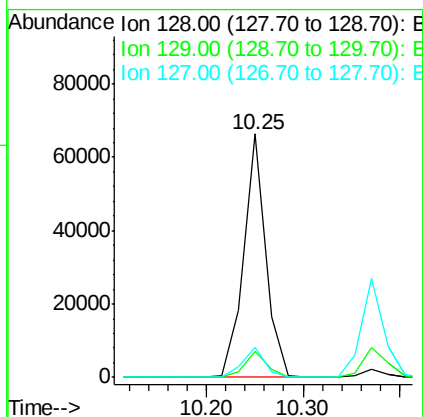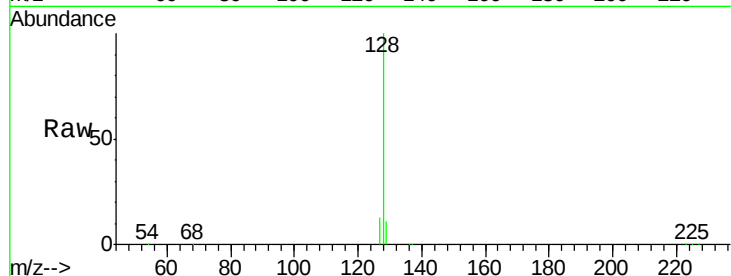

#10

Hexachlorobutadiene

Concen: 9.71 ng




RT: 10.54 min Scan# 556


Delta R.T. 0.00 min

Lab File: BM001353.D

Acq: 21 May 2015 09:47

Tgt Ion:	225	Resp:	19647
Ion Ratio	Lower	Upper	
225	100		
223	63.0	50.3	75.5
227	63.9	50.6	75.8

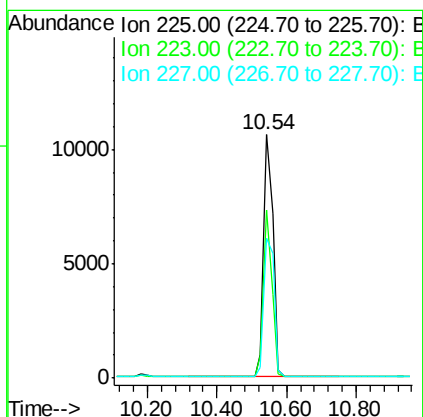

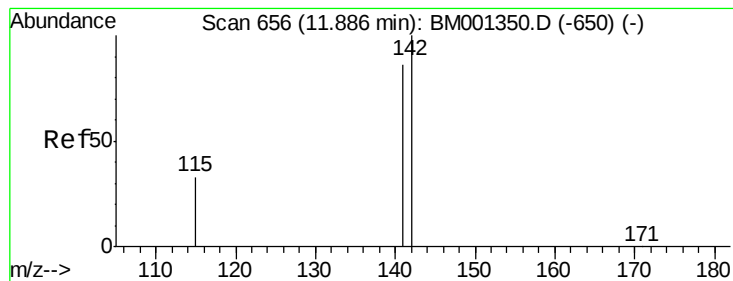

#11

2-Methylnaphthalene

Concen: 10.15 ng

RT: 11.89 min Scan# 656

Delta R.T. 0.00 min

Lab File: BM001353.D

Acq: 21 May 2015 09:47

Instrument :

BNA_M





ClientSampleId :

SSTDIC010

Tot Ion:	142	Resp:	76307
Ion Ratio	Lower	Upper	
142	100		
141	82.6	69.0	103.4
115	30.8	27.1	40.7

Manual Integrations
APPROVED

apatel
5/21/2015 8:53:24 PM

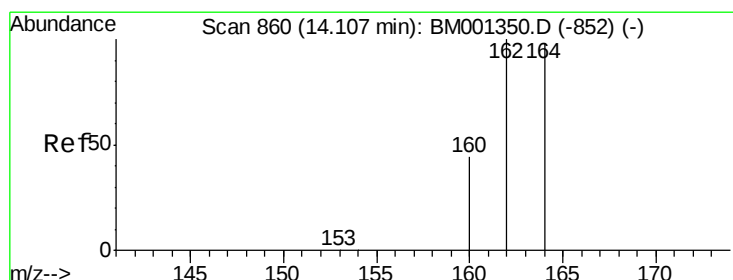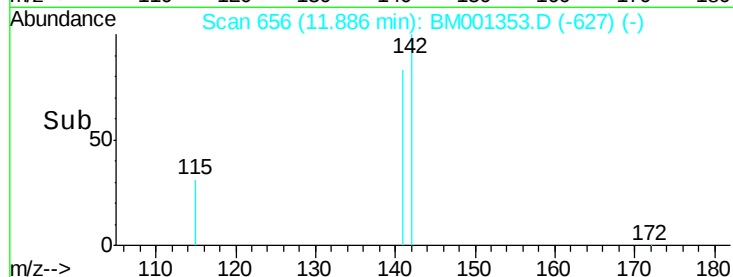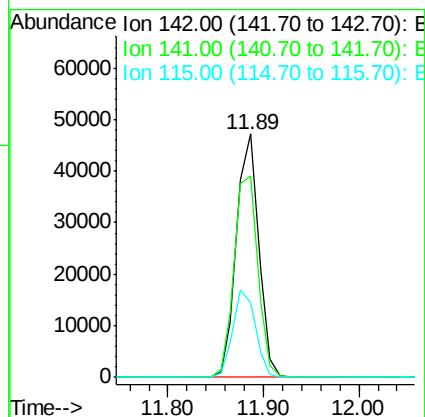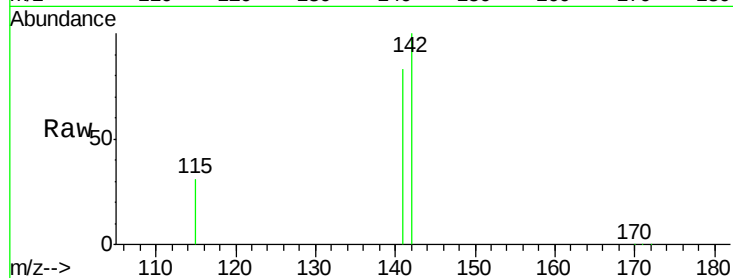

#12

Acenaphthene-d10

Concen: 5.00 ng




RT: 14.11 min Scan# 860


Delta R.T. 0.00 min

Lab File: BM001353.D

Acq: 21 May 2015 09:47

Tgt Ion:	164	Resp:	31939
Ion Ratio	Lower	Upper	
164	100		
162	103.5	81.8	122.8
160	45.2	35.8	53.8

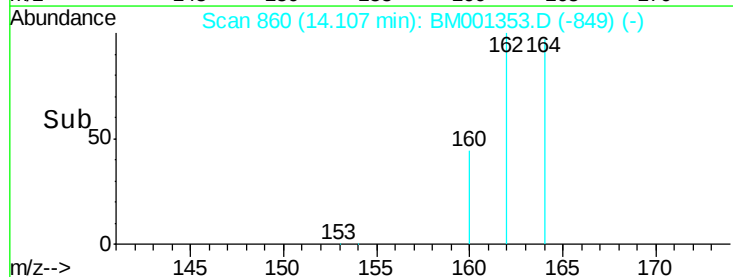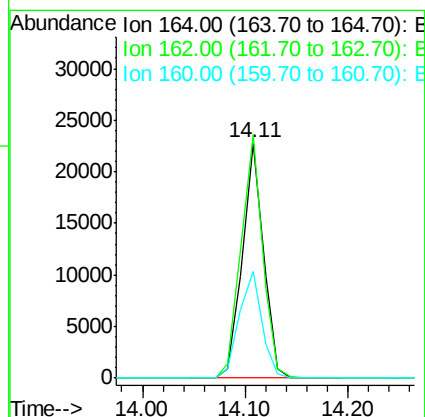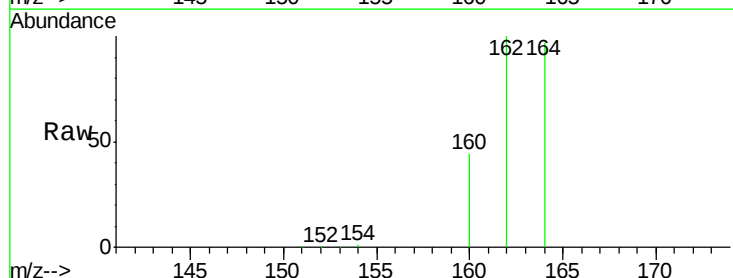







#13
 2,4,6-Tribromophenol
 Concen: 13.47 ng
 RT: 15.59 min Scan# 936
 Delta R.T. 0.00 min
 Lab File: BM001353.D
 Acq: 21 May 2015 09:47

Instrument :
 BNA_M
 ClientSampleId :
 SSTDICC010

Tot Ion	Ratio	Lower	Upper
330	100		
332	79.7	65.4	98.2
141	0.0	20.2	30.4




Manual Integrations
 APPROVED


apatel
 5/21/2015 8:53:24 PM

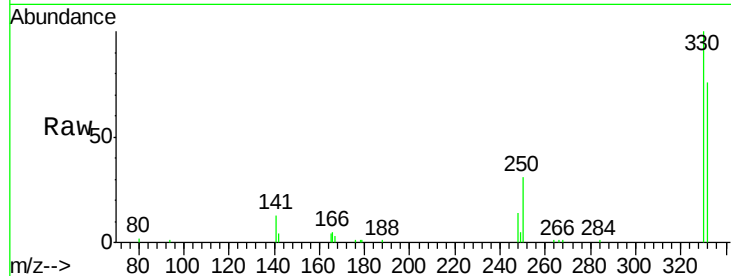

#14
 2-Fluorobiphenyl
 Concen: 9.73 ng
 RT: 12.72 min Scan# 736
 Delta R.T. 0.00 min
 Lab File: BM001353.D
 Acq: 21 May 2015 09:47

Tgt Ion	Ratio	Lower	Upper
172	100		
171	31.3	25.4	38.2
170	18.6	15.7	23.5



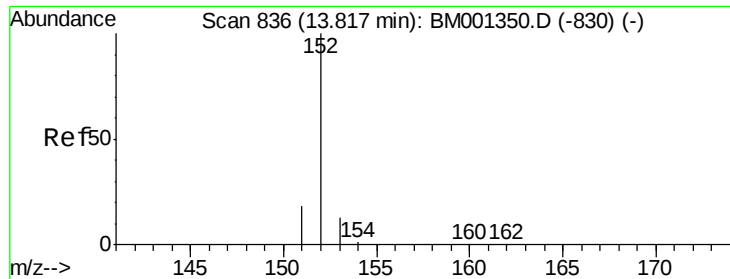





#15
Acenaphthylene
Concen: 10.52 ng
RT: 13.82 min Scan# 836
Delta R.T. 0.00 min
Lab File: BM001353.D
Acq: 21 May 2015 09:47

Instrument :
BNA_M
ClientSampleId :
SSTDIC010

Tot Ion	Ratio	Lower	Upper
152	100		
151	19.0	15.3	22.9
153	12.9	10.3	15.5




Manual Integrations
APPROVED


apatel
5/21/2015 8:53:24 PM

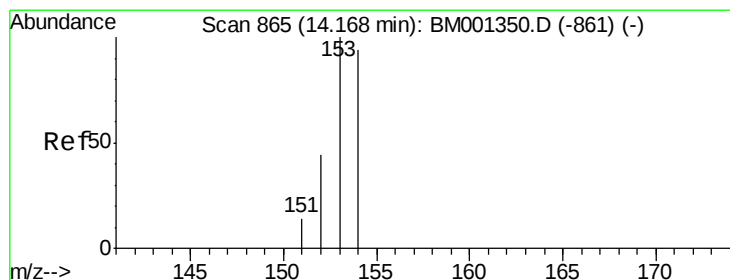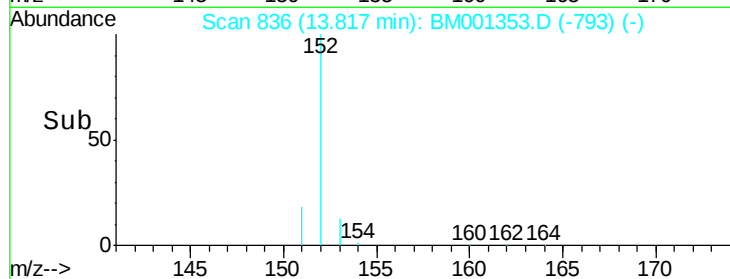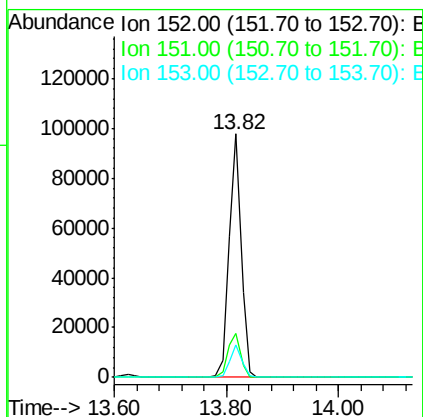

#16
Acenaphthene
Concen: 10.03 ng
RT: 14.17 min Scan# 865
Delta R.T. 0.00 min
Lab File: BM001353.D
Acq: 21 May 2015 09:47

Tgt Ion	Ratio	Lower	Upper
154	100		
153	111.9	90.6	135.8
152	52.7	43.6	65.4

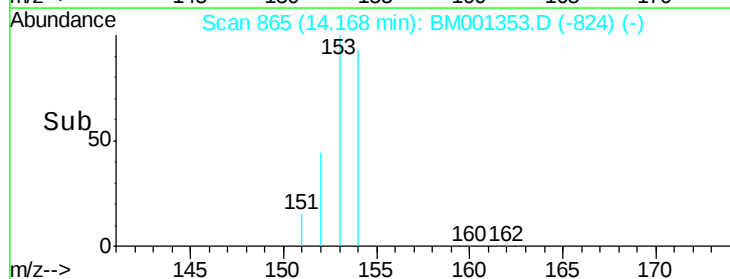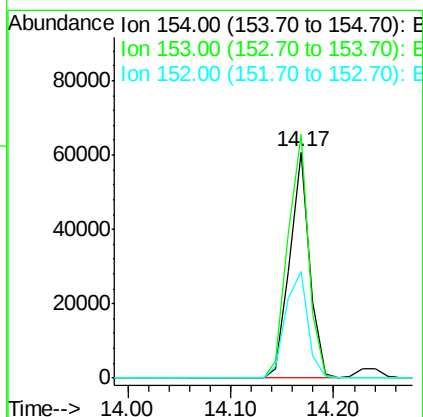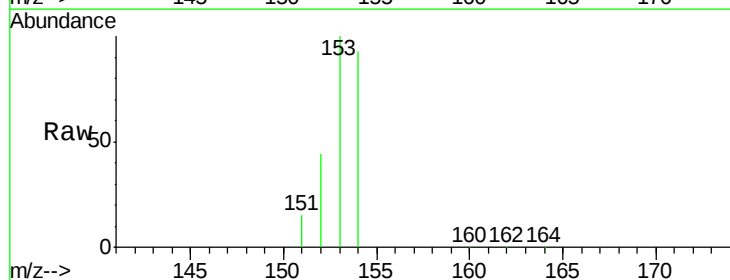







#17
Fluorene
 Concen: 7.58 ng
 RT: 15.15 min Scan# 923
 Delta R.T. 0.00 min
 Lab File: BM001353.D
 Acq: 21 May 2015 09:47

Instrument :
 BNA_M
 ClientSampleId :
 SSTDICC010

Tot Ion	Ratio	Lower	Upper
166	100		
165	87.5	72.5	108.7
167	15.5	16.0	24.0#




Manual Integrations
 APPROVED


apatel
 5/21/2015 8:53:24 PM

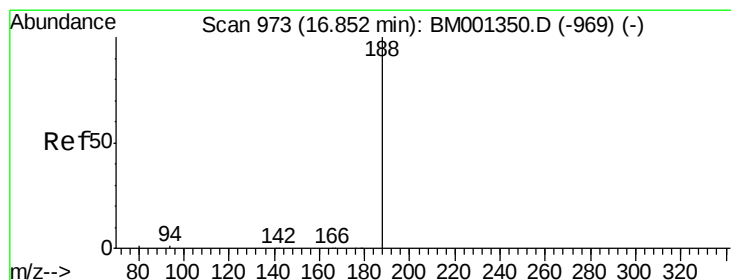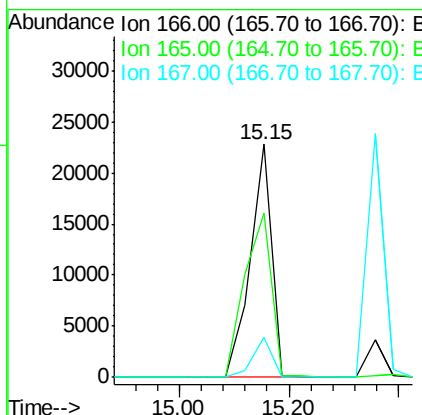

#18
Phenanthrene-d10
 Concen: 5.00 ng
 RT: 16.85 min Scan# 973
 Delta R.T. 0.00 min
 Lab File: BM001353.D
 Acq: 21 May 2015 09:47

Tgt Ion	Ratio	Lower	Upper
188	100		
94	0.7	0.6	1.0
80	0.6	0.6	0.8#

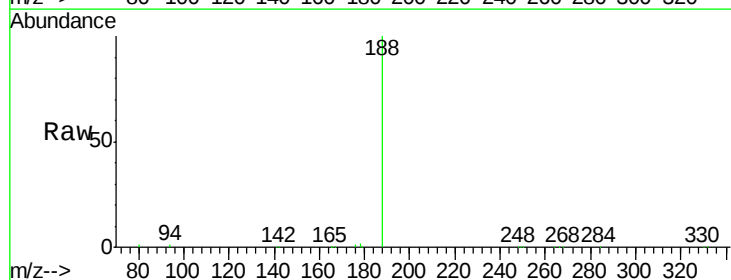







#19
4-Bromophenyl-phenylether
Concen: 14.64 ng
RT: 16.04 min Scan# 949
Delta R.T. 0.00 min
Lab File: BM001353.D
Acq: 21 May 2015 09:47

Instrument :
BNA_M
ClientSampleId :
SSTDIC010

Tot Ion:248 Resp: 34645
Ion Ratio Lower Upper
248 100
250 65.0 51.5 77.3
141 72.9 59.0 88.6




Manual Integrations
APPROVED




apatel
5/21/2015 8:53:24 PM

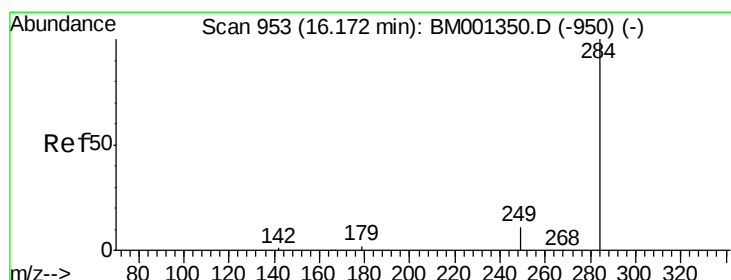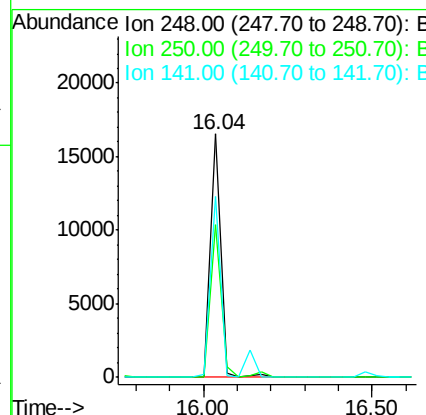

#20
Hexachlorobenzene
Concen: 11.13 ng
RT: 16.17 min Scan# 953
Delta R.T. 0.00 min
Lab File: BM001353.D
Acq: 21 May 2015 09:47

Tgt Ion:284 Resp: 47655
Ion Ratio Lower Upper
284 100
142 0.0 0.0 0.0
249 14.7 11.1 16.7

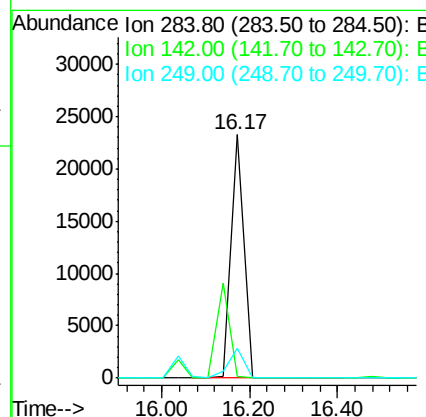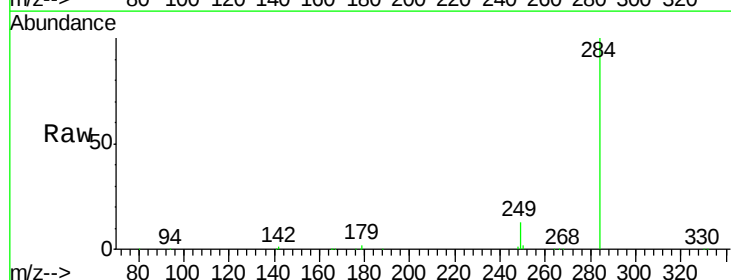

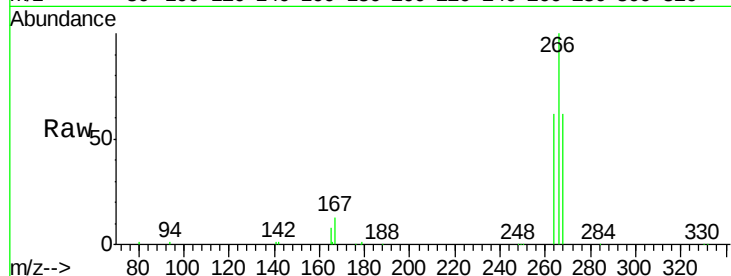

#21

Pentachlorophenol

Concen: 17.99 ng

RT: 16.51 min Scan# 963

Delta R.T. 0.00 min

Lab File: BM001353.D

Acq: 21 May 2015 09:47

Tot Ion:	266	Resp:	27616
Ion Ratio	Lower	Upper	
266	100		
268	61.6	51.2	76.8
264	62.4	53.7	80.5

Instrument :





BNA_M

ClientSampleId :

SSTDIC010

Manual Integrations
APPROVED

apatel
5/21/2015 8:53:24 PM

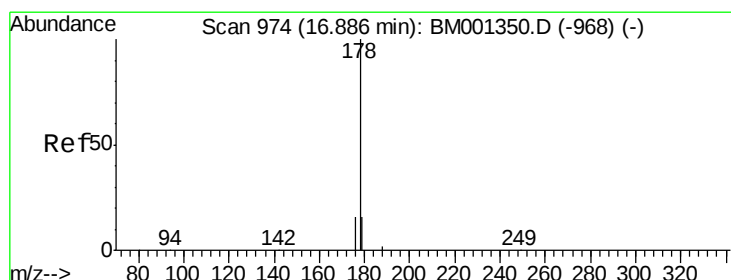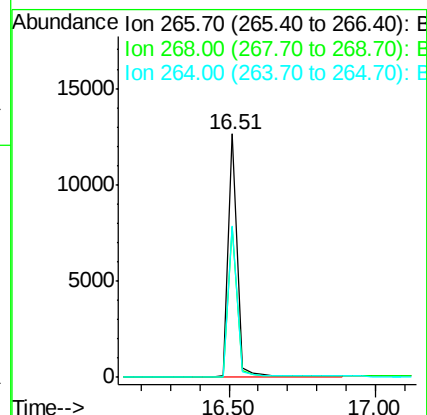

#22

Phenanthrene

Concen: 10.49 ng m


RT: 16.89 min Scan# 974


Delta R.T. 0.00 min

Lab File: BM001353.D

Acq: 21 May 2015 09:47

Tgt Ion:	178	Resp:	235664
Ion Ratio	Lower	Upper	
178	100		
176	23.3	16.6	25.0
179	18.0	12.8	19.2

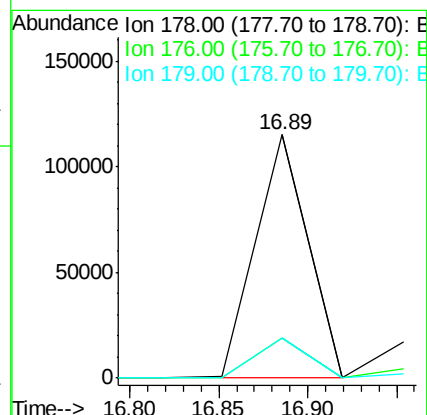



#23

Anthracene

Concen: 10.22 ng m

RT: 16.99 min Scan# 977

Delta R.T. 0.00 min

Lab File: BM001353.D

Acq: 21 May 2015 09:47

Instrument :

BNA_M

ClientSampleId :





SSTDIC010

Manual Integrations
APPROVED

apatel

5/21/2015 8:53:24 PM

Tot Ion:178	Resp:	82390
Ion Ratio	Lower	Upper
178 100		
176 66.7	46.1	69.1
179 51.6	35.4	53.0

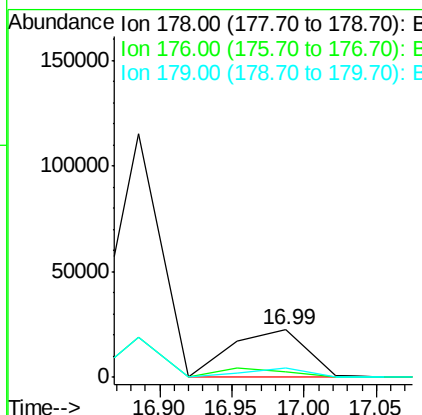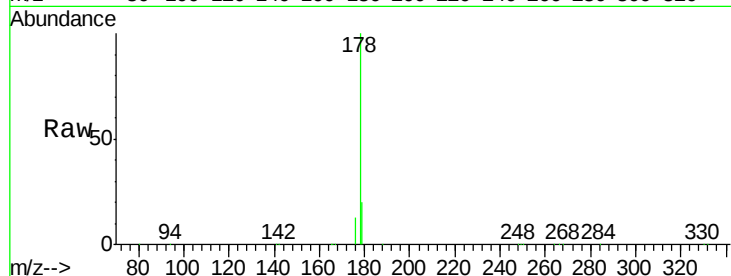

#24

Fluoranthene

Concen: 12.29 ng




RT: 18.92 min Scan# 1070


Delta R.T. 0.00 min

Lab File: BM001353.D

Acq: 21 May 2015 09:47

Tgt Ion:202	Resp:	205735
Ion Ratio	Lower	Upper
202 100		
101 11.3	8.7	13.1
203 17.2	13.8	20.6

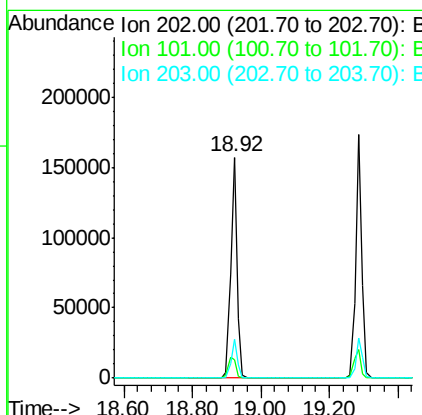







#25
Chrysene-d12
Concen: 5.00 ng
RT: 21.07 min Scan# 1238
Delta R.T. 0.00 min
Lab File: BM001353.D
Acq: 21 May 2015 09:47

Instrument :
BNA_M
ClientSampleId :
SSTDICC010

Tot Ion	Ion	Ratio	Resp	Lower	Upper
240	100		70981		
120	2.1	1.6	2.4		
236	23.9	18.5	27.7		




Manual Integrations
APPROVED


apatel
5/21/2015 8:53:24 PM

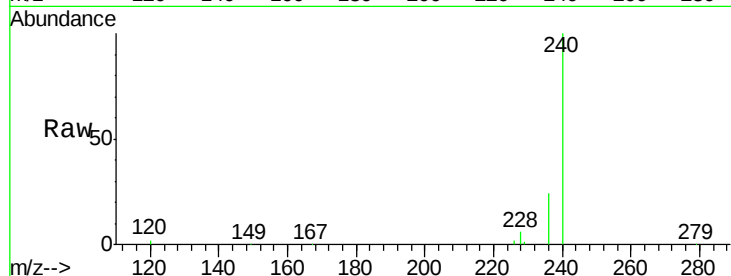

#26
Pyrene
Concen: 10.41 ng
RT: 19.29 min Scan# 1100
Delta R.T. 0.00 min
Lab File: BM001353.D
Acq: 21 May 2015 09:47

Tgt Ion	Ion	Ratio	Resp	Lower	Upper
202	100		217447		
200	20.6	16.2	24.4		
203	17.3	13.9	20.9		



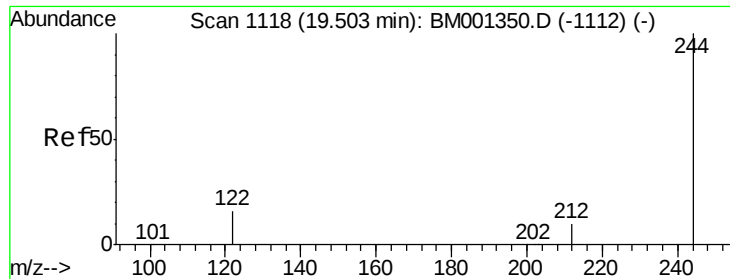

#27

Terphenyl-d14

Concen: 10.13 ng

RT: 19.50 min Scan# 1118

Delta R.T. 0.00 min

Lab File: BM001353.D

Acq: 21 May 2015 09:47

Instrument :

BNA_M


ClientSampleId :

SSTDICC010




Tot Ion	Ratio	Lower	Upper
244	100		
212	10.0	8.5	12.7
122	15.7	13.4	20.2

Manual Integrations
APPROVED

apatel
5/21/2015 8:53:24 PM



Abundance Ion 244.00 (243.70 to 244.70): E
Ion 212.00 (211.70 to 212.70): E
Ion 122.00 (121.70 to 122.70): E

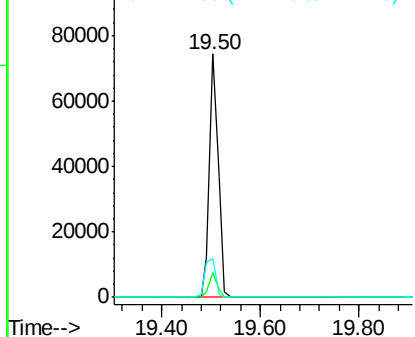

#28

Benzo(a)anthracene

Concen: 10.39 ng

RT: 21.04 min Scan# 1236




Delta R.T. 0.00 min


Lab File: BM001353.D

Acq: 21 May 2015 09:47

Tgt Ion	Ratio	Lower	Upper
228	100		
226	30.3	24.5	36.7
229	16.7	13.3	19.9

Abundance Ion 228.00 (227.70 to 228.70): E
Ion 226.00 (225.70 to 226.70): E
Ion 229.00 (228.70 to 229.70): E

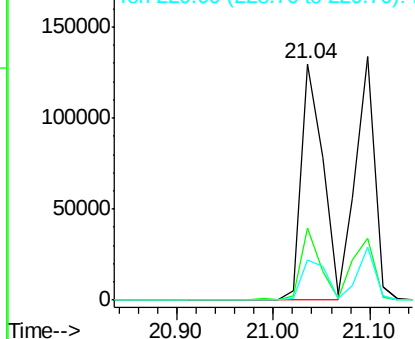

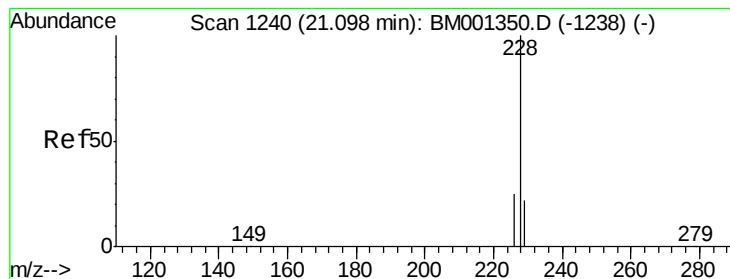

#29

Chrysene

Concen: 9.93 ng

RT: 21.10 min Scan# 1240

Delta R.T. 0.00 min

Lab File: BM001353.D

Acq: 21 May 2015 09:47

Instrument :

BNA_M


ClientSampleId :

SSTDICC010




Tot Ion:	228	Resp:	184672
Ion Ratio	Lower	Upper	
228	100		
226	25.5	20.0	30.0
229	21.5	17.6	26.4

Manual Integrations
APPROVED

apatel
5/21/2015 8:53:24 PM



Abundance Ion 228.00 (227.70 to 228.70): E
Ion 226.00 (225.70 to 226.70): E
Ion 229.00 (228.70 to 229.70): E

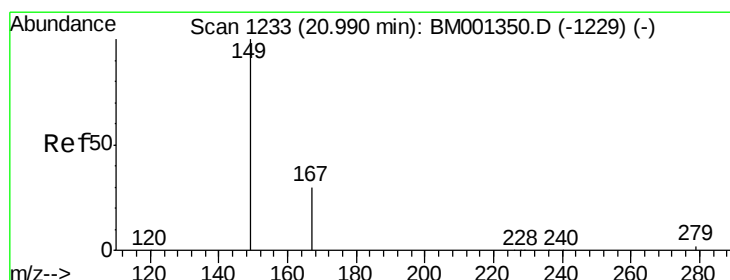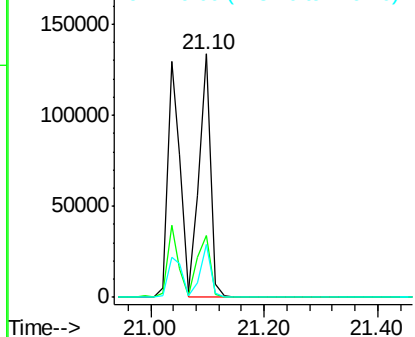

#30

Bis(2-ethylhexyl)phthalate

Concen: 11.82 ng


RT: 20.99 min Scan# 1233

Delta R.T. 0.00 min



Lab File: BM001353.D


Acq: 21 May 2015 09:47

Tgt Ion:	149	Resp:	128957
Ion Ratio	Lower	Upper	
149	100		
167	27.5	21.6	32.4
279	2.4	1.9	2.9



Abundance Ion 149.00 (148.70 to 149.70): E
Ion 167.00 (166.70 to 167.70): E
Ion 279.00 (278.70 to 279.70): E

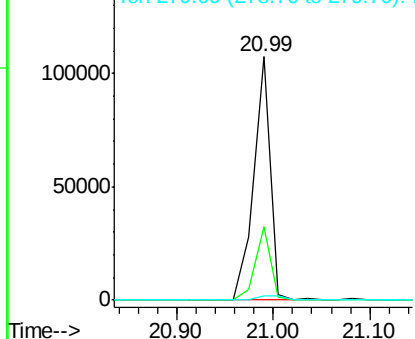




#31
Indeno(1,2,3-cd)pyrene
Concen: 10.29 ng
RT: 25.25 min Scan# 1610
Delta R.T. 0.01 min
Lab File: BM001353.D
Acq: 21 May 2015 09:47

Instrument :
BNA_M
ClientSampleId :
SSTDICC010

Tot Ion	Ratio	Resp	Lower	Upper
276	100	214225		
138	31.1	24.2	36.4	
277	24.5	19.7	29.5	

Manual Integrations
APPROVED

apatel
5/21/2015 8:53:24 PM



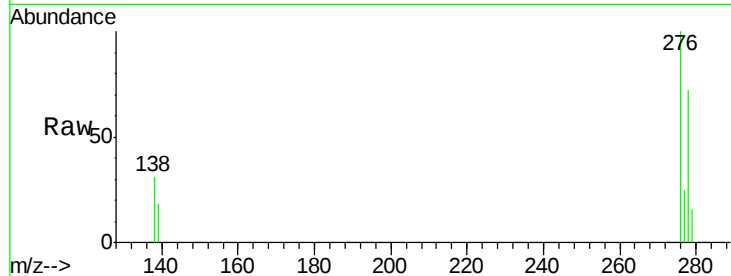


Abundance

Ion 276.00 (275.70 to 276.70): E


Ion 138.00 (137.70 to 138.70): E

Ion 277.00 (276.70 to 277.70): E

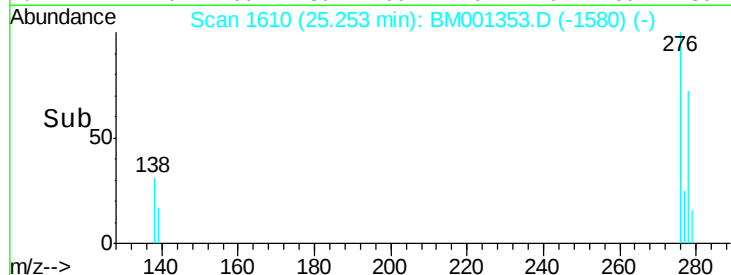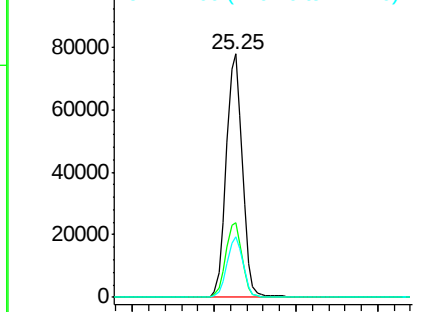

#32
Perylene-d12
Concen: 5.00 ng
RT: 23.17 min Scan# 1410
Delta R.T. 0.00 min
Lab File: BM001353.D
Acq: 21 May 2015 09:47

Tgt Ion	Ratio	Resp	Lower	Upper
264	100	67208		
260	26.2	20.4	30.6	
265	20.6	16.6	24.8	






Abundance

Ion 264.00 (263.70 to 264.70): E

Ion 260.00 (259.70 to 260.70): E

Ion 265.00 (264.70 to 265.70): E

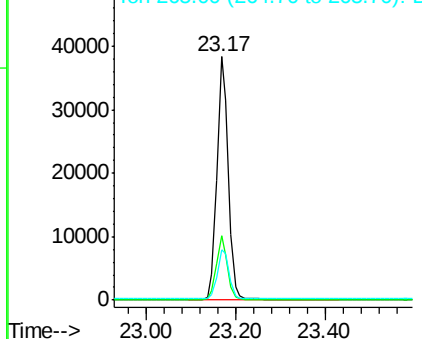



#33

Benzo(b)fluoranthene

Concen: 10.26 ng

RT: 22.54 min Scan# 1350

Delta R.T. 0.00 min

Lab File: BM001353.D

Acq: 21 May 2015 09:47





Instrument :
BNA_M

ClientSampleId :
SSTDIC010

Tot Ion	Ratio	Lower	Upper
252	100		
253	20.9	17.9	26.9
125	12.1	9.8	14.8

Manual Integrations
APPROVED

apatel
5/21/2015 8:53:24 PM

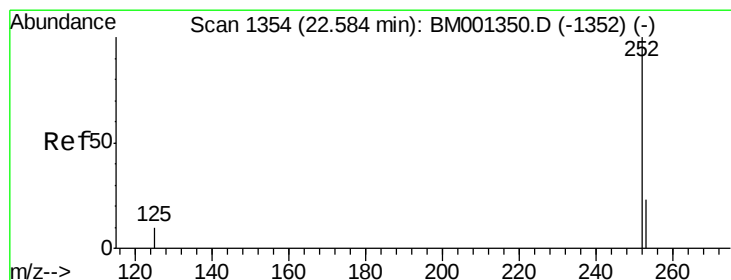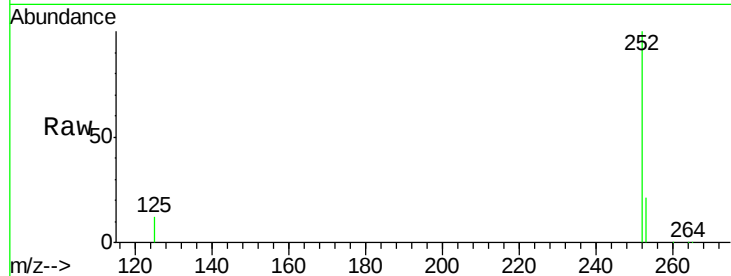

#34

Benzo(k)fluoranthene

Concen: 10.02 ng




RT: 22.58 min Scan# 1354


Delta R.T. 0.00 min

Lab File: BM001353.D

Acq: 21 May 2015 09:47

Tgt Ion	Ratio	Lower	Upper
252	100		
253	21.4	18.6	28.0
125	11.8	9.3	13.9





#35

Benzo(a)pyrene

Concen: 10.43 ng

RT: 23.07 min Scan# 1401

Delta R.T. 0.00 min

Lab File: BM001353.D


Acq: 21 May 2015 09:47

Instrument :

BNA_M

ClientSampleId :



SSTDICC010

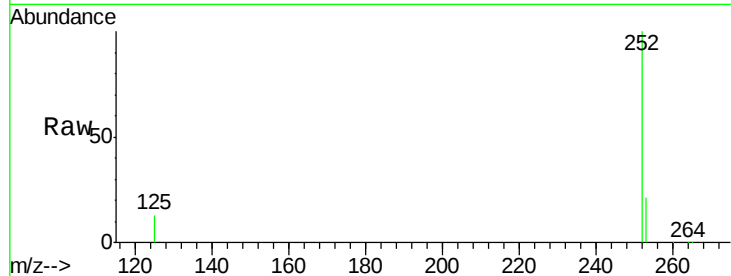

Tot Ion	Ratio	Resp	Lower	Upper
252	100			
253	21.0	18.9	28.3	
125	13.3	10.6	15.8	

Manual Integrations
APPROVED

apatel
5/21/2015 8:53:24 PM



#36

Dibenzo(a,h)anthracene

Concen: 10.23 ng




RT: 25.26 min Scan# 1611


Delta R.T. 0.01 min

Lab File: BM001353.D

Acq: 21 May 2015 09:47

Tgt Ion	Ratio	Resp	Lower	Upper
278	100			
139	19.6	17.5	26.3	
279	23.2	18.7	28.1	



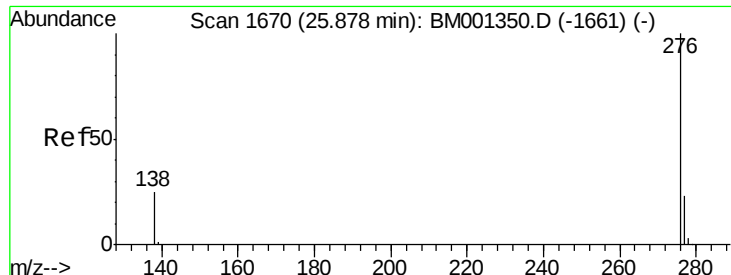

#37
 Benzo(a,h,i)perylene
 Concen: 10.00 ng
 RT: 25.88 min Scan# 1670
 Delta R.T. 0.00 min
 Lab File: BM001353.D
 Acq: 21 May 2015 09:47

Instrument :
 BNA_M
 ClientSampleId :
 SSTDICC010

Tot Ion	Ratio	Lower	Upper
276	100		
277	22.5	19.2	28.8
138	27.8	20.2	30.4

Manual Integrations
 APPROVED

apatel
 5/21/2015 8:53:24 PM

