


Data Path : Z:\HPCHEM1\BNA_M\Data\BM052015\
 Data File : BM001364.D
 Acq On : 21 May 2015 17:31
 Operator : TP/IZ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_M\METHODS\8270-BM031115.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Sat Mar 28 05:37:34 2015

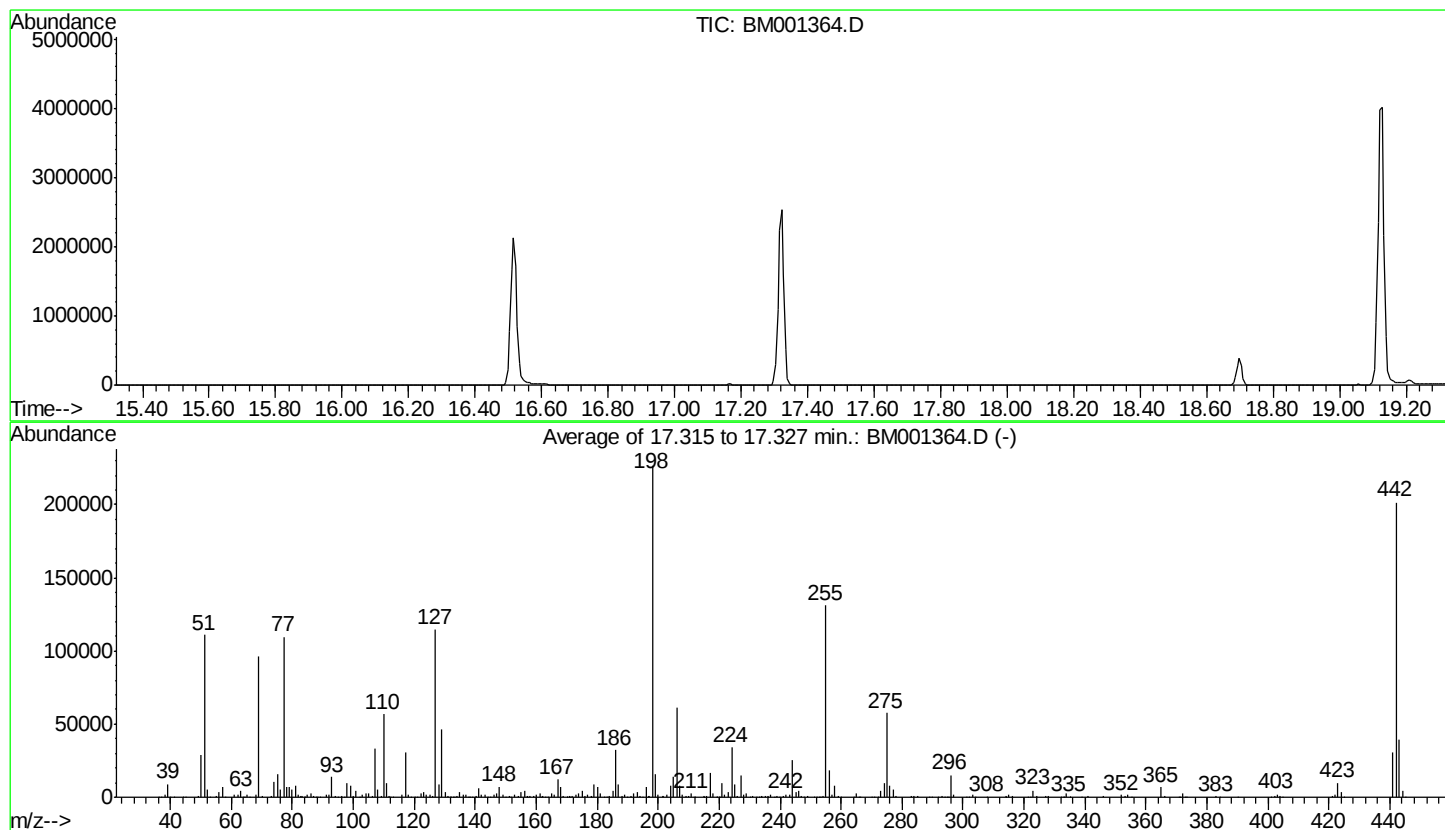

AutoFind: Scans 2487, 2488, 2489; Background Corrected with Scan 2480

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	48.9	110781	PASS
68	69	0.00	2	1.8	1752	PASS
69	198	0.00	100	42.5	96234	PASS
70	69	0.00	2	0.5	476	PASS
127	198	10	80	50.5	114365	PASS
197	198	0.00	2	0.4	879	PASS
198	198	100	100	100.0	226666	PASS
199	198	5	9	7.0	15820	PASS
275	198	10	60	25.3	57386	PASS
365	198	1	100	2.9	6595	PASS
441	442	0.01	24	15.0	30242	PASS
442	198	50	100	88.9	201578	PASS
443	442	15	24	19.7	39733	PASS