

Data Path : Z:\HPCHEM1\BNA M\DATA\BM052016\
 Data File : BM005542.D
 Acq On : 21 May 2016 05:34
 Operator : UM/SJ
 Sample : H3058-15
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BD3F0

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM052016.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.652	8	11	25	rVB2	44193	98951	3.48%	0.390%
2	6.981	741	747	755	rVB	125406	198821	6.99%	0.784%
3	7.157	770	777	784	rBV	320226	496215	17.45%	1.957%
4	7.351	804	810	820	rBV	365880	597590	21.02%	2.357%
5	7.822	883	890	897	rVB	374507	592645	20.84%	2.337%
6	8.522	999	1009	1020	rBV	322185	523727	18.42%	2.065%
7	8.975	1077	1086	1094	rBV	412006	675910	23.77%	2.666%
8	9.692	1201	1208	1215	rBV	342882	574452	20.20%	2.266%
9	10.228	1292	1299	1307	rBV	516625	843961	29.68%	3.328%
10	10.610	1357	1364	1373	rBV	505014	856250	30.11%	3.377%
11	10.745	1381	1387	1393	rVB	40788	66454	2.34%	0.262%
12	13.863	1910	1917	1923	rBV	1009374	1433307	50.41%	5.653%
13	14.145	1958	1965	1972	rBV	1116750	1653538	58.15%	6.521%
14	14.451	2010	2017	2027	rVB2	717458	1139069	40.06%	4.492%
15	14.639	2043	2049	2060	rBV	131553	191494	6.73%	0.755%
16	15.445	2179	2186	2193	rBV	1459535	2139733	75.25%	8.439%
17	15.557	2199	2205	2214	rBV	452390	607440	21.36%	2.396%
18	17.192	2477	2483	2490	rBV2	928766	1335455	46.97%	5.267%
19	17.292	2493	2500	2510	rBV	1653716	2393687	84.19%	9.440%
20	19.580	2883	2889	2897	rBV	1992468	2746574	96.60%	10.832%
21	21.362	3187	3192	3198	rBV	1330389	1671791	58.80%	6.593%
22	23.497	3547	3555	3569	rVB2	1489626	2843349	100.00%	11.214%
23	23.639	3572	3579	3593	rVB	840770	1675670	58.93%	6.609%


Sum of corrected areas: 25356083

Data Path : Z:\HPCHEM1\BNA M\DATA\BM052016\
Data File : BM005542.D
Acq On : 21 May 2016 05:34
Operator : UM/SJ
Sample : H3058-15
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BD3F0

Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM02.2-EPA-BM052016.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

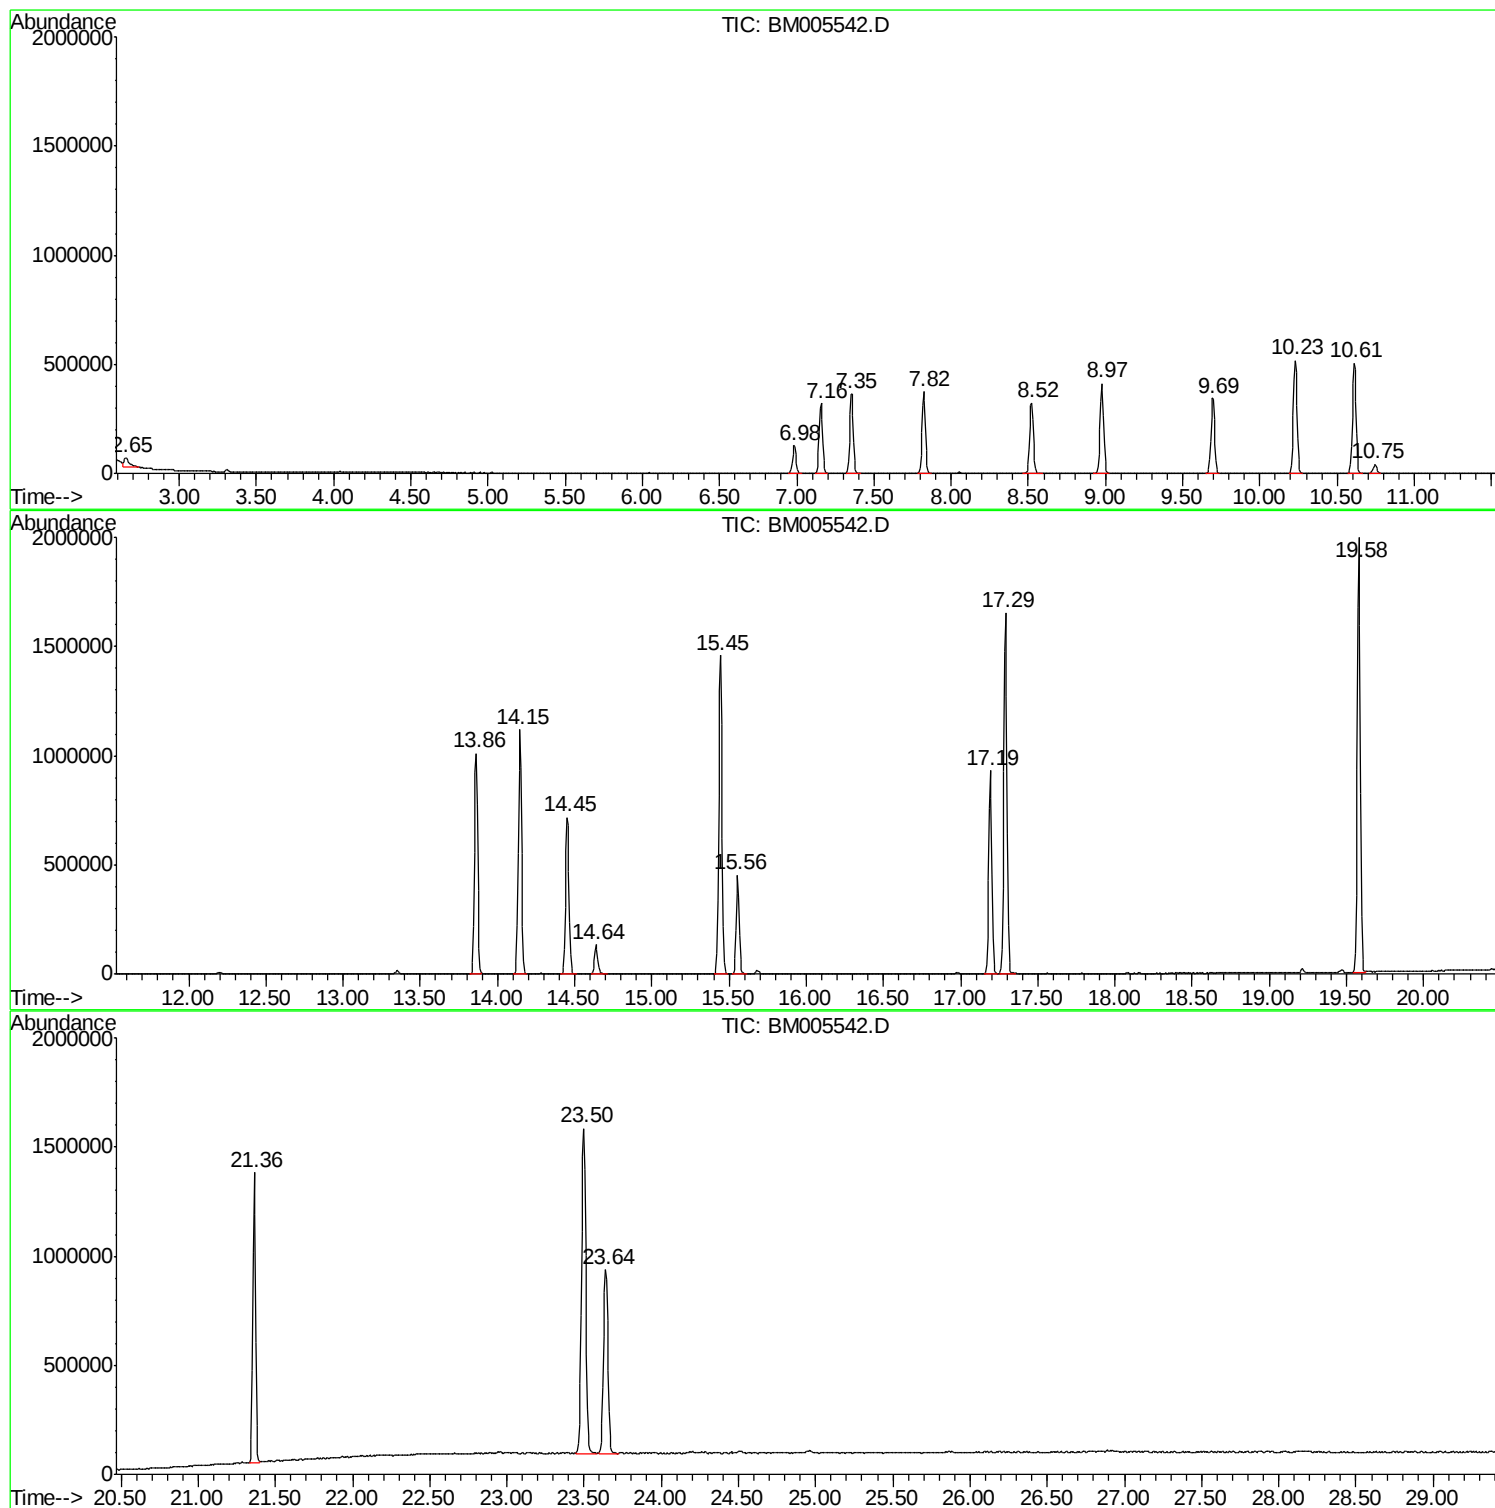

Data Path : Z:\HPCHEM1\BNA M\DATA\BM052016\
Data File : BM005542.D
Acq On : 21 May 2016 05:34
Operator : UM/SJ
Sample : H3058-15
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BD3F0










Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM02.2-EPA-BM052016.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Methane, oxybis[dichloro- Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
2.65	3.34 ng/ul	98951	1,4-Dichlorobenzene-d4	7.82

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Methane, oxybis[dichloro-	182	C2H2Cl4O	020524-86-1	83
2			Trichloromethane	118	CHCl3	000067-66-3	78
3			Trichloromethane	118	CHCl3	000067-66-3	74
4			Ethane, 1,2,2-trichloro-1,1-difl...	168	C2HCl3F2	000354-21-2	72
5			Methane, dichloronitro-	129	CHCl2NO2	007119-89-3	39

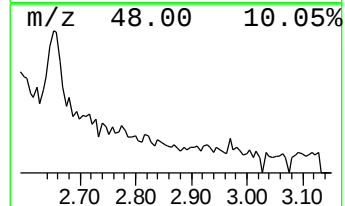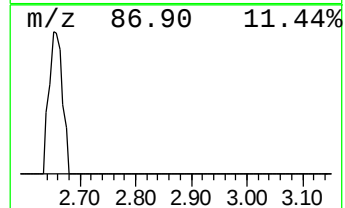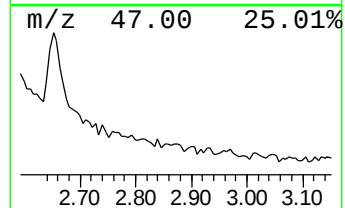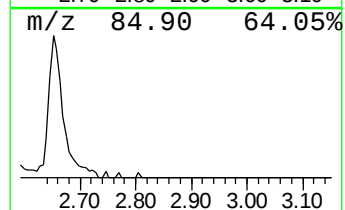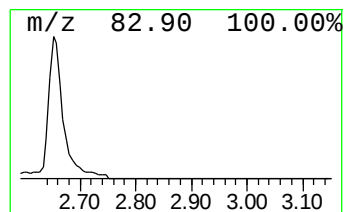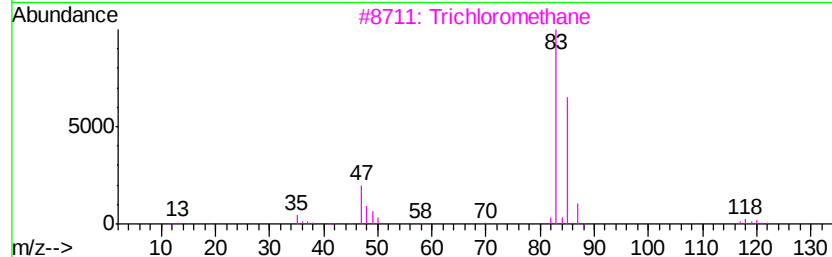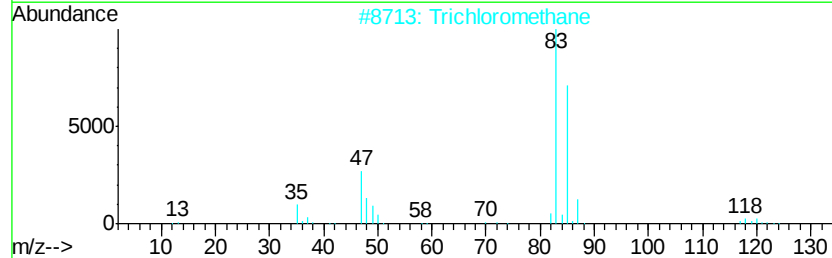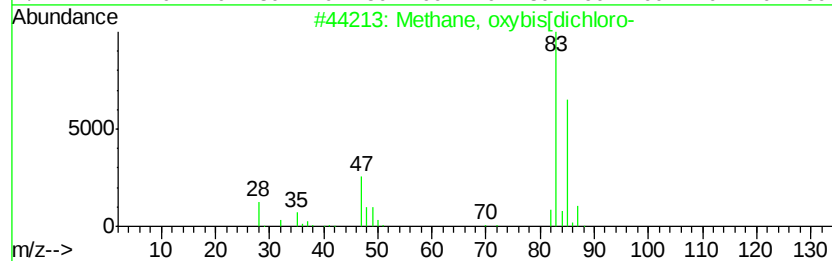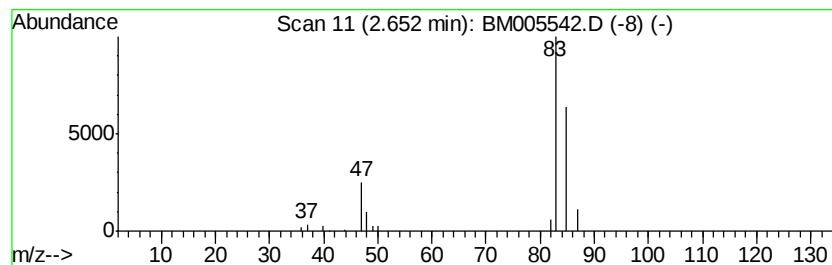

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM052016\
Data File : BM005542.D
Acq On : 21 May 2016 05:34
Operator : UM/SJ
Sample : H3058-15
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BD3F0

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM052016.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Methane, oxybis[d...	2.65	3.3	ng/ul	98951	1	7.82	592645	20.0