

Data Path : Z:\HPCHEM1\BNA M\DATA\BM052016\
 Data File : BM005547.D
 Acq On : 21 May 2016 08:36
 Operator : UM/SJ
 Sample : H3058-18
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BD3F3

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM052016.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.652	8	11	20	rVB	47928	93535	2.39%	0.284%
2	6.981	741	747	757	rVB	135193	215818	5.52%	0.655%
3	7.157	770	777	785	rVB	368033	571154	14.62%	1.734%
4	7.351	804	810	818	rVB	428930	681663	17.45%	2.069%
5	7.822	883	890	897	rBV	559553	899220	23.02%	2.729%
6	8.516	999	1008	1020	rBV	351451	575407	14.73%	1.747%
7	8.975	1079	1086	1094	rBV	433915	720343	18.44%	2.186%
8	9.692	1202	1208	1215	rBV	353550	585699	14.99%	1.778%
9	10.228	1292	1299	1308	rBV	559686	914462	23.41%	2.776%
10	10.381	1320	1325	1334	rVB	26494	43572	1.12%	0.132%
11	10.610	1357	1364	1376	rVB	748037	1253329	32.08%	3.804%
12	13.863	1910	1917	1923	rBV	1100175	1536931	39.34%	4.665%
13	14.145	1957	1965	1974	rBV	1206182	1775984	45.46%	5.391%
14	14.451	2011	2017	2026	rVB2	1085771	1635561	41.87%	4.964%
15	14.639	2043	2049	2061	rBV	146484	219680	5.62%	0.667%
16	15.445	2179	2186	2194	rBV	1647926	2403989	61.54%	7.297%
17	15.557	2199	2205	2214	rBV	527241	712021	18.23%	2.161%
18	17.192	2476	2483	2489	rBV	1397270	1999311	51.18%	6.068%
19	17.292	2493	2500	2511	rVB	1954324	2883245	73.80%	8.751%
20	19.580	2882	2889	2897	rBV	2612930	3527123	90.29%	10.706%
21	21.286	3176	3179	3184	rBV6	26121	48628	1.24%	0.148%
22	21.368	3187	3193	3201	rVB	2077078	2814598	72.05%	8.543%
23	23.503	3548	3556	3571	rVB2	1956737	3906601	100.00%	11.858%
24	23.644	3572	3580	3589	rBV	1457281	2831183	72.47%	8.593%
25	24.197	3670	3674	3682	rVB2	53913	96778	2.48%	0.294%


Sum of corrected areas: 32945835

Data Path : Z:\HPCHEM1\BNA M\DATA\BM052016\
Data File : BM005547.D
Acq On : 21 May 2016 08:36
Operator : UM/SJ
Sample : H3058-18
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BD3F3

Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM02.2-EPA-BM052016.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

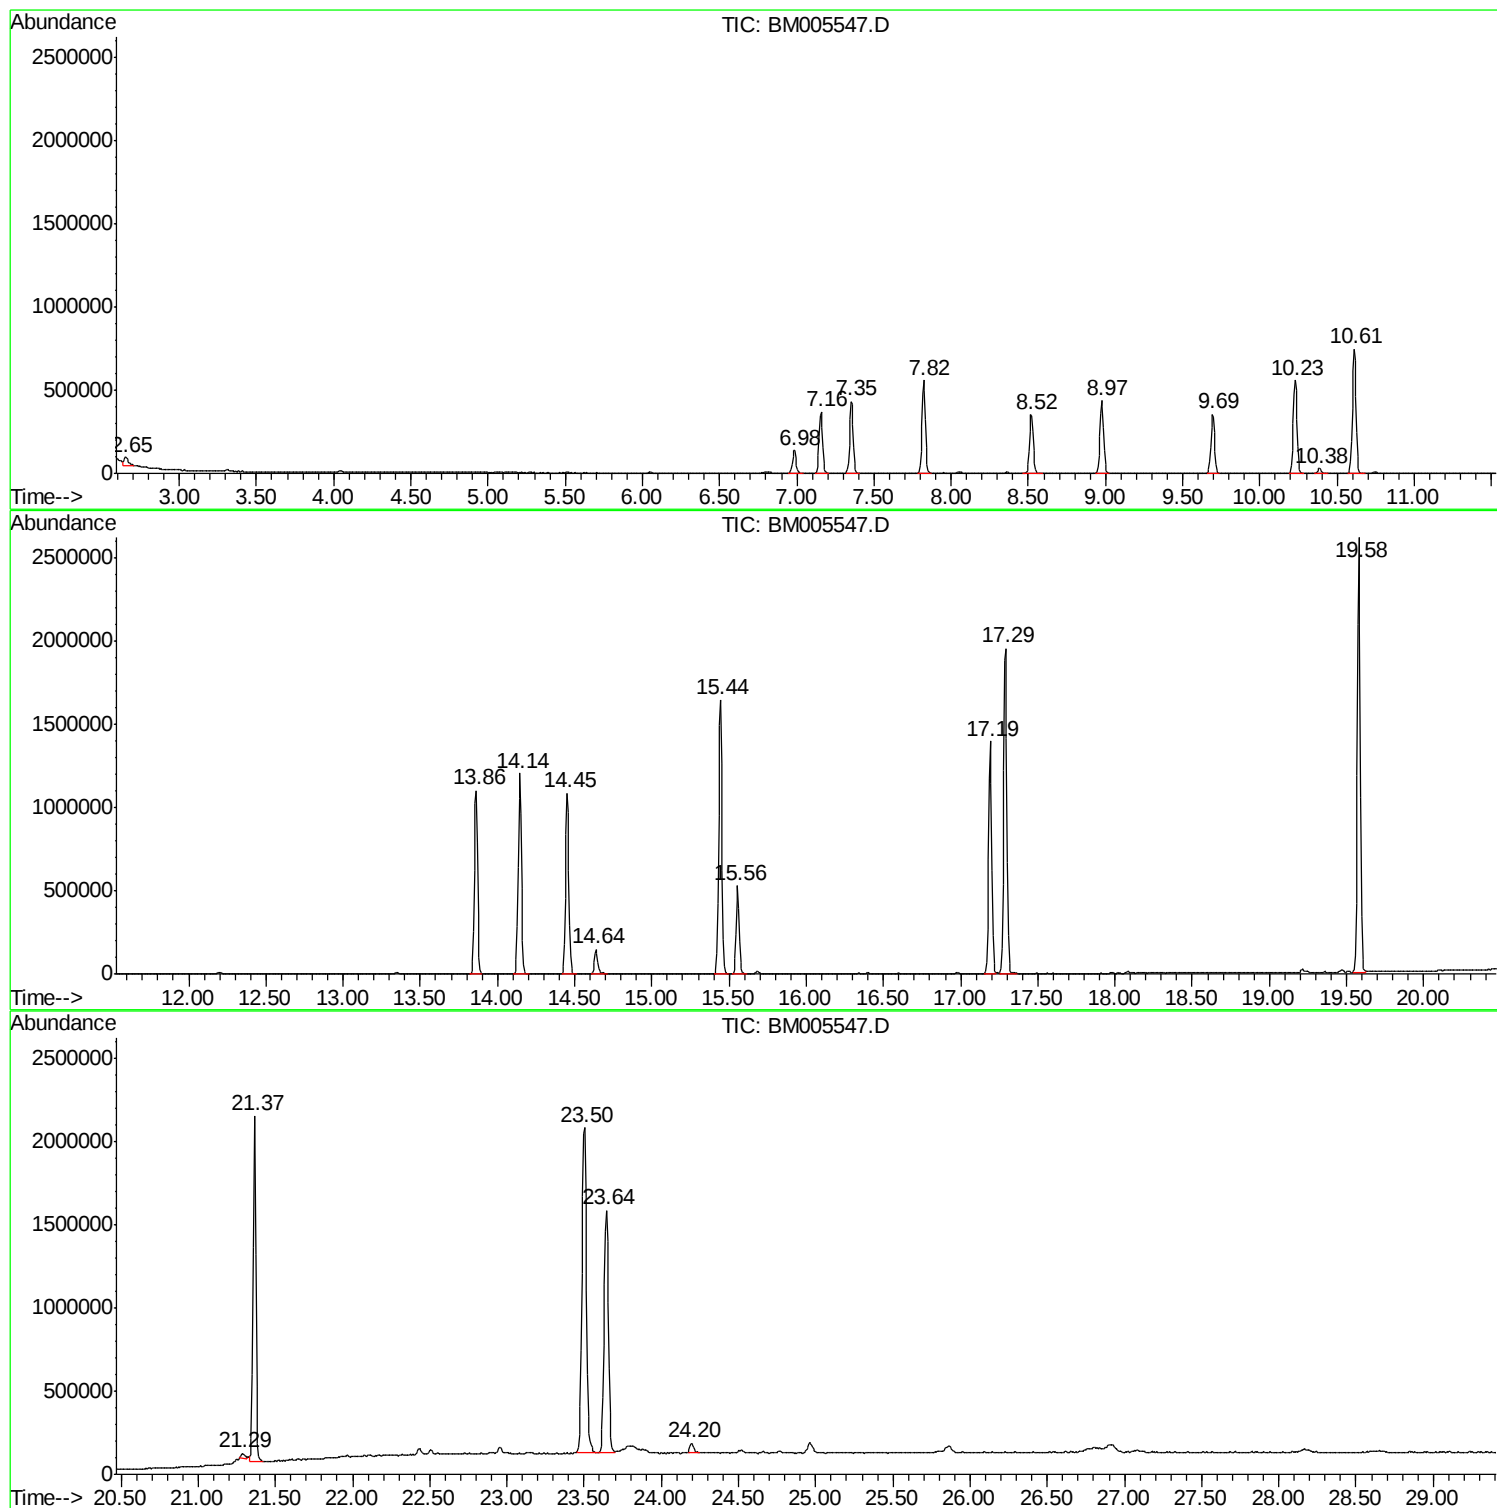

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM052016\
Data File : BM005547.D
Acq On : 21 May 2016 08:36
Operator : UM/SJ
Sample : H3058-18
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BD3F3

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM052016.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM052016\
Data File : BM005547.D
Acq On : 21 May 2016 08:36
Operator : UM/SJ
Sample : H3058-18
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BD3F3

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM052016.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc