

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM052019\
 Data File : BM020448.D
 Acq On : 21 May 2019 03:00
 Operator : JU/SJ
 Sample : K2788-01
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 A5188

Quant Time: May 21 07:49:48 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM051619MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue May 21 07:44:16 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.73	152	91347	20.00	ng/ul	0.00
18) Naphthalene-d8	10.52	136	338490	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.38	164	196294	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.13	188	457536	20.00	ng/ul	0.00
77) Chrysene-d12	21.33	240	481831	20.00	ng/ul	0.00
85) Perylene-d12	23.60	264	537846	20.00	ng/ul	-0.02

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.22	96	13670	5.52	ng/uL	0.00
5) Phenol-d5	6.90	99	215191	29.53	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.07	67	134789	29.09	ng/ul	0.00
9) 2-Chlorophenol-d4	7.26	132	166263	31.11	ng/ul	0.00
13) 4-Methylphenol-d8	8.43	113	154766	29.16	ng/ul	0.00
19) Nitrobenzene-d5	8.90	128	71351	32.40	ng/ul	0.00
22) 2-Nitrophenol-d4	9.61	143	77734	32.00	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.15	165	155524	30.28	ng/ul	0.00
29) 4-Chloroaniline-d4	10.67	131	172594	32.53	ng/ul	0.00
43) Dimethylphthalate-d6	13.79	166	456789	32.34	ng/ul	0.00
46) Acenaphthylene-d8	14.07	160	575124	32.56	ng/ul	0.00
51) 4-Nitrophenol-d4	14.60	143	41477	20.23	ng/ul	0.00
57) Fluorene-d10	15.37	176	399546	31.81	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.52	200	32304	12.40	ng/ul	-0.01
70) Anthracene-d10	17.23	188	639334	32.58	ng/ul	0.00
78) Pyrene-d10	19.53	212	768438	33.11	ng/ul	0.00
89) Benzo(a)pyrene-d12	23.46	264	814657	33.33	ng/ul	-0.02


Target Compounds	R.T.	QIon	Response	Conc	Units	Ovalue
44) Dimethylphthalate	13.84	163	181856	13.017	ng/ul	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM052019\
Data File : BM020448.D
Acq On : 21 May 2019 03:00
Operator : JU/SJ
Sample : K2788-01
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
A5188

Quant Time: May 21 07:49:48 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM051619MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue May 21 07:44:16 2019
Response via : Initial Calibration

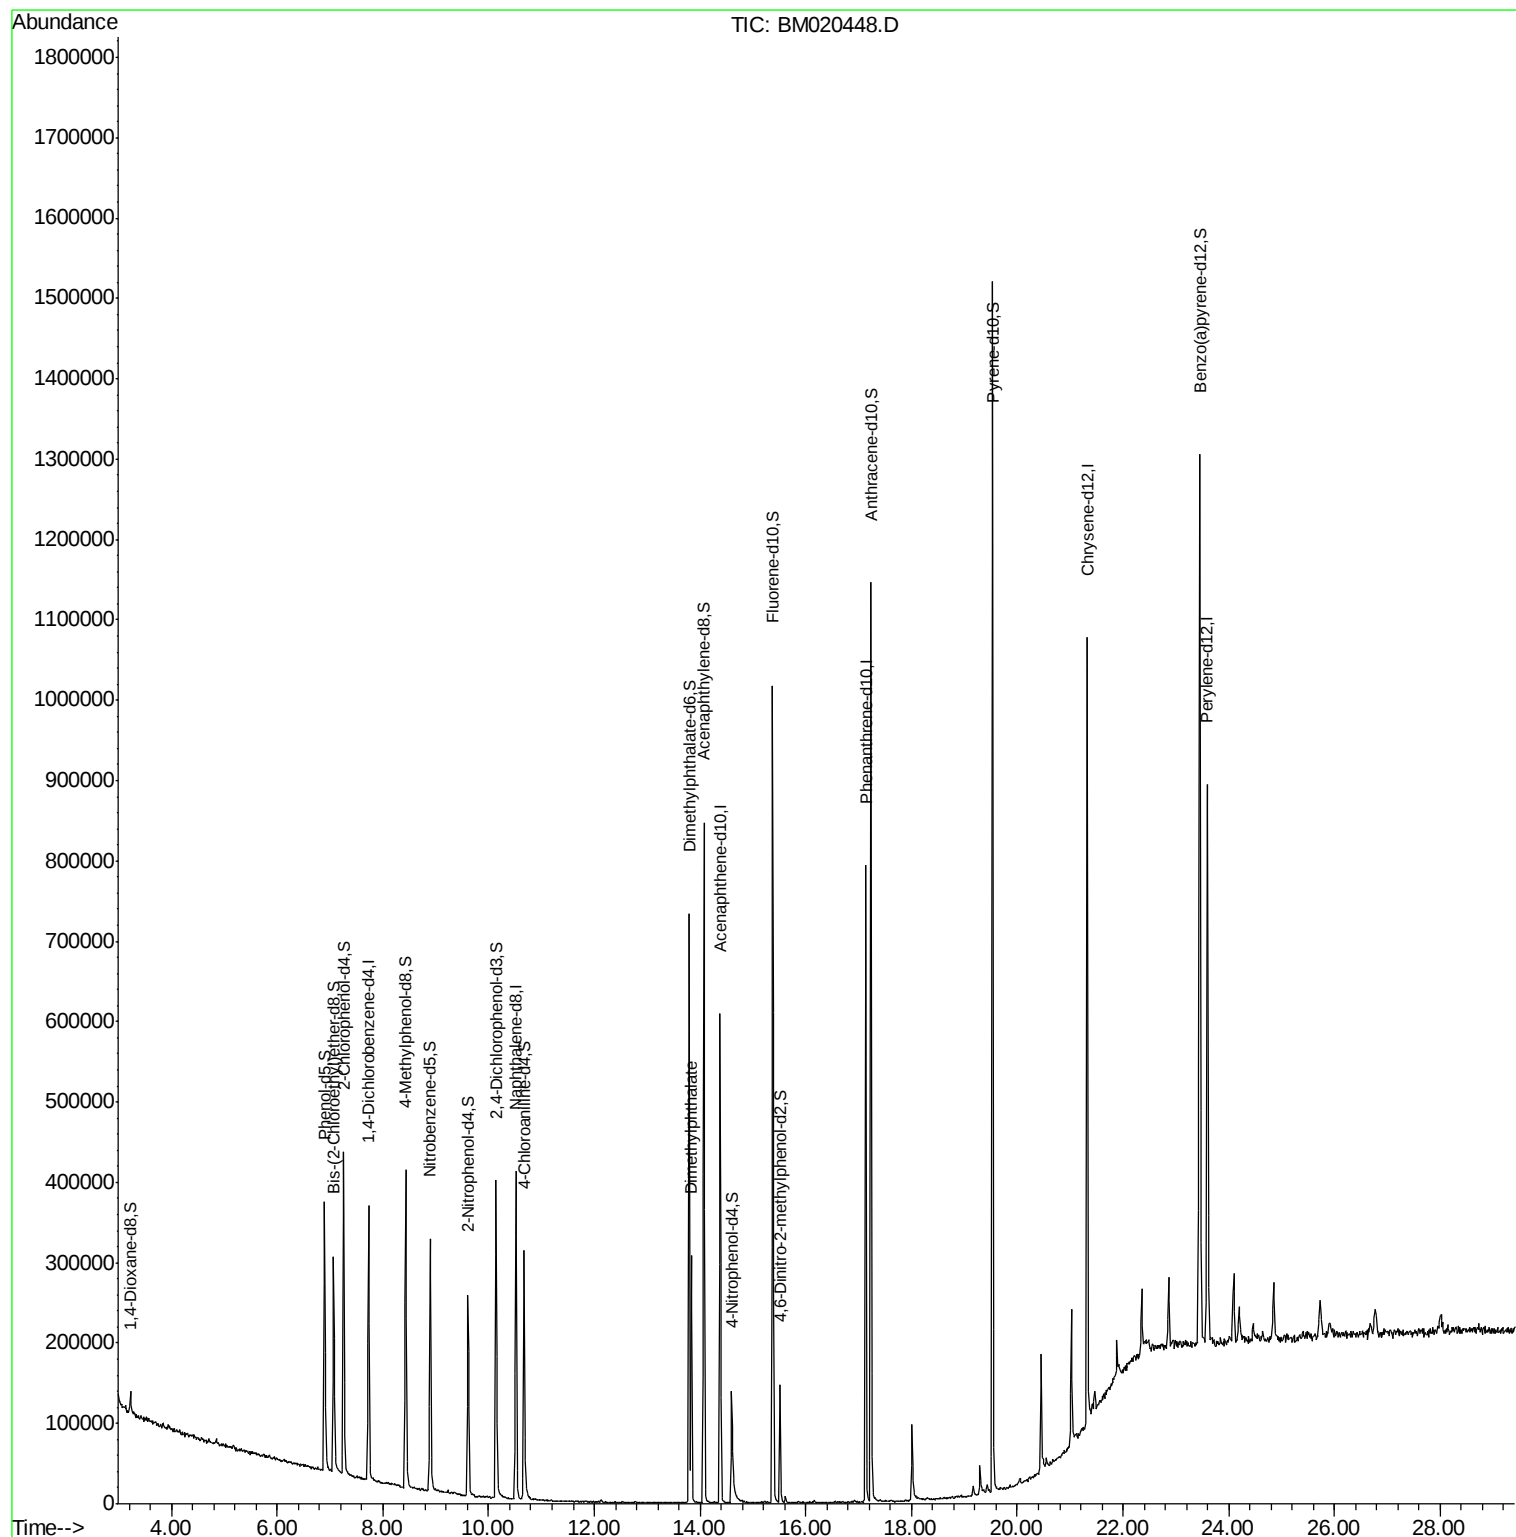

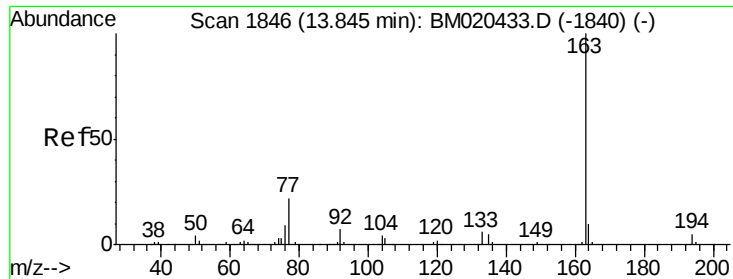

#44

Dimethylphthalate

Concen: 13.017 ng/ul

RT: 13.84 min Scan# 1845

Delta R.T. -0.01 min

Lab File: BM020448.D

Acq: 21 May 2019 03:00

Instrument :

BNA_M

ClientSampleId :

A5188


Tot Ion:163 Resp: 181856

Ion Ratio Lower Upper

163 100

194 4.4 3.3 4.9

164 9.8 8.0 12.0

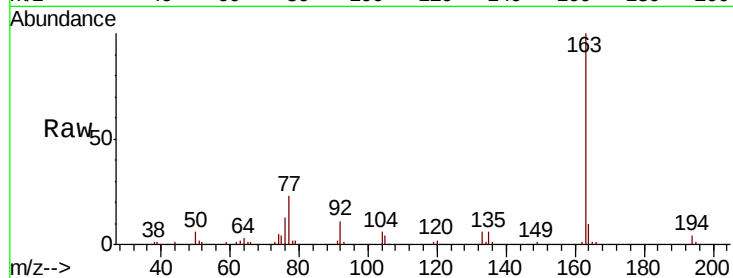

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

