

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM052020\
 Data File : BM026037.D
 Acq On : 20 May 2020 13:59
 Operator : MA/SJ
 Sample : L2653-01
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0AE0

Quant Time: May 20 14:30:19 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM051320MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed May 20 11:35:33 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.50	152	168802	20.00	ng/ul	0.00
18) Naphthalene-d8	10.26	136	721451	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.14	164	429278	20.00	ng/ul	0.00
62) Phenanthrene-d10	16.89	188	903030	20.00	ng/ul	0.00
78) Chrysene-d12	21.09	240	906686	20.00	ng/ul	0.00
86) Perylene-d12	23.21	264	943174	20.00	ng/ul	0.00

System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.08	96	25864	4.62	ng/uL	0.00
5) Phenol-d5	6.69	99	84509	5.52	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.85	67	265231	25.04	ng/ul	0.00
9) 2-Chlorophenol-d4	7.04	132	234181	19.54	ng/ul	0.00
13) 4-Methylphenol-d8	8.21	113	154251	13.37	ng/ul	0.00
19) Nitrobenzene-d5	8.65	128	143423	24.39	ng/ul	0.00
22) 2-Nitrophenol-d4	9.36	143	148478	25.52	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	9.89	165	249544	21.36	ng/ul	0.00
29) 4-Chloroaniline-d4	10.41	131	20400	1.72	ng/ul	0.00
44) Dimethylphthalate-d6	13.56	166	887749	25.79	ng/ul	0.00
47) Acenaphthylene-d8	13.83	160	1009224	24.75	ng/ul	0.00
52) 4-Nitrophenol-d4	14.36	143	26168	4.29	ng/ul	0.00
58) Fluorene-d10	15.14	176	789850	26.38	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.27	200	129405	24.58	ng/ul	0.00
71) Anthracene-d10	16.99	188	1365494	30.69	ng/ul	0.00
79) Pyrene-d10	19.29	212	1506399	32.34	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.08	264	1564428	31.16	ng/ul	0.00


Target Compounds					Ovalue	
45) Dimethylphthalate	13.61	163	115655	3.200	ng/ul	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM052020\
Data File : BM026037.D
Acq On : 20 May 2020 13:59
Operator : MA/SJ
Sample : L2653-01
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0AE0

Quant Time: May 20 14:30:19 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM051320MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed May 20 11:35:33 2020
Response via : Initial Calibration

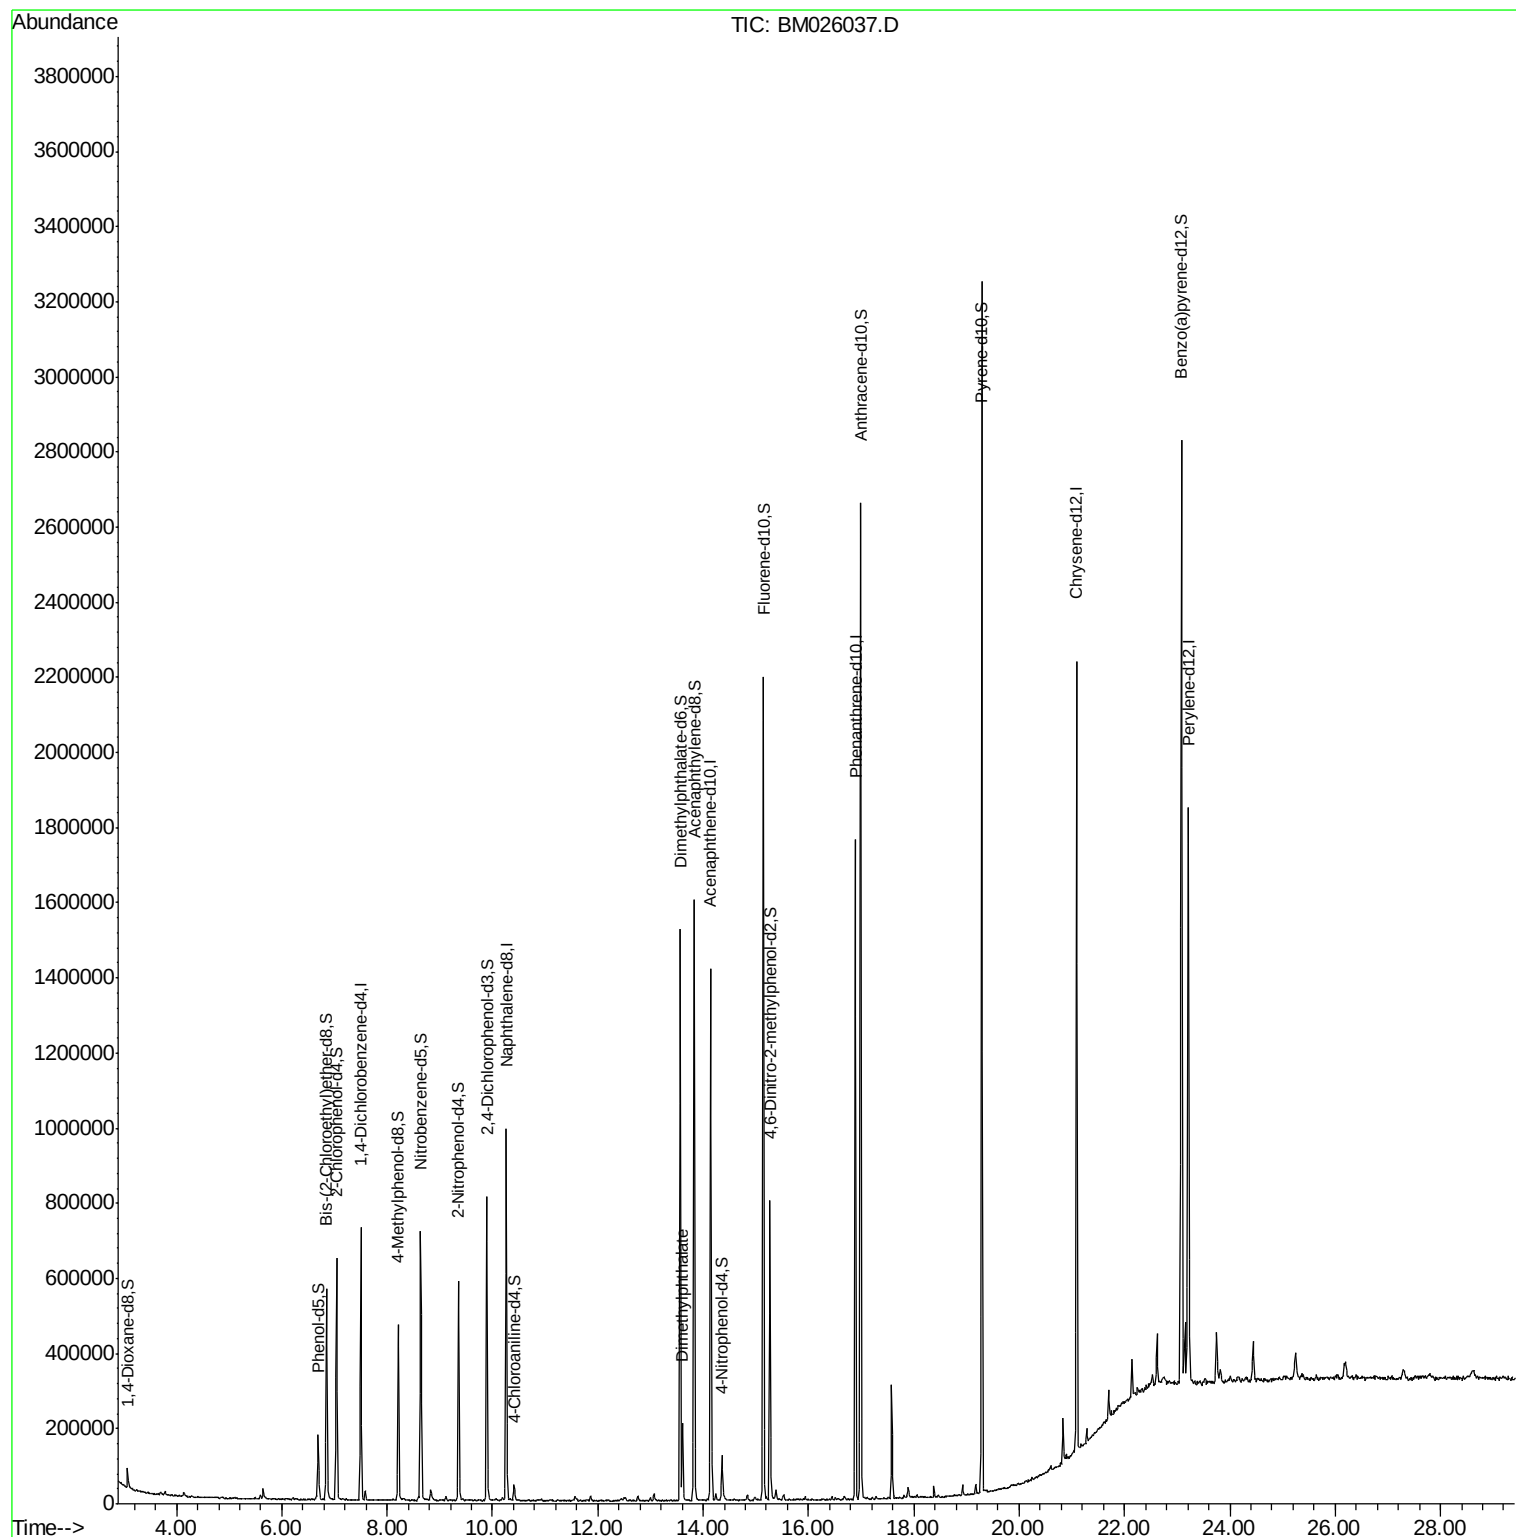

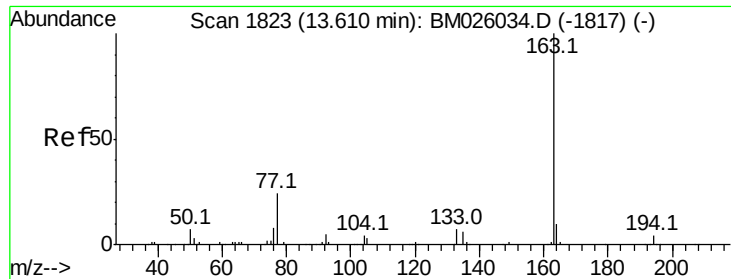

#45

Dimethylphthalate

Concen: 3.200 ng/ul

RT: 13.61 min Scan# 1823

Delta R.T. -0.00 min

Lab File: BM026037.D

Acq: 20 May 2020 13:59

Instrument :

BNA_M

ClientSampleId :

C0AE0


Tot Ion:163 Resp: 115655

Ion Ratio Lower Upper

163 100

194 4.4 3.2 4.8

164 10.5 8.0 12.0

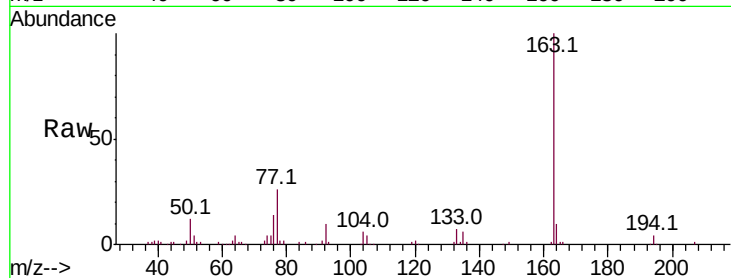

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

