

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM052020\
 Data File : BM026039.D
 Acq On : 20 May 2020 15:11
 Operator : MA/SJ
 Sample : L2653-04
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0AD9

Quant Time: May 20 15:49:40 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM051320MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed May 20 11:35:33 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.50	152	173581	20.00	ng/ul	0.00
18) Naphthalene-d8	10.26	136	729419	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.15	164	425546	20.00	ng/ul	0.00
62) Phenanthrene-d10	16.89	188	914150	20.00	ng/ul	0.00
78) Chrysene-d12	21.09	240	953384	20.00	ng/ul	0.00
86) Perylene-d12	23.22	264	1000149	20.00	ng/ul	0.00

System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.08	96	23115	4.02	ng/uL	0.00
5) Phenol-d5	6.69	99	91431	5.81	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.85	67	241529	22.17	ng/ul	0.00
9) 2-Chlorophenol-d4	7.04	132	227881	18.49	ng/ul	0.00
13) 4-Methylphenol-d8	8.21	113	166016	13.99	ng/ul	0.00
19) Nitrobenzene-d5	8.65	128	133139	22.39	ng/ul	0.00
22) 2-Nitrophenol-d4	9.36	143	141577	24.07	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	9.89	165	268060	22.70	ng/ul	0.00
29) 4-Chloroaniline-d4	10.41	131	15028	1.25	ng/ul	0.00
44) Dimethylphthalate-d6	13.56	166	878110	25.73	ng/ul	0.00
47) Acenaphthylene-d8	13.83	160	1025870	25.37	ng/ul	0.00
52) 4-Nitrophenol-d4	14.36	143	33138	5.48	ng/ul	0.00
58) Fluorene-d10	15.15	176	760203	25.61	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.27	200	126892	23.81	ng/ul	0.00
71) Anthracene-d10	16.99	188	1177996	26.15	ng/ul	0.00
79) Pyrene-d10	19.29	212	1346338	27.49	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.09	264	1401858	26.33	ng/ul	0.00


Target Compounds					Ovalue	
45) Dimethylphthalate	13.61	163	95450	2.664	ng/ul	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM052020\
Data File : BM026039.D
Acq On : 20 May 2020 15:11
Operator : MA/SJ
Sample : L2653-04
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0AD9

Quant Time: May 20 15:49:40 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM051320MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed May 20 11:35:33 2020
Response via : Initial Calibration

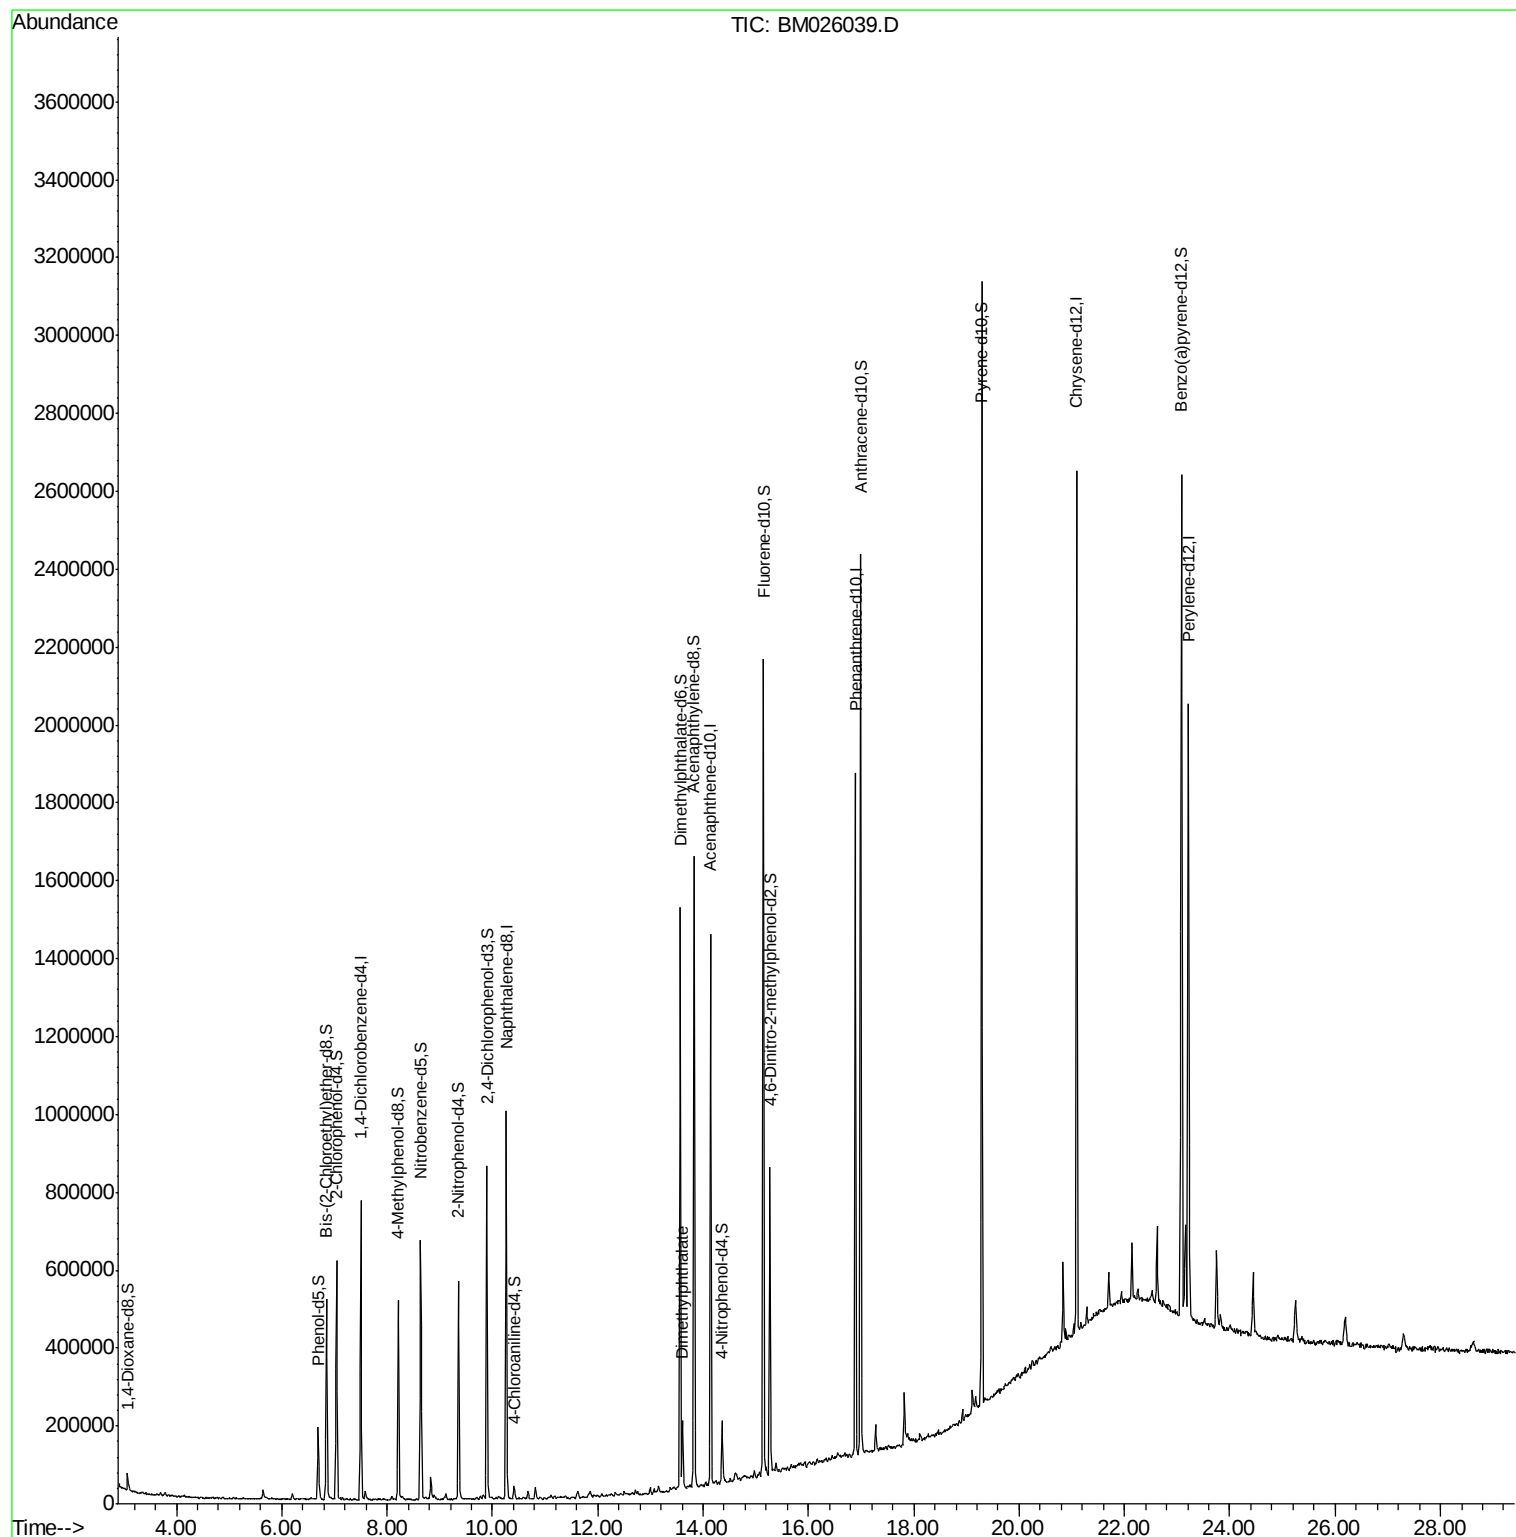

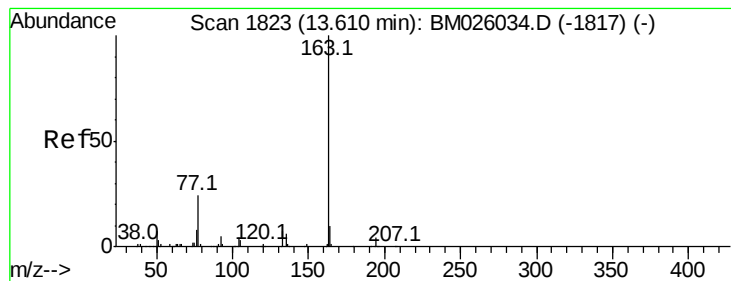

#45

Dimethylphthalate

Concen: 2.664 ng/ul

RT: 13.61 min Scan# 1823

Delta R.T. 0.00 min

Lab File: BM026039.D

Acq: 20 May 2020 15:11

Instrument :

BNA_M

ClientSampleId :

C0AD9


Tot Ion:163 Resp: 95450

Ion Ratio Lower Upper

163 100

194 4.3 3.2 4.8

164 10.3 8.0 12.0

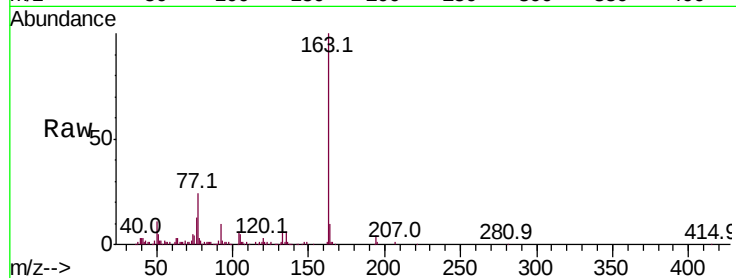

Abundance

Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

