

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM052020\
 Data File : BM026042.D
 Acq On : 20 May 2020 17:00
 Operator : MA/SJ
 Sample : L2681-09DL 50X
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C5CB1DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM051320MA.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.781	149	152	156	rVB5	9685	12471	0.57%	0.101%
2	3.928	176	177	180	rVB3	4199	3067	0.14%	0.025%
3	3.993	187	188	191	rVB3	3313	2253	0.10%	0.018%
4	4.116	208	209	213	rBV3	3189	2555	0.12%	0.021%
5	4.598	289	291	294	rBV4	2387	3727	0.17%	0.030%
6	4.846	332	333	337	rBV4	2013	2311	0.11%	0.019%
7	5.140	379	383	386	rBV5	1661	2615	0.12%	0.021%
8	5.434	429	433	436	rBV6	1676	2359	0.11%	0.019%
9	5.622	463	465	469	rVB4	3008	2834	0.13%	0.023%
10	5.934	514	518	521	rVB5	1728	2519	0.11%	0.020%
11	6.634	634	637	639	rBV4	3072	2706	0.12%	0.022%
12	6.698	644	648	653	rVV7	3388	6754	0.31%	0.055%
13	6.757	656	658	661	rBV4	2556	2679	0.12%	0.022%
14	6.851	670	674	681	rBV2	10753	18456	0.84%	0.150%
15	7.040	700	706	712	rBV4	11417	20393	0.93%	0.166%
16	7.169	724	728	731	rBV5	2214	3895	0.18%	0.032%
17	7.263	740	744	748	rVB5	2493	2756	0.13%	0.022%
18	7.498	776	784	792	rBV	611065	946227	43.10%	7.685%
19	8.222	902	907	910	rBV6	7423	11212	0.51%	0.091%
20	8.651	974	980	987	rBV2	12448	22382	1.02%	0.182%
21	9.169	1065	1068	1070	rBV4	2983	2776	0.13%	0.023%
22	9.363	1096	1101	1107	rVB7	8506	13690	0.62%	0.111%
23	9.910	1189	1194	1198	rBV6	10016	16700	0.76%	0.136%
24	10.263	1246	1254	1261	rBV	831788	1333440	60.74%	10.829%
25	11.398	1443	1447	1450	rVB6	1773	2365	0.11%	0.019%
26	11.504	1460	1465	1466	rBV4	2753	3531	0.16%	0.029%
27	11.610	1478	1483	1486	rBV6	3290	5029	0.23%	0.041%
28	11.669	1489	1493	1499	rBV6	3284	7063	0.32%	0.057%
29	12.110	1563	1568	1569	rBV4	2018	2232	0.10%	0.018%
30	12.333	1602	1606	1609	rBV4	1559	2211	0.10%	0.018%
31	12.469	1625	1629	1632	rBV4	2218	3095	0.14%	0.025%
32	13.110	1734	1738	1741	rBV4	1649	2942	0.13%	0.024%
33	13.569	1811	1816	1821	rBV	28917	38864	1.77%	0.316%
34	13.627	1821	1826	1830	rVB5	9641	17118	0.78%	0.139%

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM052020\
Data File : BM026042.D
Acq On : 20 May 2020 17:00
Operator : MA/SJ
Sample : L2681-09DL 50X
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C5CB1DL

Integration Parameters: LSCINT.P

Integrator: RTE
Smoothing : OFF
Sampling : 1
Start Thrs: 0.2
Stop Thrs : 0
Filtering: 5
Min Area: 0.1 % of largest Peak
Max Peaks: 100
Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM051320MA.M
Title : SVOA CALIBRATION

35	13.739	1841	1845	1850	rBV7	2259	4463	0.20%	0.036%
36	13.833	1853	1861	1868	rVV	32012	50784	2.31%	0.412%
37	14.145	1907	1914	1926	rVB	1171896	1693131	77.13%	13.750%
38	14.704	2006	2009	2013	rVB6	5691	6210	0.28%	0.050%
39	14.780	2016	2022	2027	rBV3	28040	41808	1.90%	0.340%
40	15.051	2064	2068	2070	rBV4	1982	2232	0.10%	0.018%
41	15.145	2078	2084	2089	rBV	46607	65433	2.98%	0.531%
42	15.198	2089	2093	2098	rVB2	10174	11952	0.54%	0.097%
43	15.298	2103	2110	2115	rVB8	9653	20018	0.91%	0.163%
44	15.386	2123	2125	2129	rVB3	2629	2810	0.13%	0.023%
45	15.868	2205	2207	2212	rBV5	3931	5734	0.26%	0.047%
46	16.192	2258	2262	2267	rBV8	2903	3941	0.18%	0.032%
47	16.274	2273	2276	2279	rBV4	2048	2633	0.12%	0.021%
48	16.445	2302	2305	2311	rVB6	6842	8721	0.40%	0.071%
49	16.551	2317	2323	2339	rBV	989873	1311011	59.72%	10.647%
50	16.674	2342	2344	2348	rVB4	5781	8959	0.41%	0.073%
51	16.768	2358	2360	2363	rVB3	2257	2273	0.10%	0.018%
52	16.892	2375	2381	2391	rBV	1466515	2004238	91.30%	16.277%
53	16.992	2393	2398	2410	rVB2	47965	73521	3.35%	0.597%
54	17.521	2484	2488	2491	rVB5	3811	5510	0.25%	0.045%
55	18.286	2616	2618	2621	rBV4	1841	2680	0.12%	0.022%
56	18.462	2644	2648	2650	rBV5	3893	4866	0.22%	0.040%
57	19.227	2776	2778	2780	rBV3	3546	2870	0.13%	0.023%
58	19.292	2784	2789	2793	rVV2	54611	77069	3.51%	0.626%
59	21.092	3090	3095	3104	rBV	1775070	2195235	100.00%	17.828%
60	23.209	3449	3455	3464	rVB	1266438	2180030	99.31%	17.705%


Sum of corrected areas: 12313359

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM052020\
Data File : BM026042.D
Acq On : 20 May 2020 17:00
Operator : MA/SJ
Sample : L2681-09DL 50X
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C5CB1DL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM051320MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

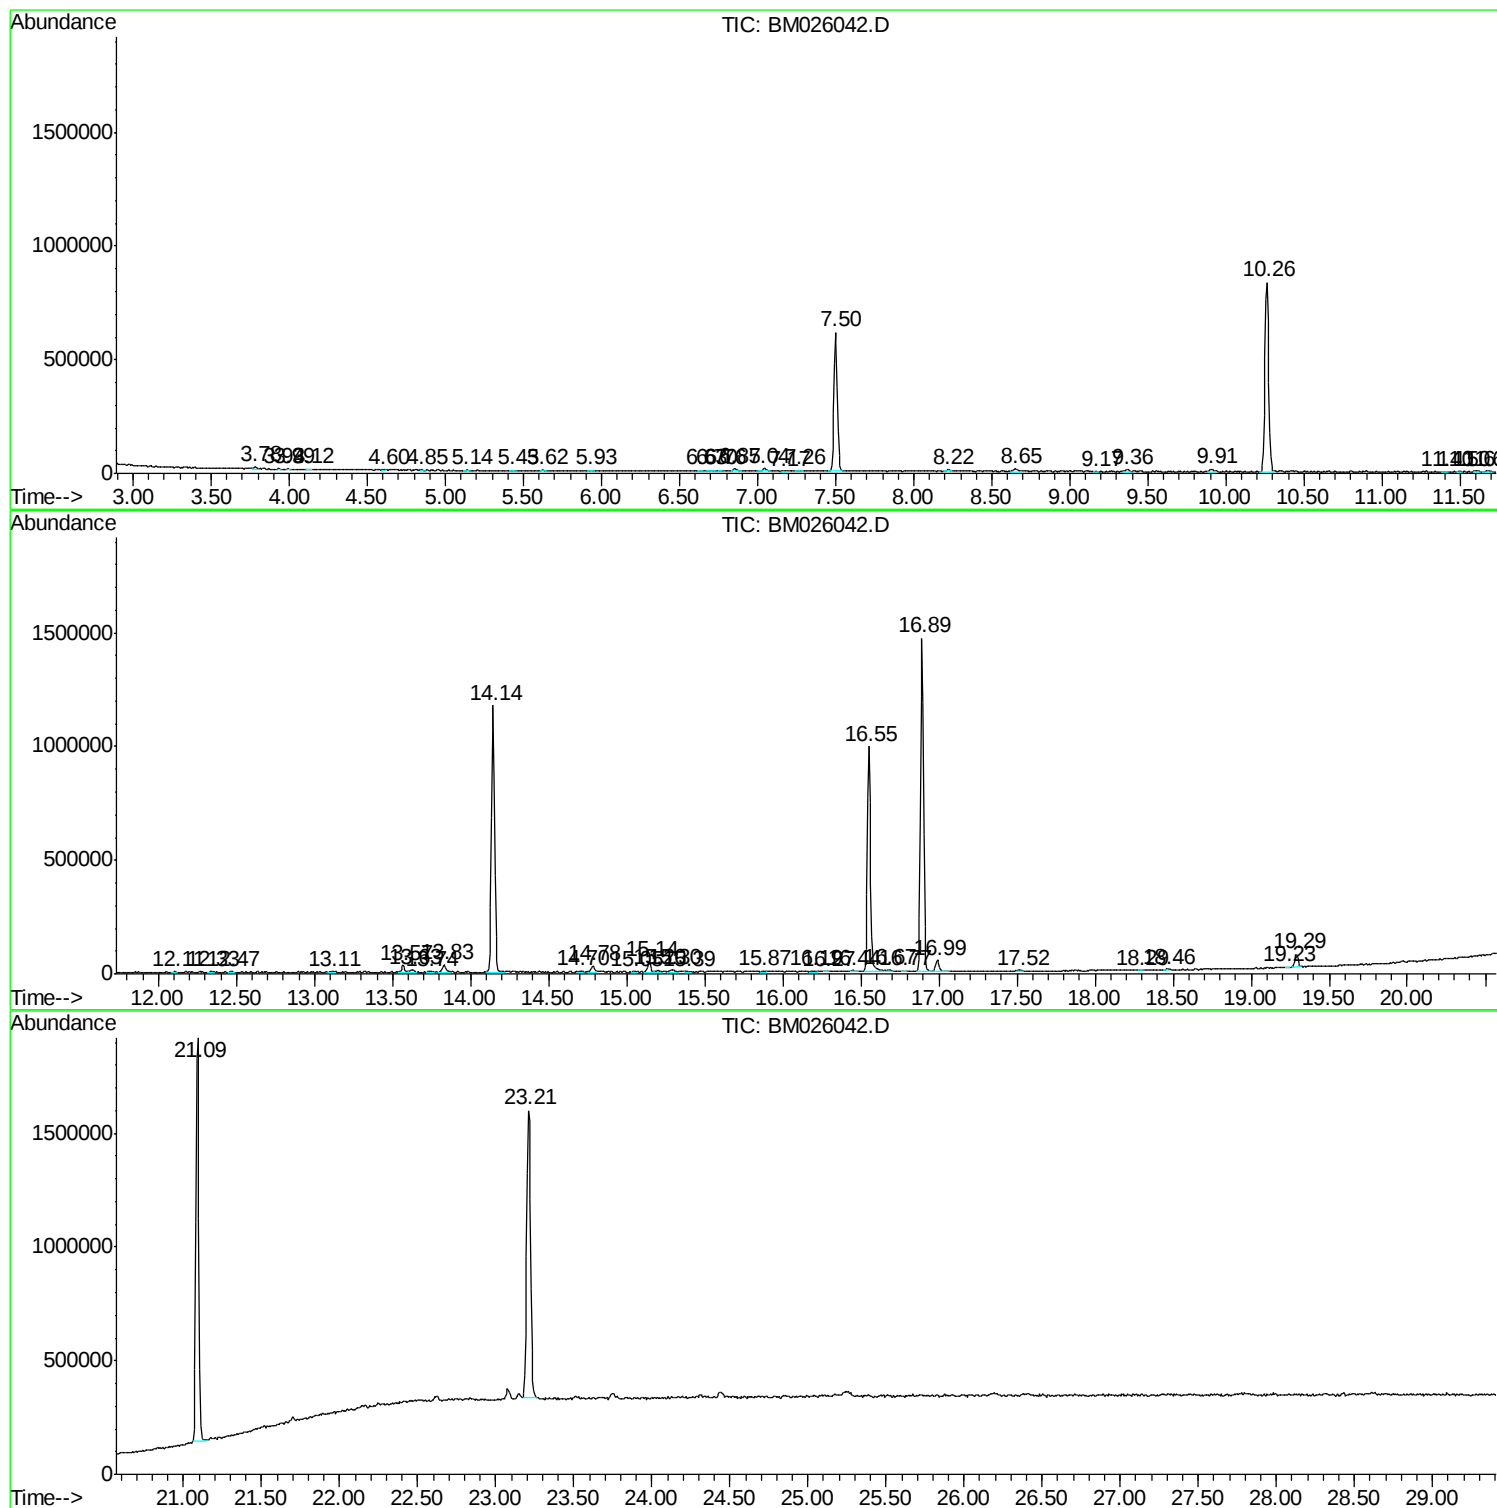

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM052020\
Data File : BM026042.D
Acq On : 20 May 2020 17:00
Operator : MA/SJ
Sample : L2681-09DL 50X
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C5CB1DL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM051320MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM052020\
Data File : BM026042.D
Acq On : 20 May 2020 17:00
Operator : MA/SJ
Sample : L2681-09DL 50X
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C5CB1DL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM051320MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	---Internal Standard---
					# RT Resp Conc