

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM052020\
 Data File : BM026043.D
 Acq On : 20 May 2020 17:36
 Operator : MA/SJ
 Sample : L2681-07DL 20X
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C5CA9DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM051320MA.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.551	111	113	116	rVB3	3363	2294	0.10%	0.017%
2	3.669	132	133	139	rBV6	2723	4373	0.20%	0.033%
3	3.781	149	152	160	rVB4	10646	16826	0.76%	0.125%
4	4.634	293	297	298	rBV3	2316	2725	0.12%	0.020%
5	4.663	298	302	305	rBV7	1415	2353	0.11%	0.018%
6	5.163	384	387	388	rBV3	2782	2741	0.12%	0.020%
7	5.222	396	397	399	rBV	2667	2429	0.11%	0.018%
8	5.828	498	500	503	rVB4	2243	2619	0.12%	0.019%
9	5.934	514	518	521	rBV5	1876	3291	0.15%	0.024%
10	6.316	580	583	585	rBV4	1994	2253	0.10%	0.017%
11	6.698	643	648	654	rVB4	6572	12632	0.57%	0.094%
12	6.851	670	674	681	rBV	26496	43904	1.98%	0.327%
13	6.934	687	688	696	rVB7	2463	4070	0.18%	0.030%
14	7.040	701	706	712	rVB3	25688	45496	2.05%	0.339%
15	7.498	778	784	796	rBV	612766	934931	42.21%	6.958%
16	7.745	823	826	829	rVB5	2213	2232	0.10%	0.017%
17	7.875	843	848	850	rBV3	2649	3891	0.18%	0.029%
18	8.216	901	906	912	rBV4	16662	28176	1.27%	0.210%
19	8.598	967	971	972	rVV2	2585	2392	0.11%	0.018%
20	8.645	974	979	990	rVB2	29576	63688	2.88%	0.474%
21	8.939	1026	1029	1035	rVB6	3113	4718	0.21%	0.035%
22	9.110	1056	1058	1064	rVB5	2997	4417	0.20%	0.033%
23	9.363	1096	1101	1109	rVB2	21577	38453	1.74%	0.286%
24	9.481	1117	1121	1127	rVB8	3806	6670	0.30%	0.050%
25	9.675	1151	1154	1159	rVB4	5502	8531	0.39%	0.063%
26	9.904	1187	1193	1202	rBV2	28585	56855	2.57%	0.423%
27	9.986	1204	1207	1211	rVV5	1877	2333	0.11%	0.017%
28	10.051	1215	1218	1224	rVB5	2019	3942	0.18%	0.029%
29	10.104	1224	1227	1229	rBV3	2374	2521	0.11%	0.019%
30	10.263	1246	1254	1261	rBV	817692	1308969	59.09%	9.742%
31	10.328	1261	1265	1269	rVV6	4484	8554	0.39%	0.064%
32	10.392	1269	1276	1279	rVV6	3579	5427	0.25%	0.040%
33	10.639	1314	1318	1323	rBV6	2637	4633	0.21%	0.034%
34	10.727	1331	1333	1338	rVB6	3010	3433	0.15%	0.026%

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM052020\
 Data File : BM026043.D
 Acq On : 20 May 2020 17:36
 Operator : MA/SJ
 Sample : L2681-07DL 20X
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C5CA9DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM051320MA.M
 Title : SVOA CALIBRATION

35	10.845	1349	1353	1356	rBV6	4613	7679	0.35%	0.057%
36	10.886	1356	1360	1365	rVB7	4823	8599	0.39%	0.064%
37	11.375	1439	1443	1449	rVB8	3249	5897	0.27%	0.044%
38	11.492	1459	1463	1467	rBV7	4736	8065	0.36%	0.060%
39	11.563	1470	1475	1477	rBV5	2177	3131	0.14%	0.023%
40	11.598	1477	1481	1485	rVV6	6020	9365	0.42%	0.070%
41	11.663	1487	1492	1499	rVB6	11054	21004	0.95%	0.156%
42	11.780	1511	1512	1515	rVB3	2801	2350	0.11%	0.017%
43	11.833	1518	1521	1524	rBV5	2400	2886	0.13%	0.021%
44	11.910	1531	1534	1536	rVV4	2183	2503	0.11%	0.019%
45	11.951	1540	1541	1544	rVB3	3271	2640	0.12%	0.020%
46	11.992	1544	1548	1550	rBV4	1933	2248	0.10%	0.017%
47	12.051	1555	1558	1562	rVB5	1343	2235	0.10%	0.017%
48	12.110	1565	1568	1572	rBV5	4982	8295	0.37%	0.062%
49	12.216	1583	1586	1587	rBV3	2163	2267	0.10%	0.017%
50	12.233	1587	1589	1592	rVV4	3958	4728	0.21%	0.035%
51	12.274	1592	1596	1602	rVB8	6848	11184	0.50%	0.083%
52	12.345	1602	1608	1614	rBV5	6665	13896	0.63%	0.103%
53	12.404	1616	1618	1624	rBV7	3707	5126	0.23%	0.038%
54	12.469	1624	1629	1633	rBV6	4632	8265	0.37%	0.062%
55	12.627	1654	1656	1661	rBV5	4362	6155	0.28%	0.046%
56	12.680	1661	1665	1671	rVB7	6064	10421	0.47%	0.078%
57	12.757	1676	1678	1681	rVB4	2413	2854	0.13%	0.021%
58	13.063	1725	1730	1732	rBV6	1903	2604	0.12%	0.019%
59	13.110	1732	1738	1745	rVB9	5569	11575	0.52%	0.086%
60	13.192	1749	1752	1755	rVB5	3611	3909	0.18%	0.029%
61	13.274	1762	1766	1769	rBV4	3882	6479	0.29%	0.048%
62	13.316	1769	1773	1777	rVV5	5276	7501	0.34%	0.056%
63	13.568	1810	1816	1820	rBV	71013	98571	4.45%	0.734%
64	13.616	1820	1824	1832	rVB3	20369	39893	1.80%	0.297%
65	13.827	1854	1860	1867	rBV	74538	109414	4.94%	0.814%
66	14.145	1907	1914	1923	rVB	1138003	1663863	75.12%	12.384%
67	14.333	1942	1946	1951	rVV6	2532	3793	0.17%	0.028%
68	14.398	1951	1957	1959	rVV5	3335	6482	0.29%	0.048%
69	14.704	2003	2009	2012	rVV6	6912	8888	0.40%	0.066%
70	14.780	2018	2022	2033	rVB3	33106	50523	2.28%	0.376%
71	14.980	2053	2056	2060	rBV5	2002	3054	0.14%	0.023%

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM052020\
 Data File : BM026043.D
 Acq On : 20 May 2020 17:36
 Operator : MA/SJ
 Sample : L2681-07DL 20X
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C5CA9DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM051320MA.M
 Title : SVOA CALIBRATION

72	15.080	2069	2073	2077	rBV6	1680	2824	0.13%	0.021%
73	15.145	2077	2084	2089	rBV	105394	148805	6.72%	1.108%
74	15.198	2090	2093	2100	rVB3	8687	11194	0.51%	0.083%
75	15.274	2102	2106	2108	rBV4	13009	18461	0.83%	0.137%
76	15.362	2118	2121	2126	rVB5	4427	5876	0.27%	0.044%
77	15.668	2166	2173	2174	rBV7	1862	3105	0.14%	0.023%
78	15.868	2203	2207	2212	rBV4	13385	18970	0.86%	0.141%
79	16.074	2241	2242	2245	rBV3	2473	2511	0.11%	0.019%
80	16.445	2302	2305	2309	rVB4	5932	8169	0.37%	0.061%
81	16.551	2313	2323	2339	rBV	1167115	1616142	72.96%	12.028%
82	16.674	2339	2344	2350	rVB6	5891	9797	0.44%	0.073%
83	16.762	2356	2359	2363	rVB5	4598	5242	0.24%	0.039%
84	16.892	2373	2381	2389	rBV	1475615	1980793	89.42%	14.742%
85	16.992	2392	2398	2408	rVV2	108485	163504	7.38%	1.217%
86	17.515	2482	2487	2491	rVB5	7196	9151	0.41%	0.068%
87	17.556	2491	2494	2495	rBV3	2240	2676	0.12%	0.020%
88	17.827	2537	2540	2542	rBV4	2030	2525	0.11%	0.019%
89	17.874	2546	2548	2551	rBV4	2302	2515	0.11%	0.019%
90	17.998	2568	2569	2573	rBV4	1702	2306	0.10%	0.017%
91	18.203	2603	2604	2607	rBV3	2202	2469	0.11%	0.018%
92	18.233	2607	2609	2612	rBV3	3107	4172	0.19%	0.031%
93	18.298	2619	2620	2623	rBV3	2814	2427	0.11%	0.018%
94	18.462	2646	2648	2653	rVB6	5422	7024	0.32%	0.052%
95	18.668	2679	2683	2684	rBV4	3827	5045	0.23%	0.038%
96	19.021	2741	2743	2744	rVB2	4534	2335	0.11%	0.017%
97	19.292	2783	2789	2796	rBV	136920	187700	8.47%	1.397%
98	21.092	3090	3095	3100	rBV	1744831	2184085	98.60%	16.256%
99	23.209	3450	3455	3467	rVB2	1275787	2215035	100.00%	16.486%


Sum of corrected areas: 13435972

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM052020\
Data File : BM026043.D
Acq On : 20 May 2020 17:36
Operator : MA/SJ
Sample : L2681-07DL 20X
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampled :
C5CA9DL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM051320MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

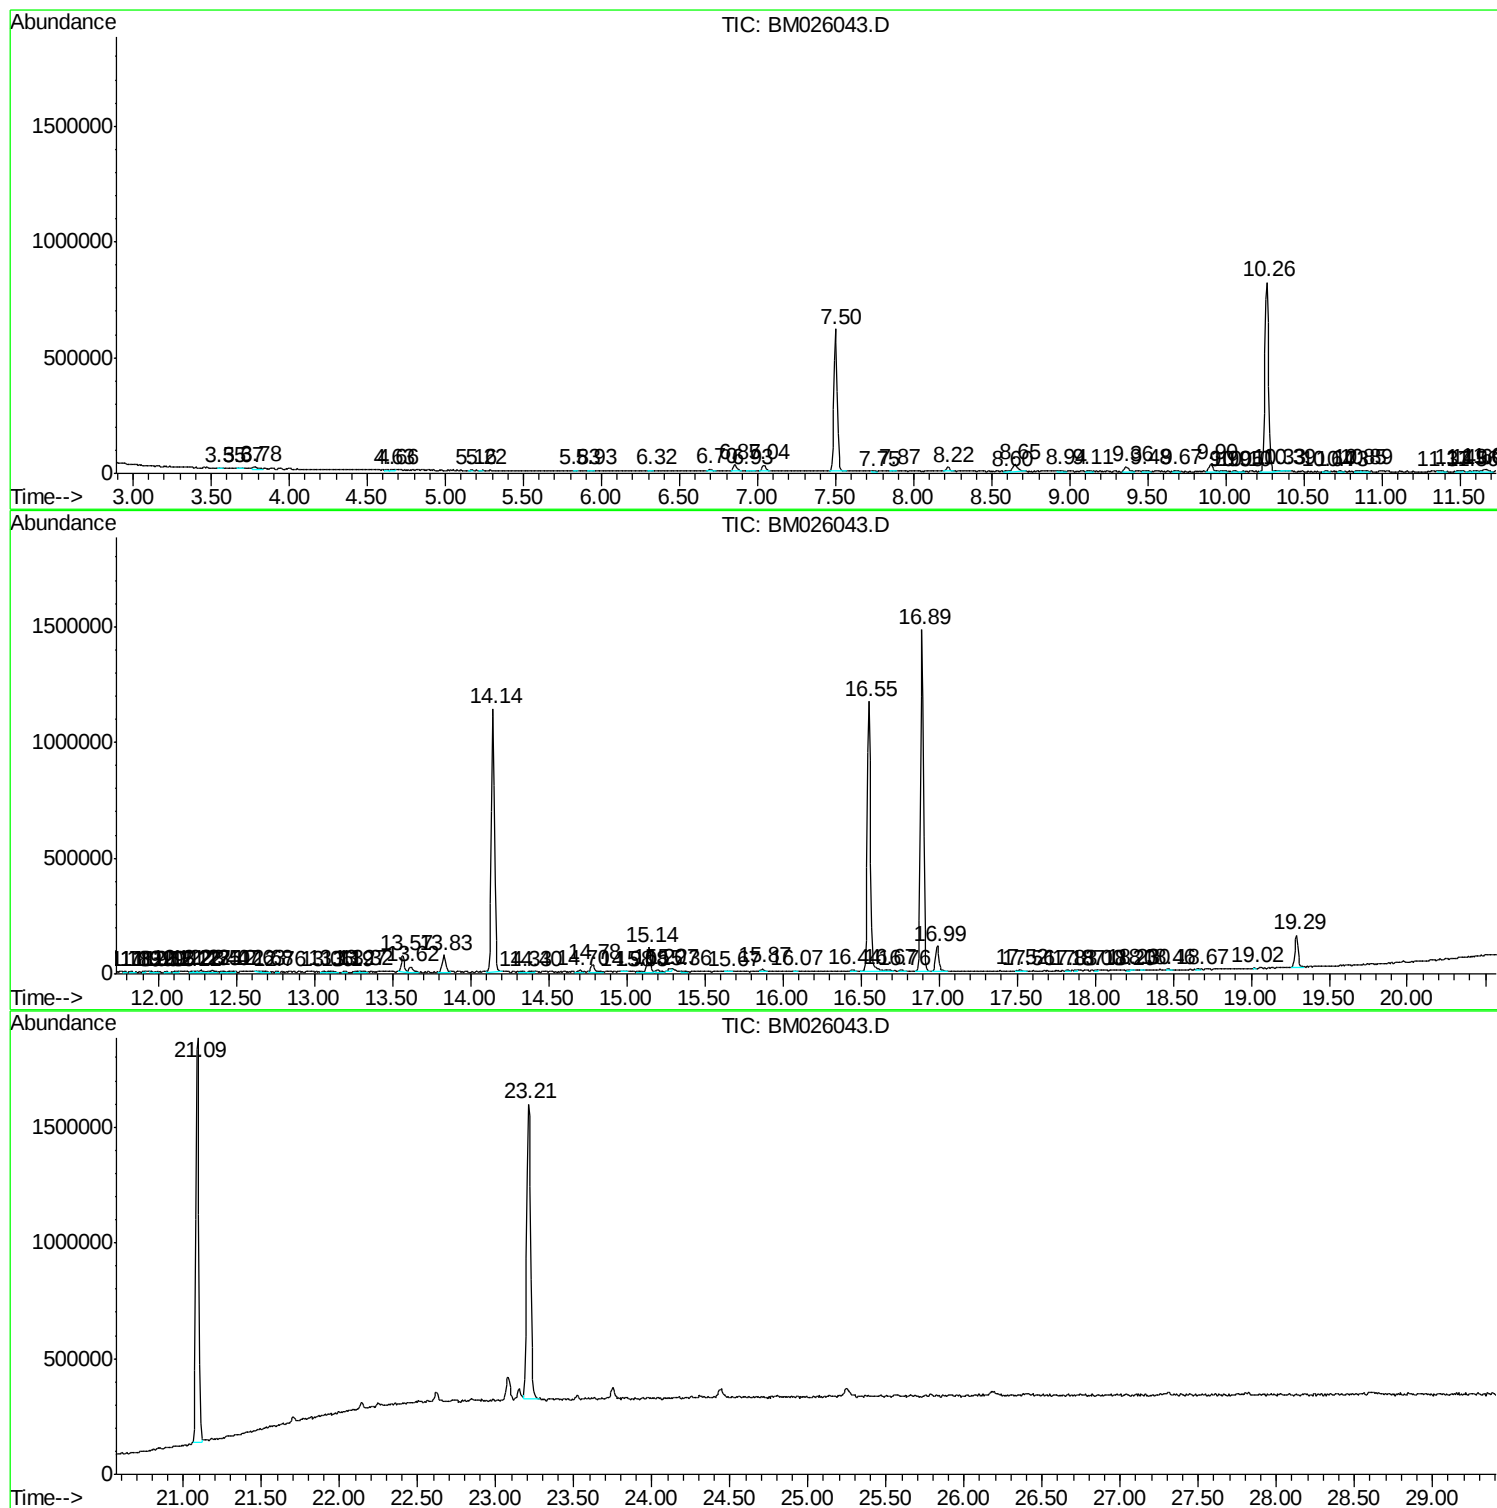

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM052020\
Data File : BM026043.D
Acq On : 20 May 2020 17:36
Operator : MA/SJ
Sample : L2681-07DL 20X
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C5CA9DL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM051320MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM052020\
Data File : BM026043.D
Acq On : 20 May 2020 17:36
Operator : MA/SJ
Sample : L2681-07DL 20X
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C5CA9DL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM051320MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	---Internal Standard---
					# RT Resp Conc