

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM052020\
 Data File : BM026044.D
 Acq On : 20 May 2020 18:12
 Operator : MA/SJ
 Sample : L2681-08DL2 50X
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C5CB0DL2

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM051320MA.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.334	74	76	79	rVB3	3818	3581	0.14%	0.025%
2	3.781	148	152	157	rVB2	8610	11897	0.47%	0.083%
3	4.210	223	225	229	rVB4	3467	3299	0.13%	0.023%
4	4.787	320	323	324	rBV3	3187	3559	0.14%	0.025%
5	4.904	341	343	345	rBV3	2700	2776	0.11%	0.019%
6	5.334	412	416	417	rBV3	1848	2618	0.10%	0.018%
7	5.545	450	452	459	rBV8	1814	3562	0.14%	0.025%
8	6.698	646	648	652	rBV4	2696	3378	0.13%	0.024%
9	6.857	669	675	681	rBV	9324	17540	0.69%	0.122%
10	7.045	699	707	716	rBV3	11454	22602	0.89%	0.157%
11	7.498	777	784	794	rBV	660508	1000596	39.36%	6.966%
12	8.222	902	907	914	rVV9	6824	12922	0.51%	0.090%
13	8.439	940	944	949	rVB7	1770	3161	0.12%	0.022%
14	8.575	963	967	971	rBV3	1742	2944	0.12%	0.020%
15	8.651	975	980	987	rVB2	12274	21950	0.86%	0.153%
16	8.945	1029	1030	1035	rVB4	2209	2565	0.10%	0.018%
17	9.363	1095	1101	1105	rBV5	7500	12373	0.49%	0.086%
18	9.910	1188	1194	1198	rBV7	9025	17705	0.70%	0.123%
19	10.157	1231	1236	1241	rBV7	1355	2757	0.11%	0.019%
20	10.263	1247	1254	1265	rBV	889111	1428149	56.17%	9.943%
21	10.427	1278	1282	1289	rVB8	2308	3635	0.14%	0.025%
22	10.898	1357	1362	1365	rVB7	2021	3152	0.12%	0.022%
23	11.604	1479	1482	1487	rBV4	3345	4984	0.20%	0.035%
24	12.168	1574	1578	1581	rBV6	1536	2644	0.10%	0.018%
25	12.886	1693	1700	1704	rBV7	1952	3420	0.13%	0.024%
26	13.568	1810	1816	1820	rBV	31942	43528	1.71%	0.303%
27	13.627	1820	1826	1831	rVB6	11254	19356	0.76%	0.135%
28	13.827	1855	1860	1867	rBV	30000	47049	1.85%	0.328%
29	14.145	1907	1914	1921	rBV	1258044	1816898	71.46%	12.649%
30	14.192	1921	1922	1926	rVB4	3963	3457	0.14%	0.024%
31	14.698	2005	2008	2014	rVB4	8193	11574	0.46%	0.081%
32	14.780	2017	2022	2028	rVB	50263	72098	2.84%	0.502%
33	15.086	2071	2074	2077	rVB5	3559	4280	0.17%	0.030%
34	15.145	2077	2084	2089	rBV	42922	66711	2.62%	0.464%

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM052020\
 Data File : BM026044.D
 Acq On : 20 May 2020 18:12
 Operator : MA/SJ
 Sample : L2681-08DL2 50X
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C5CB0DL2

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM051320MA.M
 Title : SVOA CALIBRATION

35	15.198	2089	2093	2097	rVB	9217	11626	0.46%	0.081%
36	15.298	2104	2110	2117	rBV8	13480	27021	1.06%	0.188%
37	15.656	2167	2171	2173	rBV4	2106	3271	0.13%	0.023%
38	15.756	2183	2188	2189	rBV5	1943	2616	0.10%	0.018%
39	15.962	2220	2223	2225	rBV4	2710	3226	0.13%	0.022%
40	16.051	2233	2238	2239	rVB4	2342	2827	0.11%	0.020%
41	16.186	2257	2261	2264	rVB6	2332	2636	0.10%	0.018%
42	16.451	2302	2306	2309	rVB3	7466	7933	0.31%	0.055%
43	16.551	2317	2323	2339	rBV	1962055	2542484	100.00%	17.701%
44	16.680	2342	2345	2349	rVB3	8807	12060	0.47%	0.084%
45	16.892	2375	2381	2389	rVV	1602628	2151215	84.61%	14.977%
46	16.992	2392	2398	2407	rVB2	48996	75507	2.97%	0.526%
47	17.433	2471	2473	2478	rVV6	2375	3565	0.14%	0.025%
48	17.515	2483	2487	2491	rVB4	6030	8039	0.32%	0.056%
49	17.703	2515	2519	2523	rVB6	1919	2654	0.10%	0.018%
50	18.286	2615	2618	2619	rBV3	2739	2908	0.11%	0.020%
51	18.427	2638	2642	2644	rBV5	2655	3488	0.14%	0.024%
52	18.462	2644	2648	2650	rBV3	4939	6871	0.27%	0.048%
53	18.780	2698	2702	2705	rVV6	2890	5074	0.20%	0.035%
54	19.292	2784	2789	2796	rVB	57343	78899	3.10%	0.549%
55	21.086	3090	3094	3102	rBV	1881917	2353284	92.56%	16.384%
56	23.209	3449	3455	3465	rVB	1412020	2373550	93.36%	16.525%


Sum of corrected areas: 14363474

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM052020\
Data File : BM026044.D
Acq On : 20 May 2020 18:12
Operator : MA/SJ
Sample : L2681-08DL2 50X
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C5CB0DL2

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM051320MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

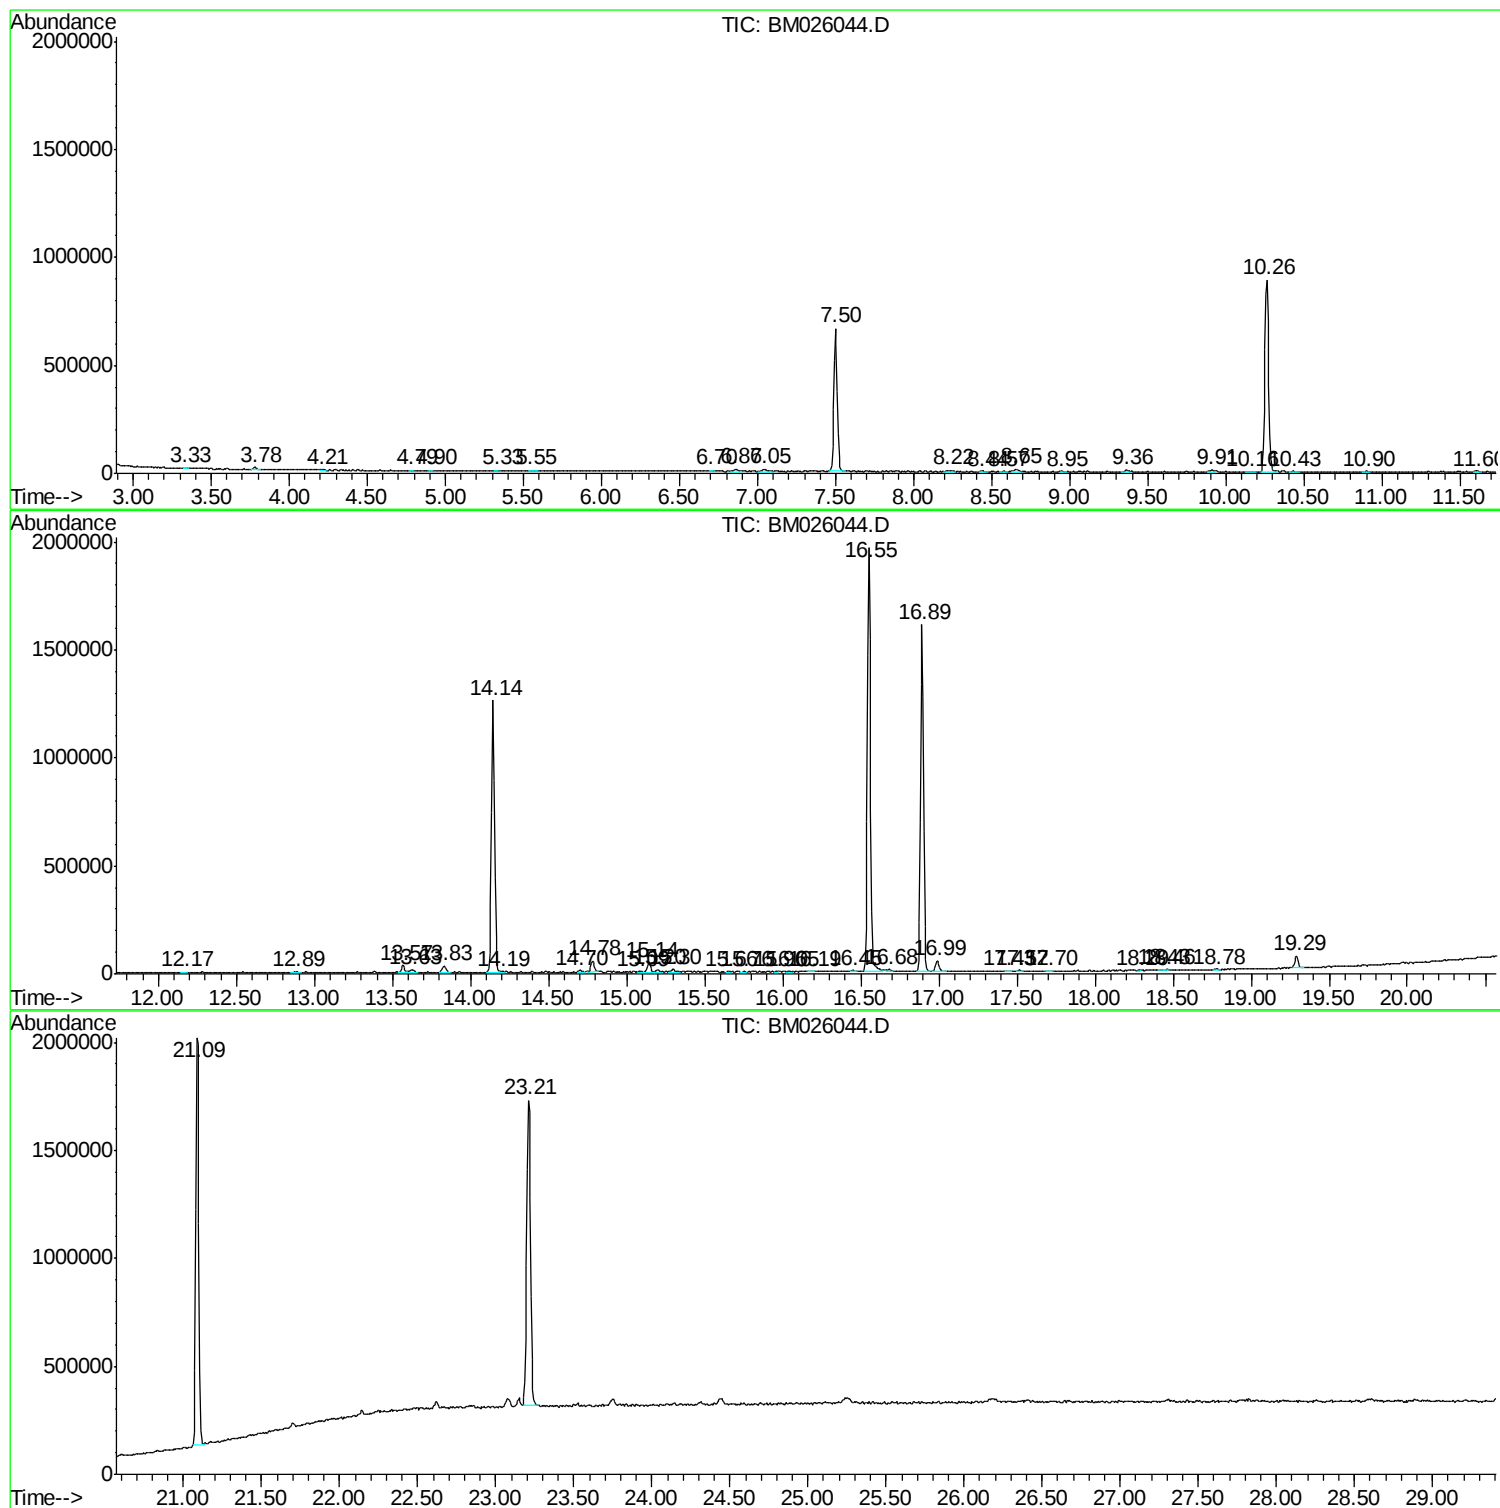

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM052020\
Data File : BM026044.D
Acq On : 20 May 2020 18:12
Operator : MA/SJ
Sample : L2681-08DL2 50X
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C5CB0DL2

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM051320MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM052020\
Data File : BM026044.D
Acq On : 20 May 2020 18:12
Operator : MA/SJ
Sample : L2681-08DL2 50X
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C5CB0DL2

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM051320MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc