


Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM052021\
Data File : BM030090.D
Acq On : 20 May 2021 15:27
Operator : CG/JU
Sample : M2463-07
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampled :
GB3Z0

Manual Integrations
APPROVED

mohammad
5/21/2021 3:37:51 PM

Quant Time: May 20 16:00:10 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM050721.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu May 20 15:21:53 2021
Response via : Initial Calibration

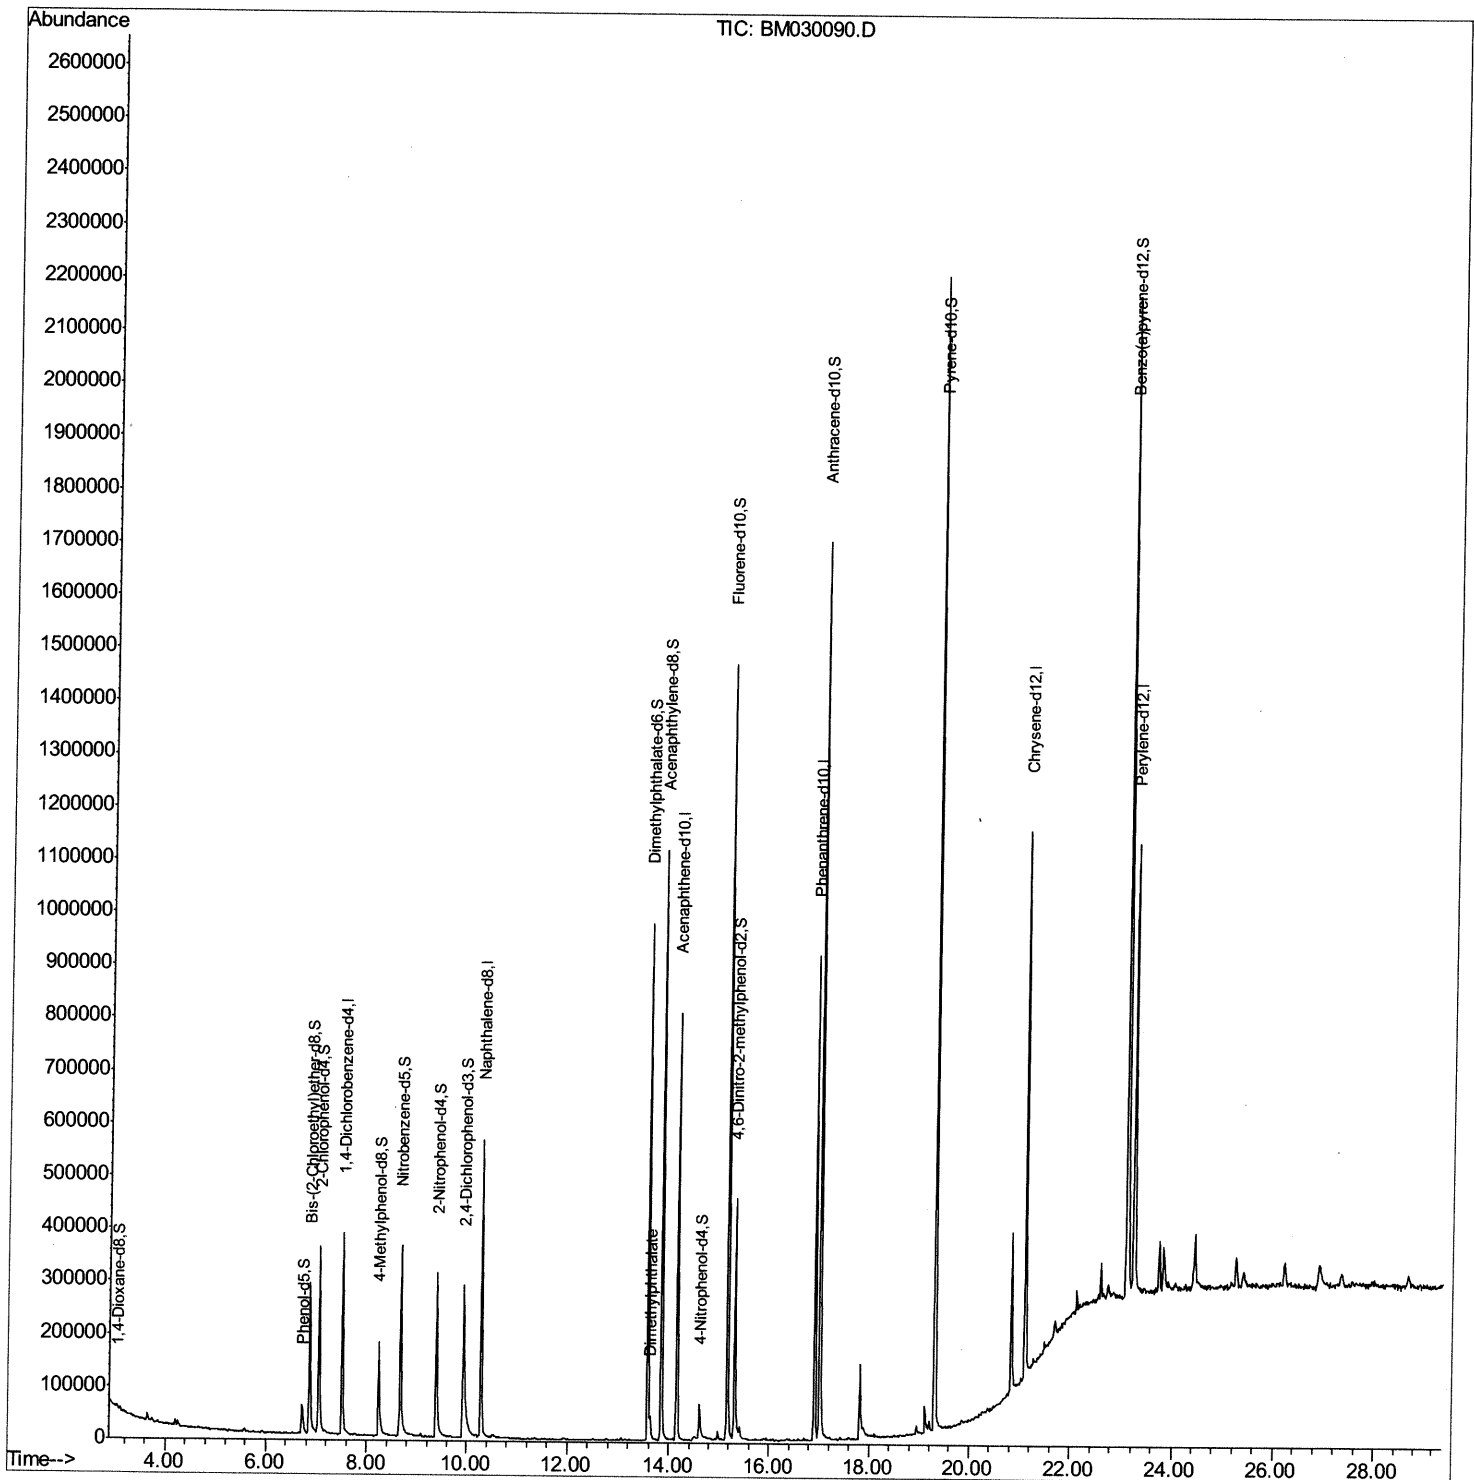

Quantitation Report (Qedit)




Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM052021\
 Data File : BM030090.D
 Acq On : 20 May 2021 15:27
 Operator : CG/JU
 Sample : M2463-07
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_M
ClientSampleId :
 GB3Z0

Manual Integrations
APPROVED

mohammad
 5/21/2021 3:37:51 PM

Quant Time: May 20 15:59:00 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM050721.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu May 20 15:21:53 2021
 Response via : Initial Calibration

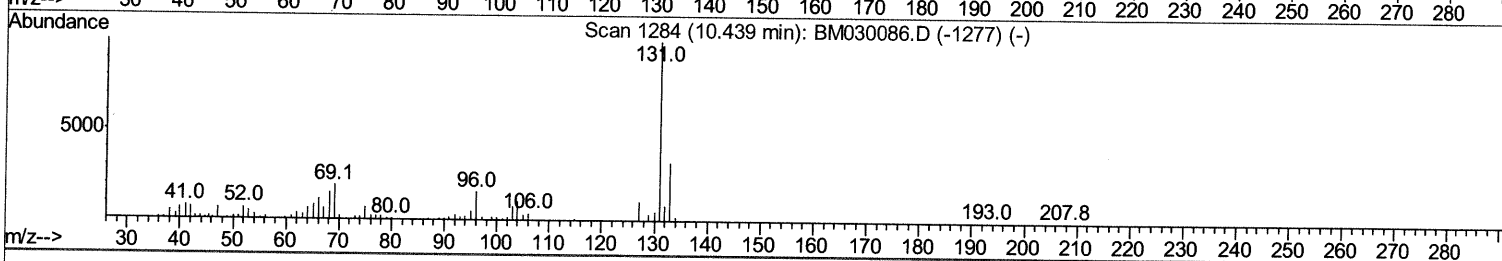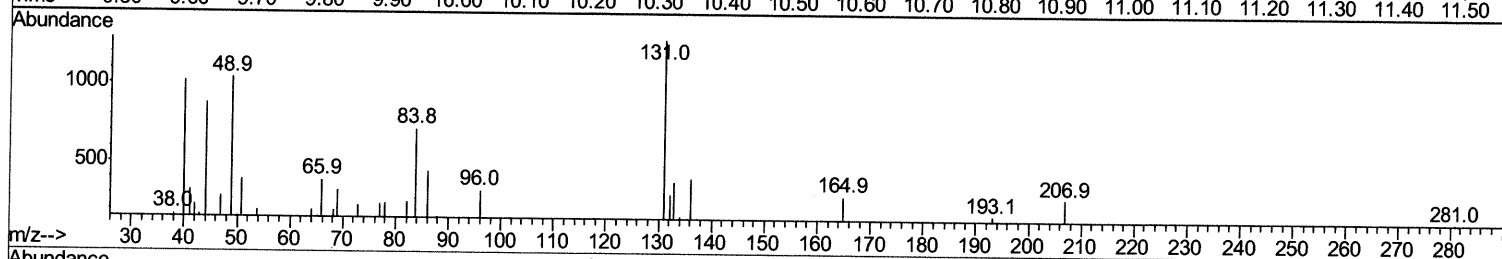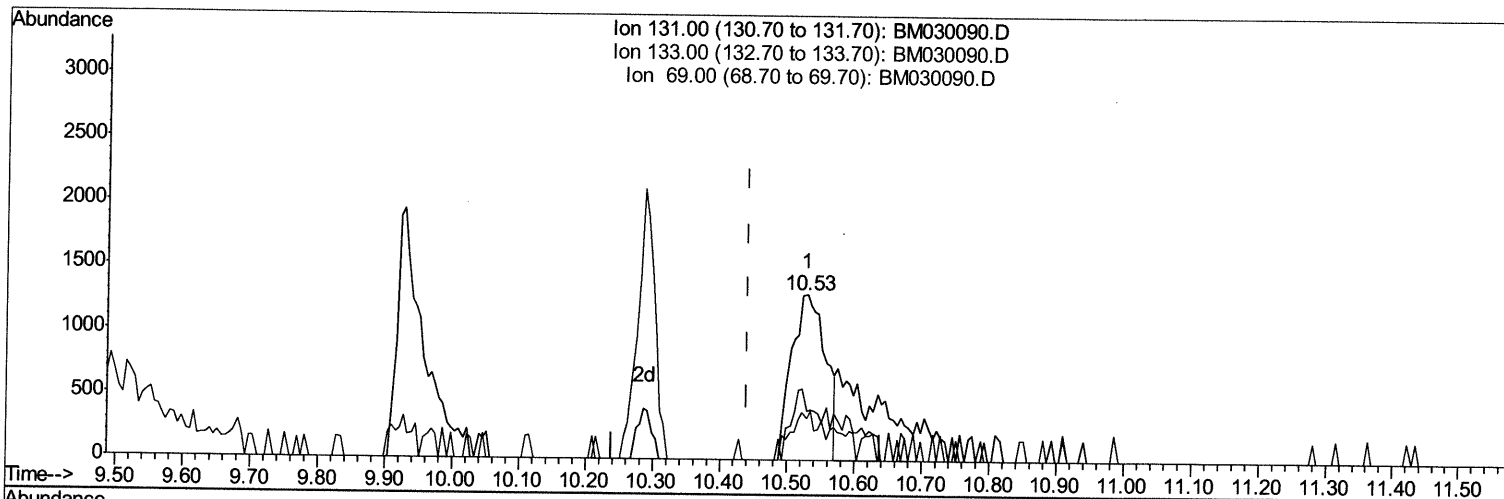

TIC: BM030090.D

(31) 4-Chloroaniline-d4 (S)

10.528min (+0.088) 0.42ng/ul

response 4511

Ion	Exp%	Act%
131.00	100	100
133.00	33.00	29.62
69.00	18.00	25.14#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM052021\
 Data File : BM030090.D
 Acq On : 20 May 2021 15:27
 Operator : CG/JU
 Sample : M2463-07
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_M
ClientSampleId :
 GB3Z0

Manual Integrations
APPROVED

mohammad
 5/21/2021 3:37:51 PM

Quant Time: May 20 15:59:00 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM050721.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu May 20 15:21:53 2021
 Response via : Initial Calibration

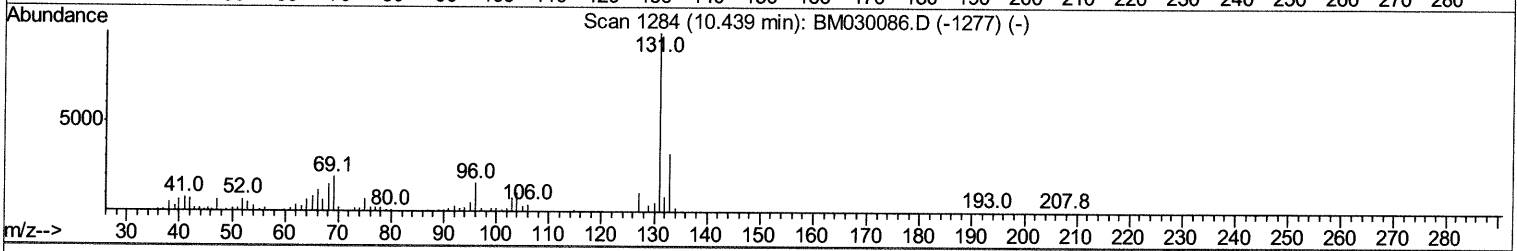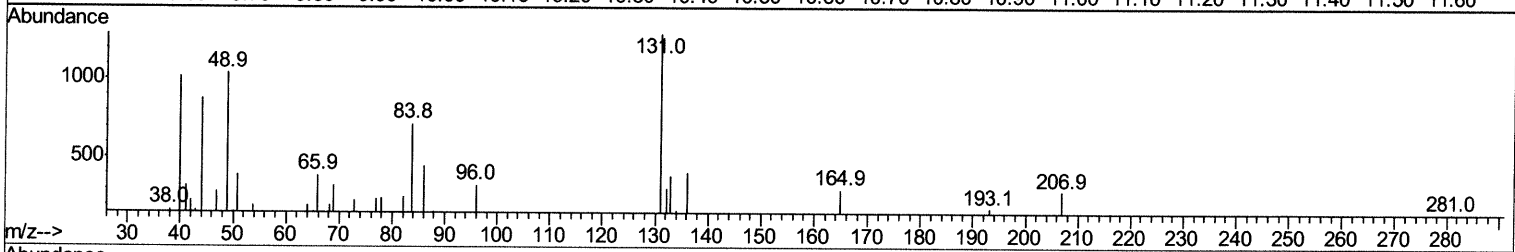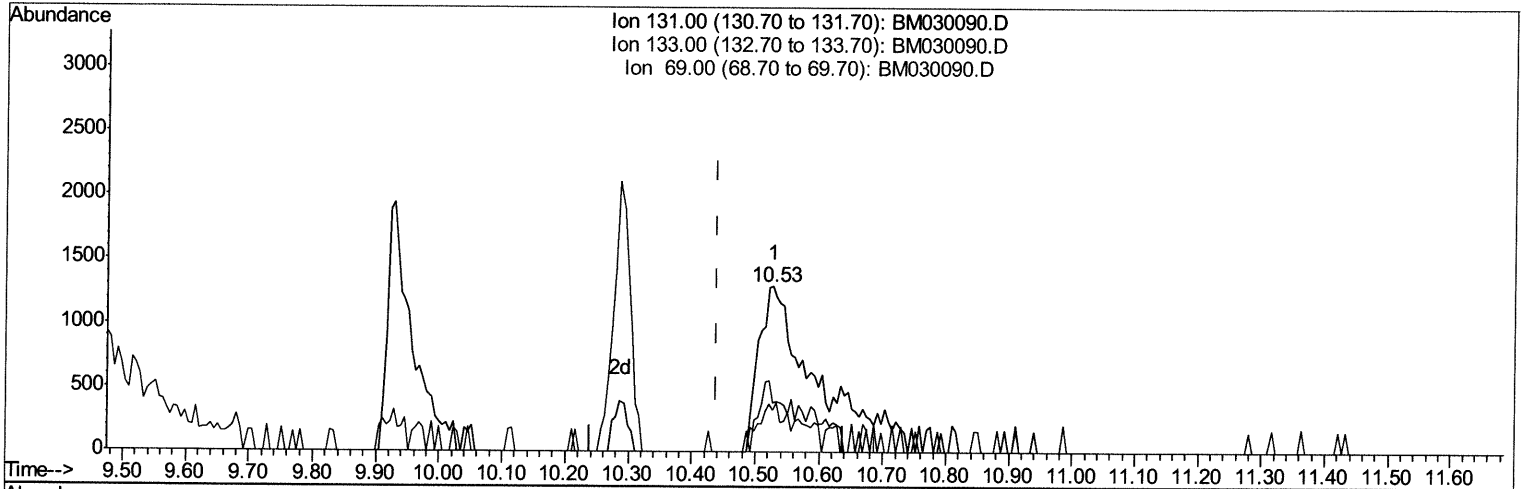

TIC: BM030090.D

(31) 4-Chloroaniline-d4 (S)

10.528min (+0.088) 0.70ng/ul m 05/24/21 JU

response 7537

Ion	Exp%	Act%
131.00	100	100
133.00	33.00	29.62
69.00	18.00	25.14#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM052021\
 Data File : BM030090.D
 Acq On : 20 May 2021 15:27
 Operator : CG/JU
 Sample : M2463-07
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 GB3Z0

Manual Integrations
 APPROVED

mohammad
 5/21/2021 3:37:51 PM

Quant Time: May 20 15:59:00 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM050721.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu May 20 15:21:53 2021
 Response via : Initial Calibration

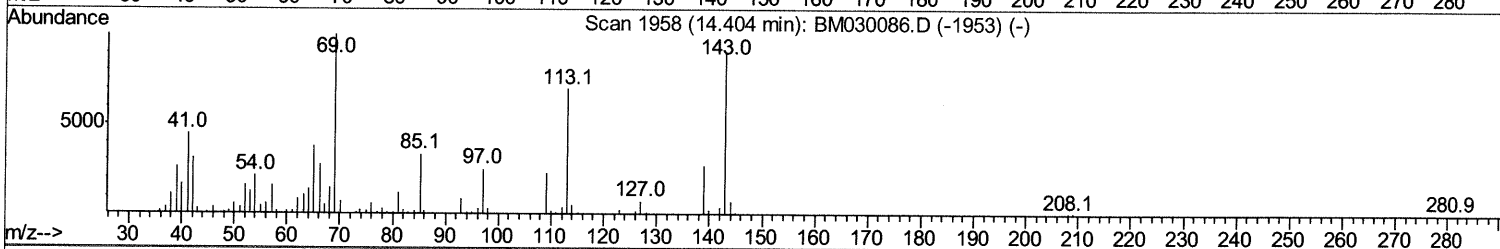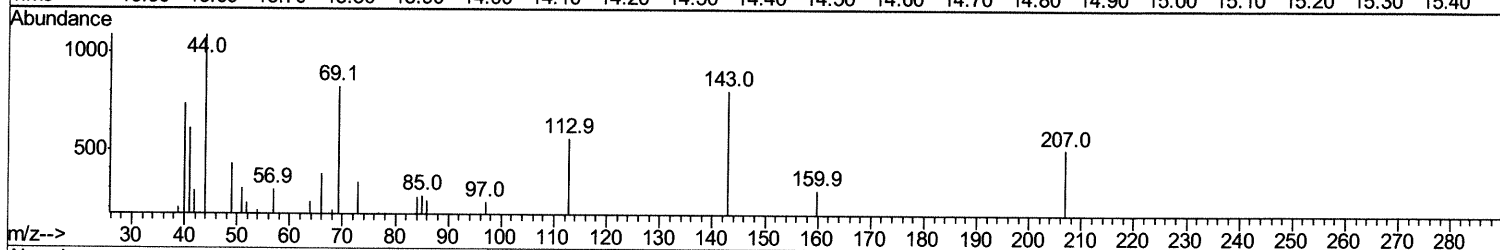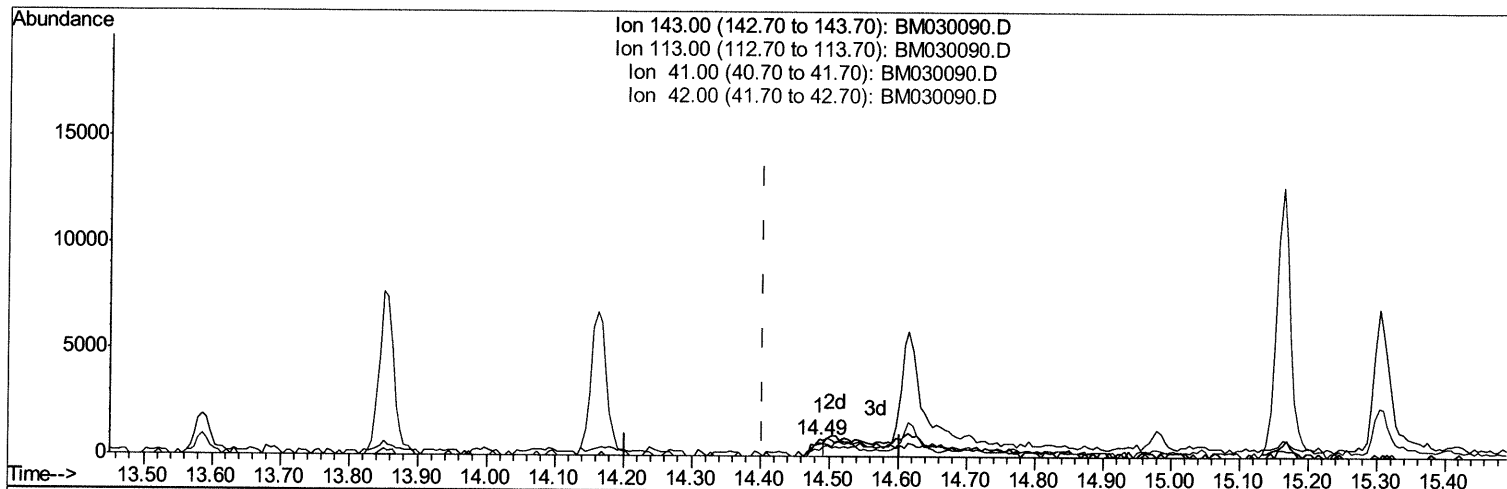

TIC: BM030090.D

(54) 4-Nitrophenol-d4 (S)

14.486min (+0.082) 0.27ng/ul

response 928

Ion	Exp%	Act%
143.00	100	100
113.00	71.10	69.73
41.00	44.70	75.93#
42.00	28.30	35.73#

Quantitation Report (Qedit)




Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM052021\
 Data File : BM030090.D
 Acq On : 20 May 2021 15:27
 Operator : CG/JU
 Sample : M2463-07
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 GB3Z0

Manual Integrations
 APPROVED

mohammad
 5/21/2021 3:37:51 PM

Quant Time: May 20 15:59:00 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM050721.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu May 20 15:21:53 2021
 Response via : Initial Calibration

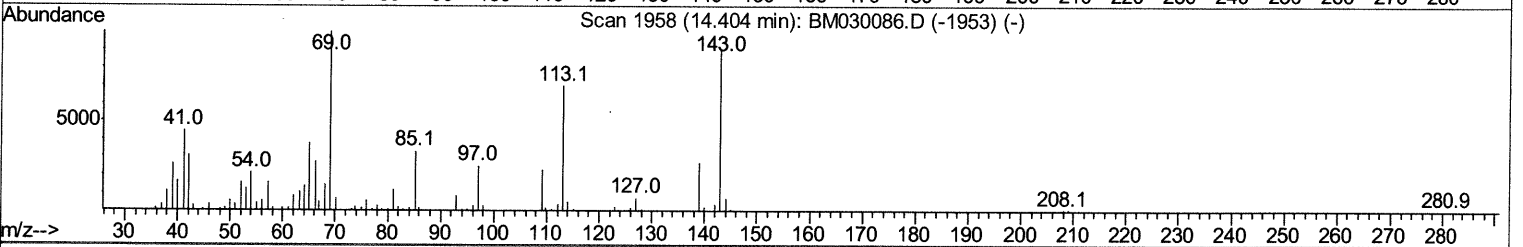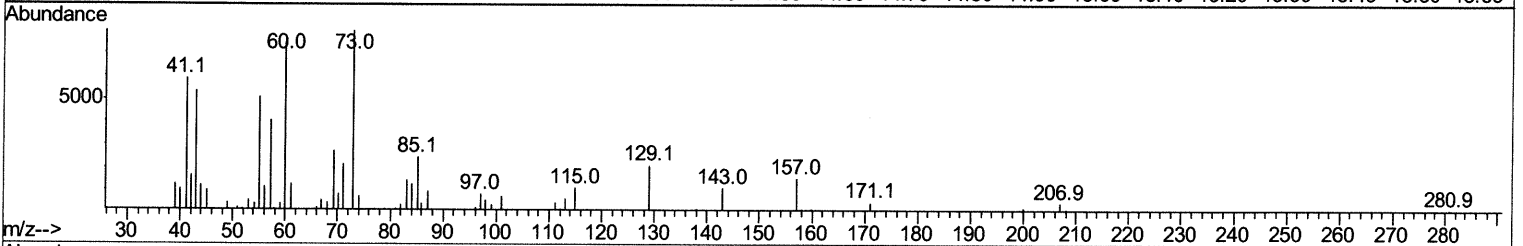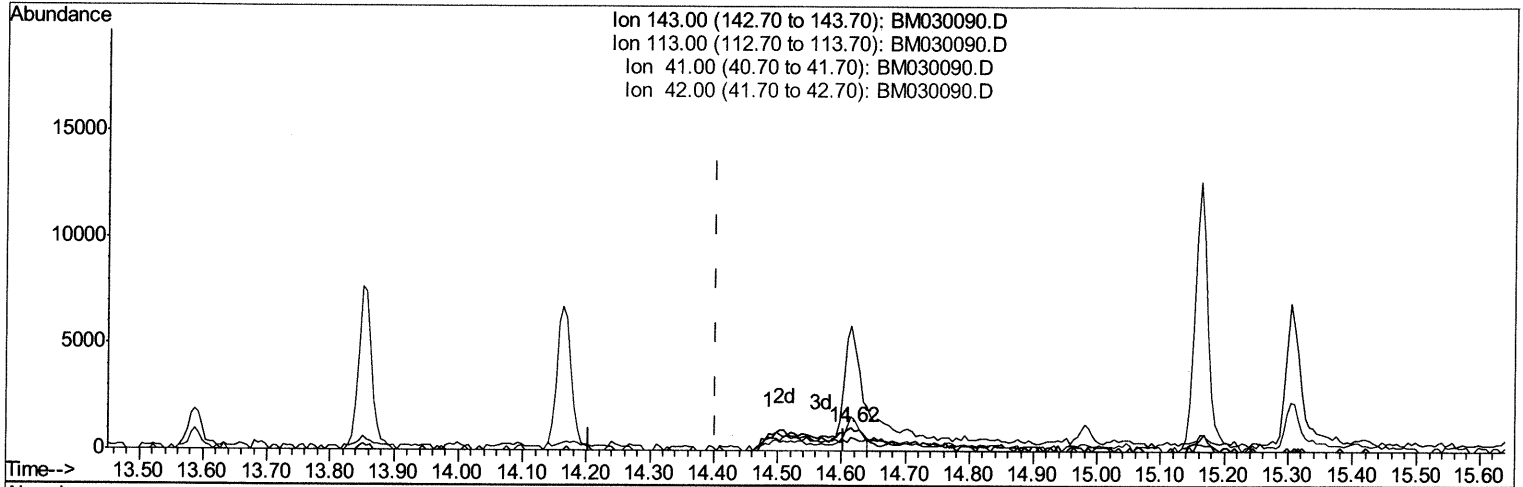

TIC: BM030090.D

(54) 4-Nitrophenol-d4 (S)

14.616min (+0.212) 2.31ng/ul m 05/24/21 JU

response 7844

Ion	Exp%	Act%
143.00	100	100
113.00	71.10	58.59
41.00	44.70	531.01#
42.00	28.30	147.92#

Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM052021\
 Data File : BM030090.D
 Acq On : 20 May 2021 15:27
 Operator : CG/JU
 Sample : M2463-07
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 GB3Z0

Manual Integrations
 APPROVED

mohammad
 5/21/2021 3:37:51 PM

Quant Time: May 20 16:00:10 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM050721.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu May 20 15:21:53 2021
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.52	152	110263	20.00	ng/ul	0.00
20) Naphthalene-d8	10.29	136	451672	20.00	ng/ul	0.00
38) Acenaphthene-d10	14.16	164	269505	20.00	ng/ul	0.00
64) Phenanthrene-d10	16.92	188	521263	20.00	ng/ul	0.00
79) Chrysene-d12	21.10	240	522520	20.00	ng/ul	0.00
88) Perylene-d12	23.25	264	580752	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.05	96	3978	1.44	ng/uL	0.02
4) Pyridine-d5	0.00	84	0d	0.00	ng/ul	
7) Phenol-d5	6.72	99	42037	4.10	ng/ul	0.01
9) Bis-(2-Chloroethyl)ether-d	6.86	67	161470	25.39	ng/ul	0.00
11) 2-Chlorophenol-d4	7.05	132	167533	21.17	ng/ul	0.00
15) 4-Methylphenol-d8	8.24	113	87982	10.37	ng/ul	0.00
21) Nitrobenzene-d5	8.67	128	90990	29.23	ng/ul	0.00
24) 2-Nitrophenol-d4	9.39	143	103835	29.56	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	9.93	165	148980	21.15	ng/ul	0.00
31) 4-Chloroaniline-d4	10.53	131	7537m	0.70	ng/ul	0.09
46) Dimethylphthalate-d6	13.59	166	645544	30.90	ng/ul	0.00
49) Acenaphthylene-d8	13.86	160	774948	29.27	ng/ul	0.00
54) 4-Nitrophenol-d4	14.62	143	7844m	2.31	ng/ul	0.21
60) Fluorene-d10	15.16	176	557470	31.44	ng/ul	0.00
65) 4,6-Dinitro-2-methylphenol	15.30	200	100243	29.61	ng/ul	0.00
73) Anthracene-d10	17.01	188	955033	36.38	ng/ul	0.00
81) Pyrene-d10	19.31	212	1121604	41.84	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.11	264	1227819	37.30	ng/ul	0.00

Target Compounds

Target Compounds	R.T.	QIon	Response	Conc	Units	Ovalue
47) Dimethylphthalate	13.64	163	23858	1.141	ng/ul#	97

(#) = qualifier out of range (m) = manual integration (+) = signals summed