


Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM052021\
Data File : BM030091.D
Acq On : 20 May 2021 16:03
Operator : CG/JU
Sample : M2463-08
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
GB3Z1

Manual Integrations
APPROVED

mohammad
5/21/2021 3:37:53 PM

Quant Time: May 20 16:39:20 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM050721.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu May 20 15:21:53 2021
Response via : Initial Calibration

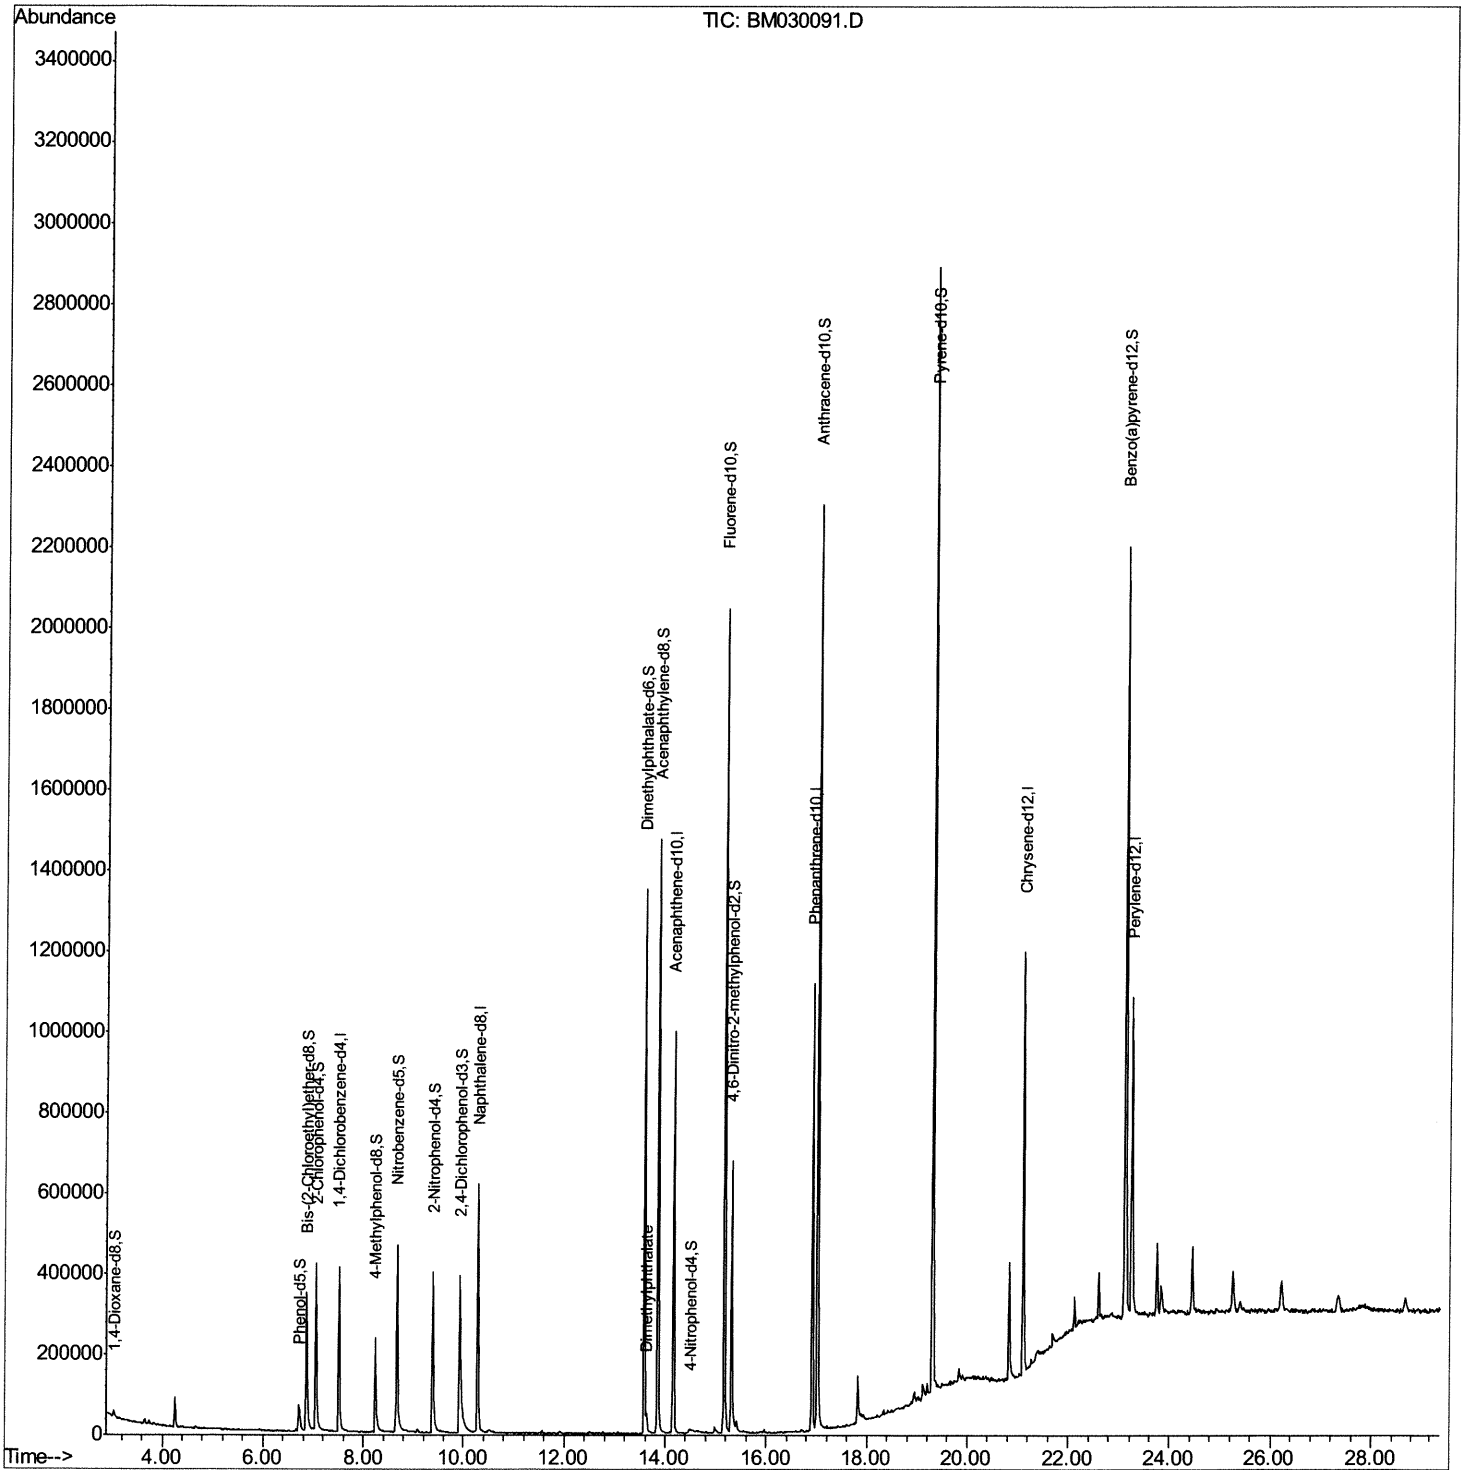

Quantitation Report (Qedit)




Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM052021\
 Data File : BM030091.D
 Acq On : 20 May 2021 16:03
 Operator : CG/JU
 Sample : M2463-08
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 GB3Z1

Manual Integrations
 APPROVED

mohammad
 5/21/2021 3:37:53 PM

Quant Time: May 20 16:34:58 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM050721.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu May 20 15:21:53 2021
 Response via : Initial Calibration

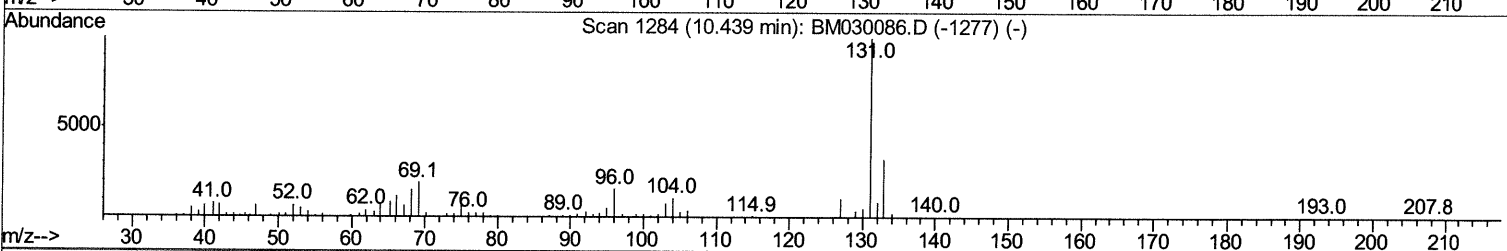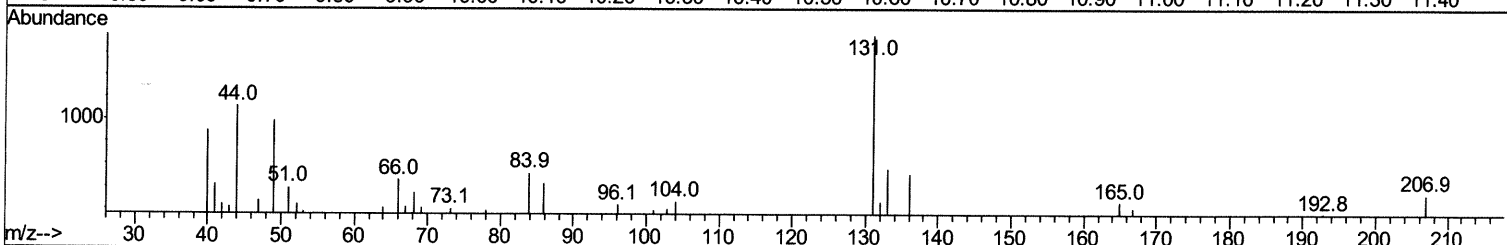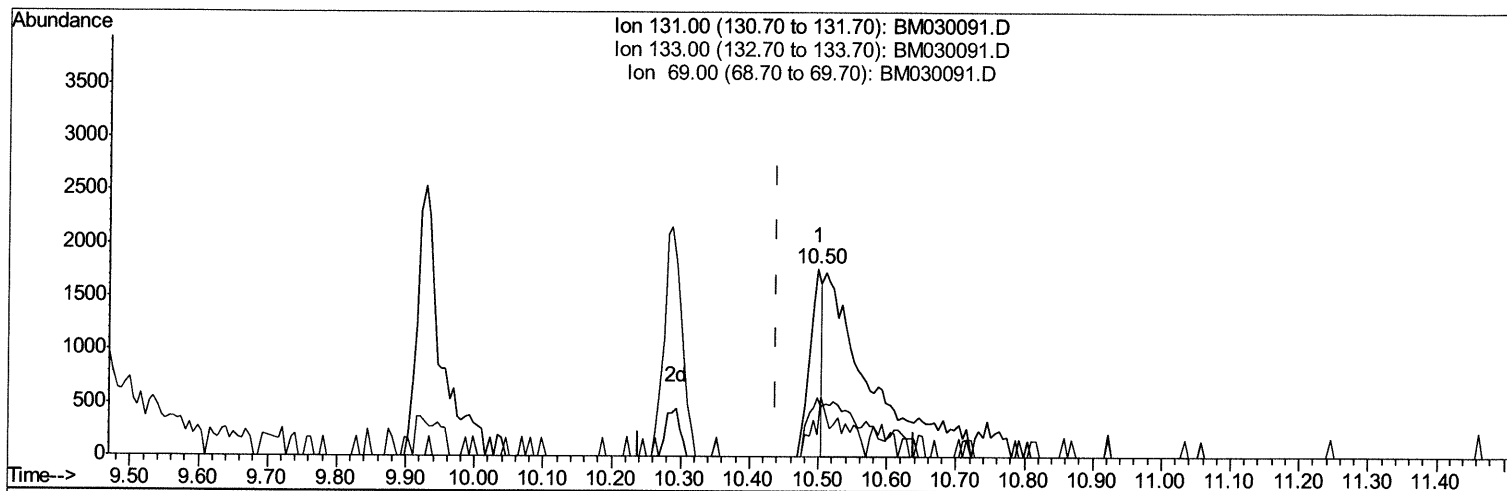

TIC: BM030091.D

(31) 4-Chloroaniline-d4 (S)

10.498min (+0.059) 0.19ng/ul

response 2306

Ion	Exp%	Act%
131.00	100	100
133.00	33.00	31.71
69.00	18.00	11.89#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM052021\
 Data File : BM030091.D
 Acq On : 20 May 2021 16:03
 Operator : CG/JU
 Sample : M2463-08
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 GB3Z1

Manual Integrations
 APPROVED

mohammad
 5/21/2021 3:37:53 PM

Quant Time: May 20 16:34:58 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM050721.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu May 20 15:21:53 2021
 Response via : Initial Calibration

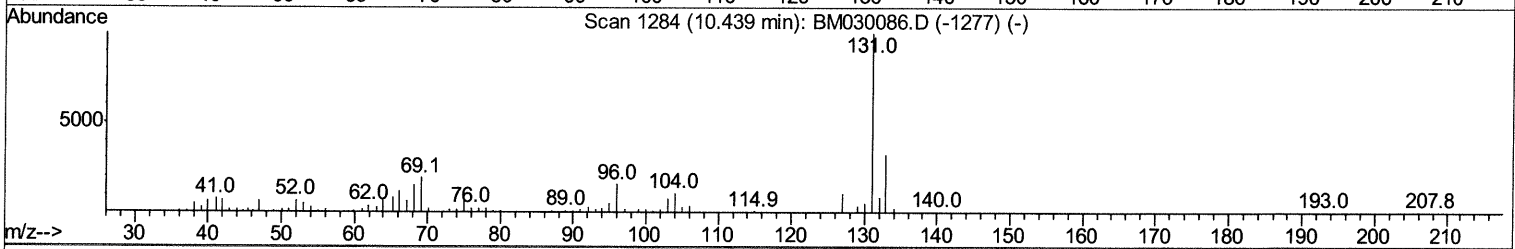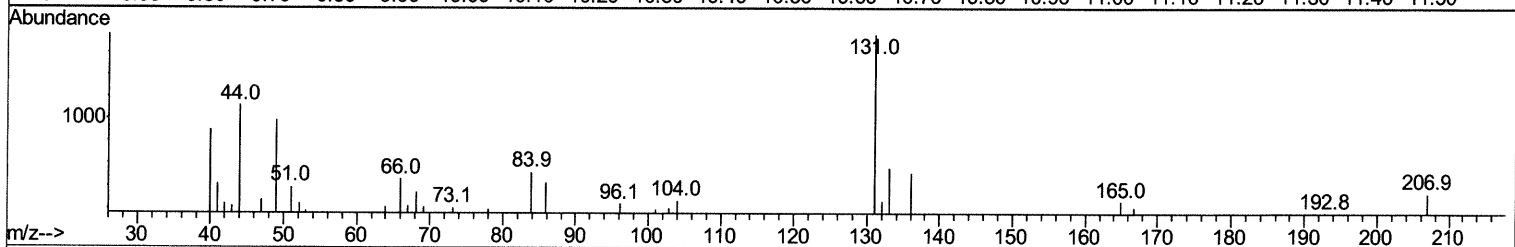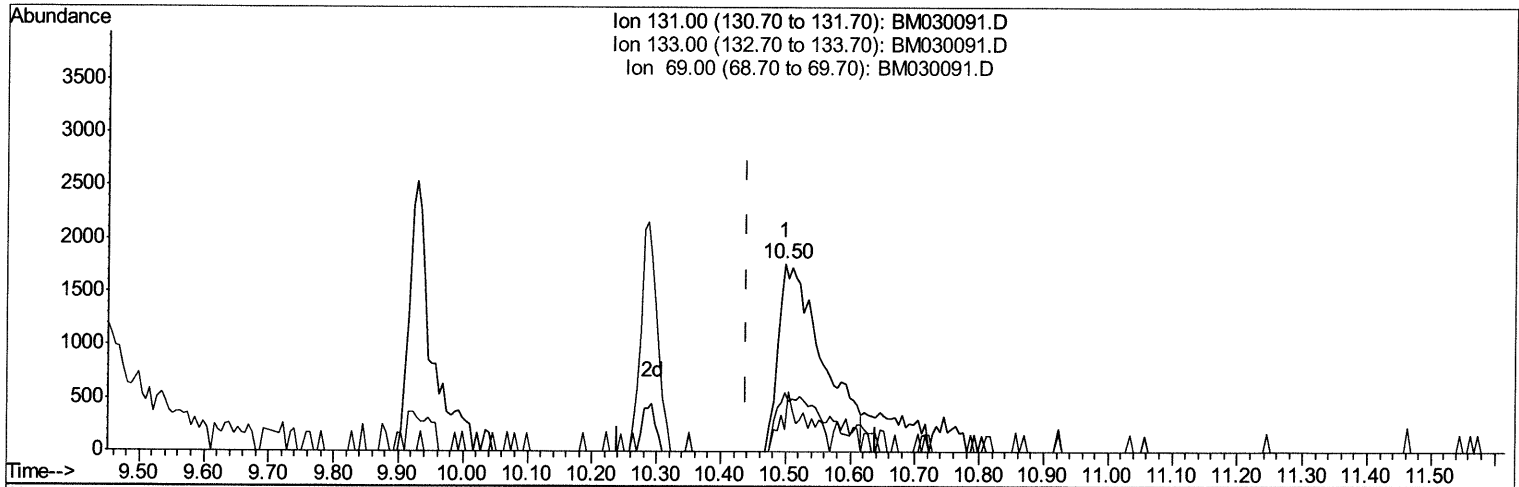

TIC: BM030091.D

(31) 4-Chloroaniline-d4 (S)

10.498min (+0.059) 0.70ng/ul m 05/24/21 JU

response 8457

Ion	Exp%	Act%
131.00	100	100
133.00	33.00	31.71
69.00	18.00	11.89#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM052021\
 Data File : BM030091.D
 Acq On : 20 May 2021 16:03
 Operator : CG/JU
 Sample : M2463-08
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_M
ClientSampleId :
 GB3Z1

Manual Integrations
APPROVED

mohammad
 5/21/2021 3:37:53 PM

Quant Time: May 20 16:34:58 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM050721.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu May 20 15:21:53 2021
 Response via : Initial Calibration

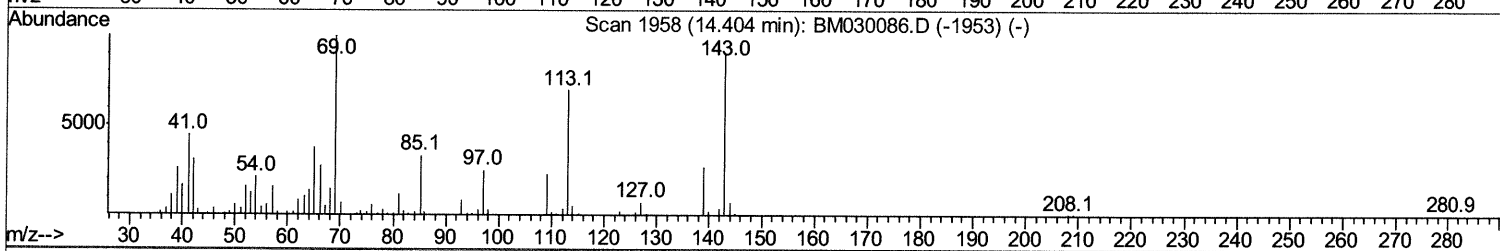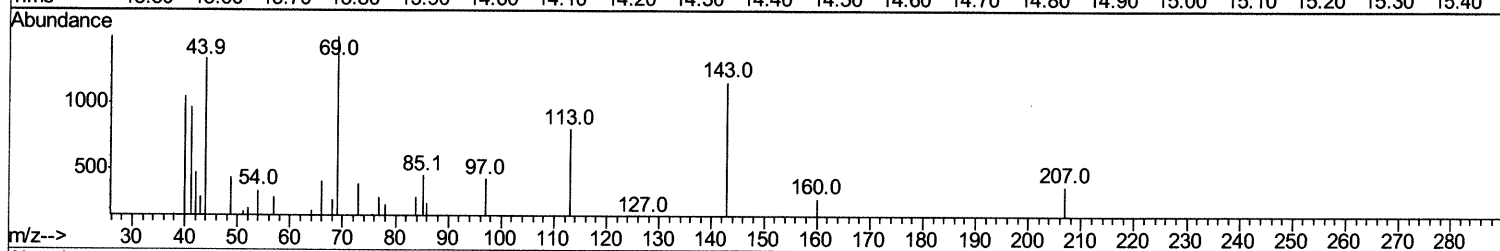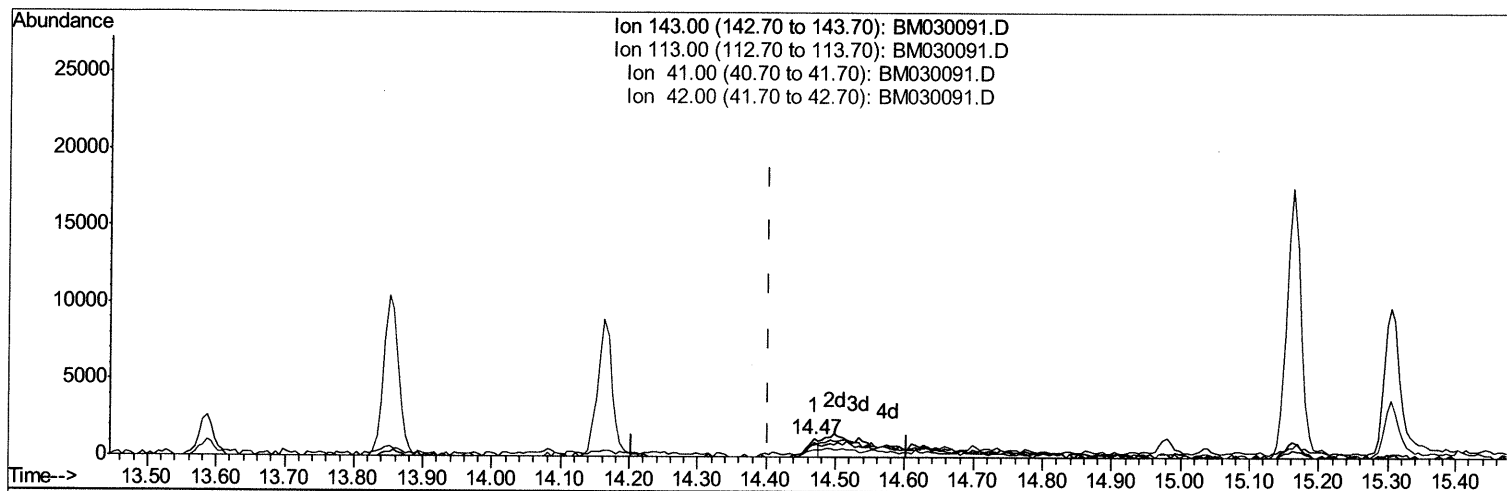

TIC: BM030091.D

(54) 4-Nitrophenol-d4 (S)

14.469min (+0.065) 0.32ng/ul

response 1327

Ion	Exp%	Act%
143.00	100	100
113.00	71.10	69.51
41.00	44.70	82.95#
42.00	28.30	41.09#

Quantitation Report (Qedit)




Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM052021\
 Data File : BM030091.D
 Acq On : 20 May 2021 16:03
 Operator : CG/JU
 Sample : M2463-08
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_M
ClientSampleId :
 GB3Z1

Manual Integrations
APPROVED

mohammad
 5/21/2021 3:37:53 PM

Quant Time: May 20 16:34:58 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM050721.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu May 20 15:21:53 2021
 Response via : Initial Calibration

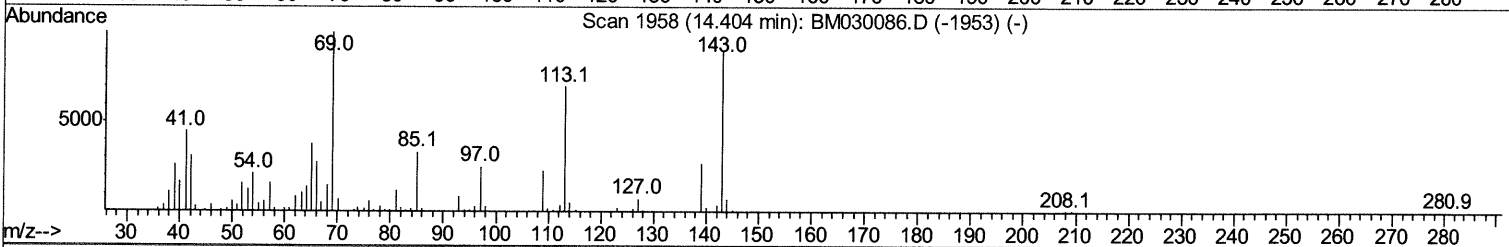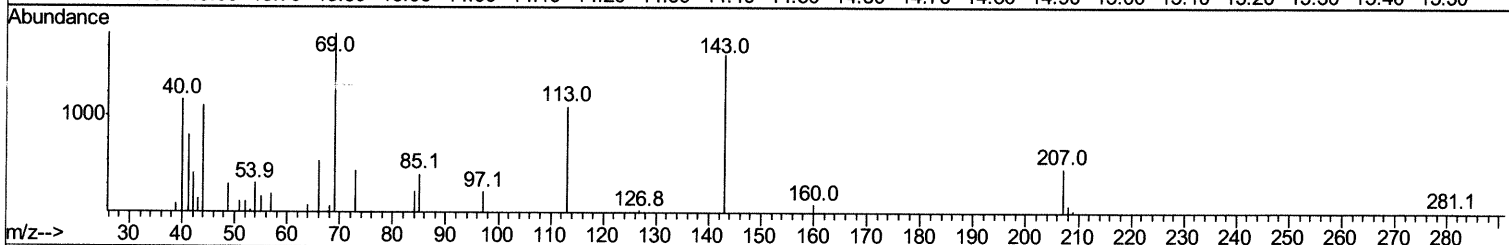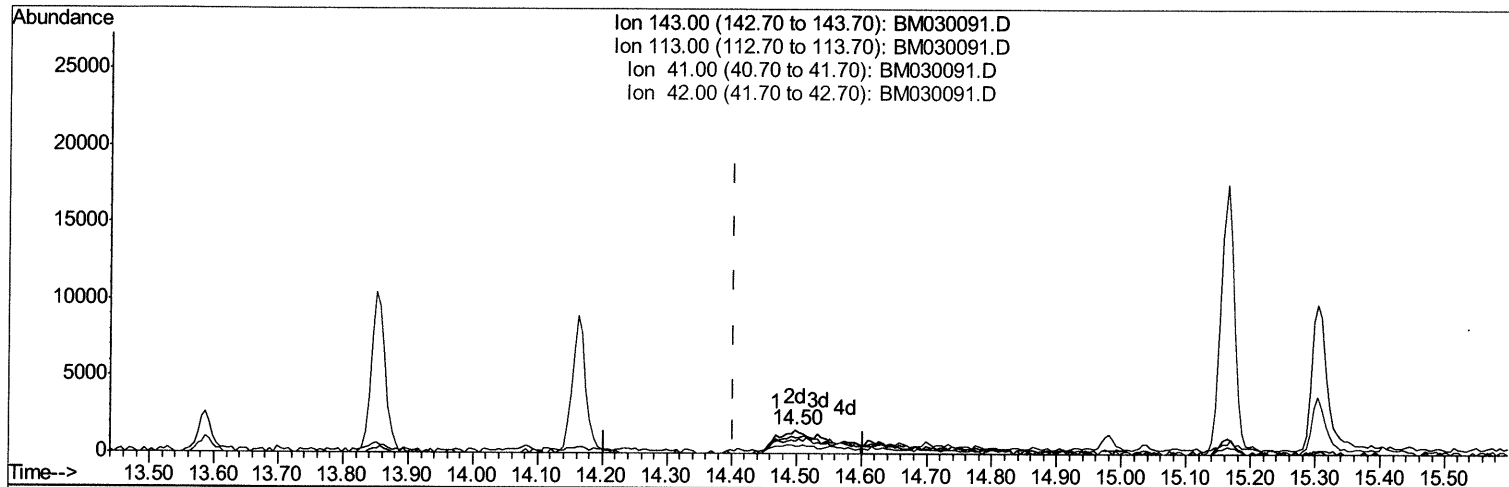

TIC: BM030091.D

(54) 4-Nitrophenol-d4 (S)

14.498min (+0.094) 2.04ng/ul m 05/24/21 JU

response 8526

Ion	Exp%	Act%
143.00	100	100
113.00	71.10	70.09
41.00	44.70	54.03#
42.00	28.30	32.44

Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM052021\
 Data File : BM030091.D
 Acq On : 20 May 2021 16:03
 Operator : CG/JU
 Sample : M2463-08
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 GB3Z1

Manual Integrations
 APPROVED

mohammad
 5/21/2021 3:37:53 PM

Quant Time: May 20 16:39:20 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM050721.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu May 20 15:21:53 2021
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.52	152	117340	20.00	ng/ul	0.00
20) Naphthalene-d8	10.29	136	508880	20.00	ng/ul	0.00
38) Acenaphthene-d10	14.16	164	330852	20.00	ng/ul	0.00
64) Phenanthrene-d10	16.92	188	640814	20.00	ng/ul	0.00
79) Chrysene-d12	21.10	240	545653	20.00	ng/ul	0.00
88) Perylene-d12	23.24	264	535774	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.04	96	8614	2.93	ng/uL	0.00
4) Pvrindine-d5	0.00	84	0d	0.00	ng/ul	
7) Phenol-d5	6.72	99	51250	4.70	ng/ul	0.01
9) Bis-(2-Chloroethyl)ether-d	6.86	67	188396	27.84	ng/ul	0.00
11) 2-Chlorophenol-d4	7.05	132	194360	23.08	ng/ul	0.00
15) 4-Methylphenol-d8	8.23	113	106318	11.78	ng/ul	0.00
21) Nitrobenzene-d5	8.67	128	110702	31.57	ng/ul	0.00
24) 2-Nitrophenol-d4	9.39	143	127822	32.29	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	9.93	165	195846	24.68	ng/ul	0.00
31) 4-Chloroaniline-d4	10.50	131	8457m>	0.70	ng/ul>	0.06 05/24/21JU
46) Dimethylphthalate-d6	13.59	166	858246	33.47	ng/ul	0.00
49) Acenaphthylene-d8	13.86	160	1030767	31.72	ng/ul	0.00
54) 4-Nitrophenol-d4	14.50	143	8526m>	2.04	ng/ul>	0.09 05/24/21JU
60) Fluorene-d10	15.16	176	757338	34.79	ng/ul	0.00
65) 4,6-Dinitro-2-methylphenol	15.30	200	143487	34.47	ng/ul	0.00
73) Anthracene-d10	17.01	188	1295491	40.15	ng/ul	0.00
81) Pyrene-d10	19.31	212	1379521	49.28	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.12	264	1212466	39.92	ng/ul	0.00

Target Compounds

				Ovalue	
47) Dimethylphthalate	13.64	163	27411	1.067	ng/ul 96

(#) = qualifier out of range (m) = manual integration (+) = signals summed