


Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM052021\
Data File : BM030100.D
Acq On : 20 May 2021 21:33
Operator : CG/JU
Sample : M2463-01
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
GB3Y6

Manual Integrations
APPROVED

mohammad
5/21/2021 3:38:18 PM

Quant Time: May 21 01:36:30 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM050721.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu May 20 12:00:20 2021
Response via : Initial Calibration

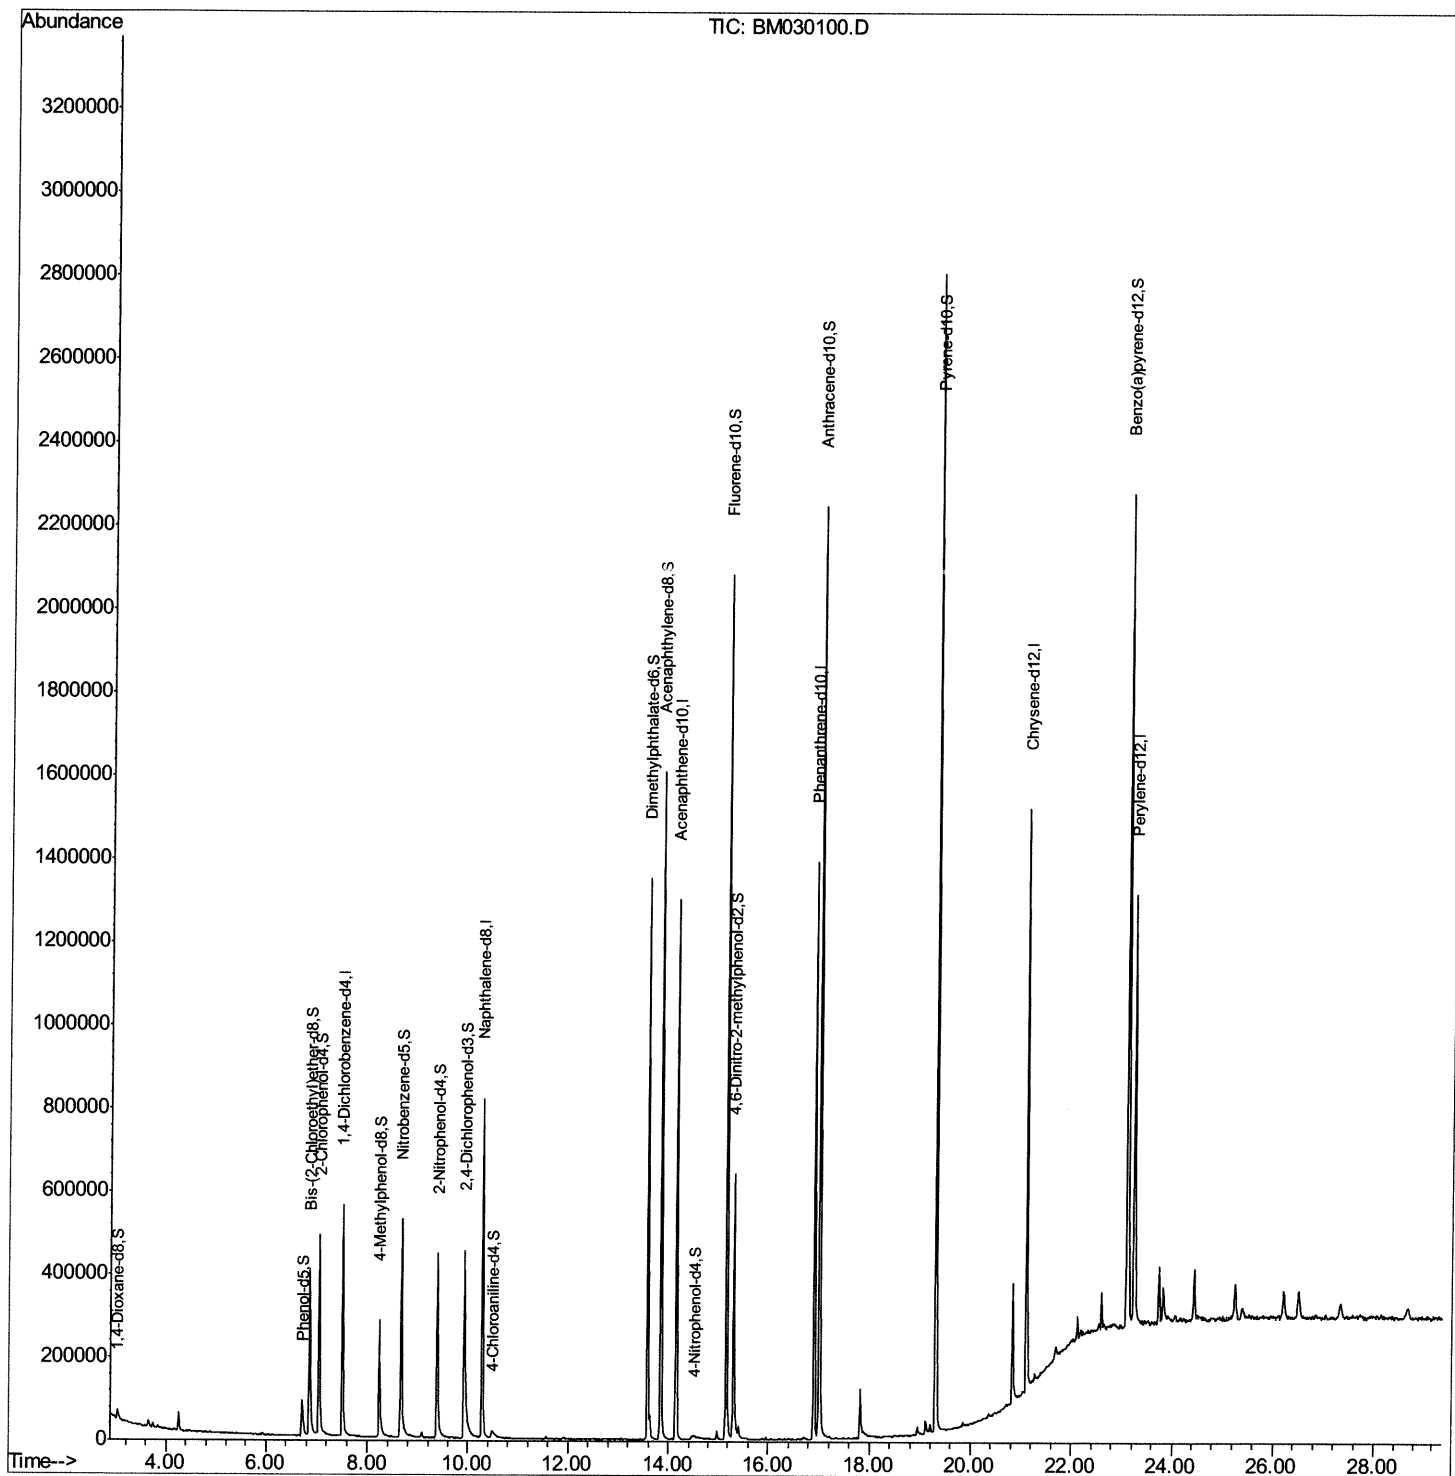

Quantitation Report (Qedit)




Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM052021\
Data File : BM030100.D
Acq On : 20 May 2021 21:33
Operator : CG/JU
Sample : M2463-01
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
GB3Y6

Manual Integrations
APPROVED

mohammad
5/21/2021 3:38:18 PM

Quant Time: May 21 01:34:56 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM050721.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu May 20 12:00:20 2021
Response via : Initial Calibration

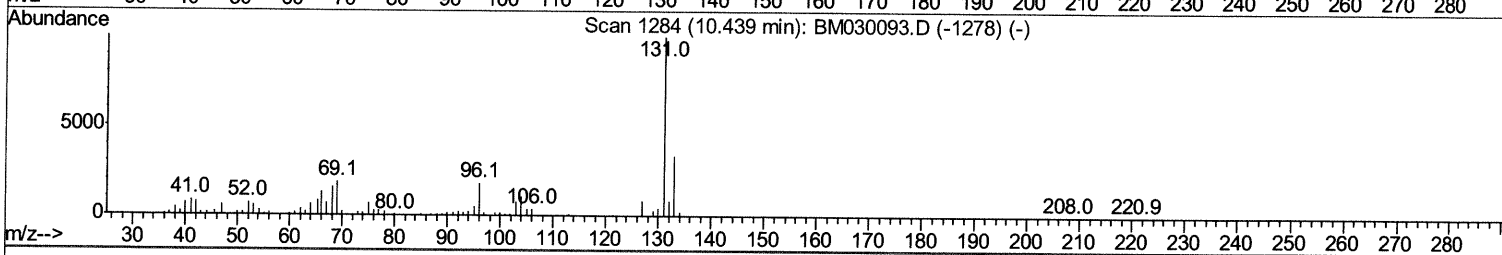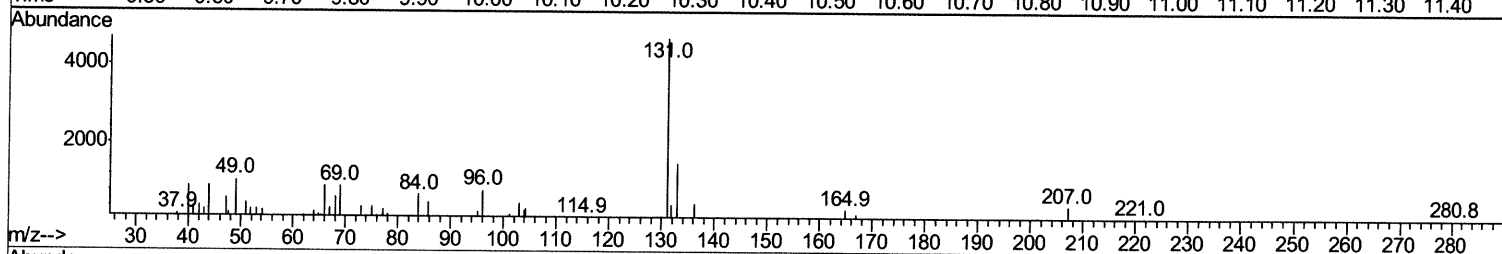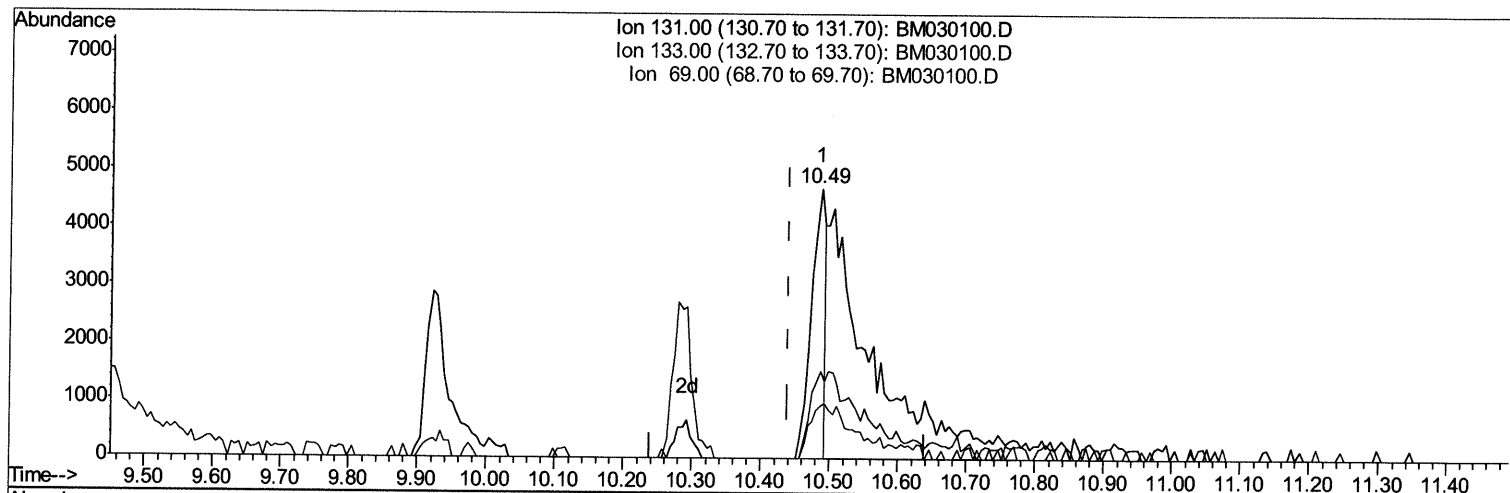

TIC: BM030100.D

(31) 4-Chloroaniline-d4 (S)

10.486min (+0.047) 0.42ng/ul

response 6701

Ion	Exp%	Act%
131.00	100	100
133.00	33.00	32.50
69.00	18.00	19.61
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM052021\
Data File : BM030100.D
Acq On : 20 May 2021 21:33
Operator : CG/JU
Sample : M2463-01
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
GB3Y6

Manual Integrations
APPROVED

mohammad
5/21/2021 3:38:18 PM

Quant Time: May 21 01:34:56 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM050721.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu May 20 12:00:20 2021
Response via : Initial Calibration

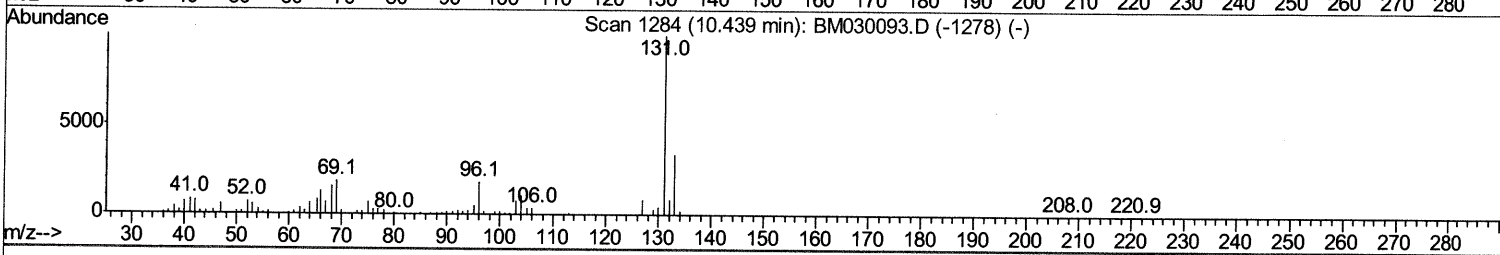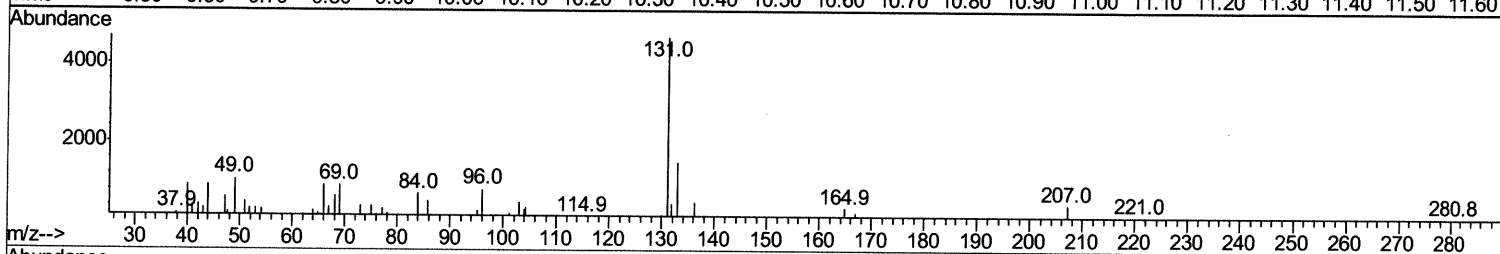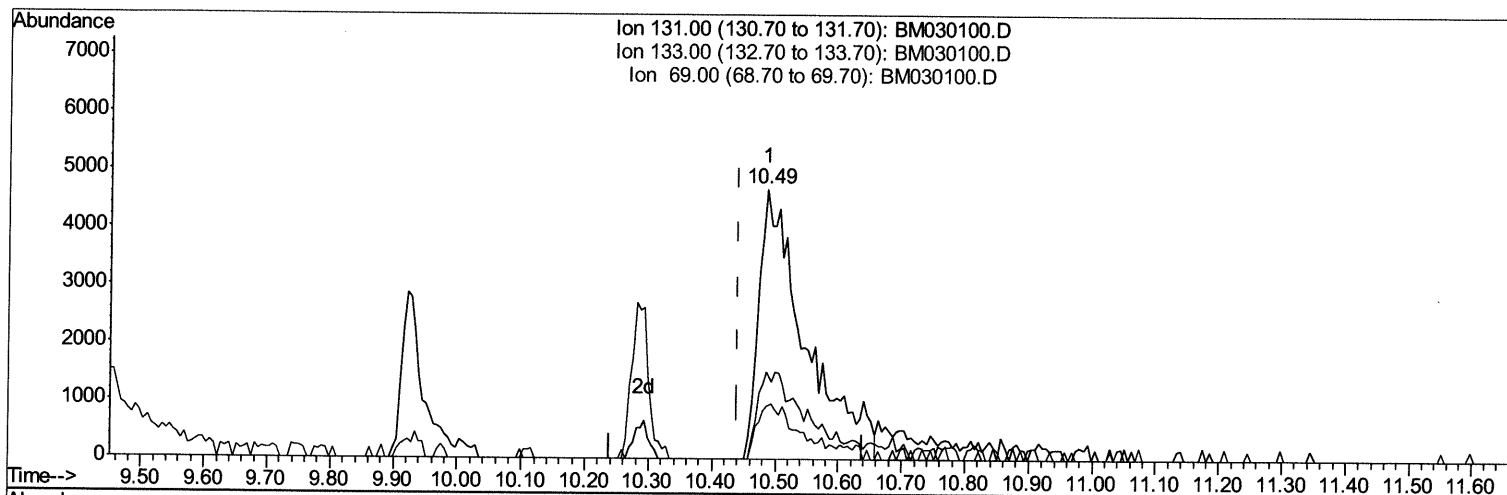

TIC: BM030100.D

(31) 4-Chloroaniline-d4 (S)

10.486min (+0.047) 1.49ng/ul m 05/24/21JU

response 23631

Ion	Exp%	Act%
131.00	100	100
133.00	33.00	32.50
69.00	18.00	19.61
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM052021\
 Data File : BM030100.D
 Acq On : 20 May 2021 21:33
 Operator : CG/JU
 Sample : M2463-01
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 GB3Y6

Manual Integrations
 APPROVED

mohammad
 5/21/2021 3:38:18 PM

Quant Time: May 21 01:35:47 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM050721.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu May 20 12:00:20 2021
 Response via : Initial Calibration

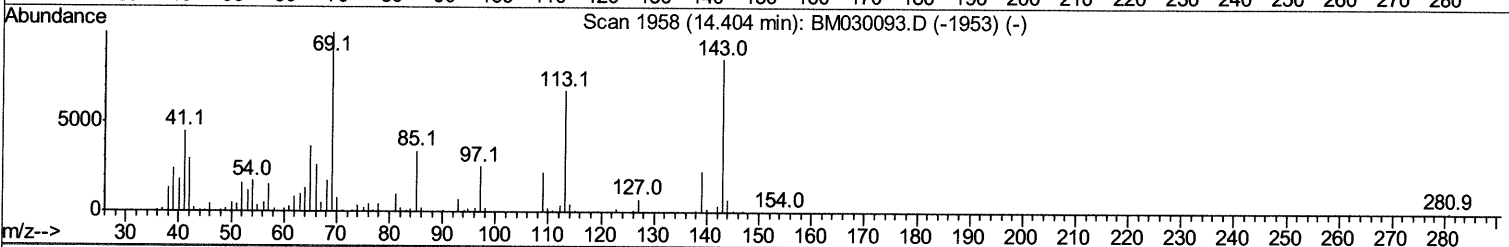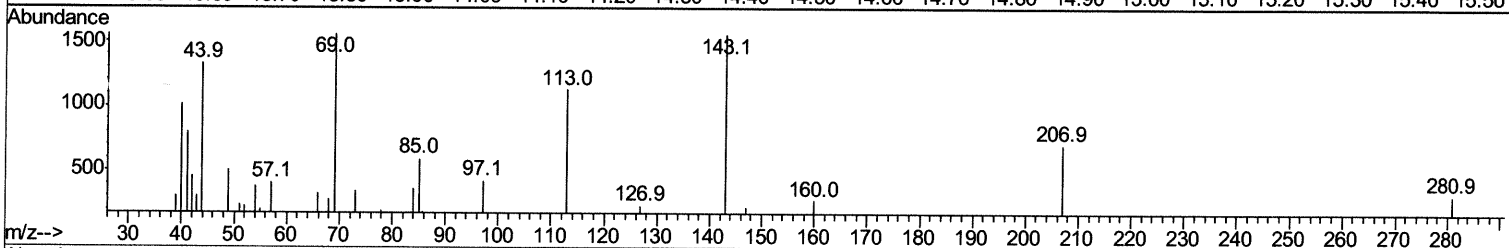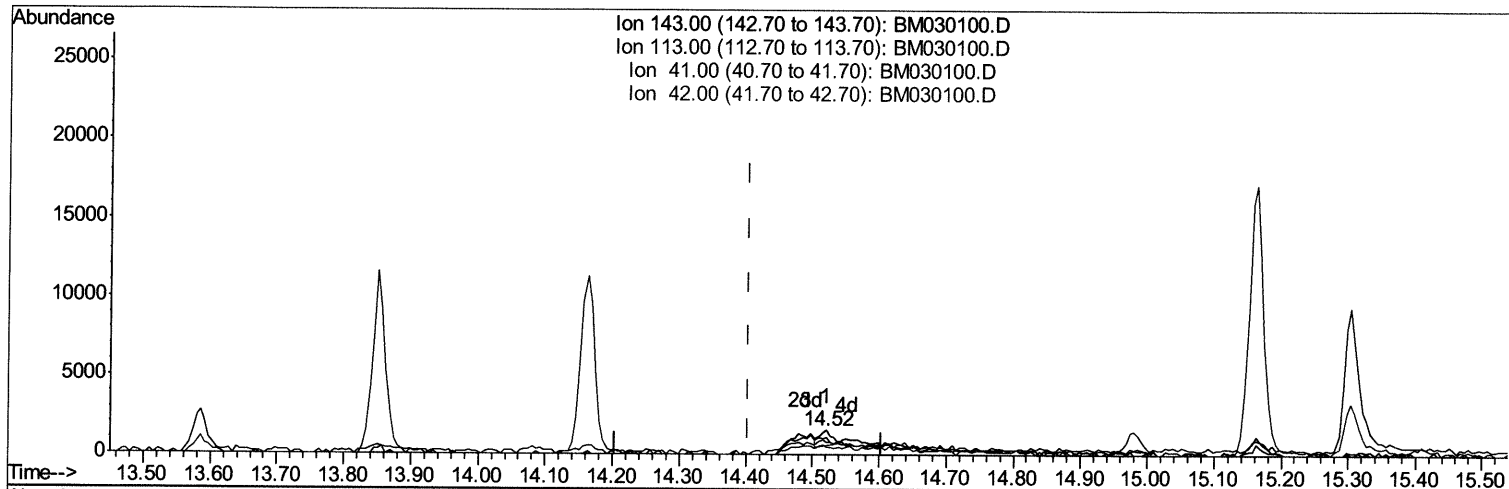

TIC: BM030100.D

(54) 4-Nitrophenol-d4 (S)

14.521min (+0.118) 0.24ng/ul

response 1262

Ion	Exp%	Act%
143.00	100	100
113.00	71.10	72.46
41.00	44.70	51.22
42.00	28.30	29.02

Quantitation Report (Qedit)




Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM052021\
Data File : BM030100.D
Acq On : 20 May 2021 21:33
Operator : CG/JU
Sample : M2463-01
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
GB3Y6

Manual Integrations
APPROVED

mohammad
5/21/2021 3:38:18 PM

Quant Time: Mav 21 01:35:47 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM050721.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu May 20 12:00:20 2021
Response via : Initial Calibration

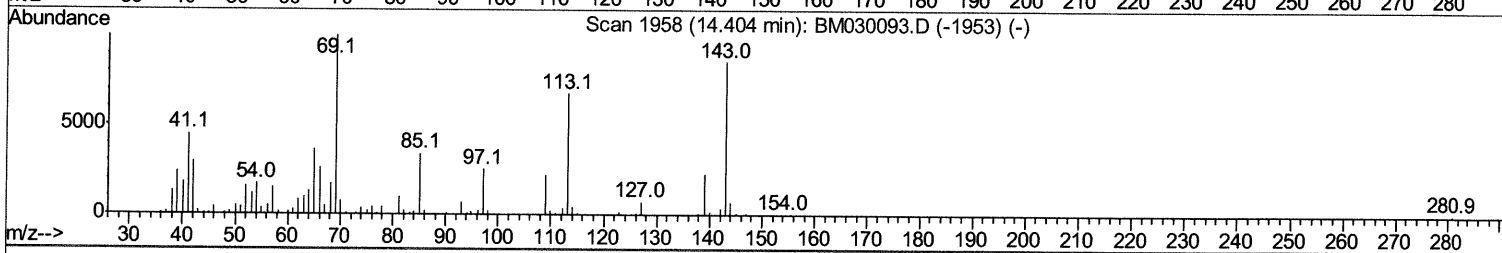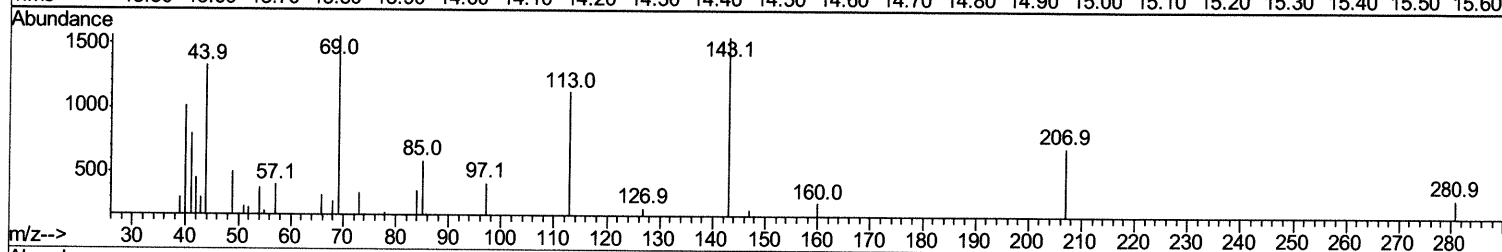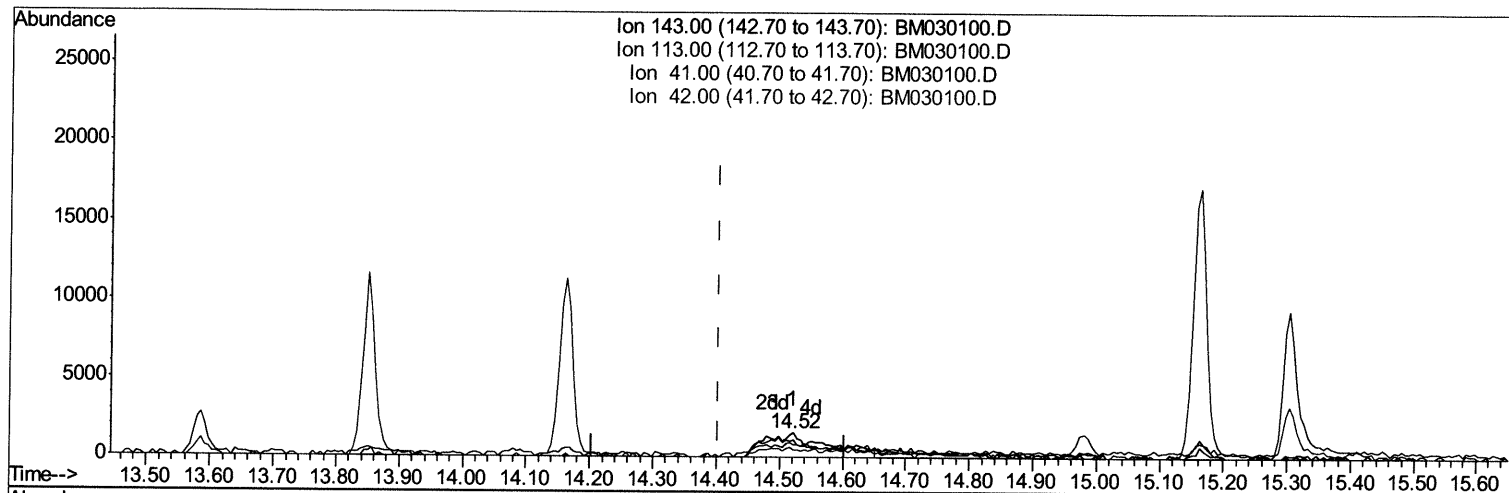

TIC: BM030100.D

(54) 4-Nitrophenol-d4 (S)

14.521min (+0.118) 2.05ng/ul m 05/24/21JU

response 10814

Ion	Exp%	Act%
143.00	100	100
113.00	71.10	72.46
41.00	44.70	51.22
42.00	28.30	29.02

Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM052021\
 Data File : BM030100.D
 Acq On : 20 May 2021 21:33
 Operator : CG/JU
 Sample : M2463-01
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 GB3Y6

Manual Integrations
 APPROVED

mohammad
 5/21/2021 3:38:18 PM

Quant Time: May 21 01:36:30 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM050721.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu May 20 12:00:20 2021
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.51	152	155944	20.00	ng/ul	0.00
20) Naphthalene-d8	10.29	136	669668	20.00	ng/ul	0.00
38) Acenaphthene-d10	14.16	164	418677	20.00	ng/ul	0.00
64) Phenanthrene-d10	16.91	188	783046	20.00	ng/ul	0.00
79) Chrysene-d12	21.10	240	674096	20.00	ng/ul	0.00
88) Perylene-d12	23.24	264	699179	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.04	96	13615	3.49	ng/uL	0.00
4) Pyridine-d5	0.00	84	0d	0.00	ng/ul	
7) Phenol-d5	6.71	99	65213	4.50	ng/ul	0.00
9) Bis-(2-Chloroethyl)ether-d	6.86	67	216509	24.08	ng/ul	0.00
11) 2-Chlorophenol-d4	7.05	132	224830	20.09	ng/ul	0.00
15) 4-Methylphenol-d8	8.23	113	129237	10.78	ng/ul	0.00
21) Nitrobenzene-d5	8.67	128	125068	27.10	ng/ul	0.00
24) 2-Nitrophenol-d4	9.39	143	142616	27.38	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	9.92	165	215370	20.62	ng/ul	0.00
31) 4-Chloroaniline-d4	10.49	131	23631m>	1.49	ng/ul>	0.05 05/24/21 Jd
46) Dimethylphthalate-d6	13.59	166	866354	26.70	ng/ul	0.00
49) Acenaphthylene-d8	13.85	160	1072454	26.08	ng/ul	0.00
54) 4-Nitrophenol-d4	14.52	143	10814m>	2.05	ng/ul>	0.12 05/24/21 Jd
60) Fluorene-d10	15.16	176	789421	28.66	ng/ul	0.00
65) 4,6-Dinitro-2-methylphenol	15.30	200	137093	26.95	ng/ul	0.00
73) Anthracene-d10	17.01	188	1258717	31.92	ng/ul	0.00
81) Pyrene-d10	19.31	212	1333153	38.55	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.11	264	1274588	32.16	ng/ul	0.00

Target Compounds

Ovalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed