


Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM052021\
Data File : BM030124.D
Acq On : 21 May 2021 22:06
Operator : CG/JU
Sample : M2474-02
Misc :
ALS Vial : 40 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
GB401

Manual Integrations
APPROVED

mohammad
5/24/2021 1:52:59 PM

Quant Time: May 22 00:31:54 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM050721.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri May 21 23:57:54 2021
Response via : Initial Calibration

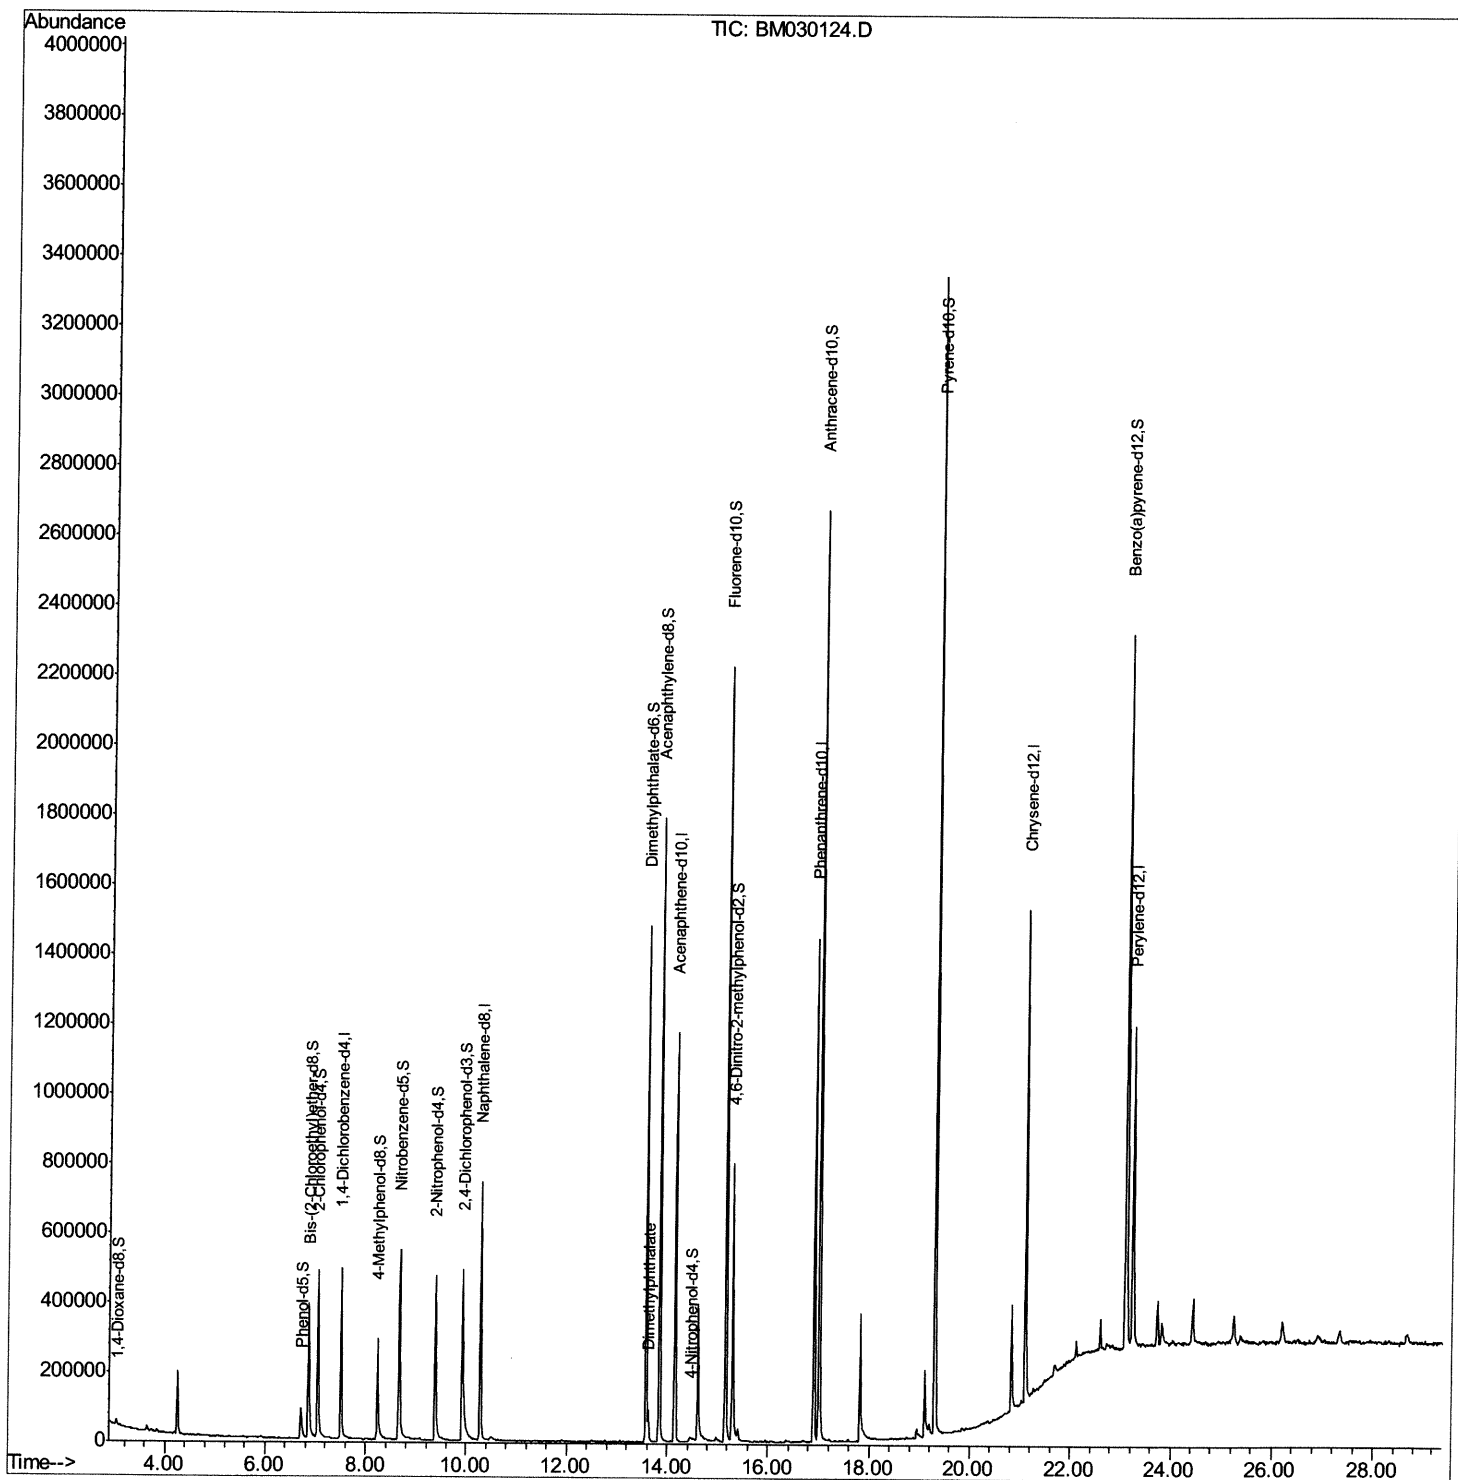

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM052021\
Data File : BM030124.D
Acq On : 21 May 2021 22:06
Operator : CG/JU
Sample : M2474-02
Misc :
ALS Vial : 40 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
GB401

Manual Integrations
APPROVED

mohammad
5/24/2021 1:52:59 PM

Quant Time: May 22 00:30:44 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM050721.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri May 21 23:57:54 2021
Response via : Initial Calibration

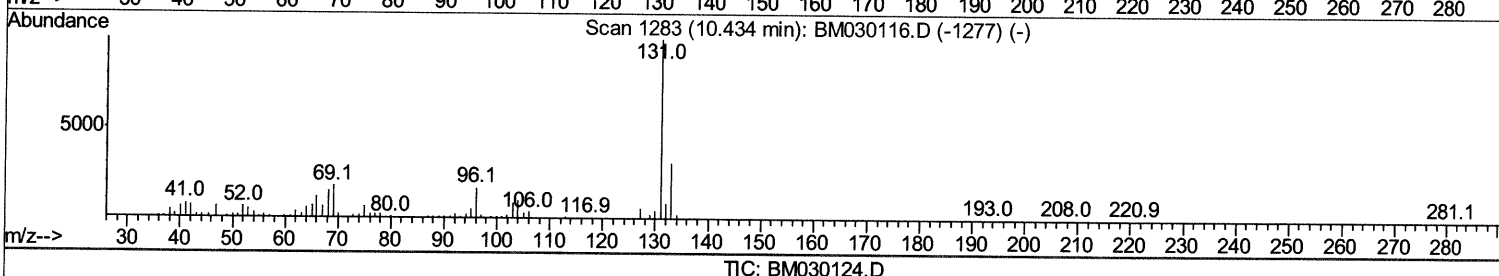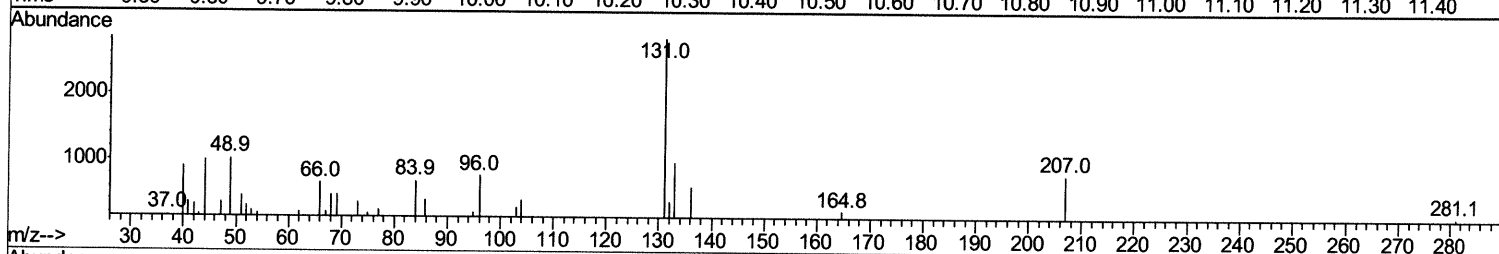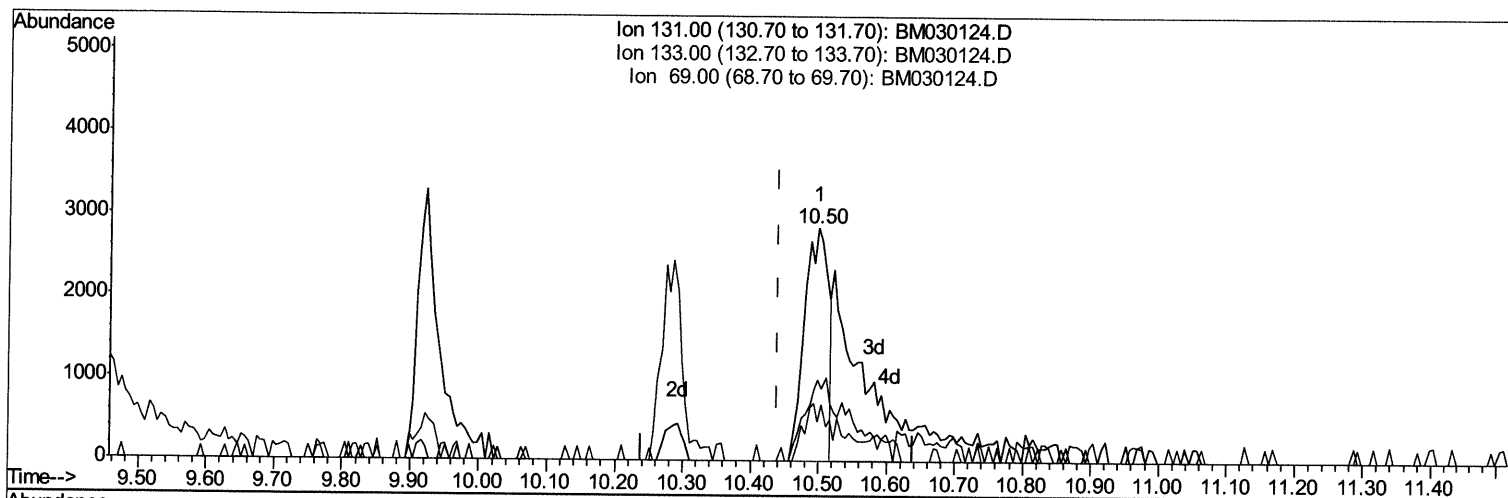

TIC: BM030124.D

(31) 4-Chloroaniline-d4 (S)

10.498min (+0.059) 0.48ng/ul

response 6842

Ion	Exp%	Act%
131.00	100	100
133.00	33.00	34.72
69.00	18.00	16.94
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM052021\
 Data File : BM030124.D
 Acq On : 21 May 2021 22:06
 Operator : CG/JU
 Sample : M2474-02
 Misc :
 ALS Vial : 40 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 GB401

Manual Integrations
 APPROVED

mohammad
 5/24/2021 1:52:59 PM

Quant Time: May 22 00:30:44 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM050721.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri May 21 23:57:54 2021
 Response via : Initial Calibration

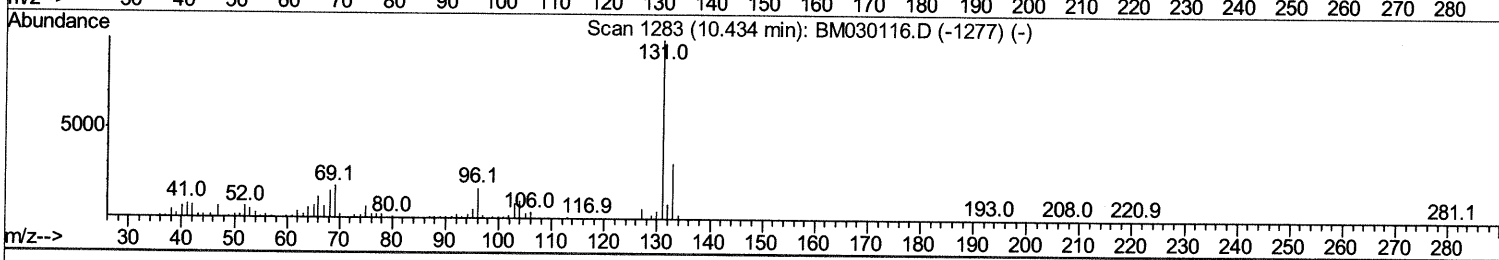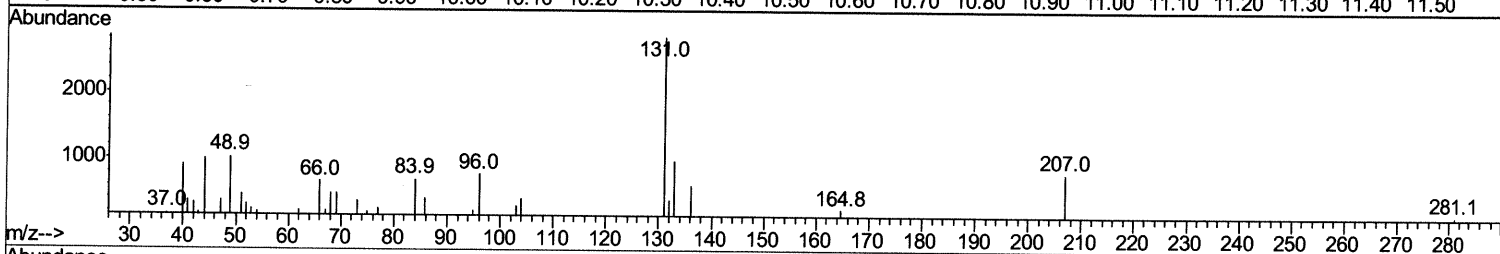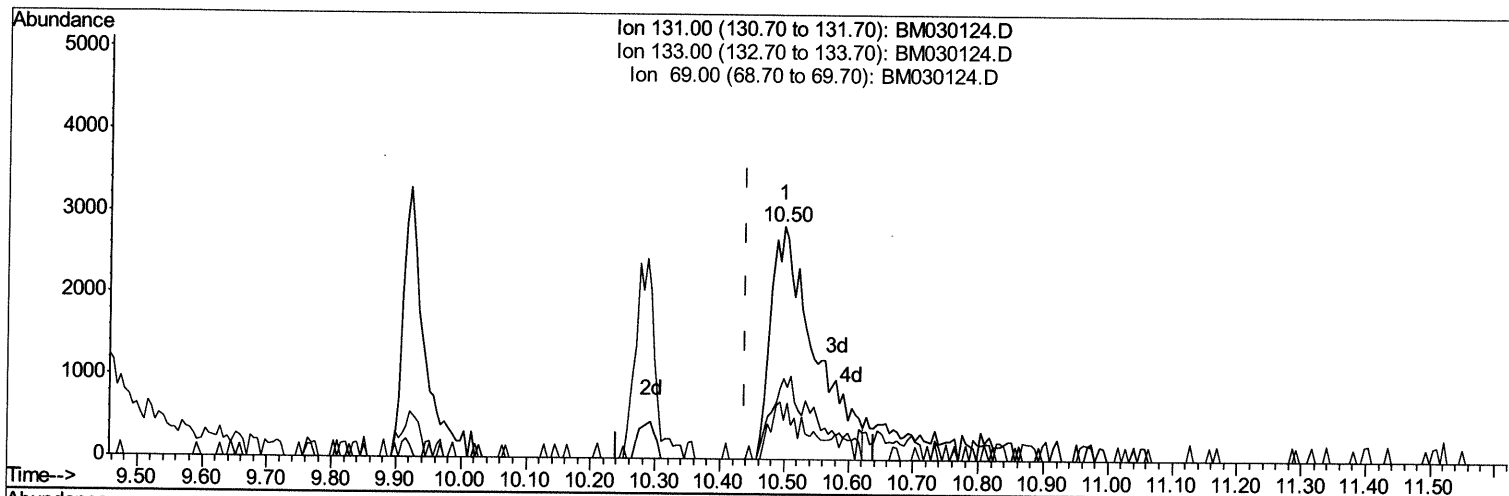

TIC: BM030124.D

(31) 4-Chloroaniline-d4 (S)

10.498min (+0.059) 0.95ng/ul m 05/23/21JU

response 13447

Ion	Exp%	Act%
131.00	100	100
133.00	33.00	34.72
69.00	18.00	16.94
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM052021\
Data File : BM030124.D
Acq On : 21 May 2021 22:06
Operator : CG/JU
Sample : M2474-02
Misc :
ALS Vial : 40 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
GB401

Manual Integrations
APPROVED

mohammad
5/24/2021 1:52:59 PM

Quant Time: May 22 00:31:15 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM050721.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri May 21 23:57:54 2021
Response via : Initial Calibration

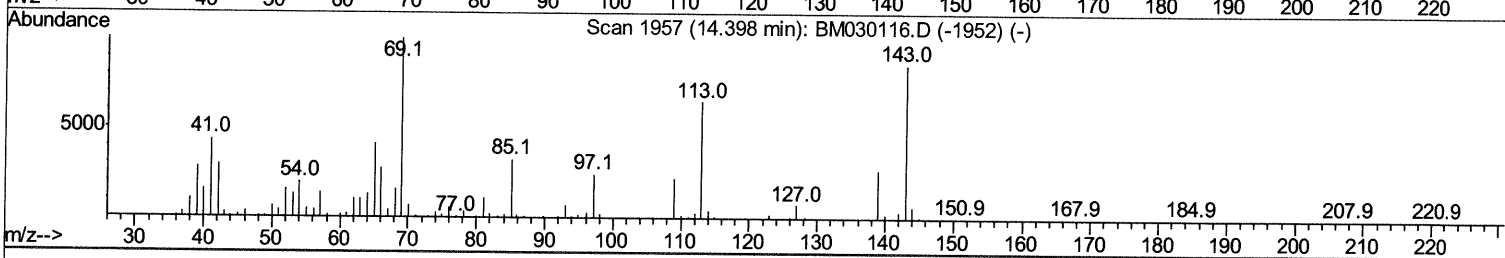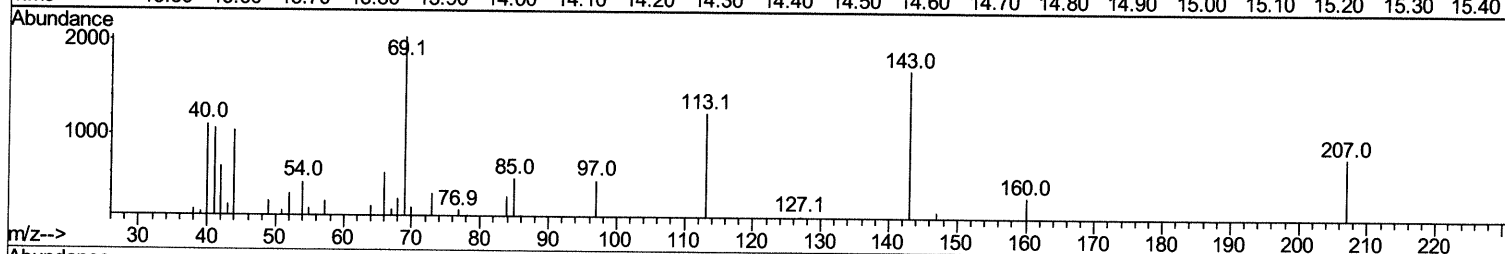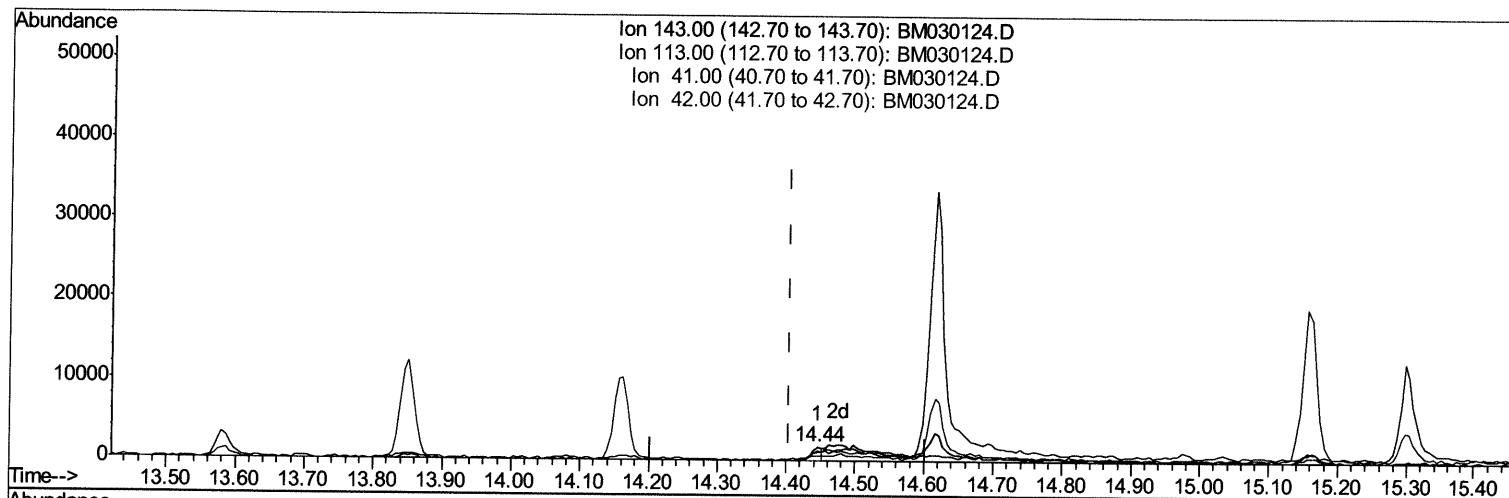

TIC: BM030124.D

(54) 4-Nitrophenol-d4 (S)

14.445min (+0.041) 0.35ng/ul

response 1764

Ion	Exp%	Act%
143.00	100	100
113.00	71.10	73.54
41.00	44.70	62.76#
42.00	28.30	39.60#

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM052021\
 Data File : BM030124.D
 Acq On : 21 May 2021 22:06
 Operator : CG/JU
 Sample : M2474-02
 Misc :
 ALS Vial : 40 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 GB401

Manual Integrations
 APPROVED

mohammad
 5/24/2021 1:52:59 PM

Quant Time: May 22 00:31:15 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM050721.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri May 21 23:57:54 2021
 Response via : Initial Calibration

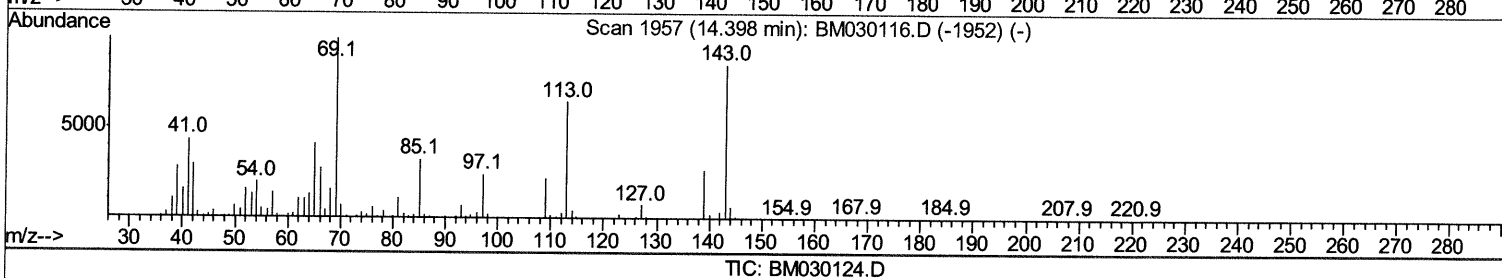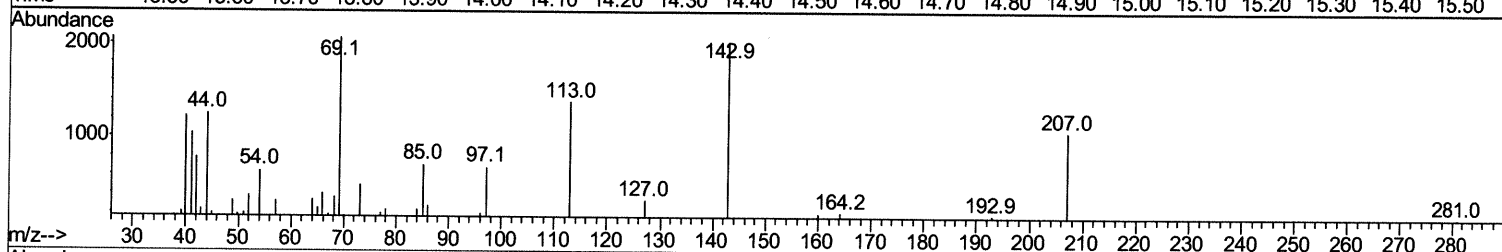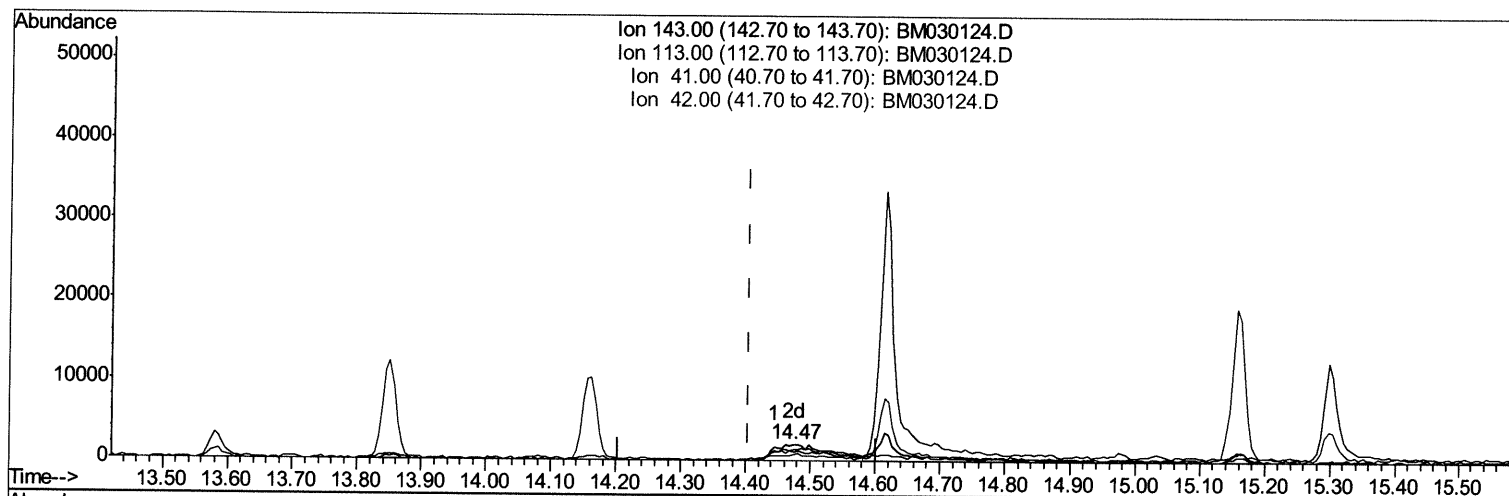

TIC: BM030124.D

(54) 4-Nitrophenol-d4 (S)

14.474min (+0.071) 2.45ng/ul m 5/25/21 JU

response 12200

Ion	Exp%	Act%
143.00	100	100
113.00	71.10	68.22
41.00	44.70	51.93
42.00	28.30	38.91#

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM052021\
 Data File : BM030124.D
 Acq On : 21 May 2021 22:06
 Operator : CG/JU
 Sample : M2474-02
 Misc :
 ALS Vial : 40 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleID :
 GB401

Manual Integrations
 APPROVED

mohammad
 5/24/2021 1:52:59 PM

Quant Time: May 22 00:31:54 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM050721.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri May 21 23:57:54 2021
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.51	152	136014	20.00	ng/ul	0.00
20) Naphthalene-d8	10.28	136	597184	20.00	ng/ul	0.00
38) Acenaphthene-d10	14.16	164	394355	20.00	ng/ul	0.00
64) Phenanthrene-d10	16.91	188	788352	20.00	ng/ul	0.00
79) Chrysene-d12	21.10	240	672759	20.00	ng/ul	0.00
88) Perylene-d12	23.24	264	615852	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.04	96	10389	3.05	ng/uL	0.00
4) Pyridine-d5	0.00	84	0d	0.00	ng/ul	
7) Phenol-d5	6.71	99	62792	4.96	ng/ul	0.00
9) Bis-(2-Chloroethyl)ether-d	6.86	67	217043	27.67	ng/ul	0.00
11) 2-Chlorophenol-d4	7.05	132	225622	23.11	ng/ul	0.00
15) 4-Methylphenol-d8	8.23	113	128369	12.27	ng/ul	0.00
21) Nitrobenzene-d5	8.67	128	131922	32.06	ng/ul	0.00
24) 2-Nitrophenol-d4	9.38	143	146536	31.55	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	9.92	165	233507	25.07	ng/ul	0.00
31) 4-Chloroaniline-d4	10.50	131	13447m >	0.95	ng/ul >	0.06051851317d
46) Dimethylphthalate-d6	13.59	166	974253	31.87	ng/ul	0.00
49) Acenaphthylene-d8	13.85	160	1170422	30.21	ng/ul	0.00
54) 4-Nitrophenol-d4	14.47	143	12200m >	2.45	ng/ul >	0.07051851317d
60) Fluorene-d10	15.16	176	855384	32.96	ng/ul	0.00
65) 4,6-Dinitro-2-methylphenol	15.30	200	162348	31.70	ng/ul	0.00
73) Anthracene-d10	17.01	188	1420207	35.77	ng/ul	0.00
81) Pyrene-d10	19.31	212	1583971	45.90	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.11	264	1297501	37.17	ng/ul	0.00

Target Compounds

Target Compounds	R.T.	QIon	Response	Conc	Units	Ovalue
47) Dimethylphthalate	13.63	163	54656	1.786	ng/ul	99

(#) = qualifier out of range (m) = manual integration (+) = signals summed