


Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM052021\
Data File : BM030140.D
Acq On : 22 May 2021 08:23
Operator : CG/JU
Sample : M2474-13
Misc :
ALS Vial : 56 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
GB410

Manual Integrations
APPROVED

mohammad
5/24/2021 1:53:46 PM

Quant Time: May 24 01:22:14 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM050721.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu May 20 12:00:20 2021
Response via : Initial Calibration

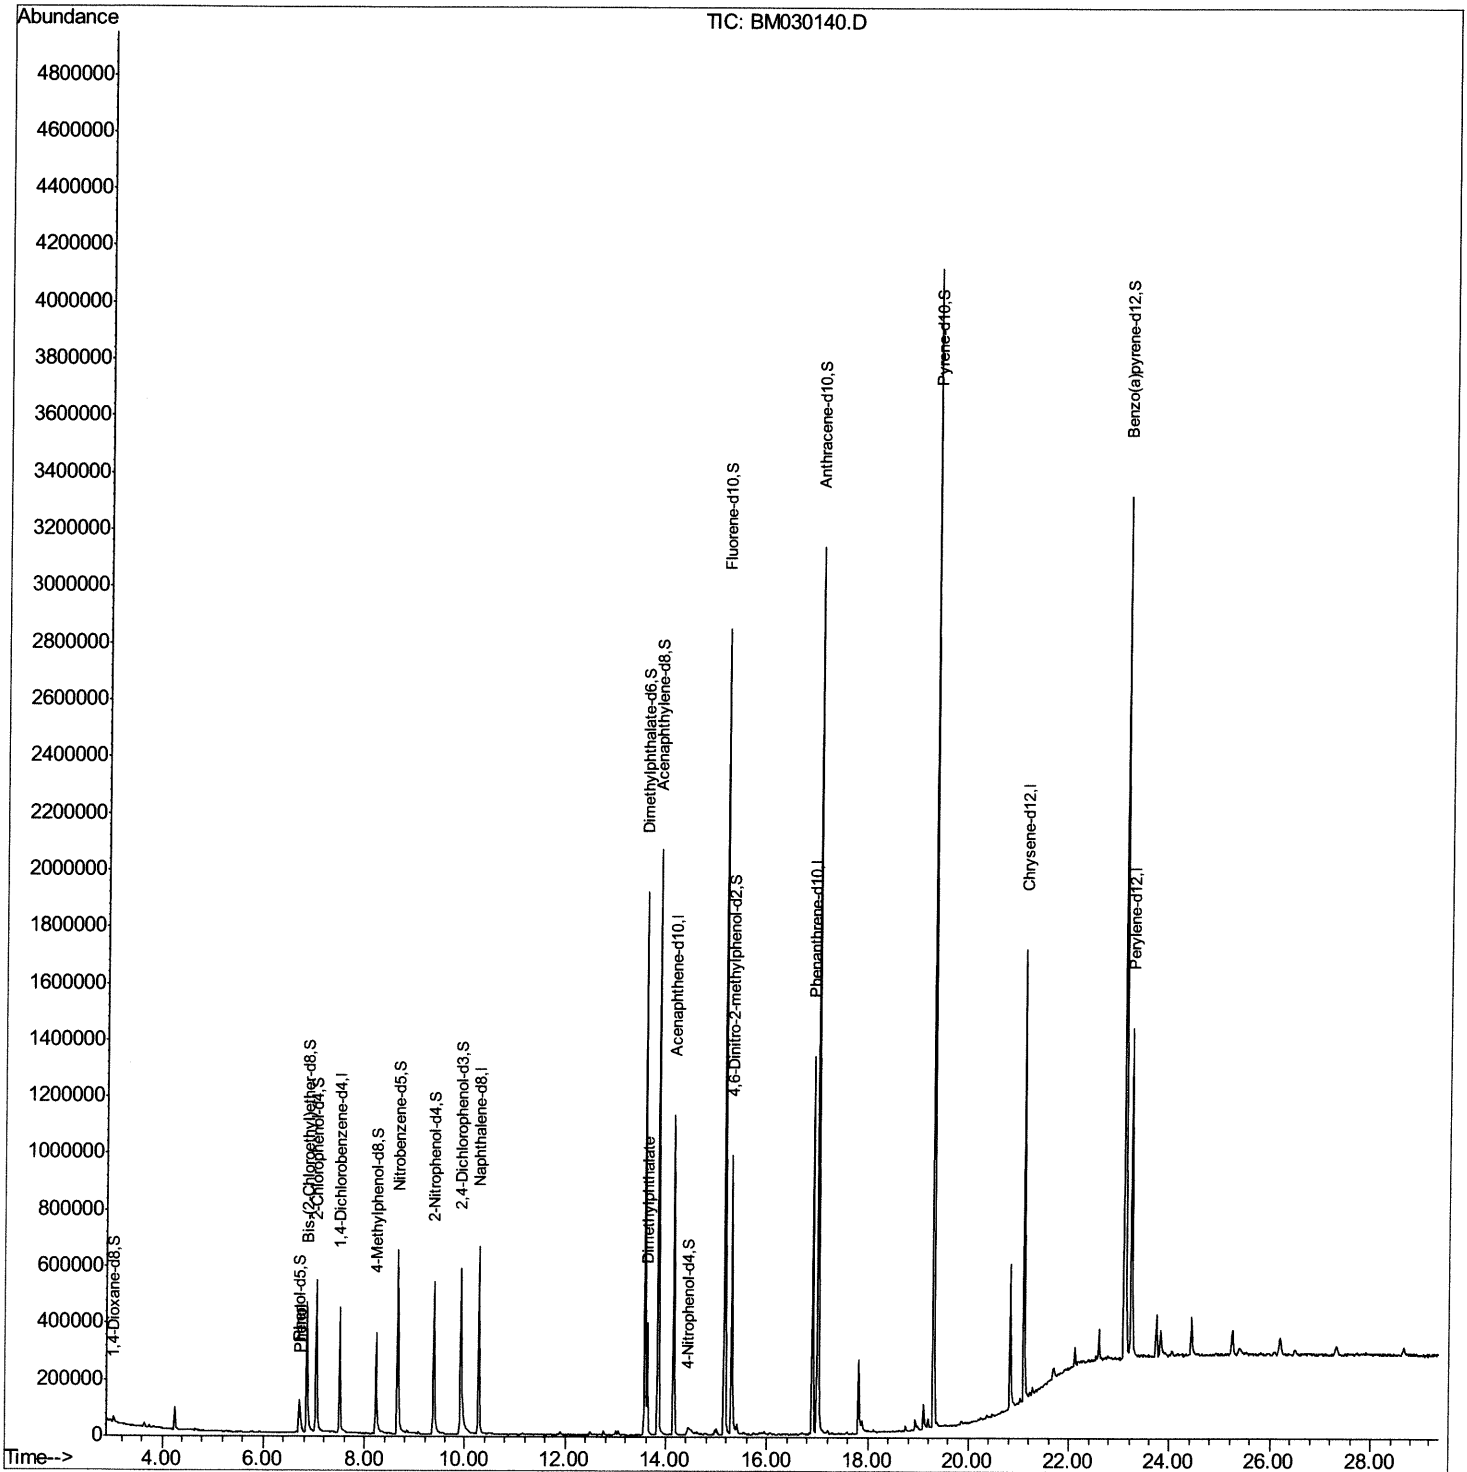

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM052021\
 Data File : BM030140.D
 Acq On : 22 May 2021 08:23
 Operator : CG/JU
 Sample : M2474-13
 Misc :
 ALS Vial : 56 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 GB410

Manual Integrations
 APPROVED

mohammad
 5/24/2021 1:53:46 PM

Quant Time: May 24 01:20:02 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM050721.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu May 20 12:00:20 2021
 Response via : Initial Calibration

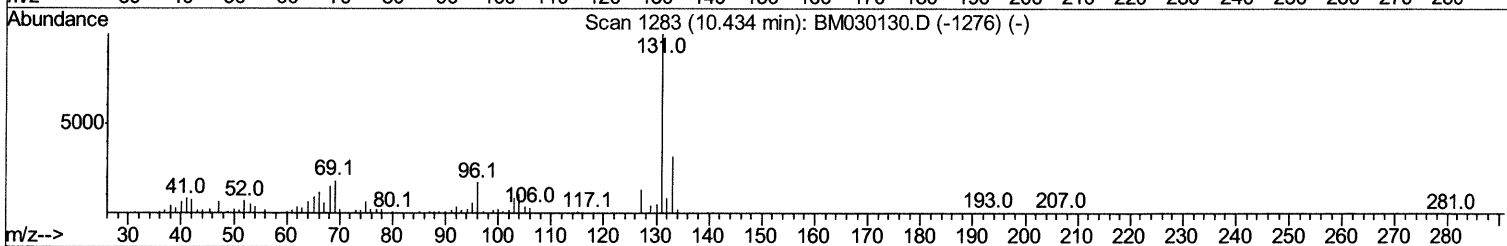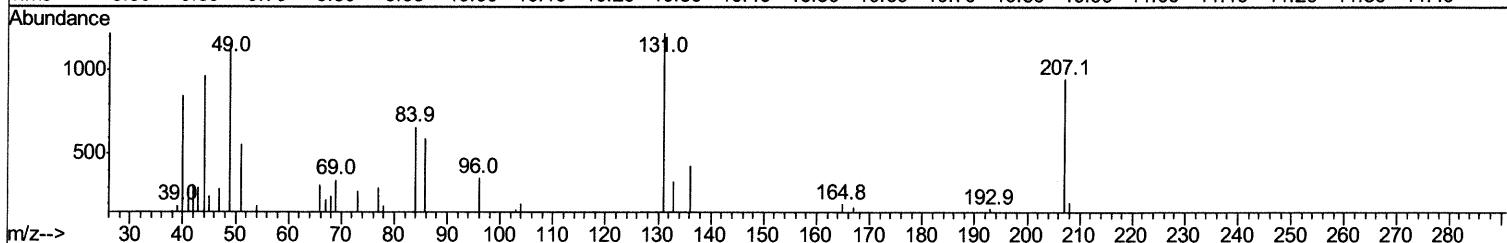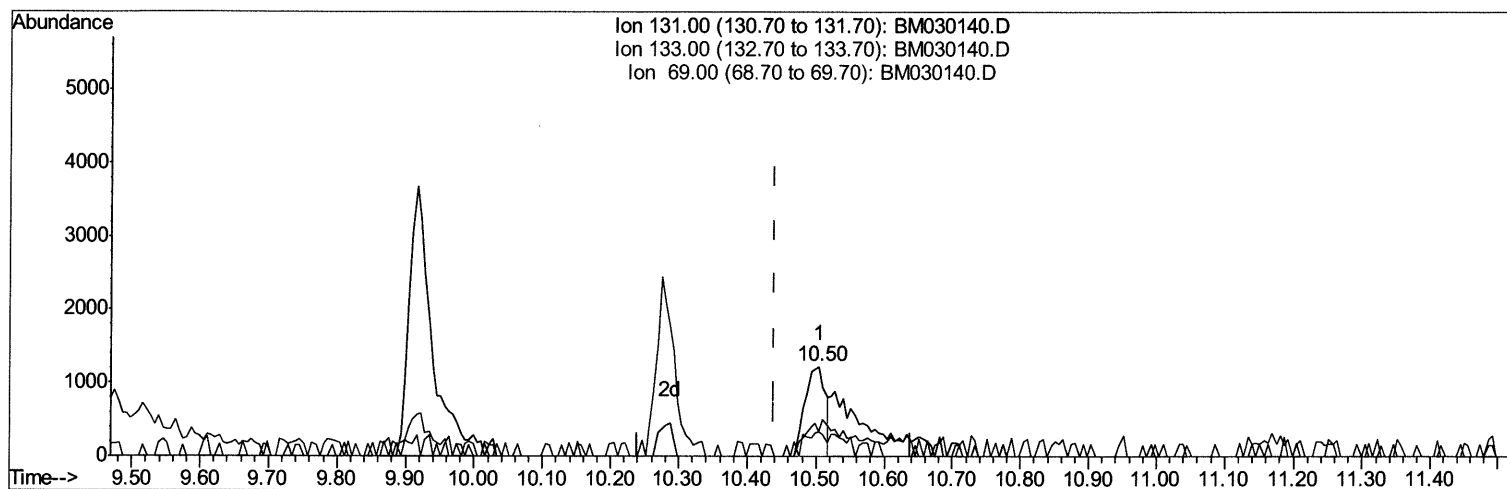

TIC: BM030140.D

(31) 4-Chloroaniline-d4 (S)

10.504min (+0.065) 0.20ng/ul

response 2510

Ion	Exp%	Act%
131.00	100	100
133.00	33.00	27.17
69.00	18.00	27.99#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM052021\
 Data File : BM030140.D
 Acq On : 22 May 2021 08:23
 Operator : CG/JU
 Sample : M2474-13
 Misc :
 ALS Vial : 56 Sample Multiplier: 1

Instrument :
 BNA_M
ClientSampleId :
 GB410

Manual Integrations
APPROVED

mohammad
 5/24/2021 1:53:46 PM

Quant Time: May 24 01:20:02 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM050721.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu May 20 12:00:20 2021
 Response via : Initial Calibration

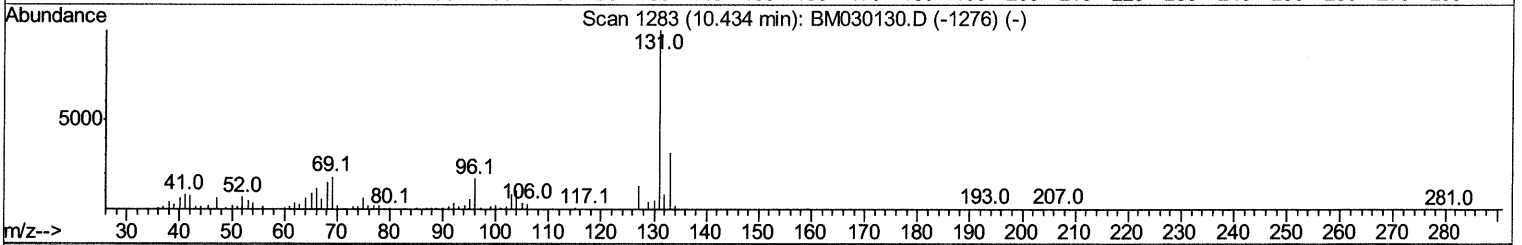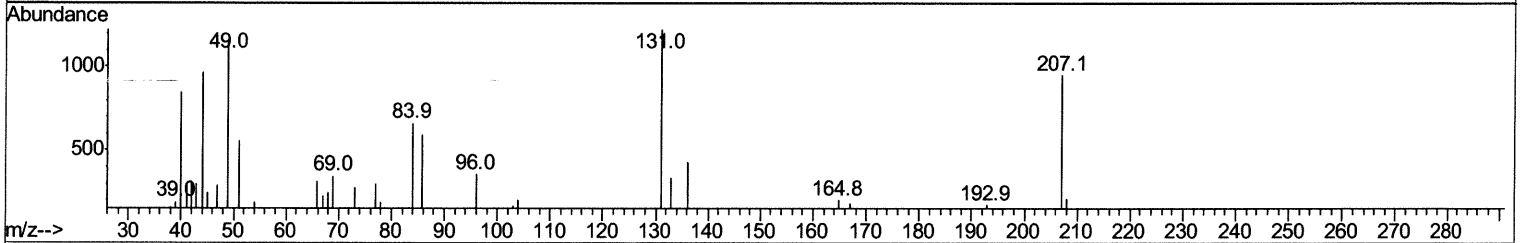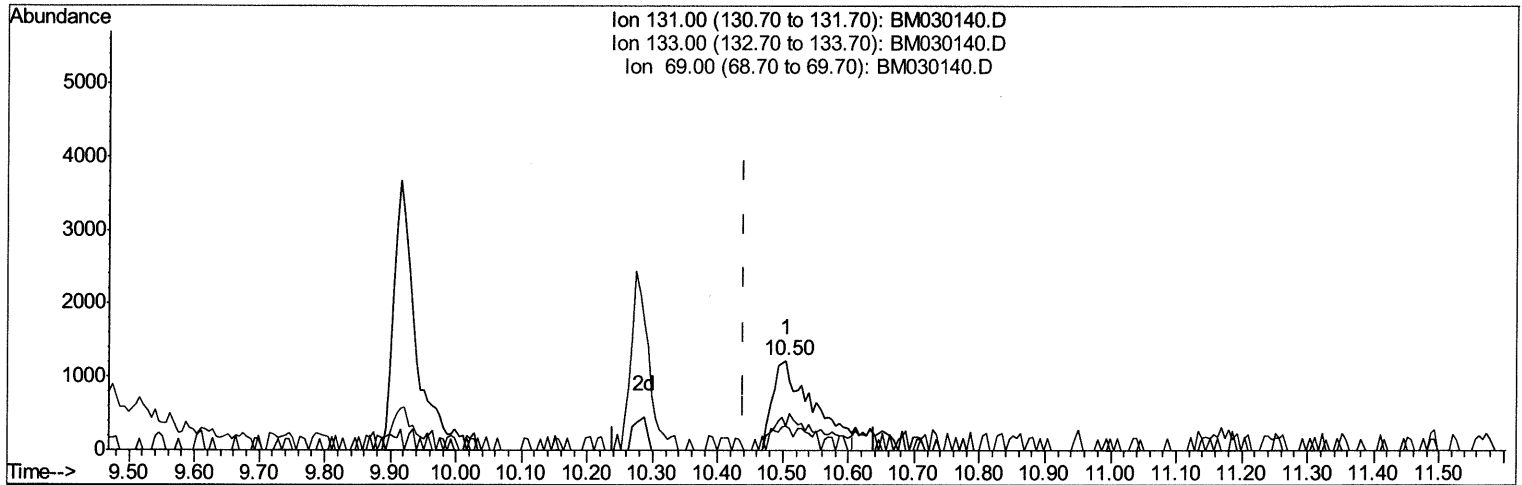

TIC: BM030140.D

(31) 4-Chloroaniline-d4 (S)

10.504min (+0.065) 0.41ng/ul m 05/25/21 JU

response 5247

Ion	Exp%	Act%
131.00	100	100
133.00	33.00	27.17
69.00	18.00	27.99#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM052021\
 Data File : BM030140.D
 Acq On : 22 May 2021 08:23
 Operator : CG/JU
 Sample : M2474-13
 Misc :
 ALS Vial : 56 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 GB410

Manual Integrations
 APPROVED

mohammad
 5/24/2021 1:53:46 PM

Quant Time: May 24 01:21:20 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM050721.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu May 20 12:00:20 2021
 Response via : Initial Calibration

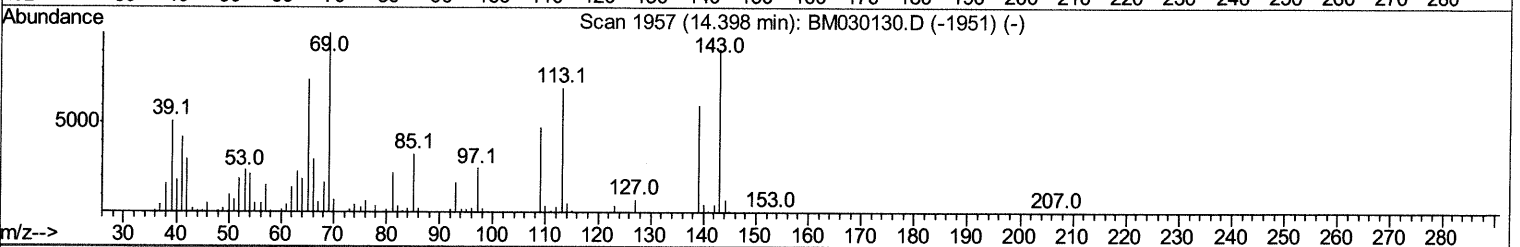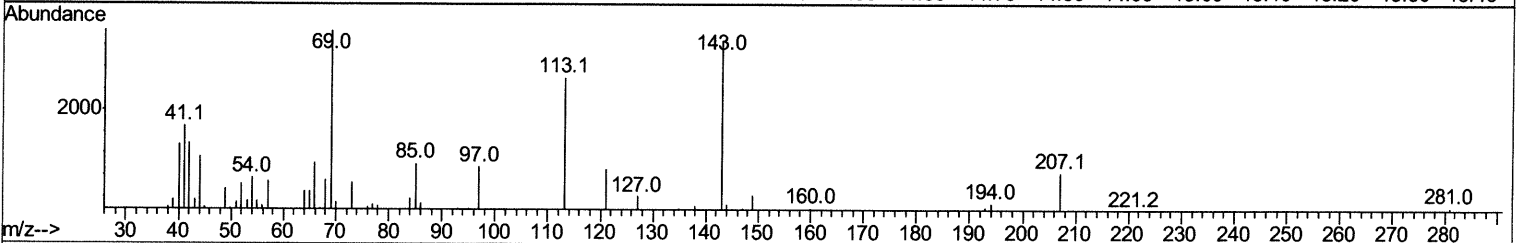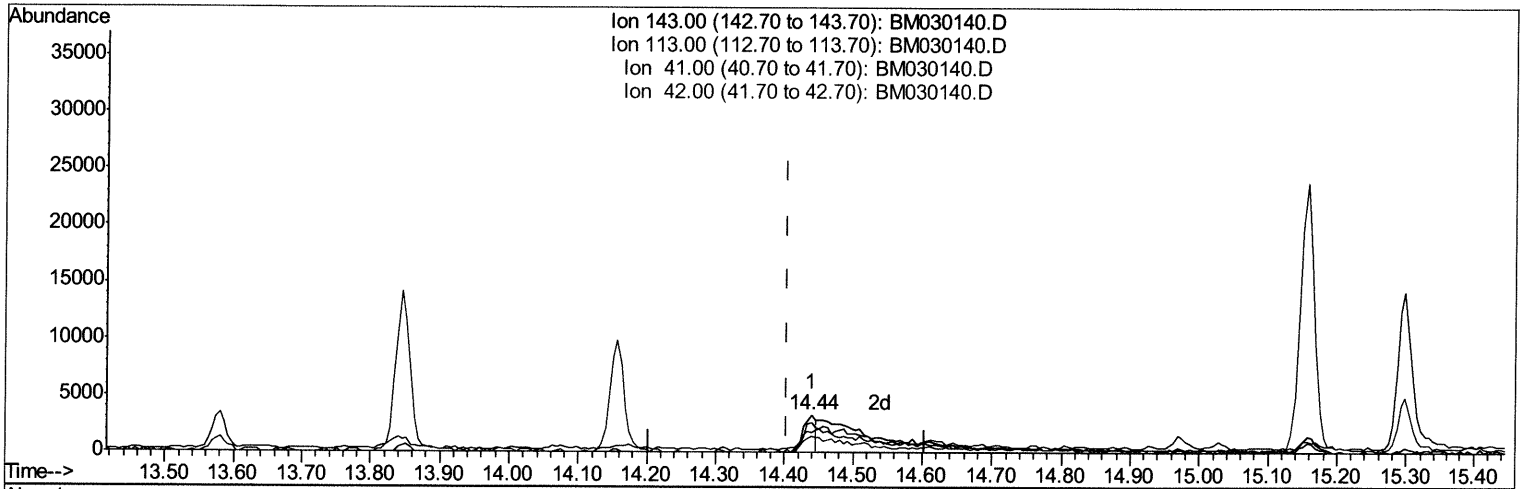

TIC: BM030140.D

(54) 4-Nitrophenol-d4 (S)

14.439min (+0.036) 0.90ng/ul

response 4147

Ion	Exp%	Act%
143.00	100	100
113.00	71.10	79.23
41.00	44.70	52.03
42.00	28.30	42.36#

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM052021\
 Data File : BM030140.D
 Acq On : 22 May 2021 08:23
 Operator : CG/JU
 Sample : M2474-13
 Misc :
 ALS Vial : 56 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 GB410

Manual Integrations
 APPROVED

mohammad
 5/24/2021 1:53:46 PM

Quant Time: May 24 01:21:20 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM050721.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu May 20 12:00:20 2021
 Response via : Initial Calibration

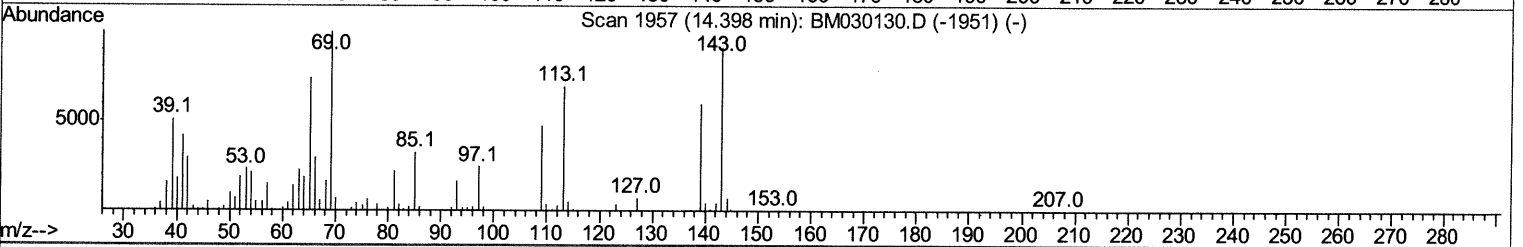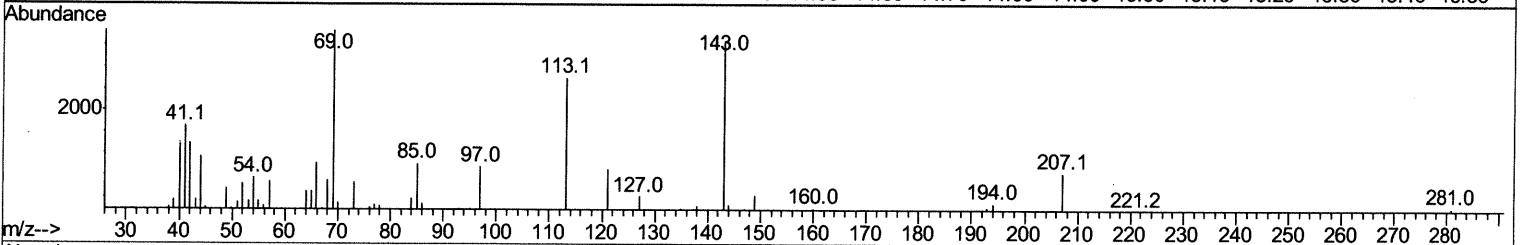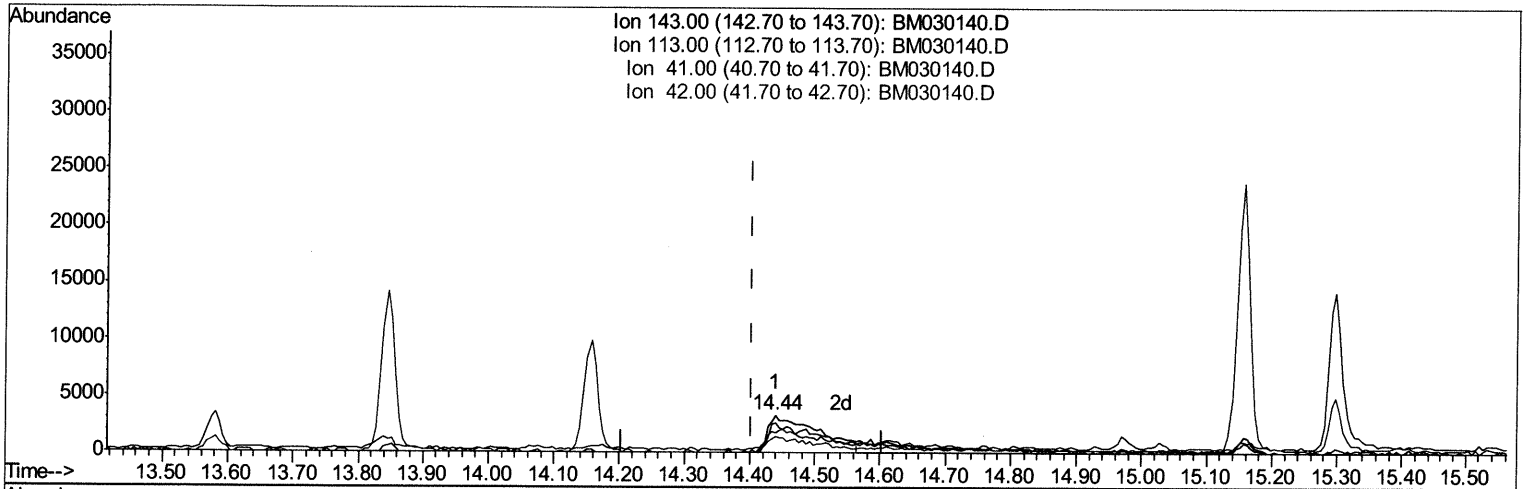

TIC: BM030140.D

(54) 4-Nitrophenol-d4 (S)

14.439min (+0.036) 3.79ng/ul m 65125121JU

response 17373

Ion	Exp%	Act%
143.00	100	100
113.00	71.10	79.23
41.00	44.70	52.03
42.00	28.30	42.36#

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM052021\
 Data File : BM030140.D
 Acq On : 22 May 2021 08:23
 Operator : CG/JU
 Sample : M2474-13
 Misc :
 ALS Vial : 56 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 GB410

Manual Integrations
 APPROVED

mohammad
 5/24/2021 1:53:46 PM

Quant Time: May 24 01:22:14 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM050721.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu May 20 12:00:20 2021
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.50	152	121341	20.00	ng/ul	-0.01
20) Naphthalene-d8	10.27	136	535003	20.00	ng/ul	-0.01
38) Acenaphthene-d10	14.16	164	363309	20.00	ng/ul	0.00
64) Phenanthrene-d10	16.90	188	759850	20.00	ng/ul	-0.01
79) Chrysene-d12	21.10	240	786812	20.00	ng/ul	0.00
88) Perylene-d12	23.24	264	771064	20.00	ng/ul	-0.01

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.03	96	11483	3.78	ng/uL	0.00
4) Pyridine-d5	0.00	84	0d	0.00	ng/ul	
7) Phenol-d5	6.70	99	71337	6.32	ng/ul	0.00
9) Bis-(2-Chloroethyl)ether-d	6.86	67	244257	34.91	ng/ul	0.00
11) 2-Chlorophenol-d4	7.05	132	255595	29.35	ng/ul	0.00
15) 4-Methylphenol-d8	8.23	113	150054	16.08	ng/ul	0.00
21) Nitrobenzene-d5	8.66	128	151871	41.19	ng/ul	0.00
24) 2-Nitrophenol-d4	9.38	143	172109	41.36	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	9.92	165	274567	32.91	ng/ul	0.00
31) 4-Chloroaniline-d4	10.50	131	5247m>	0.41	ng/ul>	0.0705/25/21JU
46) Dimethylphthalate-d6	13.58	166	1163622	41.32	ng/ul	0.00
49) Acenaphthylene-d8	13.85	160	1376654	38.58	ng/ul	0.00
54) 4-Nitrophenol-d4	14.44	143	17373m>	3.79	ng/ul>	0.0405/25/21JU
60) Fluorene-d10	15.16	176	1033996	43.25	ng/ul	0.00
65) 4,6-Dinitro-2-methylphenol	15.30	200	194607	39.43	ng/ul	0.00
73) Anthracene-d10	17.00	188	1670518	43.66	ng/ul	0.00
81) Pyrene-d10	19.30	212	1969774	48.80	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.10	264	1958018	44.80	ng/ul	-0.01

Target Compounds

					Ovalue
8) Phenol	6.73	94	20045	1.740	ng/ul 93
47) Dimethylphthalate	13.63	163	242067	8.585	ng/ul 99

(#) = qualifier out of range (m) = manual integration (+) = signals summed