

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM052021\
 Data File : BM030089.D
 Acq On : 20 May 2021 14:12
 Operator : CG/JU
 Sample : M2463-12
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 GB3Z7

Quant Time: May 20 14:46:03 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM050721.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu May 20 12:00:20 2021
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.51	152	142447	20.00	ng/ul	0.00
20) Naphthalene-d8	10.29	136	580175	20.00	ng/ul	0.00
38) Acenaphthene-d10	14.16	164	350927	20.00	ng/ul	0.00
64) Phenanthrene-d10	16.92	188	670368	20.00	ng/ul	0.00
79) Chrysene-d12	21.11	240	635615	20.00	ng/ul	0.00
88) Perylene-d12	23.25	264	690528	20.00	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.03	96	20259	5.68	ng/uL	0.00
4) Pyridine-d5	3.45	84	216150	24.20	ng/ul	0.00
7) Phenol-d5	6.70	99	343231	25.91	ng/ul	0.00
9) Bis-(2-Chloroethyl)ether-d	6.86	67	227881	27.74	ng/ul	0.00
11) 2-Chlorophenol-d4	7.05	132	288345	28.20	ng/ul	0.00
15) 4-Methylphenol-d8	8.23	113	269307	24.58	ng/ul	0.00
21) Nitrobenzene-d5	8.67	128	124404	31.12	ng/ul	0.00
24) 2-Nitrophenol-d4	9.39	143	144575	32.04	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	9.92	165	241211	26.66	ng/ul	0.00
31) 4-Chloroaniline-d4	10.44	131	329554	23.93	ng/ul	0.00
46) Dimethylphthalate-d6	13.59	166	839221	30.85	ng/ul	0.00
49) Acenaphthylene-d8	13.86	160	1022526	29.66	ng/ul	0.00
54) 4-Nitrophenol-d4	14.42	143	66830	15.08	ng/ul	0.01
60) Fluorene-d10	15.16	176	712281	30.85	ng/ul	0.00
65) 4,6-Dinitro-2-methylphenol	15.31	200	124024	28.48	ng/ul	0.00
73) Anthracene-d10	17.02	188	1083368	32.09	ng/ul	0.00
81) Pyrene-d10	19.32	212	1187182	36.41	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.12	264	1253147	32.01	ng/ul	0.00
Target Compounds						
2) 1,4-Dioxane	3.07	88	12097	3.134	ng/uL	Ovalue 96


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM052021\
Data File : BM030089.D
Acq On : 20 May 2021 14:12
Operator : CG/JU
Sample : M2463-12
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
GB3Z7

Quant Time: May 20 14:46:03 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM050721.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu May 20 12:00:20 2021
Response via : Initial Calibration

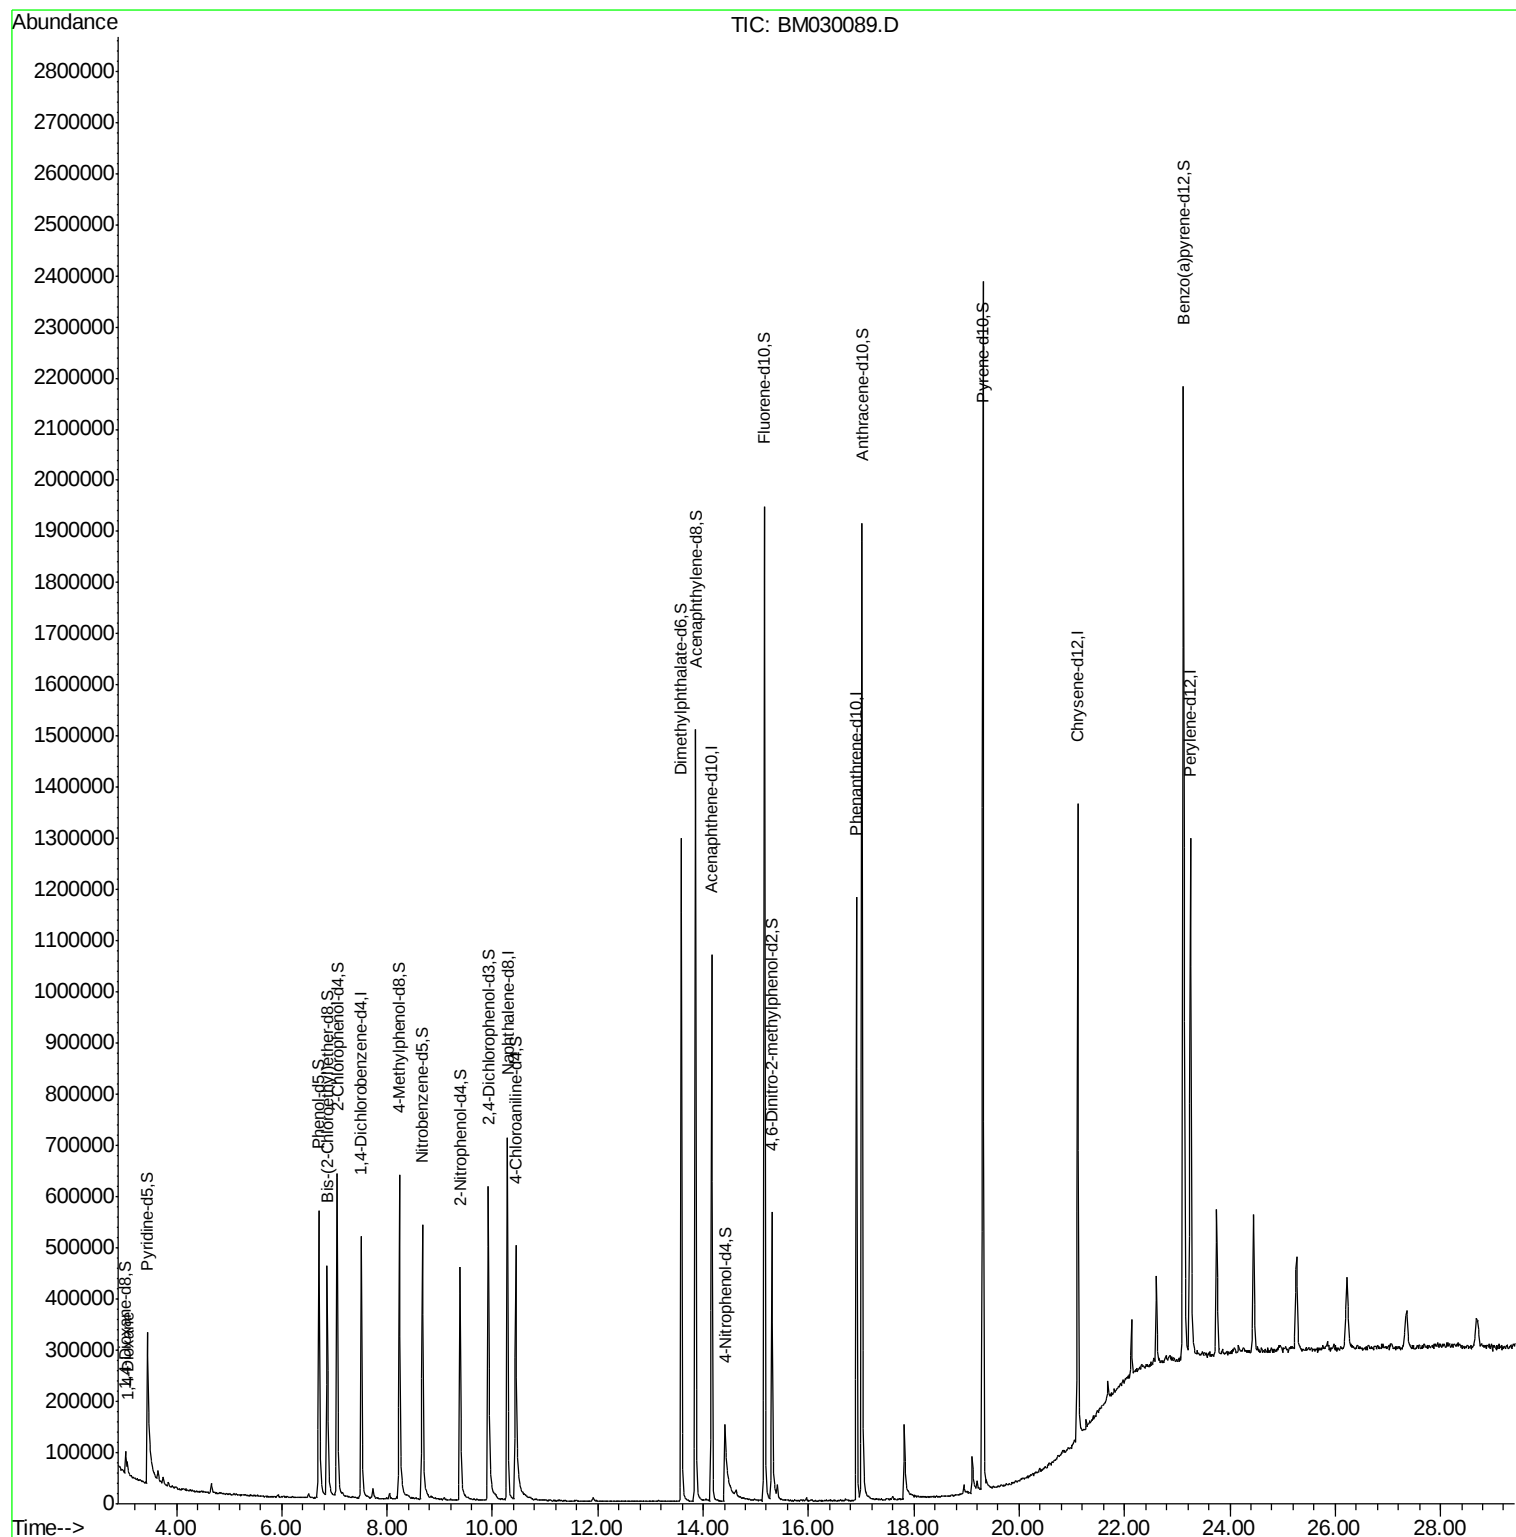

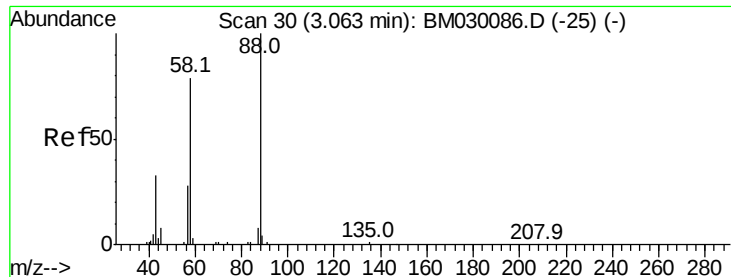

#2
 1,4-Dioxane
 Concen: 3.134 ng/uL
 RT: 3.07 min Scan# 31
 Delta R.T. 0.01 min
 Lab File: BM030089.D
 Acq: 20 May 2021 14:12

Instrument :
 BNA_M
 ClientSampleId :
 GB3Z7

Tot Ion: 88 Resp: 12097
 Ion Ratio Lower Upper
 88 100
 43 35.0 26.2 39.2
 58 77.6 59.0 88.4

