

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM052021\
 Data File : BM030101.D
 Acq On : 20 May 2021 22:09
 Operator : CG/JU
 Sample : M2463-05
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 GB3Y8

Manual Integrations
 APPROVED

mohammad
 5/21/2021 3:38:20 PM

Quant Time: May 21 01:41:33 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM050721.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu May 20 12:00:20 2021
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.51	152	155536	20.00	ng/ul	0.00
20) Naphthalene-d8	10.28	136	663861	20.00	ng/ul	0.00
38) Acenaphthene-d10	14.16	164	431054	20.00	ng/ul	0.00
64) Phenanthrene-d10	16.91	188	807583	20.00	ng/ul	0.00
79) Chrysene-d12	21.10	240	658523	20.00	ng/ul	0.00
88) Perylene-d12	23.24	264	666500	20.00	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.04	96	14636	3.76	ng/uL	0.00
4) Pyridine-d5	0.00	84	0d	0.00	ng/ul	0.00
7) Phenol-d5	6.71	99	61751	4.27	ng/ul	0.00
9) Bis-(2-Chloroethyl)ether-d	6.86	67	205231	22.88	ng/ul	0.00
11) 2-Chlorophenol-d4	7.05	132	221317	19.83	ng/ul	0.00
15) 4-Methylphenol-d8	8.23	113	123662	10.34	ng/ul	0.00
21) Nitrobenzene-d5	8.67	128	127093	27.78	ng/ul	0.00
24) 2-Nitrophenol-d4	9.39	143	139572	27.03	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	9.92	165	223509	21.59	ng/ul	0.00
31) 4-Chloroaniline-d4	10.51	131	10762m	0.68	ng/ul	0.07
46) Dimethylphthalate-d6	13.59	166	924625	27.67	ng/ul	0.00
49) Acenaphthylene-d8	13.85	160	1125350	26.58	ng/ul	0.00
54) 4-Nitrophenol-d4	14.49	143	10249m	1.88	ng/ul	0.08
60) Fluorene-d10	15.16	176	821376	28.96	ng/ul	0.00
65) 4,6-Dinitro-2-methylphenol	15.30	200	152344	29.04	ng/ul	0.00
73) Anthracene-d10	17.01	188	1360627	33.46	ng/ul	0.00
81) Pyrene-d10	19.31	212	1398124	41.39	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.11	264	1280507	33.89	ng/ul	0.00
Target Compounds						
47) Dimethylphthalate	13.63	163	37093	1.109	ng/ul	Ovalue 98

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM052021\
Data File : BM030101.D
Acq On : 20 May 2021 22:09
Operator : CG/JU
Sample : M2463-05
Misc :
ALS Vial : 17 Sample Multiplier: 1


Instrument :
BNA_M
ClientSampleId :
GB3Y8

Manual Integrations
APPROVED

mohammad
5/21/2021 3:38:20 PM

Quant Time: May 21 01:41:33 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM050721.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu May 20 12:00:20 2021
Response via : Initial Calibration

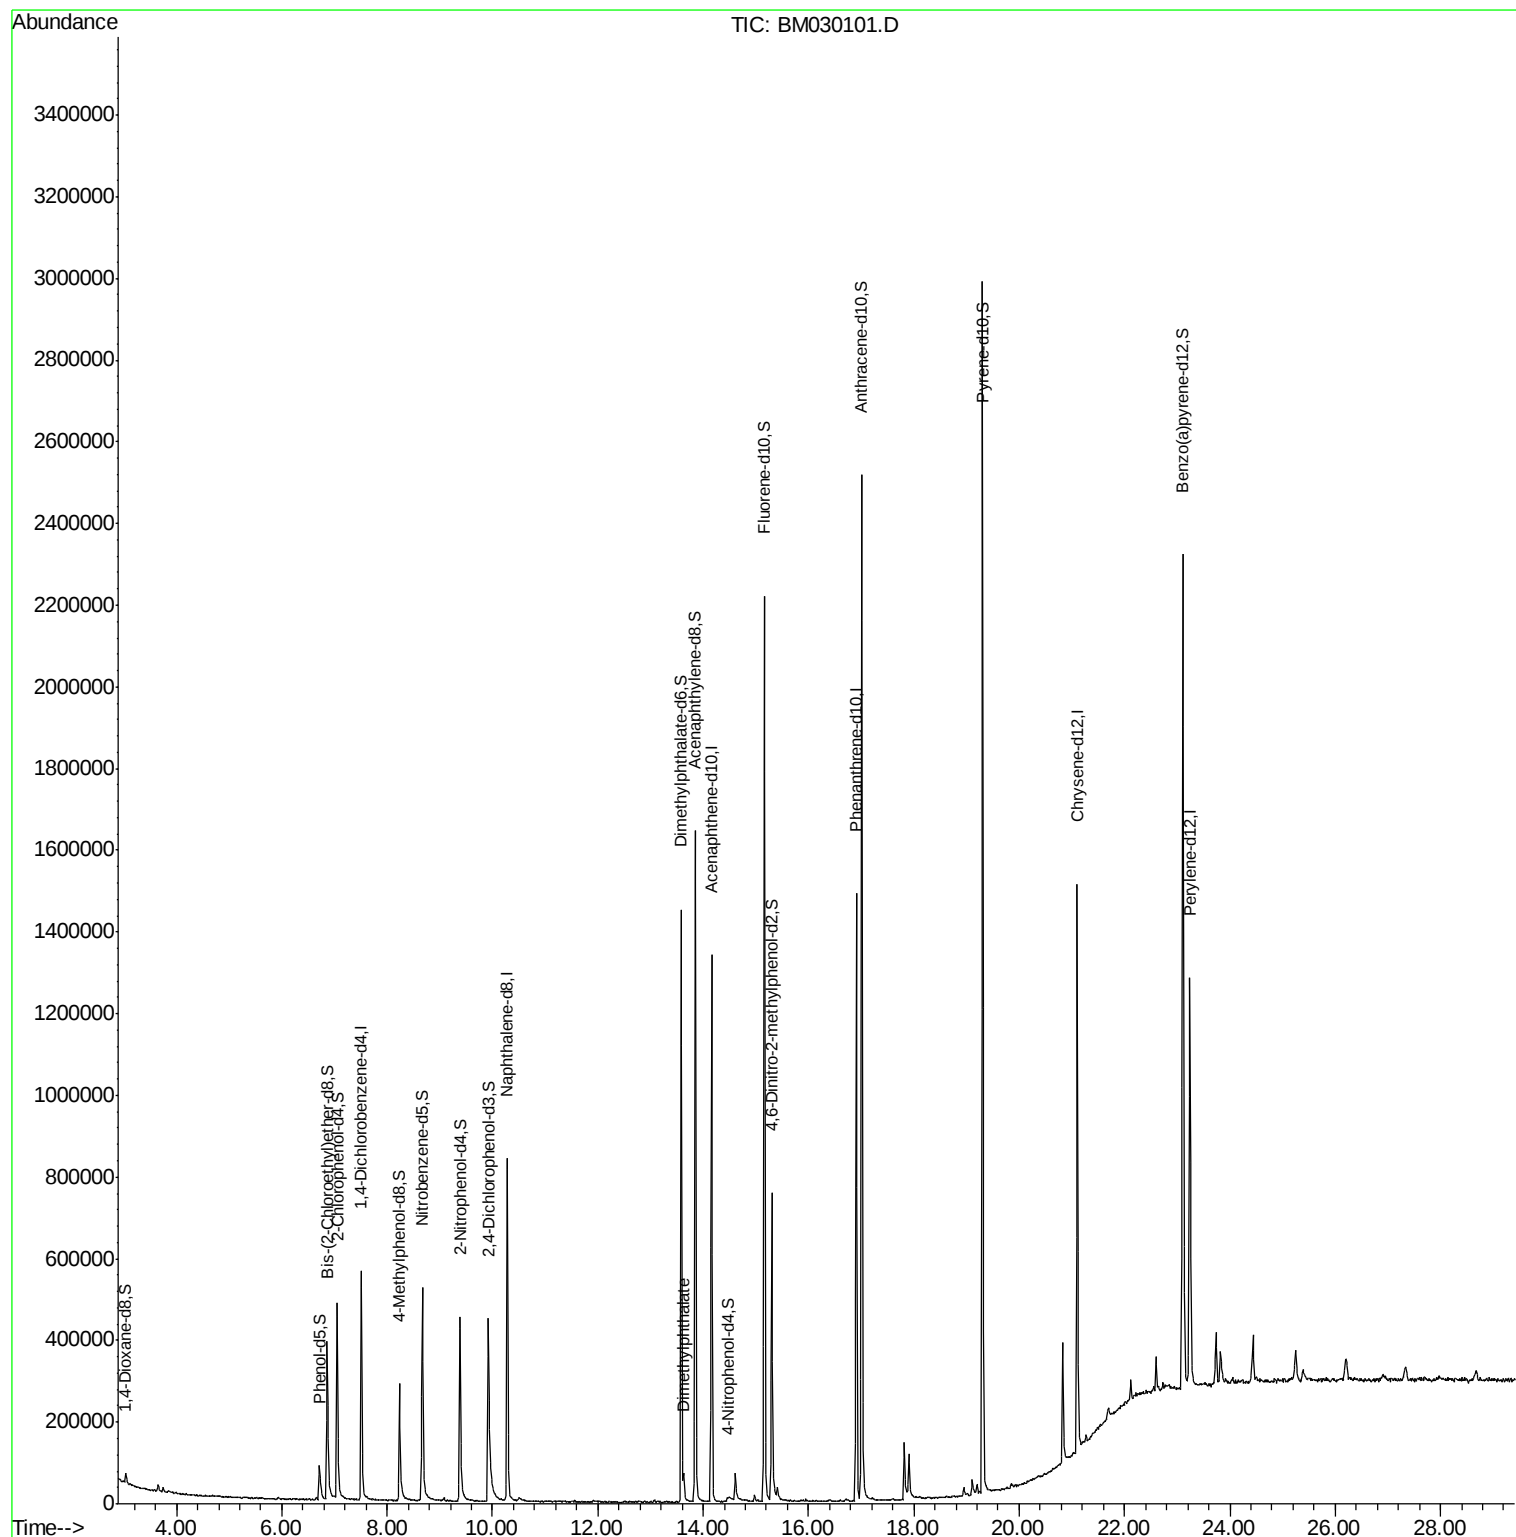

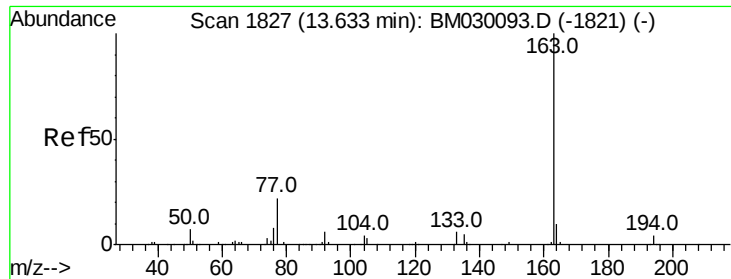

#47
 Dimethylphthalate
 Concen: 1.109 ng/ul
 RT: 13.63 min Scan# 1827
 Delta R.T. 0.00 min
 Lab File: BM030101.D
 Acq: 20 May 2021 22:09

Instrument :
 BNA_M
 ClientSampleId :
 GB3Y8

Tot Ion	Ratio	Lower	Upper
163	100		
194	3.9	3.4	5.0
164	10.9	7.8	11.8

Manual Integrations
 APPROVED

mohammad
 5/21/2021 3:38:20 PM

