

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM052021\
 Data File : BM030103.D
 Acq On : 20 May 2021 23:22
 Operator : CG/JU
 Sample : M2463-04
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 GB3Y7

Manual Integrations
 APPROVED

mohammad
 5/21/2021 3:38:28 PM

Quant Time: May 21 01:51:23 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM050721.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu May 20 12:00:20 2021
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.51	152	155664	20.00	ng/ul	0.00
20) Naphthalene-d8	10.28	136	665719	20.00	ng/ul	0.00
38) Acenaphthene-d10	14.16	164	405679	20.00	ng/ul	0.00
64) Phenanthrene-d10	16.91	188	750600	20.00	ng/ul	0.00
79) Chrysene-d12	21.10	240	664003	20.00	ng/ul	0.00
88) Perylene-d12	23.24	264	694398	20.00	ng/ul	-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.03	96	14000	3.59	ng/uL	0.00
4) Pyridine-d5	0.00	84	0d	0.00	ng/ul	
7) Phenol-d5	6.71	99	67272	4.65	ng/ul	0.00
9) Bis-(2-Chloroethyl)ether-d	6.86	67	241645	26.92	ng/ul	0.00
11) 2-Chlorophenol-d4	7.05	132	249026	22.29	ng/ul	0.00
15) 4-Methylphenol-d8	8.23	113	140441	11.73	ng/ul	0.00
21) Nitrobenzene-d5	8.67	128	139359	30.38	ng/ul	0.00
24) 2-Nitrophenol-d4	9.39	143	160877	31.07	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	9.92	165	252392	24.31	ng/ul	0.00
31) 4-Chloroaniline-d4	10.50	131	12483m	0.79	ng/ul	0.06
46) Dimethylphthalate-d6	13.59	166	962437	30.61	ng/ul	0.00
49) Acenaphthylene-d8	13.85	160	1203924	30.21	ng/ul	0.00
54) 4-Nitrophenol-d4	14.51	143	11004m	2.15	ng/ul	0.11
60) Fluorene-d10	15.16	176	845017	31.66	ng/ul	0.00
65) 4,6-Dinitro-2-methylphenol	15.30	200	143411	29.41	ng/ul	0.00
73) Anthracene-d10	17.01	188	1328262	35.14	ng/ul	0.00
81) Pyrene-d10	19.31	212	1425541	41.85	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.11	264	1386185	35.22	ng/ul	0.00
Target Compounds						
47) Dimethylphthalate	13.63	163	61627	1.957	ng/ul	Ovalue 98

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM052021\
Data File : BM030103.D
Acq On : 20 May 2021 23:22
Operator : CG/JU
Sample : M2463-04
Misc :
ALS Vial : 19 Sample Multiplier: 1


Instrument :
BNA_M
ClientSampleId :
GB3Y7

Manual Integrations
APPROVED

mohammad
5/21/2021 3:38:28 PM

Quant Time: May 21 01:51:23 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM050721.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu May 20 12:00:20 2021
Response via : Initial Calibration

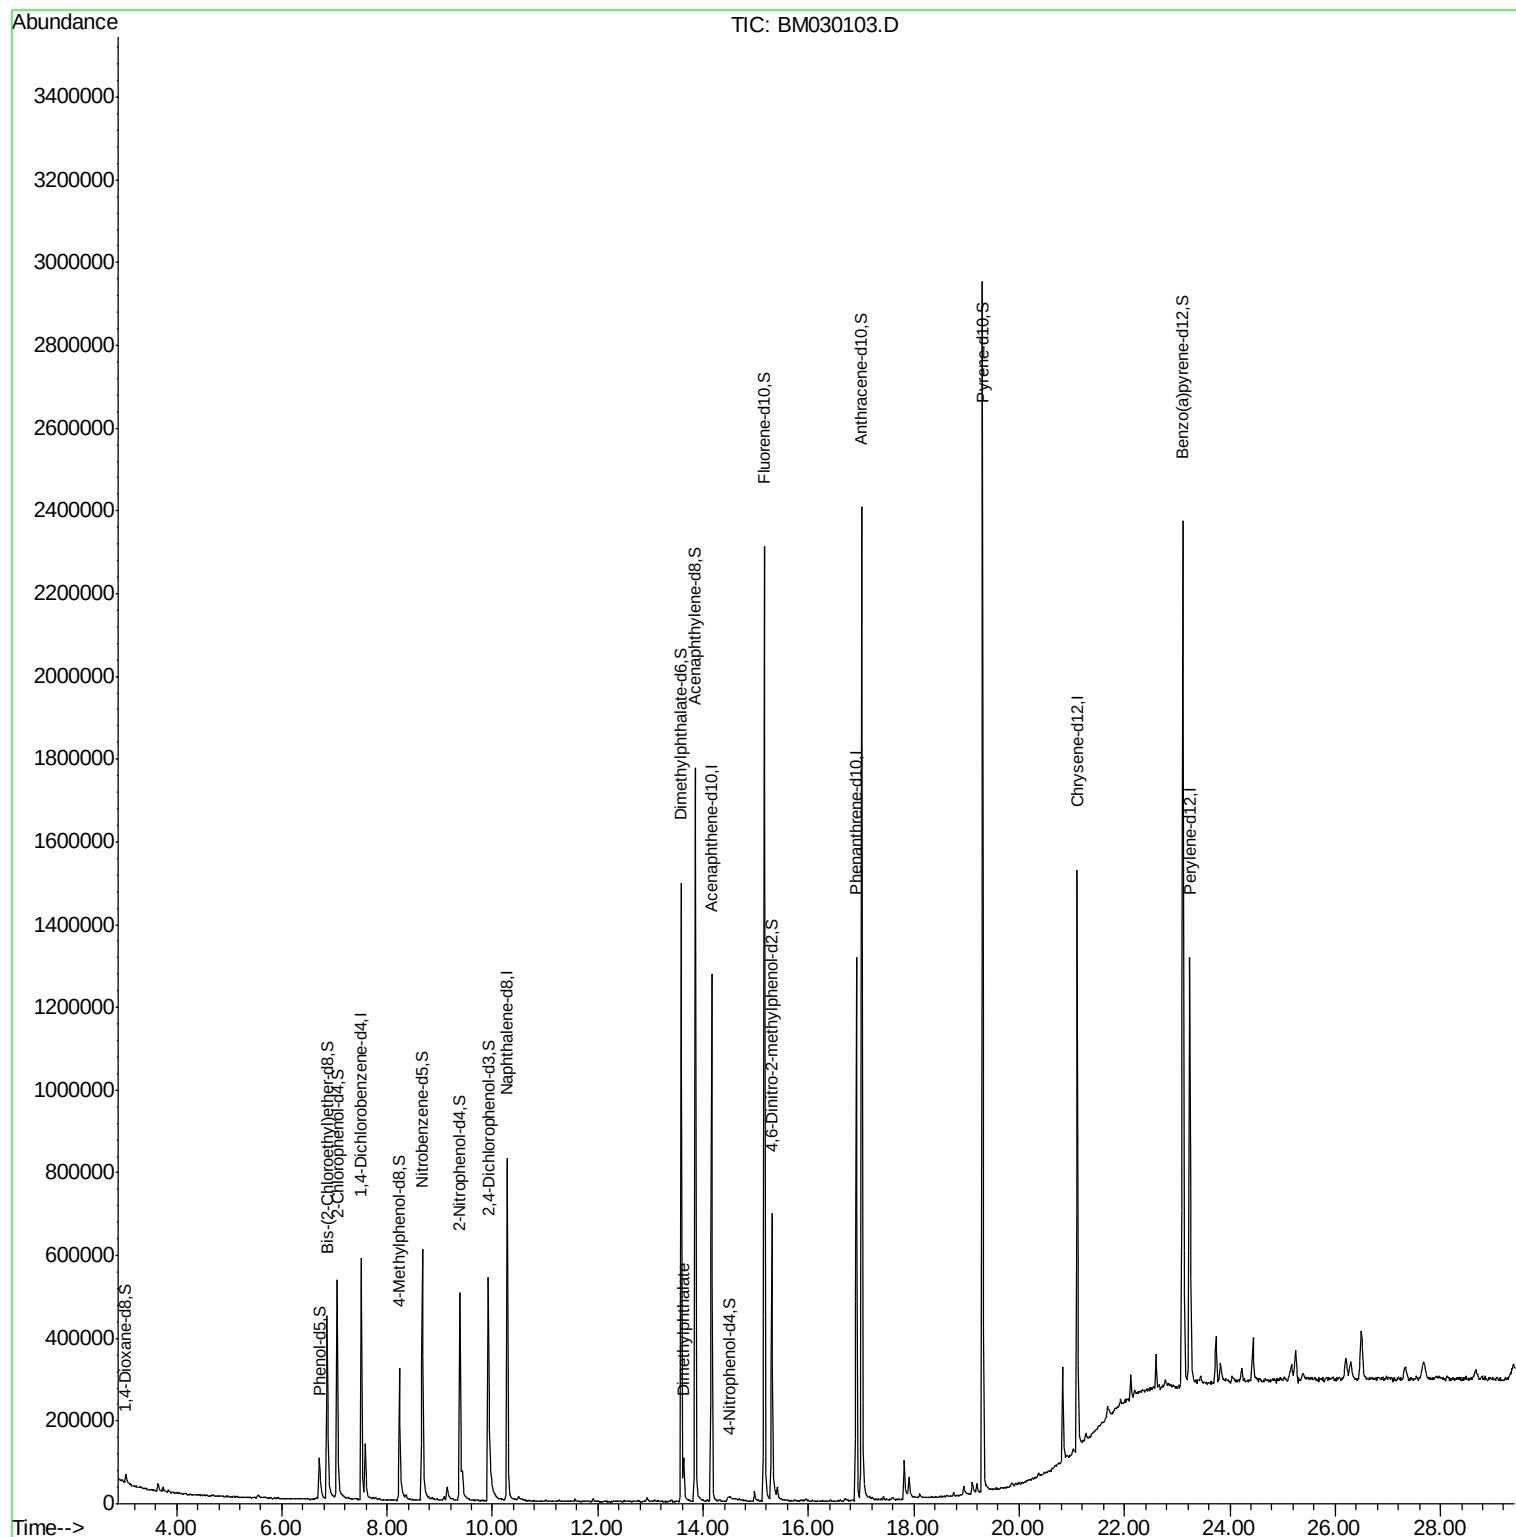

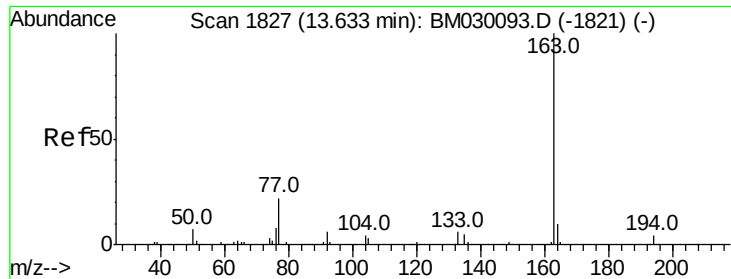

#47
 Dimethylphthalate
 Concen: 1.957 ng/ul
 RT: 13.63 min Scan# 1827
 Delta R.T. -0.00 min
 Lab File: BM030103.D
 Acq: 20 May 2021 23:22

Instrument :
 BNA_M
 ClientSampleId :
 GB3Y7

Tot Ion:	163	Resp:	61627
Ion Ratio	Lower	Upper	
163	100		
194	3.6	3.4	5.0
164	10.3	7.8	11.8

Manual Integrations
 APPROVED

mohammad
 5/21/2021 3:38:28 PM

