

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM052021\
 Data File : BM030111.D
 Acq On : 21 May 2021 10:39
 Operator : CG/JU
 Sample : M2474-06
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 GB405

Manual Integrations
 APPROVED

mohammad
 5/21/2021 3:38:58 PM

Quant Time: May 21 11:40:02 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM050721.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu May 20 12:00:20 2021
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.51	152	134590	20.00	ng/ul	0.00
20) Naphthalene-d8	10.28	136	597601	20.00	ng/ul	0.00
38) Acenaphthene-d10	14.16	164	405873	20.00	ng/ul	0.00
64) Phenanthrene-d10	16.91	188	848387	20.00	ng/ul	0.00
79) Chrysene-d12	21.10	240	836119	20.00	ng/ul	0.00
88) Perylene-d12	23.24	264	774469	20.00	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.04	96	8722	2.59	ng/uL	0.00
4) Pyridine-d5	0.00	84	0d	0.00	ng/ul	0.00
7) Phenol-d5	6.71	99	52222	4.17	ng/ul	0.00
9) Bis-(2-Chloroethyl)ether-d	6.86	67	199450	25.70	ng/ul	0.00
11) 2-Chlorophenol-d4	7.05	132	207960	21.53	ng/ul	0.00
15) 4-Methylphenol-d8	8.23	113	116231	11.23	ng/ul	0.00
21) Nitrobenzene-d5	8.67	128	124425	30.21	ng/ul	0.00
24) 2-Nitrophenol-d4	9.39	143	139009	29.91	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	9.92	165	209579	22.49	ng/ul	0.00
31) 4-Chloroaniline-d4	10.50	131	9638m	0.68	ng/ul	0.06
46) Dimethylphthalate-d6	13.59	166	1002632	31.87	ng/ul	0.00
49) Acenaphthylene-d8	13.85	160	1181021	29.62	ng/ul	0.00
54) 4-Nitrophenol-d4	14.51	143	10098m	1.97	ng/ul	0.11
60) Fluorene-d10	15.16	176	880948	32.99	ng/ul	0.00
65) 4,6-Dinitro-2-methylphenol	15.30	200	163281	29.63	ng/ul	0.00
73) Anthracene-d10	17.01	188	1480014	34.64	ng/ul	0.00
81) Pyrene-d10	19.31	212	1711482	39.90	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.11	264	1563378	35.61	ng/ul	0.00
Target Compounds						
47) Dimethylphthalate	13.63	163	41383	1.314	ng/ul	Ovalue 99

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM052021\
Data File : BM030111.D
Acq On : 21 May 2021 10:39
Operator : CG/JU
Sample : M2474-06
Misc :
ALS Vial : 27 Sample Multiplier: 1


Instrument :
BNA_M
ClientSampleId :
GB405

Manual Integrations
APPROVED

mohammad
5/21/2021 3:38:58 PM

Quant Time: May 21 11:40:02 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM050721.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu May 20 12:00:20 2021
Response via : Initial Calibration

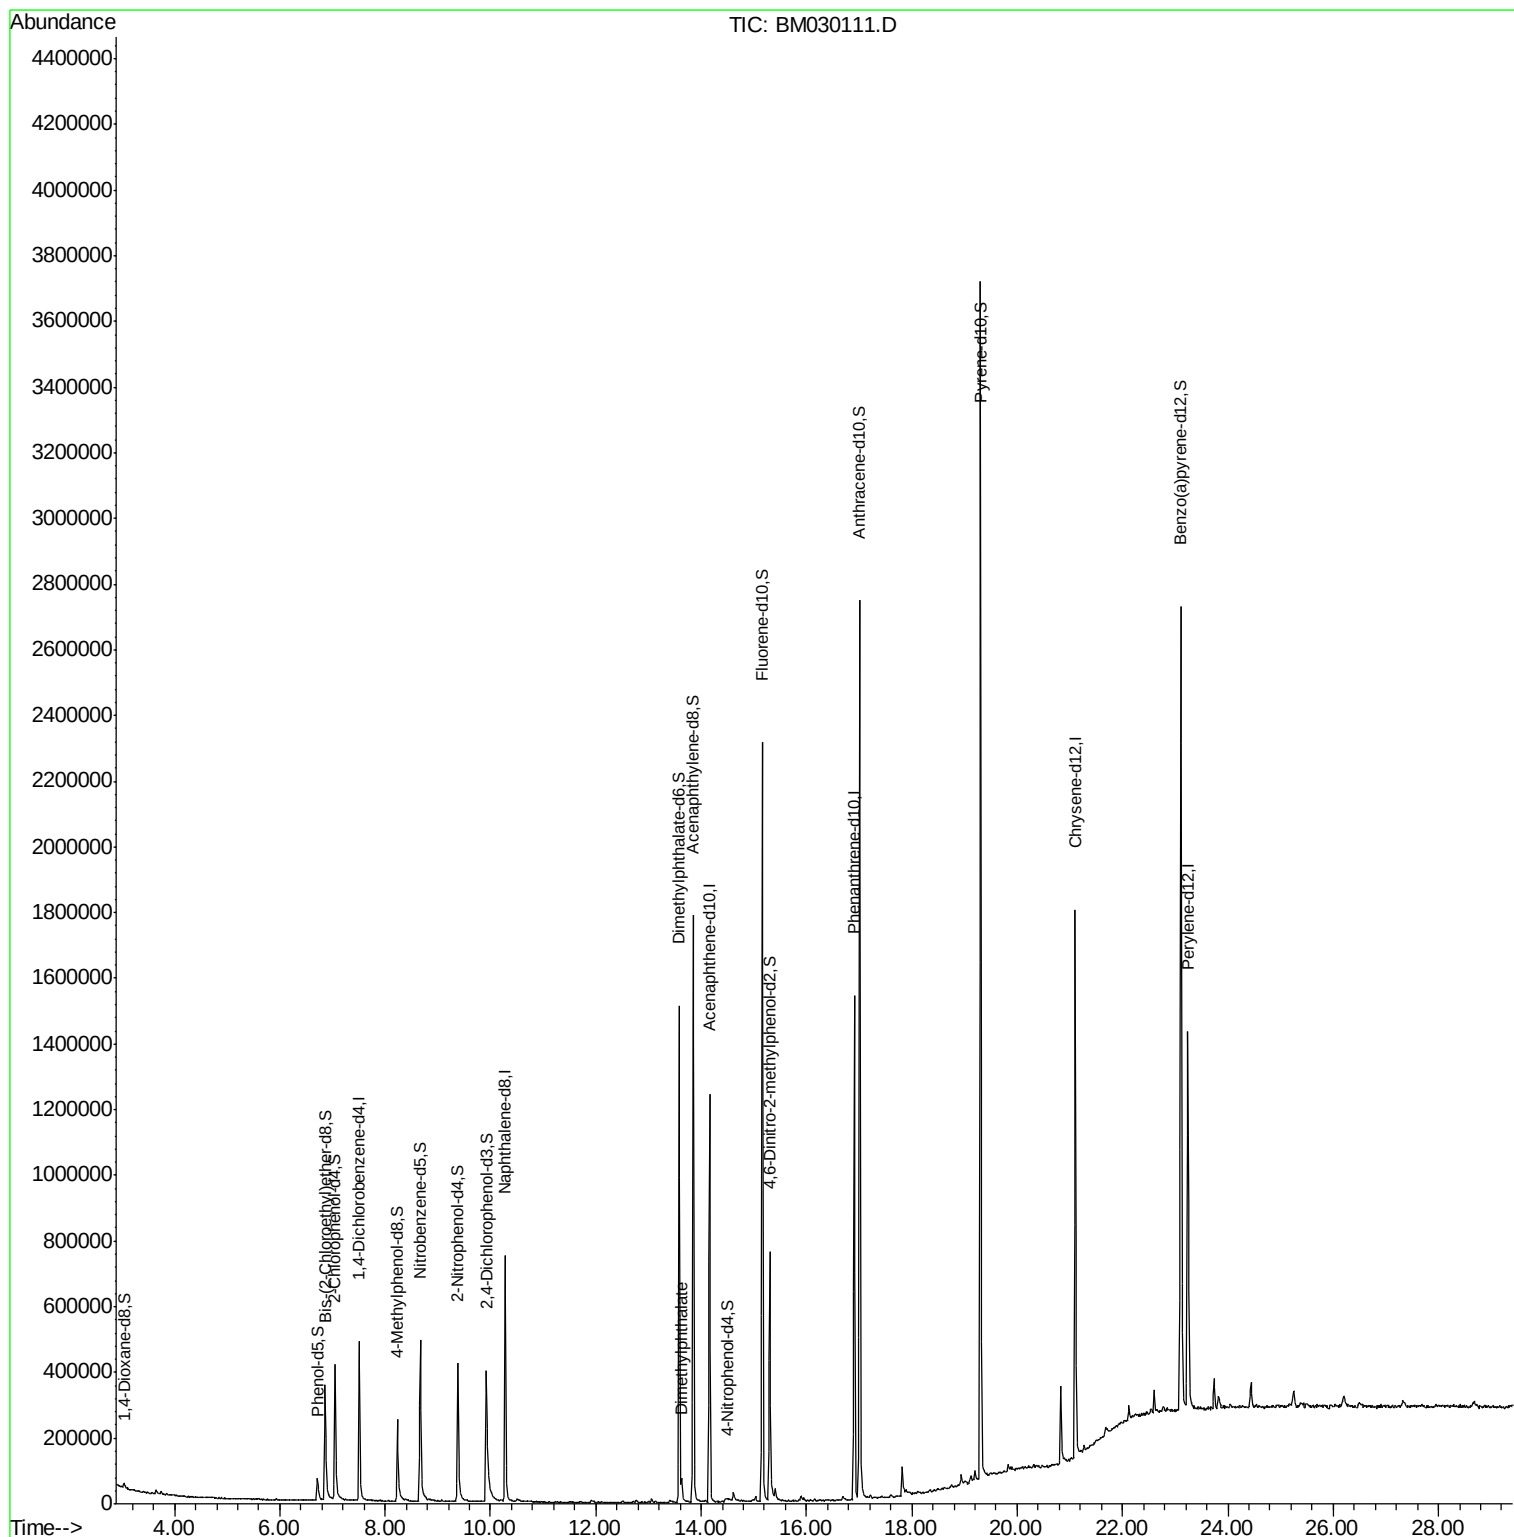

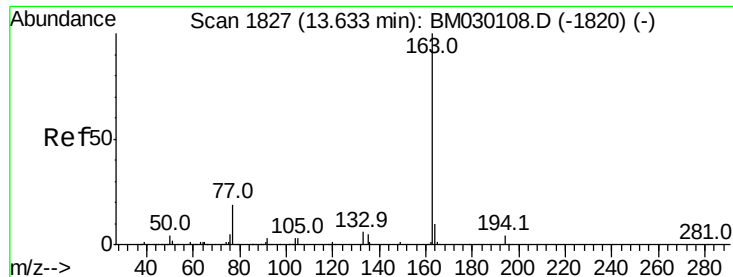

#47
 Dimethylphthalate
 Concen: 1.314 ng/ul
 RT: 13.63 min Scan# 1827
 Delta R.T. -0.00 min
 Lab File: BM030111.D
 Acq: 21 May 2021 10:39

Instrument :
 BNA_M
 ClientSampleId :
 GB405

Tot Ion	Ratio	Resp Lower	Upper
163	100		
194	4.1	3.4	5.0
164	9.2	7.8	11.8

Manual Integrations
 APPROVED

mohammad
 5/21/2021 3:38:58 PM

