

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM052021\
 Data File : BM030120.D
 Acq On : 21 May 2021 19:38
 Operator : CG/JU
 Sample : M2474-05
 Misc :
 ALS Vial : 36 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 GB404

Manual Integrations
 APPROVED

mohammad
 5/24/2021 1:52:43 PM

Quant Time: May 22 00:10:03 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM050721.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri May 21 23:57:54 2021
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.51	152	118263	20.00	ng/ul	0.00
20) Naphthalene-d8	10.28	136	532324	20.00	ng/ul	0.00
38) Acenaphthene-d10	14.16	164	355430	20.00	ng/ul	0.00
64) Phenanthrene-d10	16.91	188	727684	20.00	ng/ul	0.00
79) Chrysene-d12	21.10	240	691645	20.00	ng/ul	0.00
88) Perylene-d12	23.24	264	639586	20.00	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.04	96	9215	3.11	ng/uL	0.00
4) Pyridine-d5	0.00	84	0d	0.00	ng/ul	
7) Phenol-d5	6.72	99	54027	4.91	ng/ul	0.01
9) Bis-(2-Chloroethyl)ether-d	6.86	67	201597	29.56	ng/ul	0.00
11) 2-Chlorophenol-d4	7.05	132	204721	24.12	ng/ul	0.00
15) 4-Methylphenol-d8	8.23	113	118475	13.03	ng/ul	0.00
21) Nitrobenzene-d5	8.67	128	126592	34.51	ng/ul	0.00
24) 2-Nitrophenol-d4	9.39	143	139511	33.69	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	9.92	165	213005	25.66	ng/ul	0.00
31) 4-Chloroaniline-d4	10.52	131	8054m	0.64	ng/ul	0.08
46) Dimethylphthalate-d6	13.59	166	916893	33.28	ng/ul	0.00
49) Acenaphthylene-d8	13.85	160	1127360	32.29	ng/ul	0.00
54) 4-Nitrophenol-d4	14.50	143	8755m	1.95	ng/ul	0.10
60) Fluorene-d10	15.16	176	821786	35.14	ng/ul	0.00
65) 4,6-Dinitro-2-methylphenol	15.30	200	157717	33.37	ng/ul	0.00
73) Anthracene-d10	17.01	188	1455585	39.72	ng/ul	0.00
81) Pyrene-d10	19.31	212	1655704	46.66	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.11	264	1478900	40.79	ng/ul	0.00
Target Compounds						
47) Dimethylphthalate	13.63	163	28063	1.017	ng/ul	Ovalue 99

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM052021\
Data File : BM030120.D
Acq On : 21 May 2021 19:38
Operator : CG/JU
Sample : M2474-05
Misc :
ALS Vial : 36 Sample Multiplier: 1


Instrument :
BNA_M
ClientSampleId :
GB404

Manual Integrations
APPROVED

mohammad
5/24/2021 1:52:43 PM

Quant Time: May 22 00:10:03 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM050721.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri May 21 23:57:54 2021
Response via : Initial Calibration

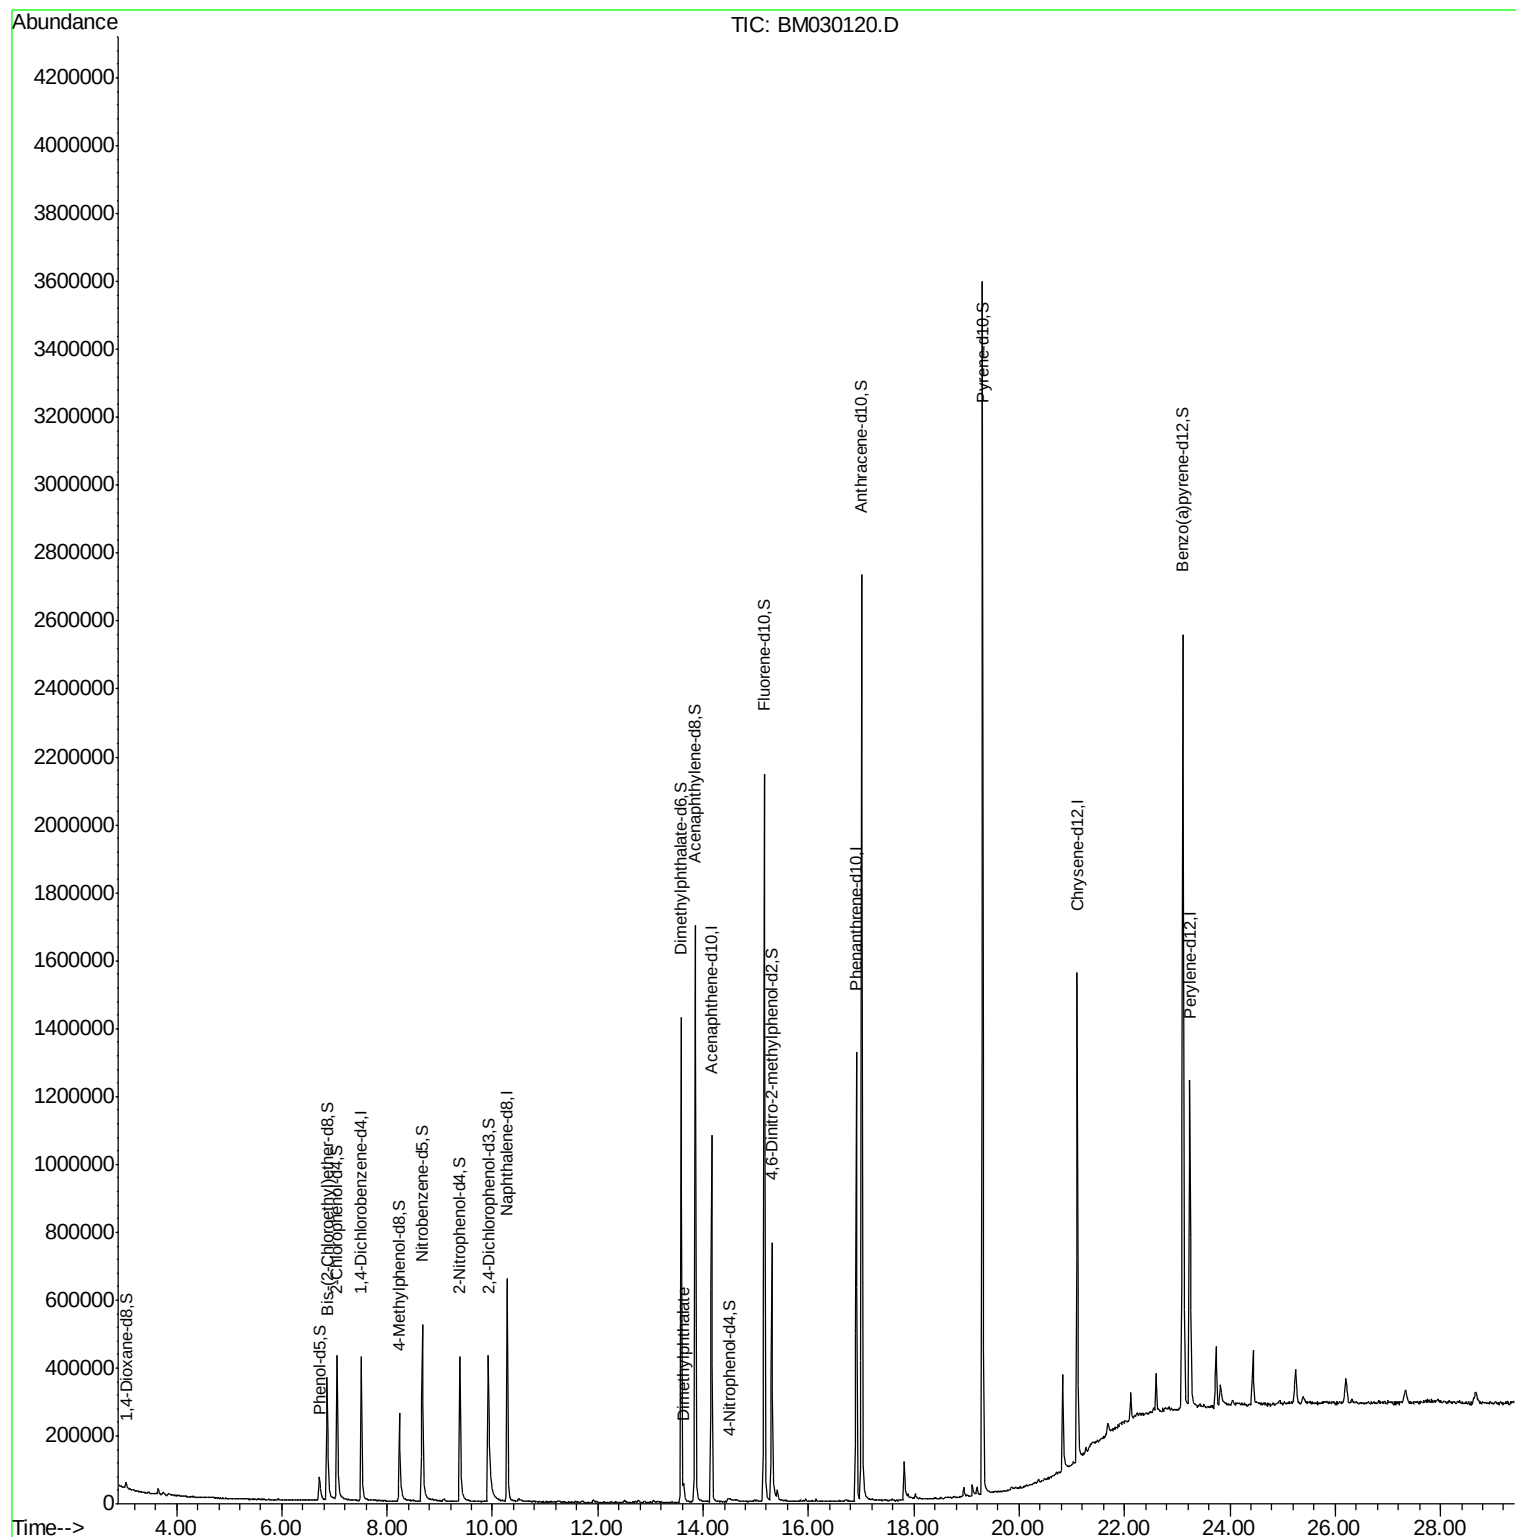

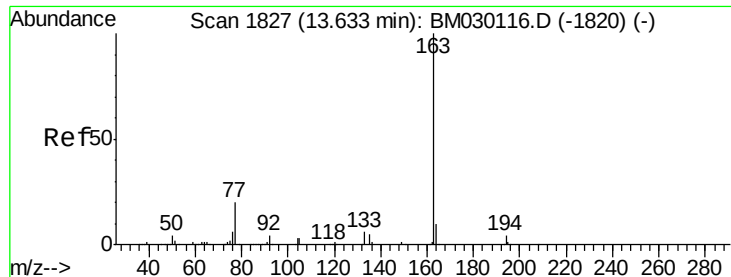


#47
 Dimethylphthalate
 Concen: 1.017 ng/ul
 RT: 13.63 min Scan# 1827
 Delta R.T. -0.00 min
 Lab File: BM030120.D
 Acq: 21 May 2021 19:38

Instrument :
 BNA_M
 ClientSampleId :
 GB404

Tot Ion:	163	Resp:	28063
Ion Ratio	Lower	Upper	
163	100		
194	3.6	3.4	5.0
164	10.2	7.8	11.8

Manual Integrations
 APPROVED

mohammad
 5/24/2021 1:52:43 PM

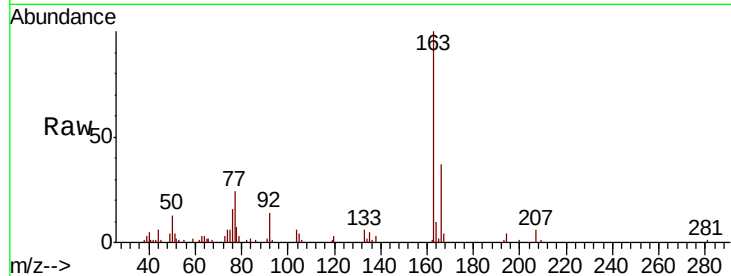

Abundance

Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

