

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM052021\
 Data File : BM030122.D
 Acq On : 21 May 2021 20:52
 Operator : CG/JU
 Sample : M2474-03
 Misc :
 ALS Vial : 38 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 GB402

Manual Integrations
 APPROVED

mohammad
 5/24/2021 1:52:51 PM

Quant Time: May 22 00:21:40 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM050721.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri May 21 23:57:54 2021
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.51	152	128063	20.00	ng/ul	0.00
20) Naphthalene-d8	10.28	136	566450	20.00	ng/ul	0.00
38) Acenaphthene-d10	14.16	164	375781	20.00	ng/ul	0.00
64) Phenanthrene-d10	16.91	188	762799	20.00	ng/ul	0.00
79) Chrysene-d12	21.10	240	665042	20.00	ng/ul	0.00
88) Perylene-d12	23.24	264	593810	20.00	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.04	96	9097	2.84	ng/uL	0.00
4) Pyridine-d5	0.00	84	0d	0.00	ng/ul	0.00
7) Phenol-d5	6.71	99	64622	5.43	ng/ul	0.00
9) Bis-(2-Chloroethyl)ether-d	6.86	67	227453	30.80	ng/ul	0.00
11) 2-Chlorophenol-d4	7.05	132	235504	25.62	ng/ul	0.00
15) 4-Methylphenol-d8	8.23	113	138076	14.02	ng/ul	0.00
21) Nitrobenzene-d5	8.67	128	139201	35.66	ng/ul	0.00
24) 2-Nitrophenol-d4	9.38	143	157503	35.75	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	9.92	165	241187	27.30	ng/ul	0.00
31) 4-Chloroaniline-d4	10.50	131	11781m	0.88	ng/ul	0.06
46) Dimethylphthalate-d6	13.59	166	1044211	35.85	ng/ul	0.00
49) Acenaphthylene-d8	13.85	160	1273529	34.50	ng/ul	0.00
54) 4-Nitrophenol-d4	14.50	143	12897m	2.72	ng/ul	0.10
60) Fluorene-d10	15.16	176	920369	37.22	ng/ul	0.00
65) 4,6-Dinitro-2-methylphenol	15.30	200	178721	36.07	ng/ul	0.00
73) Anthracene-d10	17.01	188	1526900	39.75	ng/ul	0.00
81) Pyrene-d10	19.31	212	1703468	49.93	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.11	264	1413038	41.98	ng/ul	0.00
Target Compounds						
47) Dimethylphthalate	13.63	163	46159	1.583	ng/ul	Ovalue 98

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM052021\
Data File : BM030122.D
Acq On : 21 May 2021 20:52
Operator : CG/JU
Sample : M2474-03
Misc :
ALS Vial : 38 Sample Multiplier: 1


Instrument :
BNA_M
ClientSampleId :
GB402

Manual Integrations
APPROVED

mohammad
5/24/2021 1:52:51 PM

Quant Time: May 22 00:21:40 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM050721.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri May 21 23:57:54 2021
Response via : Initial Calibration

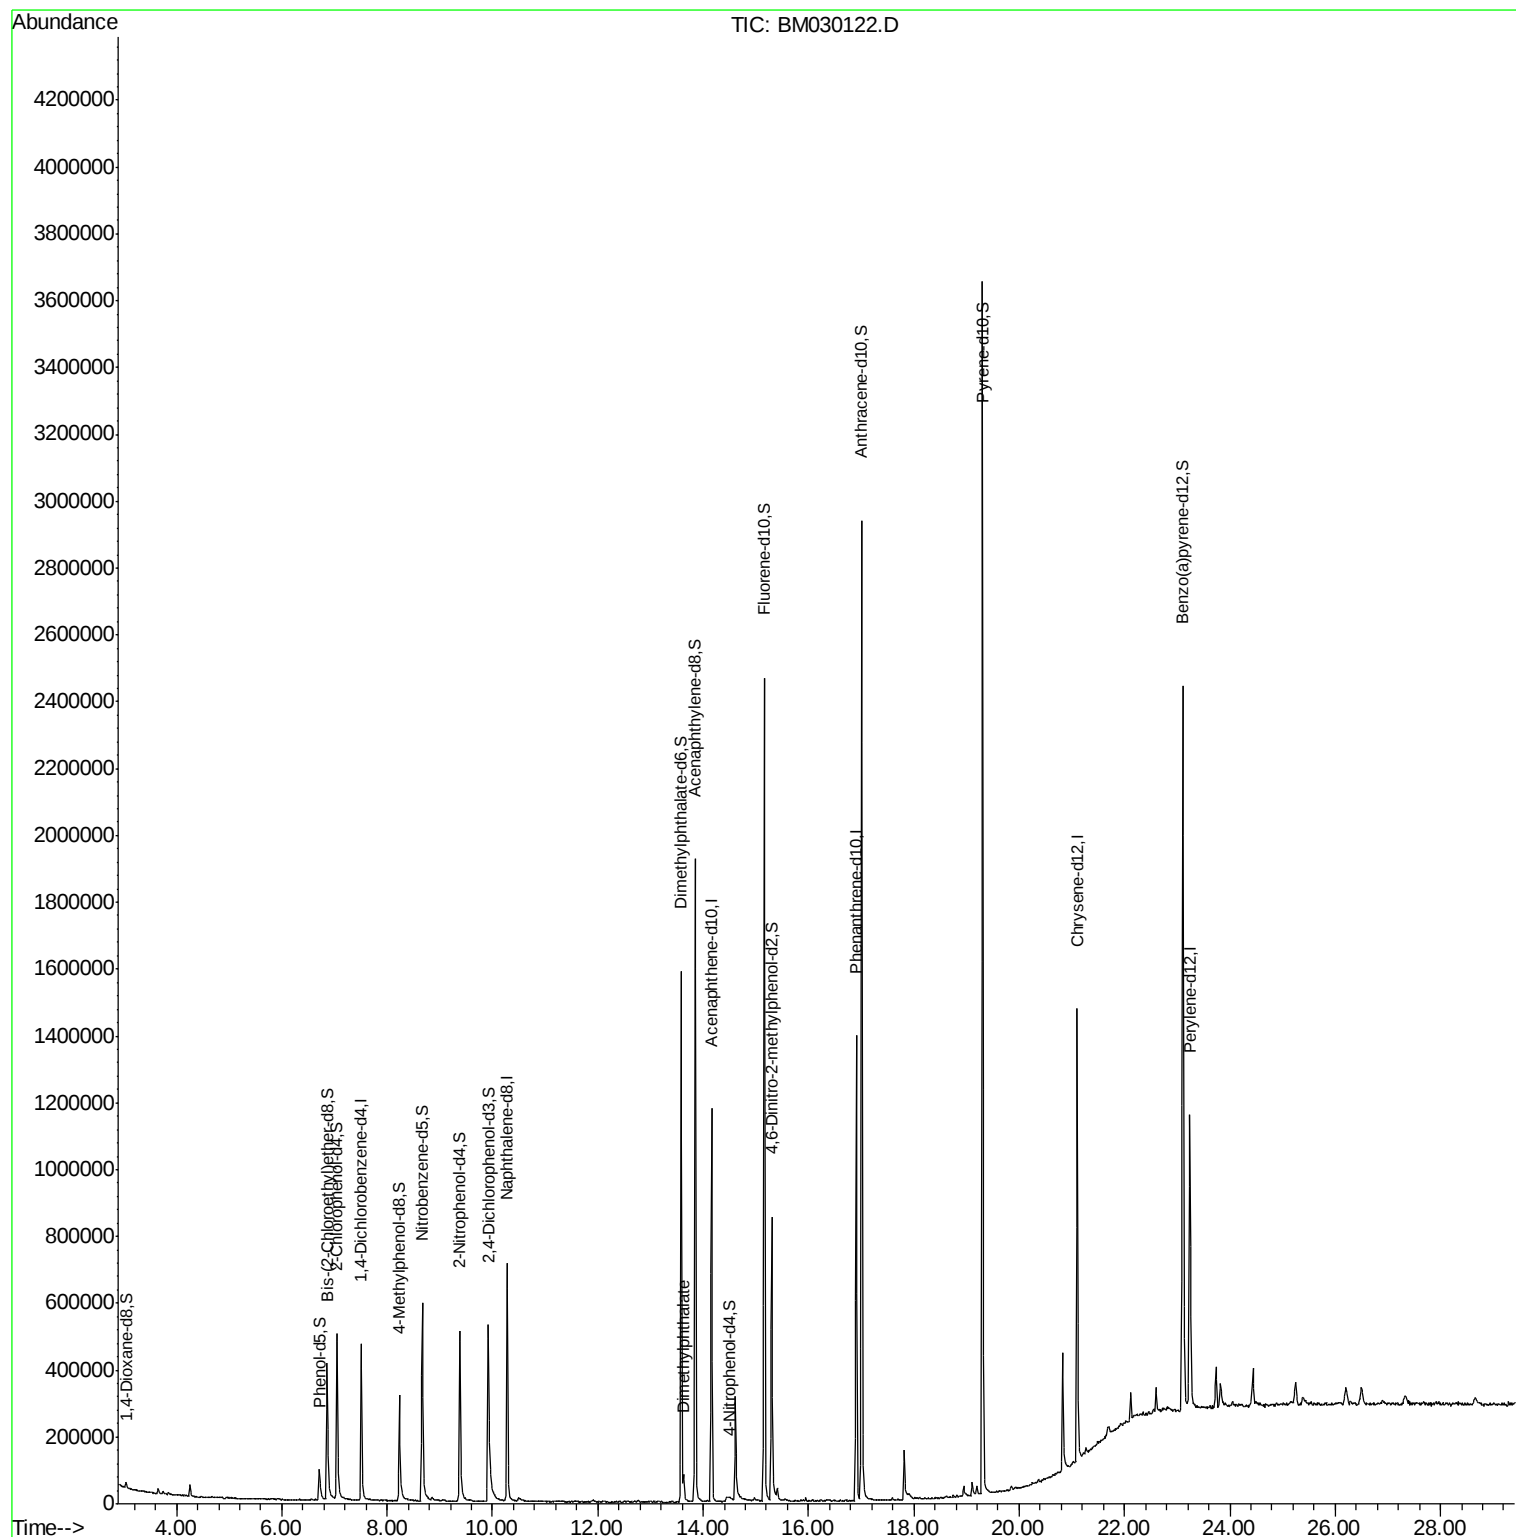

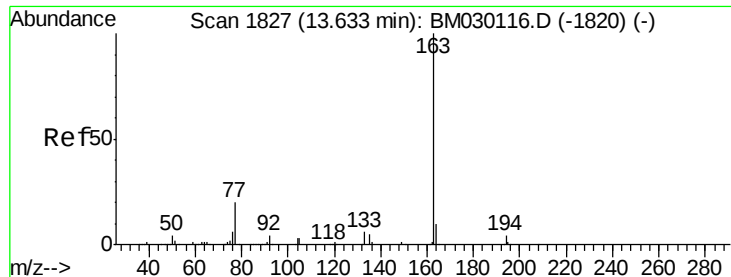

#47
 Dimethylphthalate
 Concen: 1.583 ng/ul
 RT: 13.63 min Scan# 1827
 Delta R.T. 0.00 min
 Lab File: BM030122.D
 Acq: 21 May 2021 20:52

Instrument :
 BNA_M
 ClientSampleId :
 GB402

Tot Ion:	163	Resp:	46159
Ion Ratio	Lower	Upper	
163	100		
194	4.0	3.4	5.0
164	10.8	7.8	11.8

Manual Integrations
 APPROVED

mohammad
 5/24/2021 1:52:51 PM

