

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM052021\  
 Data File : BM030123.D  
 Acq On : 21 May 2021 21:29  
 Operator : CG/JU  
 Sample : M2474-08  
 Misc :  
 ALS Vial : 39 Sample Multiplier: 1

Instrument :  
 BNA\_M  
 ClientSampleId :  
 GB407

Manual Integrations  
 APPROVED

mohammad  
 5/24/2021 1:52:55 PM

Quant Time: May 22 00:26:52 2021  
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA\_M\METHODS\SFAM-EPA-BM050721.M  
 Quant Title : SVOA CALIBRATION  
 QLast Update : Fri May 21 23:57:54 2021  
 Response via : Initial Calibration

| Internal Standards             | R.T.  | QIon | Response | Conc  | Units | Dev(Min) |
|--------------------------------|-------|------|----------|-------|-------|----------|
| 1) 1,4-Dichlorobenzene-d4      | 7.51  | 152  | 125692   | 20.00 | ng/ul | 0.00     |
| 20) Naphthalene-d8             | 10.28 | 136  | 556800   | 20.00 | ng/ul | 0.00     |
| 38) Acenaphthene-d10           | 14.16 | 164  | 361440   | 20.00 | ng/ul | 0.00     |
| 64) Phenanthrene-d10           | 16.91 | 188  | 707637   | 20.00 | ng/ul | 0.00     |
| 79) Chrysene-d12               | 21.10 | 240  | 576850   | 20.00 | ng/ul | 0.00     |
| 88) Perylene-d12               | 23.24 | 264  | 548305   | 20.00 | ng/ul | 0.00     |
| System Monitoring Compounds    |       |      |          |       |       |          |
| 3) 1,4-Dioxane-d8              | 3.03  | 96   | 10798    | 3.43  | ng/uL | 0.00     |
| 4) Pyridine-d5                 | 0.00  | 84   | 0d       | 0.00  | ng/ul | 0.00     |
| 7) Phenol-d5                   | 6.71  | 99   | 59219    | 5.07  | ng/ul | 0.00     |
| 9) Bis-(2-Chloroethyl)ether-d  | 6.86  | 67   | 228573   | 31.53 | ng/ul | 0.00     |
| 11) 2-Chlorophenol-d4          | 7.05  | 132  | 231117   | 25.62 | ng/ul | 0.00     |
| 15) 4-Methylphenol-d8          | 8.23  | 113  | 127370   | 13.18 | ng/ul | 0.00     |
| 21) Nitrobenzene-d5            | 8.67  | 128  | 141137   | 36.78 | ng/ul | 0.00     |
| 24) 2-Nitrophenol-d4           | 9.38  | 143  | 158010   | 36.49 | ng/ul | 0.00     |
| 28) 2,4-Dichlorophenol-d3      | 9.92  | 165  | 234138   | 26.96 | ng/ul | 0.00     |
| 31) 4-Chloroaniline-d4         | 10.50 | 131  | 11074m   | 0.84  | ng/ul | 0.06     |
| 46) Dimethylphthalate-d6       | 13.59 | 166  | 1007712  | 35.97 | ng/ul | 0.00     |
| 49) Acenaphthylene-d8          | 13.85 | 160  | 1225071  | 34.51 | ng/ul | 0.00     |
| 54) 4-Nitrophenol-d4           | 14.50 | 143  | 10818m   | 2.37  | ng/ul | 0.10     |
| 60) Fluorene-d10               | 15.16 | 176  | 905757   | 38.08 | ng/ul | 0.00     |
| 65) 4,6-Dinitro-2-methylphenol | 15.30 | 200  | 158745   | 34.54 | ng/ul | 0.00     |
| 73) Anthracene-d10             | 17.01 | 188  | 1494616  | 41.94 | ng/ul | 0.00     |
| 81) Pyrene-d10                 | 19.31 | 212  | 1564923  | 52.88 | ng/ul | 0.00     |
| 92) Benzo(a)pyrene-d12         | 23.11 | 264  | 1306834  | 42.05 | ng/ul | 0.00     |
| Target Compounds               |       |      |          |       |       |          |
| 47) Dimethylphthalate          | 13.63 | 163  | 44333    | 1.580 | ng/ul | 100      |

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM052021\  
Data File : BM030123.D  
Acq On : 21 May 2021 21:29  
Operator : CG/JU  
Sample : M2474-08  
Misc :  
ALS Vial : 39 Sample Multiplier: 1


Instrument :  
BNA\_M  
ClientSampleId :  
GB407

Quant Time: May 22 00:26:52 2021  
Quant Method : Z:\SVOASRV\HPCHEM1\BNA\_M\METHODS\SFAM-EPA-BM050721.M  
Quant Title : SVOA CALIBRATION  
QLast Update : Fri May 21 23:57:54 2021  
Response via : Initial Calibration

Manual Integrations  
APPROVED

mohammad  
5/24/2021 1:52:55 PM

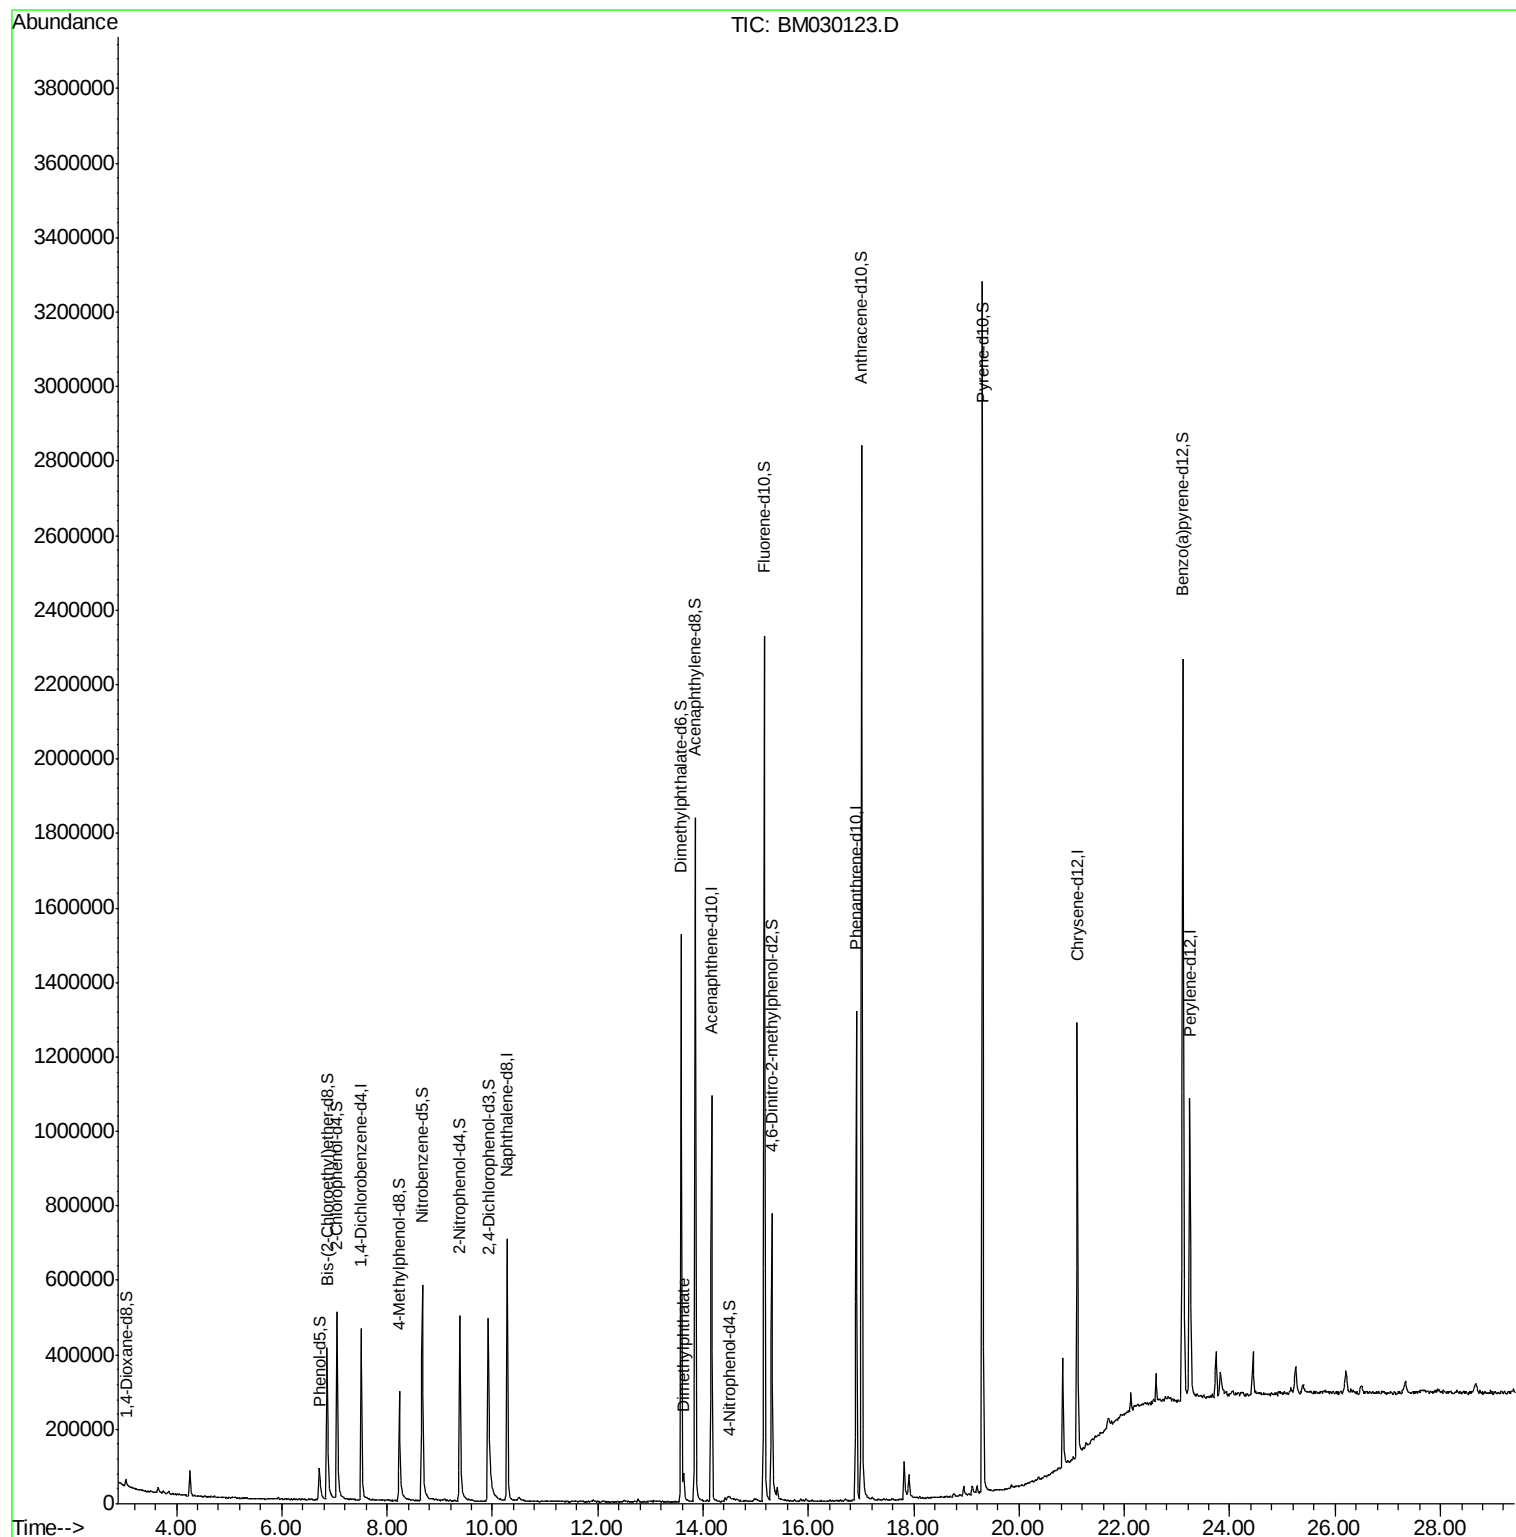

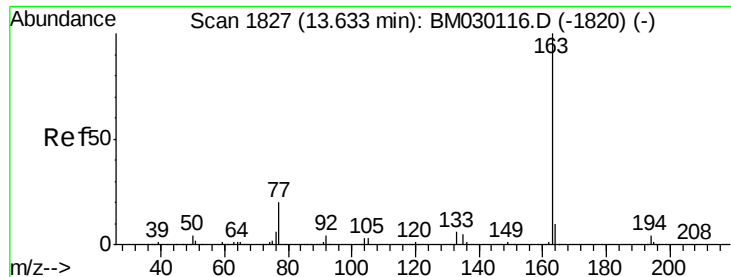

#47  
 Dimethylphthalate  
 Concen: 1.580 ng/ul  
 RT: 13.63 min Scan# 1827  
 Delta R.T. 0.00 min  
 Lab File: BM030123.D  
 Acq: 21 May 2021 21:29

Instrument :  
 BNA\_M  
 ClientSampleId :  
 GB407

| Tot Ion | Ratio | Lower | Upper |
|---------|-------|-------|-------|
| 163     | 100   |       |       |
| 194     | 4.2   | 3.4   | 5.0   |
| 164     | 10.0  | 7.8   | 11.8  |

Manual Integrations  
 APPROVED

mohammad  
 5/24/2021 1:52:55 PM

