

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM052021\
 Data File : BM030131.D
 Acq On : 22 May 2021 02:58
 Operator : CG/JU
 Sample : PB136596BL
 Misc :
 ALS Vial : 47 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK596

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM050721.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.028	21	24	33	rVB	34355	50083	1.04%	0.109%
2	3.452	93	96	121	rBV	247413	750219	15.52%	1.631%
3	6.698	642	648	669	rBV	582046	1084175	22.42%	2.357%
4	6.857	670	675	694	rVV	456482	802584	16.60%	1.745%
5	7.045	701	707	725	rBV	652280	1155196	23.89%	2.511%
6	7.504	778	785	801	rBV	512829	922002	19.07%	2.004%
7	8.228	902	908	925	rBV	717477	1333323	27.58%	2.898%
8	8.663	974	982	1000	rBV	580208	1106754	22.89%	2.406%
9	9.381	1097	1104	1125	rBV	503655	944553	19.54%	2.053%
10	9.916	1189	1195	1217	rBV	657223	1349796	27.92%	2.934%
11	10.281	1249	1257	1267	rBV	797691	1386347	28.67%	3.014%
12	10.433	1277	1283	1311	rBV	578016	1384105	28.63%	3.009%
13	11.922	1528	1536	1541	rBV5	6423	15019	0.31%	0.033%
14	13.580	1811	1818	1837	rBV	1567290	2334925	48.29%	5.075%
15	13.851	1857	1864	1890	rBV	1762173	2697378	55.79%	5.863%
16	14.157	1910	1916	1933	rBV	1329029	1967276	40.69%	4.276%
17	14.404	1952	1958	1980	rBV	242785	773414	16.00%	1.681%
18	15.157	2080	2086	2105	rBV	2370877	3418102	70.70%	7.430%
19	15.298	2105	2110	2124	rVV	646415	1081167	22.36%	2.350%
20	15.404	2124	2128	2136	rVB2	30705	54784	1.13%	0.119%
21	15.945	2216	2220	2224	rBV2	6926	9729	0.20%	0.021%
22	16.704	2346	2349	2354	rVB2	4695	6246	0.13%	0.014%
23	16.909	2377	2384	2394	rBV	1608193	2284926	47.26%	4.967%
24	17.009	2394	2401	2422	rVV	2464359	3755326	77.67%	8.163%
25	17.833	2538	2541	2543	rBV4	4981	6652	0.14%	0.014%
26	18.951	2726	2731	2736	rBV	22462	35103	0.73%	0.076%
27	19.198	2769	2773	2779	rBV	20019	28089	0.58%	0.061%
28	19.309	2785	2792	2811	rBV	3127631	4473390	92.53%	9.724%
29	21.097	3091	3096	3110	rBV	1914677	2686511	55.57%	5.840%
30	22.597	3349	3351	3357	rVB	84488	93016	1.92%	0.202%
31	23.103	3430	3437	3452	rBV2	2699785	4834718	100.00%	10.509%
32	23.238	3454	3460	3470	rVB2	1460055	2707441	56.00%	5.885%
33	23.738	3541	3545	3552	rVB	126942	225488	4.66%	0.490%
34	24.433	3660	3663	3671	rVB2	134107	246241	5.09%	0.535%

LSC Area Percent Report

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM052021\
Data File : BM030131.D
Acq On : 22 May 2021 02:58
Operator : CG/JU
Sample : PB136596BL
Misc :
ALS Vial : 47 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK596

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM050721.M
Title : SVOA CALIBRATION


Sum of corrected areas: 46004078

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM052021\
Data File : BM030131.D
Acq On : 22 May 2021 02:58
Operator : CG/JU
Sample : PB136596BL
Misc :
ALS Vial : 47 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK596

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM050721.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

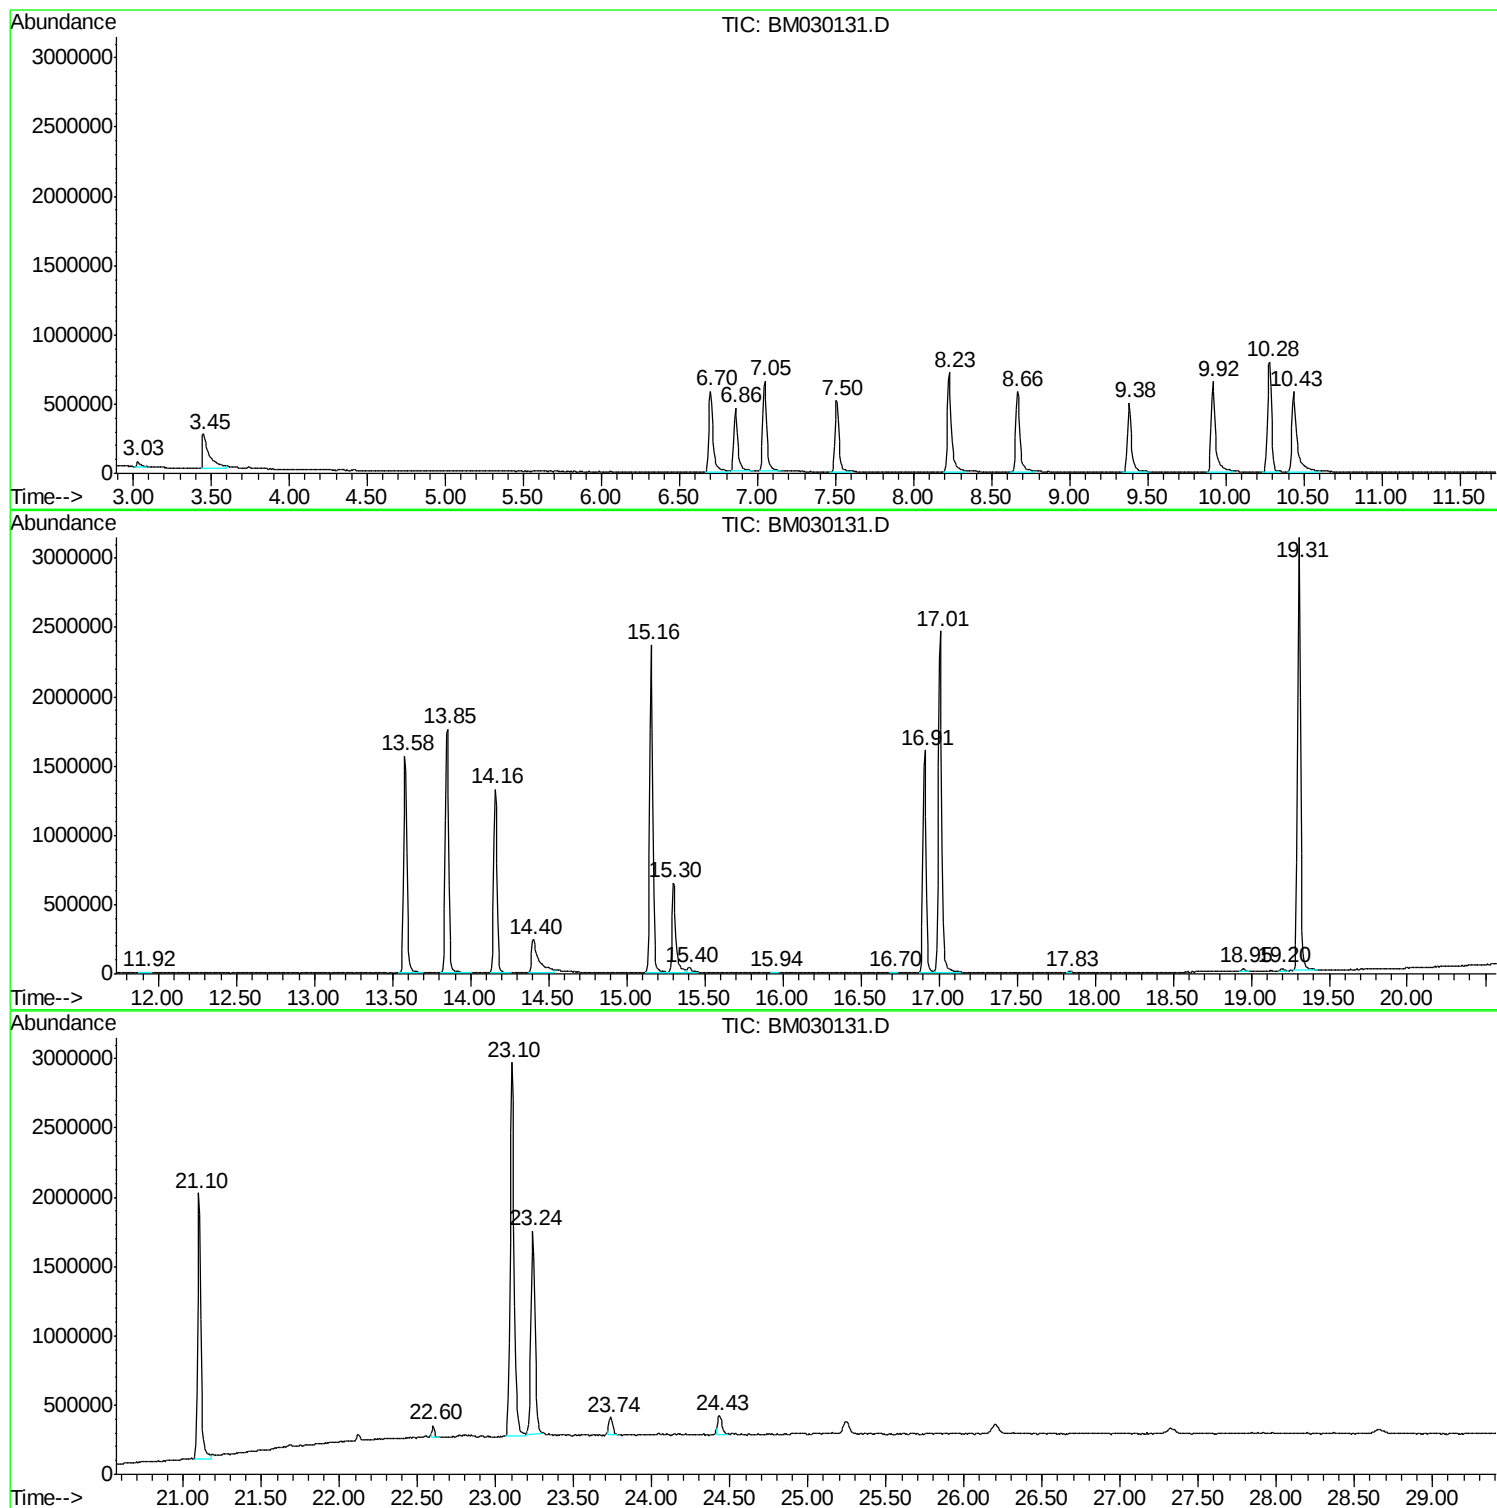

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM052021\
Data File : BM030131.D
Acq On : 22 May 2021 02:58
Operator : CG/JU
Sample : PB136596BL
Misc :
ALS Vial : 47 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK596

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM050721.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM052021\
Data File : BM030131.D
Acq On : 22 May 2021 02:58
Operator : CG/JU
Sample : PB136596BL
Misc :
ALS Vial : 47 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK596

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM050721.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	---Internal Standard---
					# RT Resp Conc