

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM052021\
 Data File : BM030150.D
 Acq On : 22 May 2021 15:03
 Operator : CG/JU
 Sample : PB136569BL
 Misc :
 ALS Vial : 66 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK569

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM050721.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.934	4	8	21	rVB	1197230	1165219	59.37%	10.768%
2	3.263	61	64	68	rVB2	30127	33408	1.70%	0.309%
3	3.740	141	145	147	rBV2	7185	9173	0.47%	0.085%
4	6.299	578	580	584	rBV5	1892	2200	0.11%	0.020%
5	6.546	620	622	626	rBV5	1898	2039	0.10%	0.019%
6	6.622	633	635	639	rBV5	1942	2577	0.13%	0.024%
7	7.340	755	757	760	rBV4	1500	2006	0.10%	0.019%
8	7.504	779	785	803	rBV	447330	851925	43.41%	7.873%
9	8.298	918	920	924	rBV5	1627	2442	0.12%	0.023%
10	8.551	962	963	970	rVB5	1220	2188	0.11%	0.020%
11	8.781	999	1002	1006	rVV5	1359	1964	0.10%	0.018%
12	9.498	1123	1124	1130	rBV5	1527	2156	0.11%	0.020%
13	9.928	1195	1197	1201	rBV4	1335	2061	0.11%	0.019%
14	10.281	1250	1257	1281	rBV	551166	1152885	58.74%	10.654%
15	10.439	1283	1284	1288	rVB3	2454	2847	0.15%	0.026%
16	12.451	1621	1626	1628	rVB5	1327	2039	0.10%	0.019%
17	14.157	1910	1916	1938	rVV	963824	1570320	80.01%	14.512%
18	14.922	2042	2046	2049	rVB4	1561	2317	0.12%	0.021%
19	14.963	2049	2053	2056	rBV3	1541	3076	0.16%	0.028%
20	16.004	2226	2230	2234	rVB5	1821	2331	0.12%	0.022%
21	16.710	2347	2350	2353	rBV4	3710	4879	0.25%	0.045%
22	16.910	2377	2384	2403	rBV	1065795	1826463	93.06%	16.879%
23	17.098	2415	2416	2419	rBV3	1829	2046	0.10%	0.019%
24	19.121	2757	2760	2764	rBV5	3688	7188	0.37%	0.066%
25	19.257	2779	2783	2788	rVV2	31900	39629	2.02%	0.366%
26	19.333	2793	2796	2800	rVV3	9879	12477	0.64%	0.115%
27	19.374	2800	2803	2810	rVB6	13306	19147	0.98%	0.177%
28	19.874	2885	2888	2891	rVB3	9963	11610	0.59%	0.107%
29	20.304	2958	2961	2965	rBV2	31124	37150	1.89%	0.343%
30	20.368	2968	2972	2976	rVV2	25970	32415	1.65%	0.300%
31	20.833	3048	3051	3054	rBV2	21503	23657	1.21%	0.219%
32	21.103	3091	3097	3107	rBV	1316544	1962654	100.00%	18.138%
33	21.268	3122	3125	3130	rVB2	33450	41132	2.10%	0.380%
34	21.680	3193	3195	3199	rVB3	37176	39257	2.00%	0.363%

LSC Area Percent Report

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM052021\
Data File : BM030150.D
Acq On : 22 May 2021 15:03
Operator : CG/JU
Sample : PB136569BL
Misc :
ALS Vial : 66 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK569

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM050721.M
Title : SVOA CALIBRATION

35	23.239	3454	3460	3474	rBV2	1007235	1945793	99.14%	17.982%
----	--------	------	------	------	------	---------	---------	--------	---------


Sum of corrected areas: 10820670

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM052021\
Data File : BM030150.D
Acq On : 22 May 2021 15:03
Operator : CG/JU
Sample : PB136569BL
Misc :
ALS Vial : 66 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK569

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM050721.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

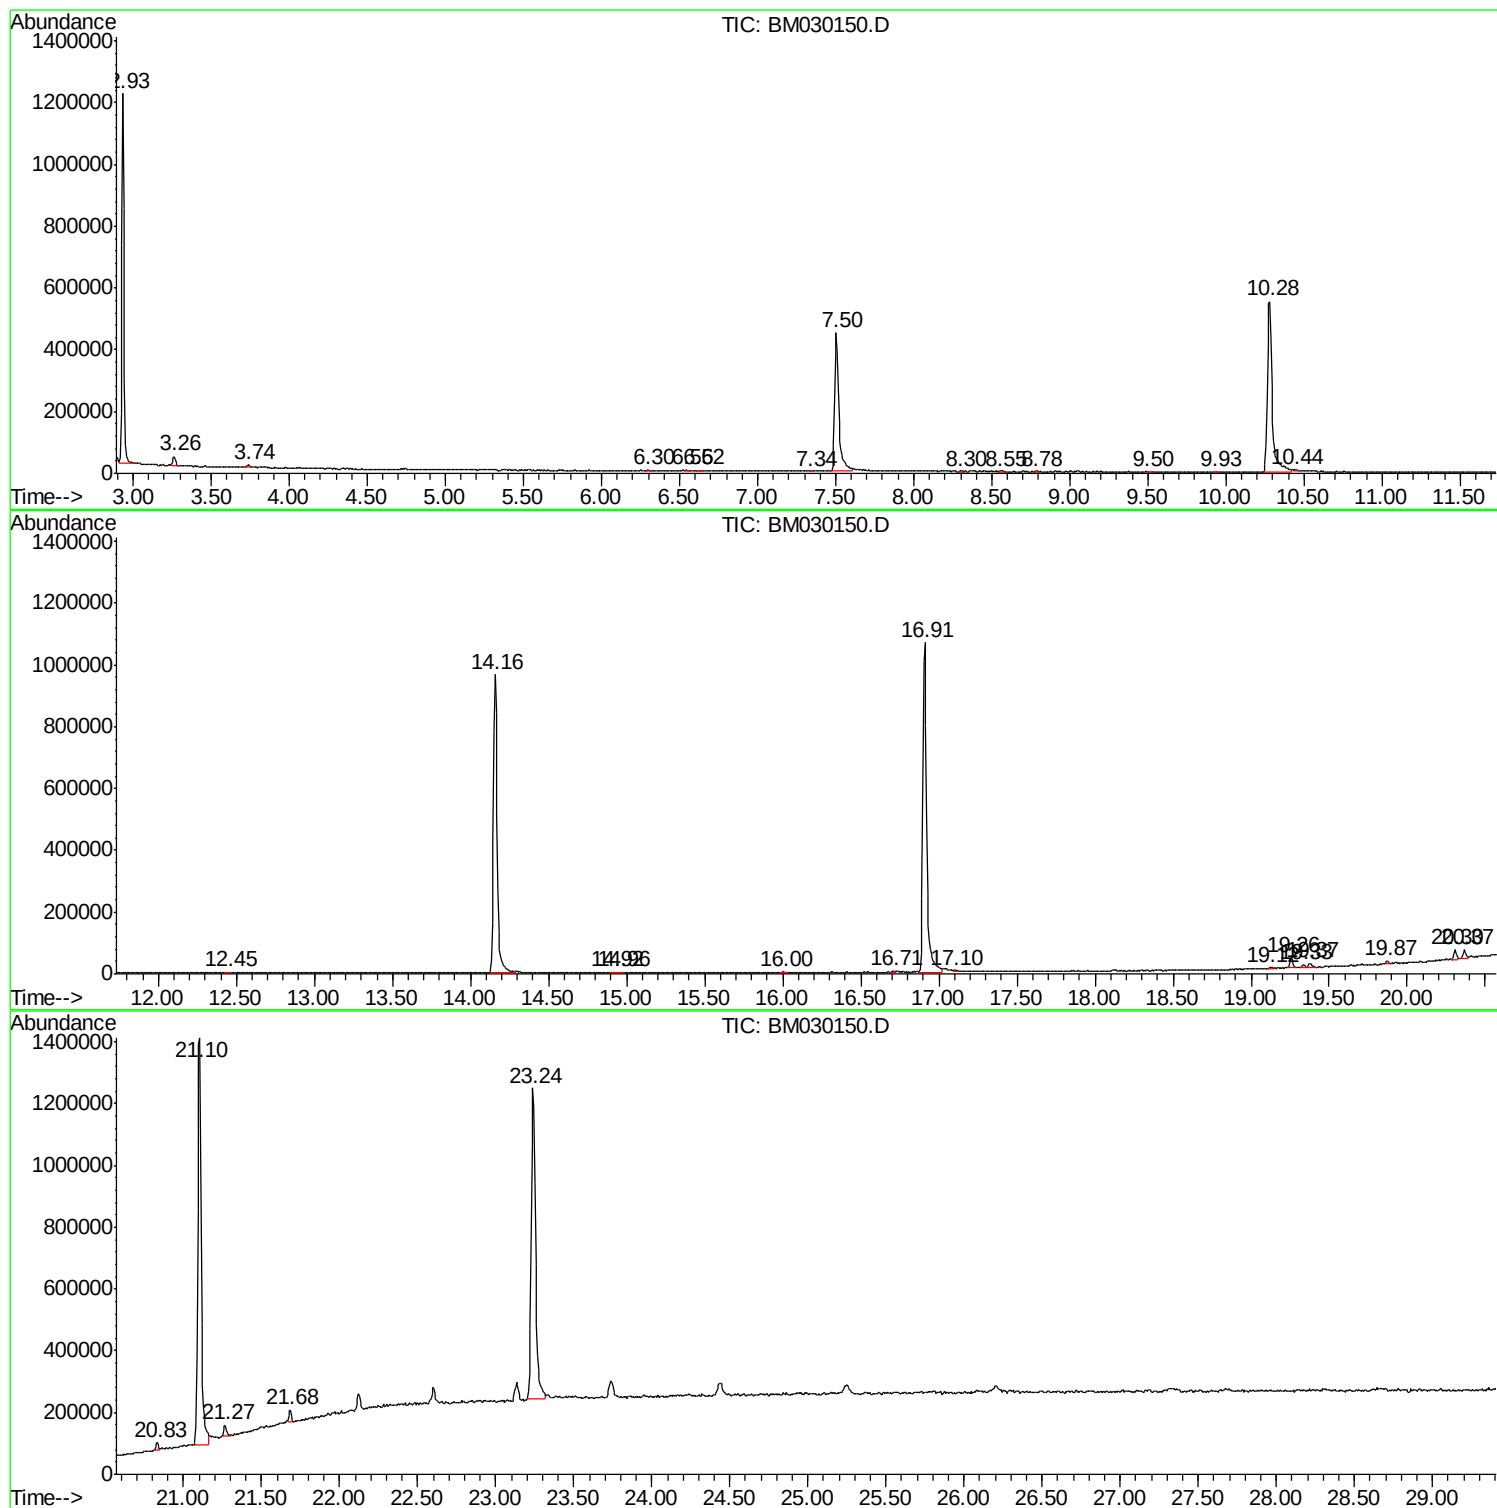

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM052021\
Data File : BM030150.D
Acq On : 22 May 2021 15:03
Operator : CG/JU
Sample : PB136569BL
Misc :
ALS Vial : 66 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK569










Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM050721.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 (DEL) Alkane: Straight-Chai... Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
2.93	27.36 ng/ul	1165220	1,4-Dichlorobenzene-d4	7.50

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	Heptane	100	C7H16	000142-82-5	95
2		Heptane	100	C7H16	000142-82-5	94
3		Heptane	100	C7H16	000142-82-5	91
4		Heptane	100	C7H16	000142-82-5	90
5		Hexane, 3-methyl-	100	C7H16	000589-34-4	42

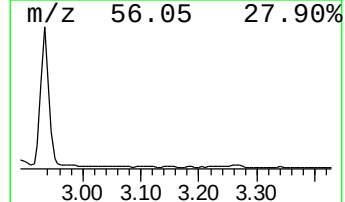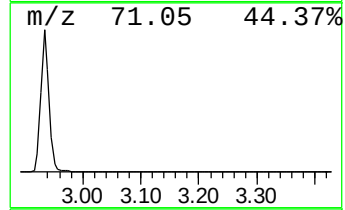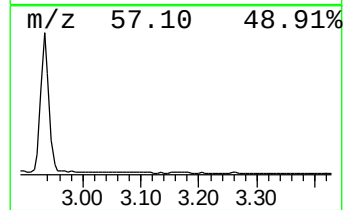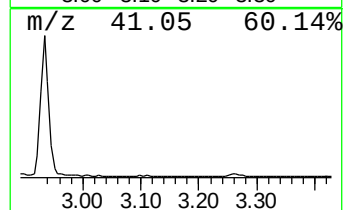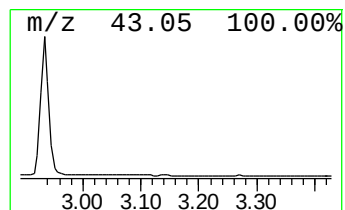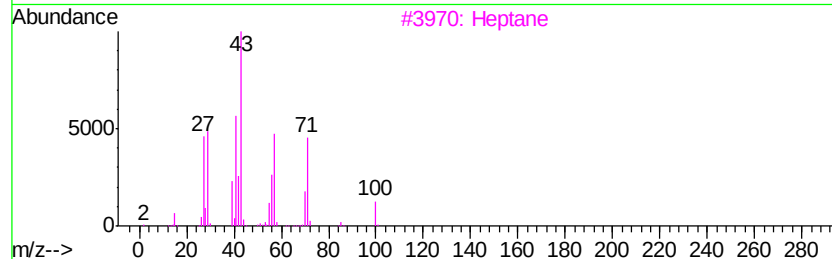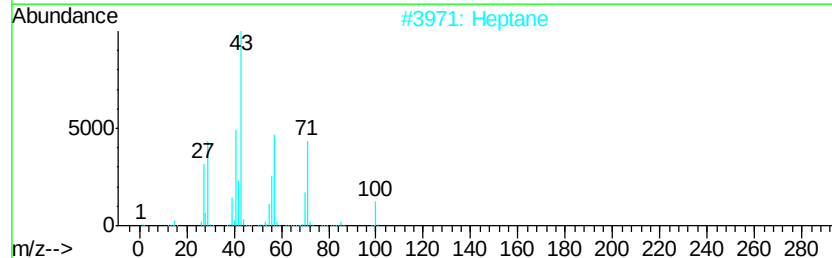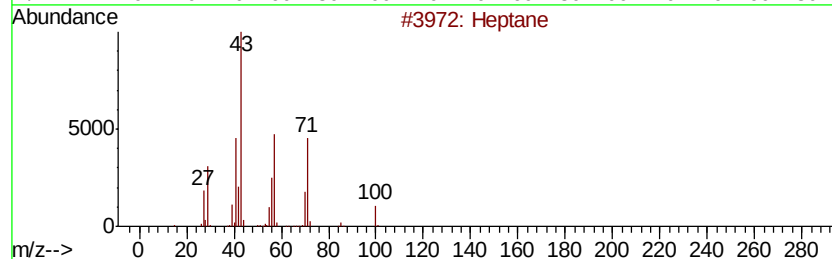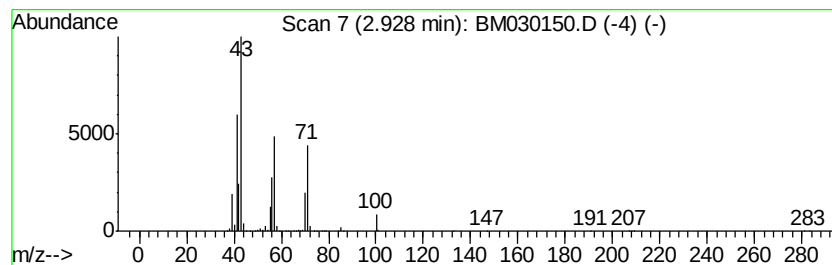

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM052021\
Data File : BM030150.D
Acq On : 22 May 2021 15:03
Operator : CG/JU
Sample : PB136569BL
Misc :
ALS Vial : 66 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK569

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM050721.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	---Internal Standard---			
					#	RT	Resp	Conc
(DEL) Alkane: Str...	2.93	27.4	ng/ul	1165220	1	7.50	851925	20.0