
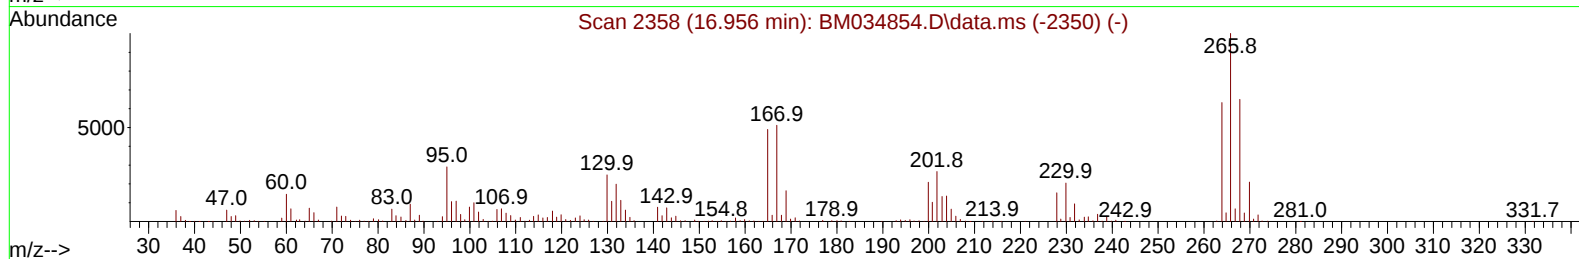
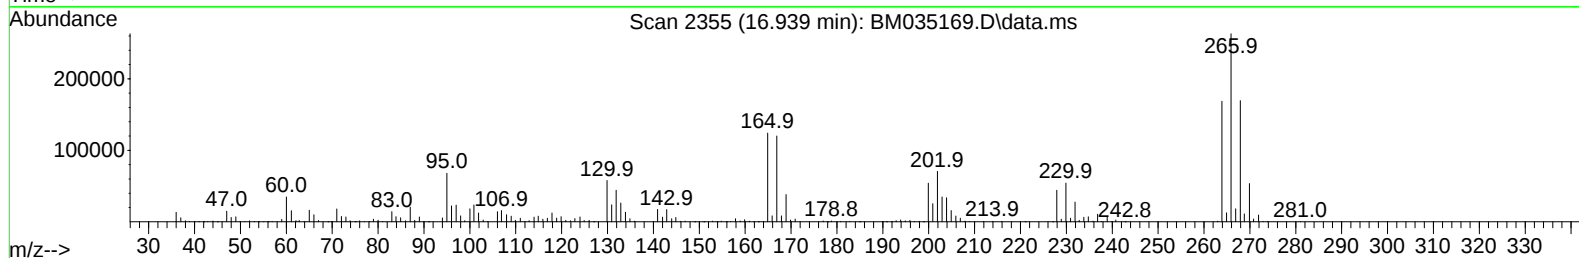


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM052022\
Data File : BM035169.D
Acq On : 20 May 2022 09:20
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 23 05:30:05 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM042722.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri May 20 04:53:59 2022
Response via : Initial Calibration

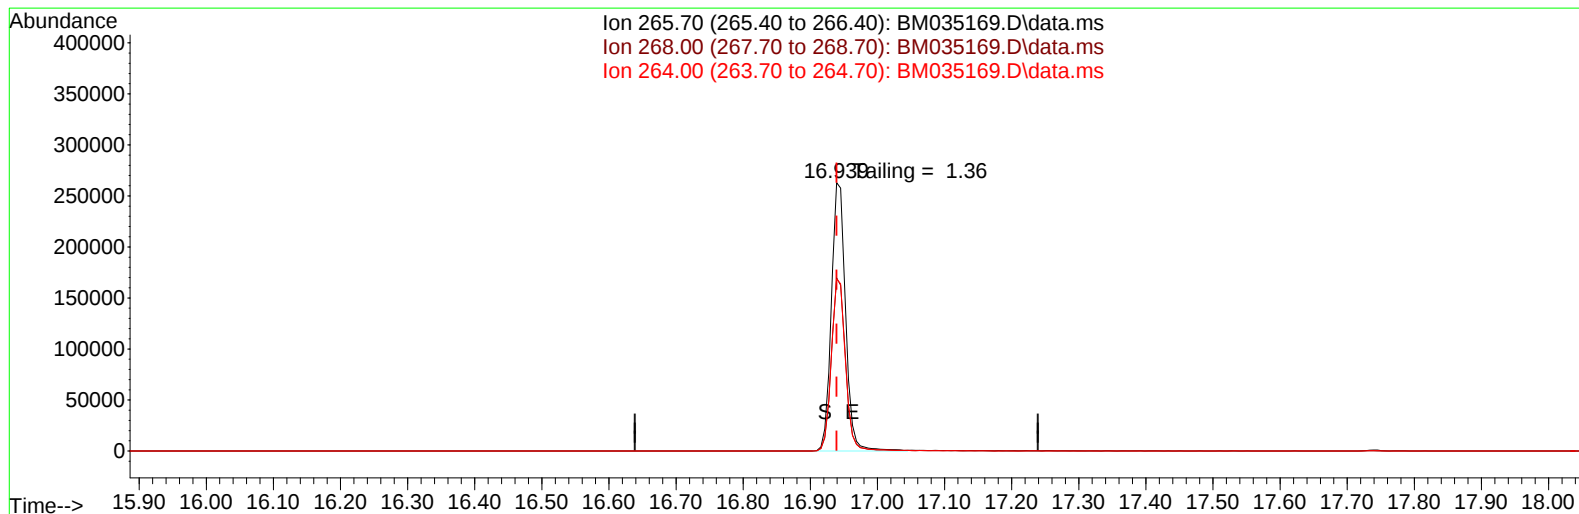

TIC: BM035169.D\data.ms

(70) Pentachlorophenol (C)




16.939min (+ 0.000) 189338.60 ng

response 386653

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.90	64.45
264.00	63.30	64.14
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM052022\
Data File : BM035169.D
Acq On : 20 May 2022 09:20
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 23 05:30:05 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM042722.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri May 20 04:53:59 2022
Response via : Initial Calibration

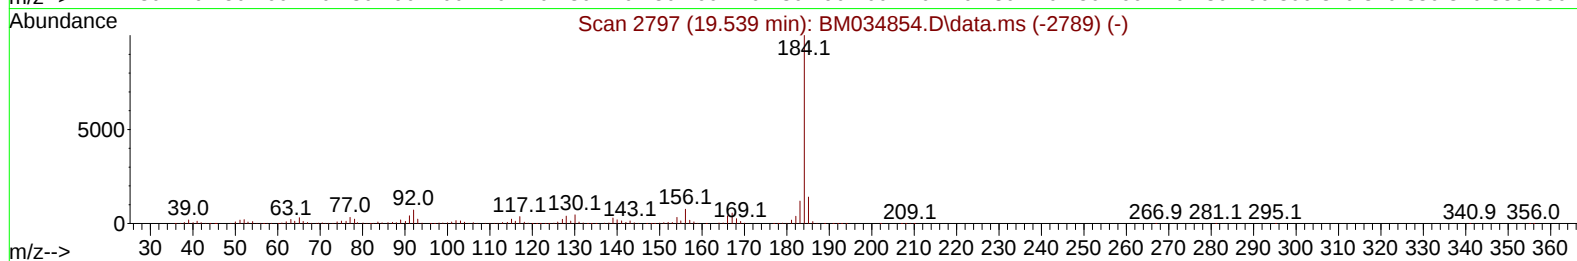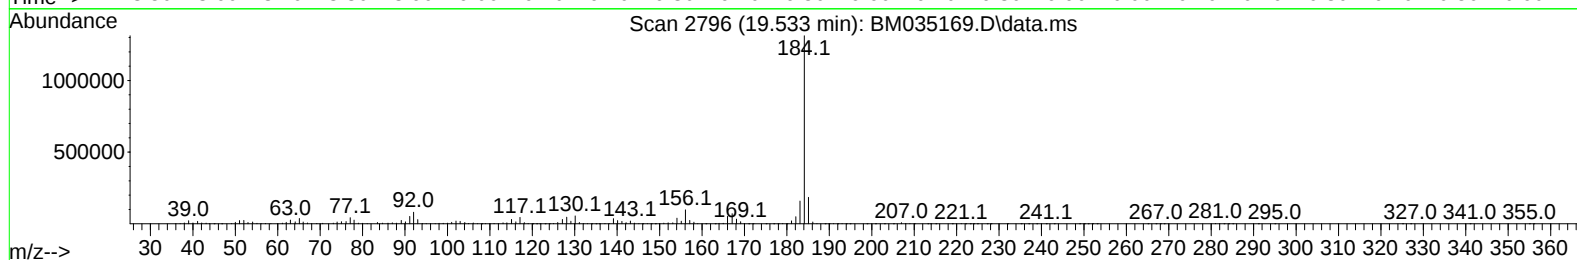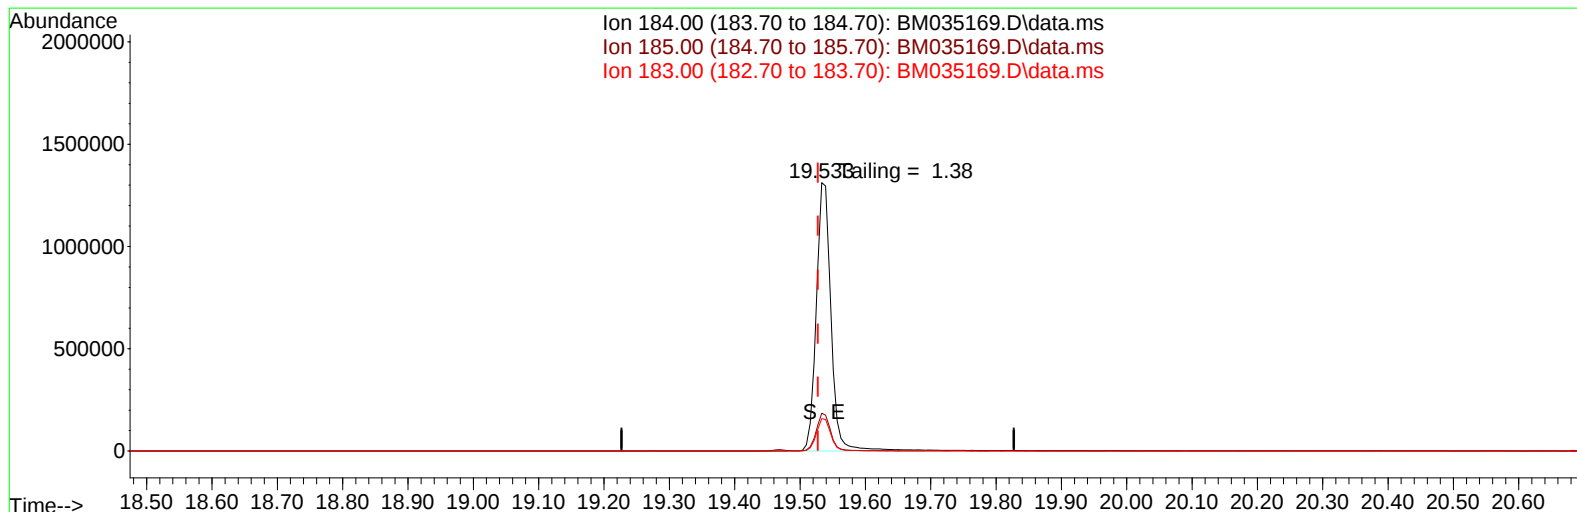

TIC: BM035169.D\data.ms

(77) Benzidine**19.533min (+ 0.006) 107574.34 ng****response 2060526**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.10	14.07
183.00	11.90	12.08
0.00	0.00	0.00