

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM052022\
 Data File : BM035186.D
 Acq On : 20 May 2022 21:01
 Operator : CG/JU
 Sample : N2880-02DL 5X
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 EFF-WWDL

Quant Time: May 23 04:21:52 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM042722.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri May 20 04:53:59 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.904	152	160899	20.000	ng	0.00
21) Naphthalene-d8	10.704	136	675554	20.000	ng	0.00
39) Acenaphthene-d10	14.545	164	462128	20.000	ng	0.00
64) Phenanthrene-d10	17.309	188	1058927	20.000	ng	0.02
76) Chrysene-d12	21.474	240	1127460	20.000	ng	# 0.00
86) Perylene-d12	23.856	264	1159018	20.000	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.487	112	37949	4.161	ng	0.00
7) Phenol-d6	7.081	99	47499	4.034	ng	0.00
23) Nitrobenzene-d5	9.063	82	112903	9.025	ng	0.00
42) 2,4,6-Tribromophenol	16.039	330	38075	7.574	ng	0.00
45) 2-Fluorobiphenyl	13.168	172	267210	8.394	ng	0.00
79) Terphenyl-d14	19.915	244	192046	3.298	ng	0.00
Target Compounds						
32) Benzoic acid	9.969	122	16846	2.480	ng	Qvalue 94


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM052022\
Data File : BM035186.D
Acq On : 20 May 2022 21:01
Operator : CG/JU
Sample : N2880-02DL 5X
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
EFF-WWDL

Quant Time: May 23 04:21:52 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM042722.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri May 20 04:53:59 2022
Response via : Initial Calibration




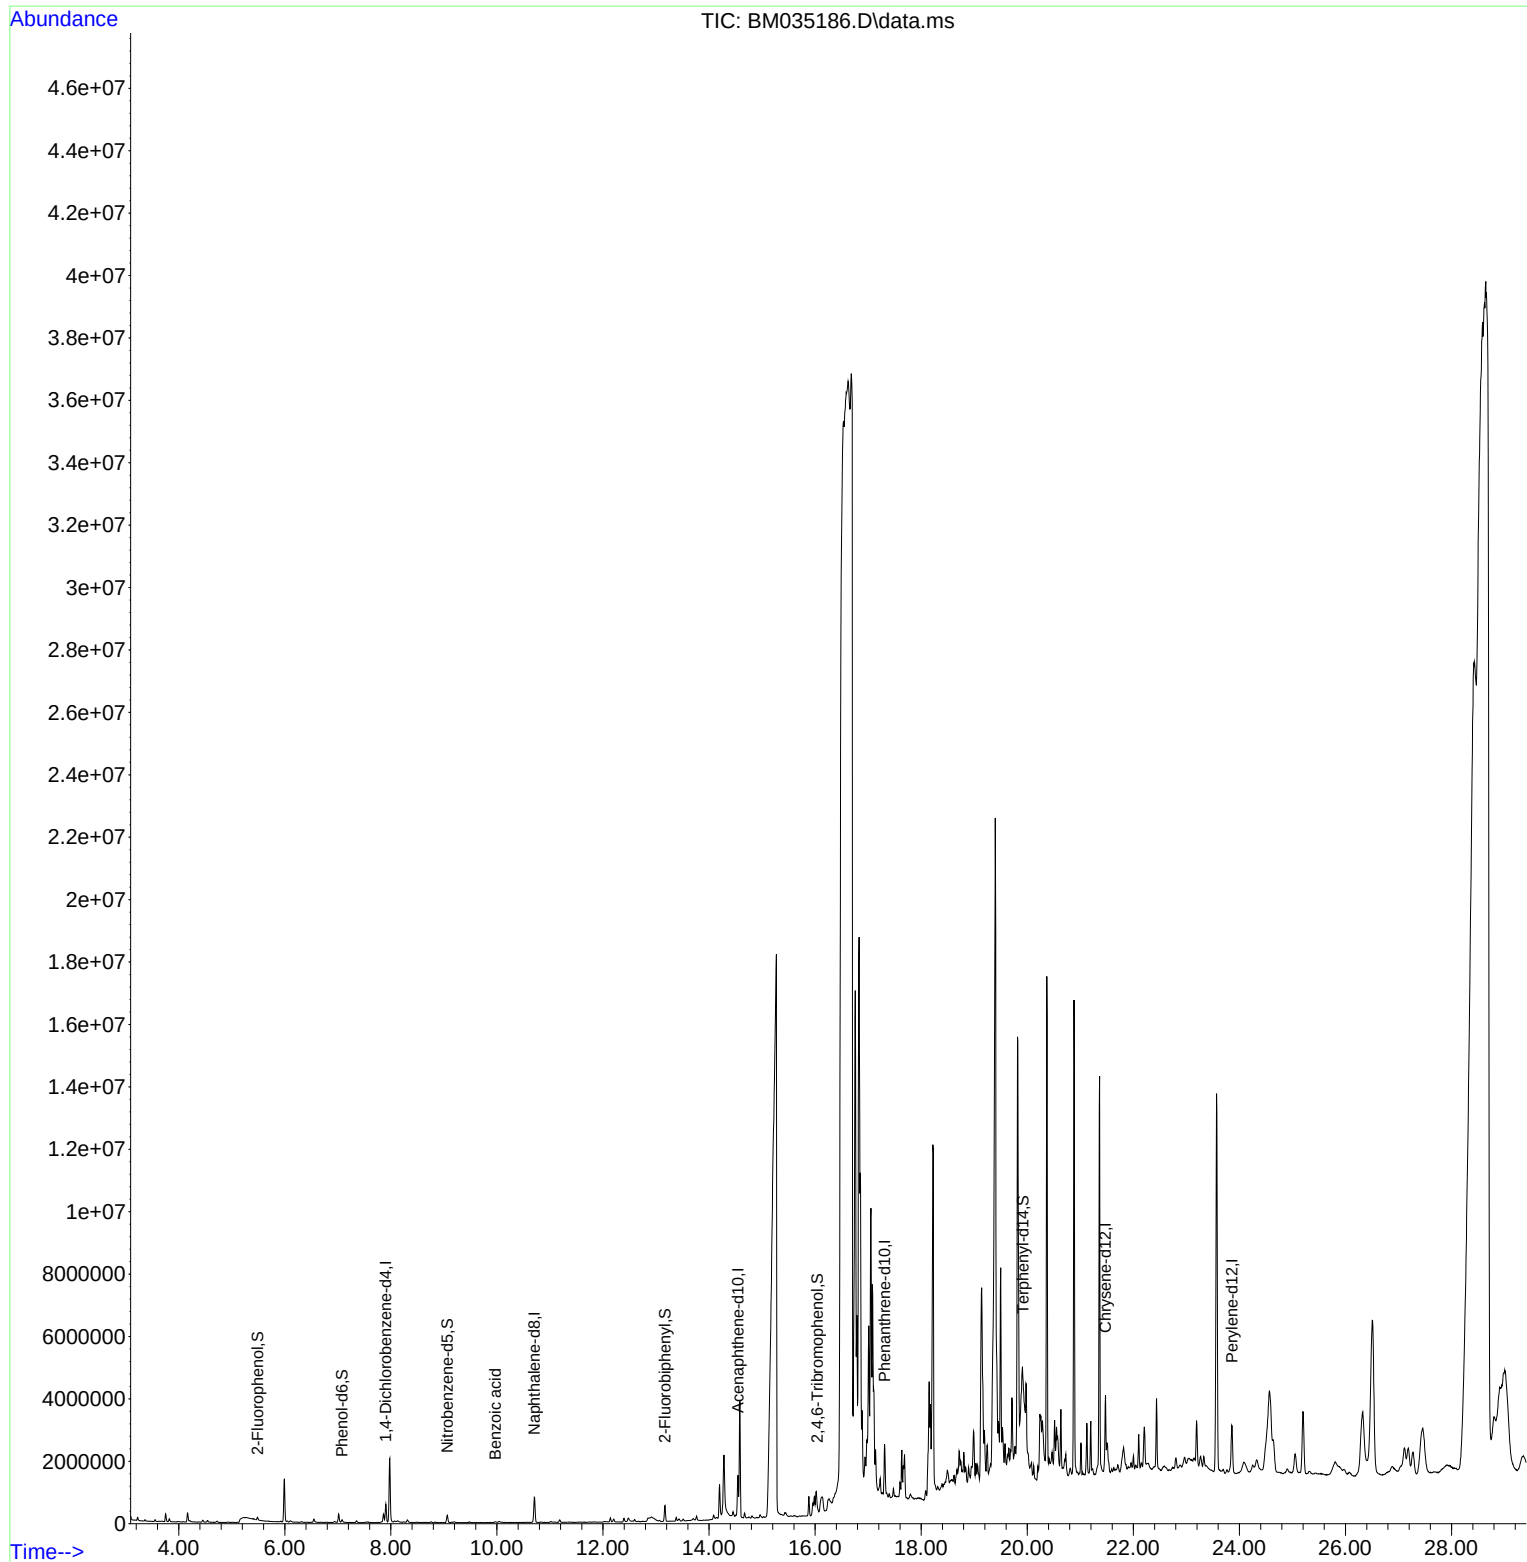


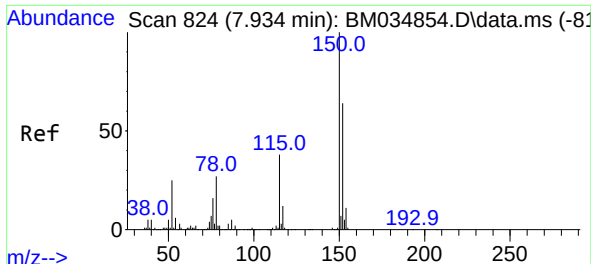

#1
1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 7.904 min Scan# 81
Delta R.T. 0.000 min
Lab File: BM035186.D
Acq: 20 May 2022 21:01




Instrument :
BNA_M
ClientSampleId :
EFF-WWDL


Tgt Ion:152 Resp: 160899
Ion Ratio Lower Upper
152 100
150 154.9 124.9 187.3
115 57.4 47.9 71.9

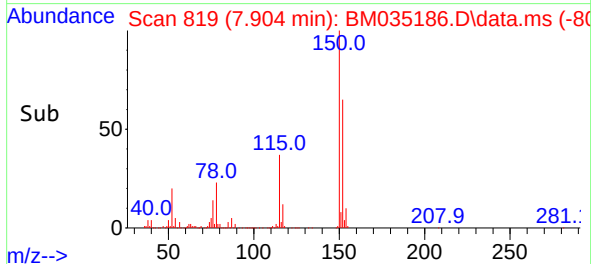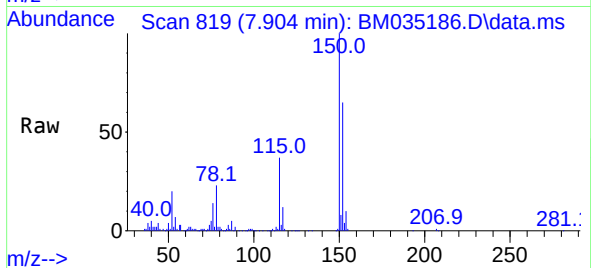

#5
2-Fluorophenol
Concen: 4.161 ng
RT: 5.487 min Scan# 408
Delta R.T. 0.006 min
Lab File: BM035186.D
Acq: 20 May 2022 21:01

Tgt Ion:112 Resp: 37949
Ion Ratio Lower Upper
112 100
64 58.2 47.8 71.6
63 31.2 26.6 40.0


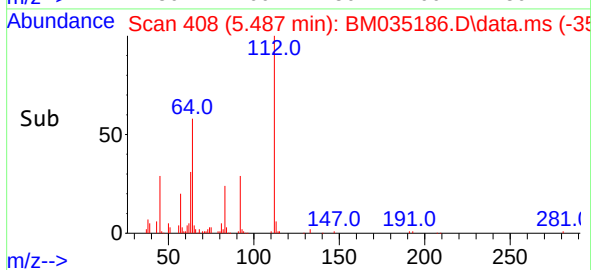

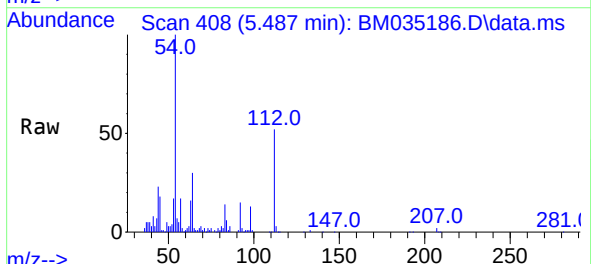




#7
Phenol-d6
Concen: 4.034 ng
RT: 7.081 min Scan# 61
Delta R.T. 0.006 min
Lab File: BM035186.D
Acq: 20 May 2022 21:01




Instrument :
BNA_M
ClientSampleId :
EFF-WWDL


Tgt Ion: 99 Resp: 47499
Ion Ratio Lower Upper
99 100
42 22.9 18.8 28.2
71 37.0 30.2 45.2

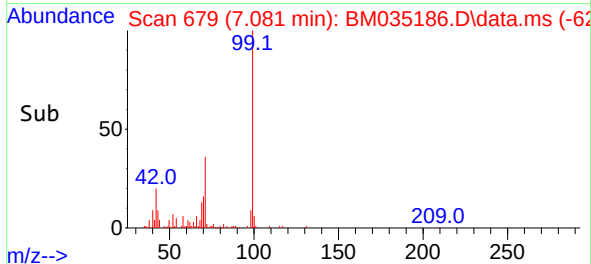

#21
Naphthalene-d8
Concen: 20.000 ng
RT: 10.704 min Scan# 1295
Delta R.T. -0.006 min
Lab File: BM035186.D
Acq: 20 May 2022 21:01

Tgt Ion: 136 Resp: 675554
Ion Ratio Lower Upper
136 100
137 11.4 8.9 13.3
54 7.7 7.0 10.4
68 4.7 4.3 6.5

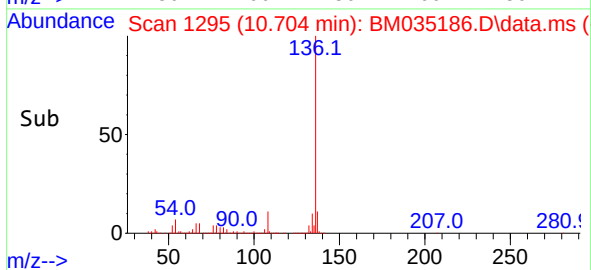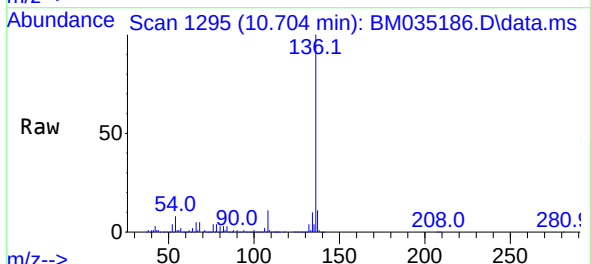



#23

Nitrobenzene-d5

Concen: 9.025 ng

RT: 9.063 min Scan# 1

Delta R.T. -0.000 min

Lab File: BM035186.D

Acq: 20 May 2022 21:01

Instrument :

BNA_M

ClientSampleId :

EFF-WWDL





Tgt Ion: 82 Resp: 112903

Ion Ratio Lower Upper

82 100

128 43.9 33.7 50.5

54 53.2 43.2 64.8

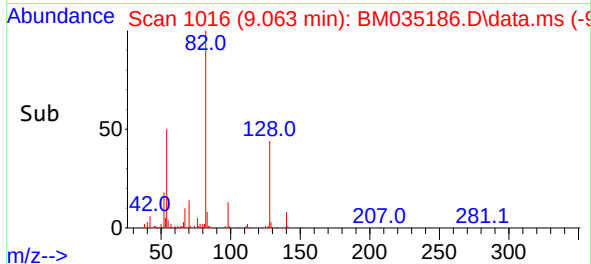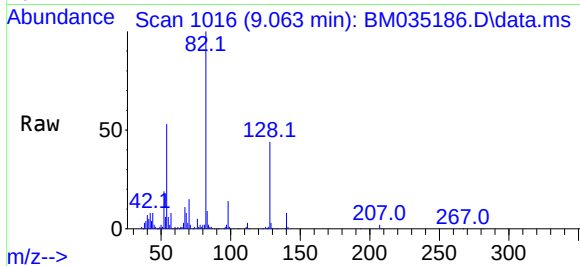

#32

Benzoic acid

Concen: 2.480 ng

RT: 9.969 min Scan# 1170

Delta R.T. -0.053 min

Lab File: BM035186.D

Acq: 20 May 2022 21:01




Tgt Ion:122 Resp: 16846


Ion Ratio Lower Upper

122 100

105 132.7 105.7 145.7

77 107.0 80.0 120.0


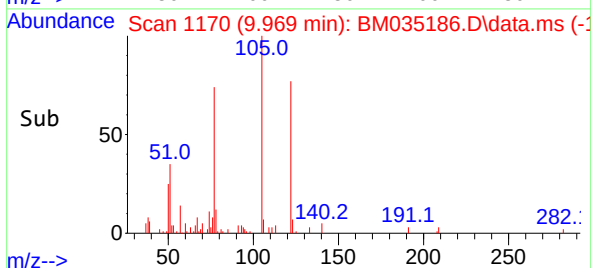
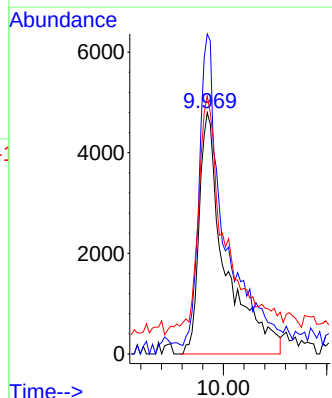
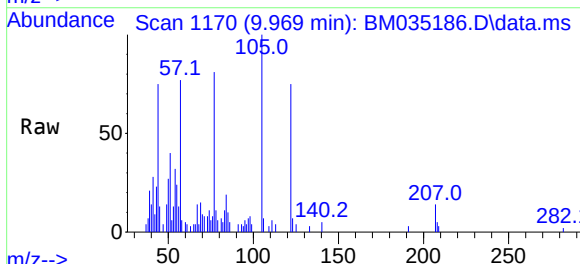




#39
Acenaphthene-d10
Concen: 20.000 ng
RT: 14.545 min Scan# 1948
Delta R.T. -0.000 min
Lab File: BM035186.D
Acq: 20 May 2022 21:01




Instrument :
BNA_M
ClientSampleId :
EFF-WWDL


Tgt Ion:164 Resp: 462128
Ion Ratio Lower Upper
164 100
162 104.1 83.0 124.6
160 45.4 37.0 55.4

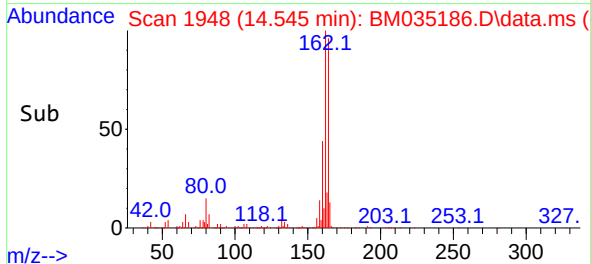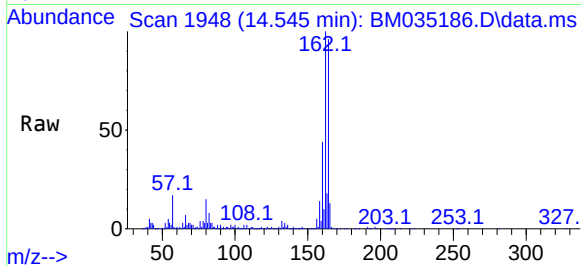

#42
2,4,6-Tribromophenol
Concen: 7.574 ng
RT: 16.039 min Scan# 2202
Delta R.T. 0.006 min
Lab File: BM035186.D
Acq: 20 May 2022 21:01

Tgt Ion:330 Resp: 38075
Ion Ratio Lower Upper
330 100
332 98.4 77.0 115.4
141 32.3 35.3 52.9#


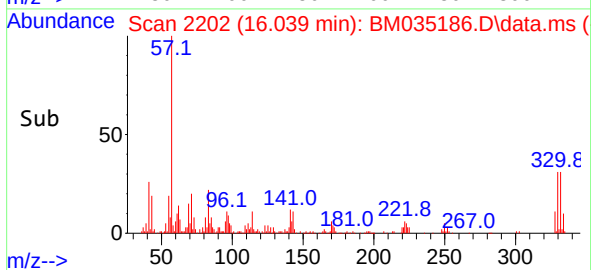

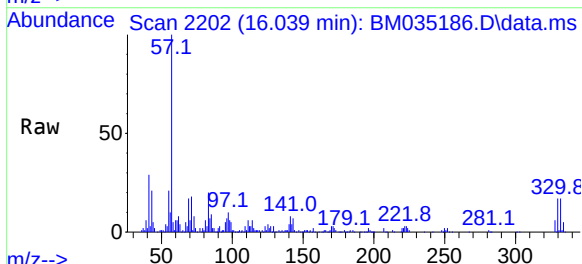




#45
2-Fluorobiphenyl
Concen: 8.394 ng
RT: 13.168 min Scan# 1
Delta R.T. -0.000 min
Lab File: BM035186.D
Acq: 20 May 2022 21:01




Instrument :
BNA_M
ClientSampleId :
EFF-WWDL


Tgt Ion:172 Resp: 267210
Ion Ratio Lower Upper
172 100
171 35.4 28.5 42.7
170 23.3 18.7 28.1

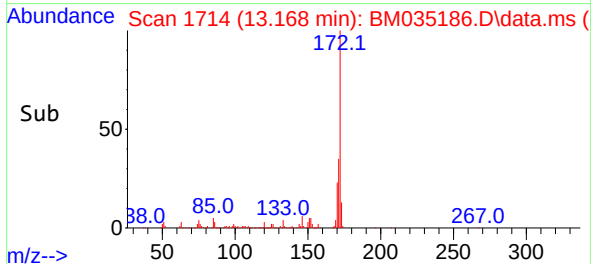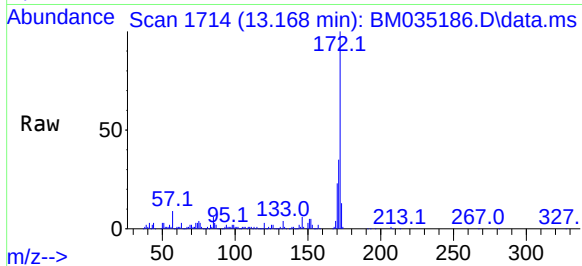

#64
Phenanthrene-d10
Concen: 20.000 ng
RT: 17.309 min Scan# 2418
Delta R.T. 0.023 min
Lab File: BM035186.D
Acq: 20 May 2022 21:01

Tgt Ion:188 Resp: 1058927
Ion Ratio Lower Upper
188 100
94 7.2 7.0 10.4
80 8.0 7.6 11.4


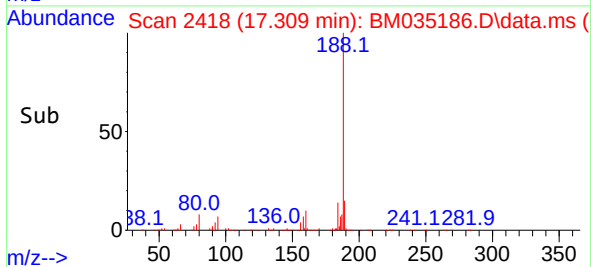

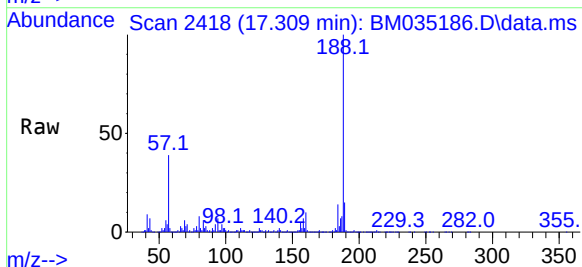


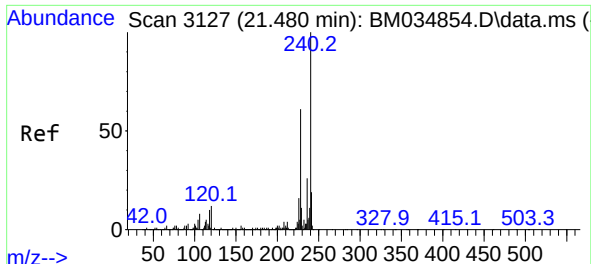

#76
Chrysene-d12
Concen: 20.000 ng
RT: 21.474 min Scan# 31
Delta R.T. -0.000 min
Lab File: BM035186.D
Acq: 20 May 2022 21:01




Instrument :
BNA_M
ClientSampleId :
EFF-WWDL


Tgt Ion:240 Resp: 1127460
Ion Ratio Lower Upper
240 100
120 8.2 9.4 14.0#
236 25.1 20.6 30.8

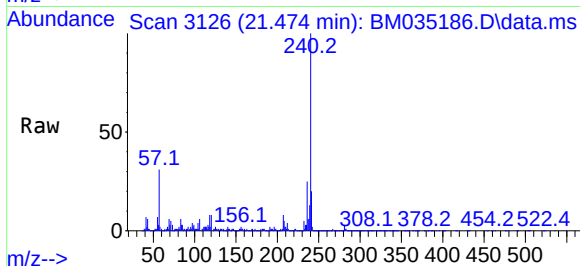

#79
Terphenyl-d14
Concen: 3.298 ng
RT: 19.915 min Scan# 2861
Delta R.T. -0.000 min
Lab File: BM035186.D
Acq: 20 May 2022 21:01

Tgt Ion:244 Resp: 192046
Ion Ratio Lower Upper
244 100
212 7.2 6.2 9.4
122 8.7 8.3 12.5

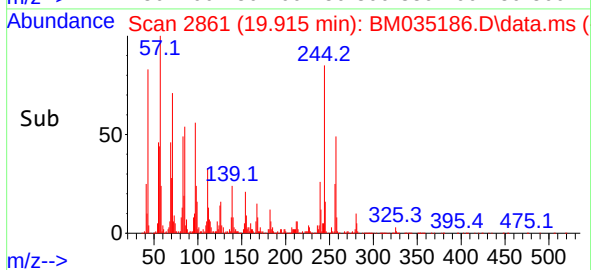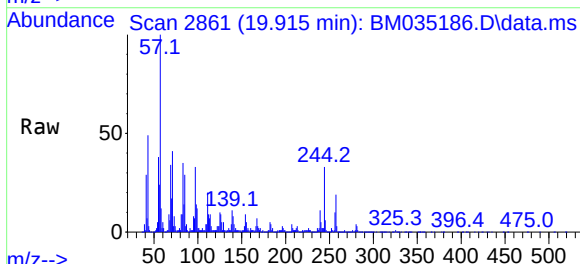

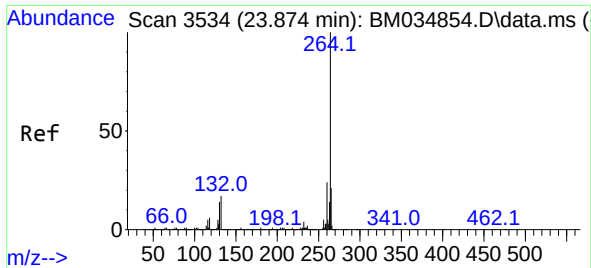

#86

Perylene-d12

Concen: 20.000 ng

RT: 23.856 min Scan# 3

Delta R.T. -0.000 min

Lab File: BM035186.D


Acq: 20 May 2022 21:01

Instrument :

BNA_M

ClientSampleId :

EFF-WWDL

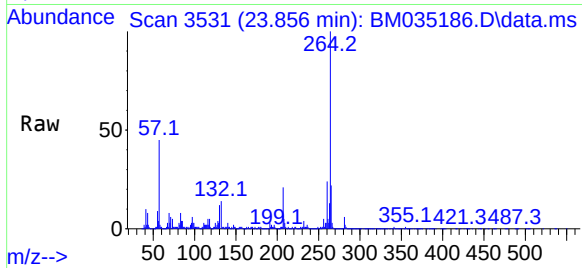

Tgt Ion:264 Resp: 1159018

Ion Ratio Lower Upper

264 100

260 23.8 18.9 28.3

265 22.0 17.5 26.3

