

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM052022\
 Data File : BM035175.D
 Acq On : 20 May 2022 14:12
 Operator : CG/JU
 Sample : PB144911BL
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 PB144911BL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM042722.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BM035175.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.481	400	407	420	rBV	3410401	5008744	38.75%	9.524%
2	7.075	671	678	696	rBV	3239496	5281643	40.86%	10.043%
3	7.904	810	819	833	rVB	608885	960377	7.43%	1.826%
4	9.063	1008	1016	1029	rBV	2009369	3343935	25.87%	6.358%
5	10.704	1287	1295	1307	rBV	777141	1340038	10.37%	2.548%
6	13.168	1707	1714	1726	rBV	5754761	8218611	63.58%	15.627%
7	14.545	1941	1948	1961	rBV	1269297	1916233	14.82%	3.644%
8	16.033	2193	2201	2215	rBV	4390255	6407204	49.57%	12.183%
9	17.286	2407	2414	2427	rBV	1636119	2304587	17.83%	4.382%
10	19.915	2855	2861	2866	rBV	10761395	12926257	100.00%	24.578%
11	21.468	3120	3125	3133	rBV	2028799	2505464	19.38%	4.764%
12	23.856	3525	3531	3544	rVB2	1119995	2379092	18.41%	4.524%


Sum of corrected areas: 52592185

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM052022\
Data File : BM035175.D
Acq On : 20 May 2022 14:12
Operator : CG/JU
Sample : PB144911BL
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB144911BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM042722.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

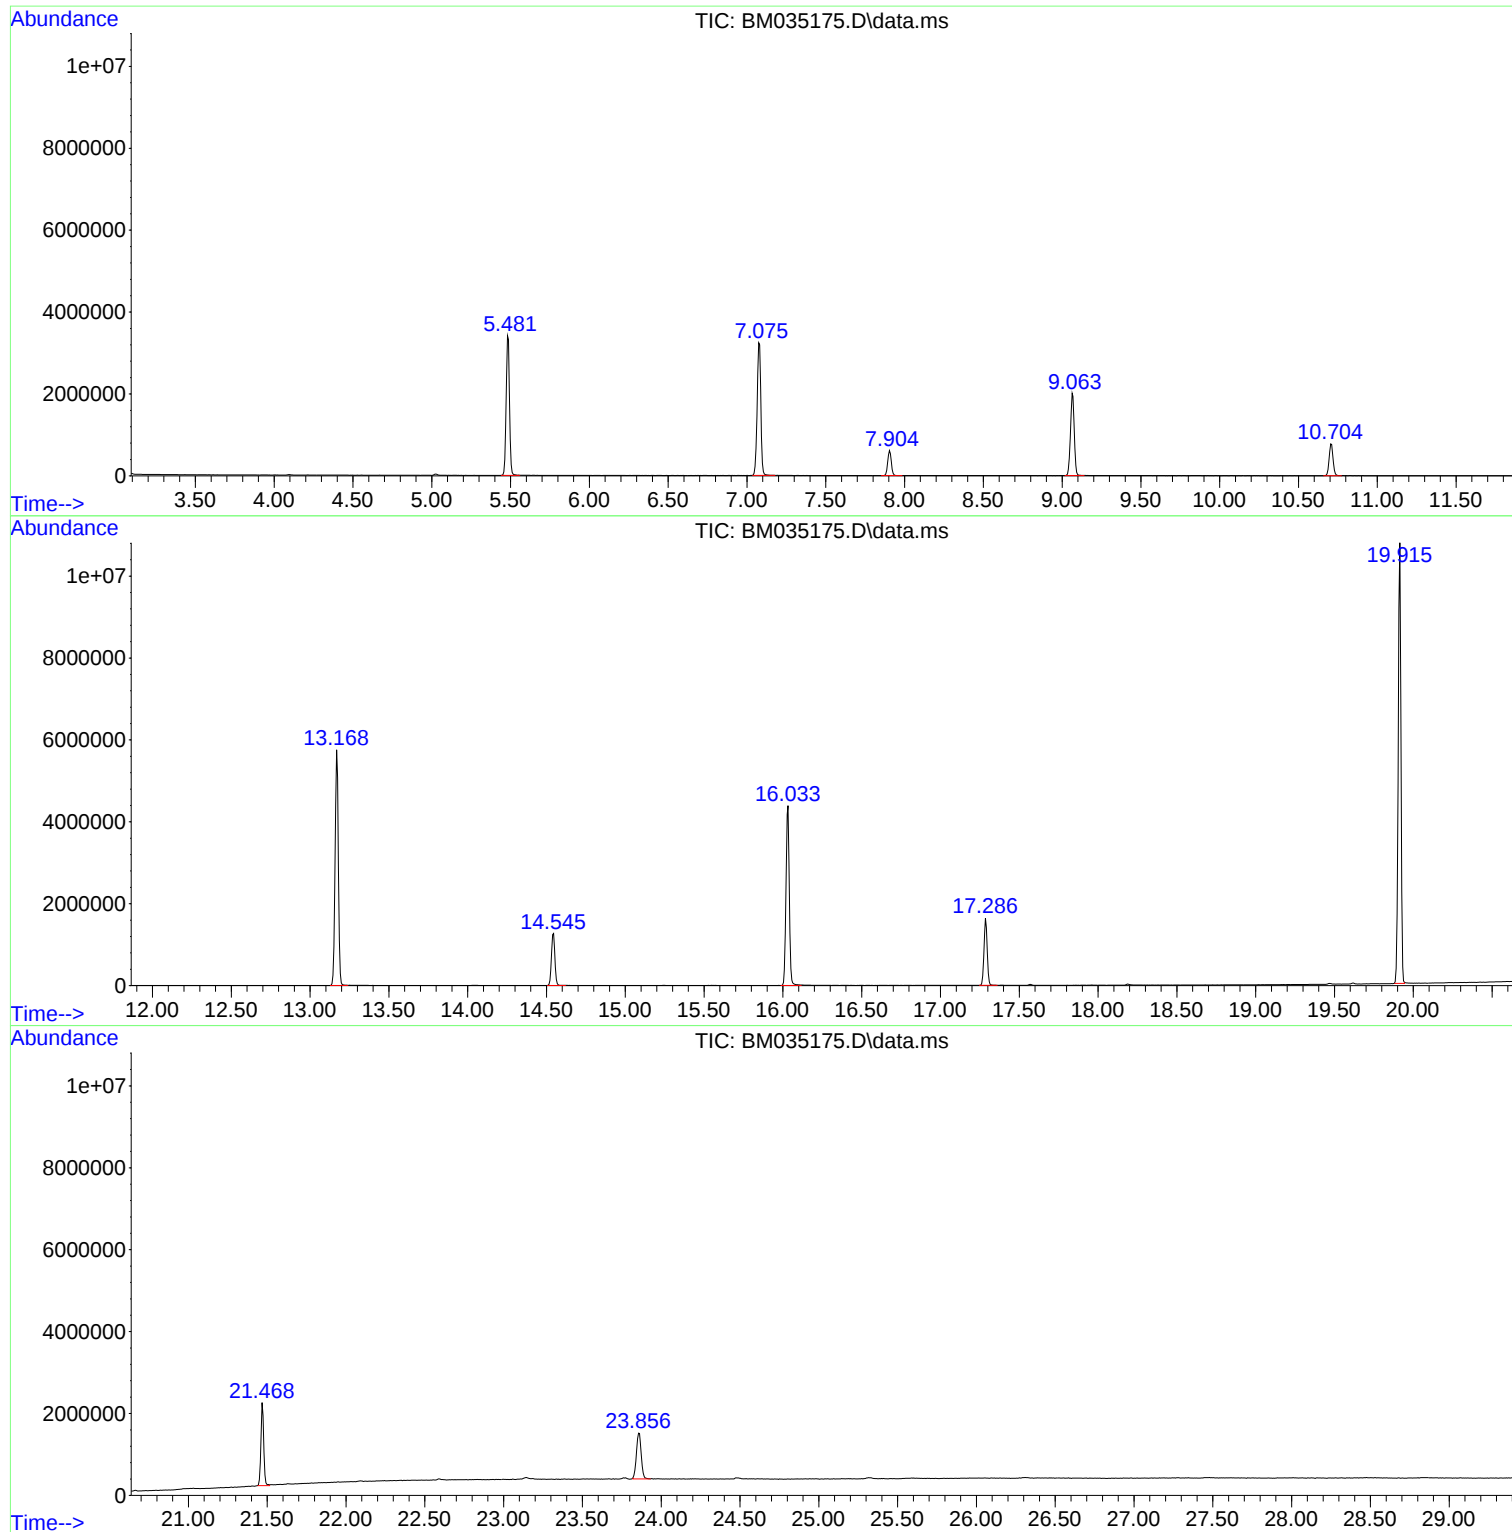

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM052022\
Data File : BM035175.D
Acq On : 20 May 2022 14:12
Operator : CG/JU
Sample : PB144911BL
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB144911BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM042722.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM052022\
Data File : BM035175.D
Acq On : 20 May 2022 14:12
Operator : CG/JU
Sample : PB144911BL
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB144911BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM042722.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------