
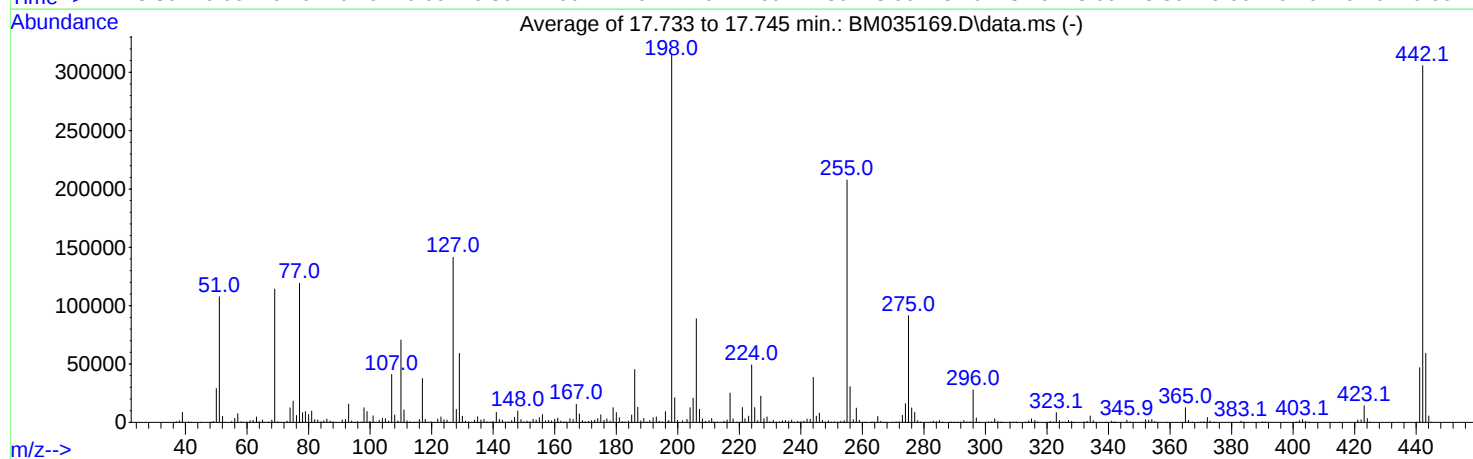


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM052022\
 Data File : BM035169.D
 Acq On : 20 May 2022 09:20
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM042722.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri May 20 04:53:59 2022

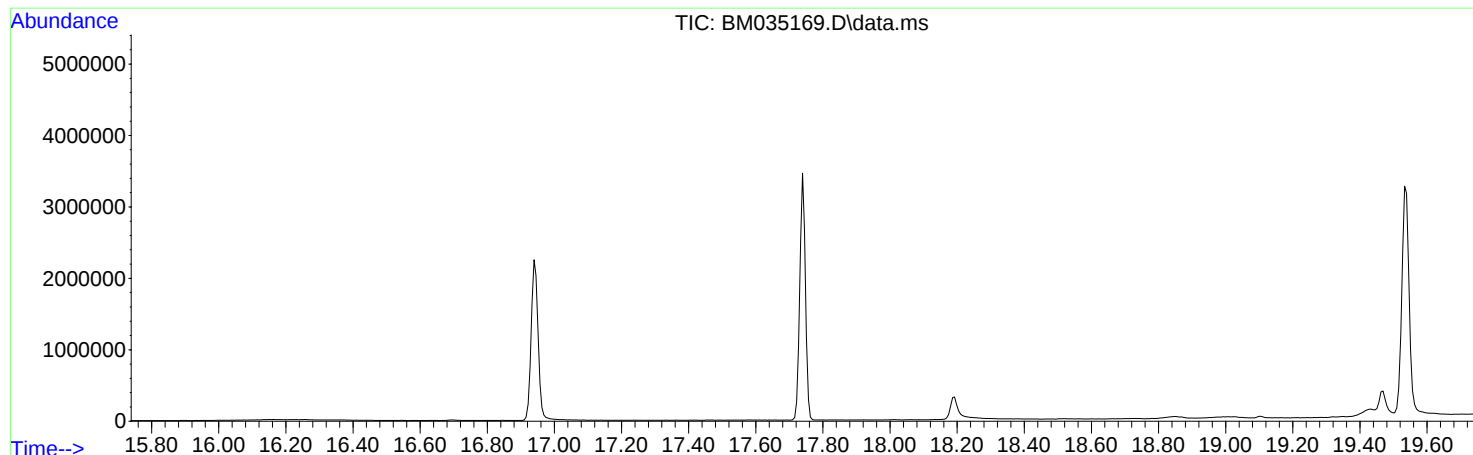




AutoFind: Scans 2490, 2491, 2492; Background Corrected with Scan 2483

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	34.1	107588	PASS
68	69	0.00	2	1.8	2089	PASS
69	198	0.00	100	36.3	114288	PASS
70	69	0.00	2	0.5	597	PASS
127	198	10	80	44.9	141416	PASS
197	198	0.00	2	0.5	1643	PASS
198	198	100	100	100.0	315264	PASS
199	198	5	9	6.7	21171	PASS
275	198	10	60	28.9	91267	PASS
365	198	1	100	4.0	12620	PASS
441	198	0.01	100	14.9	46933	PASS
442	442	50	100	100.0	305813	PASS
443	442	15	24	19.3	59101	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM052022\
 Data File : BM035169.D
 Acq On : 20 May 2022 09:20
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Quant Time: May 23 05:30:05 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM042722.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri May 20 04:53:59 2022
 Response via : Initial Calibration

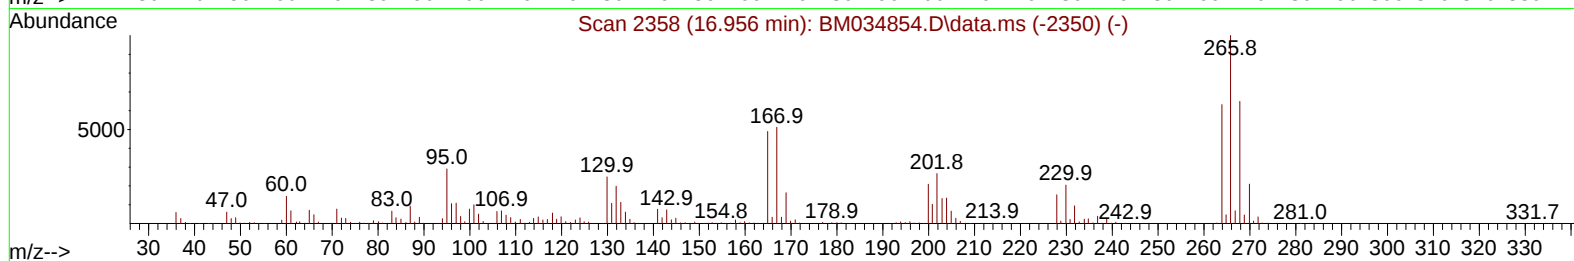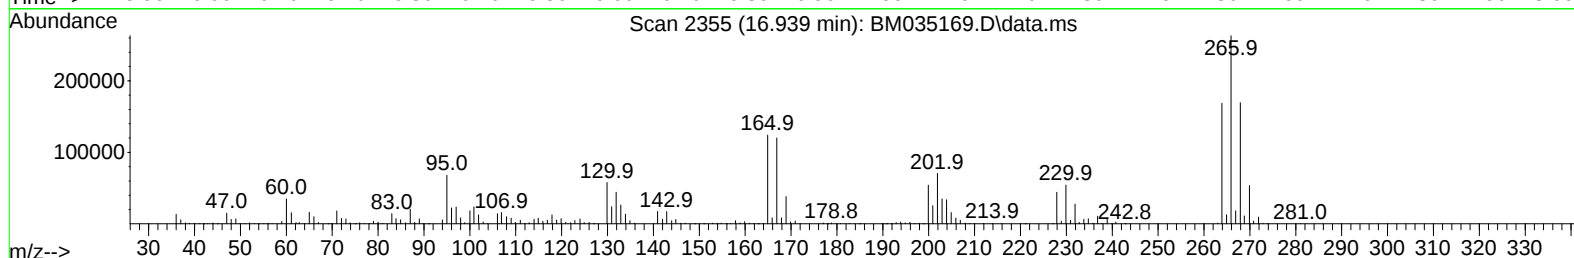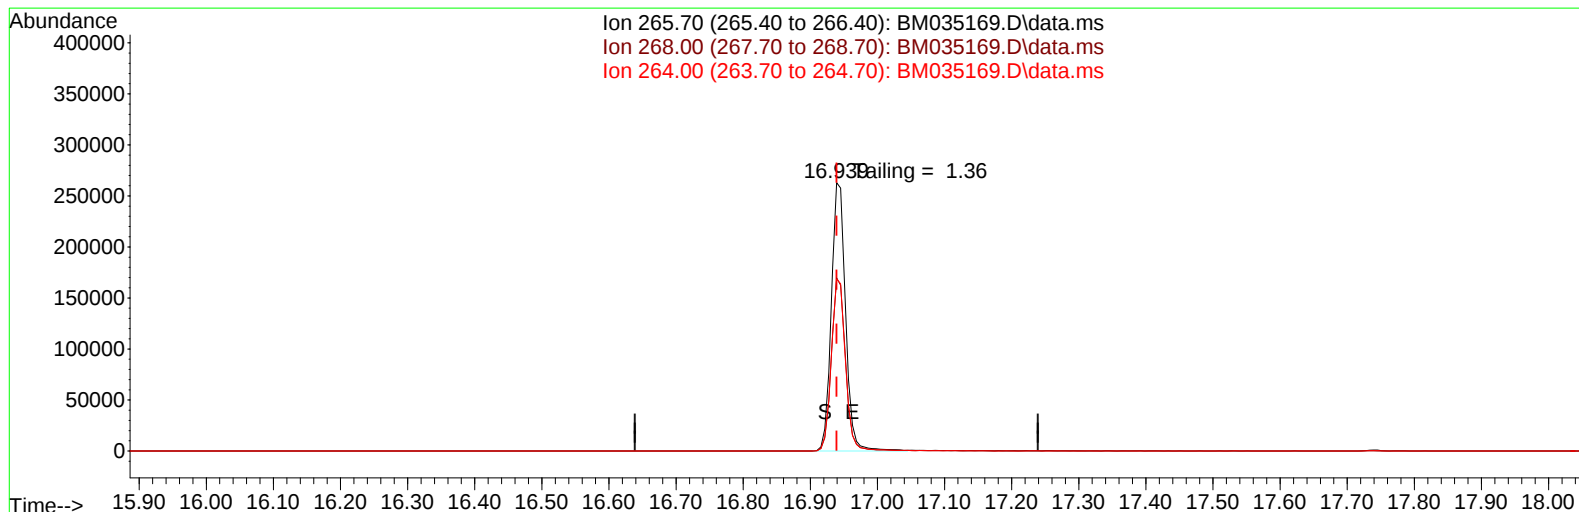

TIC: BM035169.D\data.ms

(70) Pentachlorophenol (C)

16.939min (+ 0.000) 189338.60 ng




response 386653

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.90	64.45
264.00	63.30	64.14
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM052022\
 Data File : BM035169.D
 Acq On : 20 May 2022 09:20
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Quant Time: May 23 05:30:05 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM042722.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri May 20 04:53:59 2022
 Response via : Initial Calibration

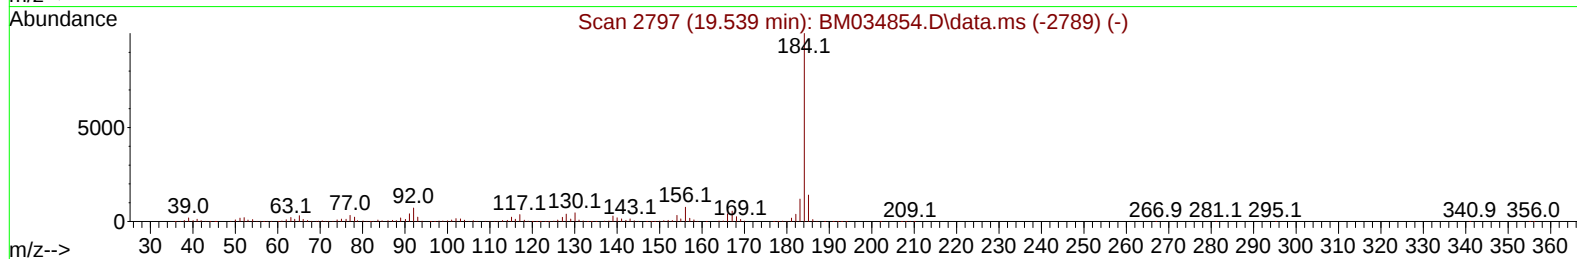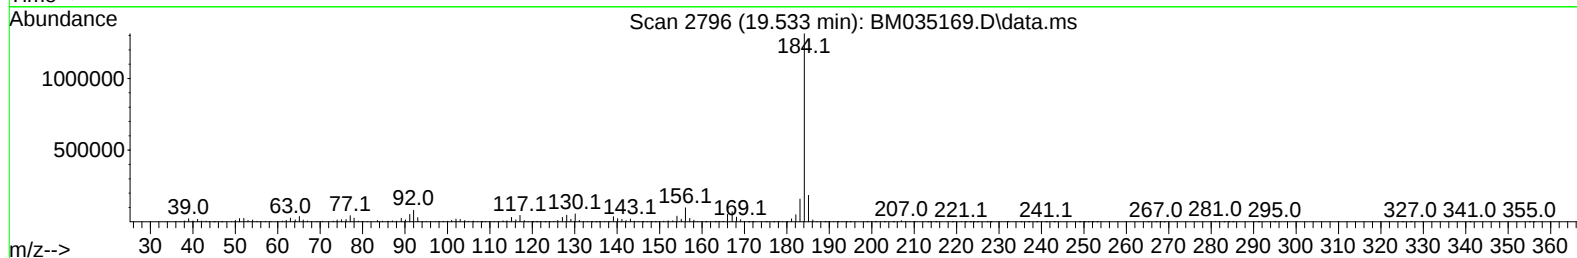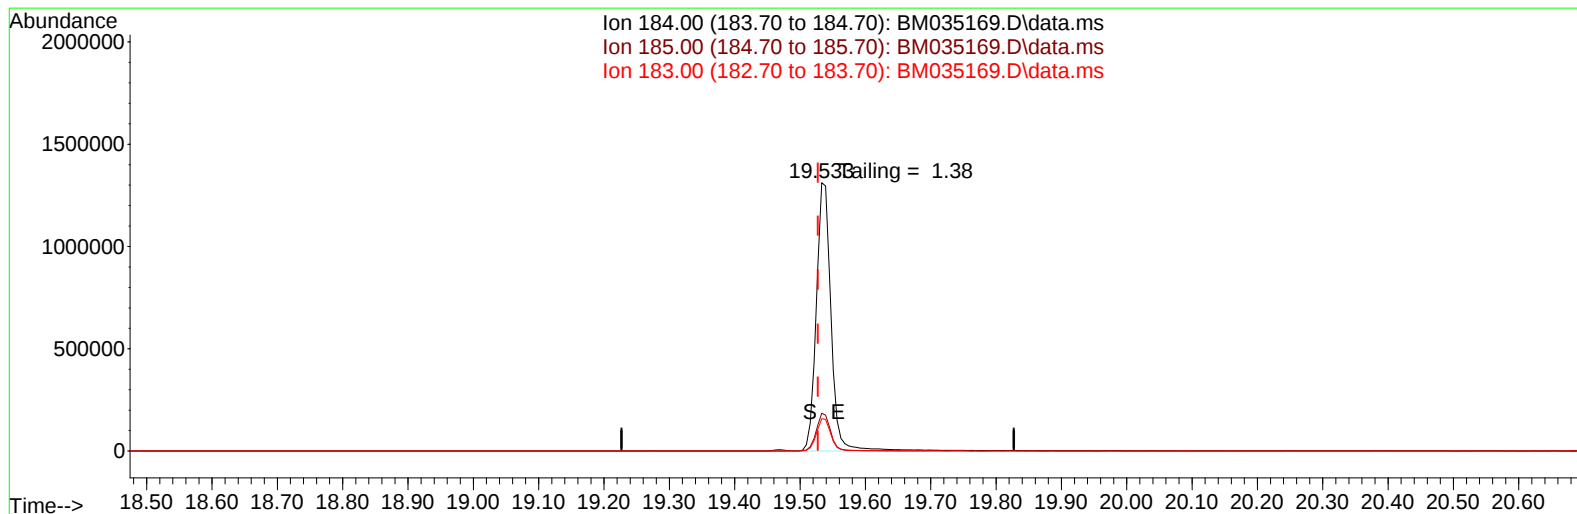

TIC: BM035169.D\data.ms

(77) Benzidine

19.533min (+ 0.006) 107574.34 ng

response 2060526

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.10	14.07
183.00	11.90	12.08
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
5/20/2022	BNA_M	<u>BM035169.D</u>
Compound Name	Response	Retention Time
DDT	1156057	20.768
DDD	14281	20.327
DDE	711	19.821
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
14992	1171049	1.28

Instrument :
BNA_M
ClientSampleId :
DFTPP