

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM052116\
 Data File : BM005570.D
 Acq On : 22 May 2016 03:01
 Operator : UM/SJ
 Sample : H2890-16
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 D9WY6

Quant Time: May 22 05:34:57 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM052016.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sun May 22 05:33:20 2016
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.82	152	122511	20.00	ng/ul	0.00
18) Naphthalene-d8	10.61	136	538229	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.46	164	307097	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.20	188	661152	20.00	ng/ul	0.00
75) Chrysene-d12	21.37	240	588612	20.00	ng/ul	0.00
83) Perylene-d12	23.65	264	600073	20.00	ng/ul	0.01

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.31	96	6574	2.35	ng/uL	0.00
5) Phenol-d5	6.99	99	155775	15.51	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.16	67	86499	14.86	ng/ul	0.00
9) 2-Chlorophenol-d4	7.36	132	123067	14.69	ng/ul	0.00
13) 4-Methylphenol-d8	8.52	113	133501	16.22	ng/ul	0.00
19) Nitrobenzene-d5	8.97	128	60556	14.72	ng/ul	0.00
22) 2-Nitrophenol-d4	9.70	143	64829	14.31	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.23	165	127577	14.95	ng/ul	0.00
29) 4-Chloroaniline-d4	10.75	131	171095	20.02	ng/ul	0.00
43) Dimethylphthalate-d6	13.86	166	426237	17.00	ng/ul	0.00
46) Acenaphthylene-d8	14.14	160	509285	16.25	ng/ul	0.00
51) 4-Nitrophenol-d4	14.65	143	3775	0.80	ng/ul	0.00
57) Fluorene-d10	15.44	176	368436	16.89	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.56	200	1941	0.51	ng/ul	0.00
70) Anthracene-d10	17.29	188	564989	17.94	ng/ul	0.00
76) Pyrene-d10	19.58	212	571509	21.44	ng/ul	0.00
87) Benzo(a)pyrene-d12	23.50	264	510096	18.20	ng/ul	0.00

Target Compounds


						Qvalue
28) Naphthalene	10.66	128	31891	1.18	ng/ul	97
34) 2-Methylnaphthalene	12.27	142	202124	10.22	ng/ul	99
40) 1,1'-Biphenyl	13.29	154	36514	1.42	ng/ul	99
44) Dimethylphthalate	13.91	163	155664	6.28	ng/ul	100
69) Phenanthrene	17.24	178	205429	5.56	ng/ul	99
71) Anthracene	17.33	178	53370	1.42	ng/ul	99
73) Di-n-butylphthalate	18.16	149	575766	14.52	ng/ul	100
74) Fluoranthene	19.25	202	377675	9.08	ng/ul	99
77) Pyrene	19.61	202	305150	9.02	ng/ul	99
79) 3,3'-Dichlorobenzidine	21.29	252	11406	1.07	ng/ul#	93
80) Benzo(a)anthracene	21.35	228	158914	4.59	ng/ul	97
82) Chrysene	21.35	228	158914	4.83	ng/ul	96
85) Benzo(b)fluoranthene	22.96	252	194360	5.49	ng/ul#	90
86) Benzo(k)fluoranthene	22.96	252	194360	5.80	ng/ul#	91
88) Benzo(a)pyrene	23.55	252	142250	4.14	ng/ul#	90
89) Indeno(1,2,3-cd)pyrene	25.96	276	97359	2.39	ng/ul	99
91) Benzo(g,h,i)perylene	26.66	276	89912	2.62	ng/ul	94


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM052116\
Data File : BM005570.D
Acq On : 22 May 2016 03:01
Operator : UM/SJ
Sample : H2890-16
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
D9WY6

Quant Time: May 22 05:34:57 2016
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM052016.M
Quant Title : SVOA CALIBRATION
QLast Update : Sun May 22 05:33:20 2016
Response via : Initial Calibration

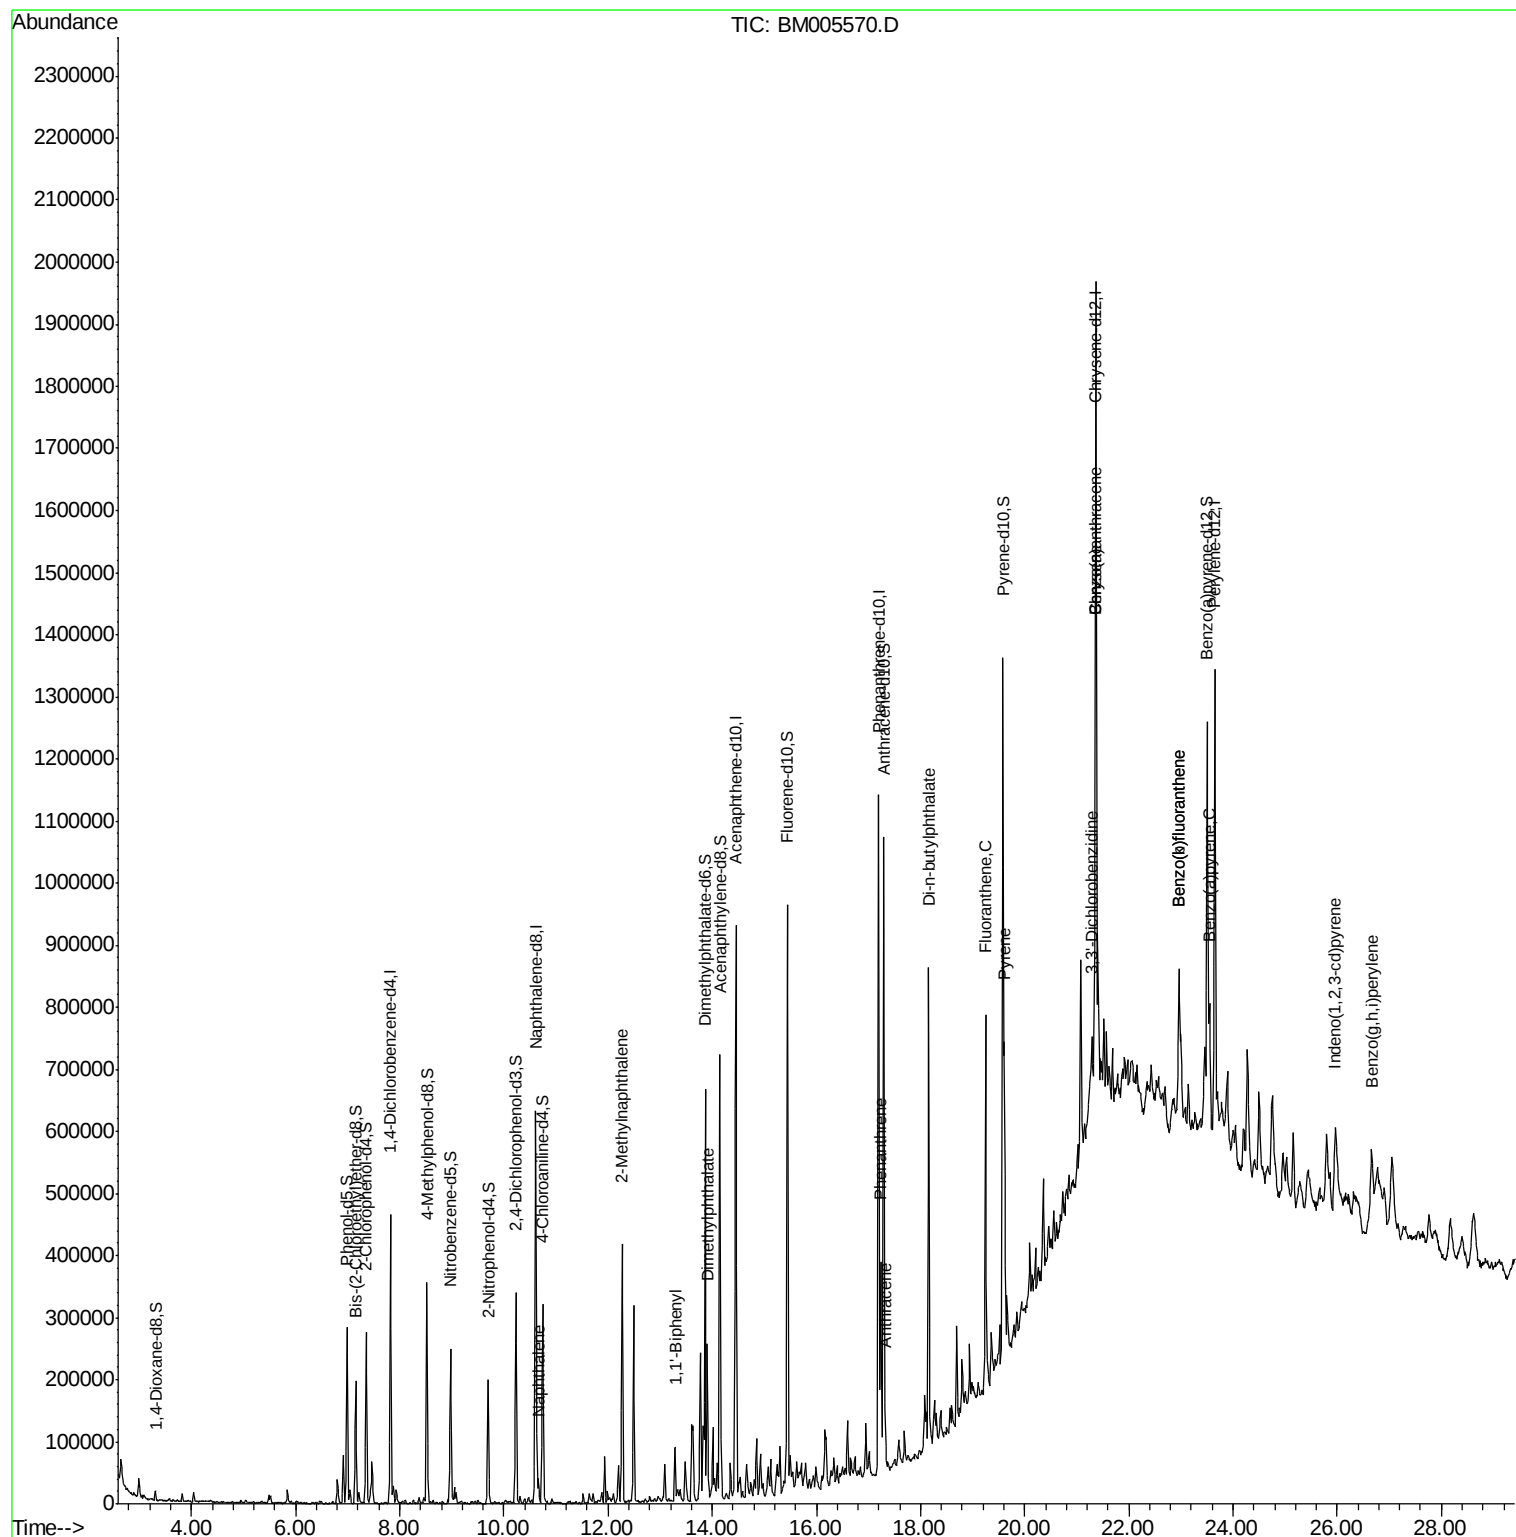

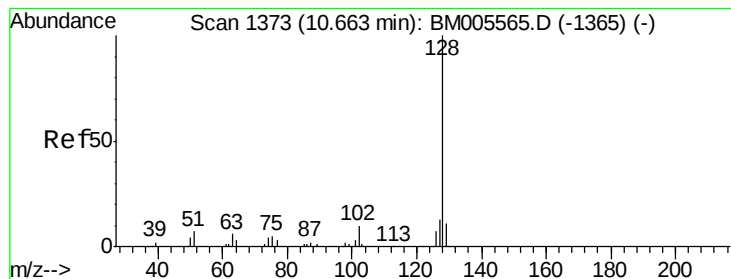

#28

Naphthalene

Concen: 1.18 ng/ul

RT: 10.66 min Scan# 1373

Delta R.T. -0.00 min

Lab File: BM005570.D

Acq: 22 May 2016 03:01

Instrument :

BNA_M

ClientSampleId :

D9WY6


Tgt Ion:128 Resp: 31891

Ion Ratio Lower Upper

128 100

129 12.4 8.6 13.0




127 13.8 10.6 15.8



Abundance Ion 128.00 (127.70 to 128.70): E

Ion 129.00 (128.70 to 129.70): E

Ion 127.00 (126.70 to 127.70): E

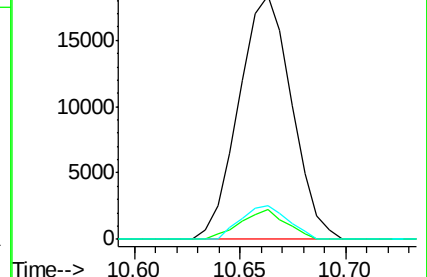

#34

2-Methylnaphthalene

Concen: 10.22 ng/ul

RT: 12.27 min Scan# 1647

Delta R.T. 0.01 min

Lab File: BM005570.D


Acq: 22 May 2016 03:01

Tgt Ion:142 Resp: 202124

Ion Ratio Lower Upper



142 100


141 87.2 70.6 106.0



Abundance Ion 142.00 (141.70 to 142.70): E

Ion 141.00 (140.70 to 141.70): E



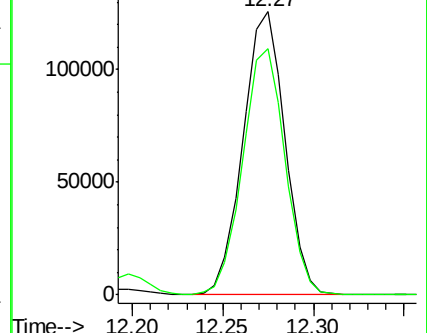



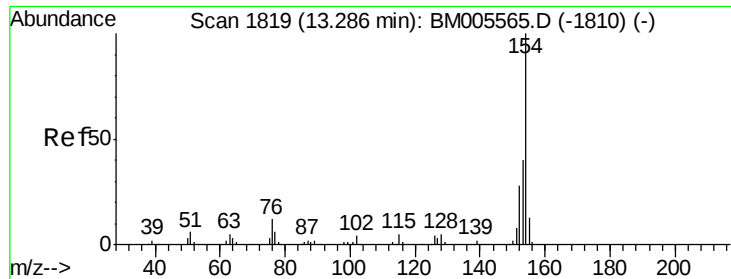

#40
 1,1'-Biphenyl
 Concen: 1.42 ng/ul
 RT: 13.29 min Scan# 1819
 Delta R.T. -0.00 min
 Lab File: BM005570.D
 Acq: 22 May 2016 03:01




Instrument :
 BNA_M
 ClientSampleId :
 D9WY6


Tgt Ion:154 Resp: 36514
 Ion Ratio Lower Upper
 154 100
 153 39.9 31.7 47.5
 76 13.6 10.1 15.1

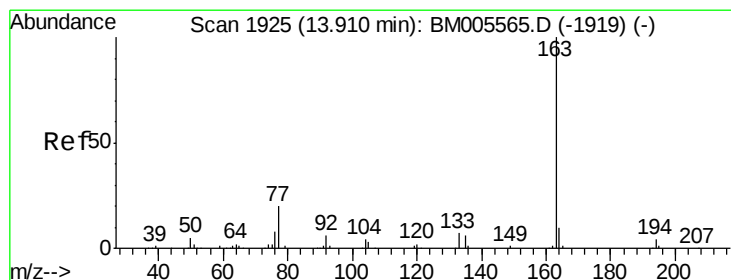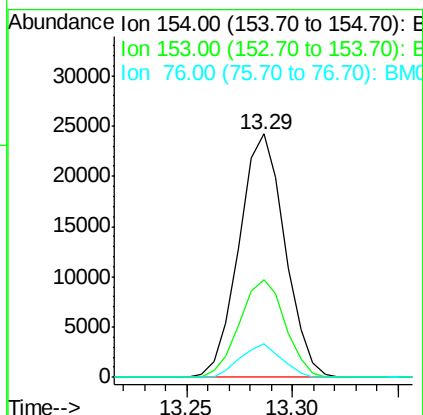

#44
 Dimethylphthalate
 Concen: 6.28 ng/ul
 RT: 13.91 min Scan# 1925
 Delta R.T. -0.00 min
 Lab File: BM005570.D
 Acq: 22 May 2016 03:01

Tgt Ion:163 Resp: 155664
 Ion Ratio Lower Upper
 163 100
 194 4.2 3.4 5.0
 164 10.3 8.0 12.0

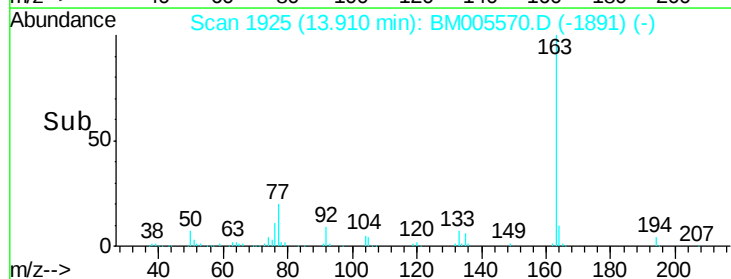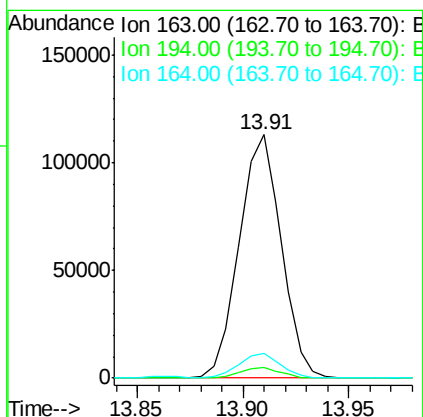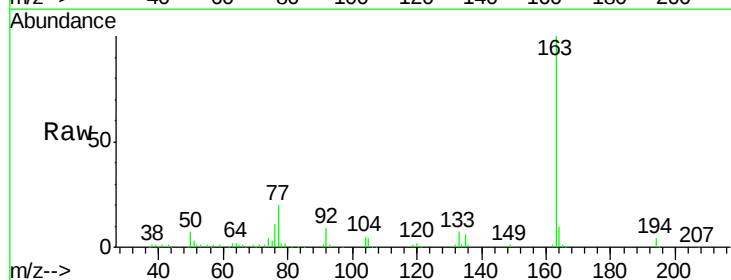







#69
Phenanthrene
Concen: 5.56 ng/ul
RT: 17.24 min Scan# 2491
Delta R.T. 0.01 min
Lab File: BM005570.D
Acq: 22 May 2016 03:01

Instrument :
BNA_M
ClientSampleId :
D9WY6

Tgt Ion:178 Resp: 205429
Ion Ratio Lower Upper
178 100
179 15.5 12.2 18.2
176 19.0 15.8 23.6

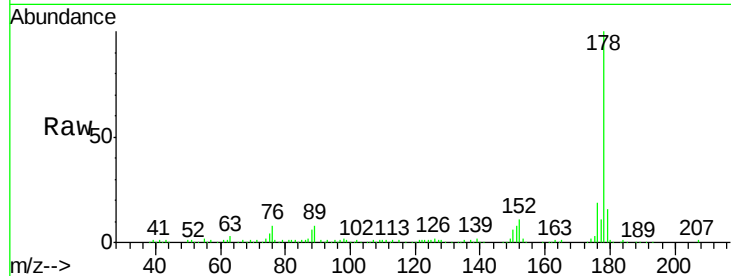


Abundance Ion 178.00 (177.70 to 178.70): E
Ion 179.00 (178.70 to 179.70): E
Ion 176.00 (175.70 to 176.70): E


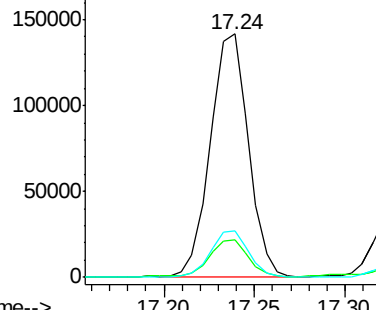



#71
Anthracene
Concen: 1.42 ng/ul
RT: 17.33 min Scan# 2506
Delta R.T. -0.00 min
Lab File: BM005570.D
Acq: 22 May 2016 03:01

Tgt Ion:178 Resp: 53370
Ion Ratio Lower Upper
178 100
179 16.8 12.6 18.8
176 18.5 15.0 22.4



Abundance Ion 178.00 (177.70 to 178.70): E
Ion 179.00 (178.70 to 179.70): E
Ion 176.00 (175.70 to 176.70): E

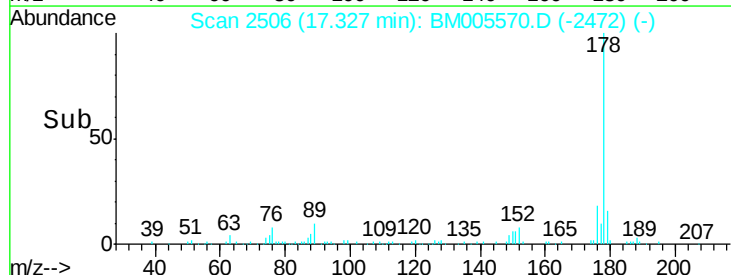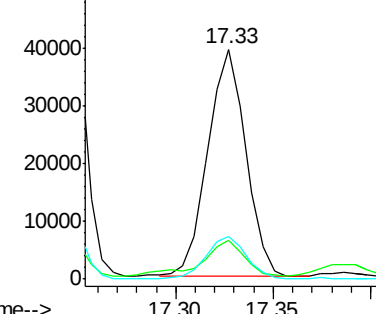

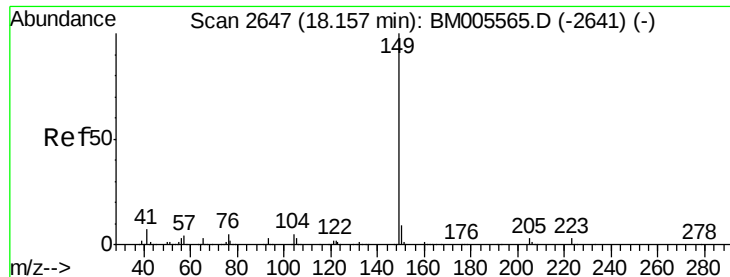

#73

Di-n-butylphthalate

Concen: 14.52 ng/ul

RT: 18.16 min Scan# 2648

Delta R.T. 0.01 min

Lab File: BM005570.D

Acq: 22 May 2016 03:01

Instrument :

BNA_M

ClientSampleId :

D9WY6


Tgt Ion:149 Resp: 575766

Ion Ratio Lower Upper

149 100

150 9.0 7.4 11.0




104 5.5 4.4 6.6

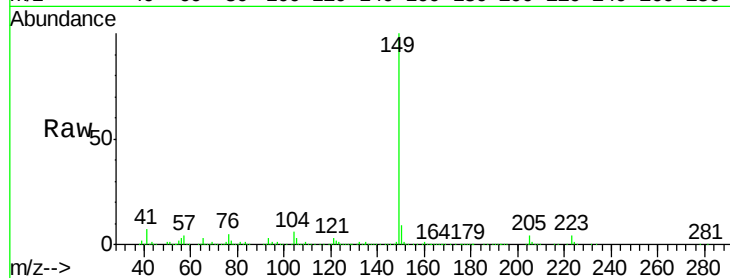

Abundance Ion 149.00 (148.70 to 149.70): E

Ion 150.00 (149.70 to 150.70): E

Ion 104.00 (103.70 to 104.70): E

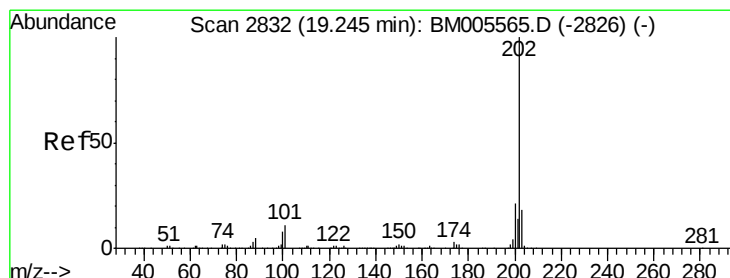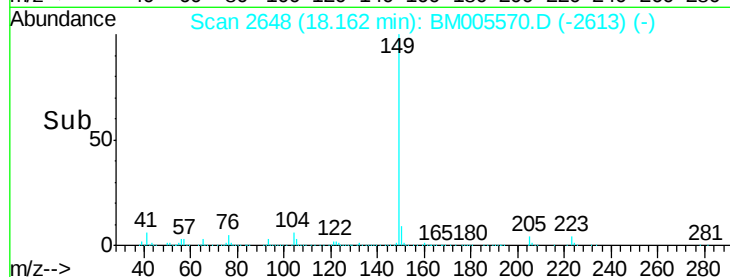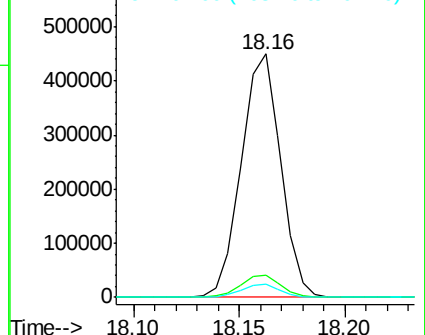

#74

Fluoranthene

Concen: 9.08 ng/ul

RT: 19.25 min Scan# 2833

Delta R.T. 0.01 min

Lab File: BM005570.D

Acq: 22 May 2016 03:01


Tgt Ion:202 Resp: 377675

Ion Ratio Lower Upper

202 100

101 9.2 7.9 11.9



100 7.3 5.6 8.4

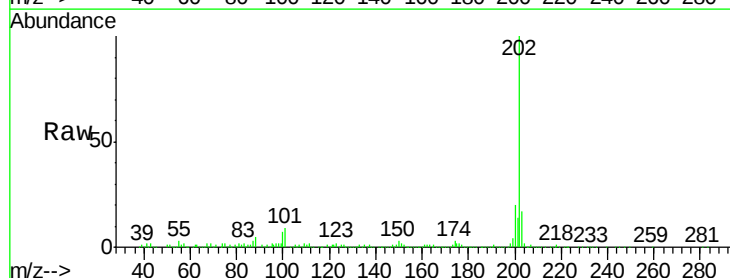


Abundance Ion 202.00 (201.70 to 202.70): E

Ion 101.00 (100.70 to 101.70): E

Ion 100.00 (99.70 to 100.70): B



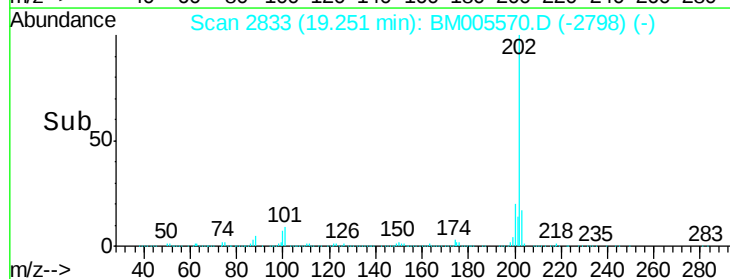
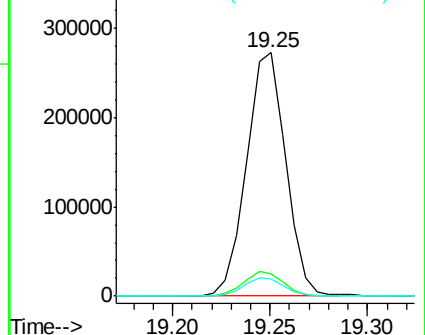


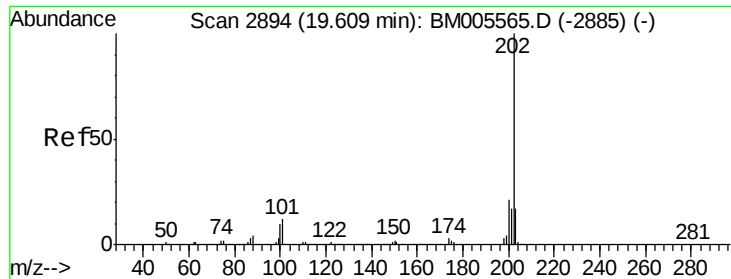

#77
 Pyrene
 Concen: 9.02 ng/ul
 RT: 19.61 min Scan# 2894
 Delta R.T. -0.00 min
 Lab File: BM005570.D
 Acq: 22 May 2016 03:01




Instrument :
 BNA_M
 ClientSampleId :
 D9WY6


Tgt Ion:	202	Resp:	305150
Ion	Ratio	Lower	Upper
202	100		
101	12.4	9.6	14.4
100	9.9	7.8	11.6

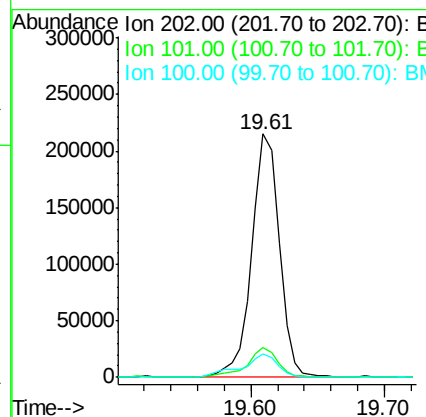

#79
 3,3'-Dichlorobenzidine
 Concen: 1.07 ng/ul
 RT: 21.29 min Scan# 3180
 Delta R.T. 0.01 min
 Lab File: BM005570.D
 Acq: 22 May 2016 03:01

Tgt Ion:	252	Resp:	11406
Ion	Ratio	Lower	Upper
252	100		
254	66.3	51.7	77.5
126	24.7	7.9	11.9#

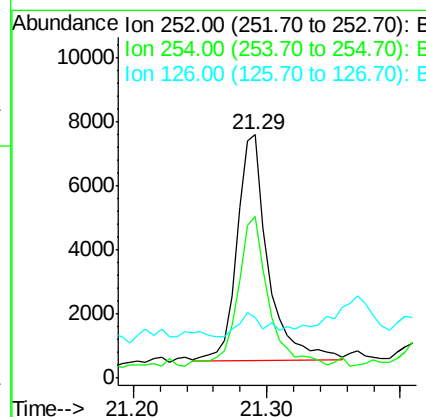

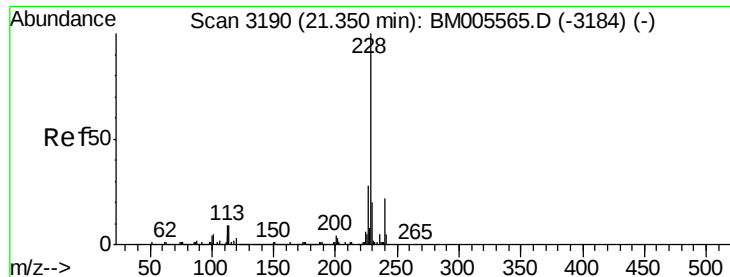

#80

Benzo(a)anthracene

Concen: 4.59 ng/ul

RT: 21.35 min Scan# 3190

Delta R.T. -0.00 min

Lab File: BM005570.D

Acq: 22 May 2016 03:01

Instrument :

BNA_M

ClientSampled :

D9WY6


Tgt Ion:228 Resp: 158914

Ion Ratio Lower Upper

228 100

229 21.2 15.4 23.2




226 27.1 21.0 31.4

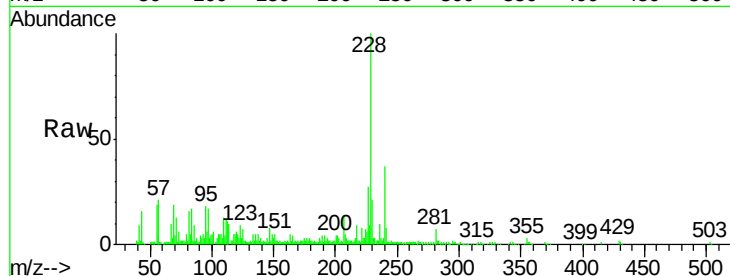

Abundance Ion 228.00 (227.70 to 228.70): E

Ion 229.00 (228.70 to 229.70): E

Ion 226.00 (225.70 to 226.70): E

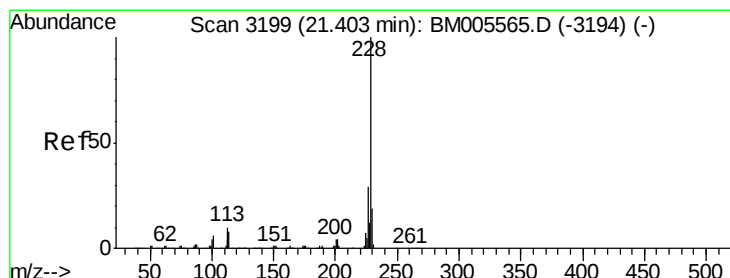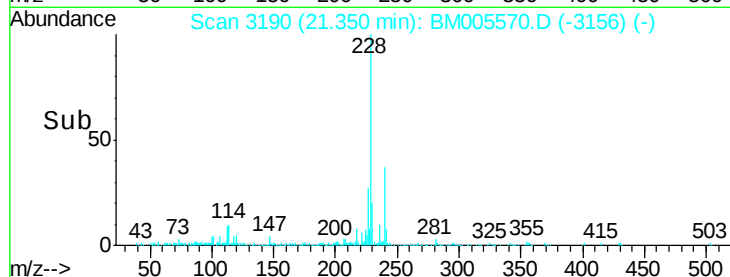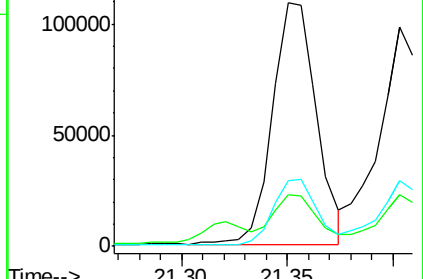

#82

Chrysene

Concen: 4.83 ng/ul

RT: 21.35 min Scan# 3190

Delta R.T. -0.05 min

Lab File: BM005570.D

Acq: 22 May 2016 03:01


Tgt Ion:228 Resp: 158914

Ion Ratio Lower Upper

228 100

226 27.1 23.7 35.5



229 21.2 15.5 23.3

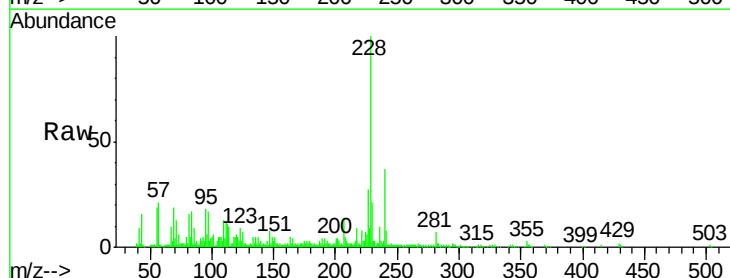


Abundance Ion 228.00 (227.70 to 228.70): E

Ion 226.00 (225.70 to 226.70): E

Ion 229.00 (228.70 to 229.70): E



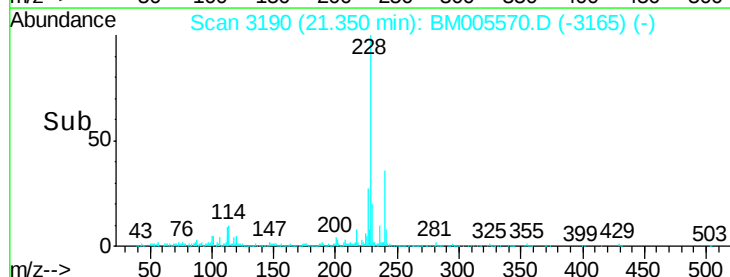
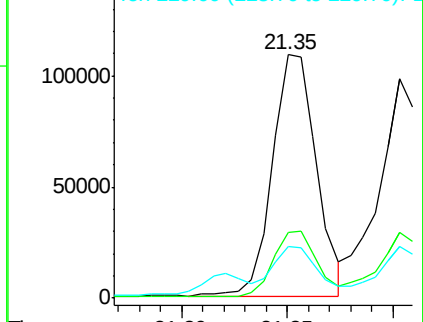




#85
Benzo(b)fluoranthene
Concen: 5.49 ng/ul
RT: 22.96 min Scan# 3464
Delta R.T. 0.01 min
Lab File: BM005570.D
Acq: 22 May 2016 03:01




Instrument :
BNA_M
ClientSampleId :
D9WY6


Tgt Ion	Ratio	Lower	Upper
252	100		
253	23.8	17.3	25.9
125	16.5	7.0	10.4

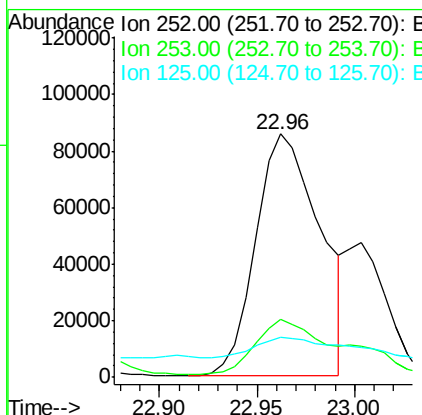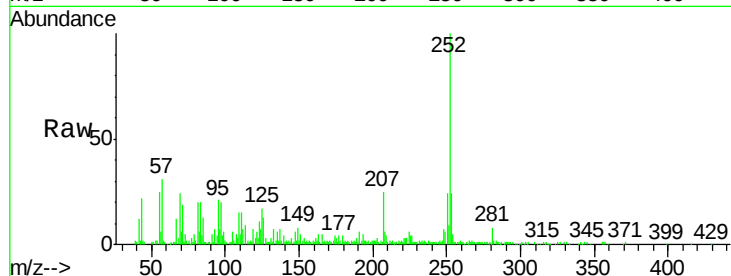

#86
Benzo(k)fluoranthene
Concen: 5.80 ng/ul
RT: 22.96 min Scan# 3464
Delta R.T. -0.04 min
Lab File: BM005570.D
Acq: 22 May 2016 03:01

Tgt Ion	Ratio	Lower	Upper
252	100		
253	23.8	17.5	26.3
125	16.5	7.0	10.6

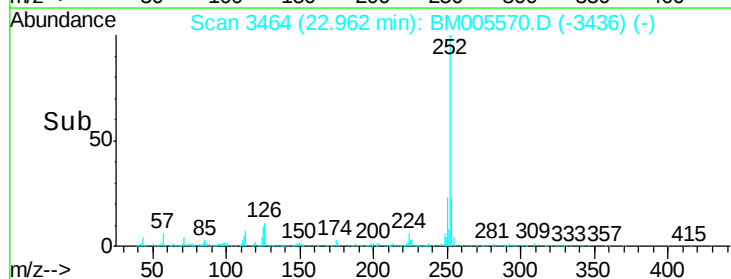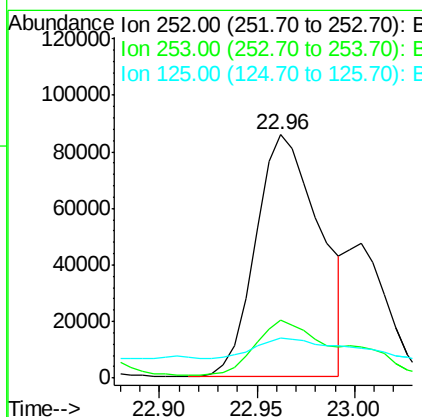

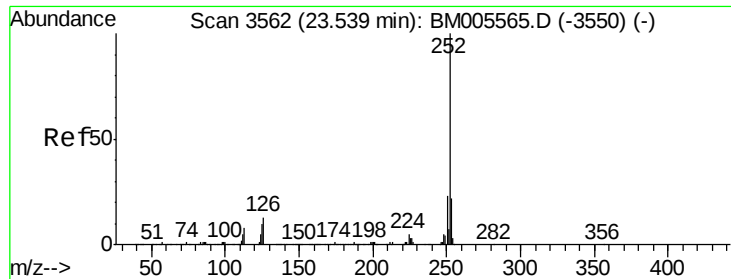

#88

Benzo(a)pyrene

Concen: 4.14 ng/ul

RT: 23.55 min Scan# 3564

Delta R.T. 0.01 min

Lab File: BM005570.D

Acq: 22 May 2016 03:01

Instrument :

BNA_M

ClientSampleId :

D9WY6


Tgt Ion:252 Resp: 142250

Ion Ratio Lower Upper

252 100

253 24.6 17.6 26.4




125 17.5 7.6 11.4#



Abundance Ion 252.00 (251.70 to 252.70): E

Ion 253.00 (252.70 to 253.70): E

Ion 125.00 (124.70 to 125.70): E

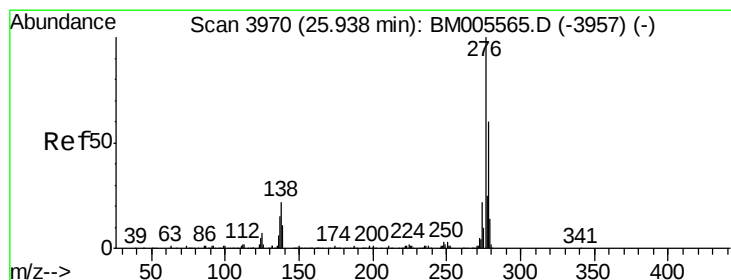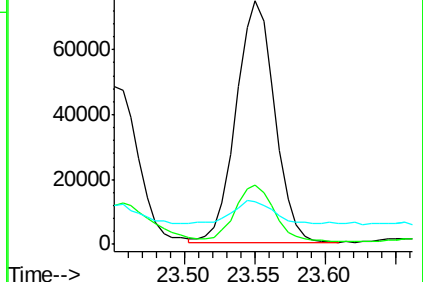

#89

Indeno(1,2,3-cd)pyrene

Concen: 2.39 ng/ul

RT: 25.96 min Scan# 3973

Delta R.T. 0.02 min

Lab File: BM005570.D

Acq: 22 May 2016 03:01


Tgt Ion:276 Resp: 97359

Ion Ratio Lower Upper

276 100

138 21.1 16.9 25.3



277 25.8 20.2 30.4




Abundance Ion 276.00 (275.70 to 276.70): E

Ion 138.00 (137.70 to 138.70): E

Ion 277.00 (276.70 to 277.70): E

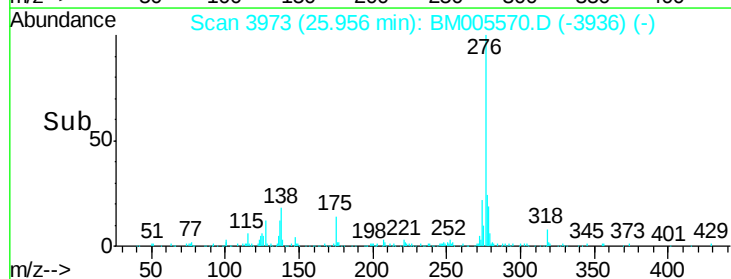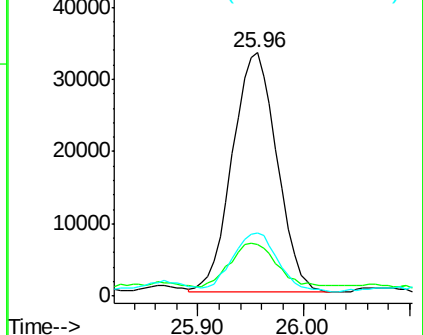

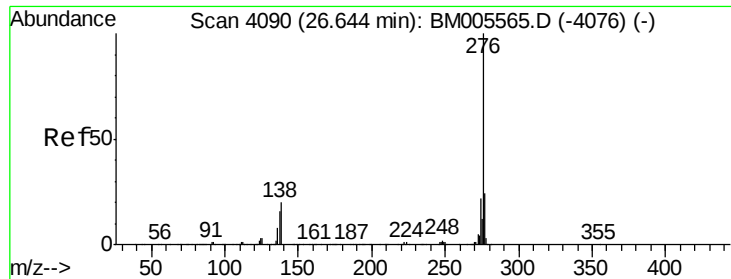

#91

Benzo(g,h,i)perylene

Concen: 2.62 ng/ul

RT: 26.66 min Scan# 4093

Delta R.T. 0.02 min

Lab File: BM005570.D

Acq: 22 May 2016 03:01

Instrument :

BNA_M

ClientSampleId :

D9WY6


Tgt Ion: 276 Resp: 89912

Ion Ratio Lower Upper

276 100

138 21.1 15.0 22.6

277 26.3 18.6 28.0



Abundance Ion 276.00 (275.70 to 276.70): E

Ion 138.00 (137.70 to 138.70): E

Ion 277.00 (276.70 to 277.70): E

