

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM052116\
 Data File : BM005563.D
 Acq On : 21 May 2016 22:47
 Operator : UM/SJ
 Sample : H3086-15
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 JHGJ9

Quant Time: May 22 05:10:31 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM052016.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sun May 22 05:09:34 2016
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.82	152	73016	20.00	ng/ul	0.00
18) Naphthalene-d8	10.61	136	300207	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.45	164	173515	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.19	188	406077	20.00	ng/ul	0.00
75) Chrysene-d12	21.36	240	516721	20.00	ng/ul	0.00
83) Perylene-d12	23.64	264	538509	20.00	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.31	96	5151	3.09	ng/uL	0.00
5) Phenol-d5	6.98	99	104519	17.46	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.15	67	62119	17.91	ng/ul	0.00
9) 2-Chlorophenol-d4	7.35	132	86835	17.39	ng/ul	0.00
13) 4-Methylphenol-d8	8.52	113	83968	17.12	ng/ul	0.00
19) Nitrobenzene-d5	8.97	128	39827	17.35	ng/ul	0.00
22) 2-Nitrophenol-d4	9.69	143	43367	17.16	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.23	165	80713	16.96	ng/ul	0.00
29) 4-Chloroaniline-d4	10.74	131	110394	23.16	ng/ul	0.00
43) Dimethylphthalate-d6	13.86	166	263894	18.63	ng/ul	0.00
46) Acenaphthylene-d8	14.15	160	326036	18.41	ng/ul	0.00
51) 4-Nitrophenol-d4	14.64	143	43252	16.14	ng/ul	0.00
57) Fluorene-d10	15.44	176	236799	19.21	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.56	200	32133	13.76	ng/ul	0.00
70) Anthracene-d10	17.29	188	366095	18.93	ng/ul	0.00
76) Pyrene-d10	19.58	212	453854	19.40	ng/ul	0.00
87) Benzo(a)pyrene-d12	23.50	264	492958	19.60	ng/ul	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
44) Dimethylphthalate	13.90	163	46171	3.30	ng/ul	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM052116\
Data File : BM005563.D
Acq On : 21 May 2016 22:47
Operator : UM/SJ
Sample : H3086-15
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
JHGJ9

Quant Time: May 22 05:10:31 2016
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM052016.M
Quant Title : SVOA CALIBRATION
QLast Update : Sun May 22 05:09:34 2016
Response via : Initial Calibration

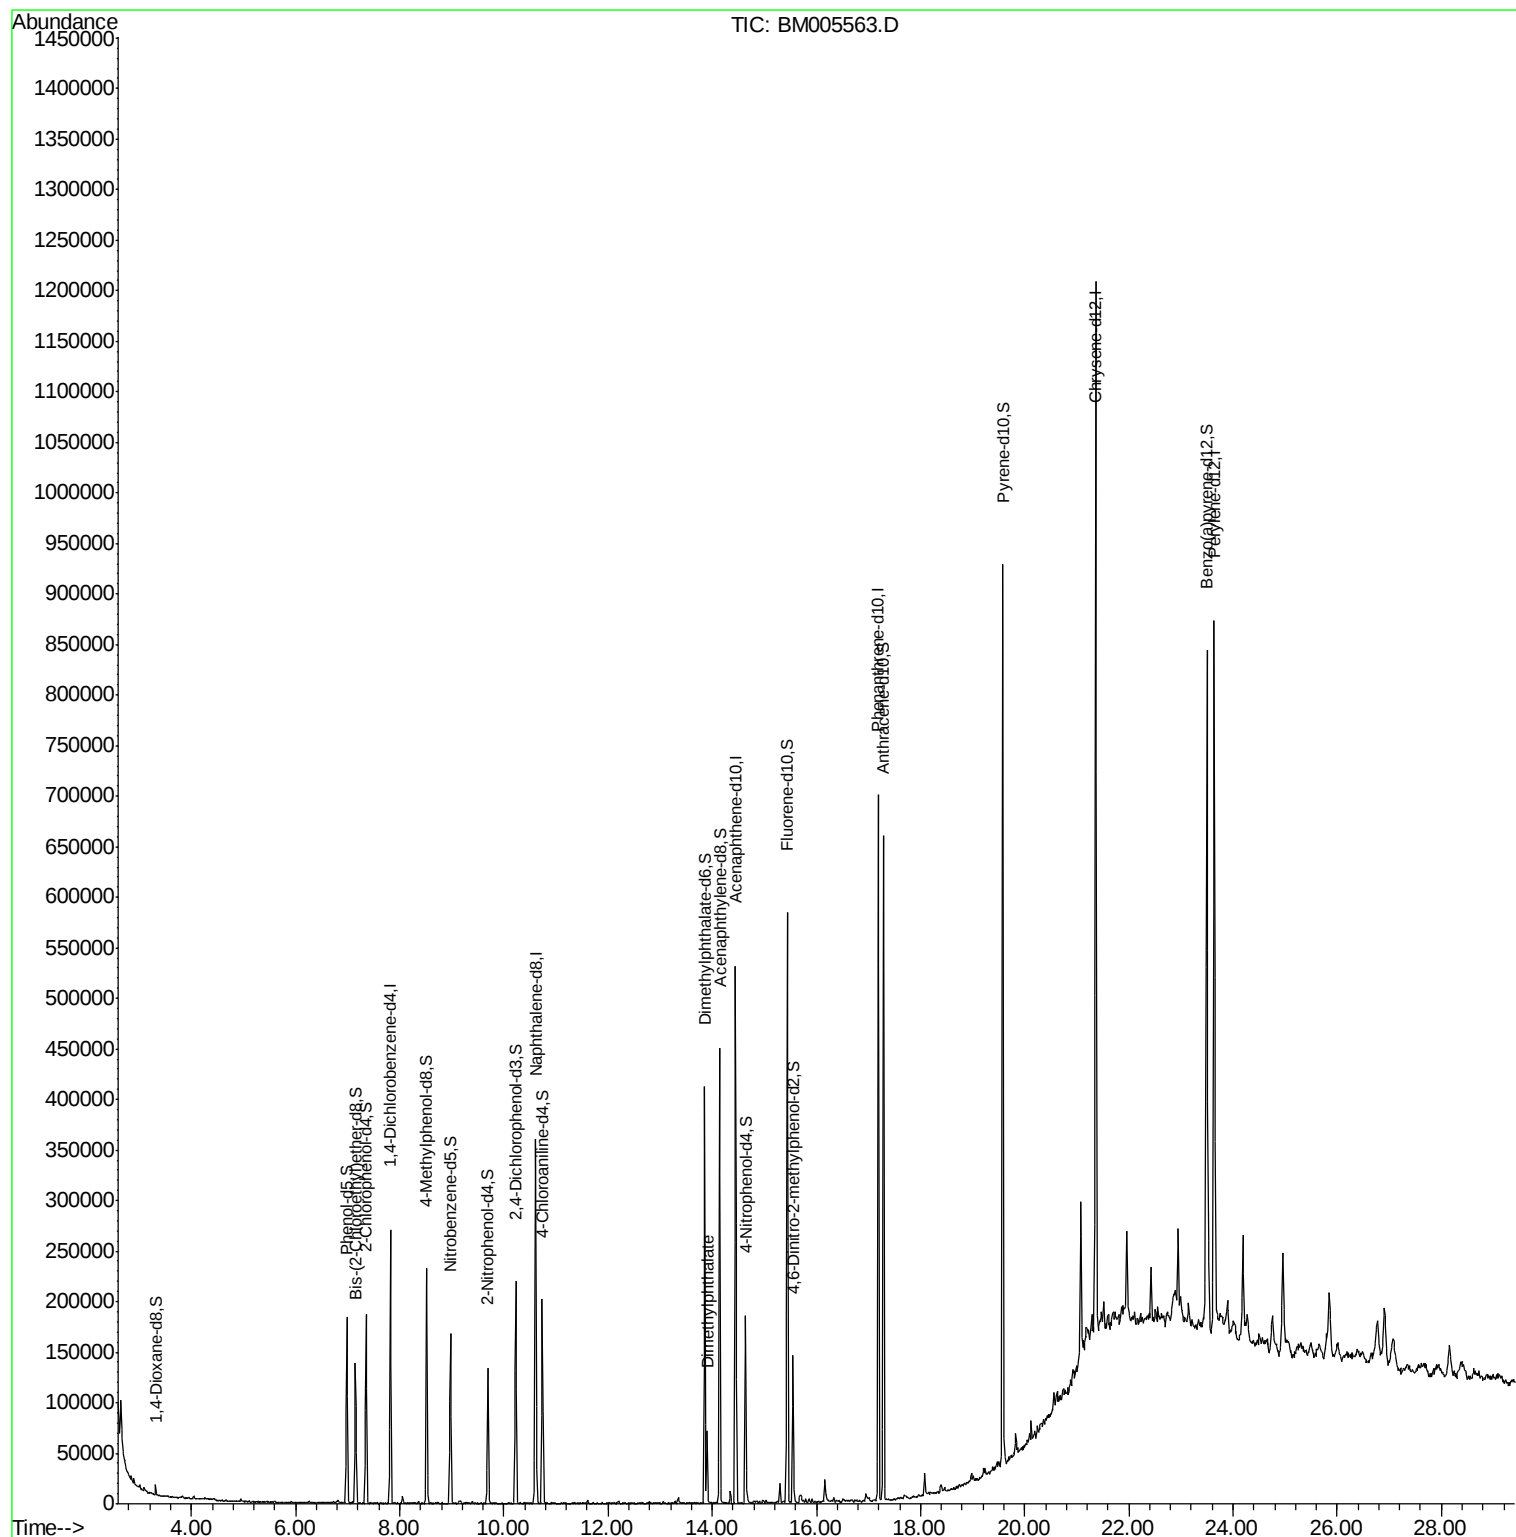


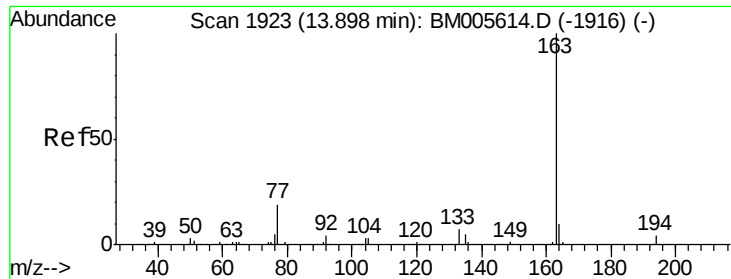

#44
 Dimethylphthalate
 Concen: 3.30 ng/ul
 RT: 13.90 min Scan# 1924
 Delta R.T. -0.01 min
 Lab File: BM005563.D
 Acq: 21 May 2016 22:47

Instrument :
 BNA_M
 ClientSampleId :
 JHGJ9

Tgt Ion:163 Resp: 46171
 Ion Ratio Lower Upper
 163 100
 194 4.8 3.4 5.0
 164 9.6 8.0 12.0

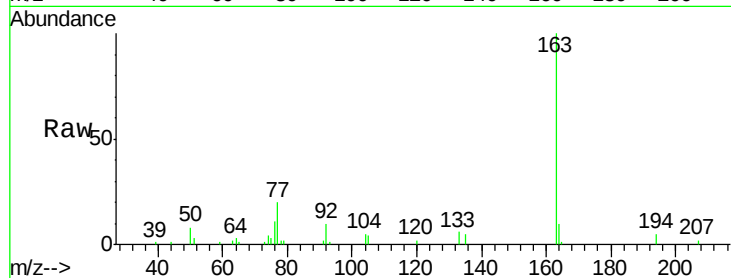

Abundance Ion 163.00 (162.70 to 163.70): E
 Ion 194.00 (193.70 to 194.70): E
 Ion 164.00 (163.70 to 164.70): E

