

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM052116\
 Data File : BM005573.D
 Acq On : 22 May 2016 04:50
 Operator : UM/SJ
 Sample : H2841-15
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 D9WT0

Quant Time: May 22 05:35:23 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM052016.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sun May 22 05:33:20 2016
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.82	152	155940	20.00	ng/ul	0.00
18) Naphthalene-d8	10.62	136	650853	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.46	164	355771	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.20	188	772973	20.00	ng/ul	0.00
75) Chrysene-d12	21.37	240	853021	20.00	ng/ul	0.00
83) Perylene-d12	23.66	264	872564	20.00	ng/ul	0.02

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.31	96	8757	2.46	ng/uL	0.00
5) Phenol-d5	6.99	99	195762	15.32	ng/ul	0.01
7) Bis-(2-Chloroethyl)ether-d	7.16	67	113702	15.35	ng/ul	0.00
9) 2-Chlorophenol-d4	7.36	132	160265	15.03	ng/ul	0.00
13) 4-Methylphenol-d8	8.53	113	154378	14.74	ng/ul	0.00
19) Nitrobenzene-d5	8.98	128	76236	15.32	ng/ul	0.00
22) 2-Nitrophenol-d4	9.70	143	86688	15.83	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.23	165	154906	15.02	ng/ul	0.00
29) 4-Chloroaniline-d4	10.75	131	141997	13.74	ng/ul	0.00
43) Dimethylphthalate-d6	13.86	166	455542	15.69	ng/ul	0.00
46) Acenaphthylene-d8	14.15	160	573876	15.81	ng/ul	0.00
51) 4-Nitrophenol-d4	14.65	143	81308	14.80	ng/ul	0.00
57) Fluorene-d10	15.44	176	394407	15.61	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.56	200	62527	14.06	ng/ul	0.00
70) Anthracene-d10	17.29	188	594810	16.15	ng/ul	0.00
76) Pyrene-d10	19.59	212	697268	18.05	ng/ul	0.00
87) Benzo(a)pyrene-d12	23.51	264	678211	16.65	ng/ul	0.01


Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
44) Dimethylphthalate	13.91	163	108766	3.79	ng/ul	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM052116\
Data File : BM005573.D
Acq On : 22 May 2016 04:50
Operator : UM/SJ
Sample : H2841-15
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
D9WT0

Quant Time: May 22 05:35:23 2016
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM052016.M
Quant Title : SVOA CALIBRATION
QLast Update : Sun May 22 05:33:20 2016
Response via : Initial Calibration

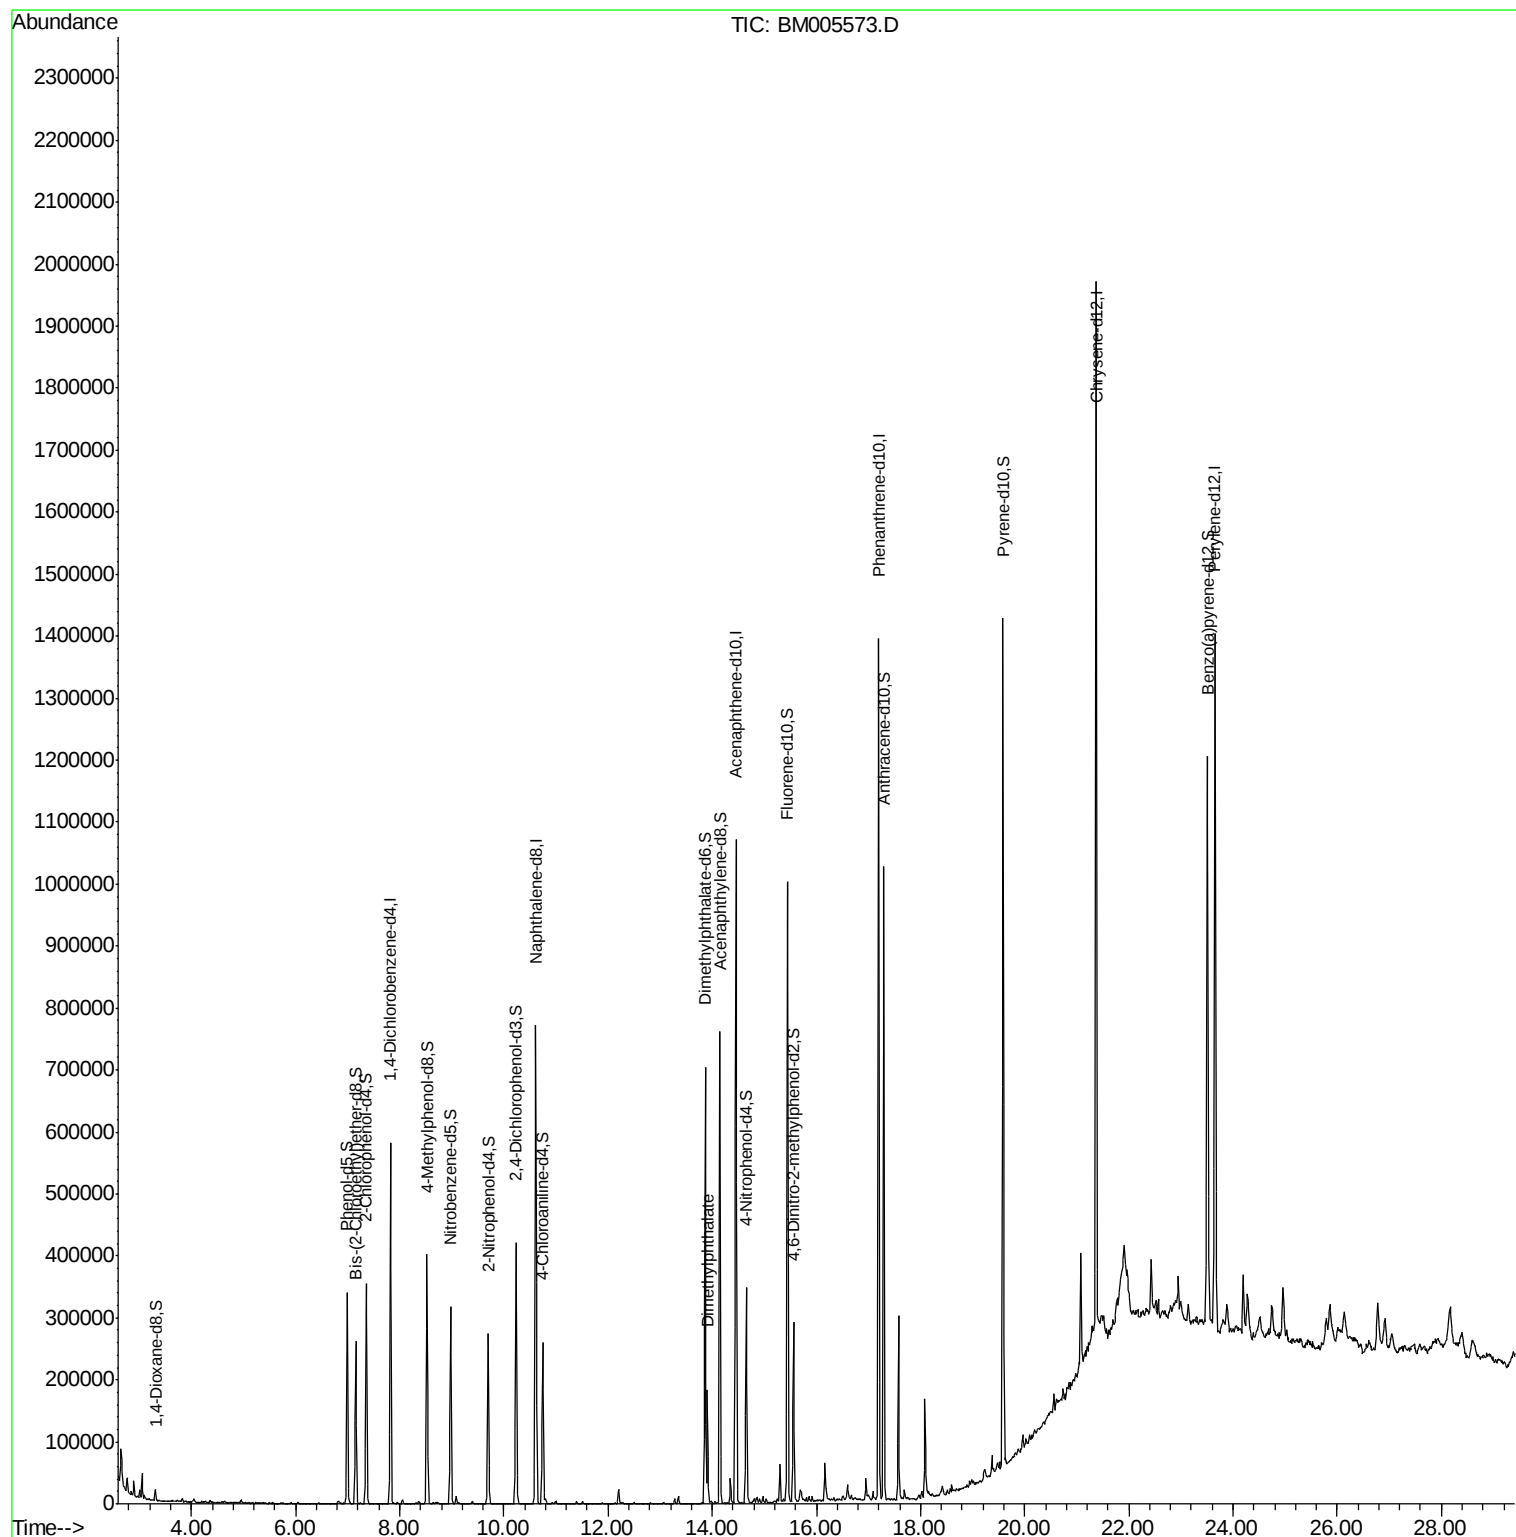

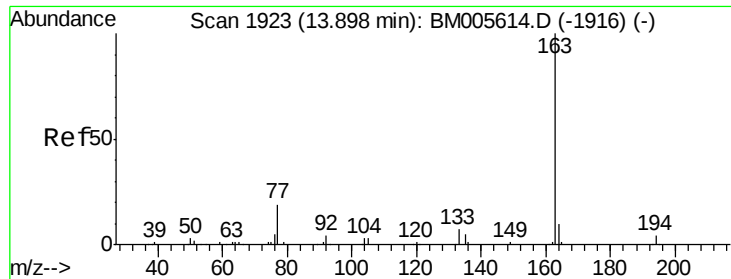

#44
 Dimethylphthalate
 Concen: 3.79 ng/ul
 RT: 13.91 min Scan# 1925
 Delta R.T. -0.00 min
 Lab File: BM005573.D
 Acq: 22 May 2016 04:50

Instrument :
 BNA_M
 ClientSampleId :
 D9WT0

Tgt Ion	Resp	Lower	Upper
163	108766		
194	4.2	3.4	5.0
164	10.5	8.0	12.0

