

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM052120\
 Data File : BM026050.D
 Acq On : 21 May 2020 10:23
 Operator : MA/SJ
 Sample : PB129023BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK23

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM051320MA.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.069	28	31	42	rVB	58332	90565	2.34%	0.211%
2	3.610	119	123	130	rBV	32041	44667	1.16%	0.104%
3	3.775	147	151	157	rBV3	12857	15173	0.39%	0.035%
4	6.687	639	646	656	rVV	936139	1437446	37.21%	3.346%
5	6.845	667	673	684	rBV	668946	1017738	26.34%	2.369%
6	7.039	699	706	715	rBV	897688	1398717	36.21%	3.256%
7	7.498	777	784	793	rBV	622515	951243	24.62%	2.214%
8	8.210	898	905	915	rBV	1068806	1613294	41.76%	3.756%
9	8.639	970	978	991	rBV	806988	1264669	32.74%	2.944%
10	9.357	1093	1100	1110	rBV	624721	988176	25.58%	2.300%
11	9.892	1183	1191	1201	rBV	975756	1562474	40.44%	3.637%
12	10.257	1245	1253	1264	rBV	833861	1370252	35.47%	3.190%
13	10.404	1269	1278	1291	rBV	945891	1591217	41.19%	3.704%
14	11.604	1478	1482	1486	rVB6	3401	6012	0.16%	0.014%
15	11.821	1513	1519	1520	rBV4	3098	3920	0.10%	0.009%
16	11.863	1523	1526	1532	rVB3	11428	17258	0.45%	0.040%
17	13.563	1809	1815	1823	rBV	1566196	2071061	53.61%	4.821%
18	13.627	1823	1826	1830	rVB2	11102	13340	0.35%	0.031%
19	13.827	1853	1860	1869	rBV	1677736	2423941	62.74%	5.643%
20	14.139	1907	1913	1925	rBV	1226236	1750928	45.32%	4.076%
21	14.357	1944	1950	1967	rBV	764102	1088047	28.16%	2.533%
22	14.504	1973	1975	1983	rVB9	3404	6389	0.17%	0.015%
23	14.633	1994	1997	2001	rVB3	2664	4050	0.10%	0.009%
24	15.139	2076	2083	2090	rBV	2118158	3003751	77.75%	6.992%
25	15.198	2090	2093	2097	rVV2	12036	14141	0.37%	0.033%
26	15.268	2099	2105	2117	rVV	626663	831077	21.51%	1.935%
27	15.386	2119	2125	2130	rVB	24647	38781	1.00%	0.090%
28	15.927	2213	2217	2223	rBV6	7570	11012	0.29%	0.026%
29	16.445	2302	2305	2308	rBV3	6289	7152	0.19%	0.017%
30	16.680	2340	2345	2351	rVB5	4986	9889	0.26%	0.023%
31	16.892	2373	2381	2391	rBV	1565080	2127484	55.07%	4.952%
32	16.986	2391	2397	2409	rBV2	2334690	3230659	83.63%	7.521%
33	17.515	2481	2487	2491	rBV8	4631	9102	0.24%	0.021%
34	18.927	2723	2727	2731	rVB2	25145	29591	0.77%	0.069%

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM052120\
Data File : BM026050.D
Acq On : 21 May 2020 10:23
Operator : MA/SJ
Sample : PB129023BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK23

Integration Parameters: LSCINT.P

Integrator: RTE
Smoothing : OFF
Sampling : 1
Start Thrs: 0.2
Stop Thrs : 0
Filtering: 5
Min Area: 0.1 % of largest Peak
Max Peaks: 100
Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM051320MA.M
Title : SVOA CALIBRATION

35	19.180	2766	2770	2774	rVB2	21100	27288	0.71%	0.064%
36	19.292	2782	2789	2795	rBV	2957338	3834350	99.25%	8.926%
37	21.086	3089	3094	3102	rBV	2004520	2507894	64.92%	5.838%
38	23.080	3427	3433	3440	rBV	2407418	3863253	100.00%	8.993%
39	23.144	3441	3444	3449	rVV	142353	203309	5.26%	0.473%
40	23.209	3449	3455	3463	rVB2	1413871	2478500	64.16%	5.770%


Sum of corrected areas: 42957810

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM052120\
Data File : BM026050.D
Acq On : 21 May 2020 10:23
Operator : MA/SJ
Sample : PB129023BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK23

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM051320MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

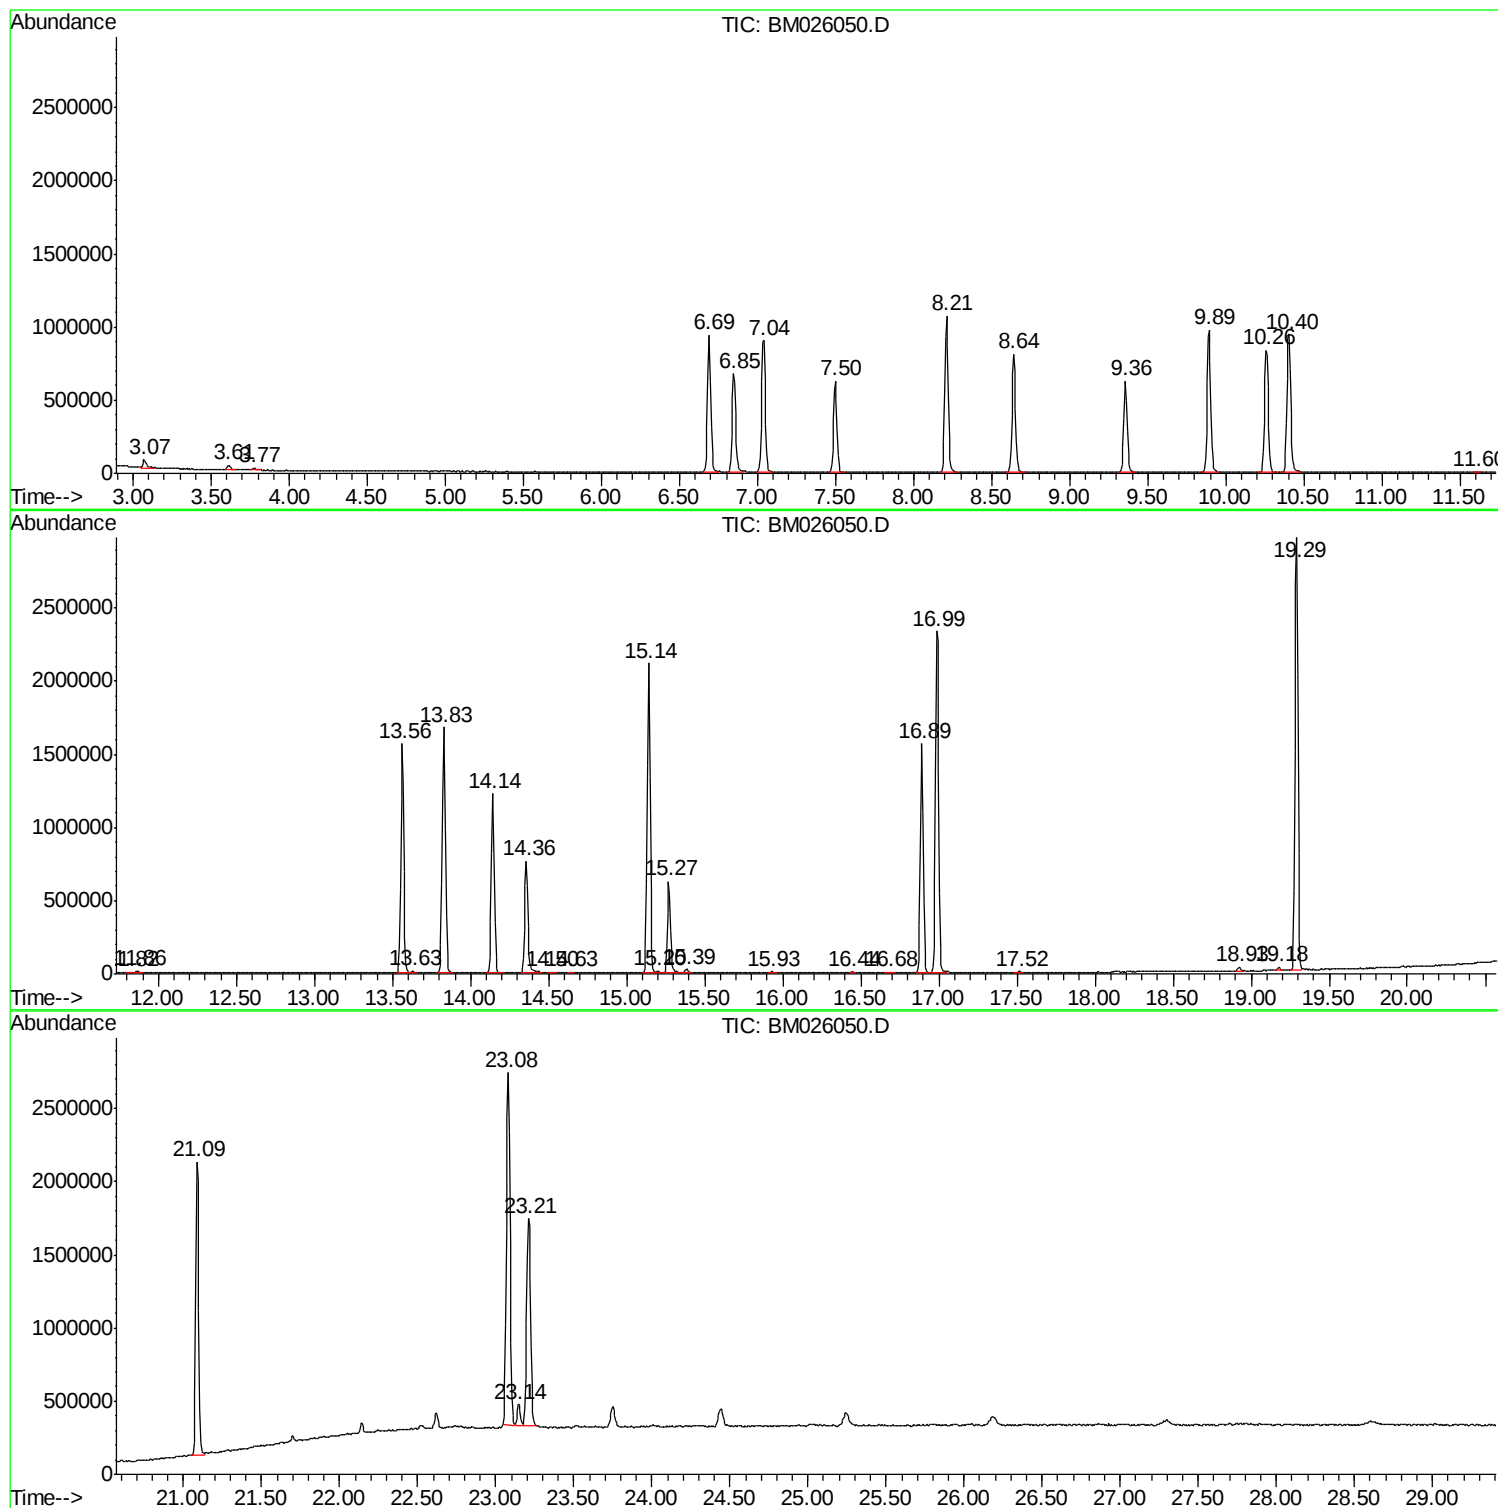

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM052120\
Data File : BM026050.D
Acq On : 21 May 2020 10:23
Operator : MA/SJ
Sample : PB129023BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK23

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM051320MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM052120\
Data File : BM026050.D
Acq On : 21 May 2020 10:23
Operator : MA/SJ
Sample : PB129023BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK23

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM051320MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc