



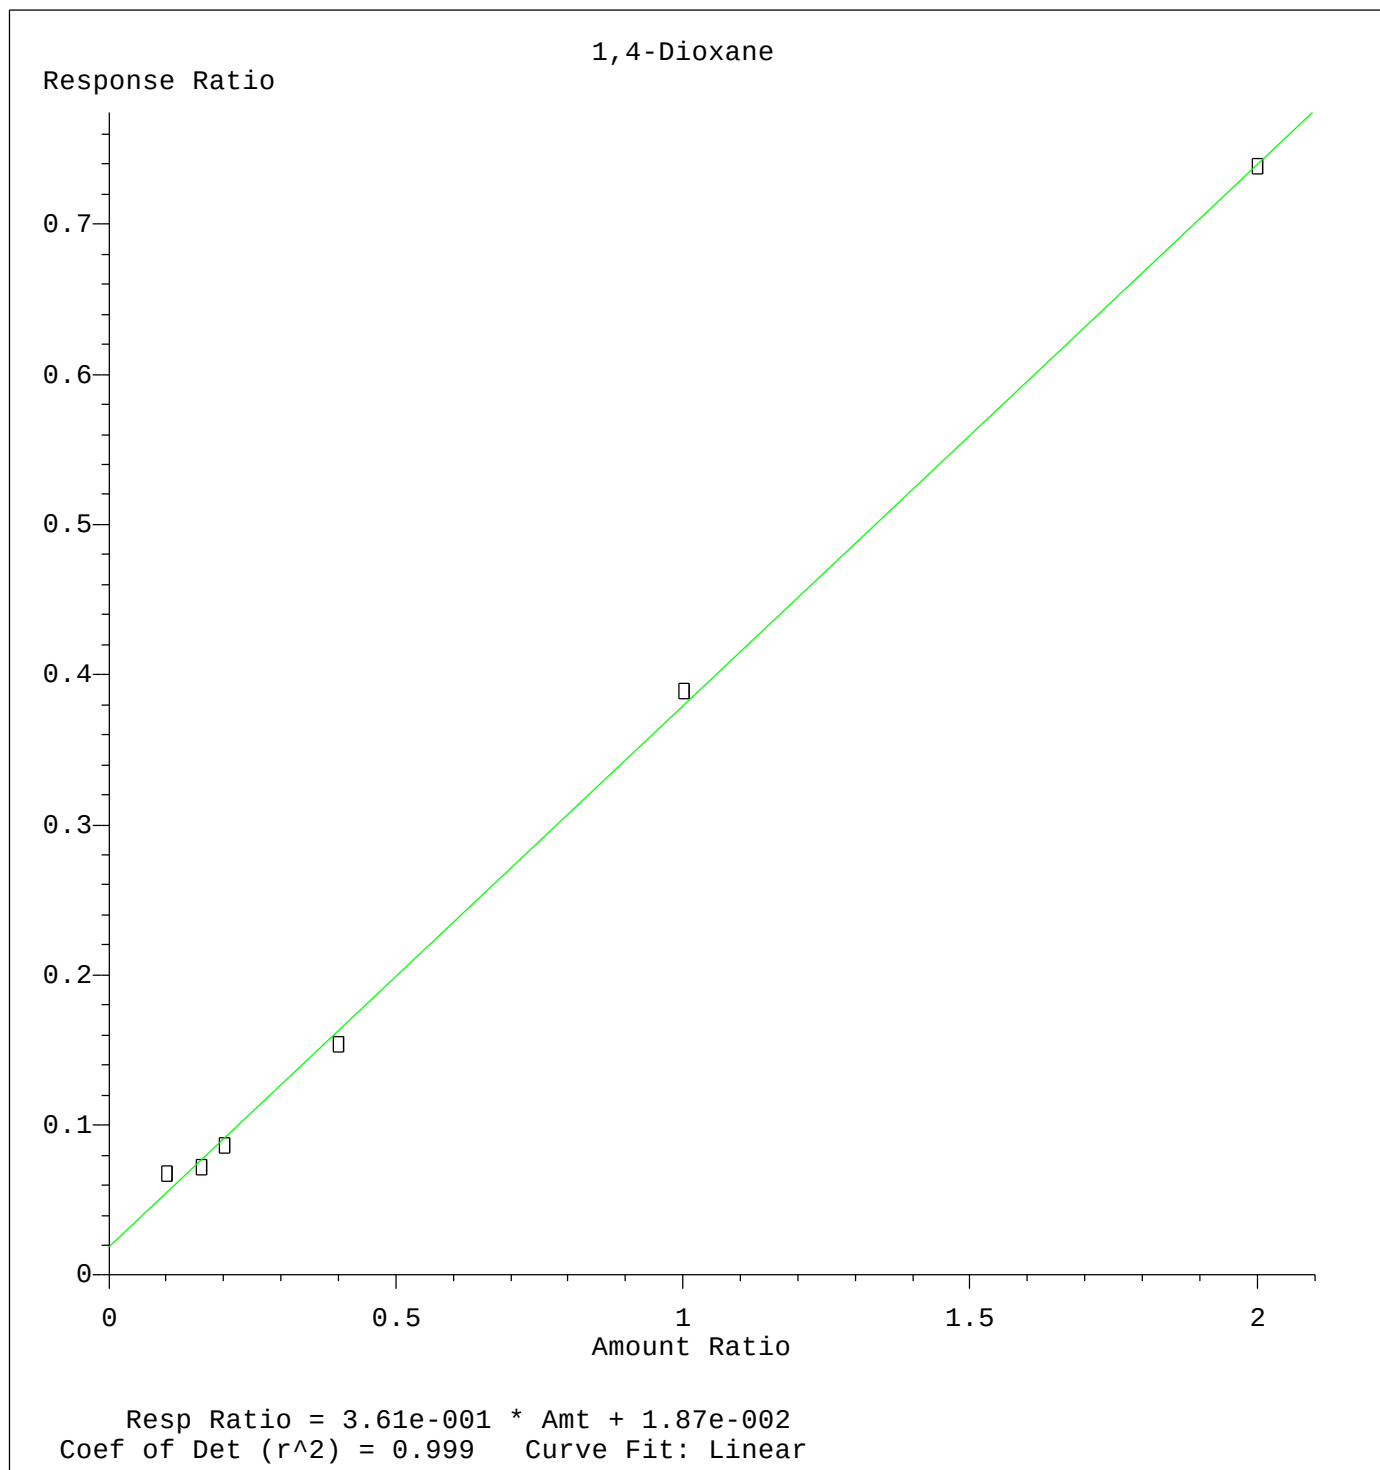


Method Name: Z:\HPCHEM1\BNA_M\METHODS\SIMPAH-BM052215.M
Calibration Table Last Updated: Sat May 23 04:33:49 2015

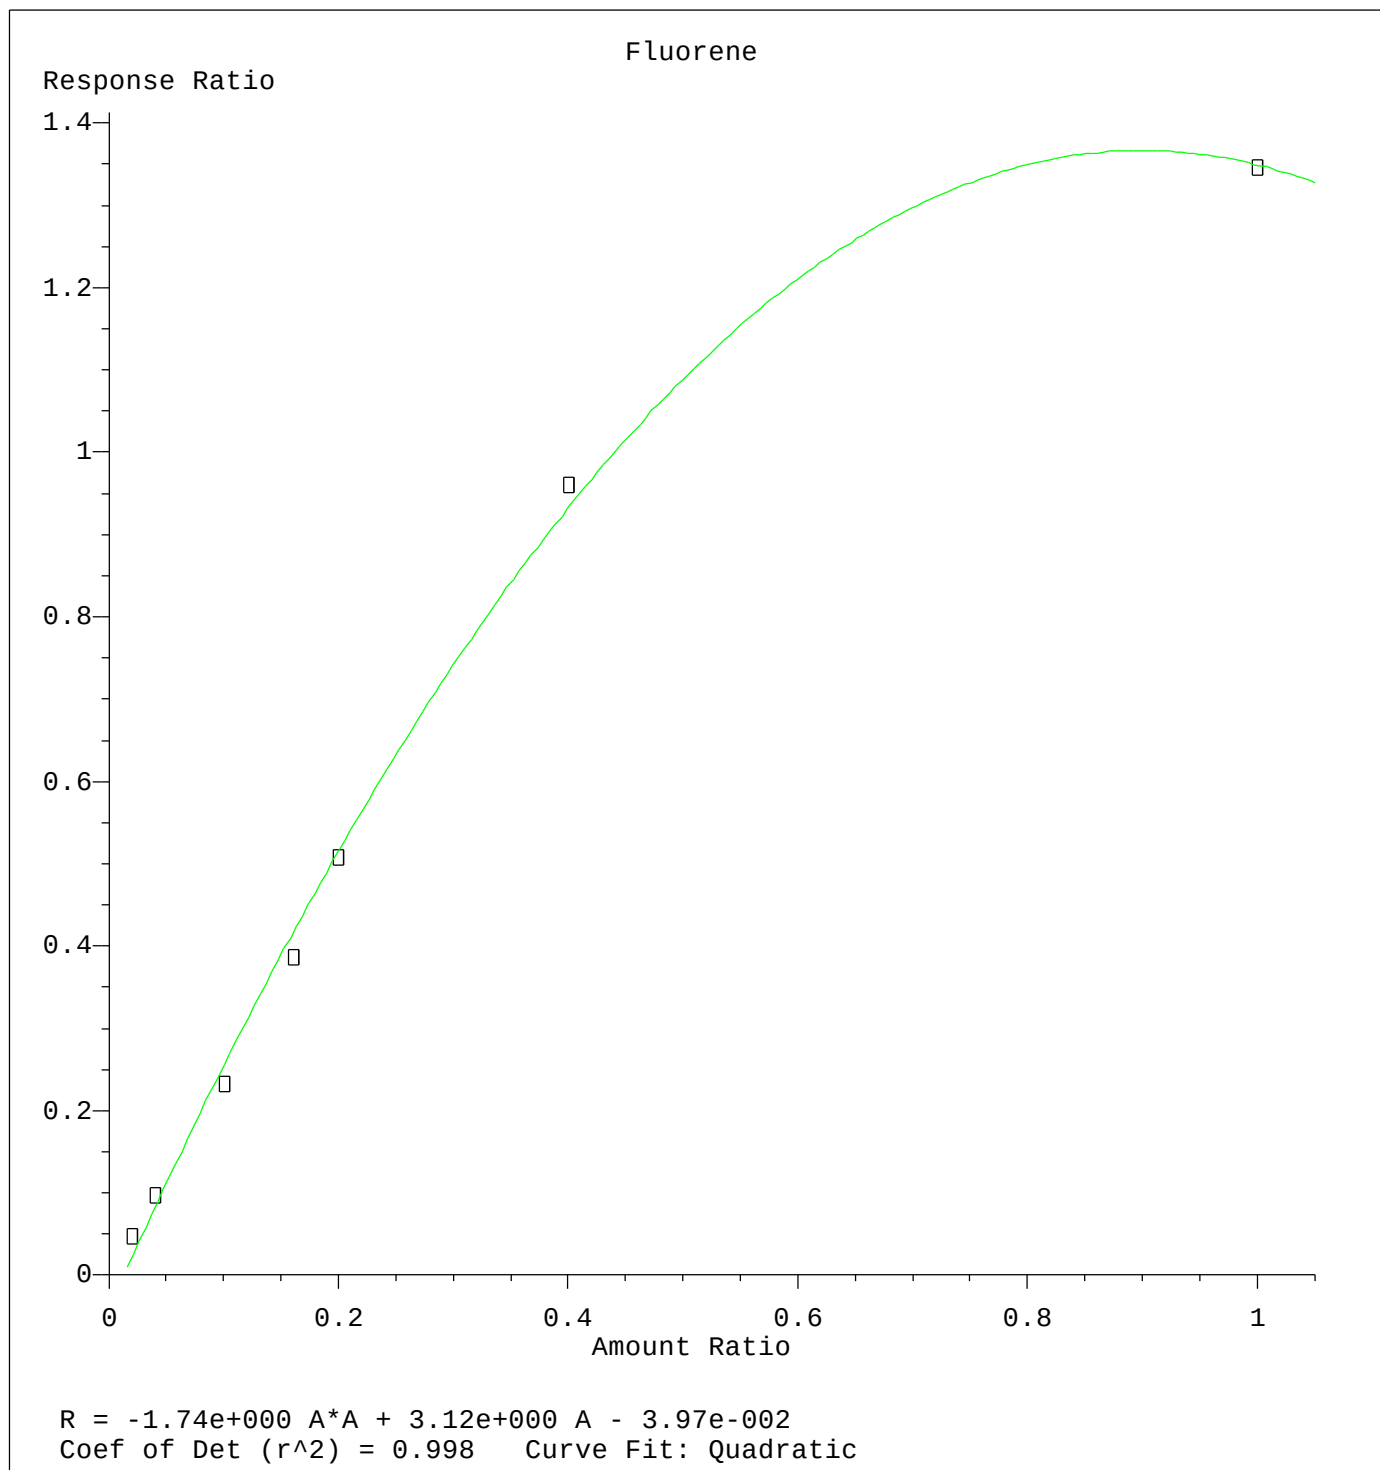


Method Name: Z:\HPCHEM1\BNA_M\METHODS\SIMPAH-BM052215.M
Calibration Table Last Updated: Sat May 23 04:41:38 2015

4-Bromophenyl-phenylether

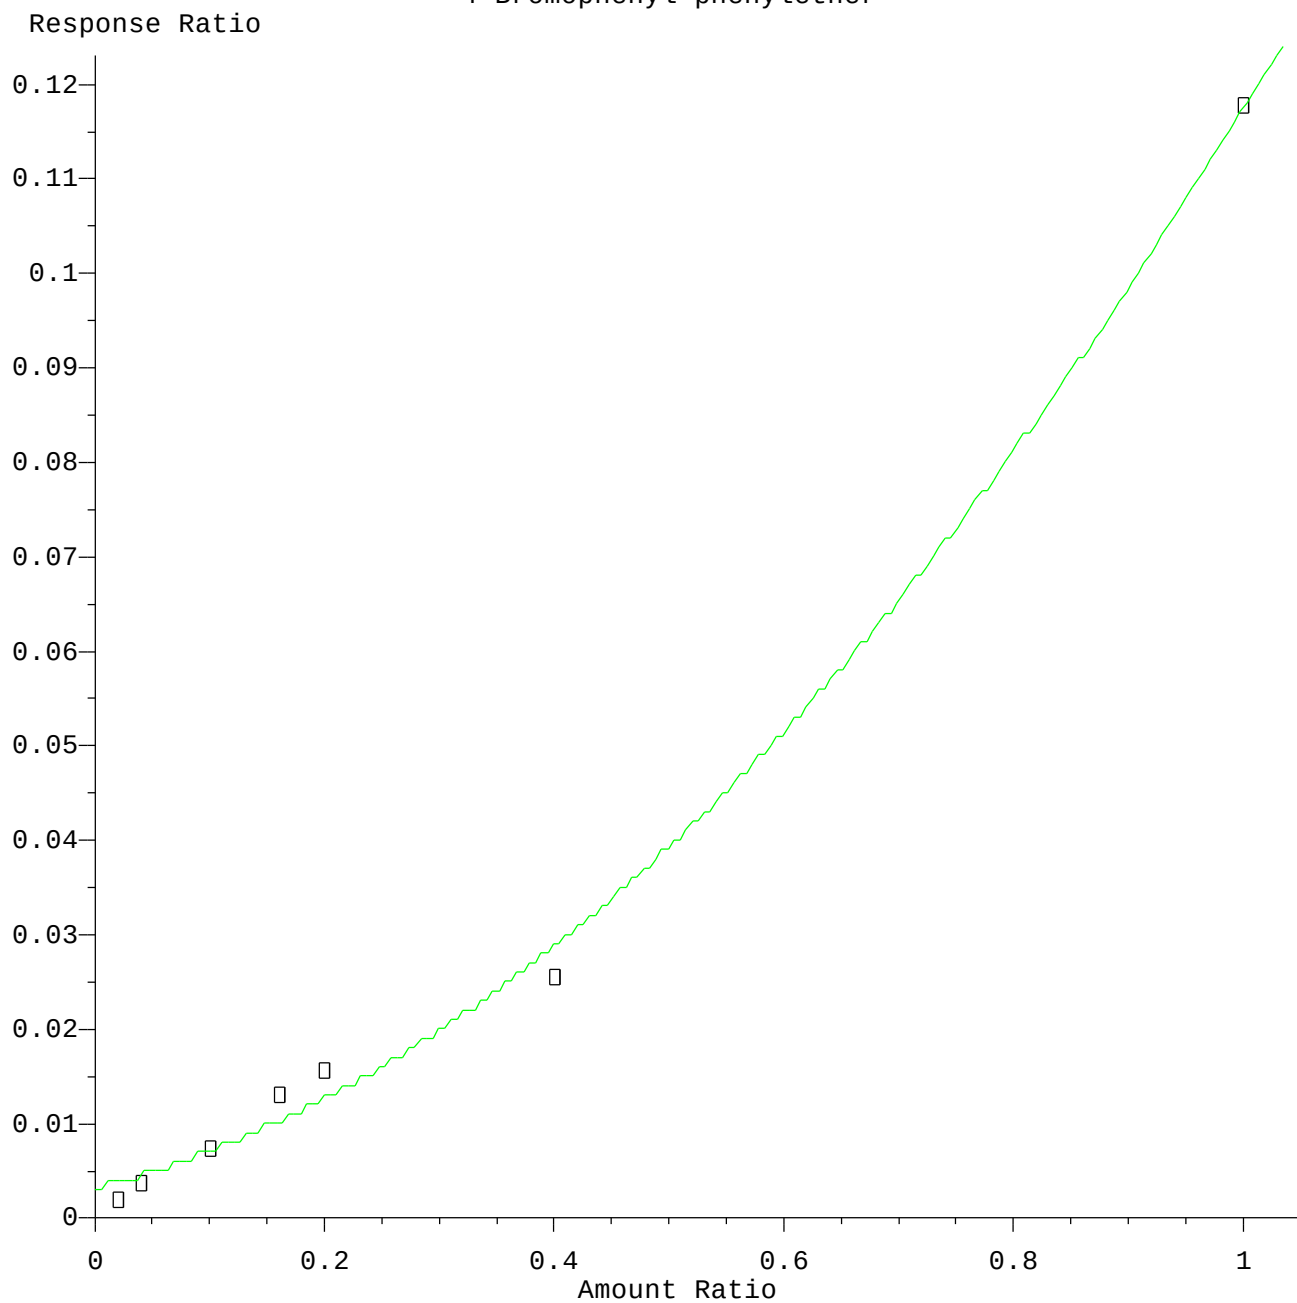


$R = 8.39e-002 A^2 + 3.02e-002 A + 3.26e-003$
Coef of Det (r^2) = 0.997 Curve Fit: Quadratic

Method Name: Z:\HPCHEM1\BNA_M\METHODS\SIMPAH-BM052215.M
Calibration Table Last Updated: Sat May 23 04:41:38 2015

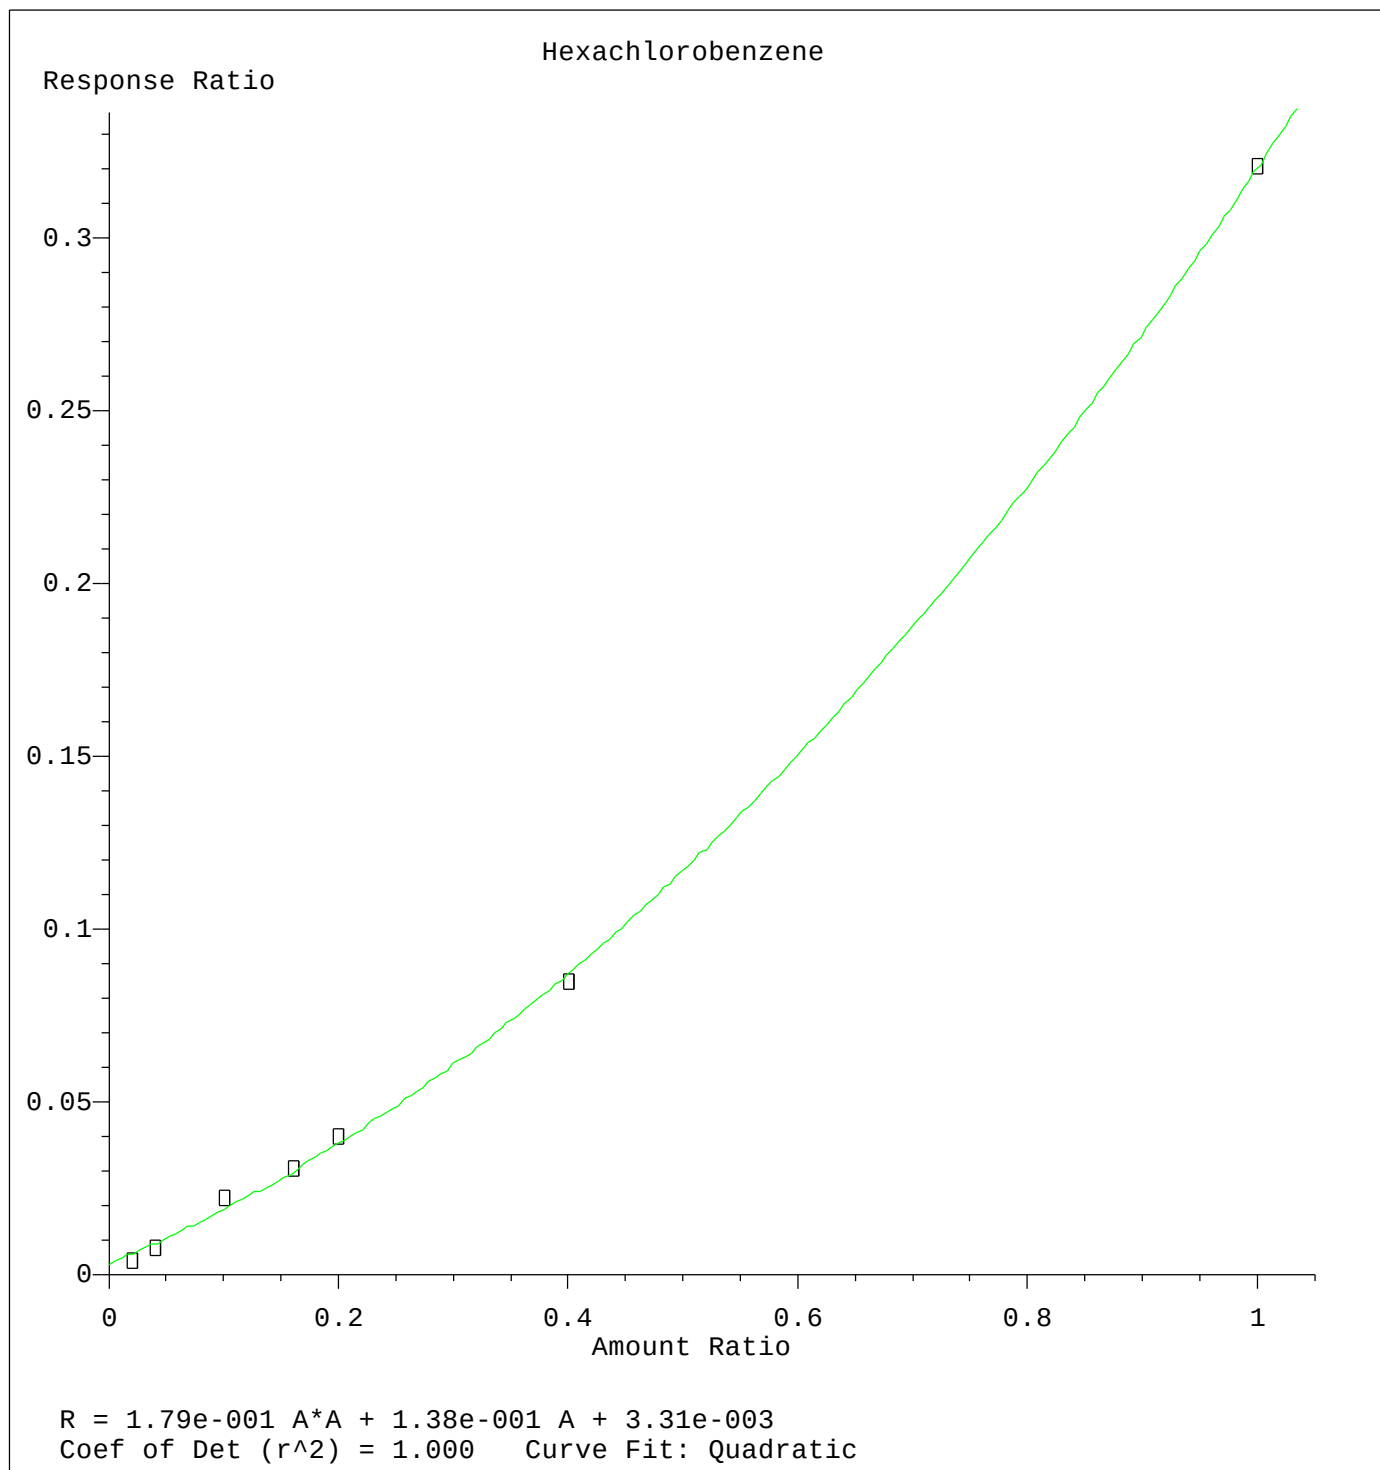


Method Name: Z:\HPCHEM1\BNA_M\METHODS\SIMPAH-BM052215.M
Calibration Table Last Updated: Sat May 23 04:44:00 2015

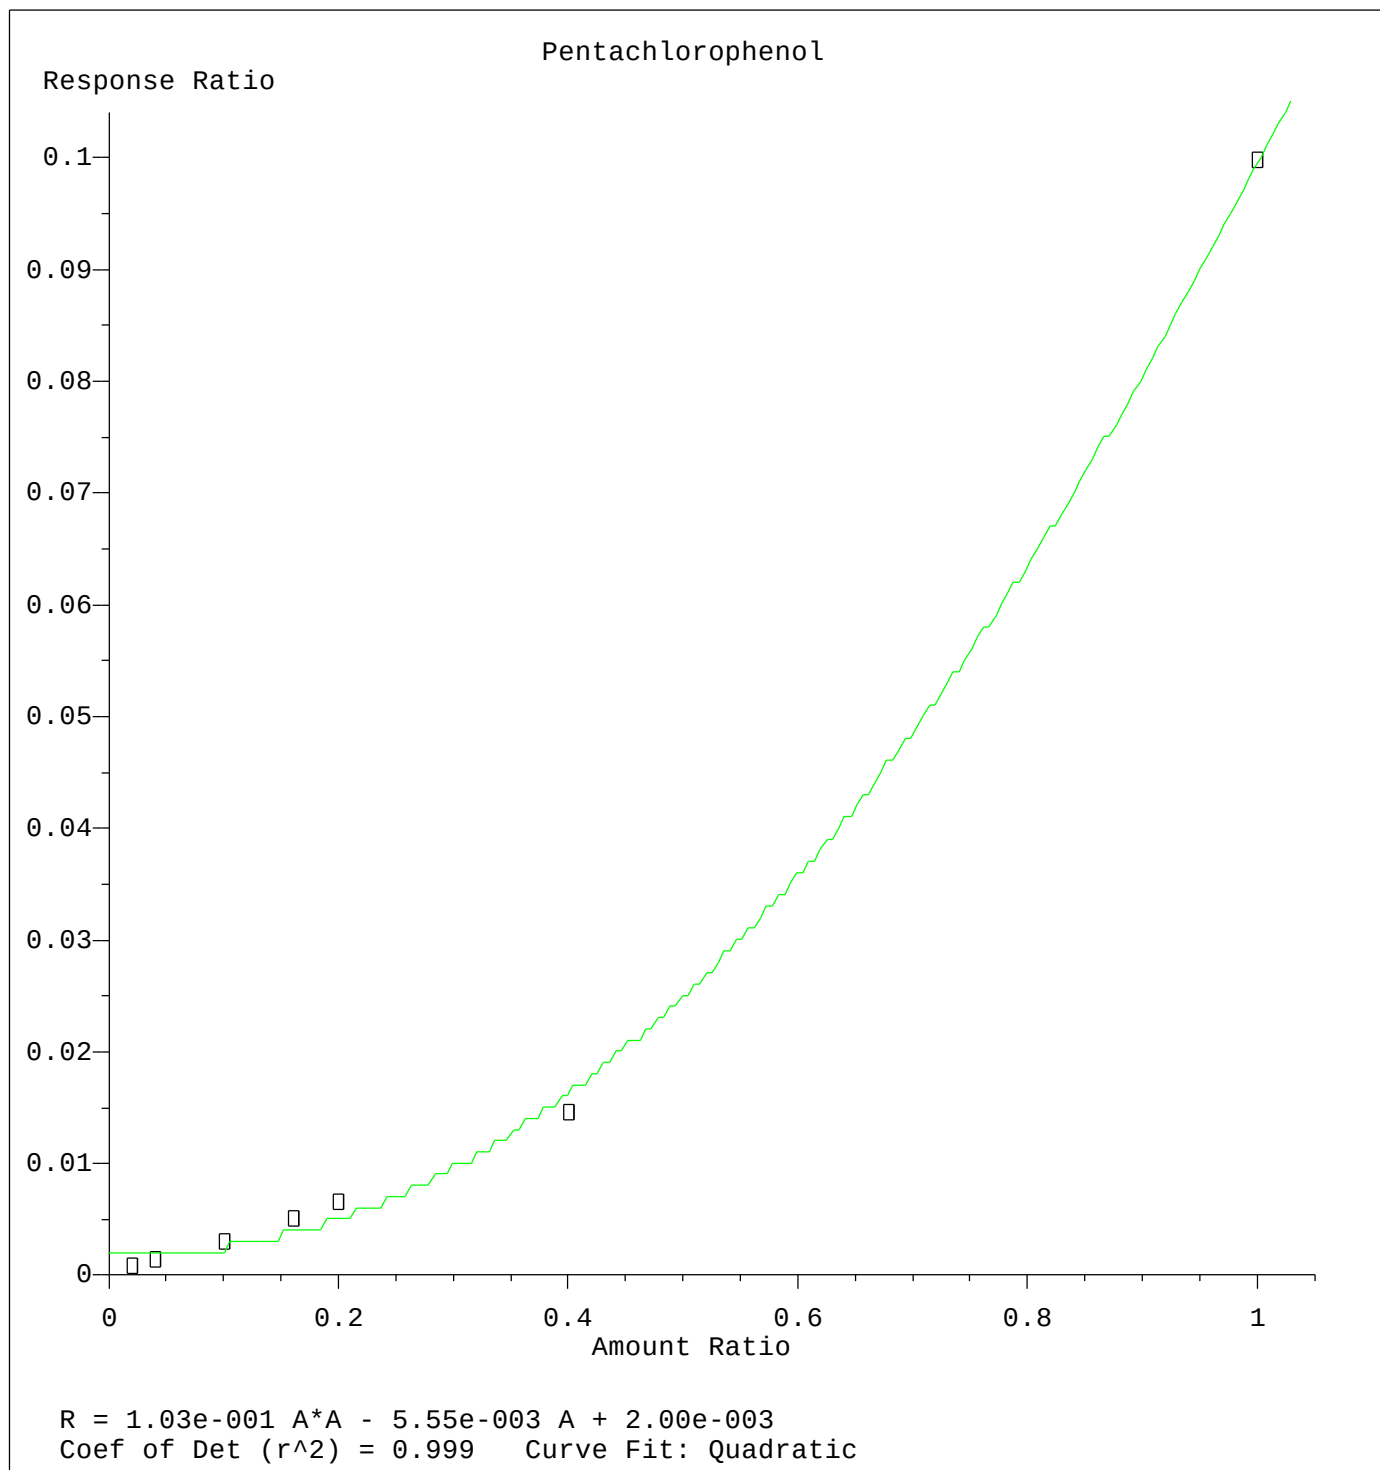

Method Name: Z:\HPCHEM1\BNA_M\METHODS\SIMPAH-BM052215.M
Calibration Table Last Updated: Sat May 23 04:44:29 2015

Phenanthrene

Response Ratio

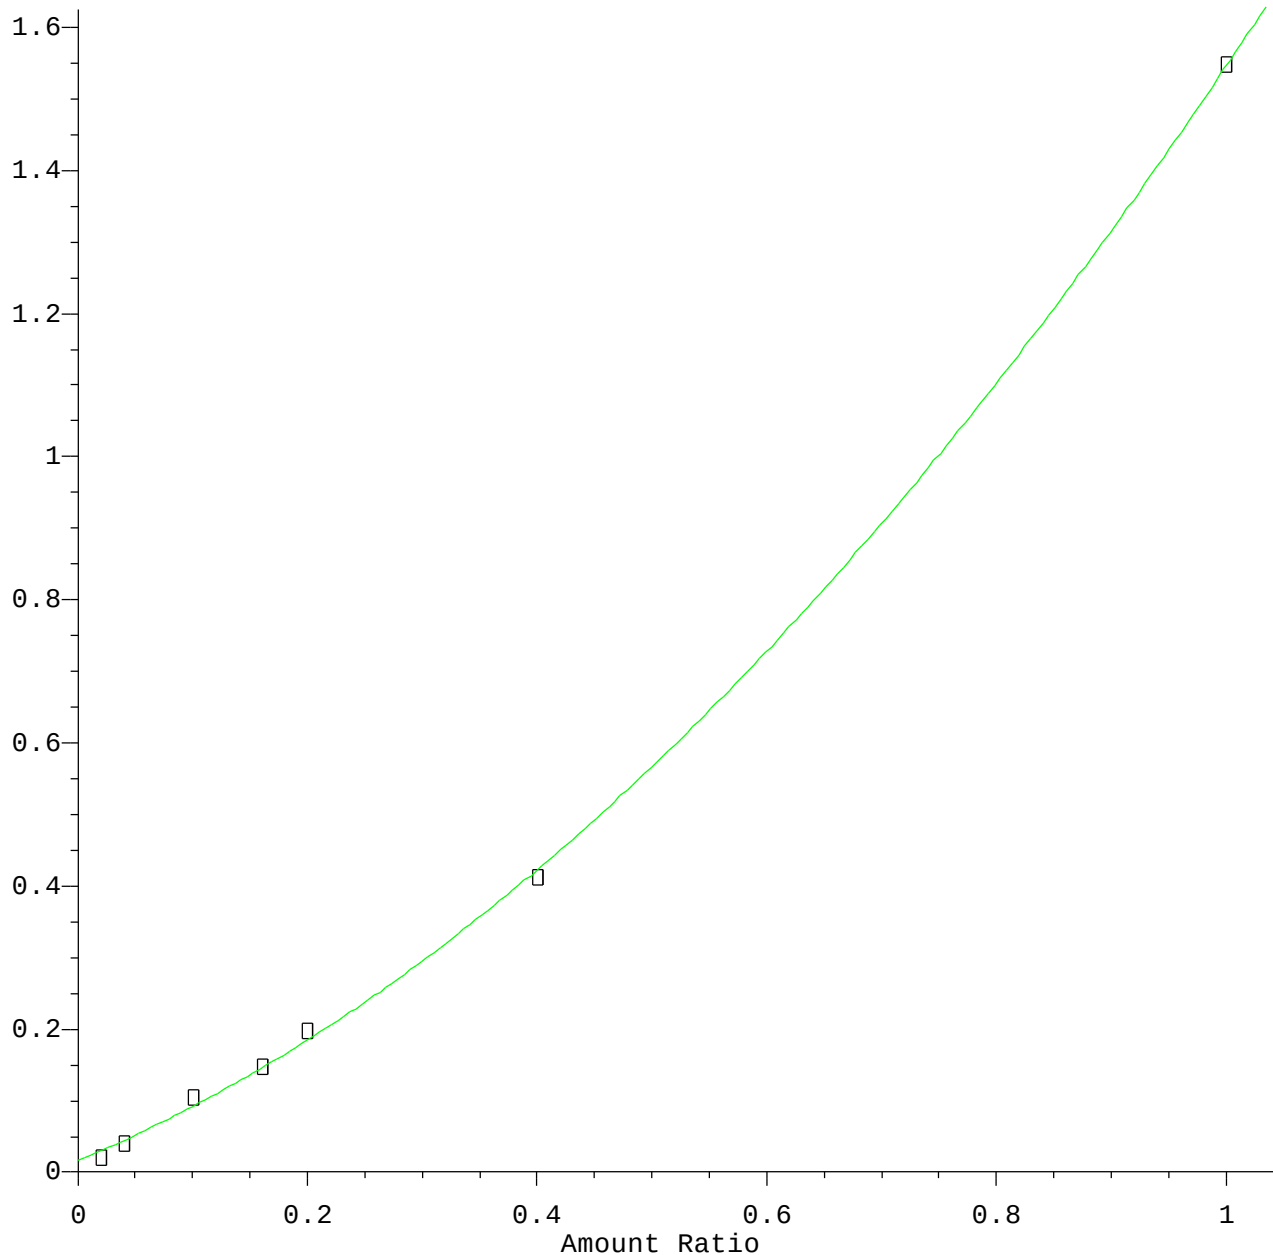

$R = 8.57e-001 A^2 + 6.73e-001 A + 1.57e-002$
Coef of Det (r^2) = 1.000 Curve Fit: Quadratic

Method Name: Z:\HPCHEM1\BNA_M\METHODS\SIMPAH-BM052215.M
Calibration Table Last Updated: Sat May 23 04:45:06 2015