

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM052215\
 Data File : BM001386.D
 Acq On : 22 May 2015 17:18
 Operator : TP/IZ
 Sample : SSTDICC0.2
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SSTDICC0.2

Quant Time: May 23 04:36:19 2015
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SIMPAH-BM052215.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat May 23 04:19:45 2015
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.40	152	14697	5.00	ng	0.00
6) Naphthalene-d8	10.18	136	51193	5.00	ng	0.00
12) Acenaphthene-d10	14.08	164	28580	5.00	ng	0.00
18) Phenanthrene-d10	16.82	188	95806	5.00	ng	0.00
25) Chrysene-d12	21.04	240	62028	5.00	ng	0.00
32) Perylene-d12	23.14	264	59128	5.00	ng	0.00

System Monitoring Compounds						
4) 2-Fluorophenol	4.99	112	572	0.20	ng	0.00
5) Phenol-d6	6.60	99	654	0.18	ng	0.00
7) Nitrobenzene-d5	8.55	82	539	0.19	ng	0.00
13) 2,4,6-Tribromophenol	15.59	330	194	0.20	ng	0.00
14) 2-Fluorobiphenyl	12.70	172	1760	0.20	ng	0.01
27) Terphenyl-d14	19.49	244	1638	0.20	ng	0.00


Target Compounds						Qvalue
3) n-Nitrosodimethylamine	3.20	42	402	0.24	ng	# 84
8) Nitrobenzene	8.60	77	549	0.19	ng	99
9) Naphthalene	10.22	128	2206	0.20	ng	# 93
10) Hexachlorobutadiene	10.52	225	460	0.21	ng	100
11) 2-Methylnaphthalene	11.86	142	1437	0.19	ng	95
15) Acenaphthylene	13.79	152	2195	0.18	ng	99
16) Acenaphthene	14.14	154	1499	0.20	ng	100
17) Fluorene	15.12	166	2753	0.39	ng	92
19) 4-Bromophenyl-phenylether	16.04	248	348	0.08	ng	# 91
20) Hexachlorobenzene	16.14	284	730	0.11	ng	94
21) Pentachlorophenol	16.51	266	128	0.05	ng	# 83
22) Phenanthrene	16.85	178	3711	0.12	ng	98
23) Anthracene	16.95	178	3601	0.26	ng	96
24) Fluoranthene	18.90	202	3420	0.12	ng	99
26) Pyrene	19.26	202	3579	0.19	ng	99
28) Benzo(a)anthracene	21.02	228	3492	0.19	ng	97
29) Chrysene	21.07	228	3277	0.19	ng	96
30) Bis(2-ethylhexyl)phthalate	20.97	149	1908	0.21	ng	99
31) Indeno(1,2,3-cd)pyrene	25.20	276	3658	0.20	ng	99
33) Benzo(b)fluoranthene	22.52	252	3662	0.20	ng	# 86
34) Benzo(k)fluoranthene	22.56	252	3044	0.19	ng	# 88
35) Benzo(a)pyrene	23.04	252	3080	0.20	ng	# 87
36) Dibenzo(a,h)anthracene	25.21	278	2805	0.20	ng	# 89
37) Benzo(g,h,i)perylene	25.83	276	3083	0.20	ng	95


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM052215\
Data File : BM001386.D
Acq On : 22 May 2015 17:18
Operator : TP/IZ
Sample : SSTDICC0.2
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SSTDICC0.2

Quant Time: May 23 04:36:19 2015
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SIMPAH-BM052215.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat May 23 04:19:45 2015
Response via : Initial Calibration



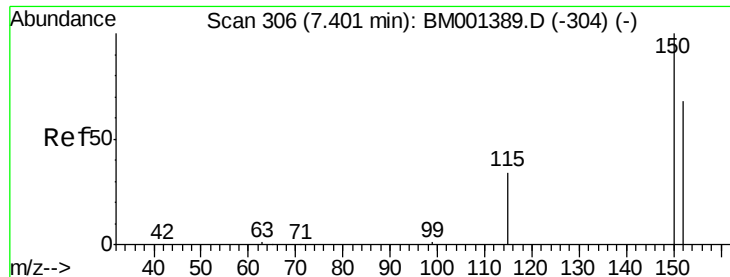

#1

1,4-Dichlorobenzene-d4

Concen: 5.00 ng

RT: 7.40 min Scan# 306

Delta R.T. 0.00 min

Lab File: BM001386.D

Acq: 22 May 2015 17:18

Instrument :

BNA_M

ClientSampleId :

SSTDICC0.2


Tgt Ion:152 Resp: 14697

Ion Ratio Lower Upper

152 100

150 147.4 119.0 178.6




115 51.7 41.8 62.8



Abundance Ion 152.00 (151.70 to 152.70): E

Ion 150.00 (149.70 to 150.70): E

Ion 115.00 (114.70 to 115.70): E



#3

n-Nitrosodimethylamine

Concen: 0.24 ng

RT: 3.20 min Scan# 34

Delta R.T. 0.00 min

Lab File: BM001386.D

Acq: 22 May 2015 17:18


Tgt Ion: 42 Resp: 402

Ion Ratio Lower Upper

42 100

74 74.6 72.2 108.2



44 10.7 6.2 9.2#




Abundance Ion 42.00 (41.70 to 42.70): BM0

Ion 74.00 (73.70 to 74.70): BM0

Ion 44.00 (43.70 to 44.70): BM0





#4

2-Fluorophenol

Concen: 0.20 ng

RT: 4.99 min Scan# 150

Delta R.T. 0.00 min

Lab File: BM001386.D

Acq: 22 May 2015 17:18

Instrument :

BNA_M

ClientSampleId :

SSTDICC0.2


Tgt Ion: 112 Resp: 572

Ion Ratio Lower Upper

112 100

64 65.7 51.7 77.5




63 37.1 29.7 44.5



Abundance Ion 112.00 (111.70 to 112.70): B

Ion 64.00 (63.70 to 64.70): BM

Ion 63.00 (62.70 to 63.70): BM



#5

Phenol-d6

Concen: 0.18 ng

RT: 6.60 min Scan# 254

Delta R.T. 0.00 min

Lab File: BM001386.D

Acq: 22 May 2015 17:18


Tgt Ion: 99 Resp: 654

Ion Ratio Lower Upper

99 100

42 27.7 21.8 32.6



71 37.6 29.2 43.8




Abundance Ion 99.00 (98.70 to 99.70): B

Ion 42.00 (41.70 to 42.70): B

Ion 71.00 (70.70 to 71.70): B





#6

Naphthalene-d8

Concen: 5.00 ng

RT: 10.18 min Scan# 535

Delta R.T. 0.00 min

Lab File: BM001386.D

Acq: 22 May 2015 17:18

Instrument :

BNA_M

ClientSampleId :

SSTDIC0.2

Tgt Ion:136 Resp: 51193


Ion Ratio Lower Upper

136 100

137 11.7 9.1 13.7

54 5.5 4.3 6.5

68 3.4 2.6 4.0




Abundance Ion 136.00 (135.70 to 136.70): E


Ion 137.00 (136.70 to 137.70): E

Ion 54.00 (53.70 to 54.70): BM

Ion 68.00 (67.70 to 68.70): BM



Time-->



#7

Nitrobenzene-d5

Concen: 0.19 ng

RT: 8.55 min Scan# 393

Delta R.T. 0.00 min

Lab File: BM001386.D

Acq: 22 May 2015 17:18


Tgt Ion: 82 Resp: 539

Ion Ratio Lower Upper

82 100

128 44.4 30.2 45.4


54 74.4 52.9 79.3




Abundance Ion 82.00 (81.70 to 82.70): BM

Ion 128.00 (127.70 to 128.70): E

Ion 54.00 (53.70 to 54.70): BM







Time-->



#8
 Nitrobenzene
 Concen: 0.19 ng
 RT: 8.60 min Scan# 397
 Delta R.T. 0.00 min
 Lab File: BM001386.D
 Acq: 22 May 2015 17:18




Instrument :
 BNA_M
 ClientSampleId :
 SSTDICC0.2


Tgt Ion: 77 Resp: 549
 Ion Ratio Lower Upper
 77 100
 123 42.4 33.7 50.5
 65 15.3 11.3 16.9



#9
 Naphthalene
 Concen: 0.20 ng
 RT: 10.22 min Scan# 537
 Delta R.T. 0.00 min
 Lab File: BM001386.D
 Acq: 22 May 2015 17:18

Tgt Ion: 128 Resp: 2206
 Ion Ratio Lower Upper
 128 100
 129 14.1 8.6 13.0#
 127 17.2 11.7 17.5









#10
Hexachlorobutadiene
Concen: 0.21 ng
RT: 10.52 min Scan# 555
Delta R.T. 0.00 min
Lab File: BM001386.D
Acq: 22 May 2015 17:18




Instrument :
BNA_M
ClientSampleId :
SSTDIC0.2


Tgt Ion: 225 Resp: 460
Ion Ratio Lower Upper
225 100
223 62.4 50.2 75.2
227 63.7 51.1 76.7



#11
2-Methylnaphthalene
Concen: 0.19 ng
RT: 11.86 min Scan# 653
Delta R.T. 0.00 min
Lab File: BM001386.D
Acq: 22 May 2015 17:18

Tgt Ion: 142 Resp: 1437
Ion Ratio Lower Upper
142 100
141 94.4 72.6 109.0
115 44.7 31.2 46.8





#12

Acenaphthene-d10

Concen: 5.00 ng

RT: 14.08 min Scan# 858

Delta R.T. 0.00 min





Lab File: BM001386.D

Acq: 22 May 2015 17:18

Instrument :
BNA_M
ClientSampleId :
SSTDIC0.2

Tgt Ion:164 Resp: 28580

Ion	Ratio	Lower	Upper
164	100		
162	105.3	83.4	125.2
160	47.1	36.9	55.3



#13

2,4,6-Tribromophenol

Concen: 0.20 ng

RT: 15.59 min Scan# 936




Delta R.T. 0.00 min


Lab File: BM001386.D

Acq: 22 May 2015 17:18

Tgt Ion:330 Resp: 194

Ion	Ratio	Lower	Upper
330	100		
332	106.2	90.3	135.5
141	0.0	0.0	0.0









#14
2-Fluorobiphenyl
Concen: 0.20 ng
RT: 12.70 min Scan# 734
Delta R.T. 0.01 min
Lab File: BM001386.D
Acq: 22 May 2015 17:18




Instrument :
BNA_M
ClientSampleId :
SSTDIC0.2


Tgt Ion:172 Resp: 1760
Ion Ratio Lower Upper
172 100
171 33.6 29.4 44.0
170 21.6 20.2 30.4



#15
Acenaphthylene
Concen: 0.18 ng
RT: 13.79 min Scan# 834
Delta R.T. 0.00 min
Lab File: BM001386.D
Acq: 22 May 2015 17:18

Tgt Ion:152 Resp: 2195
Ion Ratio Lower Upper
152 100
151 19.4 15.1 22.7
153 12.8 10.2 15.4









#16
Acenaphthene
Concen: 0.20 ng
RT: 14.14 min Scan# 863
Delta R.T. 0.00 min
Lab File: BM001386.D
Acq: 22 May 2015 17:18




Instrument :
BNA_M
ClientSampleId :
SSTDIC0.2


Tgt Ion:154 Resp: 1499
Ion Ratio Lower Upper
154 100
153 114.5 91.4 137.2
152 55.4 44.0 66.0



#17
Fluorene
Concen: 0.39 ng
RT: 15.12 min Scan# 922
Delta R.T. 0.00 min
Lab File: BM001386.D
Acq: 22 May 2015 17:18

Tgt Ion:166 Resp: 2753
Ion Ratio Lower Upper
166 100
165 99.9 72.6 108.8
167 13.6 10.9 16.3





#18

Phenanthrene-d10

Concen: 5.00 ng

RT: 16.82 min Scan# 972

Delta R.T. 0.00 min

Lab File: BM001386.D

Acq: 22 May 2015 17:18

Instrument :

BNA_M

ClientSampleId :

SSTDIC0.2


Tgt Ion:188 Resp: 95806

Ion Ratio Lower Upper

188 100

94 4.1 3.0 4.4




80 3.7 2.5 3.7



Abundance Ion 188.00 (187.70 to 188.70): E

Ion 94.00 (93.70 to 94.70): BM

Ion 80.00 (79.70 to 80.70): BM



#19

4-Bromophenyl-phenylether

Concen: 0.08 ng

RT: 16.04 min Scan# 949

Delta R.T. 0.00 min

Lab File: BM001386.D

Acq: 22 May 2015 17:18


Tgt Ion:248 Resp: 348

Ion Ratio Lower Upper

248 100

250 135.3 117.8 176.6



141 0.0 0.0 0.0




Abundance Ion 248.00 (247.70 to 248.70): E

Ion 250.00 (249.70 to 250.70): E

Ion 141.00 (140.70 to 141.70): E





#20

Hexachlorobenzene

Concen: 0.11 ng

RT: 16.14 min Scan# 952

Delta R.T. 0.00 min

Lab File: BM001386.D

Acq: 22 May 2015 17:18

Instrument :

BNA_M

ClientSampleId :

SSTDIC0.2


Tgt Ion:284 Resp: 730

Ion Ratio Lower Upper

284 100

142 19.0 13.9 20.9

249 53.0 39.0 58.4






Abundance Ion 283.80 (283.50 to 284.50): E

Ion 142.00 (141.70 to 142.70): E

Ion 249.00 (248.70 to 249.70): E

Time-->



#21

Pentachlorophenol

Concen: 0.05 ng

RT: 16.51 min Scan# 963

Delta R.T. 0.00 min

Lab File: BM001386.D

Acq: 22 May 2015 17:18


Tgt Ion:266 Resp: 128

Ion Ratio Lower Upper

266 100

268 90.8 63.0 94.4

264 82.9 52.8 79.2#






Abundance Ion 265.70 (265.40 to 266.40): E

Ion 268.00 (267.70 to 268.70): E

Ion 264.00 (263.70 to 264.70): E

Time-->





#22

Phenanthrene

Concen: 0.12 ng

RT: 16.85 min Scan# 973

Delta R.T. 0.00 min





Lab File: BM001386.D

Acq: 22 May 2015 17:18

Instrument :
BNA_M
ClientSampleId :
SSTDIC0.2

Tgt Ion:178 Resp: 3711

Ion	Ratio	Lower	Upper
178	100		
176	21.0	16.8	25.2
179	15.2	11.0	16.4



#23

Anthracene

Concen: 0.26 ng

RT: 16.95 min Scan# 976




Delta R.T. 0.00 min


Lab File: BM001386.D

Acq: 22 May 2015 17:18

Tgt Ion:178 Resp: 3601

Ion	Ratio	Lower	Upper
178	100		
176	17.2	13.1	19.7
179	19.0	12.8	19.2









#24
 Fluoranthene
 Concen: 0.12 ng
 RT: 18.90 min Scan# 1068
 Delta R.T. 0.00 min
 Lab File: BM001386.D
 Acq: 22 May 2015 17:18




Instrument :
 BNA_M
 ClientSampleId :
 SSTDICC0.2


Tgt Ion: 202 Resp: 3420
 Ion Ratio Lower Upper
 202 100
 101 10.6 8.6 12.8
 203 16.7 13.8 20.6



#25
 Chrysene-d12
 Concen: 5.00 ng
 RT: 21.04 min Scan# 1236
 Delta R.T. 0.00 min
 Lab File: BM001386.D
 Acq: 22 May 2015 17:18

Tgt Ion: 240 Resp: 62028
 Ion Ratio Lower Upper
 240 100
 120 16.8 9.7 14.5#
 236 33.1 24.8 37.2









#26
Pyrene
Concen: 0.19 ng
RT: 19.26 min Scan# 1098
Delta R.T. 0.00 min
Lab File: BM001386.D
Acq: 22 May 2015 17:18

Instrument :
BNA_M
ClientSampleId :
SSTDIC0.2

Tgt Ion:202 Resp: 3579
Ion Ratio Lower Upper
202 100
200 20.2 16.4 24.6
203 17.1 13.9 20.9




Abundance Ion 202.00 (201.70 to 202.70): E
Ion 200.00 (199.70 to 200.70): E
Ion 203.00 (202.70 to 203.70): E






#27
Terphenyl-d14
Concen: 0.20 ng
RT: 19.49 min Scan# 1117
Delta R.T. 0.00 min
Lab File: BM001386.D
Acq: 22 May 2015 17:18

Tgt Ion:244 Resp: 1638
Ion Ratio Lower Upper
244 100
212 12.4 7.2 10.8#
122 11.7 5.1 7.7#



Abundance Ion 244.00 (243.70 to 244.70): E
Ion 212.00 (211.70 to 212.70): E
Ion 122.00 (121.70 to 122.70): E









#28
Benzo(a)anthracene
Concen: 0.19 ng
RT: 21.02 min Scan# 1235
Delta R.T. 0.00 min
Lab File: BM001386.D
Acq: 22 May 2015 17:18




Instrument :
BNA_M
ClientSampleId :
SSTDICC0.2


Tgt Ion:228 Resp: 3492
Ion Ratio Lower Upper
228 100
226 29.3 21.9 32.9
229 20.0 15.1 22.7



#29
Chrysene
Concen: 0.19 ng
RT: 21.07 min Scan# 1238
Delta R.T. 0.00 min
Lab File: BM001386.D
Acq: 22 May 2015 17:18

Tgt Ion:228 Resp: 3277
Ion Ratio Lower Upper
228 100
226 36.9 27.6 41.4
229 19.1 13.6 20.4





#30

Bis(2-ethylhexyl)phthalate

Concen: 0.21 ng

RT: 20.97 min Scan# 1232

Delta R.T. 0.00 min

Lab File: BM001386.D

Acq: 22 May 2015 17:18

Instrument :

BNA_M

ClientSampleId :

SSTDICC0.2


Tgt Ion:149 Resp: 1908

Ion Ratio Lower Upper




149 100

167 26.6 21.0 31.6

279 2.8 2.2 3.2



Abundance Ion 149.00 (148.70 to 149.70): E
Ion 167.00 (166.70 to 167.70): E
Ion 279.00 (278.70 to 279.70): E



#31

Indeno(1,2,3-cd)pyrene

Concen: 0.20 ng

RT: 25.20 min Scan# 1605

Delta R.T. 0.00 min

Lab File: BM001386.D

Acq: 22 May 2015 17:18


Tgt Ion:276 Resp: 3658

Ion Ratio Lower Upper



276 100


138 28.5 23.4 35.0

277 24.0 19.5 29.3



Abundance Ion 276.00 (275.70 to 276.70): E
Ion 138.00 (137.70 to 138.70): E
Ion 277.00 (276.70 to 277.70): E









#32
 Perylene-d12
 Concen: 5.00 ng
 RT: 23.14 min Scan# 1407
 Delta R.T. 0.00 min
 Lab File: BM001386.D
 Acq: 22 May 2015 17:18




Instrument :
 BNA_M
 ClientSampleId :
 SSTDICC0.2


Tgt Ion: 264 Resp: 59128
 Ion Ratio Lower Upper
 264 100
 260 26.5 20.1 30.1
 265 20.6 17.1 25.7



#33
 Benzo(b)fluoranthene
 Concen: 0.20 ng
 RT: 22.52 min Scan# 1348
 Delta R.T. 0.01 min
 Lab File: BM001386.D
 Acq: 22 May 2015 17:18

Tgt Ion: 252 Resp: 3662
 Ion Ratio Lower Upper
 252 100
 253 29.2 17.4 26.0#
 125 17.0 10.2 15.4#





#34

Benzo(k)fluoranthene

Concen: 0.19 ng

RT: 22.56 min Scan# 1352

Delta R.T. 0.01 min

Lab File: BM001386.D

Acq: 22 May 2015 17:18

Instrument :

BNA_M

ClientSampleId :

SSTDICC0.2


Tgt Ion:252 Resp: 3044

Ion Ratio Lower Upper

252 100

253 29.4 17.6 26.4#




125 14.4 9.7 14.5



Abundance Ion 252.00 (251.70 to 252.70): E

Ion 253.00 (252.70 to 253.70): E

Ion 125.00 (124.70 to 125.70): E



#35

Benzo(a)pyrene

Concen: 0.20 ng

RT: 23.04 min Scan# 1398

Delta R.T. 0.00 min

Lab File: BM001386.D

Acq: 22 May 2015 17:18


Tgt Ion:252 Resp: 3080

Ion Ratio Lower Upper

252 100

253 28.6 18.6 28.0#



125 19.9 10.7 16.1#




Abundance Ion 252.00 (251.70 to 252.70): E

Ion 253.00 (252.70 to 253.70): E

Ion 125.00 (124.70 to 125.70): E









#36
Dibenzo(a,h)anthracene
Concen: 0.20 ng
RT: 25.21 min Scan# 1606
Delta R.T. 0.00 min
Lab File: BM001386.D
Acq: 22 May 2015 17:18

Instrument :
BNA_M
ClientSampleId :
SSTDICC0.2

Tgt Ion: 278 Resp: 2805

Ion	Ratio	Lower	Upper
278	100		
139	24.9	15.7	23.5#
279	29.5	19.4	29.2#



#37
Benzo(g,h,i)perylene
Concen: 0.20 ng
RT: 25.83 min Scan# 1665
Delta R.T. 0.00 min
Lab File: BM001386.D
Acq: 22 May 2015 17:18

Tgt Ion: 276 Resp: 3083

Ion	Ratio	Lower	Upper
276	100		
277	26.3	19.8	29.6
138	28.4	20.2	30.2

