

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM052215\
 Data File : BM001406.D
 Acq On : 23 May 2015 06:24
 Operator : TP/IZ
 Sample : G2334-07
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 RAV-GT-106

Quant Time: May 25 08:53:40 2015
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SIMPAH-BM052215.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat May 23 04:45:39 2015
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.40	152	10020	5.00	ng	0.00
6) Naphthalene-d8	10.16	136	36278	5.00	ng	-0.02
12) Acenaphthene-d10	14.08	164	21250	5.00	ng	0.00
18) Phenanthrene-d10	16.82	188	74055	5.00	ng	0.00
25) Chrysene-d12	21.04	240	44845	5.00	ng	0.00
32) Perylene-d12	23.13	264	38118	5.00	ng	-0.01
System Monitoring Compounds						
4) 2-Fluorophenol	4.99	112	7481	3.78	ng	0.00
5) Phenol-d6	6.60	99	5595	2.44	ng	0.00
7) Nitrobenzene-d5	8.55	82	13656	6.52	ng	0.00
13) 2,4,6-Tribromophenol	15.59	330	5825	8.82	ng	0.00
14) 2-Fluorobiphenyl	12.69	172	45328	6.93	ng	0.00
27) Terphenyl-d14	19.48	244	50488	8.32	ng	-0.01
Target Compounds						
30) Bis(2-ethylhexyl)phthalate	20.96	149	1623	0.23	ng	Qvalue 95


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM052215\
Data File : BM001406.D
Acq On : 23 May 2015 06:24
Operator : TP/IZ
Sample : G2334-07
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
RAV-GT-106

Quant Time: May 25 08:53:40 2015
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SIMPAH-BM052215.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat May 23 04:45:39 2015
Response via : Initial Calibration

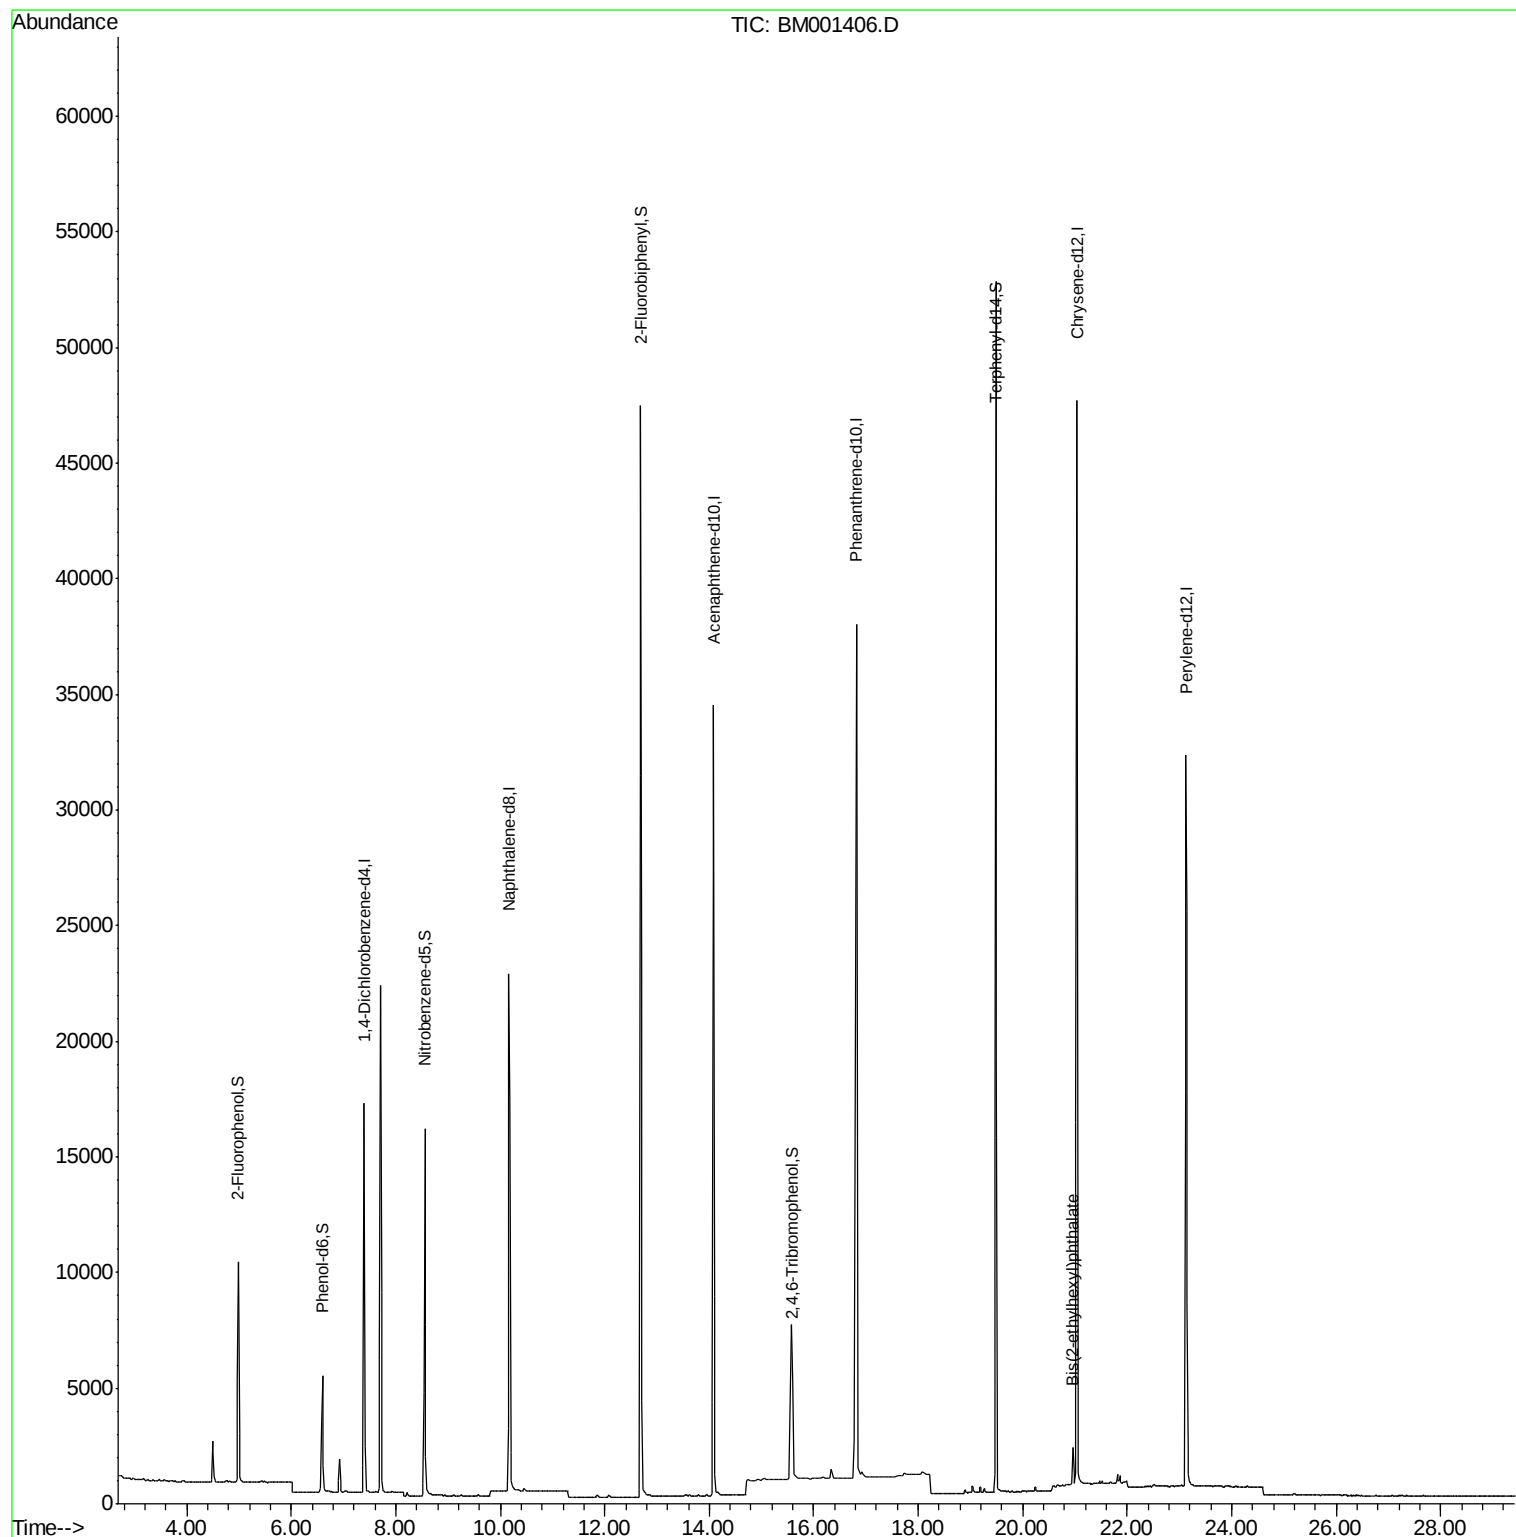

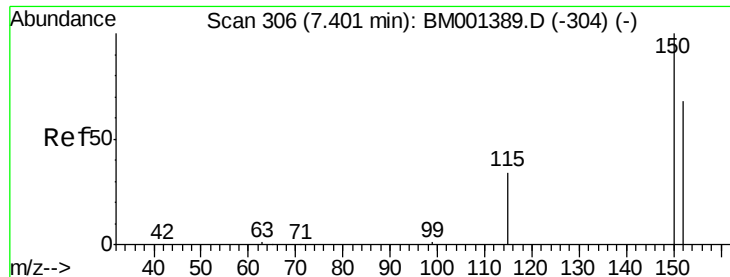

#1

1,4-Dichlorobenzene-d4

Concen: 5.00 ng

RT: 7.40 min Scan# 306

Delta R.T. 0.00 min

Lab File: BM001406.D

Acq: 23 May 2015 06:24

Instrument :

BNA_M

ClientSampleId :

RAV-GT-106


Tgt Ion:152 Resp: 10020

Ion Ratio Lower Upper

152 100

150 139.1 119.0 178.6




115 46.4 41.8 62.8

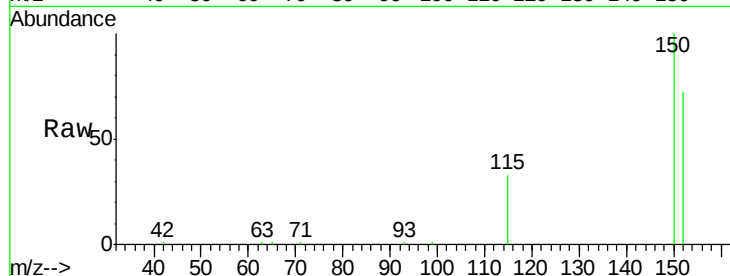

Abundance Ion 152.00 (151.70 to 152.70): E

Ion 150.00 (149.70 to 150.70): E

Ion 115.00 (114.70 to 115.70): E

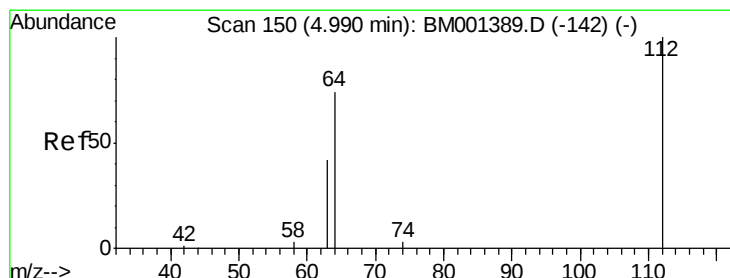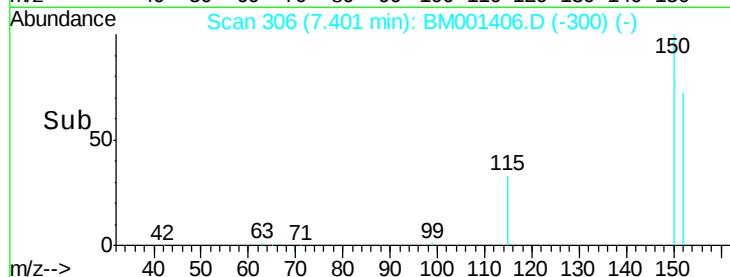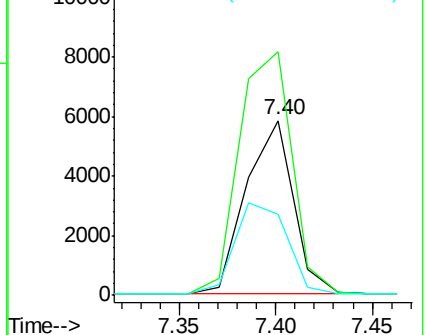

#4

2-Fluorophenol

Concen: 3.78 ng

RT: 4.99 min Scan# 150

Delta R.T. 0.00 min

Lab File: BM001406.D

Acq: 23 May 2015 06:24


Tgt Ion:112 Resp: 7481

Ion Ratio Lower Upper

112 100

64 64.1 51.7 77.5



63 37.0 29.7 44.5

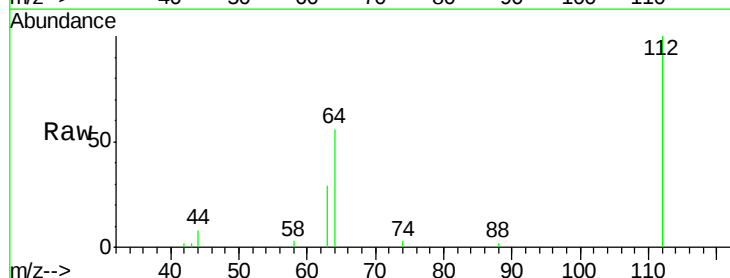


Abundance Ion 112.00 (111.70 to 112.70): E

Ion 64.00 (63.70 to 64.70): BM0

Ion 63.00 (62.70 to 63.70): BM0

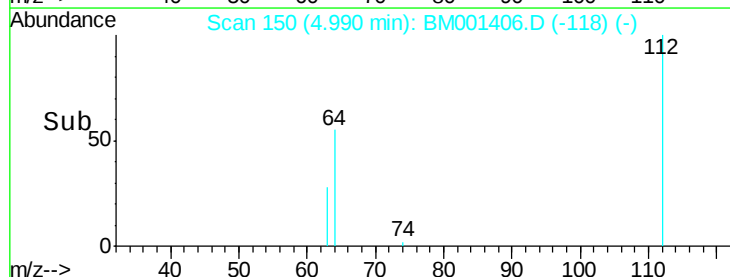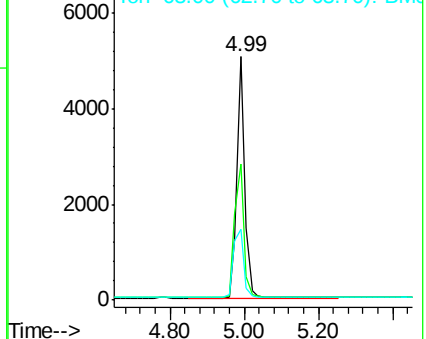

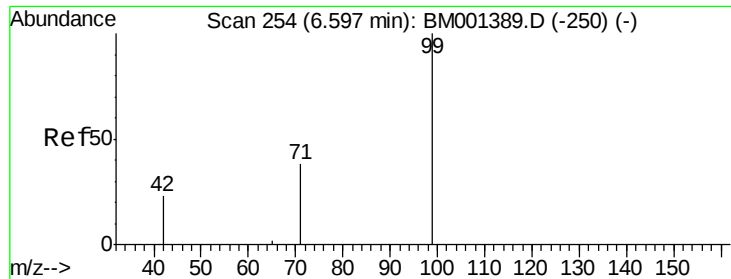

#5

Phenol-d6

Concen: 2.44 ng

RT: 6.60 min Scan# 254

Delta R.T. 0.00 min

Lab File: BM001406.D

Acq: 23 May 2015 06:24

Instrument :

BNA_M

ClientSampleId :

RAV-GT-106


Tgt Ion: 99 Resp: 5595

Ion Ratio Lower Upper




99 100

42 25.7 21.8 32.6

71 36.9 29.2 43.8

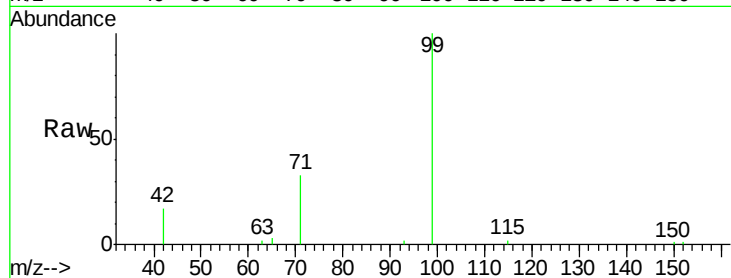

Abundance Ion 99.00 (98.70 to 99.70): BM001406.D (-222) (-)

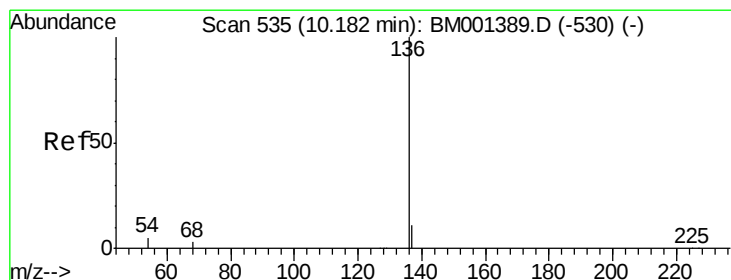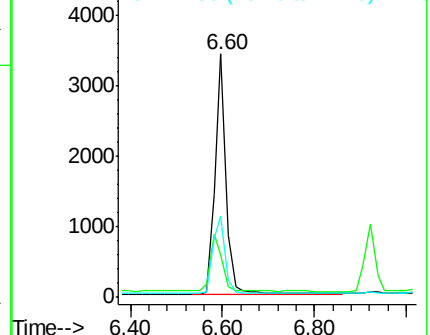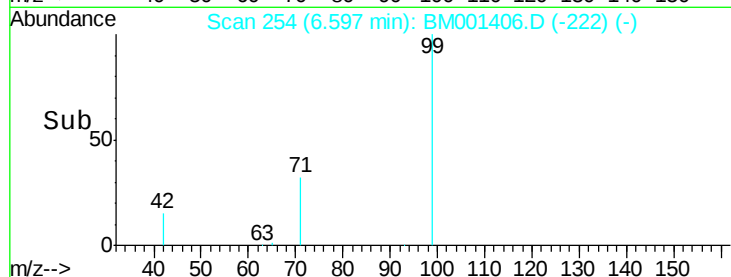

#6

Naphthalene-d8

Concen: 5.00 ng

RT: 10.16 min Scan# 534

Delta R.T. -0.02 min

Lab File: BM001406.D

Acq: 23 May 2015 06:24

Tgt Ion: 136 Resp: 36278


Ion Ratio Lower Upper

136 100



137 10.2 9.1 13.7


54 14.0 4.3 6.5#

68 7.4 2.6 4.0#

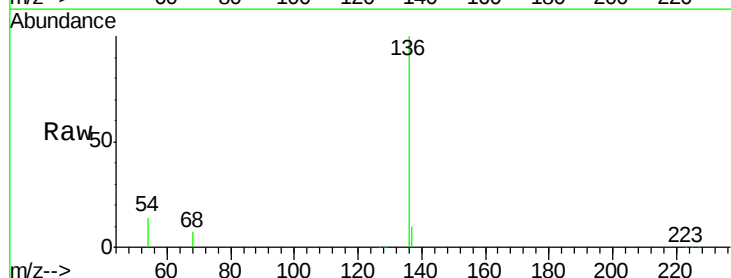

Abundance Ion 136.00 (135.70 to 136.70): BM001406.D (-518) (-)

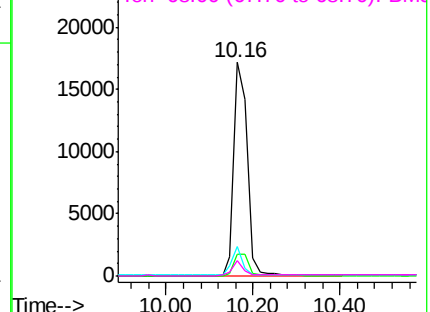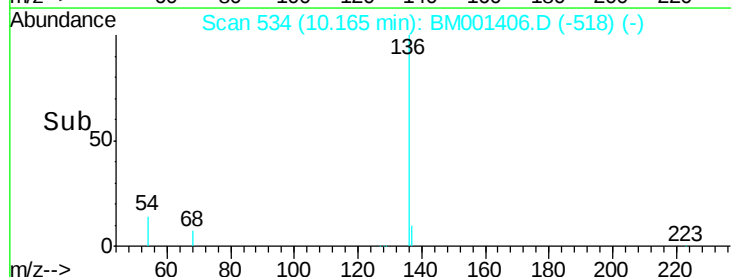

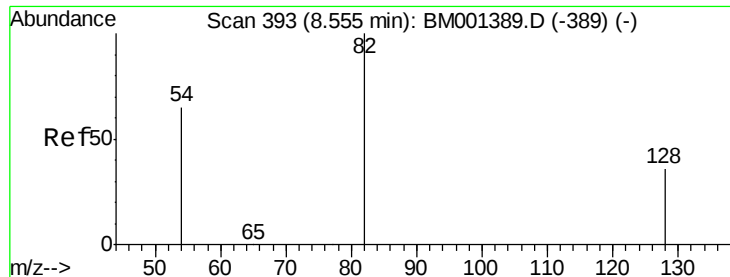

#7

Nitrobenzene-d5

Concen: 6.52 ng

RT: 8.55 min Scan# 393

Delta R.T. 0.00 min

Lab File: BM001406.D

Acq: 23 May 2015 06:24

Instrument :

BNA_M

ClientSampleId :

RAV-GT-106


Tgt Ion: 82 Resp: 13656

Ion Ratio Lower Upper

82 100

128 42.6 30.2 45.4

54 52.8 52.9 79.3#


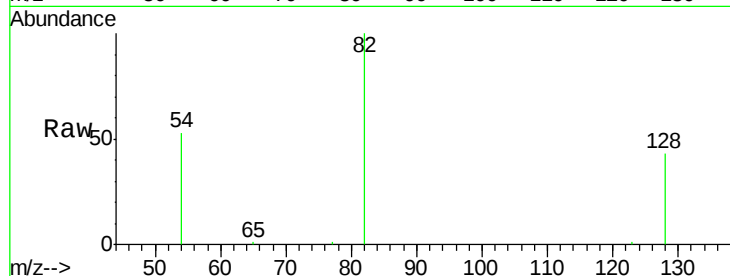


Abundance Ion 82.00 (81.70 to 82.70): BM001389.D (-389) (-)

Ion 128.00 (127.70 to 128.70): BM001389.D (-389) (-)

Ion 54.00 (53.70 to 54.70): BM001389.D (-389) (-)

Time-->

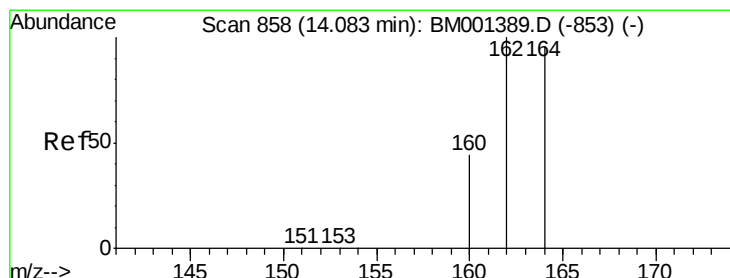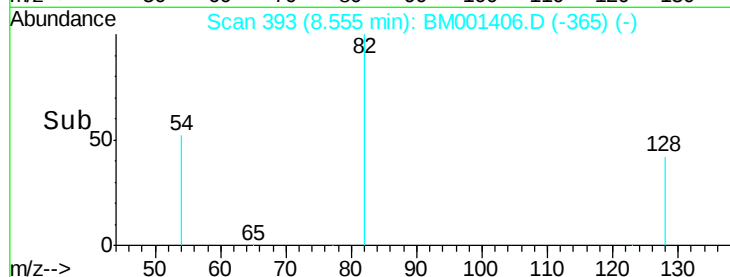

#12

Acenaphthene-d10

Concen: 5.00 ng

RT: 14.08 min Scan# 858

Delta R.T. 0.00 min

Lab File: BM001406.D

Acq: 23 May 2015 06:24


Tgt Ion: 164 Resp: 21250

Ion Ratio Lower Upper

164 100

162 98.2 83.4 125.2

160 41.2 36.9 55.3

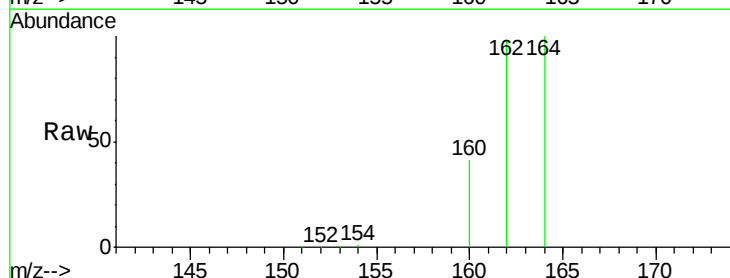



Abundance Ion 164.00 (163.70 to 164.70): BM001389.D (-853) (-)

Ion 162.00 (161.70 to 162.70): BM001389.D (-853) (-)

Ion 160.00 (159.70 to 160.70): BM001389.D (-853) (-)

Time-->

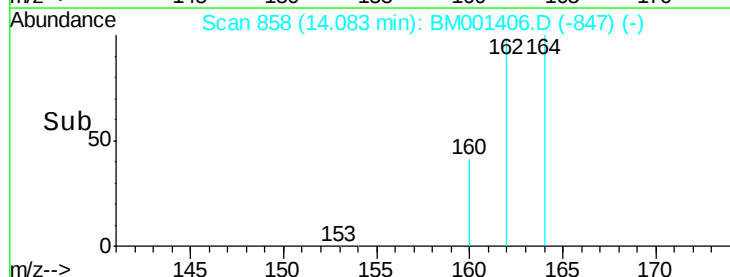


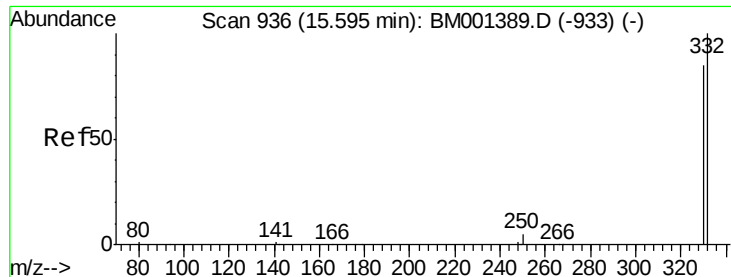




#13
 2,4,6-Tribromophenol
 Concen: 8.82 ng
 RT: 15.59 min Scan# 936
 Delta R.T. 0.00 min
 Lab File: BM001406.D
 Acq: 23 May 2015 06:24

Instrument :
 BNA_M
 ClientSampleId :
 RAV-GT-106

Tgt Ion:330 Resp: 5825
 Ion Ratio Lower Upper
 330 100
 332 106.6 90.3 135.5
 141 0.0 0.0 0.0

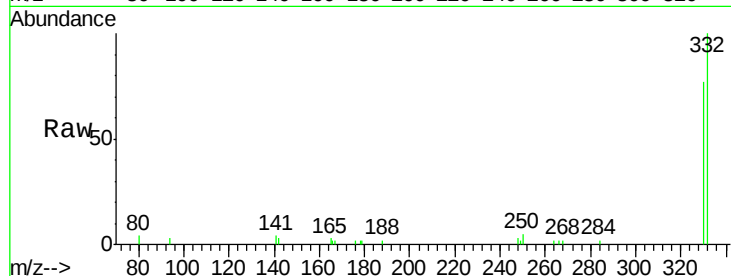


Abundance Ion 329.80 (329.50 to 330.50): E
 Ion 331.80 (331.50 to 332.50): E
 Ion 141.00 (140.70 to 141.70): E

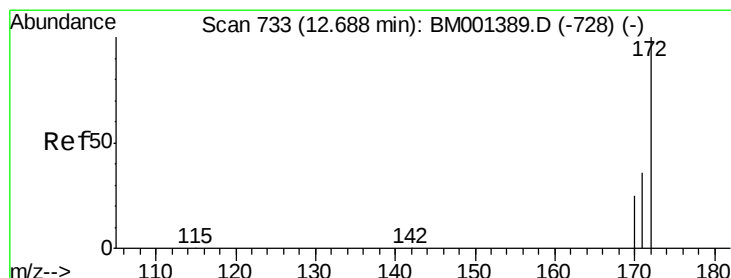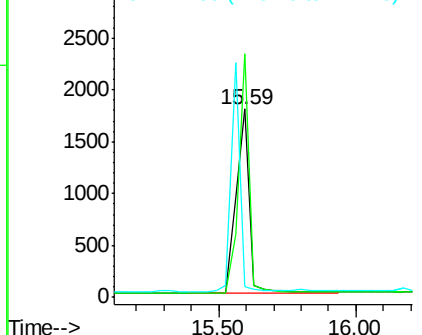
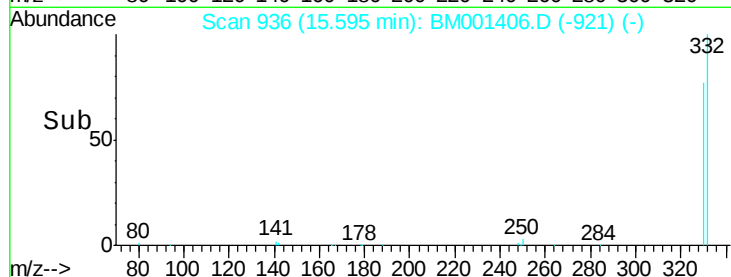



#14
 2-Fluorobiphenyl
 Concen: 6.93 ng
 RT: 12.69 min Scan# 733
 Delta R.T. 0.00 min
 Lab File: BM001406.D
 Acq: 23 May 2015 06:24

Tgt Ion:172 Resp: 45328
 Ion Ratio Lower Upper
 172 100
 171 33.5 29.4 44.0
 170 21.3 20.2 30.4

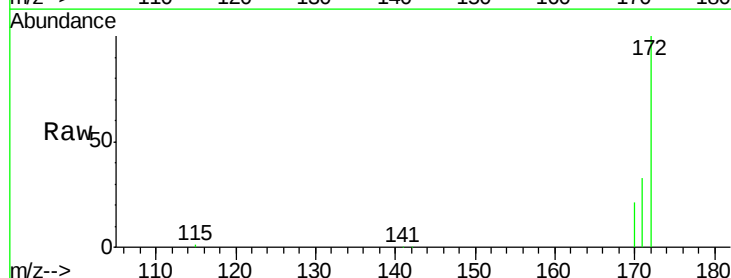

Abundance Ion 172.00 (171.70 to 172.70): E
 Ion 171.00 (170.70 to 171.70): E
 Ion 170.00 (169.70 to 170.70): E



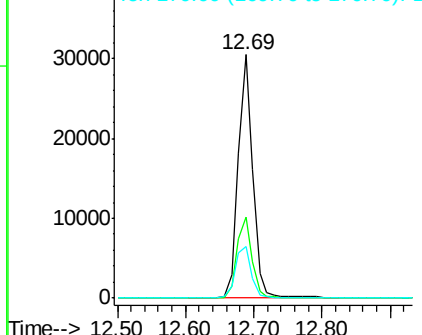
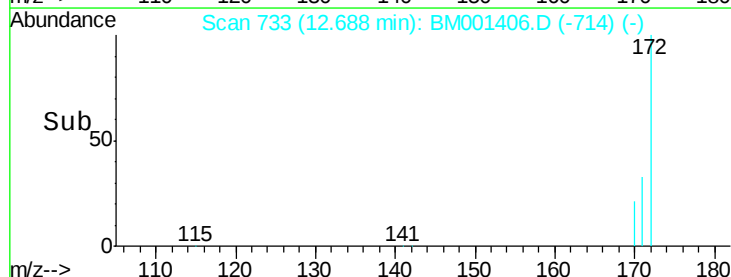


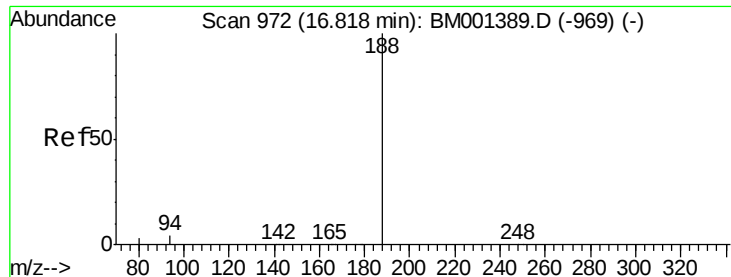

#18
Phenanthrene-d10
Concen: 5.00 ng
RT: 16.82 min Scan# 972
Delta R.T. 0.00 min
Lab File: BM001406.D
Acq: 23 May 2015 06:24




Instrument :
BNA_M
ClientSampleId :
RAV-GT-106


Tgt Ion:188 Resp: 74055
Ion Ratio Lower Upper
188 100
94 1.9 3.0 4.4#
80 1.6 2.5 3.7#

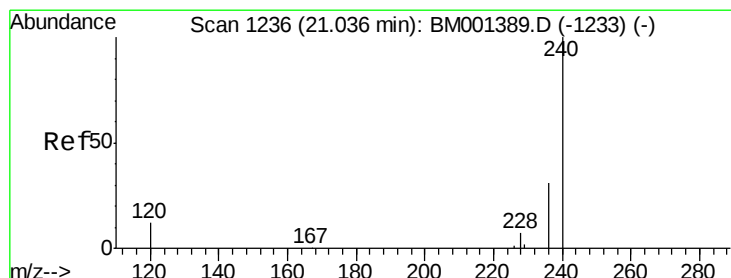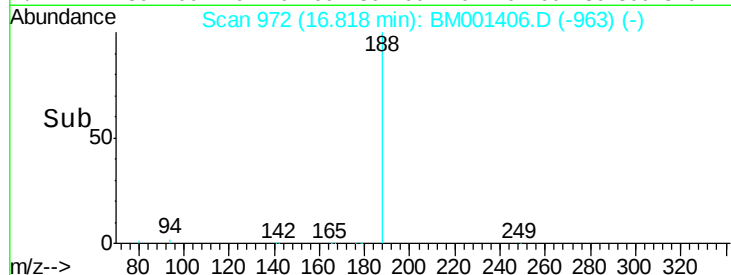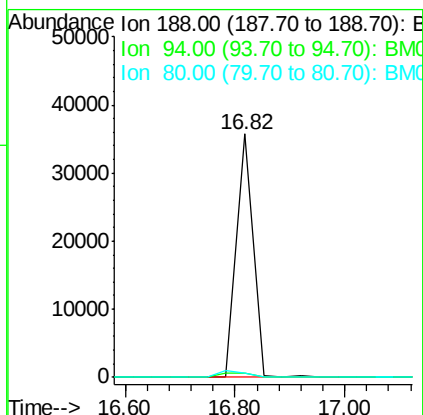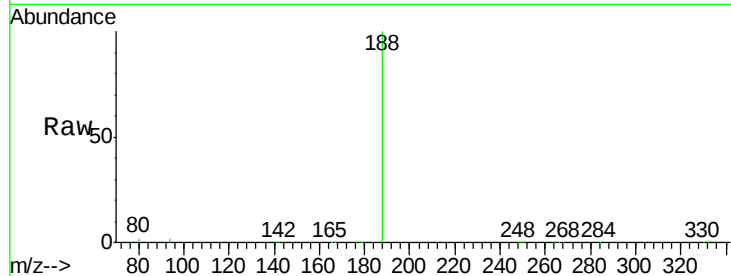

#25
Chrysene-d12
Concen: 5.00 ng
RT: 21.04 min Scan# 1236
Delta R.T. 0.00 min
Lab File: BM001406.D
Acq: 23 May 2015 06:24

Tgt Ion:240 Resp: 44845
Ion Ratio Lower Upper
240 100
120 3.6 9.7 14.5#
236 25.7 24.8 37.2

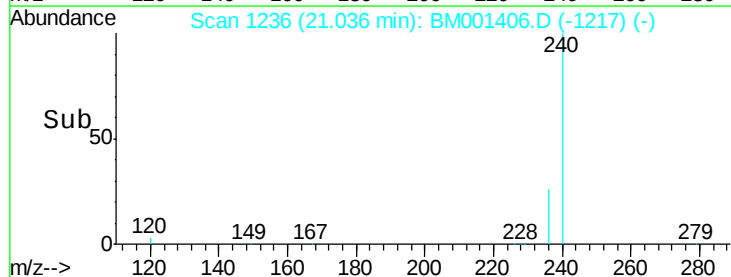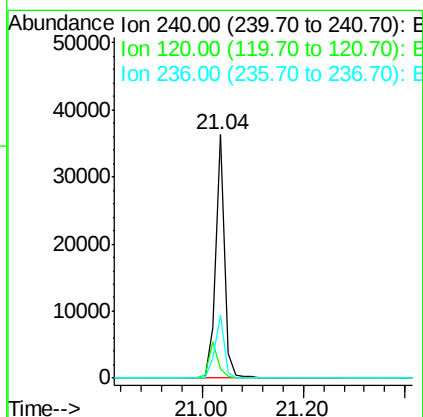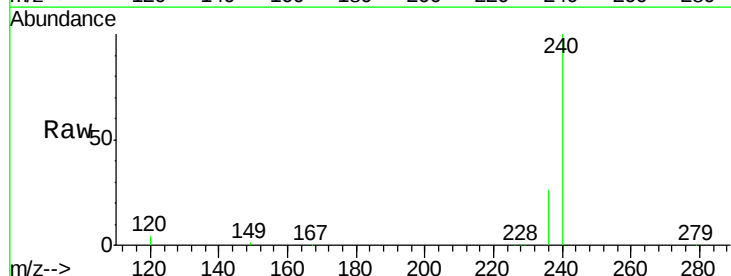

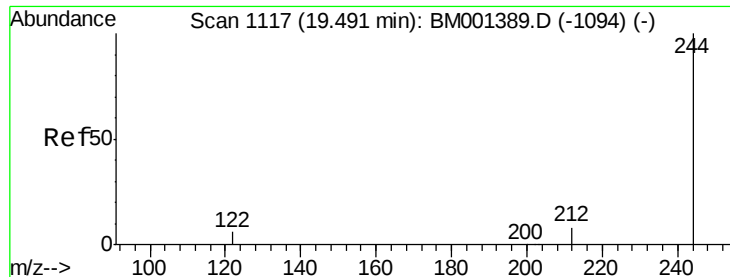

#27

Terphenyl-d14

Concen: 8.32 ng

RT: 19.48 min Scan# 1116

Delta R.T. -0.01 min

Lab File: BM001406.D

Acq: 23 May 2015 06:24

Instrument :

BNA_M

ClientSampleId :

RAV-GT-106


Tgt Ion:244 Resp: 50488

Ion Ratio Lower Upper

244 100

212 10.2 7.2 10.8




122 13.3 5.1 7.7#

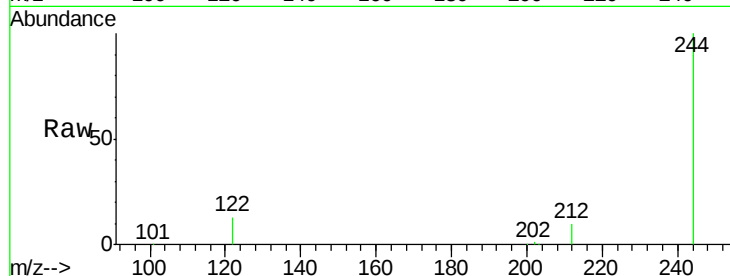

Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

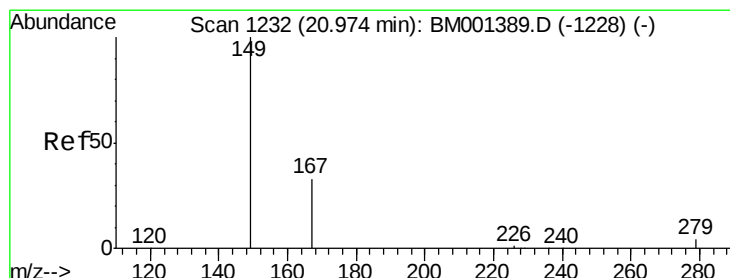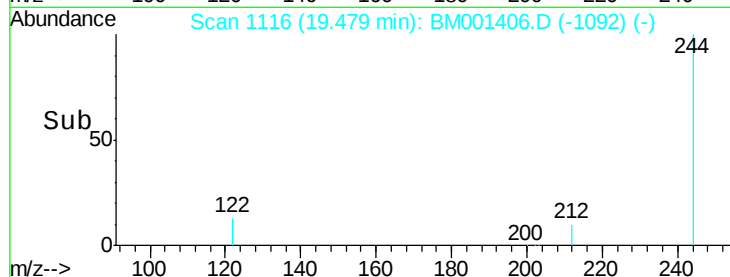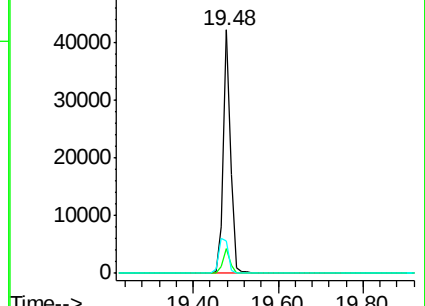

#30

Bis(2-ethylhexyl)phthalate

Concen: 0.23 ng

RT: 20.96 min Scan# 1231

Delta R.T. -0.02 min

Lab File: BM001406.D

Acq: 23 May 2015 06:24


Tgt Ion:149 Resp: 1623

Ion Ratio Lower Upper

149 100

167 23.2 21.0 31.6



279 2.5 2.2 3.2

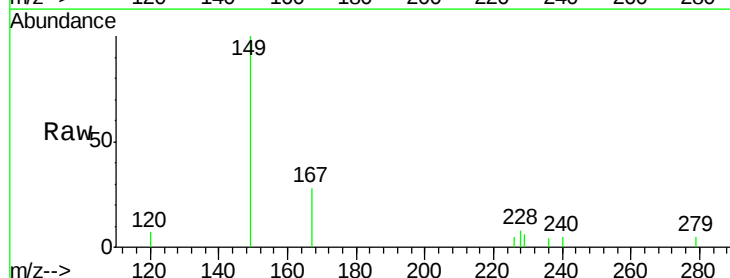


Abundance Ion 149.00 (148.70 to 149.70): E

Ion 167.00 (166.70 to 167.70): E

Ion 279.00 (278.70 to 279.70): E

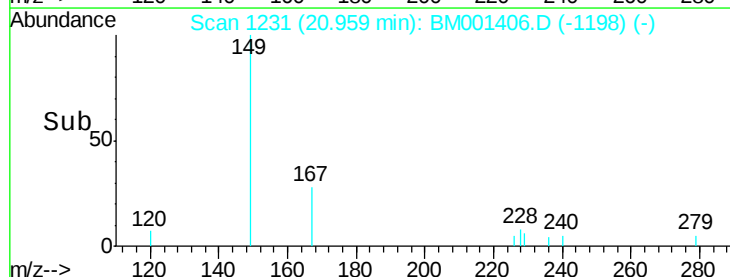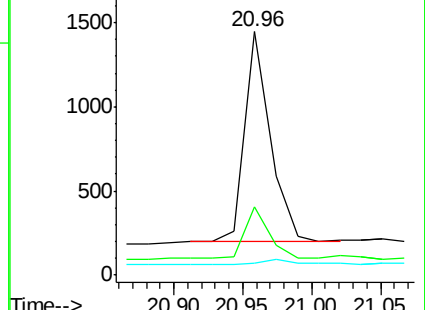

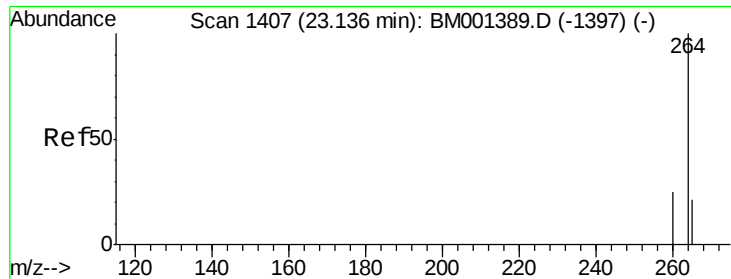

#32

Perylene-d12

Concen: 5.00 ng

RT: 23.13 min Scan# 1406

Delta R.T. -0.01 min

Lab File: BM001406.D


Acq: 23 May 2015 06:24

Instrument :

BNA_M

ClientSampleId :

RAV-GT-106

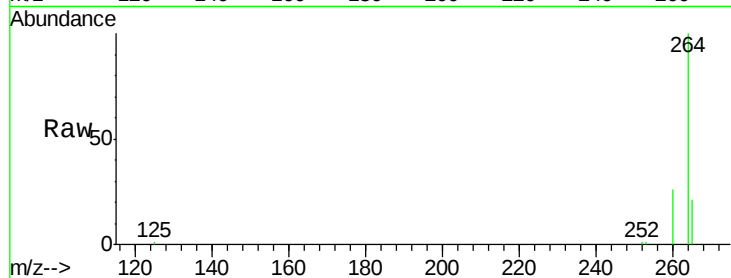

Tgt Ion: 264 Resp: 38118

Ion Ratio Lower Upper

264 100

260 26.0 20.1 30.1

265 21.3 17.1 25.7

