


Data Path : Z:\HPCHEM1\BNA_M\DATA\BM052215\
 Data File : BM001383.D
 Acq On : 22 May 2015 14:29
 Operator : TP/IZ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF043015.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed May 20 05:08:22 2015

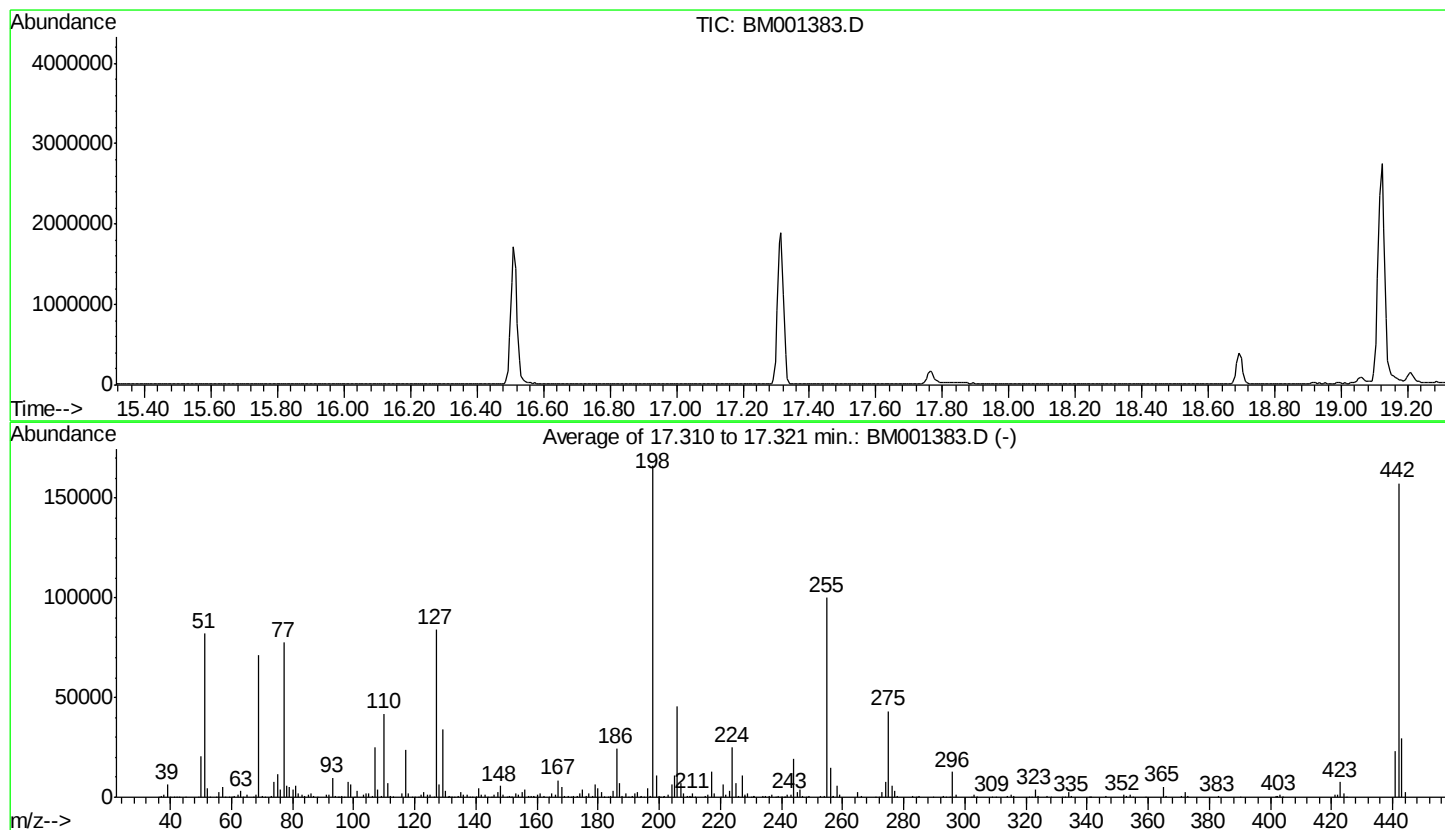

AutoFind: Scans 2486, 2487, 2488; Background Corrected with Scan 2479

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	49.3	81944	PASS
68	69	0.00	2	1.5	1077	PASS
69	198	0.00	100	42.9	71313	PASS
70	69	0.00	2	0.6	425	PASS
127	198	10	80	50.4	83856	PASS
197	198	0.00	2	0.6	951	PASS
198	198	100	100	100.0	166333	PASS
199	198	5	9	6.7	11081	PASS
275	198	10	60	26.0	43221	PASS
365	198	1	100	3.2	5370	PASS
441	442	0.01	24	14.9	23450	PASS
442	198	50	100	94.6	157312	PASS
443	442	15	24	18.8	29517	PASS