


Data Path : Z:\HPCHEM1\BNA_M\DATA\BM052215\
 Data File : BM001394.D
 Acq On : 22 May 2015 22:40
 Operator : TP/IZ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF043015.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed May 20 05:08:22 2015

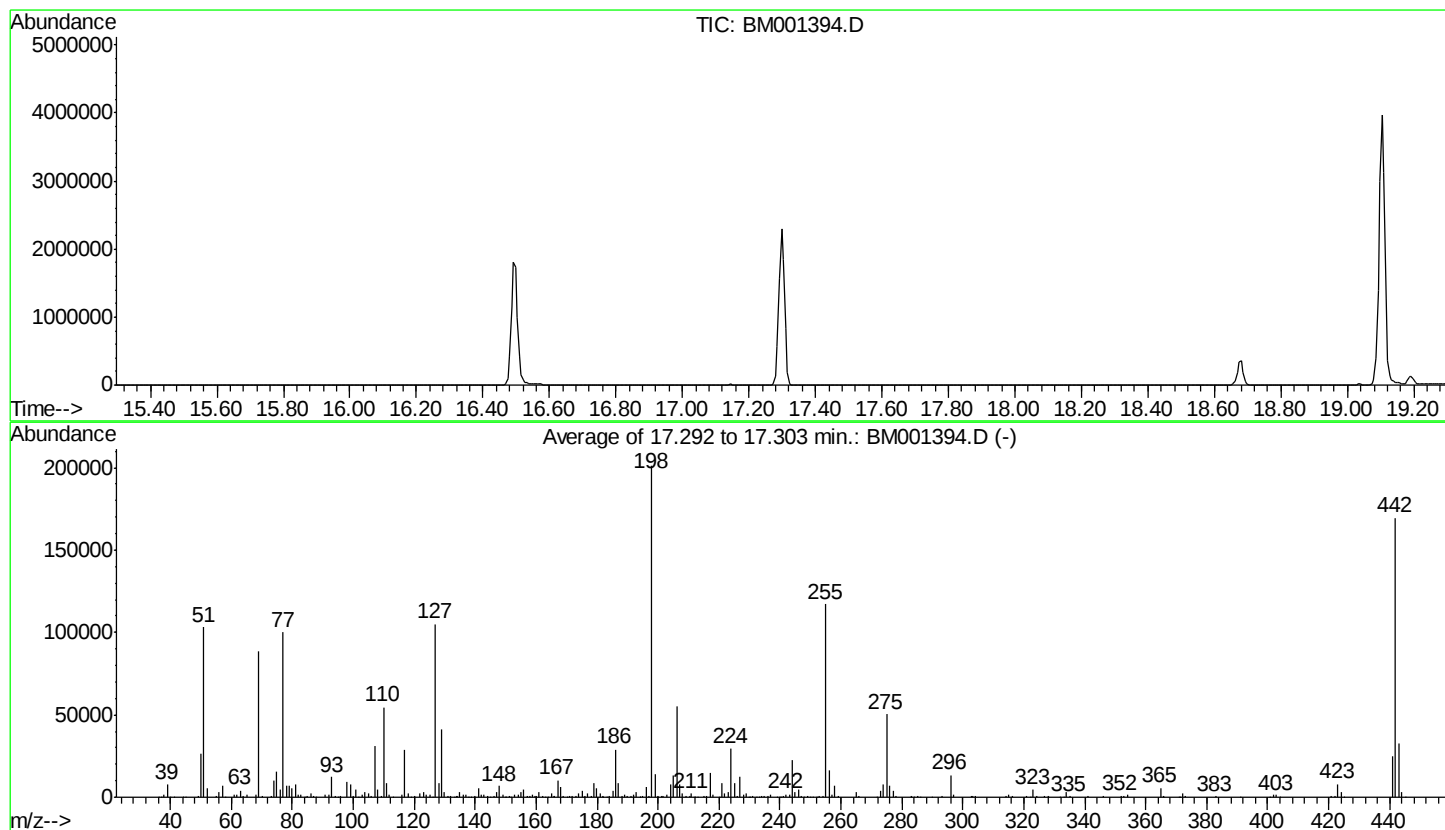

AutoFind: Scans 2483, 2484, 2485; Background Corrected with Scan 2477

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	51.3	103245	PASS
68	69	0.00	2	1.6	1462	PASS
69	198	0.00	100	44.2	88858	PASS
70	69	0.00	2	0.6	545	PASS
127	198	10	80	52.3	105208	PASS
197	198	0.00	2	0.5	1089	PASS
198	198	100	100	100.0	201216	PASS
199	198	5	9	6.9	13918	PASS
275	198	10	60	25.0	50325	PASS
365	198	1	100	2.9	5775	PASS
441	442	0.01	24	14.6	24763	PASS
442	198	50	100	84.3	169629	PASS
443	442	15	24	19.2	32613	PASS