

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM052216\
 Data File : BM005585.D
 Acq On : 22 May 2016 14:10
 Operator : UM/SJ
 Sample : H3087-01
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 JHGH0

Quant Time: May 23 05:32:33 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM052016.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon May 23 05:32:02 2016
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.81	152	38854	20.00	ng/ul	0.00
18) Naphthalene-d8	10.60	136	192611	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.44	164	128148	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.19	188	325711	20.00	ng/ul	0.00
75) Chrysene-d12	21.36	240	470206	20.00	ng/ul	0.00
83) Perylene-d12	23.64	264	530852	20.00	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.29	96	2855	3.22	ng/uL	0.00
5) Phenol-d5	6.98	99	68688	21.57	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.15	67	42023	22.77	ng/ul	0.00
9) 2-Chlorophenol-d4	7.35	132	56001	21.08	ng/ul	0.00
13) 4-Methylphenol-d8	8.52	113	57721	22.12	ng/ul	0.00
19) Nitrobenzene-d5	8.97	128	29296	19.89	ng/ul	0.00
22) 2-Nitrophenol-d4	9.69	143	33985	20.96	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.22	165	62253	20.39	ng/ul	0.00
29) 4-Chloroaniline-d4	10.74	131	82496	26.98	ng/ul	0.00
43) Dimethylphthalate-d6	13.85	166	238392	22.79	ng/ul	0.00
46) Acenaphthylene-d8	14.14	160	278175	21.27	ng/ul	0.00
51) 4-Nitrophenol-d4	14.64	143	41709	21.08	ng/ul	0.00
57) Fluorene-d10	15.44	176	210348	23.11	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.55	200	31420	16.77	ng/ul	0.00
70) Anthracene-d10	17.29	188	341703	22.02	ng/ul	0.00
76) Pyrene-d10	19.57	212	435993	20.48	ng/ul	0.00
87) Benzo(a)pyrene-d12	23.49	264	537020	21.66	ng/ul	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
44) Dimethylphthalate	13.90	163	85800	8.30	ng/ul	100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM052216\
Data File : BM005585.D
Acq On : 22 May 2016 14:10
Operator : UM/SJ
Sample : H3087-01
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
JHGH0

Quant Time: May 23 05:32:33 2016
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM052016.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon May 23 05:32:02 2016
Response via : Initial Calibration

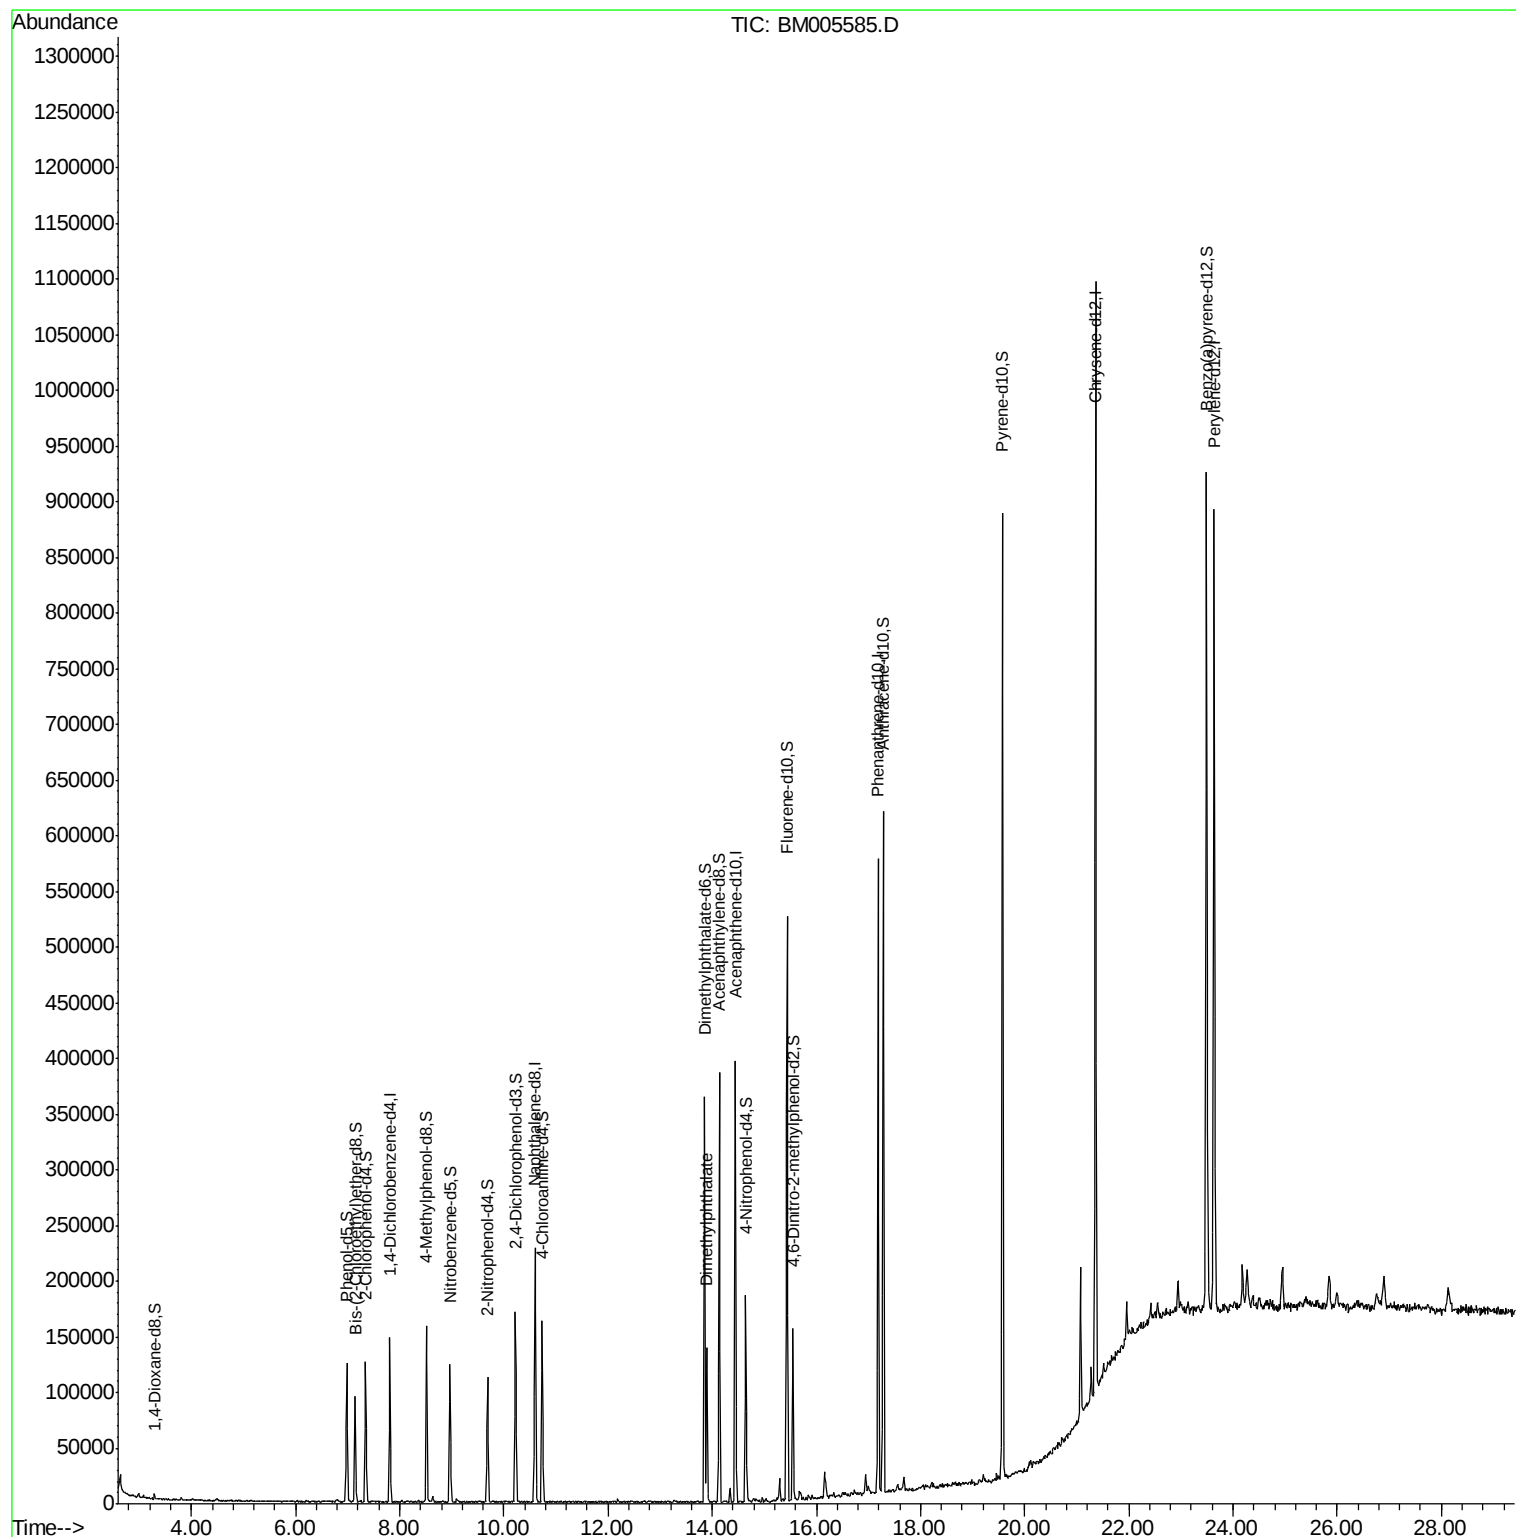

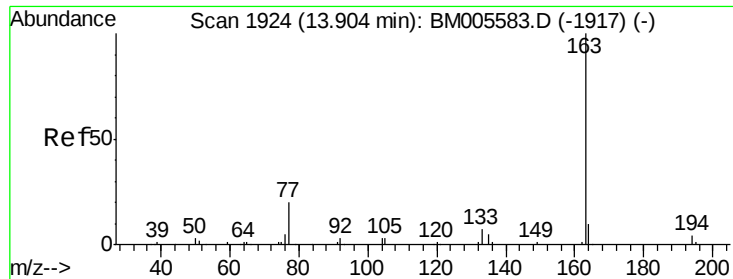

#44

Dimethylphthalate

Concen: 8.30 ng/ul

RT: 13.90 min Scan# 1923

Delta R.T. -0.01 min

Lab File: BM005585.D


Acq: 22 May 2016 14:10

Instrument :

BNA_M

ClientSampleId :

JHGH0

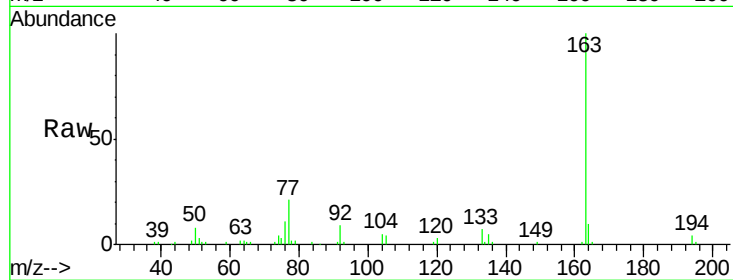

Tgt Ion:	163	Resp:	85800
Ion	Ratio	Lower	Upper
163	100		
194	4.0	3.4	5.0
164	9.9	8.0	12.0

