

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM052216\
 Data File : BM005586.D
 Acq On : 22 May 2016 14:47
 Operator : UM/SJ
 Sample : H3087-02
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 JHGH1

Quant Time: May 23 05:32:41 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM052016.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon May 23 05:32:02 2016
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.81	152	29729	20.00	ng/ul	0.00
18) Naphthalene-d8	10.60	136	149751	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.44	164	101928	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.19	188	266639	20.00	ng/ul	0.00
75) Chrysene-d12	21.36	240	404167	20.00	ng/ul	0.00
83) Perylene-d12	23.64	264	461791	20.00	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.29	96	2750	4.05	ng/uL	0.00
5) Phenol-d5	6.98	99	67111	27.54	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.15	67	43049	30.48	ng/ul	0.00
9) 2-Chlorophenol-d4	7.35	132	56875	27.98	ng/ul	0.00
13) 4-Methylphenol-d8	8.52	113	62115	31.11	ng/ul	0.00
19) Nitrobenzene-d5	8.97	128	30601	26.73	ng/ul	0.00
22) 2-Nitrophenol-d4	9.69	143	34488	27.36	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.22	165	62085	26.16	ng/ul	0.00
29) 4-Chloroaniline-d4	10.74	131	93064	39.15	ng/ul	0.00
43) Dimethylphthalate-d6	13.85	166	244454	29.38	ng/ul	0.00
46) Acenaphthylene-d8	14.14	160	282973	27.20	ng/ul	0.00
51) 4-Nitrophenol-d4	14.64	143	15651	9.94	ng/ul	0.00
57) Fluorene-d10	15.43	176	213899	29.55	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.55	200	13343	8.70	ng/ul	0.00
70) Anthracene-d10	17.29	188	358916	28.26	ng/ul	0.00
76) Pyrene-d10	19.57	212	466631	25.49	ng/ul	0.00
87) Benzo(a)pyrene-d12	23.49	264	601064	27.87	ng/ul	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
44) Dimethylphthalate	13.90	163	50077	6.09	ng/ul	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM052216\
Data File : BM005586.D
Acq On : 22 May 2016 14:47
Operator : UM/SJ
Sample : H3087-02
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
JHGH1

Quant Time: May 23 05:32:41 2016
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM052016.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon May 23 05:32:02 2016
Response via : Initial Calibration

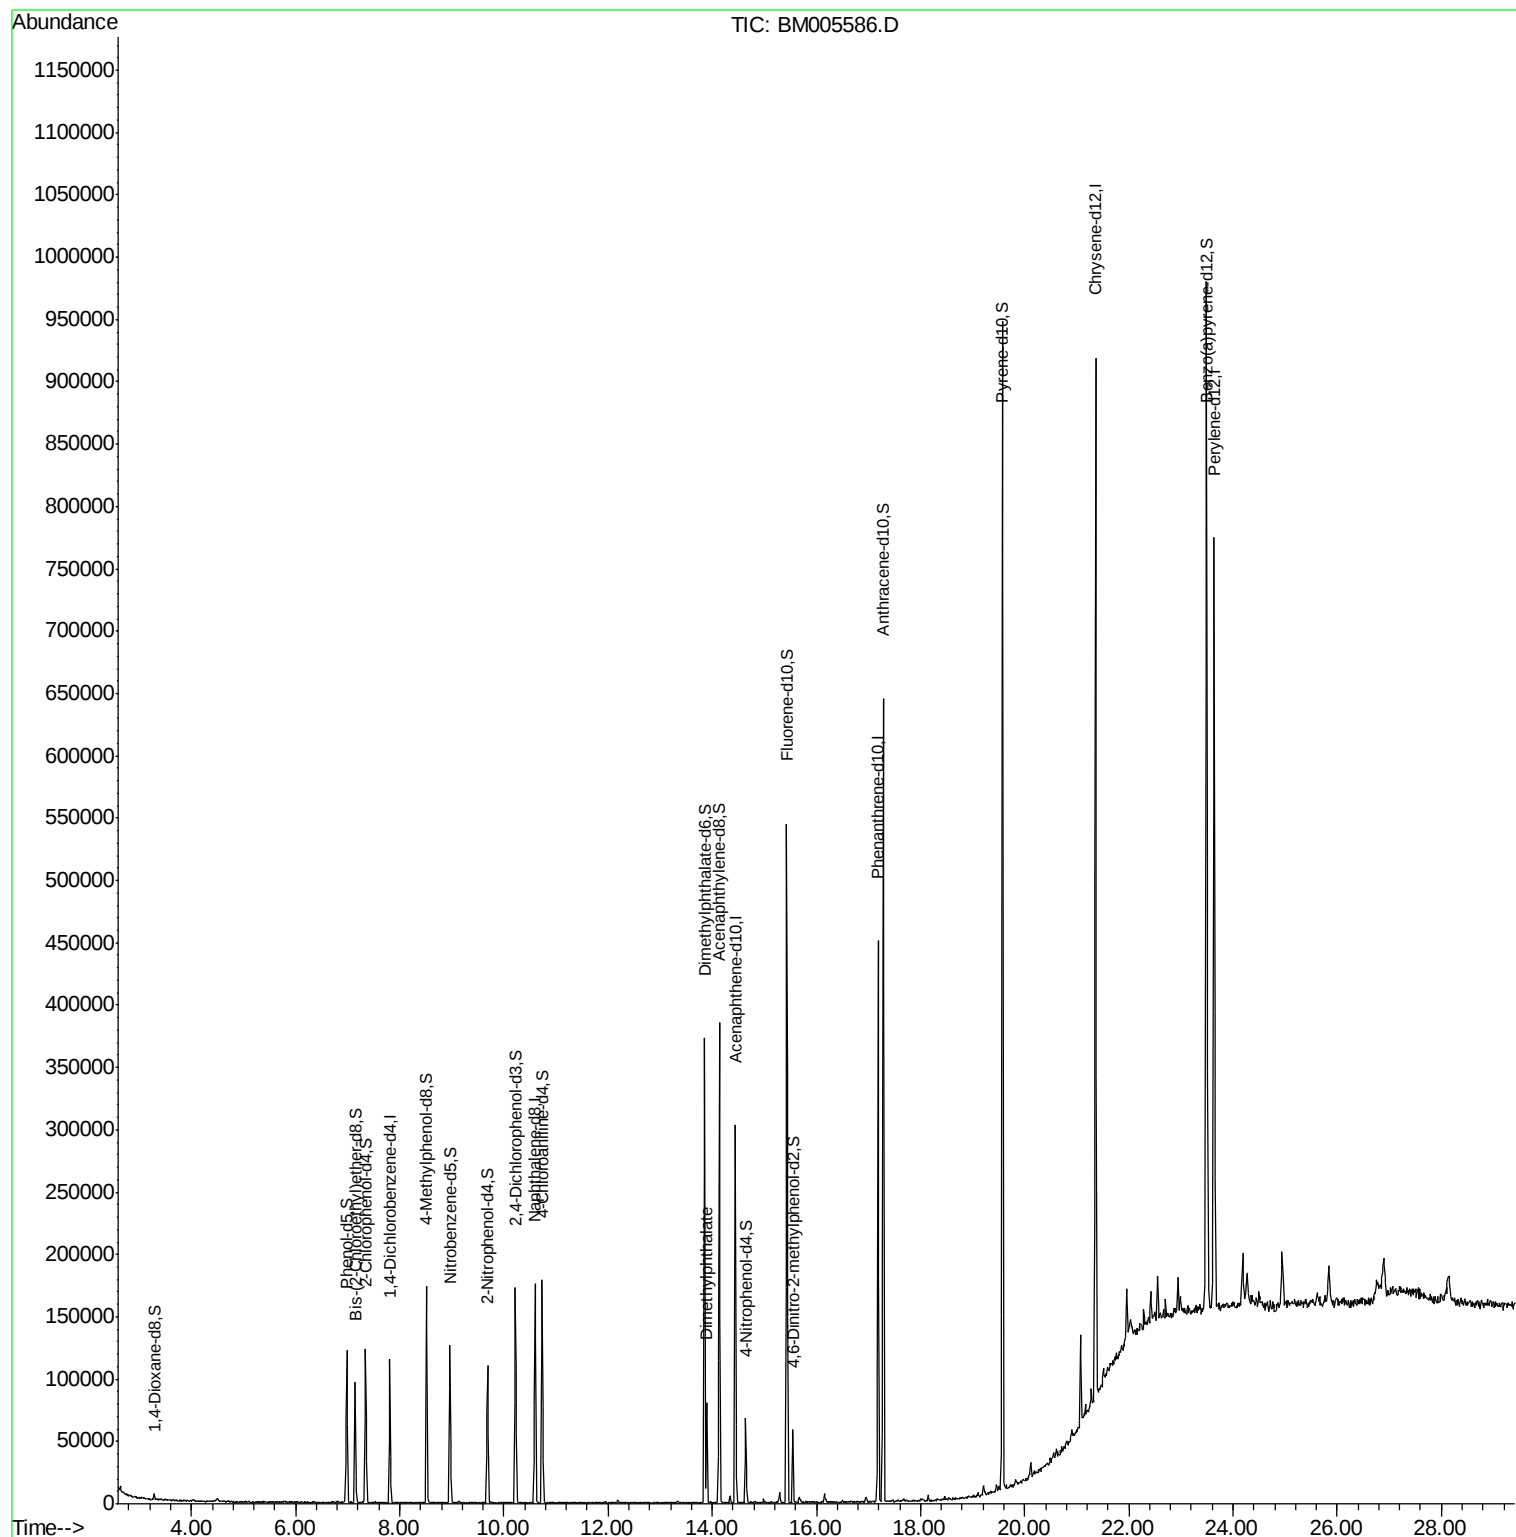


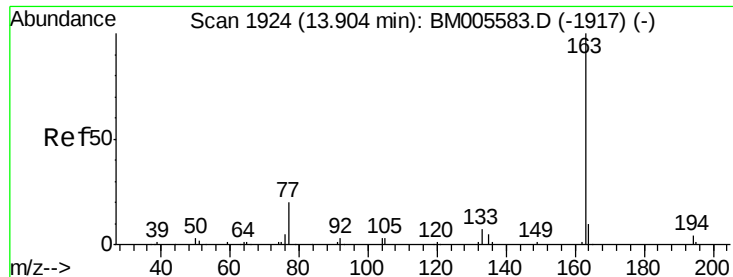

#44
 Dimethylphthalate
 Concen: 6.09 ng/ul
 RT: 13.90 min Scan# 1923
 Delta R.T. -0.01 min
 Lab File: BM005586.D
 Acq: 22 May 2016 14:47

Instrument :
 BNA_M
 ClientSampleId :
 JHGH1

Tgt Ion:	163	Resp:	50077
Ion	Ratio	Lower	Upper
163	100		
194	3.8	3.4	5.0
164	9.8	8.0	12.0

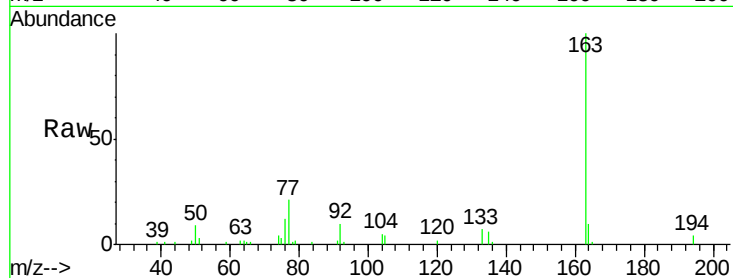

Abundance Ion 163.00 (162.70 to 163.70): E
 Ion 194.00 (193.70 to 194.70): E
 Ion 164.00 (163.70 to 164.70): E

