

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM052216\
 Data File : BM005602.D
 Acq On : 23 May 2016 00:30
 Operator : UM/SJ
 Sample : H3124-03
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 JHGG0

Manual Integrations
 APPROVED

umangi
 5/23/2016 8:36:02 PM

Quant Time: May 23 07:58:04 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM052016.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon May 23 05:32:02 2016
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.82	152	173524	20.00	ng/ul	0.01
18) Naphthalene-d8	10.61	136	757400	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.46	164	399283	20.00	ng/ul	0.01
61) Phenanthrene-d10	17.20	188	855932	20.00	ng/ul	0.02
75) Chrysene-d12	21.38	240	768052	20.00	ng/ul	0.02
83) Perylene-d12	23.67	264	698995	20.00	ng/ul	0.03

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.29	96	14333	3.62	ng/uL	0.00
5) Phenol-d5	7.00	99	356430	25.06	ng/ul	0.02
7) Bis-(2-Chloroethyl)ether-d	7.15	67	207186	25.14	ng/ul	0.00
9) 2-Chlorophenol-d4	7.36	132	294033	24.78	ng/ul	0.01
13) 4-Methylphenol-d8	8.53	113	287963	24.71	ng/ul	0.02
19) Nitrobenzene-d5	8.97	128	144754	25.00	ng/ul	0.00
22) 2-Nitrophenol-d4	9.70	143	155043	24.32	ng/ul	0.01
26) 2,4-Dichlorophenol-d3	10.24	165	287041	23.91	ng/ul	0.01
29) 4-Chloroaniline-d4	10.75	131	285464	23.74	ng/ul	0.01
43) Dimethylphthalate-d6	13.86	166	800353	24.56	ng/ul	0.00
46) Acenaphthylene-d8	14.15	160	1049068	25.75	ng/ul	0.01
51) 4-Nitrophenol-d4	14.67	143	127930	20.75	ng/ul	0.02
57) Fluorene-d10	15.45	176	719022	25.35	ng/ul	0.01
62) 4,6-Dinitro-2-methylphenol	15.57	200	33073	6.72	ng/ul	0.02
70) Anthracene-d10	17.30	188	1096339	26.89	ng/ul	0.02
76) Pyrene-d10	19.59	212	1159619	33.34	ng/ul	0.02
87) Benzo(a)pyrene-d12	23.52	264	850857	26.07	ng/ul	0.02

Target Compounds

					Qvalue
28) Naphthalene	10.66	128	177645	4.67 ng/ul	100
34) 2-Methylnaphthalene	12.27	142	117660	4.23 ng/ul	99
40) 1,1'-Biphenyl	13.29	154	45814	1.37 ng/ul	99
44) Dimethylphthalate	13.91	163	166810	5.18 ng/ul#	97
47) Acenaphthylene	14.18	152	193733	4.68 ng/ul	94
49) Acenaphthene	14.52	153	79123	2.90 ng/ul	99
53) Dibenzofuran	14.86	168	80219	2.06 ng/ul	91
58) Fluorene	15.50	166	210036	6.73 ng/ul	98
69) Phenanthrene	17.24	178	2047978	42.81 ng/ul	98
71) Anthracene	17.33	178	546388	11.21 ng/ul	98
72) Carbazole	17.60	167	99574	2.35 ng/ul#	78
74) Fluoranthene	19.26	202	2334878	43.36 ng/ul	99
77) Pyrene	19.63	202	2588865	58.63 ng/ul	98
80) Benzo(a)anthracene	21.36	228	937477m	20.77 ng/ul	
82) Chrysene	21.41	228	981769	22.86 ng/ul	96
85) Benzo(b)fluoranthene	22.98	252	911538	22.11 ng/ul#	86
86) Benzo(k)fluoranthene	23.01	252	253957m	6.51 ng/ul	
88) Benzo(a)pyrene	23.57	252	815584	20.39 ng/ul#	95
89) Indeno(1,2,3-cd)pyrene	25.99	276	506631	10.67 ng/ul	99
90) Dibenzo(a,h)anthracene	25.99	278	112583	2.85 ng/ul#	69
91) Benzo(g,h,i)perylene	26.70	276	493111	12.35 ng/ul	93

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM052216\
Data File : BM005602.D
Acq On : 23 May 2016 00:30
Operator : UM/SJ
Sample : H3124-03
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
JHGG0

Manual Integrations
APPROVED

umangi
5/23/2016 8:36:02 PM

Quant Time: May 23 07:58:04 2016
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM052016.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon May 23 05:32:02 2016
Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
--------------------	------	------	----------	------	-------	----------

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\HPCHEM1\BNA_M\DATA\BM052216\
Data File : BM005602.D
Acq On : 23 May 2016 00:30
Operator : UM/SJ
Sample : H3124-03
Misc :
ALS Vial : 20 Sample Multiplier: 1


Instrument :
BNA_M
ClientSampleId :
JHGG0

Manual Integrations
APPROVED

umangi
5/23/2016 8:36:02 PM

Quant Time: May 23 07:58:04 2016
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM052016.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon May 23 05:32:02 2016
Response via : Initial Calibration

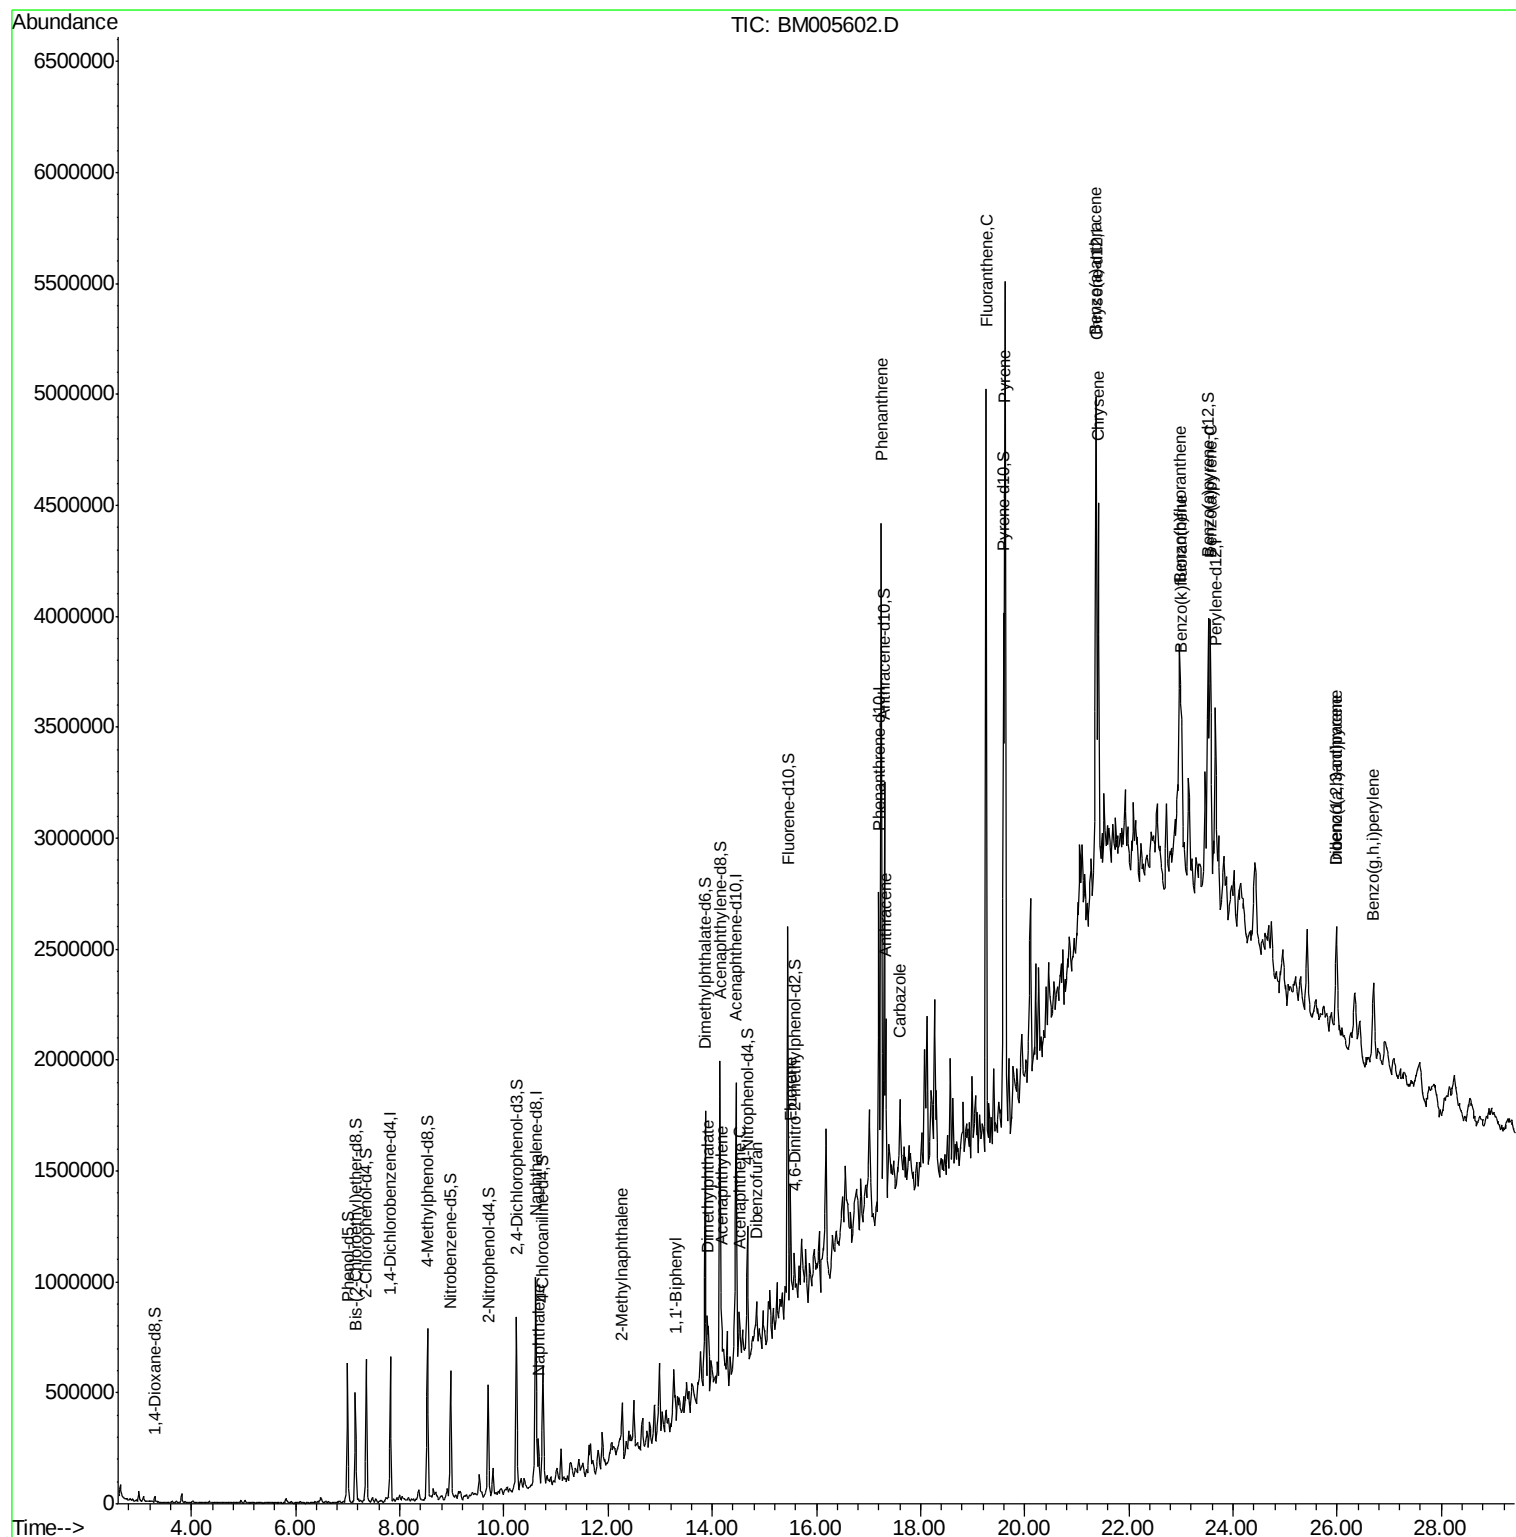

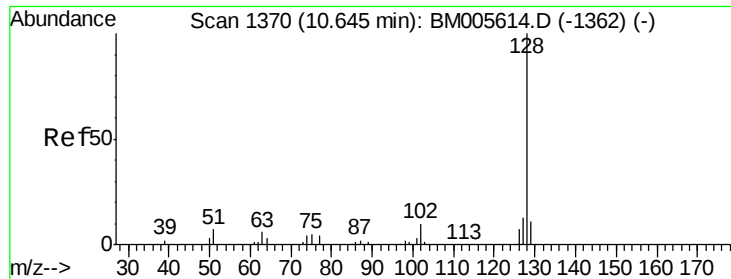





#28
Naphthalene
Concen: 4.67 ng/ul
RT: 10.66 min Scan# 1373
Delta R.T. 0.01 min
Lab File: BM005602.D
Acq: 23 May 2016 00:30

Instrument :
BNA_M
ClientSampleId :
JHGG0

Tgt Ion	Ratio	Resp	Lower	Upper
128	100	177645		
129	10.9	8.6	13.0	
127	13.2	10.6	15.8	




Manual Integrations
APPROVED


umangi
5/23/2016 8:36:02 PM

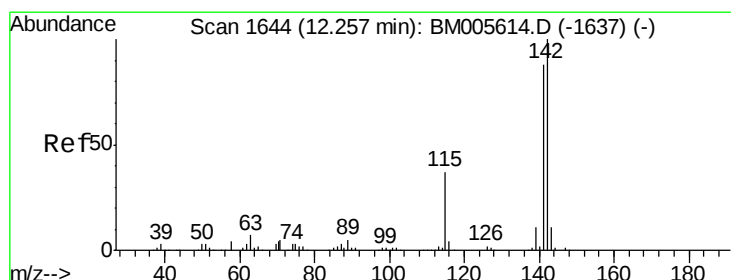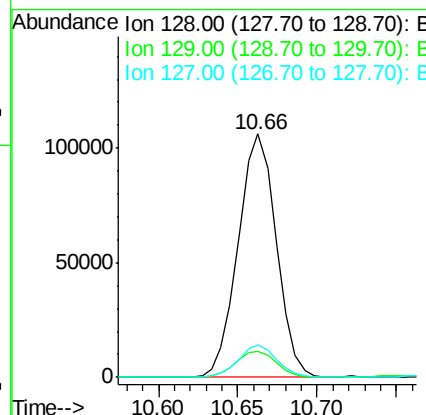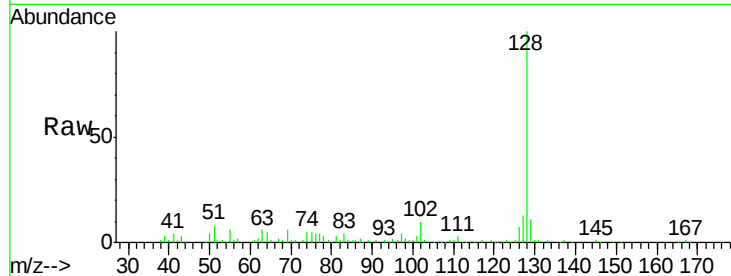

#34
2-Methylnaphthalene
Concen: 4.23 ng/ul
RT: 12.27 min Scan# 1647
Delta R.T. 0.01 min
Lab File: BM005602.D
Acq: 23 May 2016 00:30


Tgt Ion	Ratio	Resp	Lower	Upper
142	100	117660		
141	89.1	70.6	106.0	

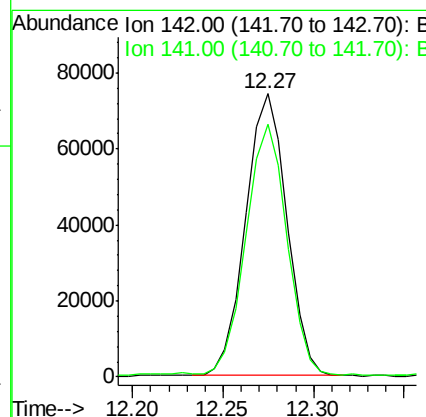

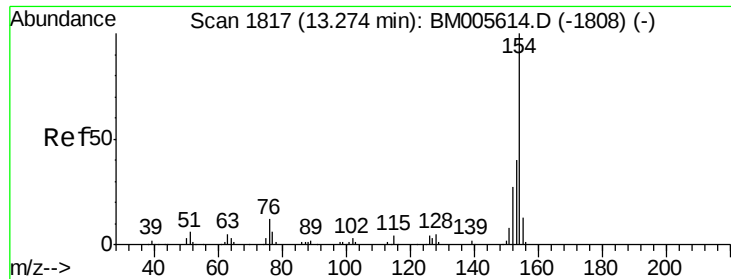

#40
1,1'-Biphenyl
Concen: 1.37 ng/ul
RT: 13.29 min Scan# 1819
Delta R.T. 0.01 min
Lab File: BM005602.D
Acq: 23 May 2016 00:30




Instrument :
BNA_M
ClientSampleId :
JHGG0



Tgt Ion	Ratio	Lower	Upper
154	100		
153	40.0	31.7	47.5
76	12.7	10.1	15.1




Manual Integrations
APPROVED


umangi
5/23/2016 8:36:02 PM

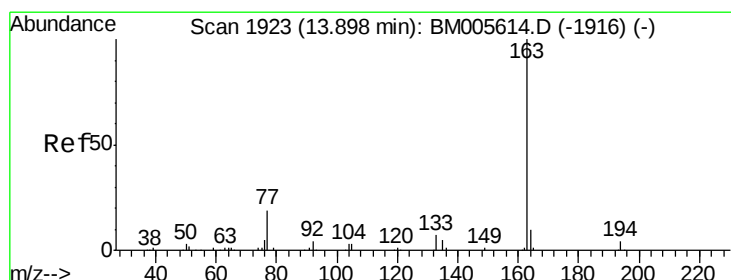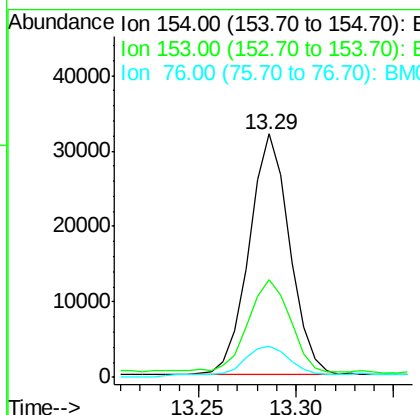

#44
Dimethylphthalate
Concen: 5.18 ng/ul
RT: 13.91 min Scan# 1925
Delta R.T. 0.01 min
Lab File: BM005602.D
Acq: 23 May 2016 00:30

Tgt Ion	Ratio	Lower	Upper
163	100		
194	5.3	3.4	5.0#
164	11.1	8.0	12.0

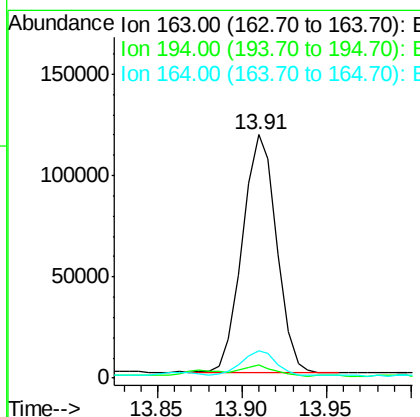

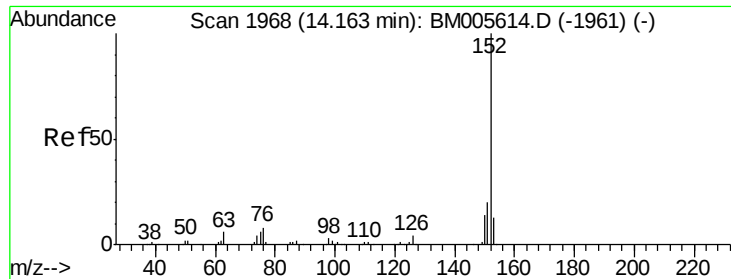





#47
Acenaphthylene
Concen: 4.68 ng/ul
RT: 14.18 min Scan# 1971
Delta R.T. 0.01 min
Lab File: BM005602.D
Acq: 23 May 2016 00:30

Instrument :
BNA_M
ClientSampleId :
JHGG0

Tgt Ion	Ratio	Resp	Lower	Upper
152	100	193733		
151	22.3		15.7	23.5
153	15.6		10.5	15.7




Manual Integrations
APPROVED


umangi
5/23/2016 8:36:02 PM

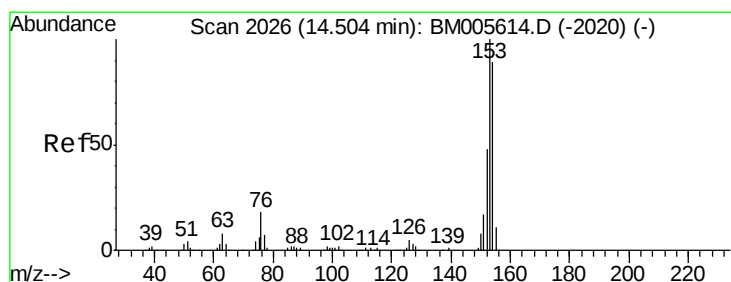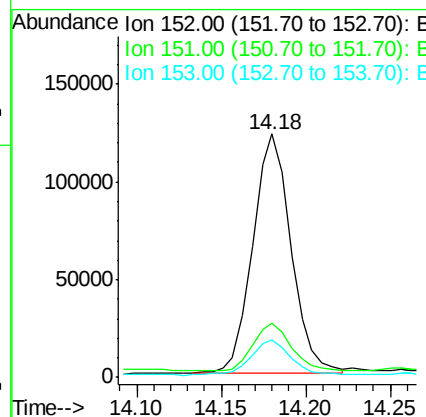

#49
Acenaphthene
Concen: 2.90 ng/ul
RT: 14.52 min Scan# 2029
Delta R.T. 0.01 min
Lab File: BM005602.D
Acq: 23 May 2016 00:30

Tgt Ion	Ratio	Resp	Lower	Upper
153	100	79123		
152	47.8		37.8	56.6
154	88.4		71.1	106.7

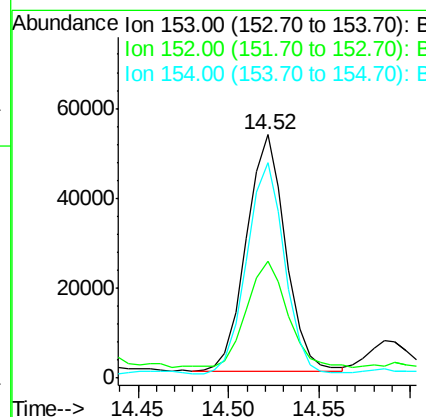

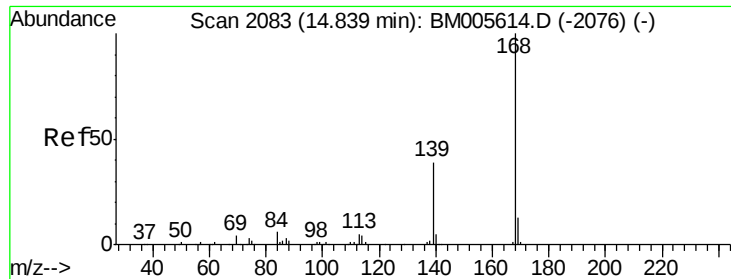

#53

Dibenzenofuran

Concen: 2.06 ng/ul

RT: 14.86 min Scan# 2086

Delta R.T. 0.01 min

Lab File: BM005602.D

Acq: 23 May 2016 00:30

Instrument :

BNA_M

ClientSampleId :

JHGG0

Tgt Ion:168 Resp: 80219

Ion Ratio Lower Upper





168 100

139 43.5 30.6 46.0

Manual Integrations
APPROVED

umangi

5/23/2016 8:36:02 PM

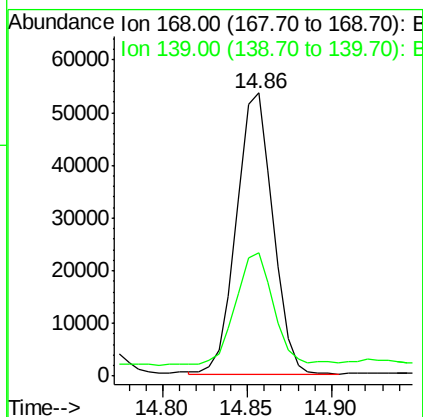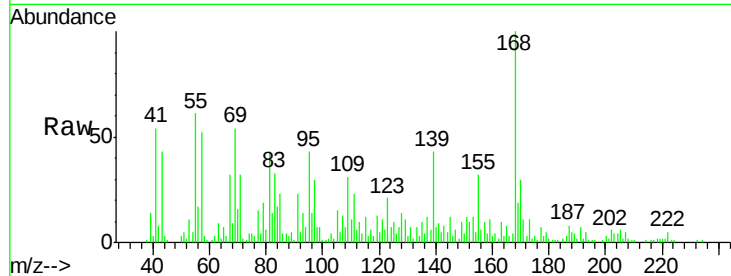

#58

Fluorene

Concen: 6.73 ng/ul

RT: 15.50 min Scan# 2196

Delta R.T. 0.01 min

Lab File: BM005602.D

Acq: 23 May 2016 00:30




Tgt Ion:166 Resp: 210036


Ion Ratio Lower Upper

166 100

165 99.3 78.0 117.0

167 14.3 10.5 15.7

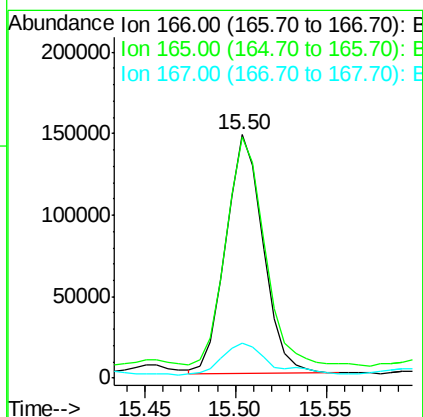

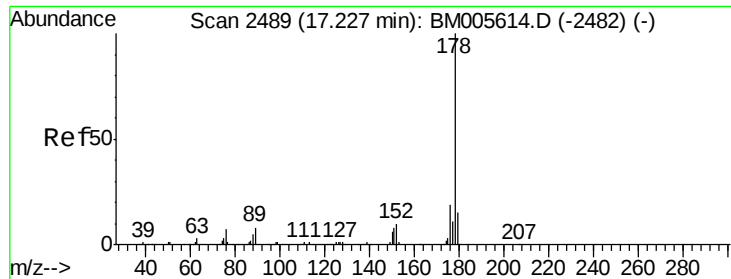





#69
Phenanthrene
Concen: 42.81 ng/ul
RT: 17.24 min Scan# 2492
Delta R.T. 0.02 min
Lab File: BM005602.D
Acq: 23 May 2016 00:30

Instrument :
BNA_M
ClientSampleId :
JHGG0

Tgt Ion:178 Resp: 2047978
Ion Ratio Lower Upper
178 100
179 16.4 12.2 18.2
176 19.4 15.8 23.6




Manual Integrations
APPROVED


umangi
5/23/2016 8:36:02 PM

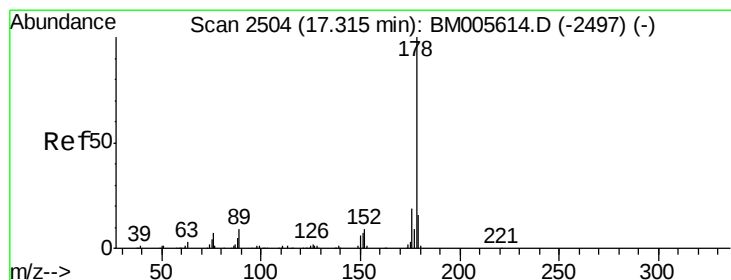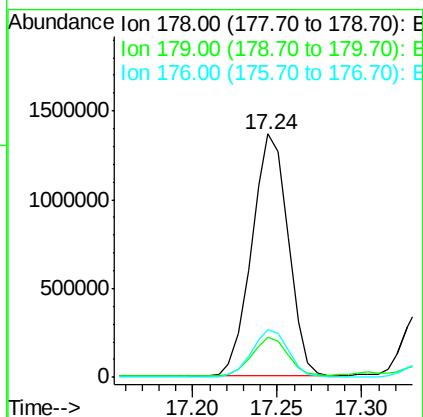

#71
Anthracene
Concen: 11.21 ng/ul
RT: 17.33 min Scan# 2507
Delta R.T. 0.01 min
Lab File: BM005602.D
Acq: 23 May 2016 00:30

Tgt Ion:178 Resp: 546388
Ion Ratio Lower Upper
178 100
179 17.5 12.6 18.8
176 18.9 15.0 22.4

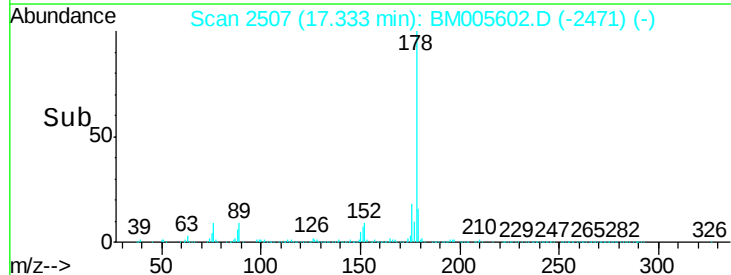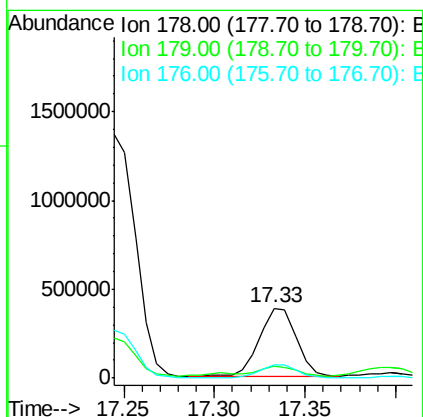

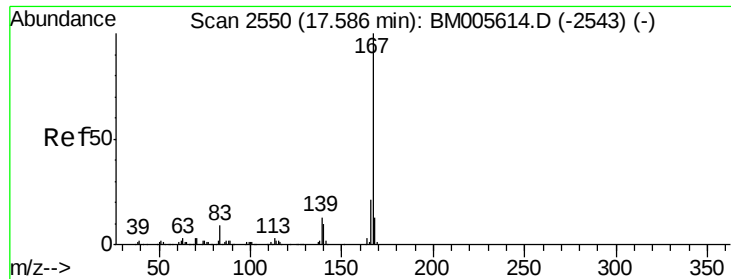

#72

Carbazole

Concen: 2.35 ng/ul

RT: 17.60 min Scan# 2553

Delta R.T. 0.01 min

Lab File: BM005602.D


Acq: 23 May 2016 00:30

Instrument :

BNA_M

ClientSampleId :




JHGG0



Tgt Ion:	167	Resp:	99574
Ion Ratio	Lower	Upper	
167	100		
166	32.2	16.9	25.3#
139	20.5	10.6	16.0#

Manual Integrations
APPROVED

umangi
5/23/2016 8:36:02 PM

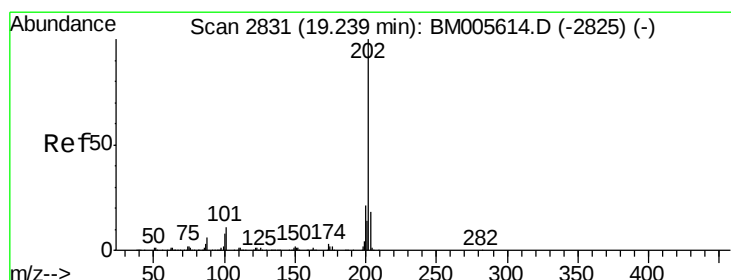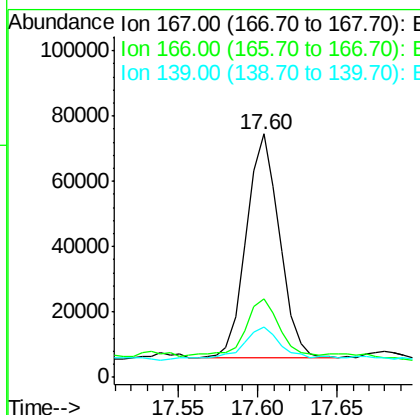

#74

Fluoranthene

Concen: 43.36 ng/ul




RT: 19.26 min Scan# 2835


Delta R.T. 0.02 min

Lab File: BM005602.D

Acq: 23 May 2016 00:30

Tgt Ion:	202	Resp:	2334878
Ion Ratio	Lower	Upper	
202	100		
101	10.1	7.9	11.9
100	7.5	5.6	8.4

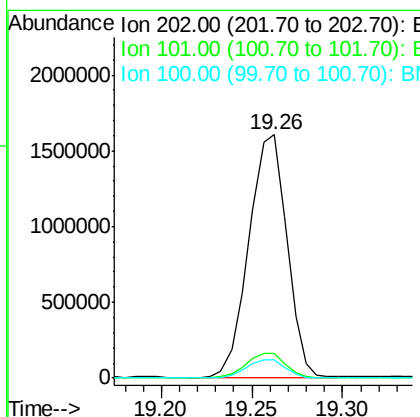



#77

Pyrene

Concen: 58.63 ng/ul

RT: 19.63 min Scan# 2897

Delta R.T. 0.02 min

Lab File: BM005602.D

Acq: 23 May 2016 00:30

Instrument :

BNA_M


ClientSampleId :

JHGG0




Tgt Ion:	202	Resp:	2588865
Ion Ratio	Lower	Upper	
202	100		
101	11.4	9.6	14.4
100	9.1	7.8	11.6

Manual Integrations
APPROVED

umangi
5/23/2016 8:36:02 PM

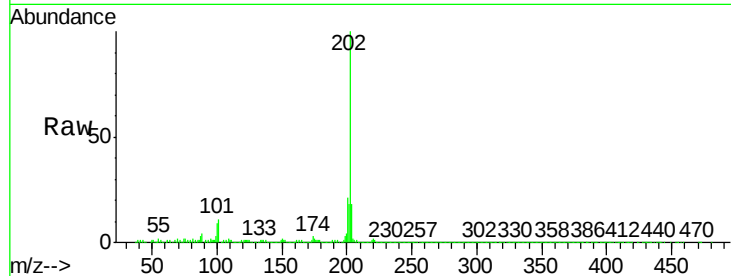

Abundance Ion 202.00 (201.70 to 202.70): E
Ion 101.00 (100.70 to 101.70): E
Ion 100.00 (99.70 to 100.70): B

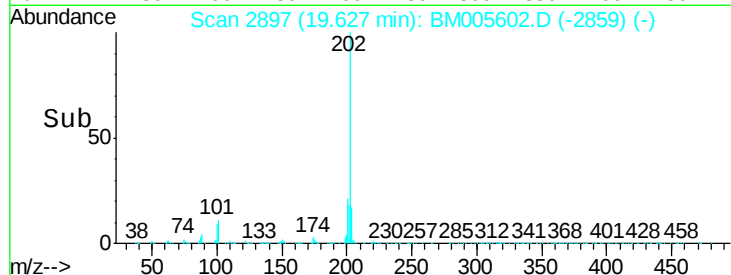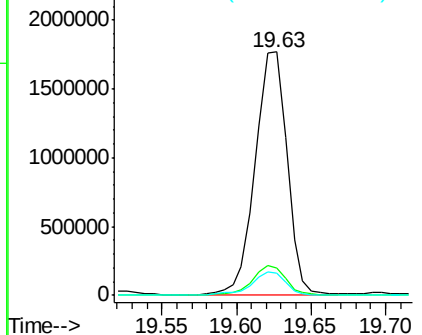

#80

Benzo(a)anthracene

Concen: 20.77 ng/ul m

RT: 21.36 min Scan# 3192




Delta R.T. 0.01 min


Lab File: BM005602.D

Acq: 23 May 2016 00:30

Tgt Ion:	228	Resp:	937477
Ion Ratio	Lower	Upper	
228	100		
229	21.8	15.4	23.2
226	32.2	21.0	31.4#

Abundance Ion 228.00 (227.70 to 228.70): E
Ion 229.00 (228.70 to 229.70): E
Ion 226.00 (225.70 to 226.70): E

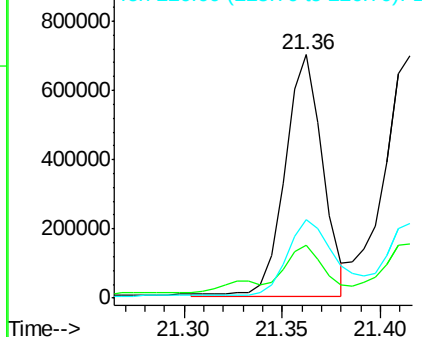

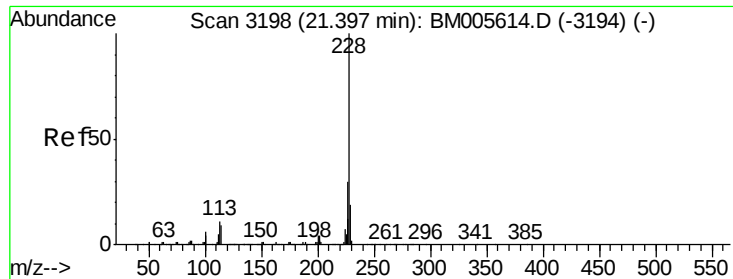

#82

Chrysene

Concen: 22.86 ng/ul

RT: 21.41 min Scan# 3201

Delta R.T. 0.02 min

Lab File: BM005602.D

Acq: 23 May 2016 00:30

Instrument :

BNA_M





ClientSampleId :

JHGG0

Tgt Ion:	228	Resp:	981769
Ion Ratio	Lower	Upper	
228	100		
226	30.6	23.7	35.5
229	22.2	15.5	23.3

Manual Integrations
APPROVED

umangi
5/23/2016 8:36:02 PM

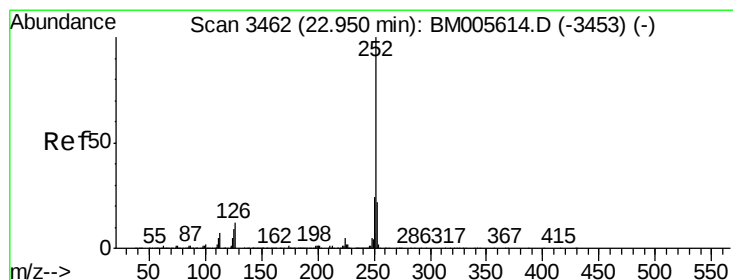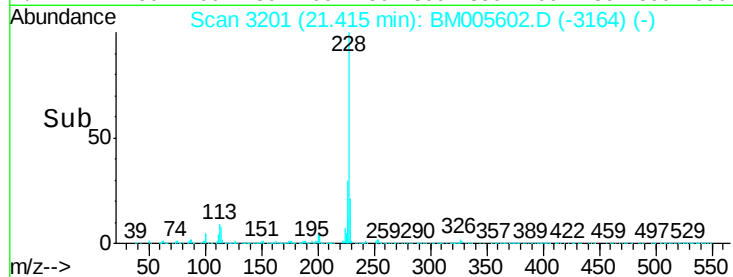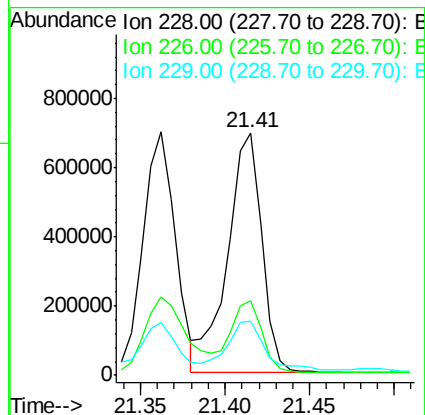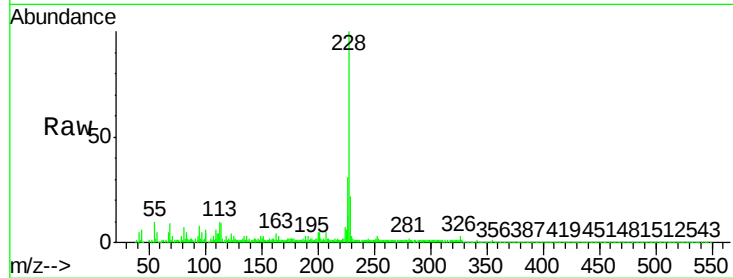

#85

Benzo(b)fluoranthene

Concen: 22.11 ng/ul




RT: 22.98 min Scan# 3467


Delta R.T. 0.02 min

Lab File: BM005602.D

Acq: 23 May 2016 00:30

Tgt Ion:	252	Resp:	911538
Ion Ratio	Lower	Upper	
252	100		
253	26.8	17.3	25.9#
125	16.5	7.0	10.4#

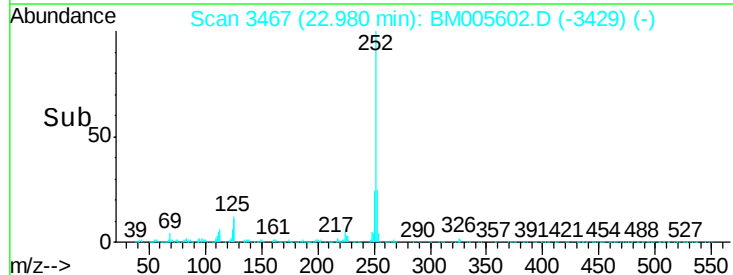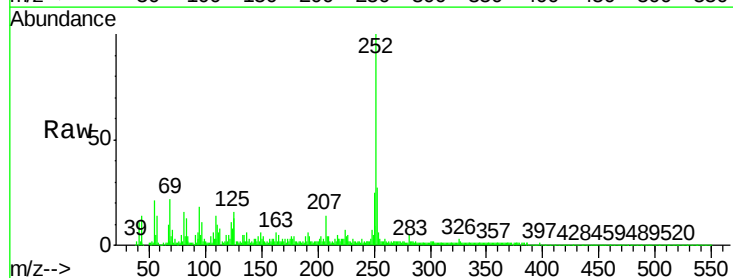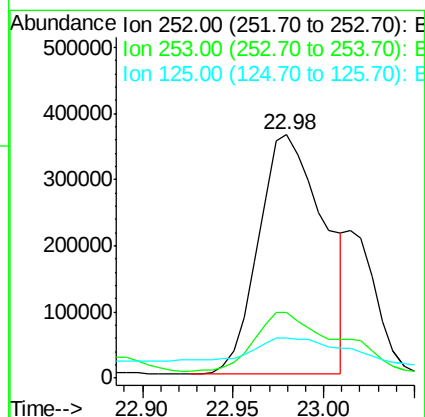

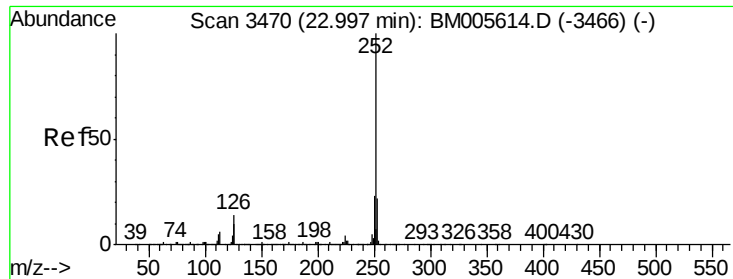





#86
Benzo(k)fluoranthene
Concen: 6.51 ng/ul m
RT: 23.01 min Scan# 3473
Delta R.T. 0.02 min
Lab File: BM005602.D
Acq: 23 May 2016 00:30

Instrument :
BNA_M
ClientSampleId :
JHGG0

Tgt Ion	Ratio	Resp Lower	Resp Upper
252	100		
253	26.5	17.5	26.3#
125	19.9	7.0	10.6#




Manual Integrations
APPROVED


umangi
5/23/2016 8:36:02 PM

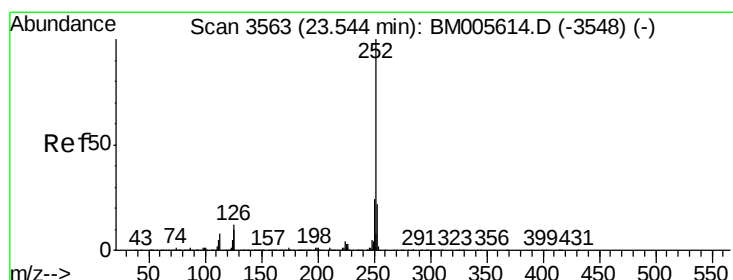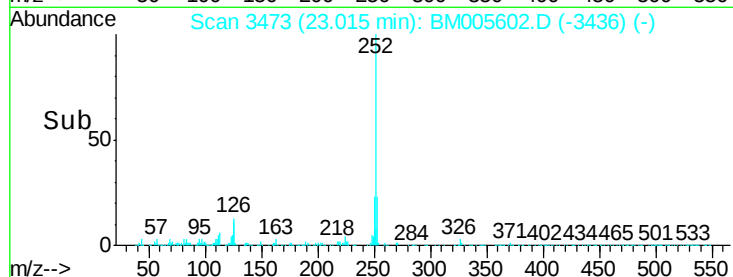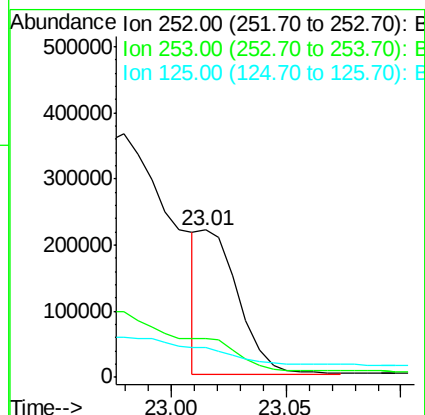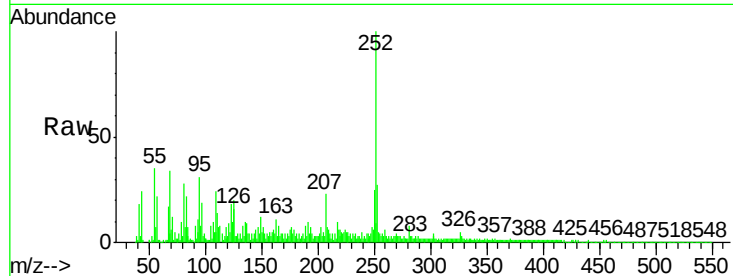

#88
Benzo(a)pyrene
Concen: 20.39 ng/ul
RT: 23.57 min Scan# 3567
Delta R.T. 0.02 min
Lab File: BM005602.D
Acq: 23 May 2016 00:30

Tgt Ion	Ratio	Resp Lower	Resp Upper
252	100		
253	23.8	17.6	26.4
125	12.8	7.6	11.4#

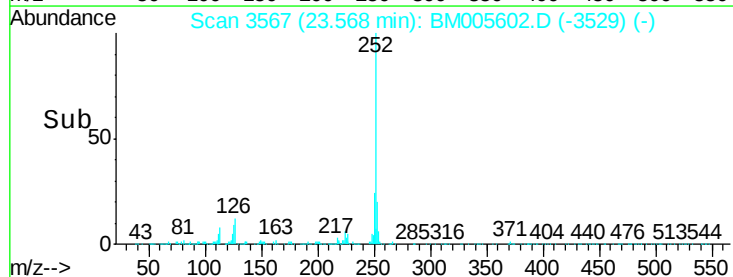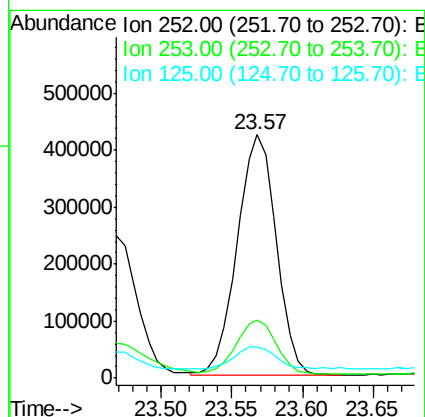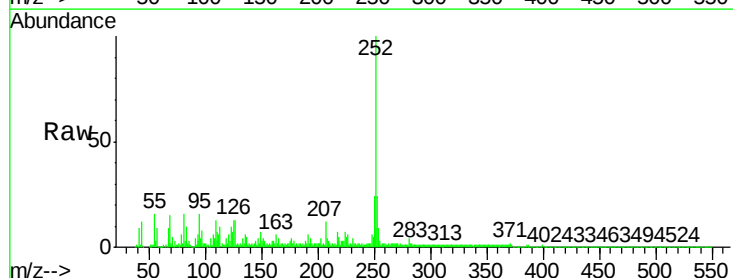

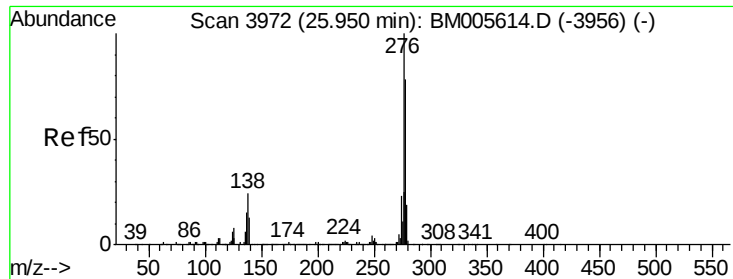





#89
Indeno(1,2,3-cd)pyrene
Concen: 10.67 ng/ul
RT: 25.99 min Scan# 3978
Delta R.T. 0.04 min
Lab File: BM005602.D
Acq: 23 May 2016 00:30

Instrument :
BNA_M
ClientSampleId :
JHGG0

Tgt Ion	Ratio	Resp Lower	Resp Upper
276	100		
138	20.7	16.9	25.3
277	25.7	20.2	30.4




Manual Integrations
APPROVED


umangi
5/23/2016 8:36:02 PM

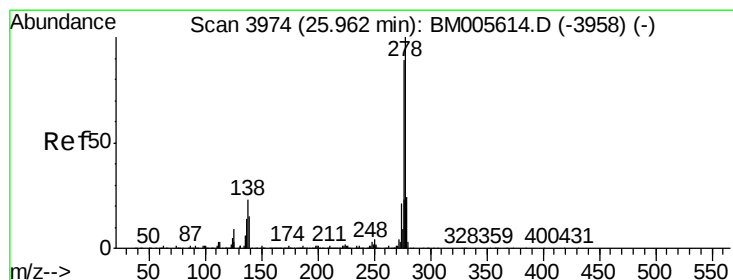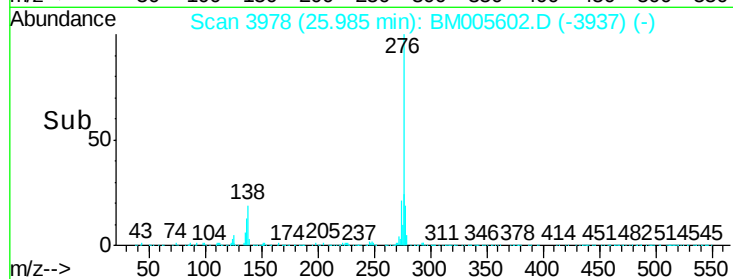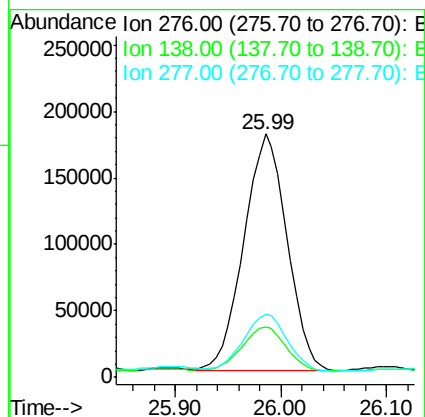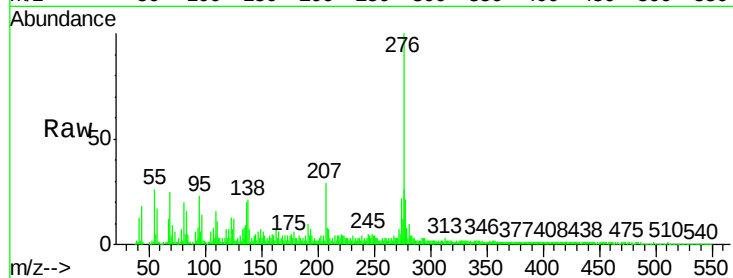

#90
Dibenzo(a,h)anthracene
Concen: 2.85 ng/ul
RT: 25.99 min Scan# 3978
Delta R.T. 0.03 min
Lab File: BM005602.D
Acq: 23 May 2016 00:30

Tgt Ion	Ratio	Resp Lower	Resp Upper
278	100		
139	30.7	11.8	17.6#
279	37.7	19.4	29.2#

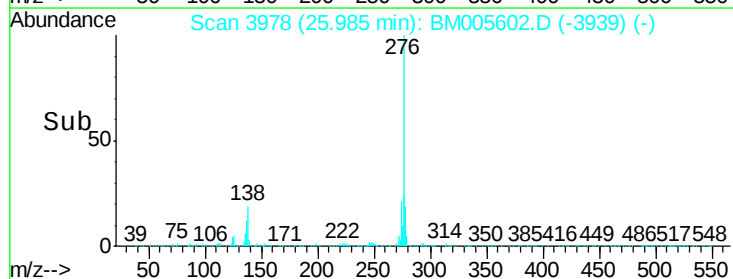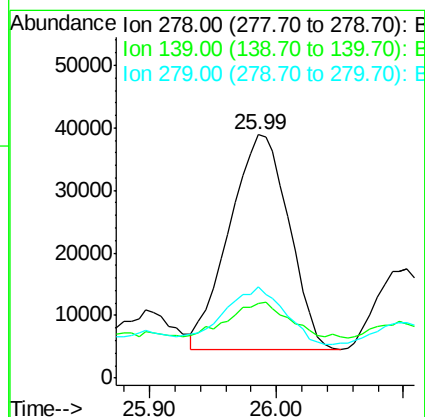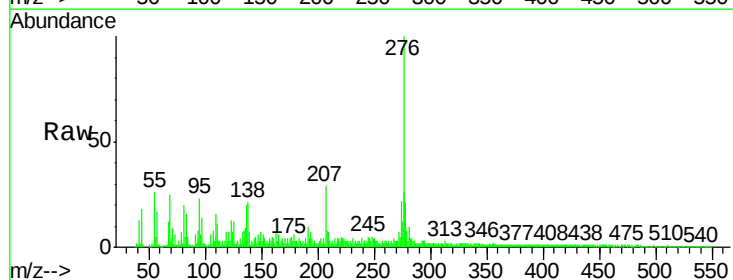

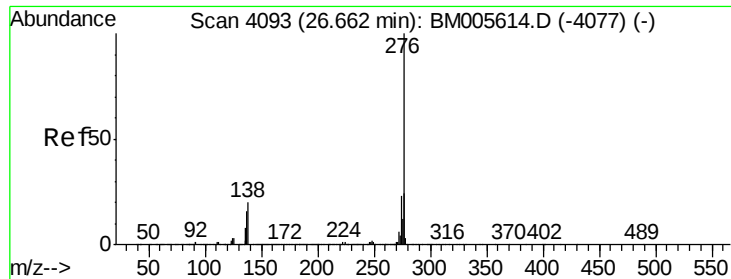

#91
 Benzo(g,h,i)perylene
 Concen: 12.35 ng/ul
 RT: 26.70 min Scan# 4100
 Delta R.T. 0.05 min
 Lab File: BM005602.D
 Acq: 23 May 2016 00:30

Instrument :
 BNA_M
 ClientSampleId :
 JHGG0

Tgt	Ion	276	Resp	493111
Ion	Ratio	Lower	Upper	
276	100			
138	22.4	15.0	22.6	
277	26.0	18.6	28.0	

Manual Integrations
 APPROVED

umangi
 5/23/2016 8:36:02 PM

