

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM052216\
 Data File : BM005606.D
 Acq On : 23 May 2016 02:55
 Operator : UM/SJ
 Sample : H3086-03
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 JHGF4

Manual Integrations
 APPROVED

umangi
 5/23/2016 8:36:12 PM

Quant Time: May 23 08:12:43 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM052016.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon May 23 05:32:02 2016
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.82	152	156226	20.00	ng/ul	0.01
18) Naphthalene-d8	10.62	136	688335	20.00	ng/ul	0.01
35) Acenaphthene-d10	14.46	164	380123	20.00	ng/ul	0.01
61) Phenanthrene-d10	17.20	188	848806	20.00	ng/ul	0.02
75) Chrysene-d12	21.39	240	708675	20.00	ng/ul	0.02
83) Perylene-d12	23.54	264	636807	20.00	ng/ul	-0.09

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.29	96	12563	3.52	ng/uL	0.00
5) Phenol-d5	7.00	99	321345	25.09	ng/ul	0.02
7) Bis-(2-Chloroethyl)ether-d	7.15	67	183080	24.67	ng/ul	0.00
9) 2-Chlorophenol-d4	7.36	132	264227	24.73	ng/ul	0.01
13) 4-Methylphenol-d8	8.54	113	257899	24.58	ng/ul	0.02
19) Nitrobenzene-d5	8.98	128	132471	25.17	ng/ul	0.01
22) 2-Nitrophenol-d4	9.70	143	138569	23.92	ng/ul	0.01
26) 2,4-Dichlorophenol-d3	10.25	165	268646	24.62	ng/ul	0.02
29) 4-Chloroaniline-d4	10.75	131	246251	22.54	ng/ul	0.01
43) Dimethylphthalate-d6	13.87	166	794192	25.59	ng/ul	0.01
46) Acenaphthylene-d8	14.15	160	1024839	26.42	ng/ul	0.01
51) 4-Nitrophenol-d4	14.69	143	117529	20.02	ng/ul	0.04
57) Fluorene-d10	15.45	176	717101	26.56	ng/ul	0.01
62) 4,6-Dinitro-2-methylphenol	15.59	200	16762	3.43	ng/ul	0.03
70) Anthracene-d10	17.30	188	1120342	27.71	ng/ul	0.02
76) Pyrene-d10	19.60	212	1144043	35.65	ng/ul	0.02
87) Benzo(a)pyrene-d12	23.54	264	672909m	22.63	ng/ul	0.05

Target Compounds

						Qvalue
16) 4-Methylphenol	8.60	108	13209	1.22	ng/ul	92
28) Naphthalene	10.66	128	35544	1.03	ng/ul	97
44) Dimethylphthalate	13.92	163	140042	4.57	ng/ul	99
47) Acenaphthylene	14.19	152	2153784	54.65	ng/ul	99
49) Acenaphthene	14.53	153	55955	2.15	ng/ul	94
58) Fluorene	15.51	166	90459	3.05	ng/ul	95
60) 4-Nitroaniline	15.52	138	8394	1.20	ng/ul	89
69) Phenanthrene	17.24	178	762874	16.08	ng/ul	98
71) Anthracene	17.34	178	1195380	24.73	ng/ul	99
72) Carbazole	17.61	167	68670	1.64	ng/ul#	87
74) Fluoranthene	19.27	202	3848794	72.08	ng/ul	99
77) Pyrene	19.63	202	4606906	113.08	ng/ul	99
80) Benzo(a)anthracene	21.37	228	2585721	62.07	ng/ul#	86
82) Chrysene	21.43	228	2717246	68.56	ng/ul	95
85) Benzo(b)fluoranthene	23.00	252	3384974	90.12	ng/ul	96
86) Benzo(k)fluoranthene	23.04	252	990927m	27.87	ng/ul	
88) Benzo(a)pyrene	23.60	252	2377396	65.25	ng/ul	97
89) Indeno(1,2,3-cd)pyrene	26.04	276	1840305m	42.52	ng/ul	
90) Dibenzo(a,h)anthracene	26.04	278	633152m	17.57	ng/ul	
91) Benzo(g,h,i)perylene	26.76	276	1396340m	38.38	ng/ul	

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\HPCHEM1\BNA_M\DATA\BM052216\
Data File : BM005606.D
Acq On : 23 May 2016 02:55
Operator : UM/SJ
Sample : H3086-03
Misc :
ALS Vial : 24 Sample Multiplier: 1


Instrument :
BNA_M
ClientSampled :
JHGF4

Manual Integrations
APPROVED

umangi
5/23/2016 8:36:12 PM

Quant Time: May 23 08:12:43 2016
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM052016.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon May 23 05:32:02 2016
Response via : Initial Calibration

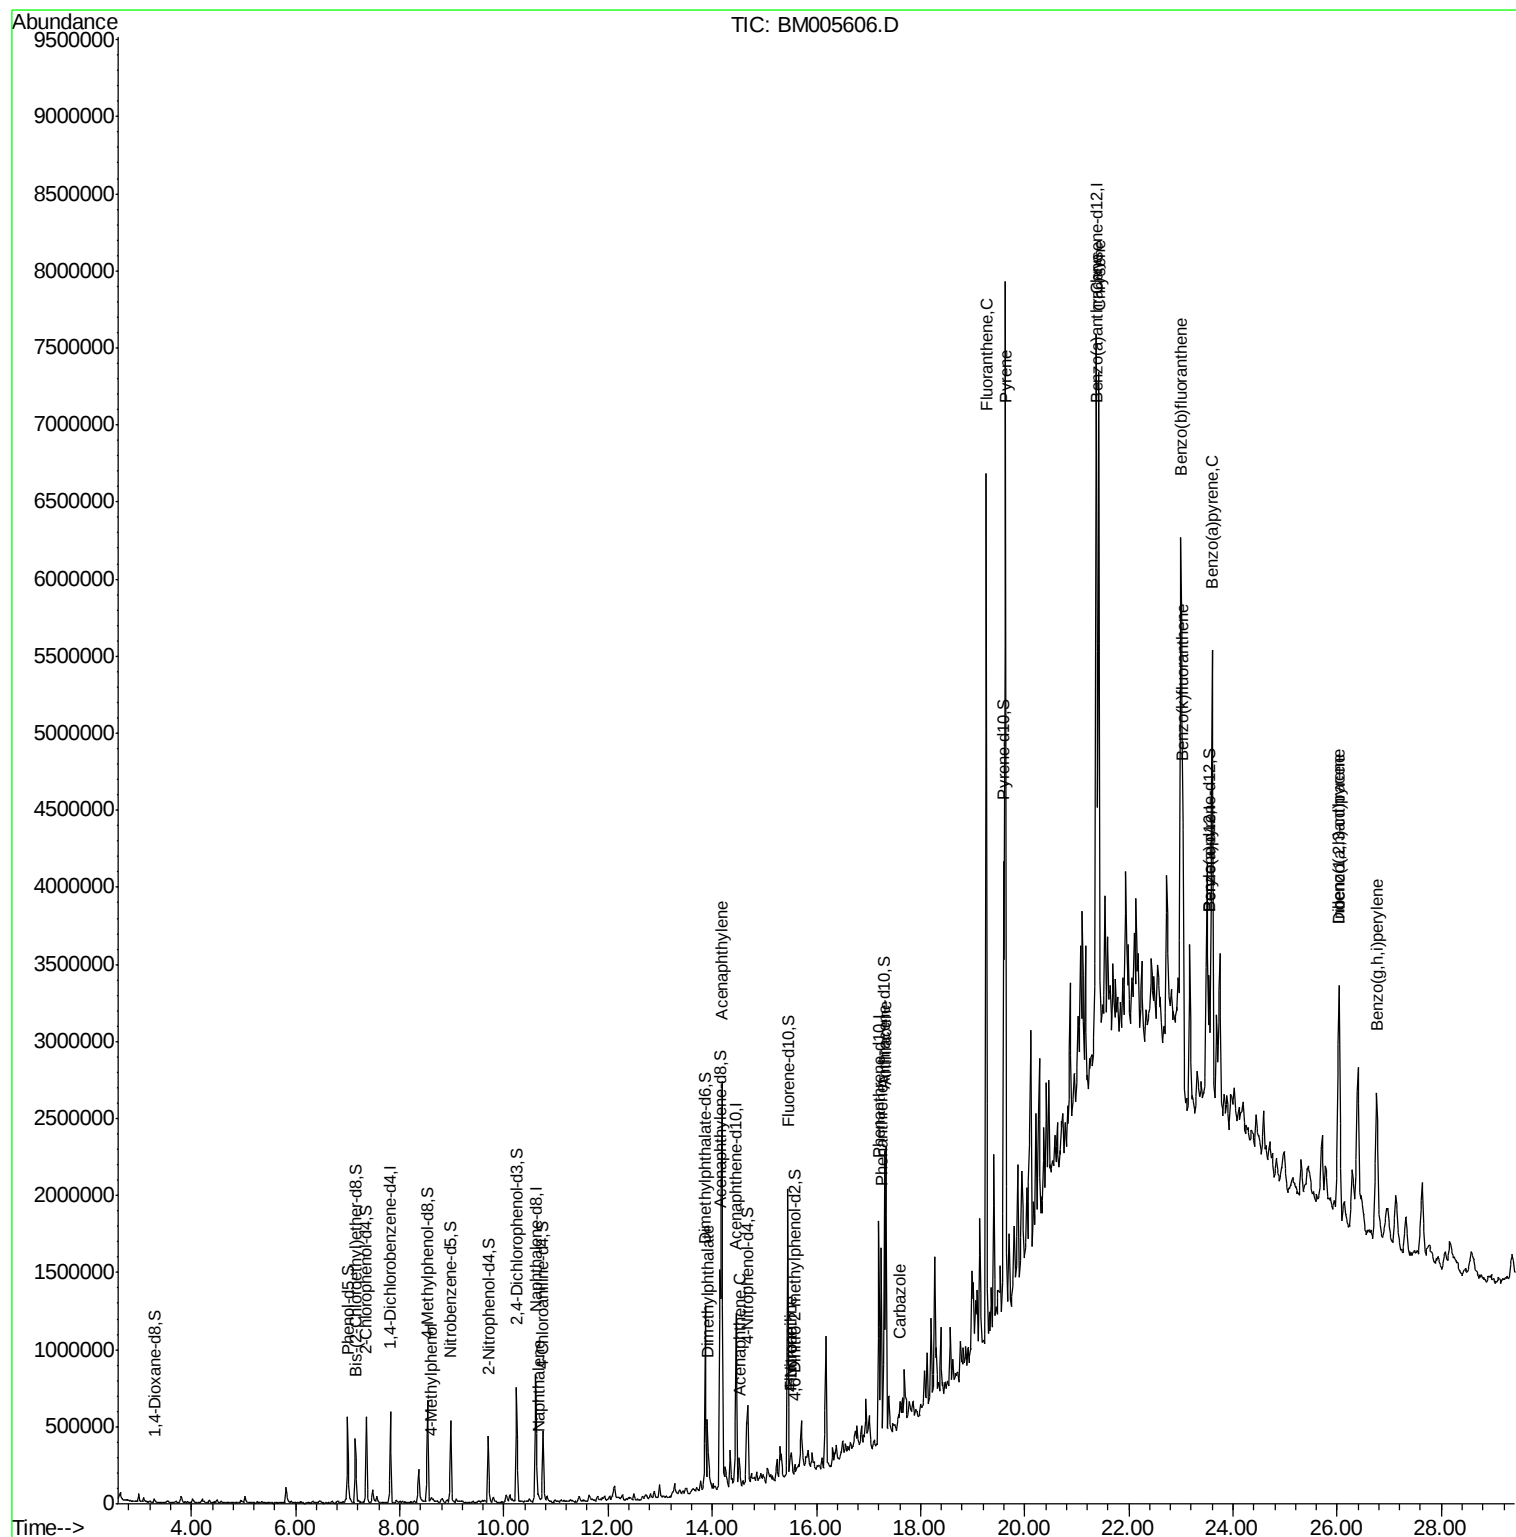

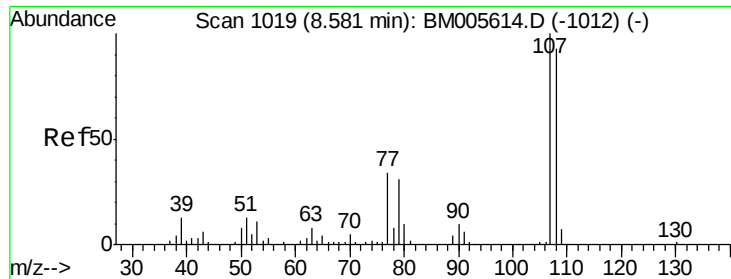





#16
4-Methylphenol
Concen: 1.22 ng/ul
RT: 8.60 min Scan# 1023
Delta R.T. 0.02 min
Lab File: BM005606.D
Acq: 23 May 2016 02:55

Instrument :
BNA_M
ClientSampleId :
JHGF4

Tgt Ion	Ratio	Lower	Upper
108	100		
107	104.8	90.3	135.5




Manual Integrations
APPROVED


umangi
5/23/2016 8:36:12 PM

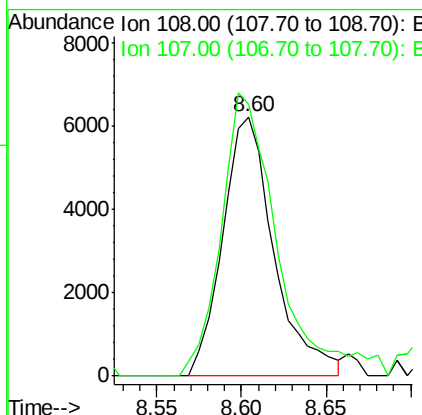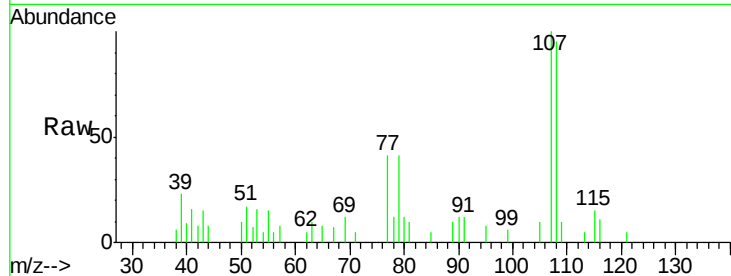

#28
Naphthalene
Concen: 1.03 ng/ul
RT: 10.66 min Scan# 1373
Delta R.T. 0.01 min
Lab File: BM005606.D
Acq: 23 May 2016 02:55

Tgt Ion	Ratio	Lower	Upper
128	100		
129	12.8	8.6	13.0
127	12.7	10.6	15.8

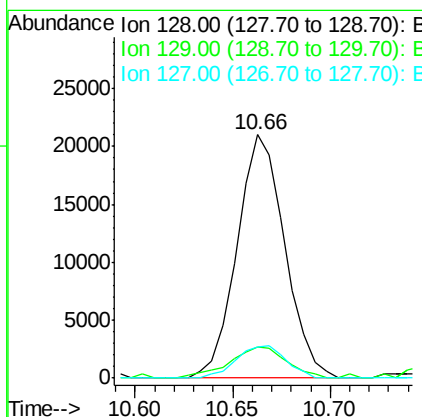

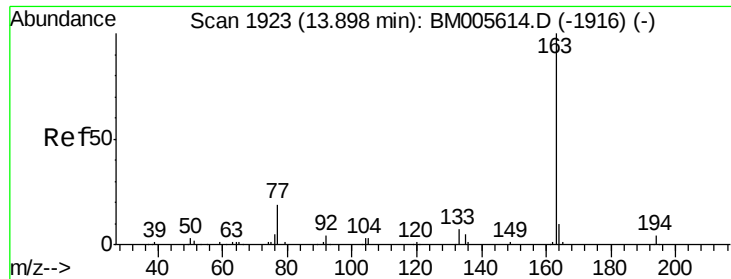


#44
Dimethylphthalate
Concen: 4.57 ng/ul
RT: 13.92 min Scan# 1926
Delta R.T. 0.01 min
Lab File: BM005606.D
Acq: 23 May 2016 02:55

Instrument :
BNA_M
ClientSampled :
JHGF4




Tgt Ion	Ratio	Resp	Lower	Upper
163	100	140042		
194	3.9		3.4	5.0
164	10.3		8.0	12.0

Manual Integrations
APPROVED

umangi
5/23/2016 8:36:12 PM




Abundance Ion 163.00 (162.70 to 163.70): E
Ion 194.00 (193.70 to 194.70): E
Ion 164.00 (163.70 to 164.70): E

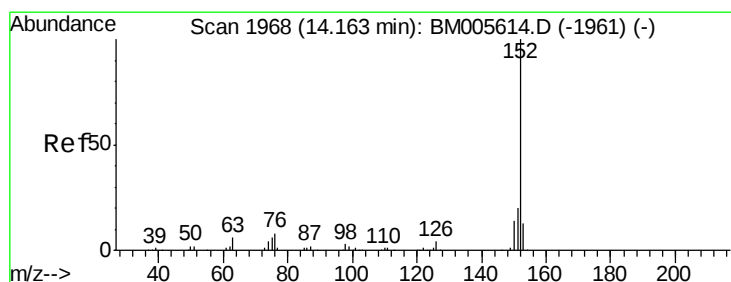
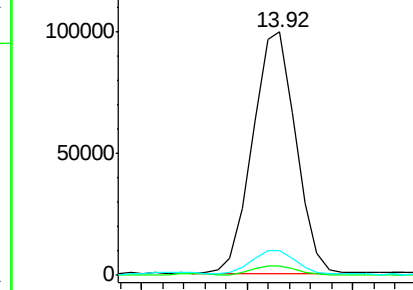



#47
Acenaphthylene
Concen: 54.65 ng/ul
RT: 14.19 min Scan# 1972
Delta R.T. 0.02 min
Lab File: BM005606.D
Acq: 23 May 2016 02:55

Tgt Ion	Ratio	Resp	Lower	Upper
152	100	2153784		
151	20.1		15.7	23.5
153	13.1		10.5	15.7



Abundance Ion 152.00 (151.70 to 152.70): E
Ion 151.00 (150.70 to 151.70): E
Ion 153.00 (152.70 to 153.70): E

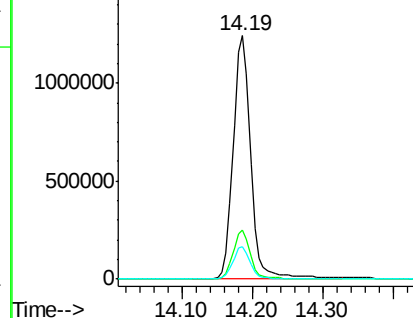

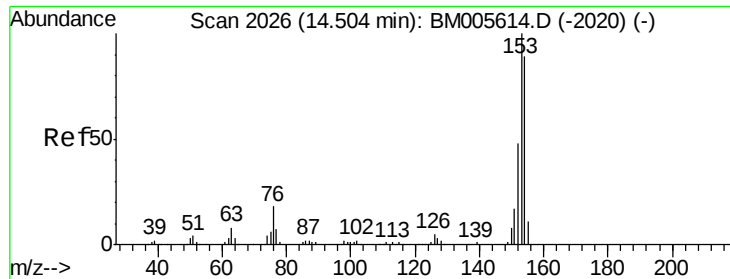

#49

Acenaphthene

Concen: 2.15 ng/ul

RT: 14.53 min Scan# 2030

Delta R.T. 0.02 min

Lab File: BM005606.D


Acq: 23 May 2016 02:55

Instrument :

BNA_M

ClientSampleId :




JHGF4

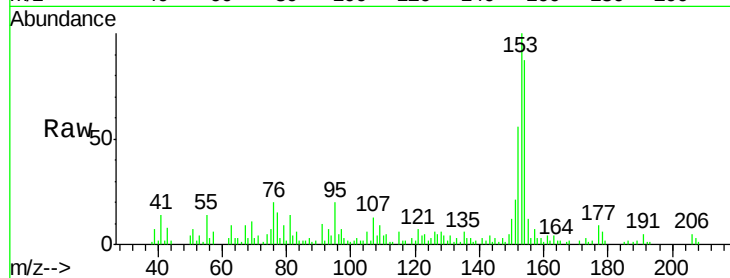

Tgt Ion:	153	Resp:	55955
Ion Ratio	Lower	Upper	
153	100		
152	55.9	37.8	56.6
154	87.5	71.1	106.7

Manual Integrations
APPROVED

umangi
5/23/2016 8:36:12 PM

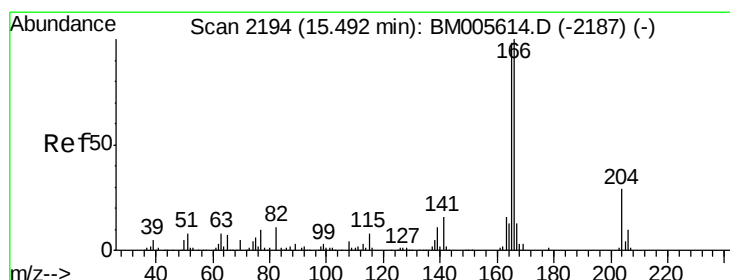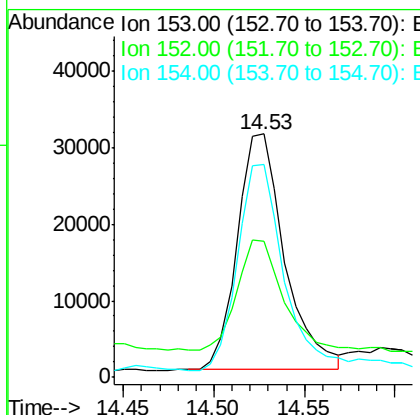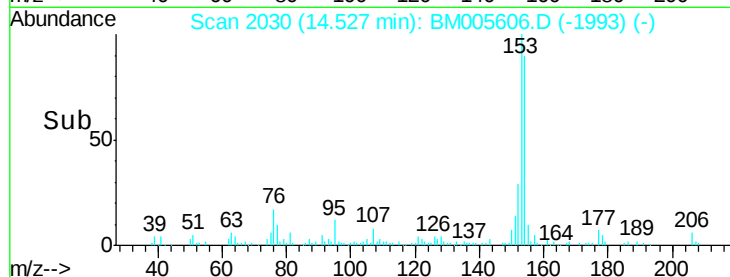

#58

Fluorene

Concen: 3.05 ng/ul




RT: 15.51 min Scan# 2197


Delta R.T. 0.02 min

Lab File: BM005606.D

Acq: 23 May 2016 02:55

Tgt Ion:	166	Resp:	90459
Ion Ratio	Lower	Upper	
166	100		
165	102.5	78.0	117.0
167	14.8	10.5	15.7

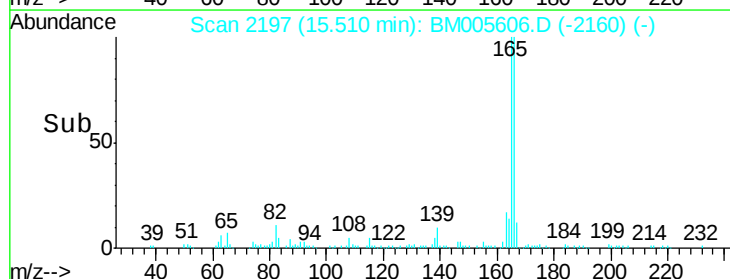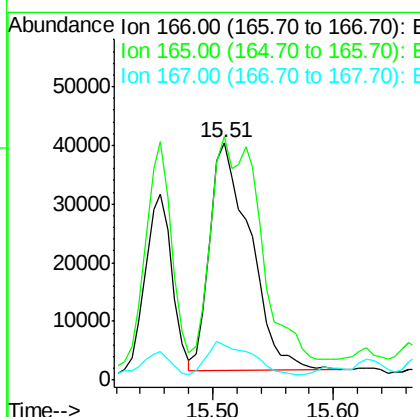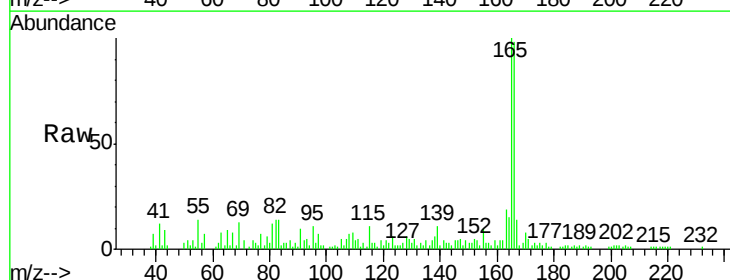







#60
4-Nitroaniline
Concen: 1.20 ng/ul
RT: 15.52 min Scan# 2199
Delta R.T. 0.01 min
Lab File: BM005606.D
Acq: 23 May 2016 02:55

Instrument :
BNA_M
ClientSampleId :
JHGF4

Tgt Ion	Ratio	Lower	Upper
138	100		
92	50.2	41.4	62.0
108	83.7	79.4	119.0




Manual Integrations
APPROVED


umangi
5/23/2016 8:36:12 PM

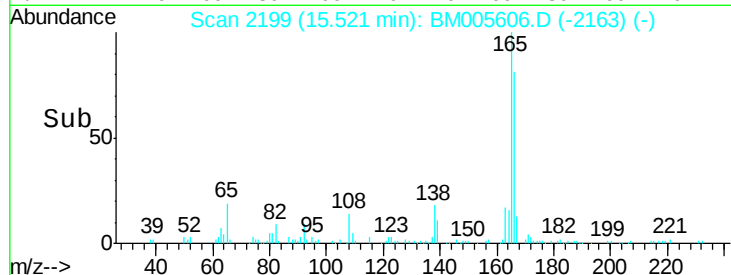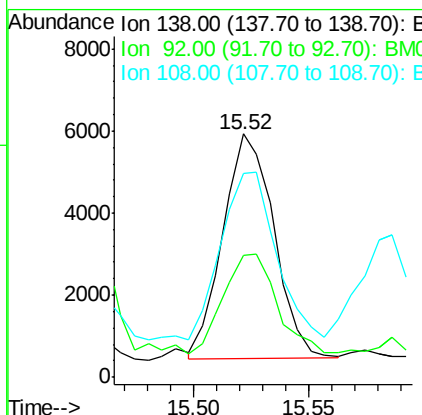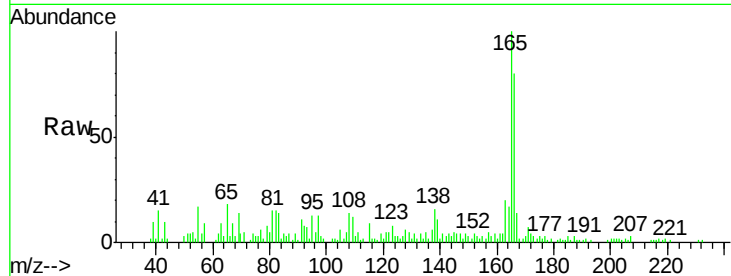

#69
Phenanthrene
Concen: 16.08 ng/ul
RT: 17.24 min Scan# 2492
Delta R.T. 0.02 min
Lab File: BM005606.D
Acq: 23 May 2016 02:55

Tgt Ion	Ratio	Lower	Upper
178	100		
179	16.0	12.2	18.2
176	19.0	15.8	23.6

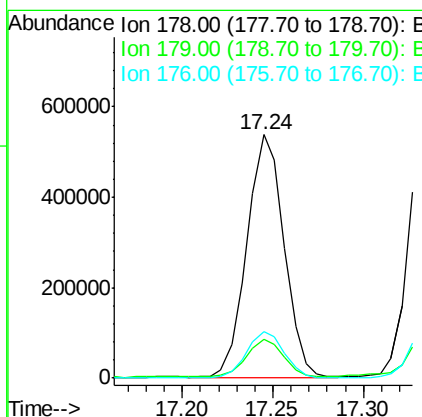







#71
 Anthracene
 Concen: 24.73 ng/ul
 RT: 17.34 min Scan# 2508
 Delta R.T. 0.02 min
 Lab File: BM005606.D
 Acq: 23 May 2016 02:55

Instrument :
 BNA_M
 ClientSampleId :
 JHGF4

Tgt Ion	Ratio	Lower	Upper
178	100		
179	15.5	12.6	18.8
176	18.3	15.0	22.4




Manual Integrations
 APPROVED


umangi
 5/23/2016 8:36:12 PM

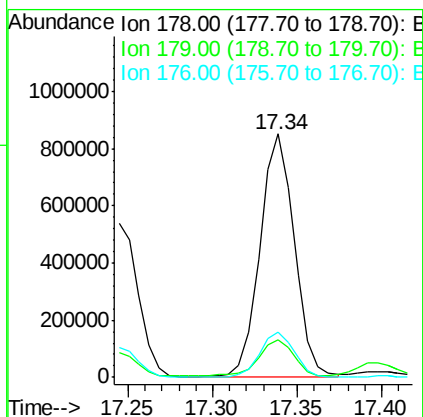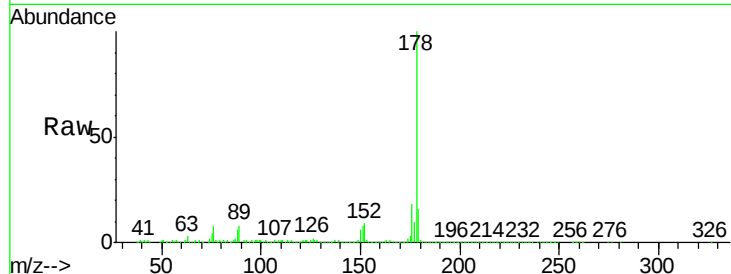

#72
 Carbazole
 Concen: 1.64 ng/ul
 RT: 17.61 min Scan# 2554
 Delta R.T. 0.02 min
 Lab File: BM005606.D
 Acq: 23 May 2016 02:55

Tgt Ion	Ratio	Lower	Upper
167	100		
166	27.9	16.9	25.3#
139	17.4	10.6	16.0#

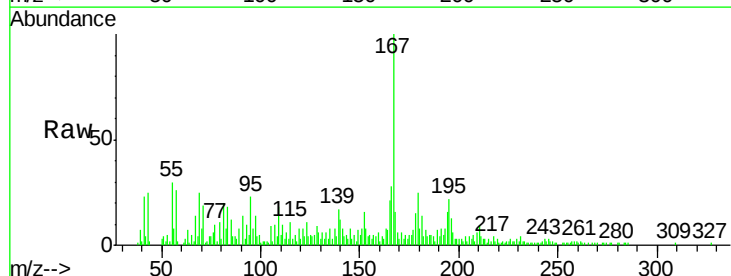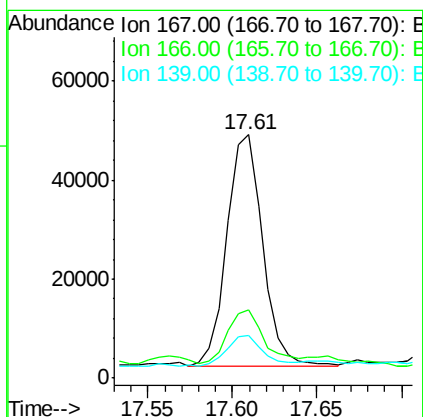

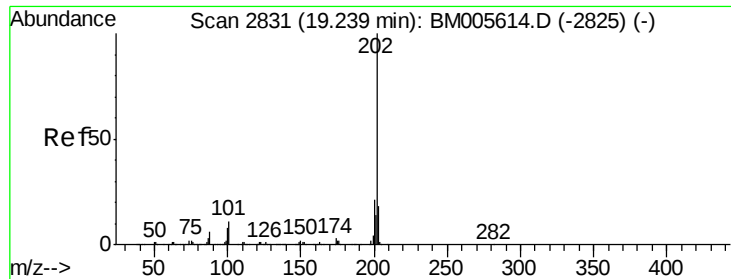





#74
 Fluoranthene
 Concen: 72.08 ng/ul
 RT: 19.27 min Scan# 2836
 Delta R.T. 0.03 min
 Lab File: BM005606.D
 Acq: 23 May 2016 02:55

Instrument :
 BNA_M
 ClientSampleId :
 JHGF4

Tgt Ion	Ratio	Lower	Upper
202	100		
101	9.9	7.9	11.9
100	7.4	5.6	8.4




Manual Integrations
 APPROVED


umangi
 5/23/2016 8:36:12 PM

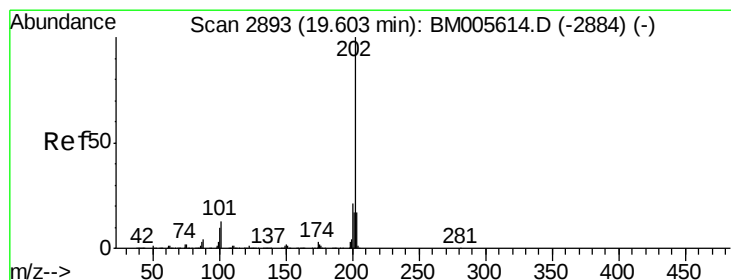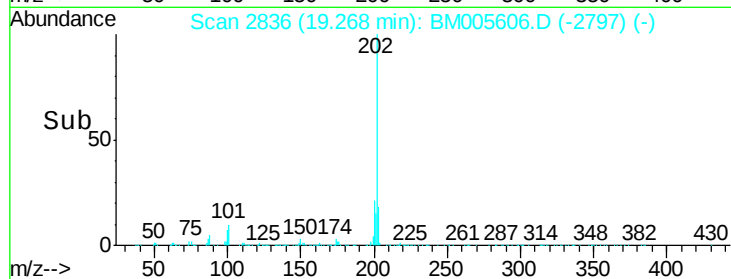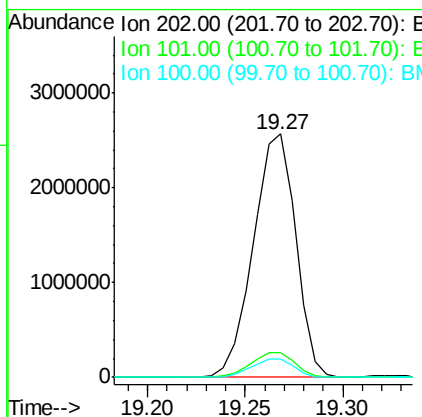

#77
 Pyrene
 Concen: 113.08 ng/ul
 RT: 19.63 min Scan# 2898
 Delta R.T. 0.03 min
 Lab File: BM005606.D
 Acq: 23 May 2016 02:55

Tgt Ion	Ratio	Lower	Upper
202	100		
101	11.7	9.6	14.4
100	9.2	7.8	11.6

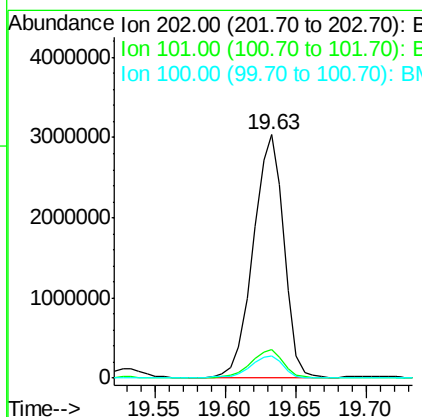

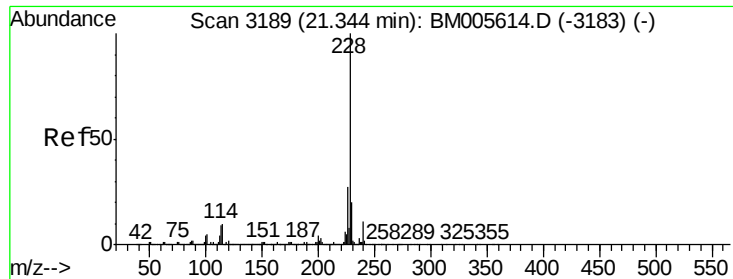





#80
Benzo(a)anthracene
Concen: 62.07 ng/ul
RT: 21.37 min Scan# 3194
Delta R.T. 0.02 min
Lab File: BM005606.D
Acq: 23 May 2016 02:55

Instrument :
BNA_M
ClientSampleId :
JHGF4

Tgt Ion	Ratio	Lower	Upper
228	100		
229	21.8	15.4	23.2
226	36.4	21.0	31.4#




Manual Integrations
APPROVED


umangi
5/23/2016 8:36:12 PM

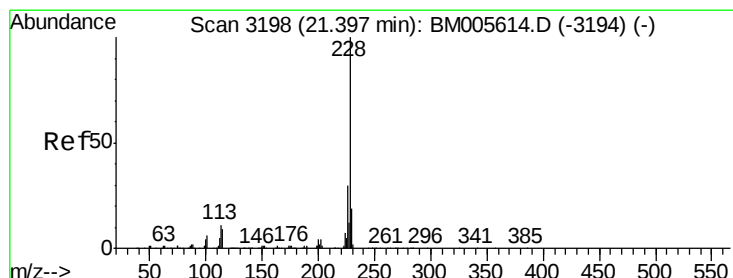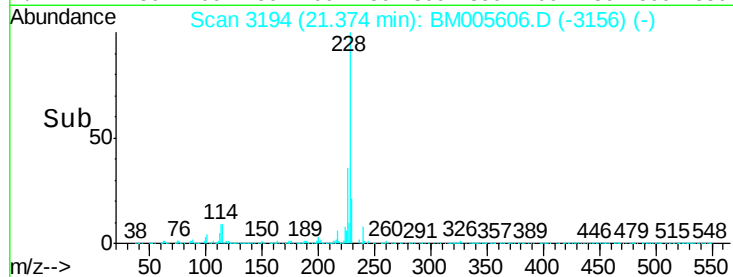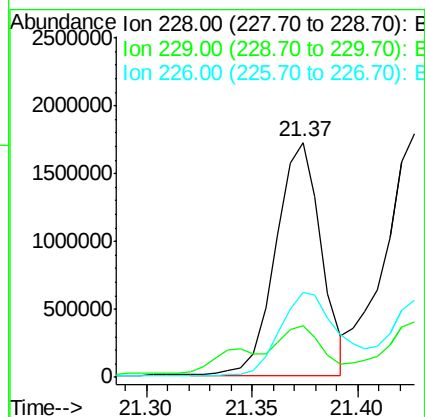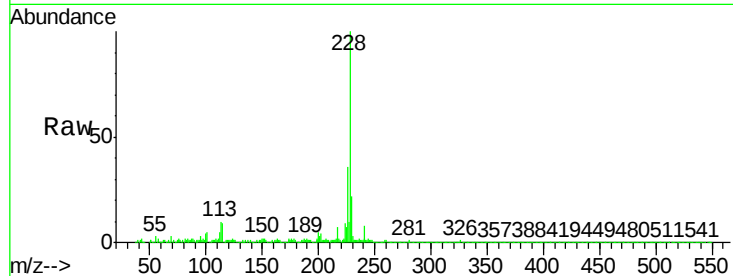

#82
Chrysene
Concen: 68.56 ng/ul
RT: 21.43 min Scan# 3203
Delta R.T. 0.03 min
Lab File: BM005606.D
Acq: 23 May 2016 02:55

Tgt Ion	Ratio	Lower	Upper
228	100		
226	31.5	23.7	35.5
229	22.7	15.5	23.3

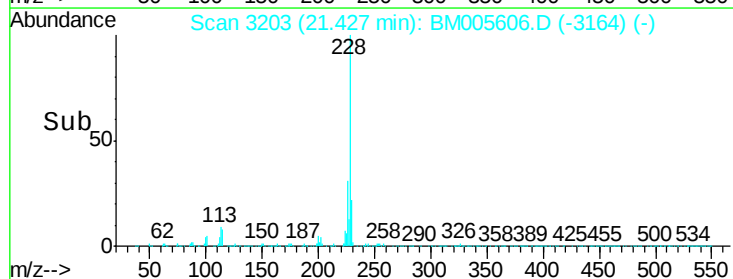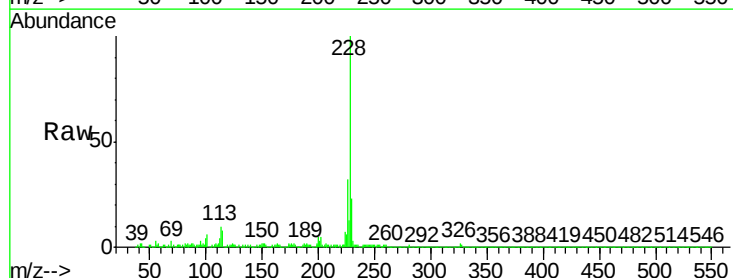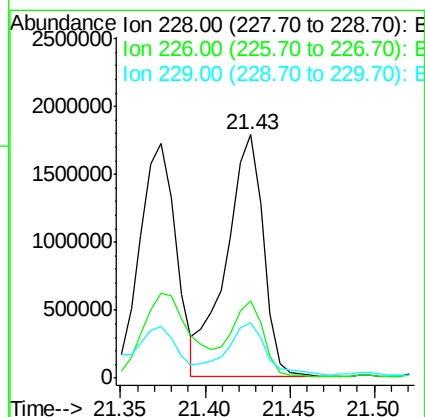

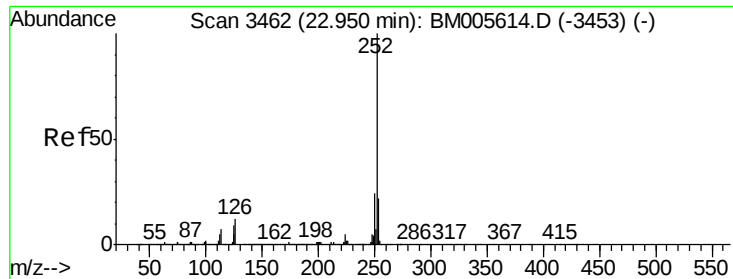





#85
Benzo(b)fluoranthene
Concen: 90.12 ng/ul
RT: 23.00 min Scan# 3471
Delta R.T. 0.05 min
Lab File: BM005606.D
Acq: 23 May 2016 02:55

Instrument :
BNA_M
ClientSampleId :
JHGF4

Tgt Ion	Ratio	Lower	Upper
252	100		
253	23.3	17.3	25.9
125	10.4	7.0	10.4




Manual Integrations
APPROVED


umangi
5/23/2016 8:36:12 PM

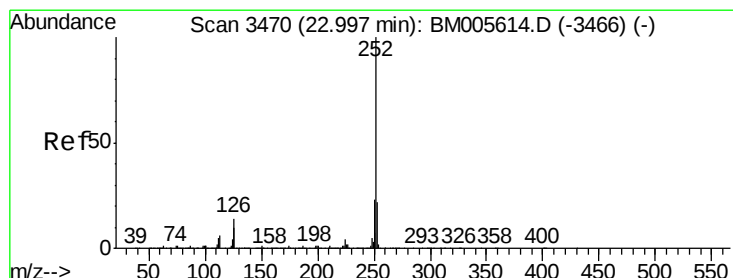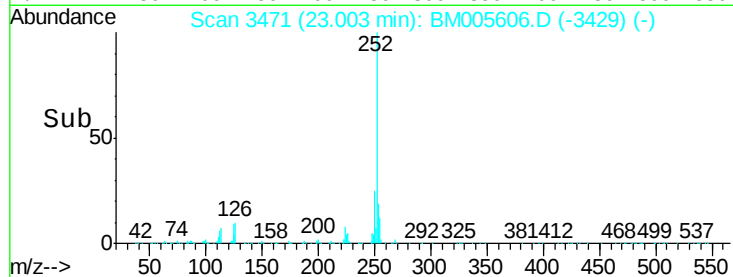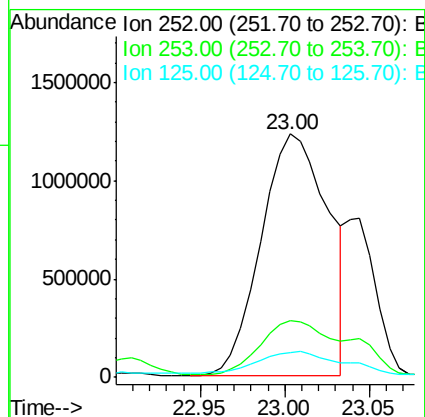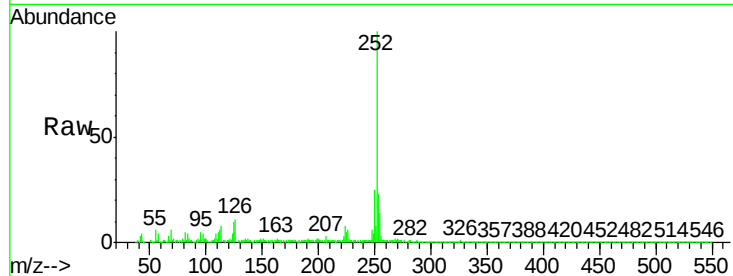

#86
Benzo(k)fluoranthene
Concen: 27.87 ng/ul m
RT: 23.04 min Scan# 3478
Delta R.T. 0.05 min
Lab File: BM005606.D
Acq: 23 May 2016 02:55

Tgt Ion	Ratio	Lower	Upper
252	100		
253	24.7	17.5	26.3
125	8.9	7.0	10.6

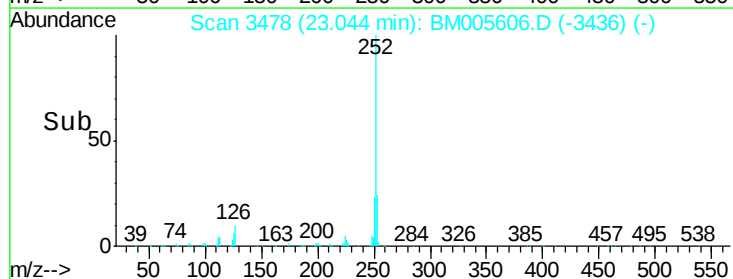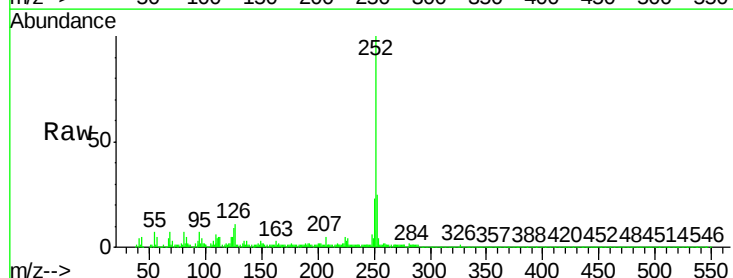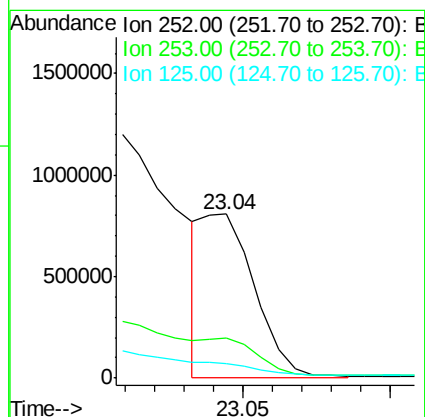

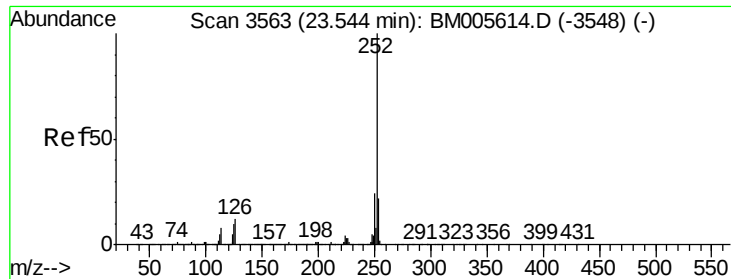

#88

Benzo(a)pyrene

Concen: 65.25 ng/ul

RT: 23.60 min Scan# 3572

Delta R.T. 0.05 min

Lab File: BM005606.D


Acq: 23 May 2016 02:55

Instrument :

BNA_M

ClientSampleId :




JHGF4



Tgt Ion	Ratio	Lower	Upper
252	100		
253	24.0	17.6	26.4
125	9.1	7.6	11.4

Manual Integrations
APPROVED

umangi
5/23/2016 8:36:12 PM

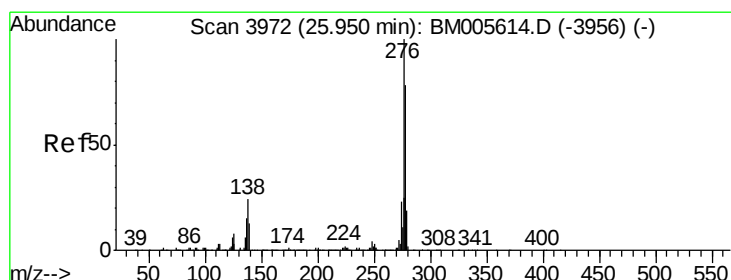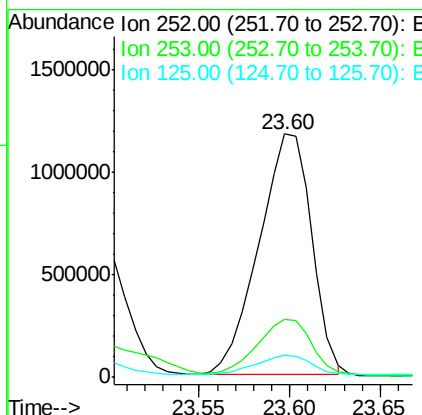

#89

Indeno(1,2,3-cd)pyrene

Concen: 42.52 ng/ul m




RT: 26.04 min Scan# 3987


Delta R.T. 0.09 min

Lab File: BM005606.D

Acq: 23 May 2016 02:55

Tgt Ion	Ratio	Lower	Upper
276	100		
138	16.3	16.9	25.3#
277	25.2	20.2	30.4

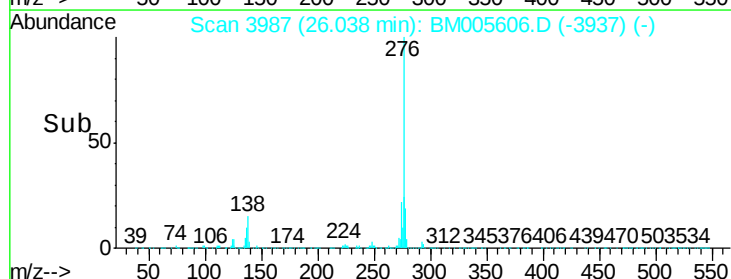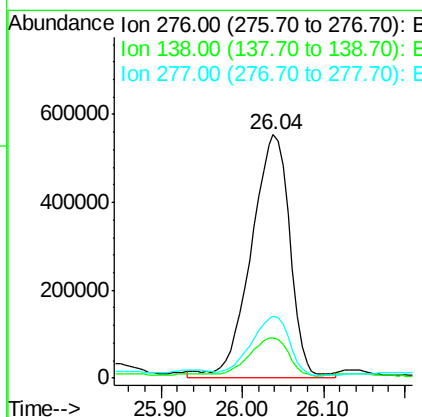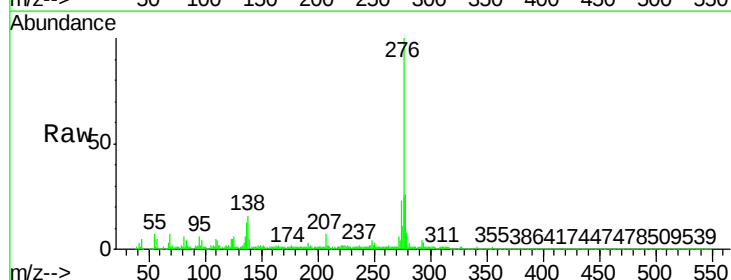

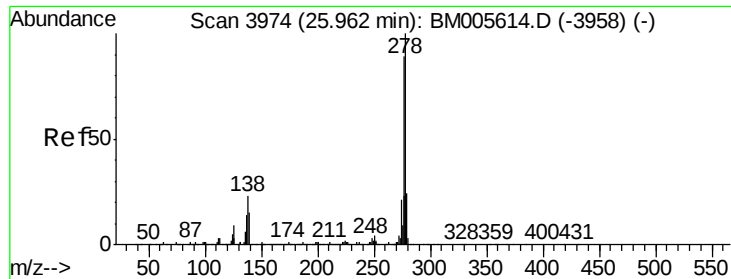





#90
Dibenzo(a,h)anthracene
Concen: 17.57 ng/ul m
RT: 26.04 min Scan# 3987
Delta R.T. 0.08 min
Lab File: BM005606.D
Acq: 23 May 2016 02:55

Instrument :
BNA_M
ClientSampleId :
JHGF4

Tgt Ion	Ratio	Lower	Upper
278	100		
139	18.6	11.8	17.6#
279	30.0	19.4	29.2#

Manual Integrations
APPROVED

umangi
5/23/2016 8:36:12 PM

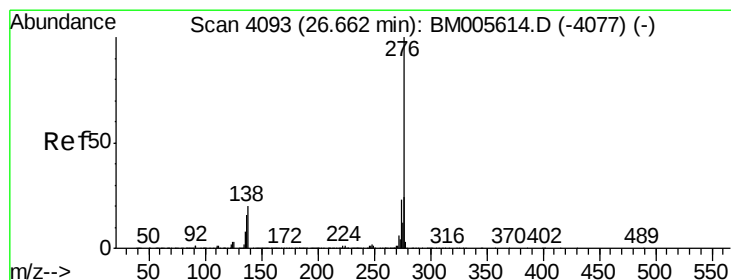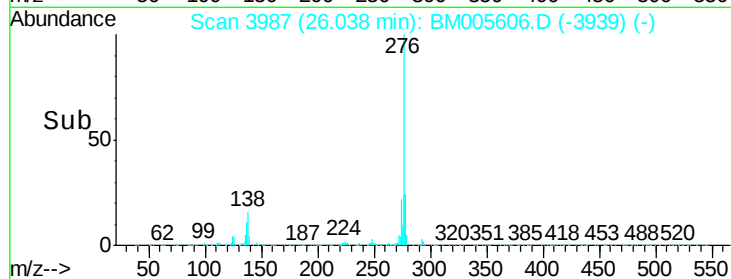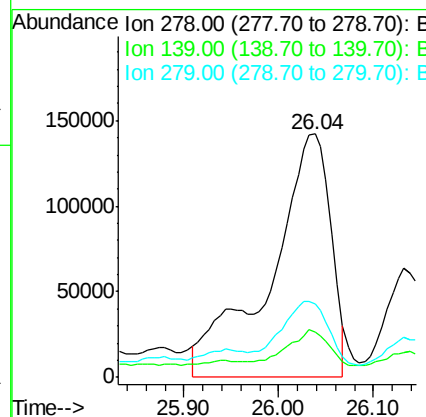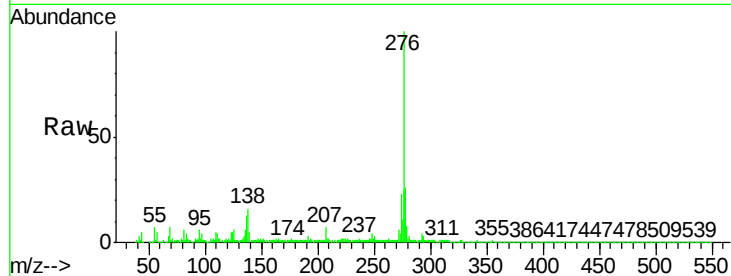

#91
Benzo(g,h,i)perylene
Concen: 38.38 ng/ul m
RT: 26.76 min Scan# 4109
Delta R.T. 0.10 min
Lab File: BM005606.D
Acq: 23 May 2016 02:55

Tgt Ion	Ratio	Lower	Upper
276	100		
138	17.2	15.0	22.6
277	24.7	18.6	28.0

