

Data Path : Z:\HPCHEM1\BNA M\DATA\BM052217\
 Data File : BM010103.D
 Acq On : 22 May 2017 15:35
 Operator : SJ/MA
 Sample : PB99141BL
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :

Quant Time: May 23 05:26:42 2017
 Quant Method : Z:\HPCHEM1\BNA M\METHODS\8270-BM051917.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat May 20 04:25:49 2017
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.96	152	159145	20.00	ng	-0.01
21) Naphthalene-d8	10.77	136	508758	20.00	ng	-0.01
38) Acenaphthene-d10	14.60	164	305668	20.00	ng	-0.01
63) Phenanthrene-d10	17.34	188	727617	20.00	ng	-0.01
75) Chrysene-d12	21.50	240	1089702	20.00	ng	-0.01
86) Perylene-d12	23.87	264	1260317	20.00	ng	-0.02
System Monitoring Compounds						
5) 2-Fluorophenol	5.55	112	1123604	127.50	ng	-0.01
7) Phenol-d6	7.16	99	1327602	117.07	ng	-0.01
23) Nitrobenzene-d5	9.15	82	855572	90.73	ng	-0.02
41) 2,4,6-Tribromophenol	16.09	330	558404	120.28	ng	-0.01
44) 2-Fluorobiphenyl	13.22	172	2132981	89.71	ng	-0.01
78) Terphenyl-d14	19.94	244	3521459	73.48	ng	-0.01
Target Compounds						
15) Benzyl Alcohol	8.29	79	18816	2.19	ng	Qvalue # 32


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA M\DATA\BM052217\
Data File : BM010103.D
Acq On : 22 May 2017 15:35
Operator : SJ/MA
Sample : PB99141BL
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :

Quant Time: May 23 05:26:42 2017
Quant Method : Z:\HPCHEM1\BNA M\METHODS\8270-BM051917.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat May 20 04:25:49 2017
Response via : Initial Calibration




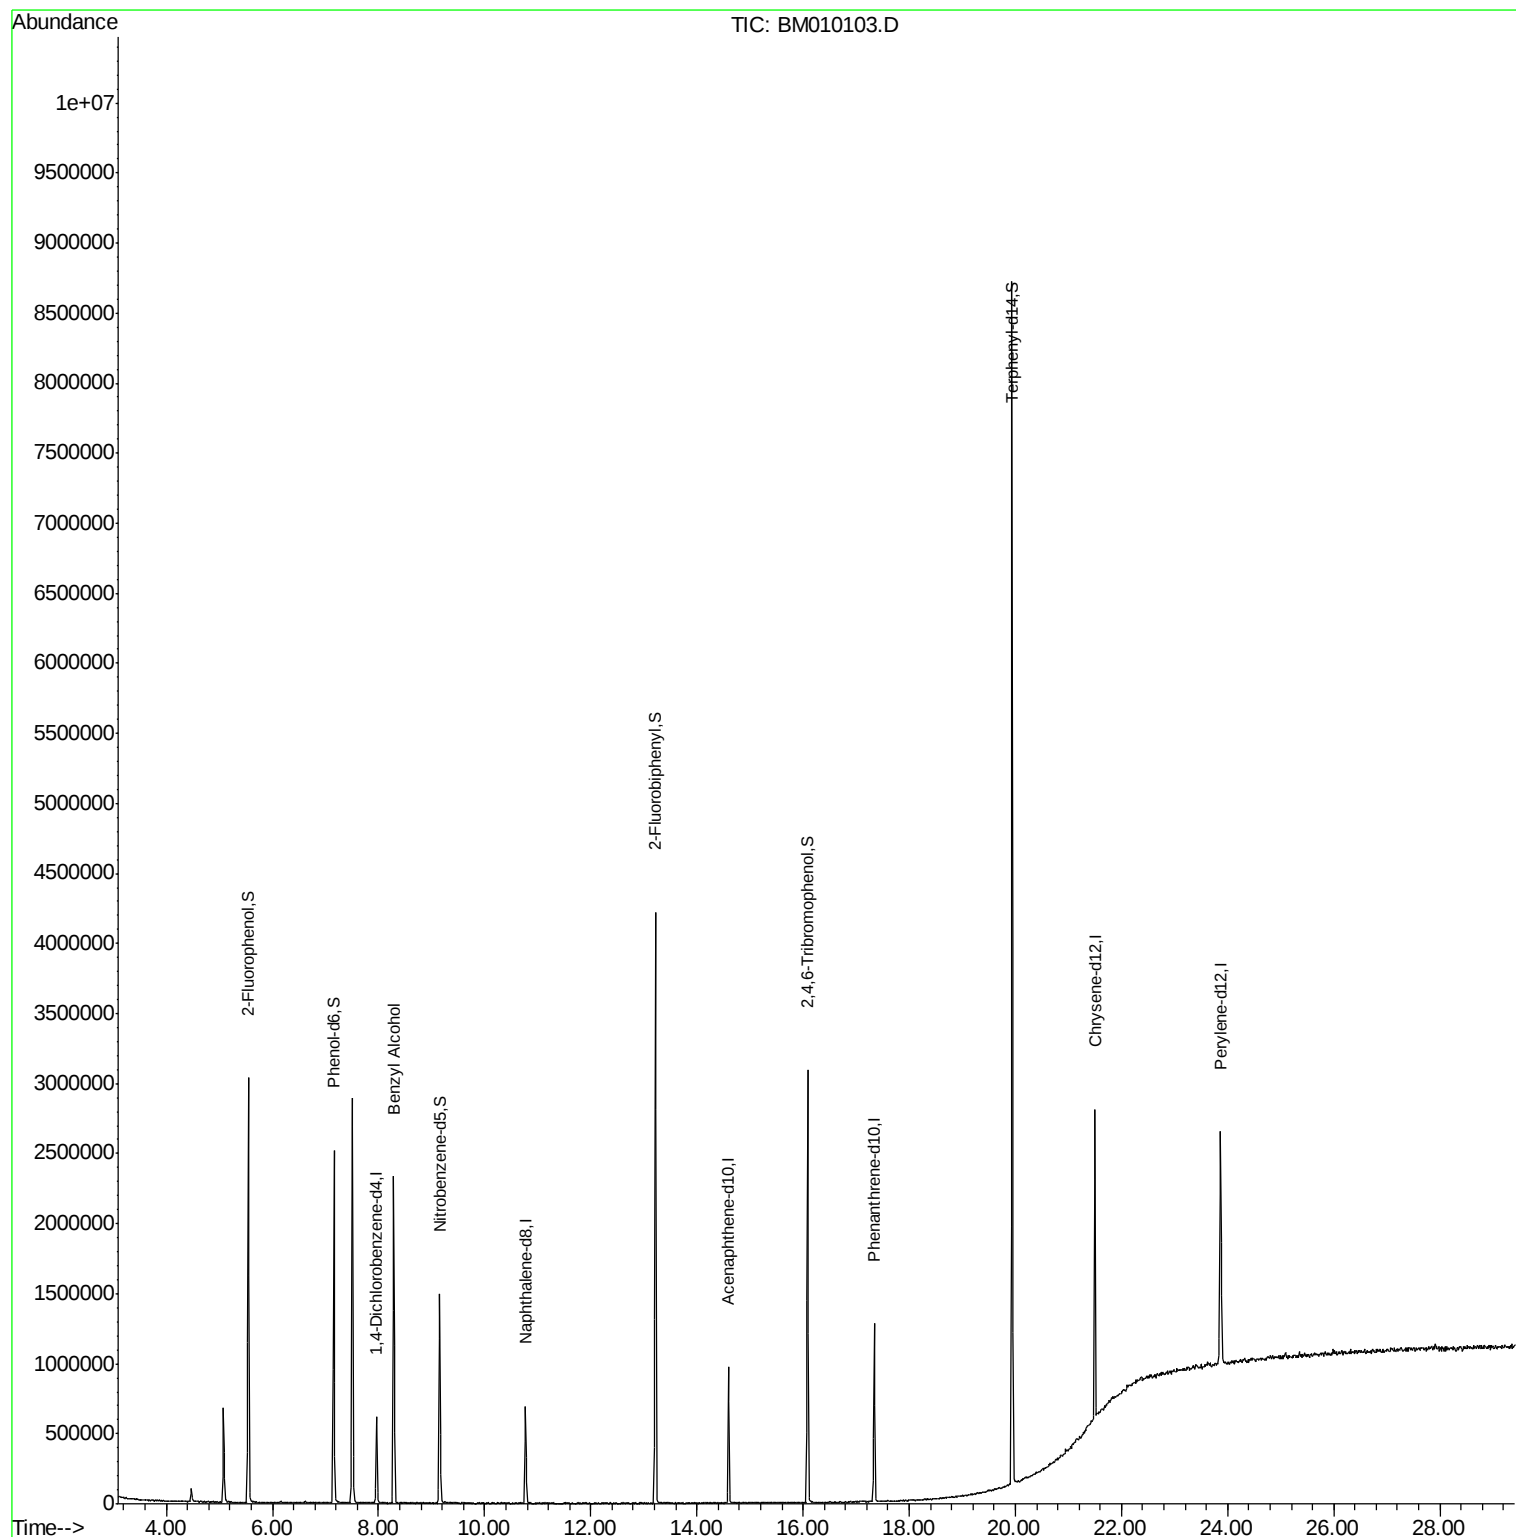


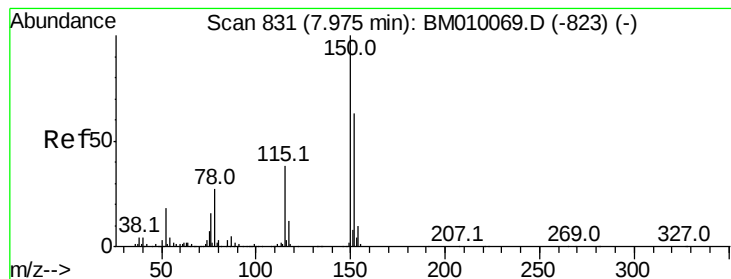

#1
 1,4-Dichlorobenzene-d4
 Concen: 20.00 ng
 RT: 7.96 min Scan# 829
 Delta R.T. -0.01 min
 Lab File: BM010103.D
 Acq: 22 May 2017 15:35




Instrument :
 BNA_M
 ClientSampleId :


Tot Ion	Ratio	Lower	Upper
152	100		
150	152.5	119.5	179.3
115	57.9	43.0	64.4

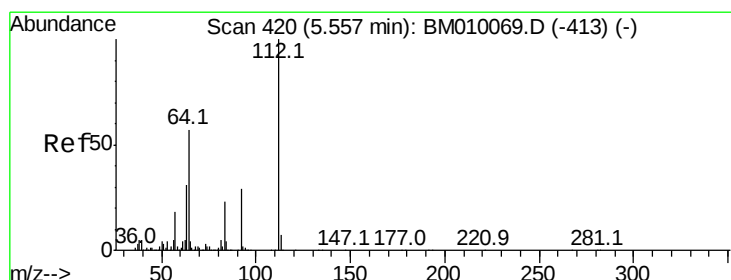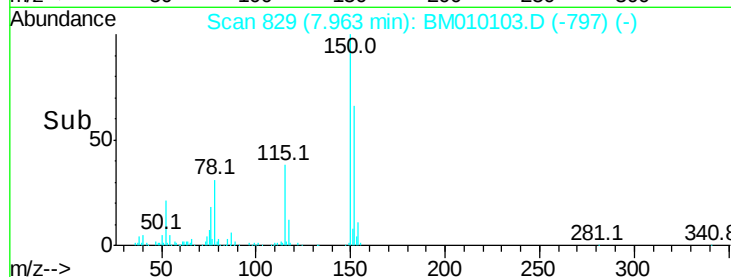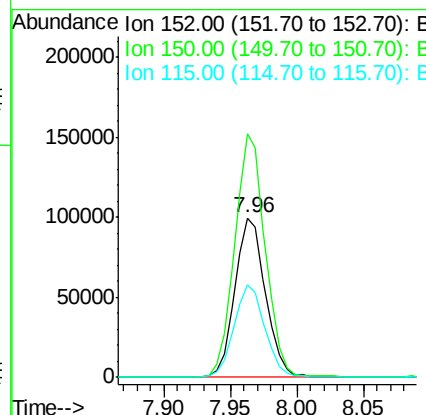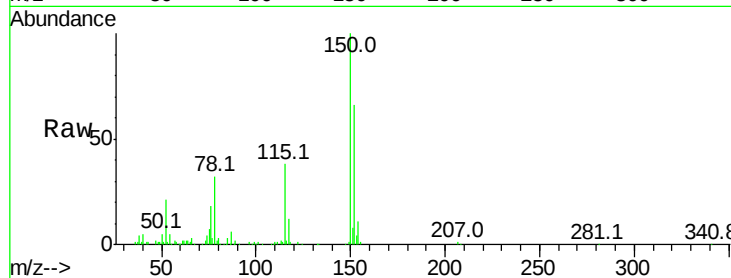

#5
 2-Fluorophenol
 Concen: 127.50 ng
 RT: 5.55 min Scan# 418
 Delta R.T. -0.01 min
 Lab File: BM010103.D
 Acq: 22 May 2017 15:35

Tgt Ion	Ratio	Lower	Upper
112	100		
64	61.2	38.6	57.8#
63	36.4	19.3	28.9#

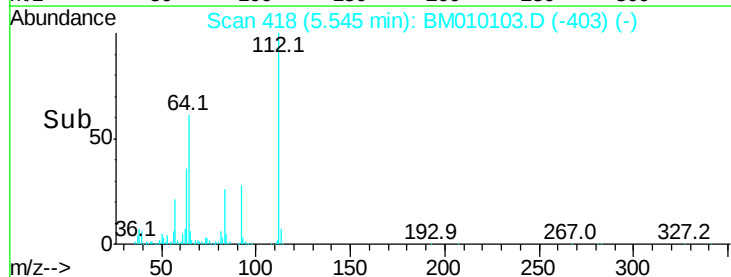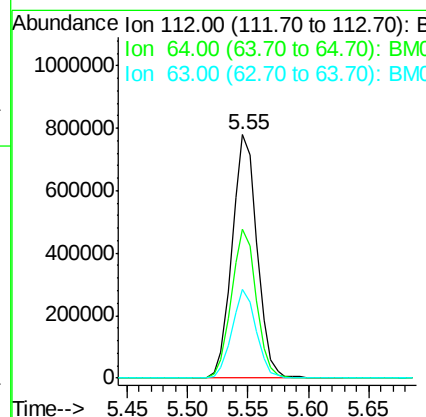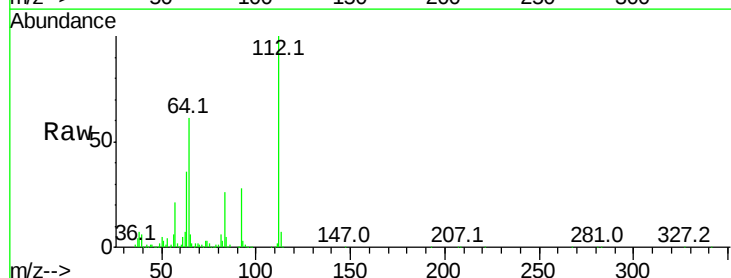

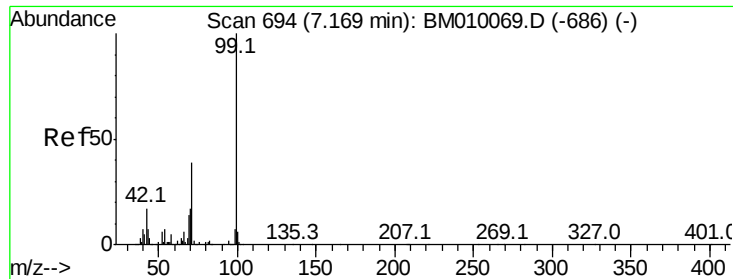

#7

Phenol-d6

Concen: 117.07 ng

RT: 7.16 min Scan# 692

Delta R.T. -0.01 min

Lab File: BM010103.D

Acq: 22 May 2017 15:35

Instrument :

BNA_M

ClientSampled :


Tot Ion: 99 Resp: 1327602

Ion Ratio Lower Upper

99 100

42 18.2 11.0 16.4#




71 44.6 23.4 35.2#

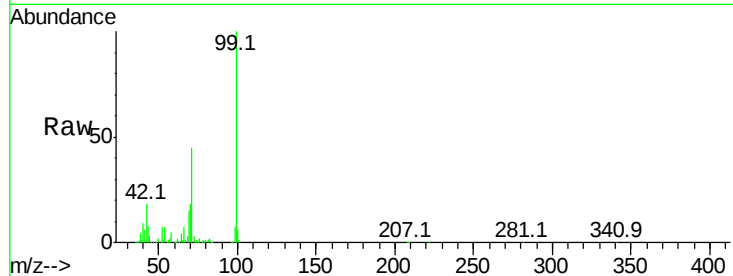

Abundance Ion 99.00 (98.70 to 99.70): BM010069.D (-686) (-)

Ion 42.00 (41.70 to 42.70): BM010069.D (-686) (-)

Ion 71.00 (70.70 to 71.70): BM010069.D (-686) (-)

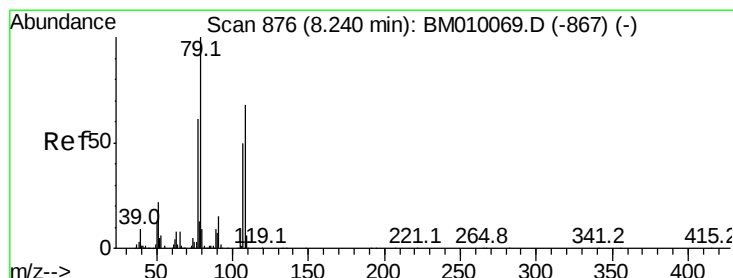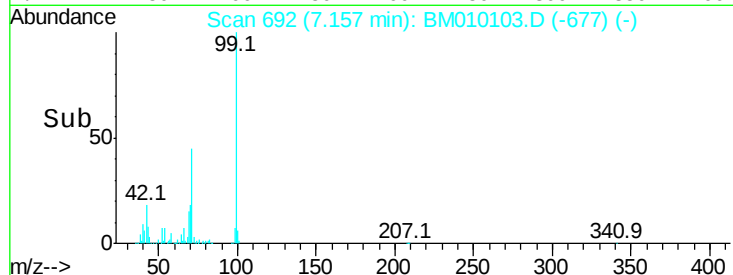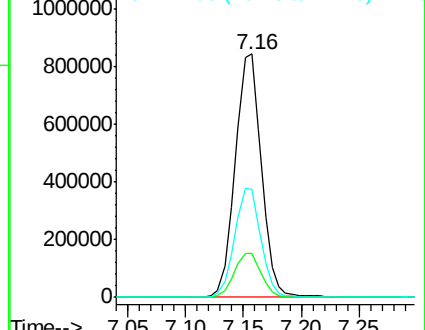

#15

Benzyl Alcohol

Concen: 2.19 ng

RT: 8.29 min Scan# 884

Delta R.T. 0.05 min

Lab File: BM010103.D

Acq: 22 May 2017 15:35


Tgt Ion: 79 Resp: 18816

Ion Ratio Lower Upper

79 100

108 37.7 65.0 97.4#



77 139.5 53.0 79.6#

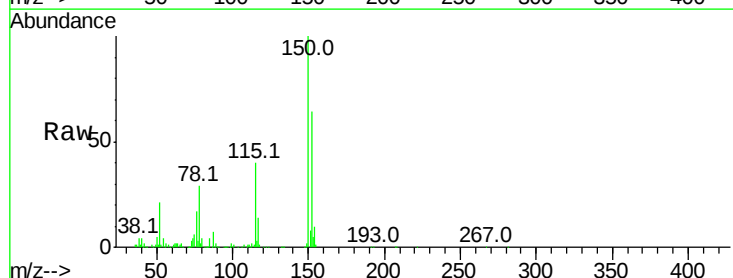

Abundance Ion 79.00 (78.70 to 79.70): BM010069.D (-867) (-)

Ion 108.00 (107.70 to 108.70): BM010069.D (-867) (-)

Ion 77.00 (76.70 to 77.70): BM010069.D (-867) (-)



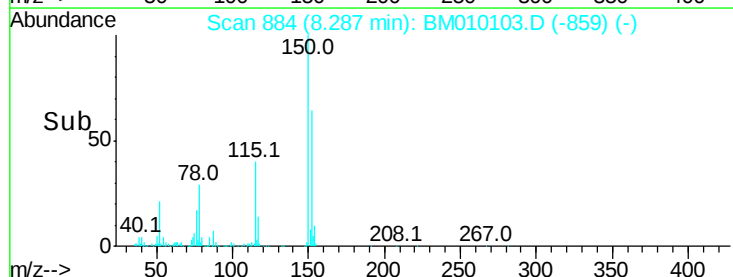
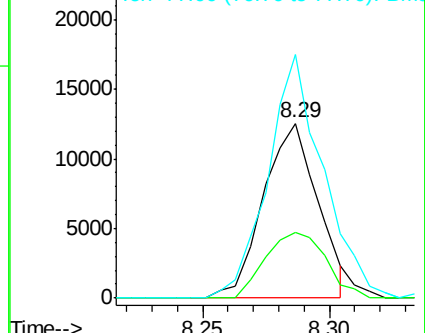




#21
Naphthalene-d8
Concen: 20.00 ng
RT: 10.77 min Scan# 1307
Delta R.T. -0.01 min
Lab File: BM010103.D
Acq: 22 May 2017 15:35




Instrument :
BNA_M
ClientSampled :


Tot Ion:136	Resp:	508758
Ion Ratio	Lower	Upper
136	100	
137	10.8	8.7 13.1
54	5.9	4.6 6.8
68	5.5	3.7 5.5

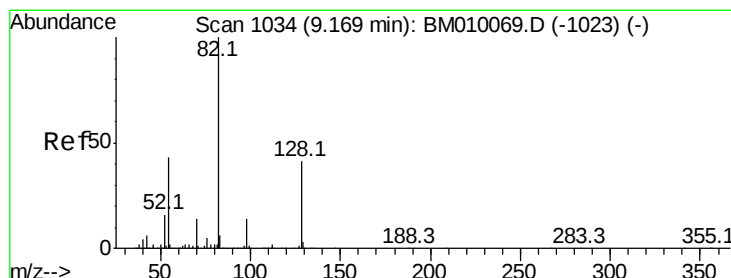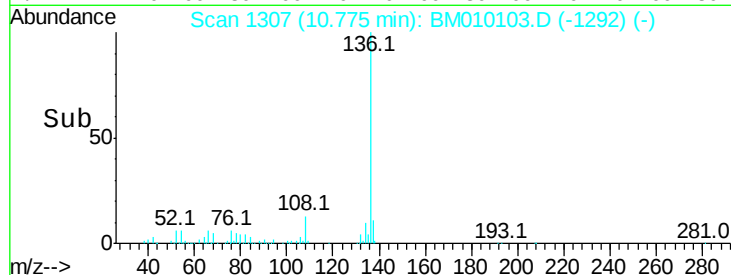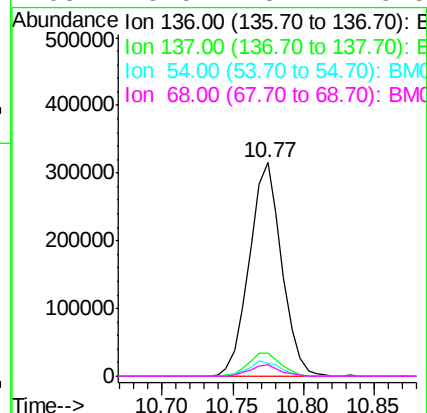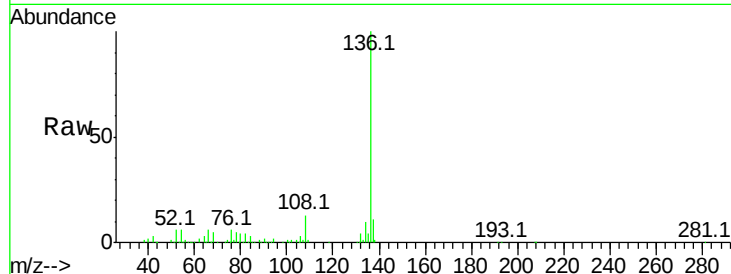

#23
Nitrobenzene-d5
Concen: 90.73 ng
RT: 9.15 min Scan# 1031
Delta R.T. -0.02 min
Lab File: BM010103.D
Acq: 22 May 2017 15:35

Tgt Ion: 82	Resp:	855572
Ion Ratio	Lower	Upper
82	100	
128	34.9	32.8 49.2
54	45.9	40.6 60.8

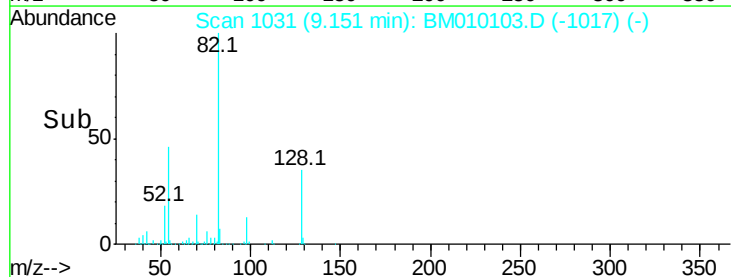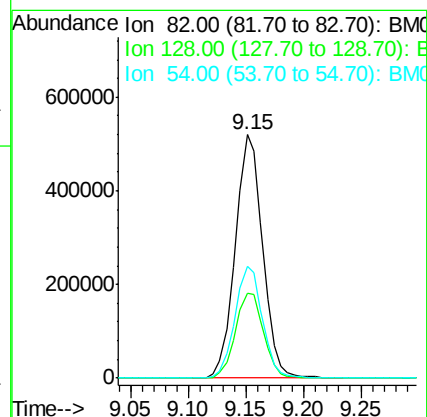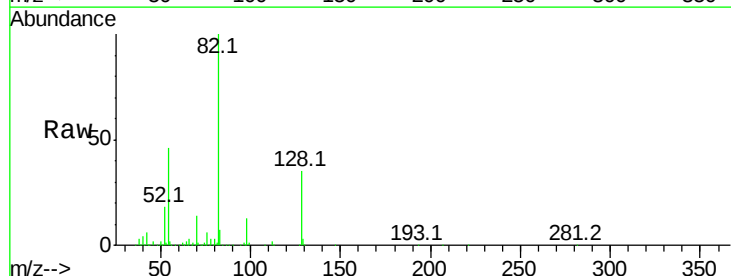

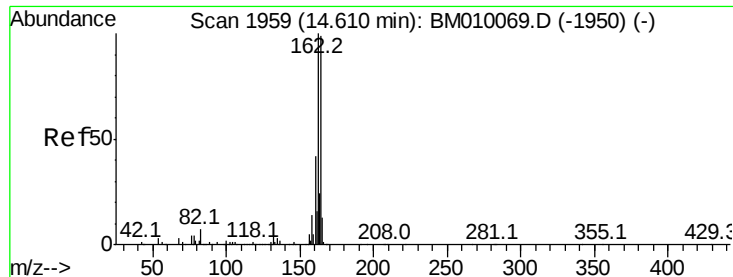

#38

Acenaphthene-d10

Concen: 20.00 ng

RT: 14.60 min Scan# 1957

Delta R.T. -0.01 min

Lab File: BM010103.D

Acq: 22 May 2017 15:35

Instrument :

BNA_M

ClientSampleId :


Tot Ion:164 Resp: 305668

Ion Ratio Lower Upper

164 100

162 99.3 82.4 123.6




160 45.7 35.8 53.6

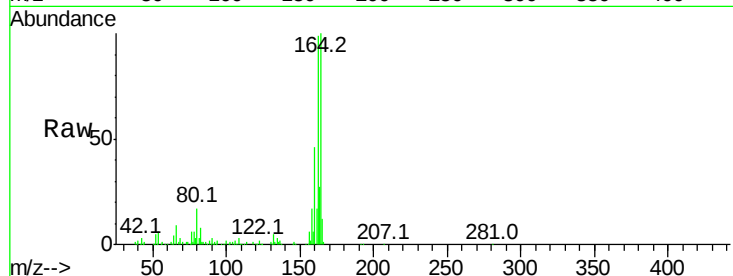

Abundance Ion 164.00 (163.70 to 164.70): E

Ion 162.00 (161.70 to 162.70): E

Ion 160.00 (159.70 to 160.70): E

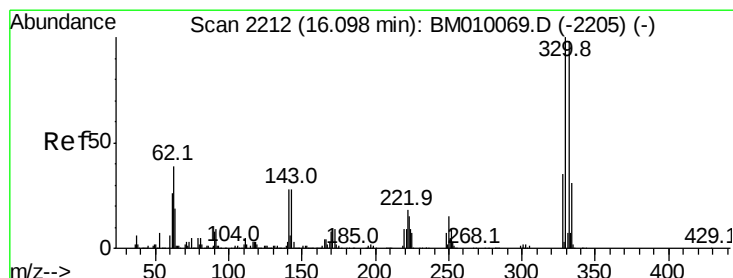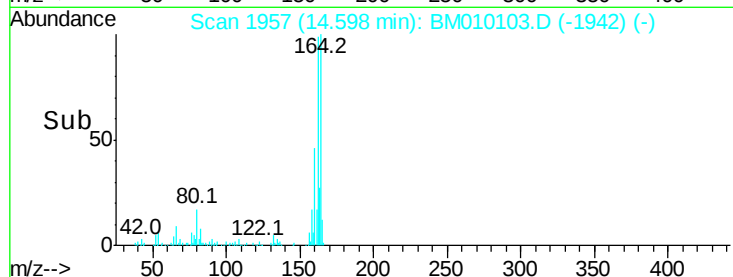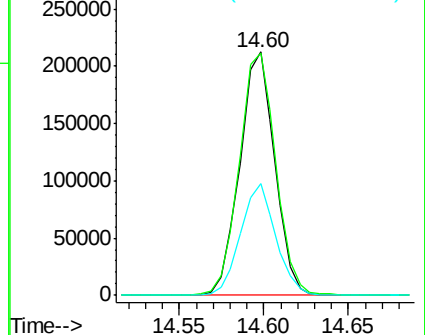

#41

2,4,6-Tribromophenol

Concen: 120.28 ng

RT: 16.09 min Scan# 2210

Delta R.T. -0.01 min

Lab File: BM010103.D

Acq: 22 May 2017 15:35


Tgt Ion:330 Resp: 558404

Ion Ratio Lower Upper

330 100

332 95.5 0.0 0.0#



141 30.9 0.0 0.0#

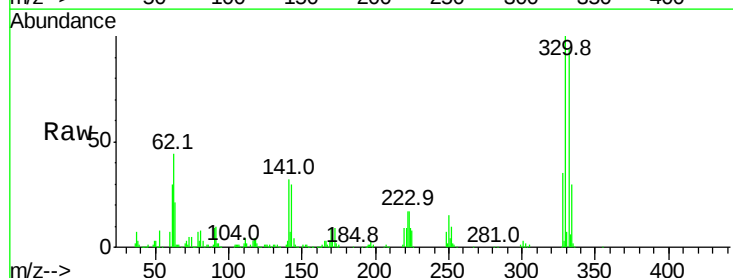

Abundance Ion 329.80 (329.50 to 330.50): E

Ion 331.80 (331.50 to 332.50): E

Ion 141.00 (140.70 to 141.70): E



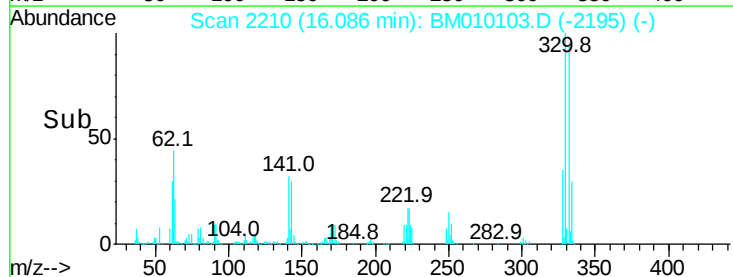
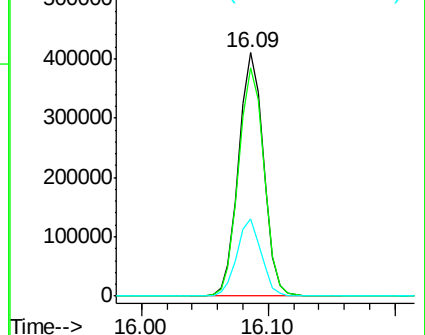




#44
2-Fluorobiphenyl
Concen: 89.71 ng
RT: 13.22 min Scan# 1723
Delta R.T. -0.01 min
Lab File: BM010103.D
Acq: 22 May 2017 15:35




Instrument :
BNA_M
ClientSampleId :


Tot Ion:172 Resp: 2132981
Ion Ratio Lower Upper
172 100
171 35.6 28.5 42.7
170 23.3 18.8 28.2

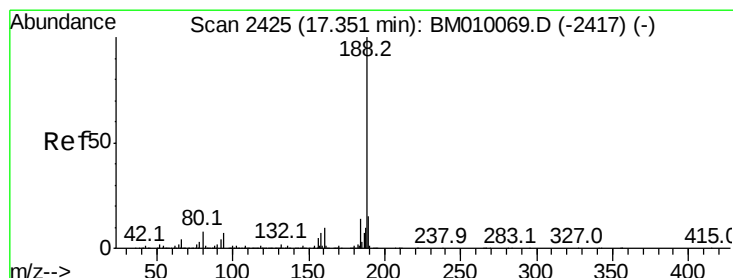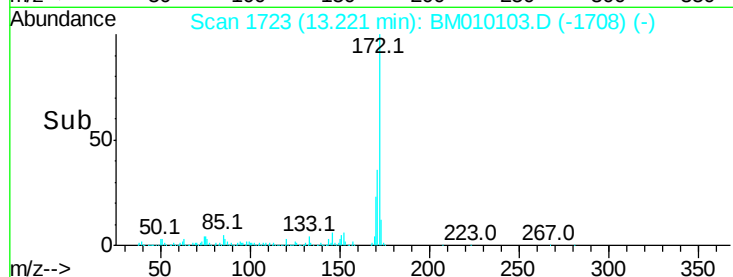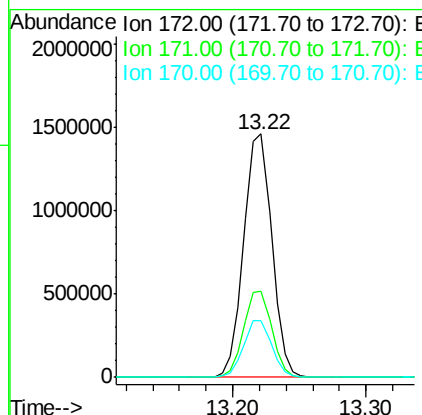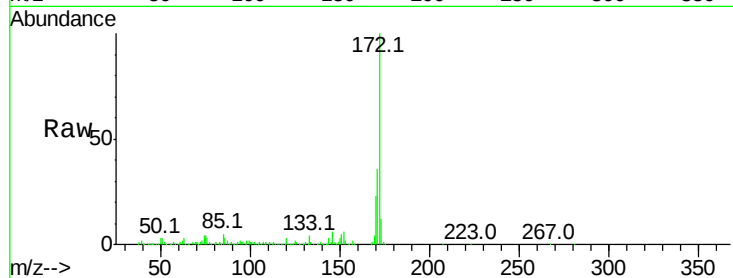

#63
Phenanthrene-d10
Concen: 20.00 ng
RT: 17.34 min Scan# 2423
Delta R.T. -0.01 min
Lab File: BM010103.D
Acq: 22 May 2017 15:35

Tgt Ion:188 Resp: 727617
Ion Ratio Lower Upper
188 100
94 5.4 8.7 13.1#
80 7.2 9.3 13.9#

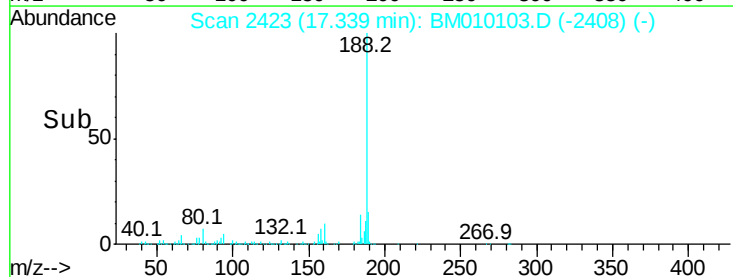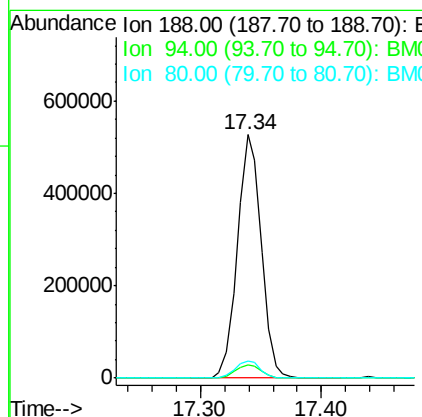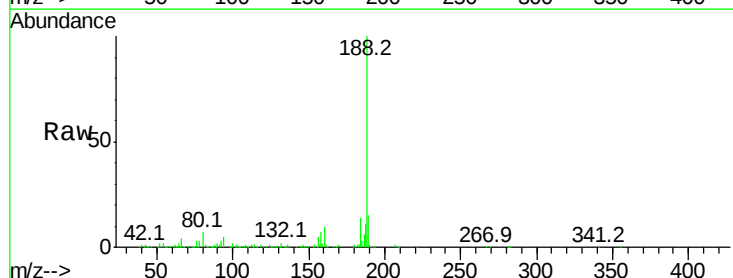

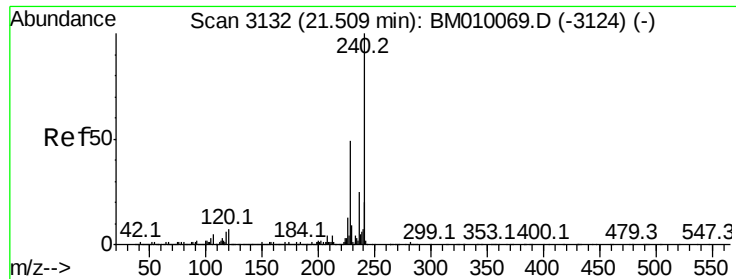

#75

Chrysene-d12

Concen: 20.00 ng

RT: 21.50 min Scan# 3130

Delta R.T. -0.01 min

Lab File: BM010103.D

Acq: 22 May 2017 15:35

Instrument :

BNA_M

ClientSampleID :


Tot Ion:240 Resp: 1089702

Ion Ratio Lower Upper

240 100

120 5.7 8.2 12.2#




236 24.5 20.0 30.0

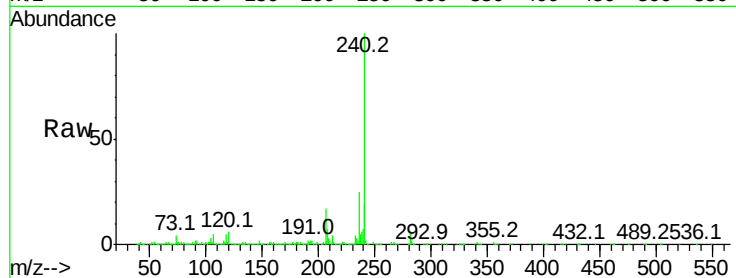

Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

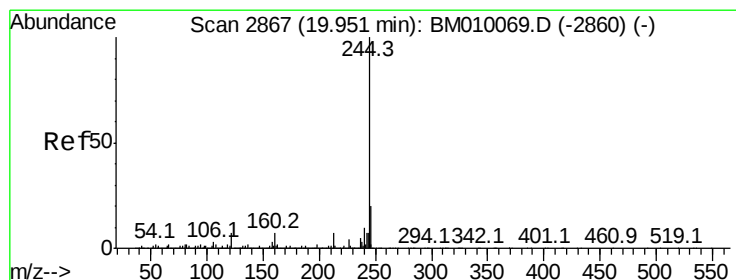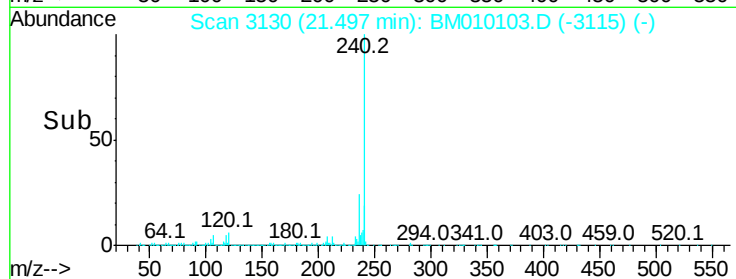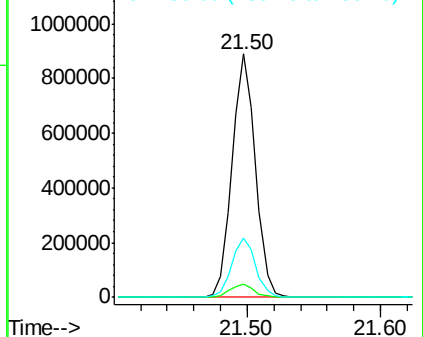

#78

Terphenyl-d14

Concen: 73.48 ng

RT: 19.94 min Scan# 2865

Delta R.T. -0.01 min

Lab File: BM010103.D

Acq: 22 May 2017 15:35


Tgt Ion:244 Resp: 3521459

Ion Ratio Lower Upper

244 100

212 7.1 4.9 7.3



122 6.9 6.2 9.4

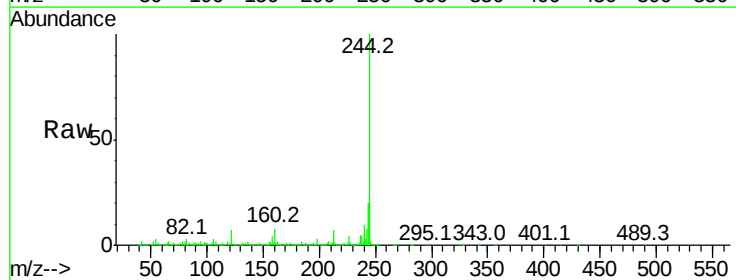


Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

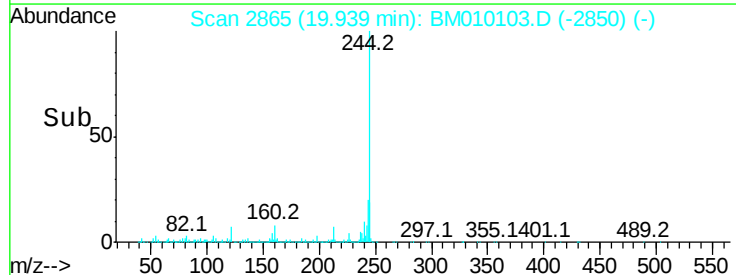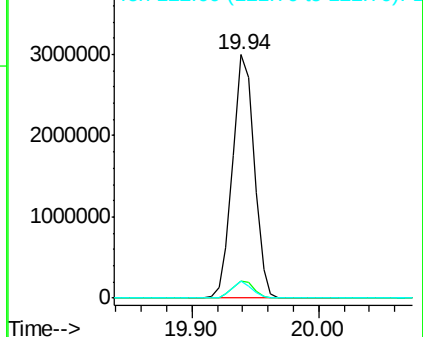

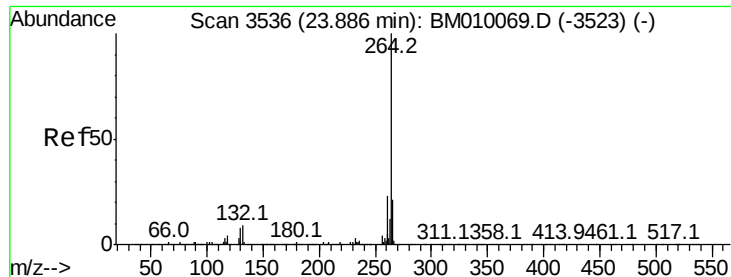

#86
Pervlene-d12
Concen: 20.00 ng
RT: 23.87 min Scan# 3533
Delta R.T. -0.02 min
Lab File: BM010103.D
Acq: 22 May 2017 15:35

Instrument :
BNA_M
ClientSampleId :

Tot Ion: 264 Resp: 1260317

Ion	Ratio	Lower	Upper
264	100		
260	23.5	18.6	27.8
265	21.9	17.3	25.9

