

Data Path : Z:\HPCHEM1\BNA M\DATA\BM052217\
 Data File : BM010121.D
 Acq On : 23 May 2017 02:23
 Operator : SJ/MA
 Sample : I3222-06
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :

Quant Time: May 23 05:33:14 2017
 Quant Method : Z:\HPCHEM1\BNA M\METHODS\8270-BM051917.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat May 20 04:25:49 2017
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.96	152	138988	20.00	ng	-0.01
21) Naphthalene-d8	10.77	136	477766	20.00	ng	-0.02
38) Acenaphthene-d10	14.59	164	301579	20.00	ng	-0.02
63) Phenanthrene-d10	17.34	188	759251	20.00	ng	-0.01
75) Chrysene-d12	21.50	240	1163815	20.00	ng	-0.01
86) Perylene-d12	23.86	264	1318988	20.00	ng	-0.02
System Monitoring Compounds						
5) 2-Fluorophenol	5.55	112	1279843	166.29	ng	-0.01
7) Phenol-d6	7.15	99	1564483	157.97	ng	-0.02
23) Nitrobenzene-d5	9.15	82	1003321	113.30	ng	-0.02
41) 2,4,6-Tribromophenol	16.09	330	758810	165.67	ng	-0.01
44) 2-Fluorobiphenyl	13.22	172	2392410	101.98	ng	-0.02
78) Terphenyl-d14	19.94	244	4312164	84.25	ng	-0.01
Target Compounds						
10) Phenol	7.17	94	33823	3.24	ng	Qvalue 89
15) Benzyl Alcohol	8.28	79	21311	2.84	ng	# 32
49) Dimethylphthalate	14.05	163	164387	6.11	ng	# 98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA M\DATA\BM052217\
Data File : BM010121.D
Acq On : 23 May 2017 02:23
Operator : SJ/MA
Sample : I3222-06
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :

Quant Time: May 23 05:33:14 2017
Quant Method : Z:\HPCHEM1\BNA M\METHODS\8270-BM051917.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat May 20 04:25:49 2017
Response via : Initial Calibration

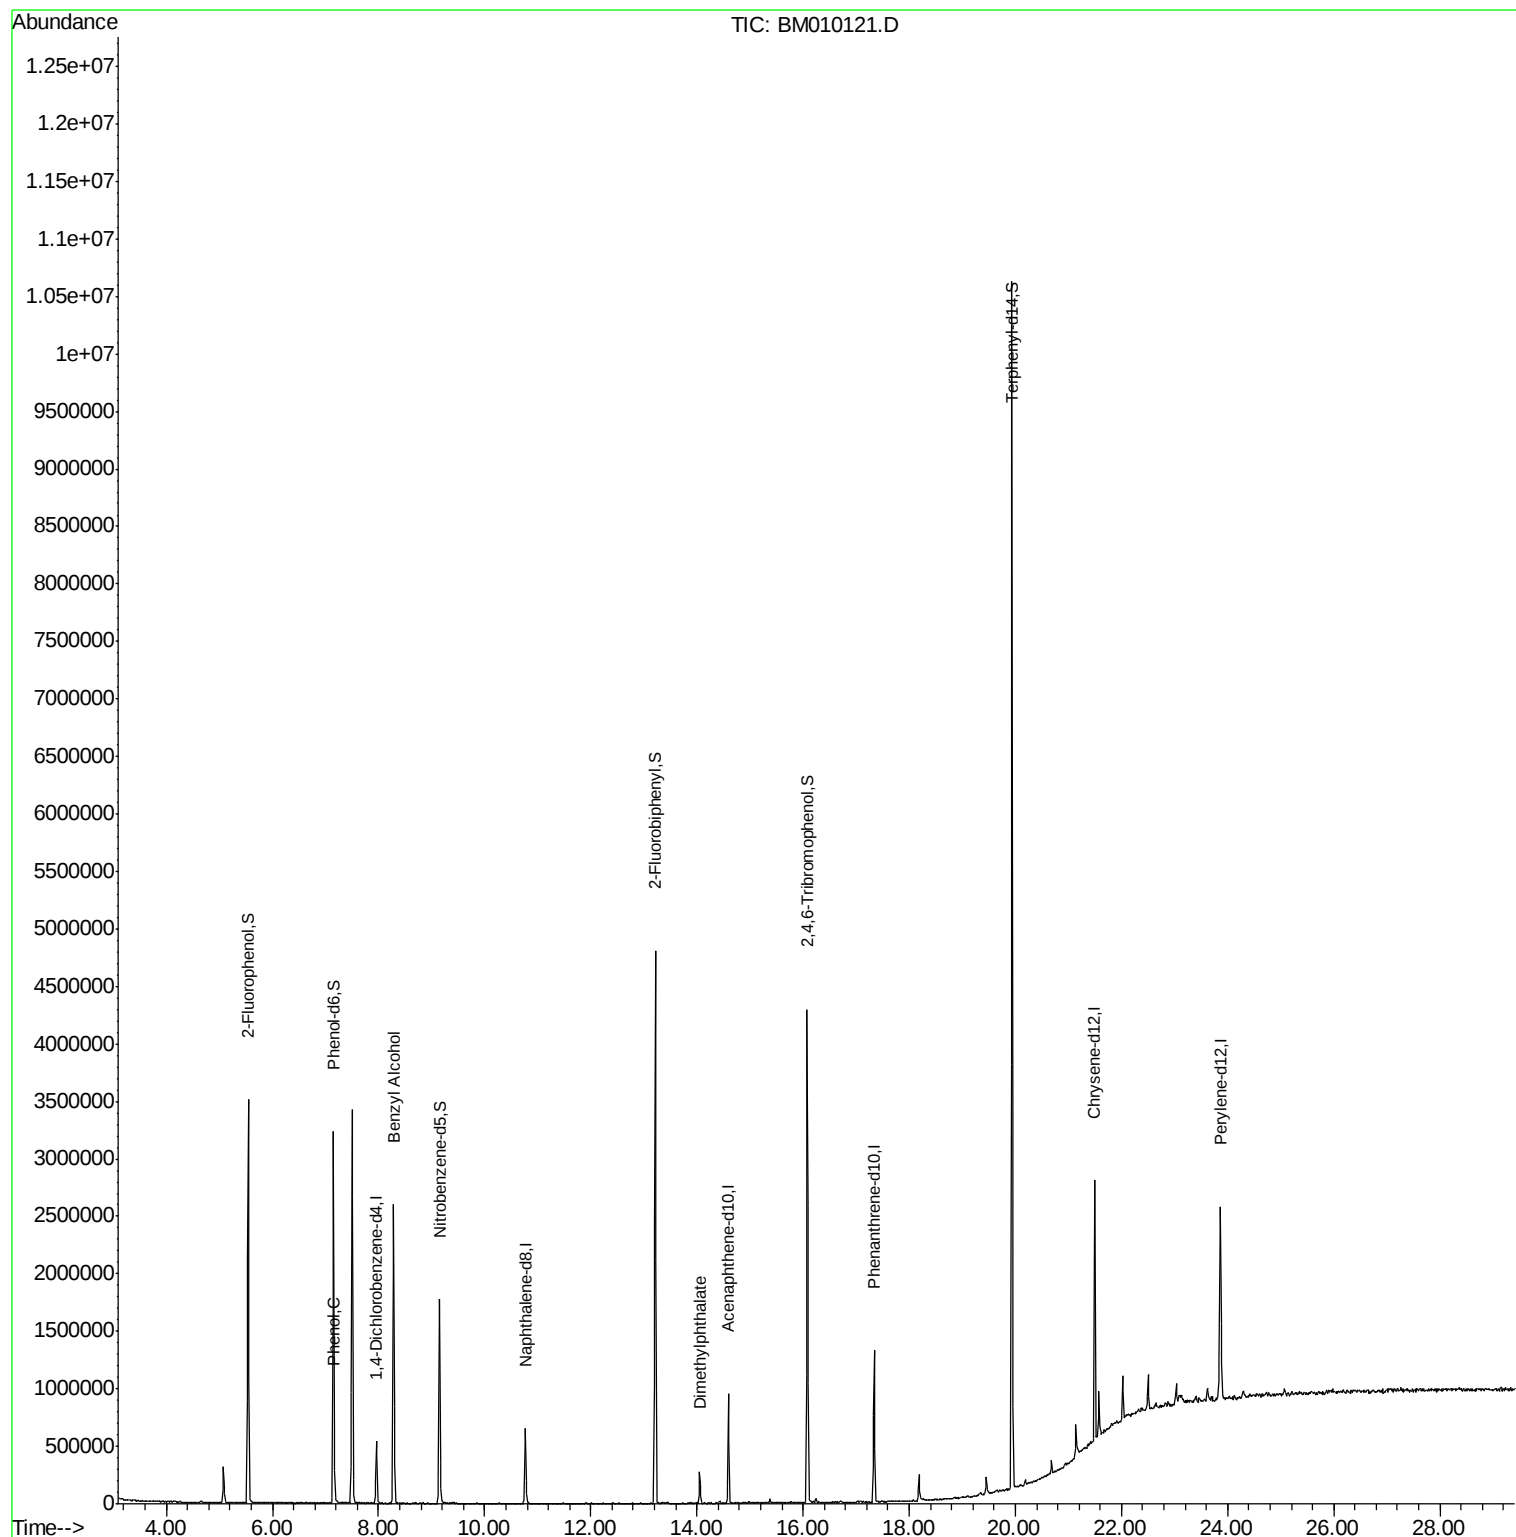

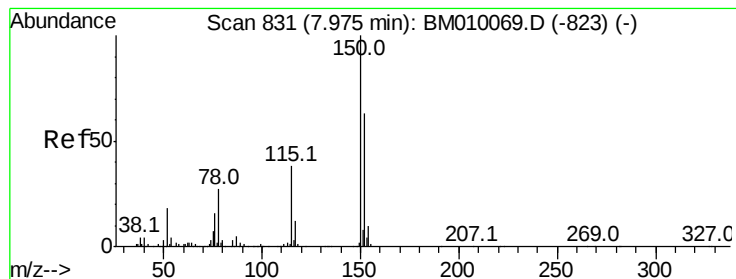

#1

1,4-Dichlorobenzene-d4

Concen: 20.00 ng

RT: 7.96 min Scan# 829

Delta R.T. -0.01 min

Lab File: BM010121.D

Acq: 23 May 2017 02:23

Instrument :

BNA_M

ClientSampleId :


Tot Ion:152 Resp: 138988

Ion Ratio Lower Upper

152 100

150 147.2 119.5 179.3




115 55.4 43.0 64.4

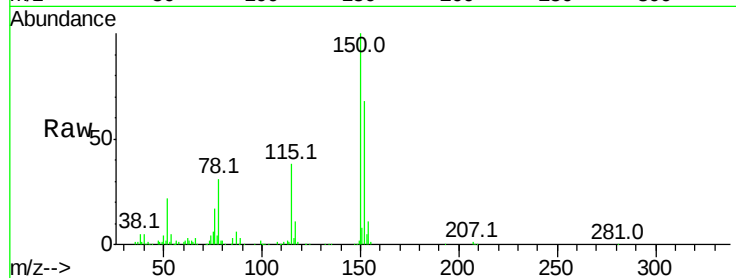

Abundance Ion 152.00 (151.70 to 152.70): E

Ion 150.00 (149.70 to 150.70): E

Ion 115.00 (114.70 to 115.70): E

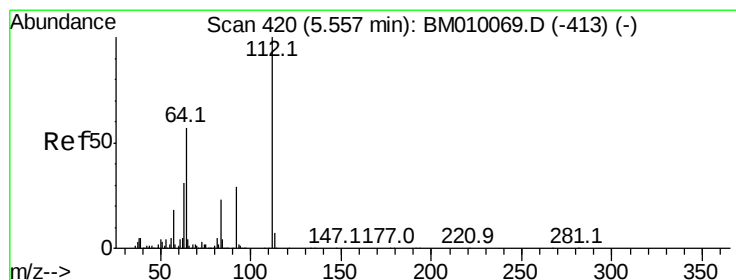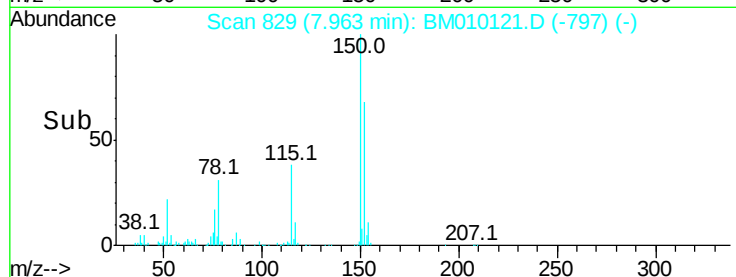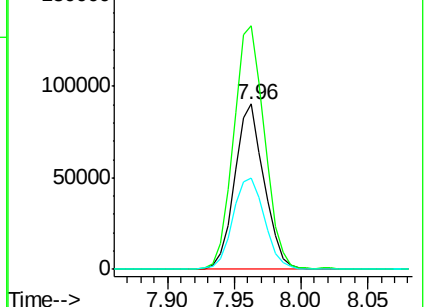

#5

2-Fluorophenol

Concen: 166.29 ng

RT: 5.55 min Scan# 418

Delta R.T. -0.01 min

Lab File: BM010121.D

Acq: 23 May 2017 02:23


Tgt Ion:112 Resp: 1279843

Ion Ratio Lower Upper

112 100

64 61.2 38.6 57.8#



63 35.8 19.3 28.9#



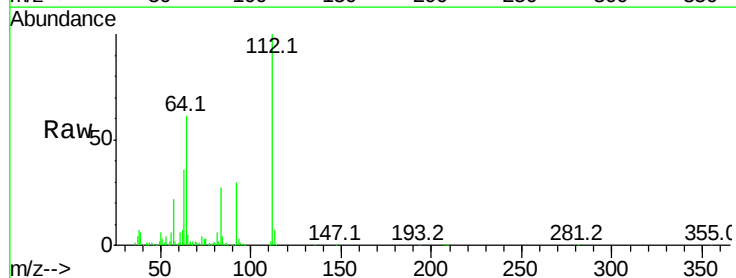


Abundance Ion 112.00 (111.70 to 112.70): E

Ion 64.00 (63.70 to 64.70): BM0

Ion 63.00 (62.70 to 63.70): BM0

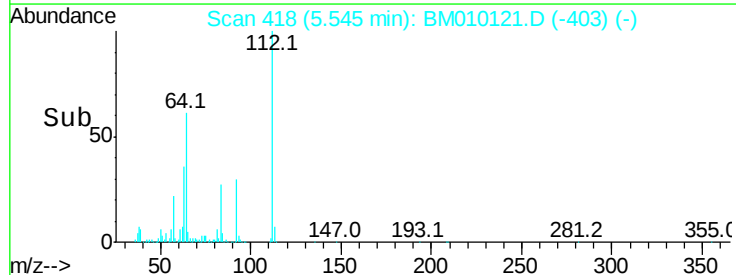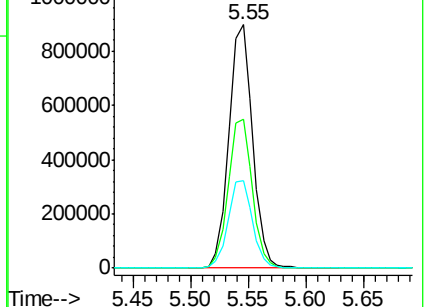

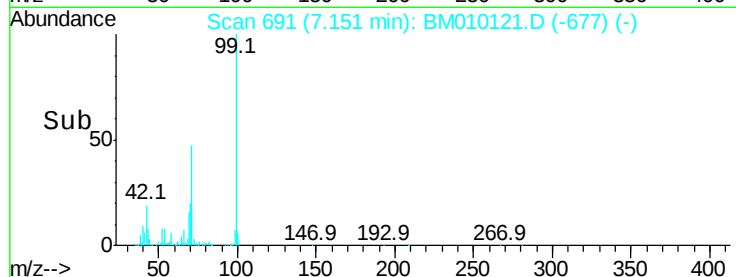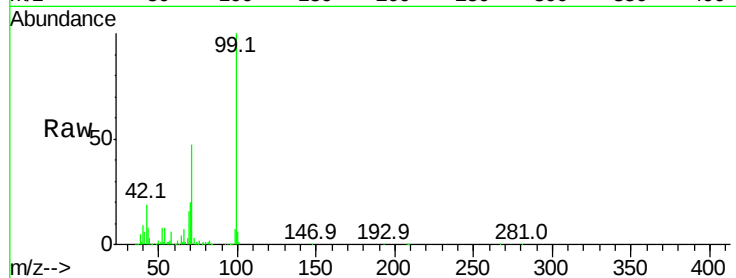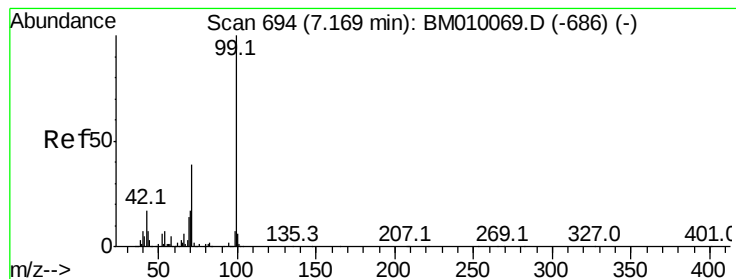

#7

Phenol-d6

Concen: 157.97 ng

RT: 7.15 min Scan# 691

Delta R.T. -0.02 min

Lab File: BM010121.D

Acq: 23 May 2017 02:23





Instrument :

BNA_M

ClientSampled :

Tot Ion: 99 Resp: 1564483

Ion	Ratio	Lower	Upper
99	100		
42	19.3	11.0	16.4#
71	47.2	23.4	35.2#

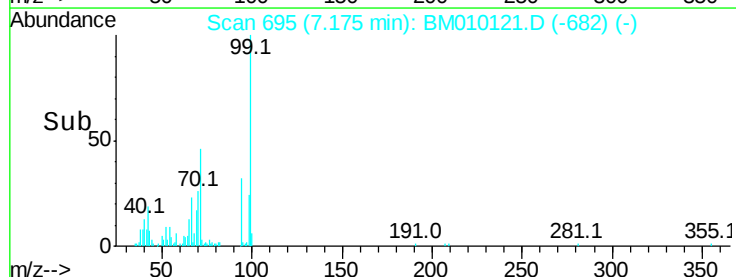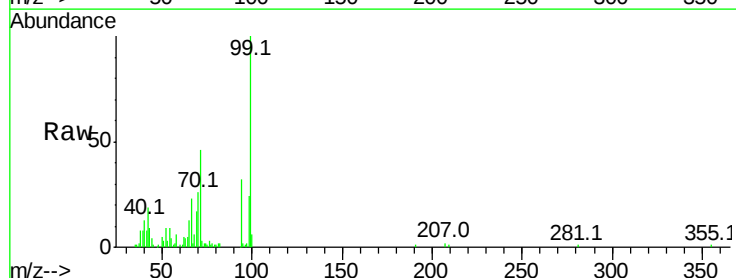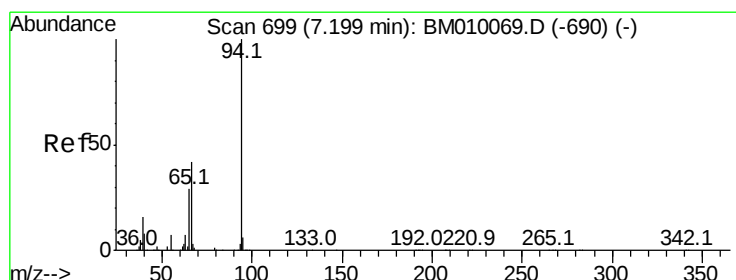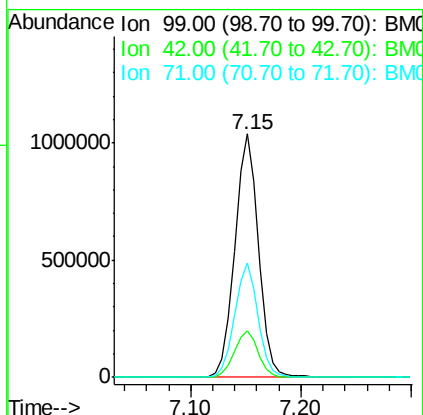

#10

Phenol

Concen: 3.24 ng

RT: 7.17 min Scan# 695


Delta R.T. -0.02 min


Lab File: BM010121.D

Acq: 23 May 2017 02:23

Tgt Ion: 94 Resp: 33823

Ion	Ratio	Lower	Upper
94	100		
65	41.1	18.8	58.8
66	71.3	39.9	79.9

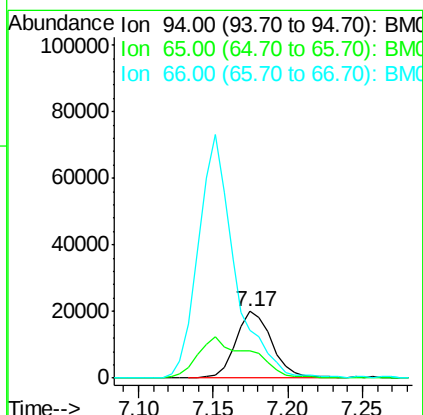

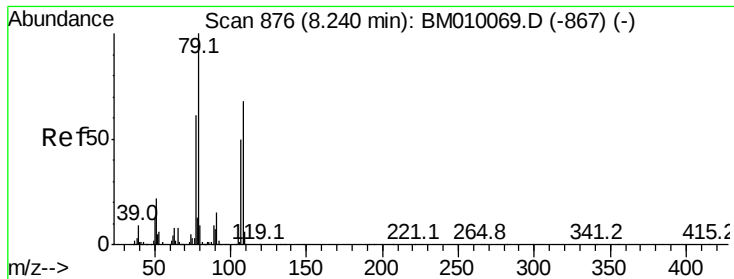

#15

Benzyl Alcohol

Concen: 2.84 ng

RT: 8.28 min Scan# 883

Delta R.T. 0.04 min

Lab File: BM010121.D

Acq: 23 May 2017 02:23

Instrument :

BNA_M

ClientSampleId :


Tot Ion: 79 Resp: 21311

Ion Ratio Lower Upper

79 100

108 42.5 65.0 97.4#




77 144.7 53.0 79.6#

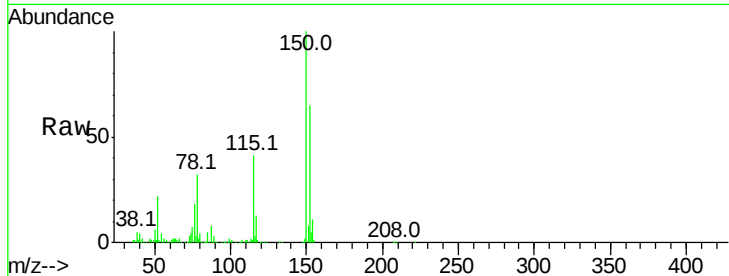

Abundance Ion 79.00 (78.70 to 79.70): BM010069.D (-867) (-)

Ion 108.00 (107.70 to 108.70): BM010069.D (-867) (-)

Ion 77.00 (76.70 to 77.70): BM010069.D (-867) (-)

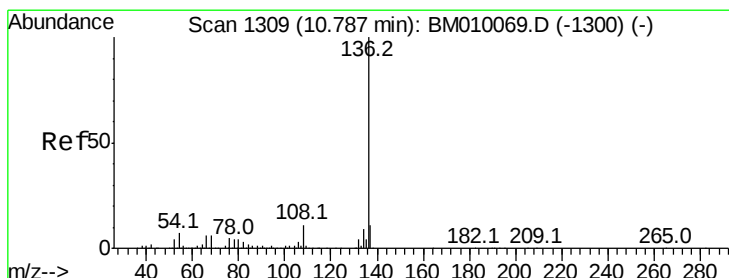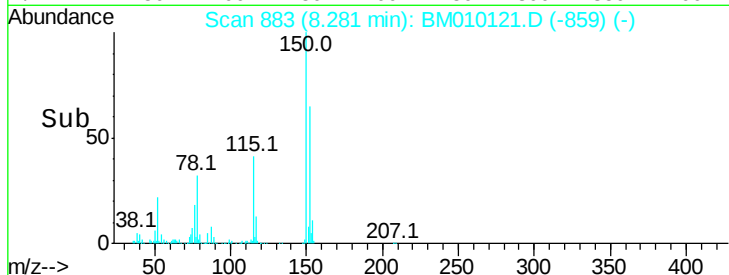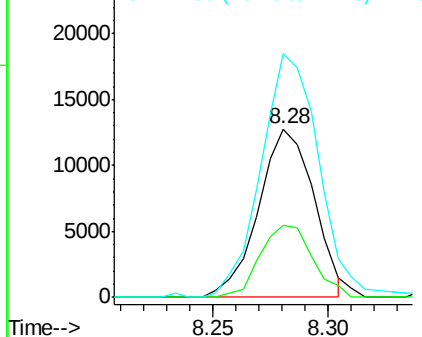

#21

Naphthalene-d8

Concen: 20.00 ng

RT: 10.77 min Scan# 1306

Delta R.T. -0.02 min

Lab File: BM010121.D

Acq: 23 May 2017 02:23

Tgt Ion: 136 Resp: 477766


Ion Ratio Lower Upper

136 100

137 11.4 8.7 13.1

54 7.3 4.6 6.8#

68 4.8 3.7 5.5


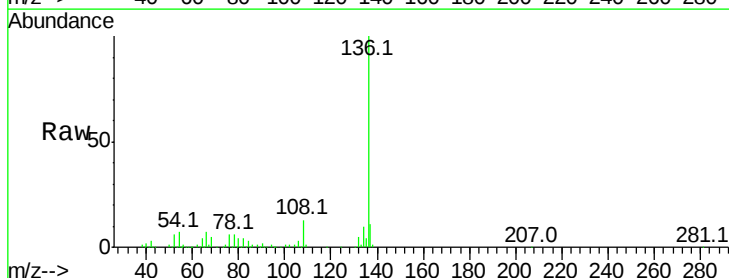



Abundance Ion 136.00 (135.70 to 136.70): BM010069.D (-1300) (-)

Ion 137.00 (136.70 to 137.70): BM010069.D (-1300) (-)

Ion 54.00 (53.70 to 54.70): BM010069.D (-1300) (-)

Ion 68.00 (67.70 to 68.70): BM010069.D (-1300) (-)



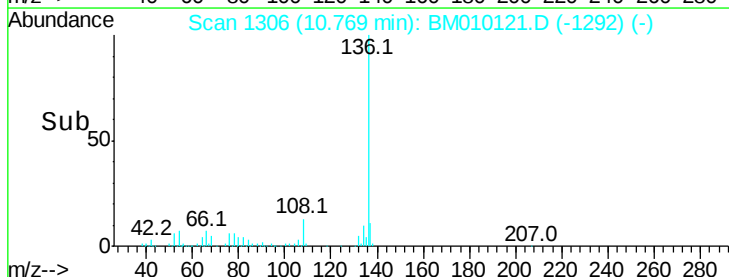
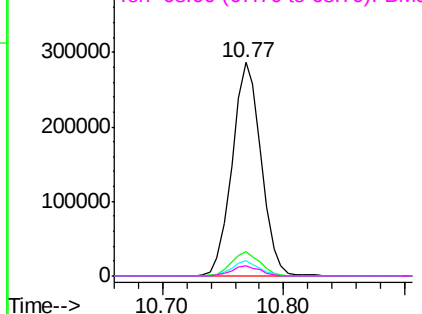


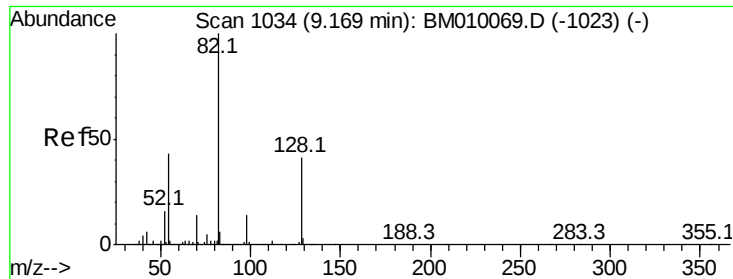

#23
 Nitrobenzene-d5
 Concen: 113.30 ng
 RT: 9.15 min Scan# 1031
 Delta R.T. -0.02 min
 Lab File: BM010121.D
 Acq: 23 May 2017 02:23




Instrument :
 BNA_M
 ClientSampleId :


Tot Ion	82	Resp	1003321
Ion	Ratio	Lower	Upper
82	100		
128	35.7	32.8	49.2
54	46.8	40.6	60.8

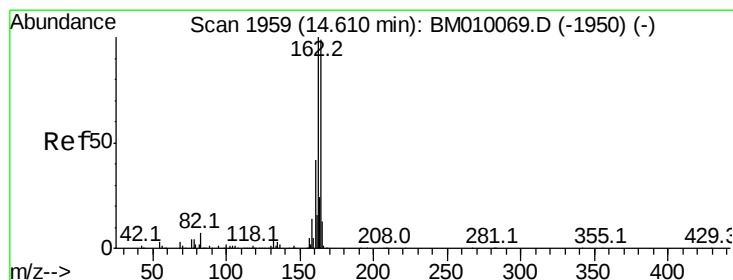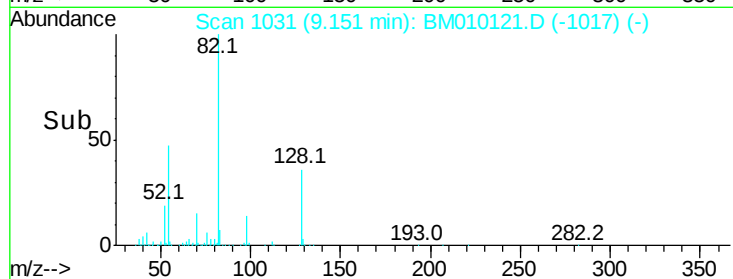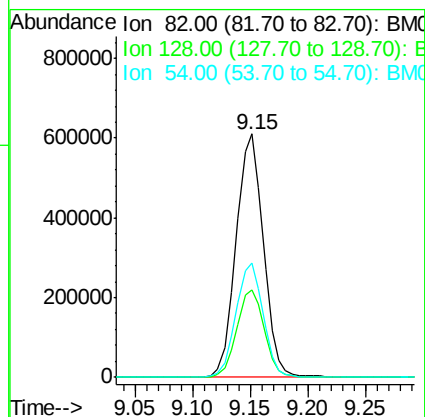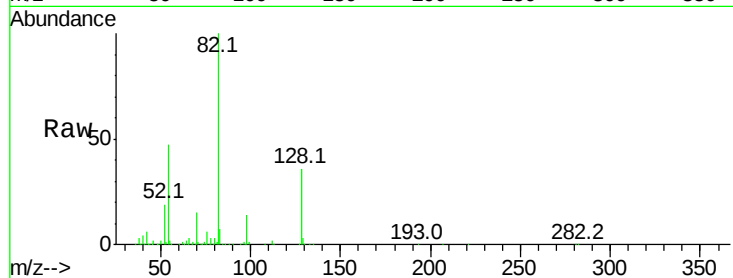

#38
 Acenaphthene-d10
 Concen: 20.00 ng
 RT: 14.59 min Scan# 1956
 Delta R.T. -0.02 min
 Lab File: BM010121.D
 Acq: 23 May 2017 02:23

Tgt Ion	164	Resp	301579
Ion	Ratio	Lower	Upper
164	100		
162	103.7	82.4	123.6
160	44.3	35.8	53.6

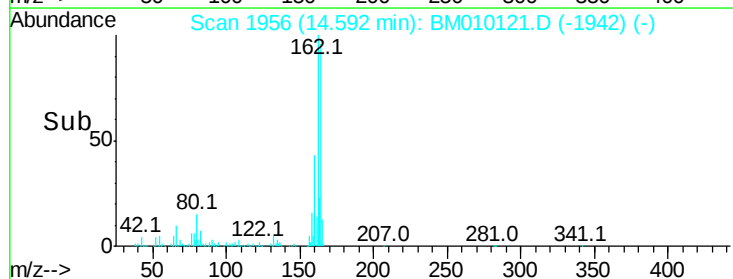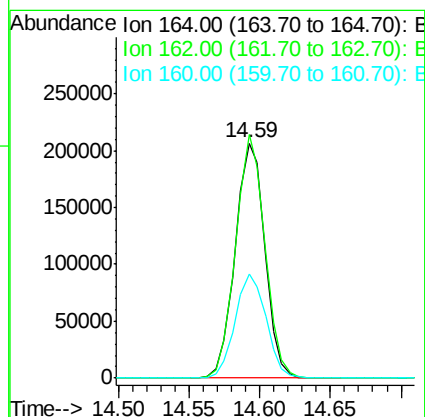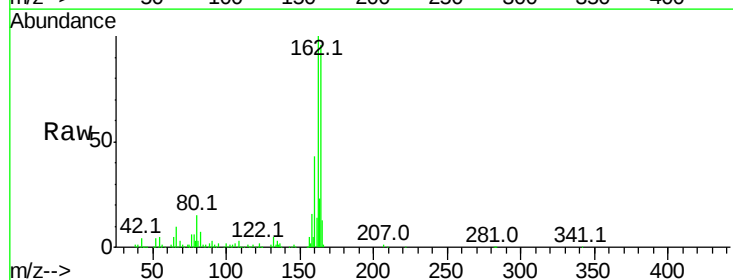


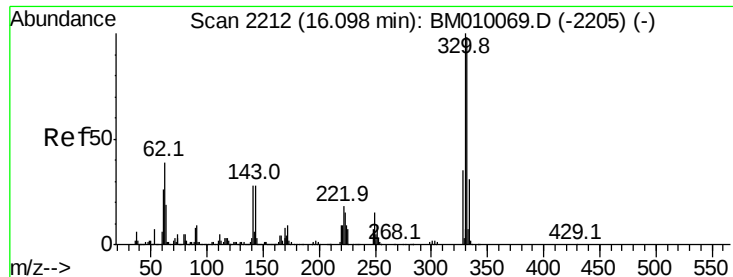




#41
2,4,6-Tribromophenol
Concen: 165.67 ng
RT: 16.09 min Scan# 2210
Delta R.T. -0.01 min
Lab File: BM010121.D
Acq: 23 May 2017 02:23

Instrument :
BNA_M
ClientSampleId :

Tot Ion:330 Resp: 758810
Ion Ratio Lower Upper
330 100
332 97.9 0.0 0.0#
141 31.6 0.0 0.0#

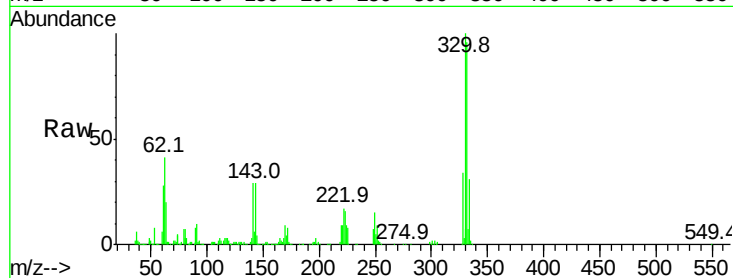


Abundance Ion 329.80 (329.50 to 330.50): E
Ion 331.80 (331.50 to 332.50): E
Ion 141.00 (140.70 to 141.70): E

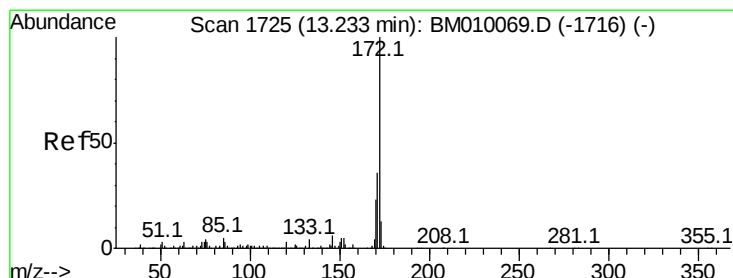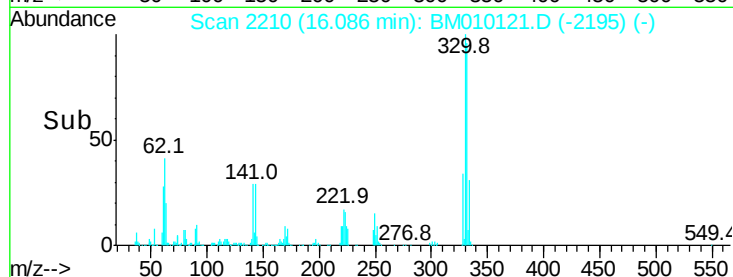
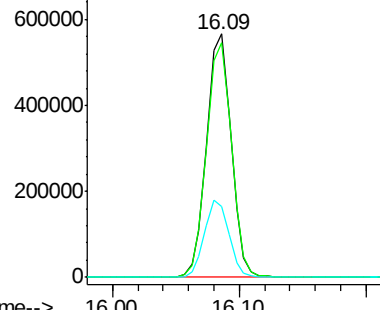



#44
2-Fluorobiphenyl
Concen: 101.98 ng
RT: 13.22 min Scan# 1722
Delta R.T. -0.02 min
Lab File: BM010121.D
Acq: 23 May 2017 02:23

Tgt Ion:172 Resp: 2392410
Ion Ratio Lower Upper
172 100
171 35.1 28.5 42.7
170 23.0 18.8 28.2

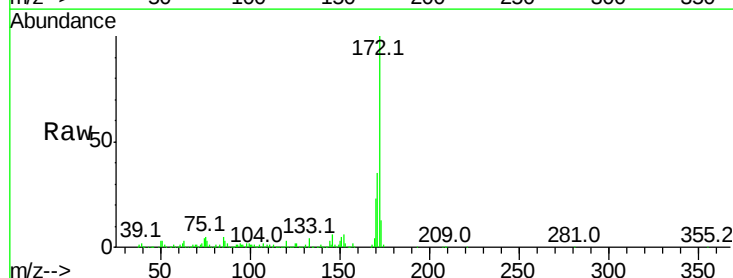

Abundance Ion 172.00 (171.70 to 172.70): E
Ion 171.00 (170.70 to 171.70): E
Ion 170.00 (169.70 to 170.70): E

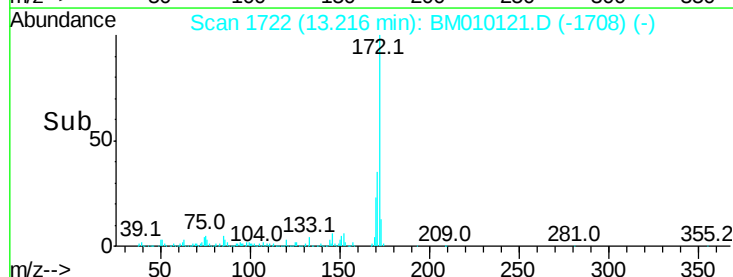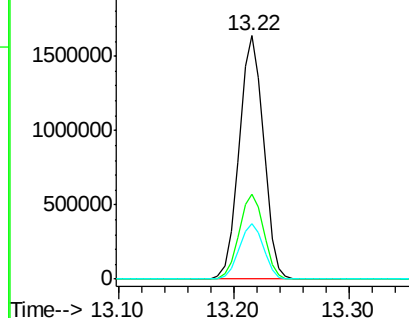

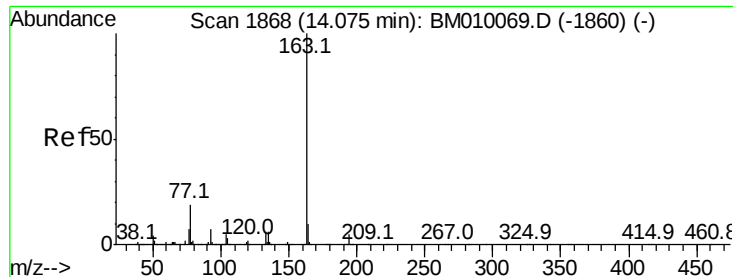

#49

Dimethylphthalate

Concen: 6.11 ng

RT: 14.05 min Scan# 1864

Delta R.T. -0.02 min

Lab File: BM010121.D





Acq: 23 May 2017 02:23

Instrument :

BNA_M

ClientSampleId :

Tot Ion:163	Resp: 164387
Ion Ratio	Lower Upper
163 100	
194 4.3	2.7 4.1#
164 11.0	8.2 12.2

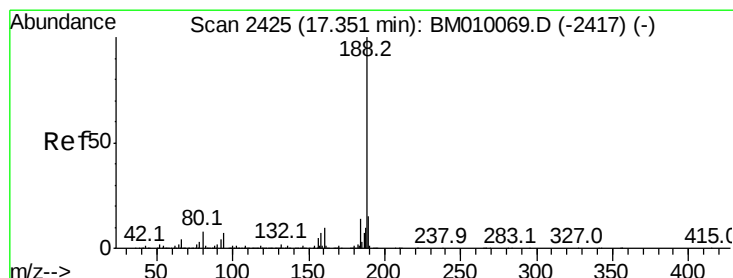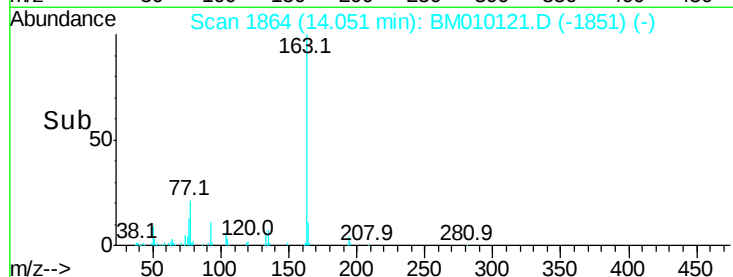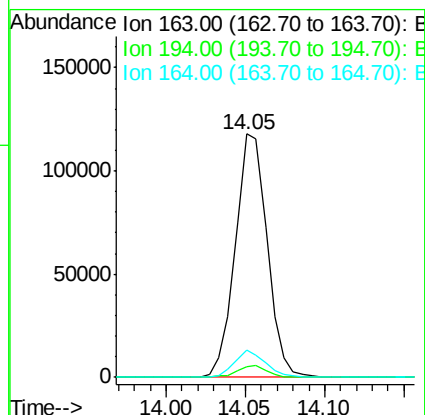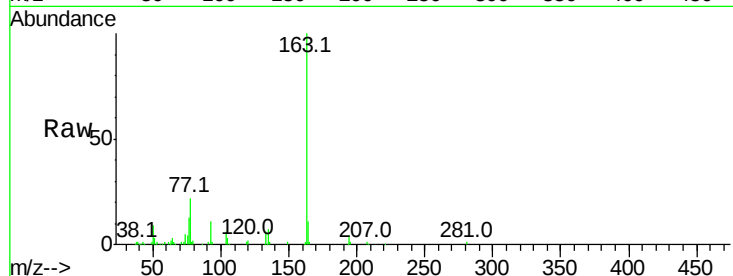

#63

Phenanthrene-d10

Concen: 20.00 ng




RT: 17.34 min Scan# 2423


Delta R.T. -0.01 min

Lab File: BM010121.D

Acq: 23 May 2017 02:23

Tgt Ion	Ion:188	Resp:	759251
	Ratio	Lower	Upper
188	100		
94	5.9	8.7	13.1#
80	6.8	9.3	13.9#

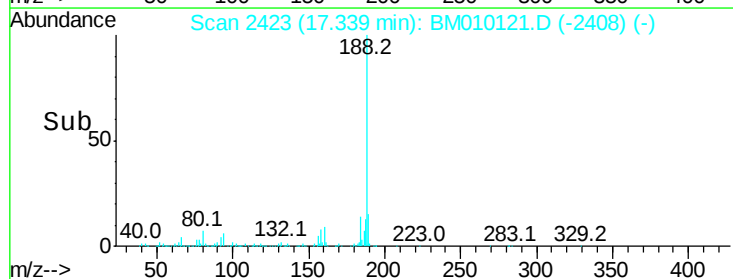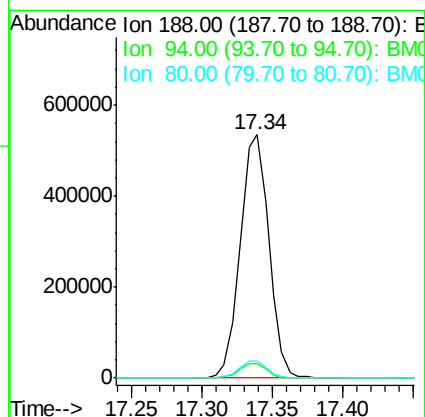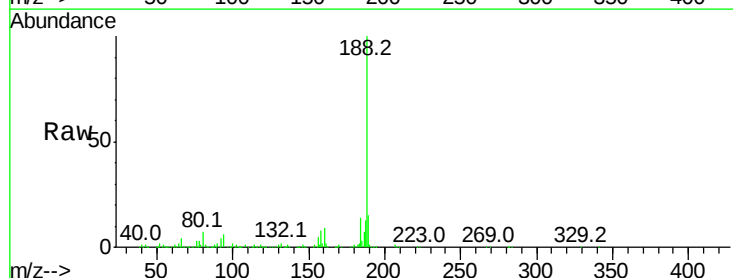

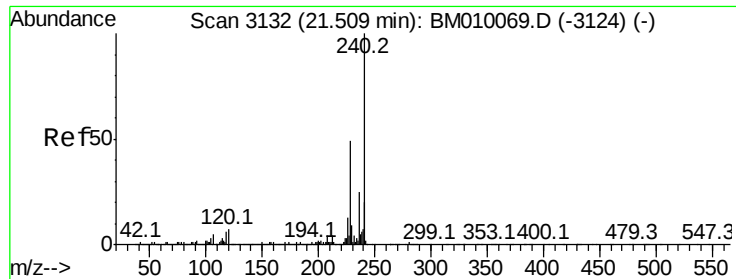

#75

Chrysene-d12

Concen: 20.00 ng

RT: 21.50 min Scan# 3130

Delta R.T. -0.01 min

Lab File: BM010121.D

Acq: 23 May 2017 02:23

Instrument :

BNA_M

ClientSampleId :


Tot Ion:240 Resp: 1163815

Ion	Ratio	Lower	Upper
240	100		
120	5.2	8.2	12.2#
236	25.7	20.0	30.0

240 100

120 5.2 8.2 12.2#

236 25.7 20.0 30.0



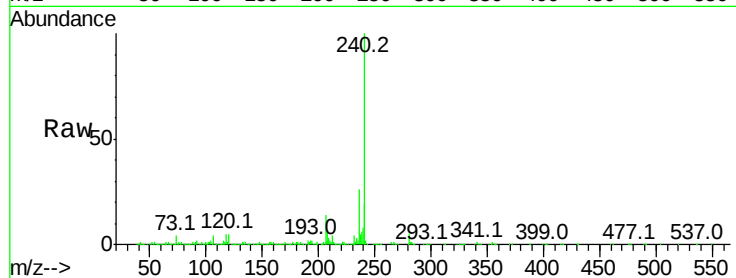


Abundance

Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

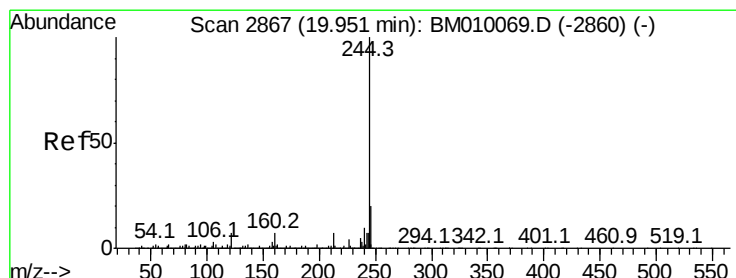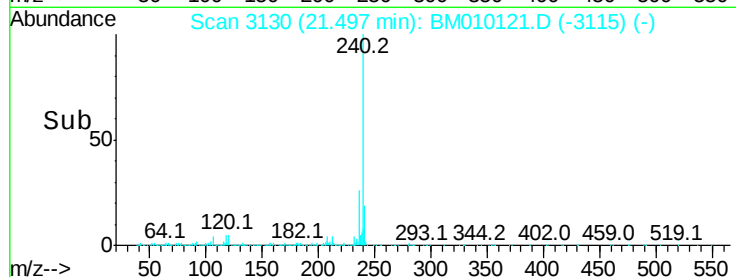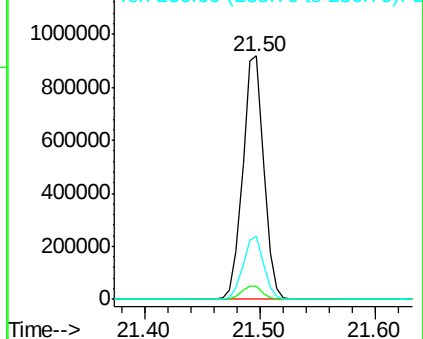

#78

Terphenyl-d14

Concen: 84.25 ng

RT: 19.94 min Scan# 2865

Delta R.T. -0.01 min

Lab File: BM010121.D

Acq: 23 May 2017 02:23


Tgt Ion:244 Resp: 4312164

Ion	Ratio	Lower	Upper
244	100		
212	7.4	4.9	7.3#
122	6.4	6.2	9.4

244 100

212 7.4 4.9 7.3#

122 6.4 6.2 9.4


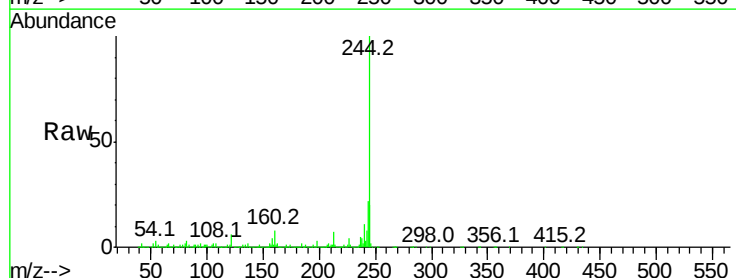



Abundance

Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

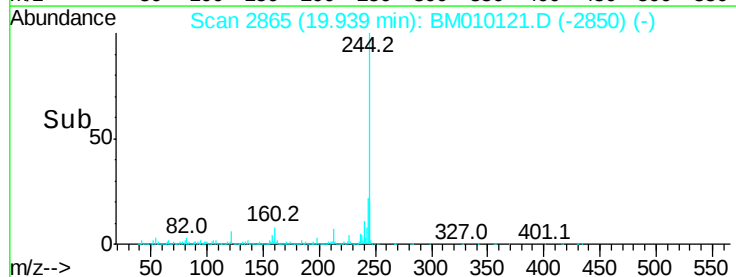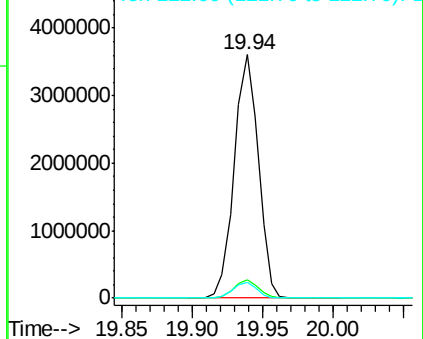

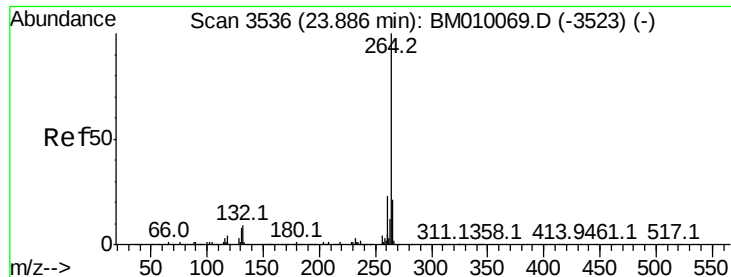

#86
Pervlene-d12
Concen: 20.00 ng
RT: 23.86 min Scan# 3532
Delta R.T. -0.02 min
Lab File: BM010121.D
Acq: 23 May 2017 02:23

Instrument :
BNA_M
ClientSampleId :

Tot Ion:264 Resp: 1318988

Ion	Ratio	Lower	Upper
264	100		
260	23.0	18.6	27.8
265	21.9	17.3	25.9

