
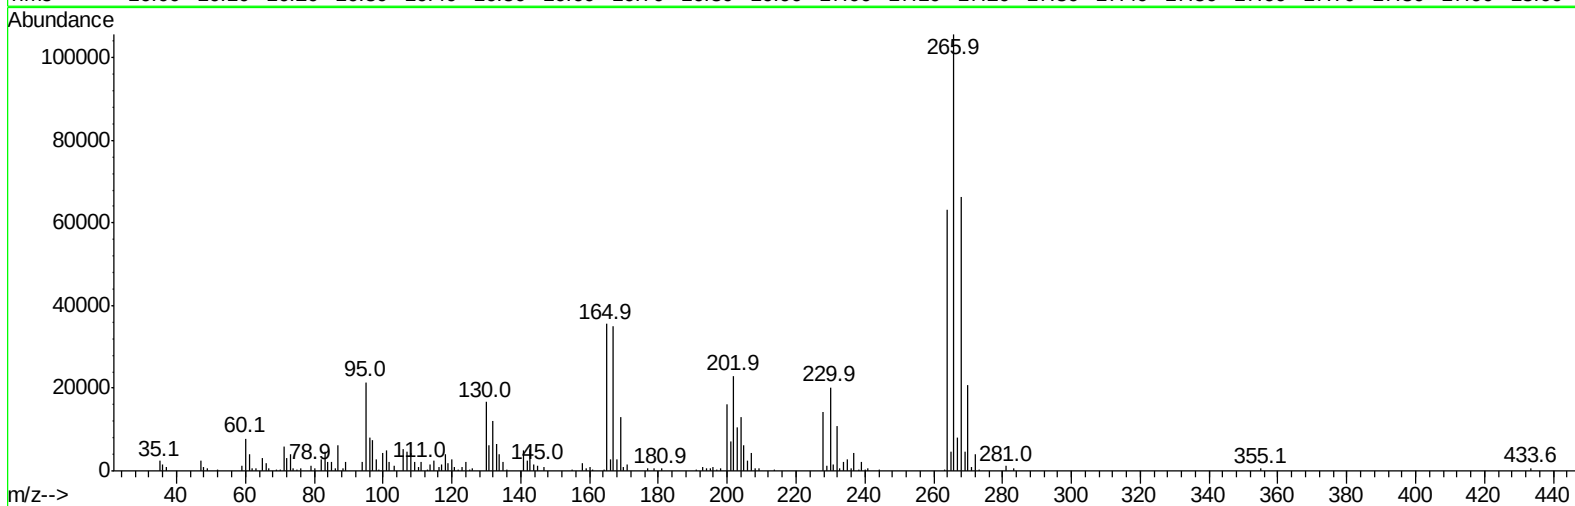


Data Path : Z:\HPCHEM1\BNA M\DATA\BM052217\
Data File : BM010113.D
Acq On : 22 May 2017 21:35
Operator : SJ/MA
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 23 07:25:36 2017
Quant Method : Z:\HPCHEM1\BNA M\METHODS\8270-BM051917.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat May 20 04:25:49 2017
Response via : Initial Calibration

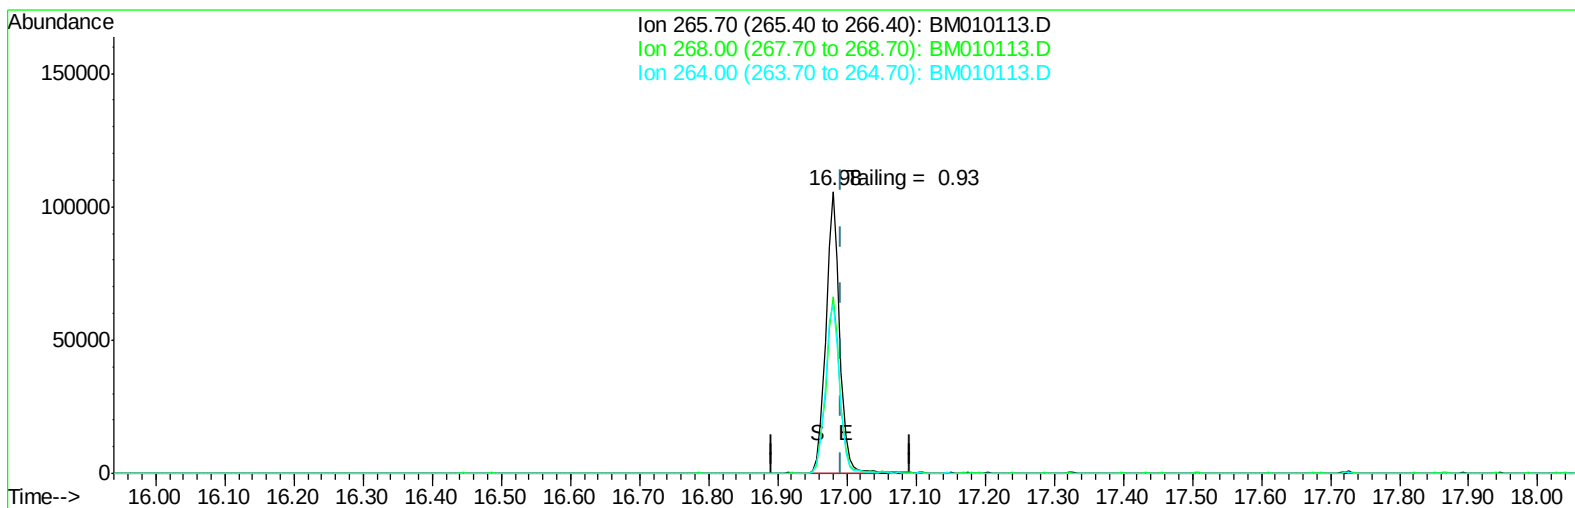

TIC: BM010113.D

(69) Pentachlorophenol (C)



16.980min (-0.012) 113462.67ng

response 145390

Ion	Exp%	Act%
265.70	100	100
268.00	65.00	62.69
264.00	61.20	59.93
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA M\DATA\BM052217\
Data File : BM010113.D
Acq On : 22 May 2017 21:35
Operator : SJ/MA
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 23 07:25:36 2017
Quant Method : Z:\HPCHEM1\BNA M\METHODS\8270-BM051917.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat May 20 04:25:49 2017
Response via : Initial Calibration

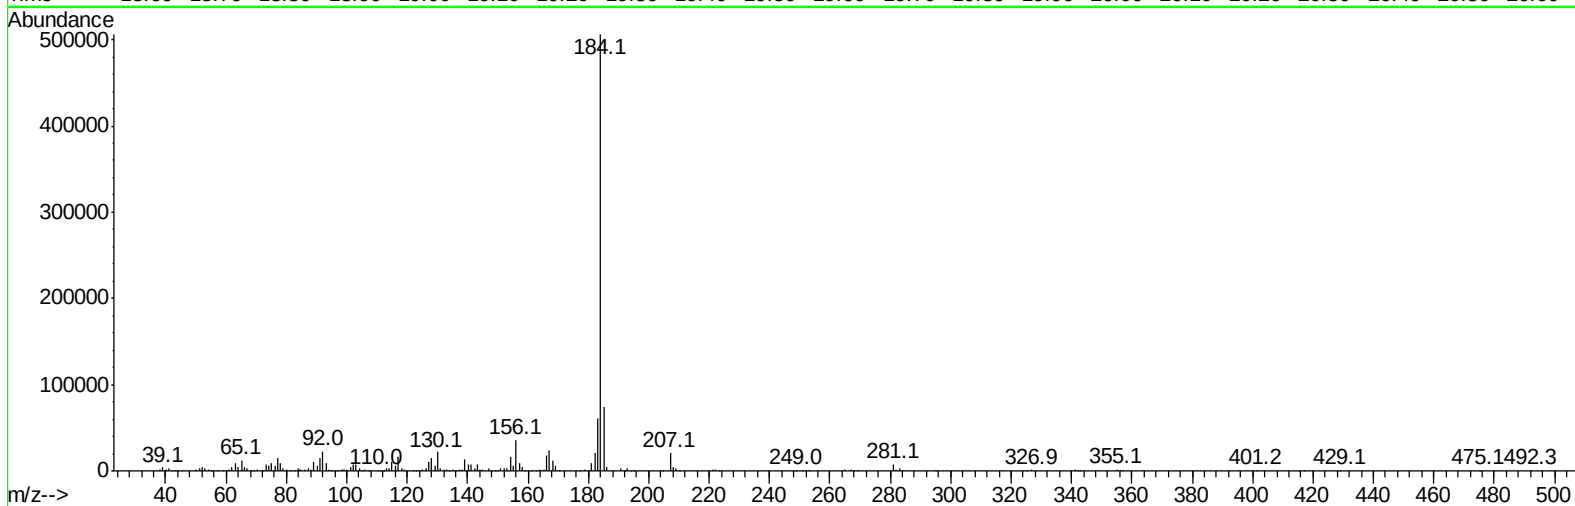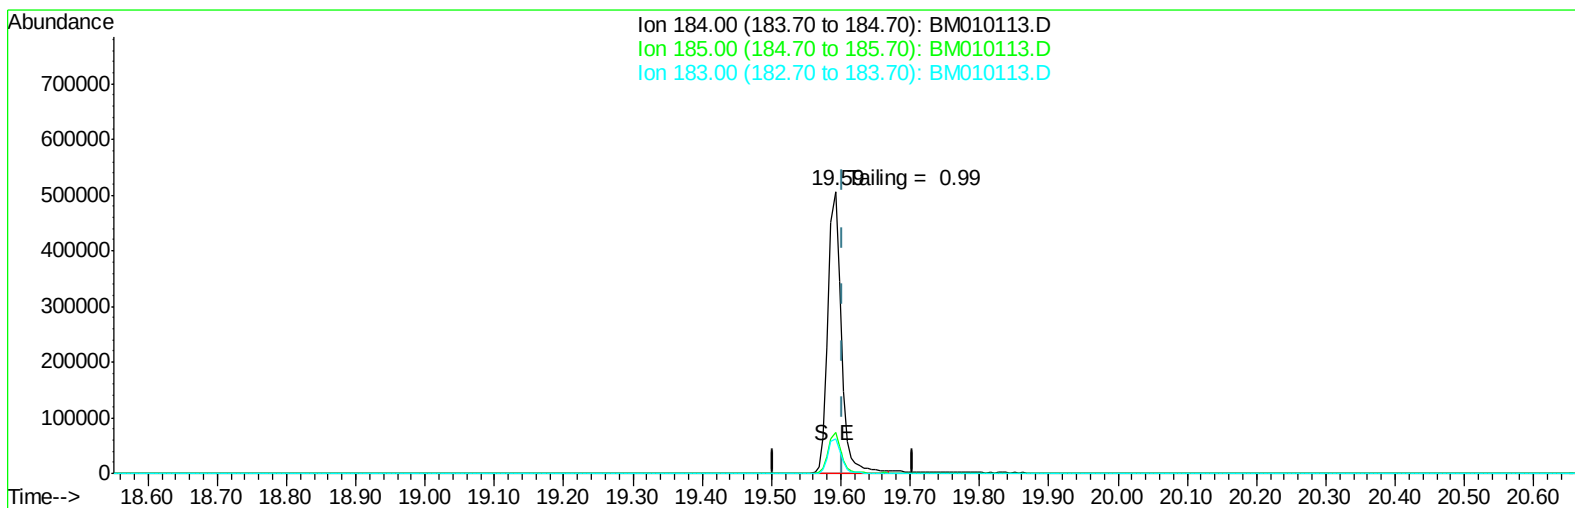

TIC: BM010113.D

(76) Benzidine

19.592min (-0.012) 42525.55ng

response 675349

Ion	Exp%	Act%
184.00	100	100
185.00	14.10	14.57
183.00	11.10	12.13
0.00	0.00	0.00