

Data Path : Z:\HPCHEM1\BNA M\DATA\BM052217\
 Data File : BM010101.D
 Acq On : 22 May 2017 14:23
 Operator : SJ/MA
 Sample : PB99134BL
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 PB99134BL

Quant Time: May 23 06:00:31 2017
 Quant Method : Z:\HPCHEM1\BNA M\METHODS\8270-BM051917.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat May 20 04:25:49 2017
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.96	152	158966	20.00	ng	-0.01
21) Naphthalene-d8	10.77	136	530668	20.00	ng	-0.01
38) Acenaphthene-d10	14.60	164	317107	20.00	ng	-0.01
63) Phenanthrene-d10	17.34	188	727794	20.00	ng	-0.01
75) Chrysene-d12	21.50	240	1049749	20.00	ng	-0.01
86) Perylene-d12	23.87	264	1277896	20.00	ng	-0.02
System Monitoring Compounds						
5) 2-Fluorophenol	5.55	112	1357793	154.24	ng	-0.01
7) Phenol-d6	7.16	99	1608754	142.03	ng	-0.01
23) Nitrobenzene-d5	9.15	82	1047881	106.54	ng	-0.02
41) 2,4,6-Tribromophenol	16.09	330	677256	140.62	ng	-0.01
44) 2-Fluorobiphenyl	13.22	172	2634957	106.82	ng	-0.01
78) Terphenyl-d14	19.94	244	4042941	87.57	ng	-0.01


Target Compounds Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA M\DATA\BM052217\
Data File : BM010101.D
Acq On : 22 May 2017 14:23
Operator : SJ/MA
Sample : PB99134BL
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB99134BL

Quant Time: May 23 06:00:31 2017
Quant Method : Z:\HPCHEM1\BNA M\METHODS\8270-BM051917.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat May 20 04:25:49 2017
Response via : Initial Calibration

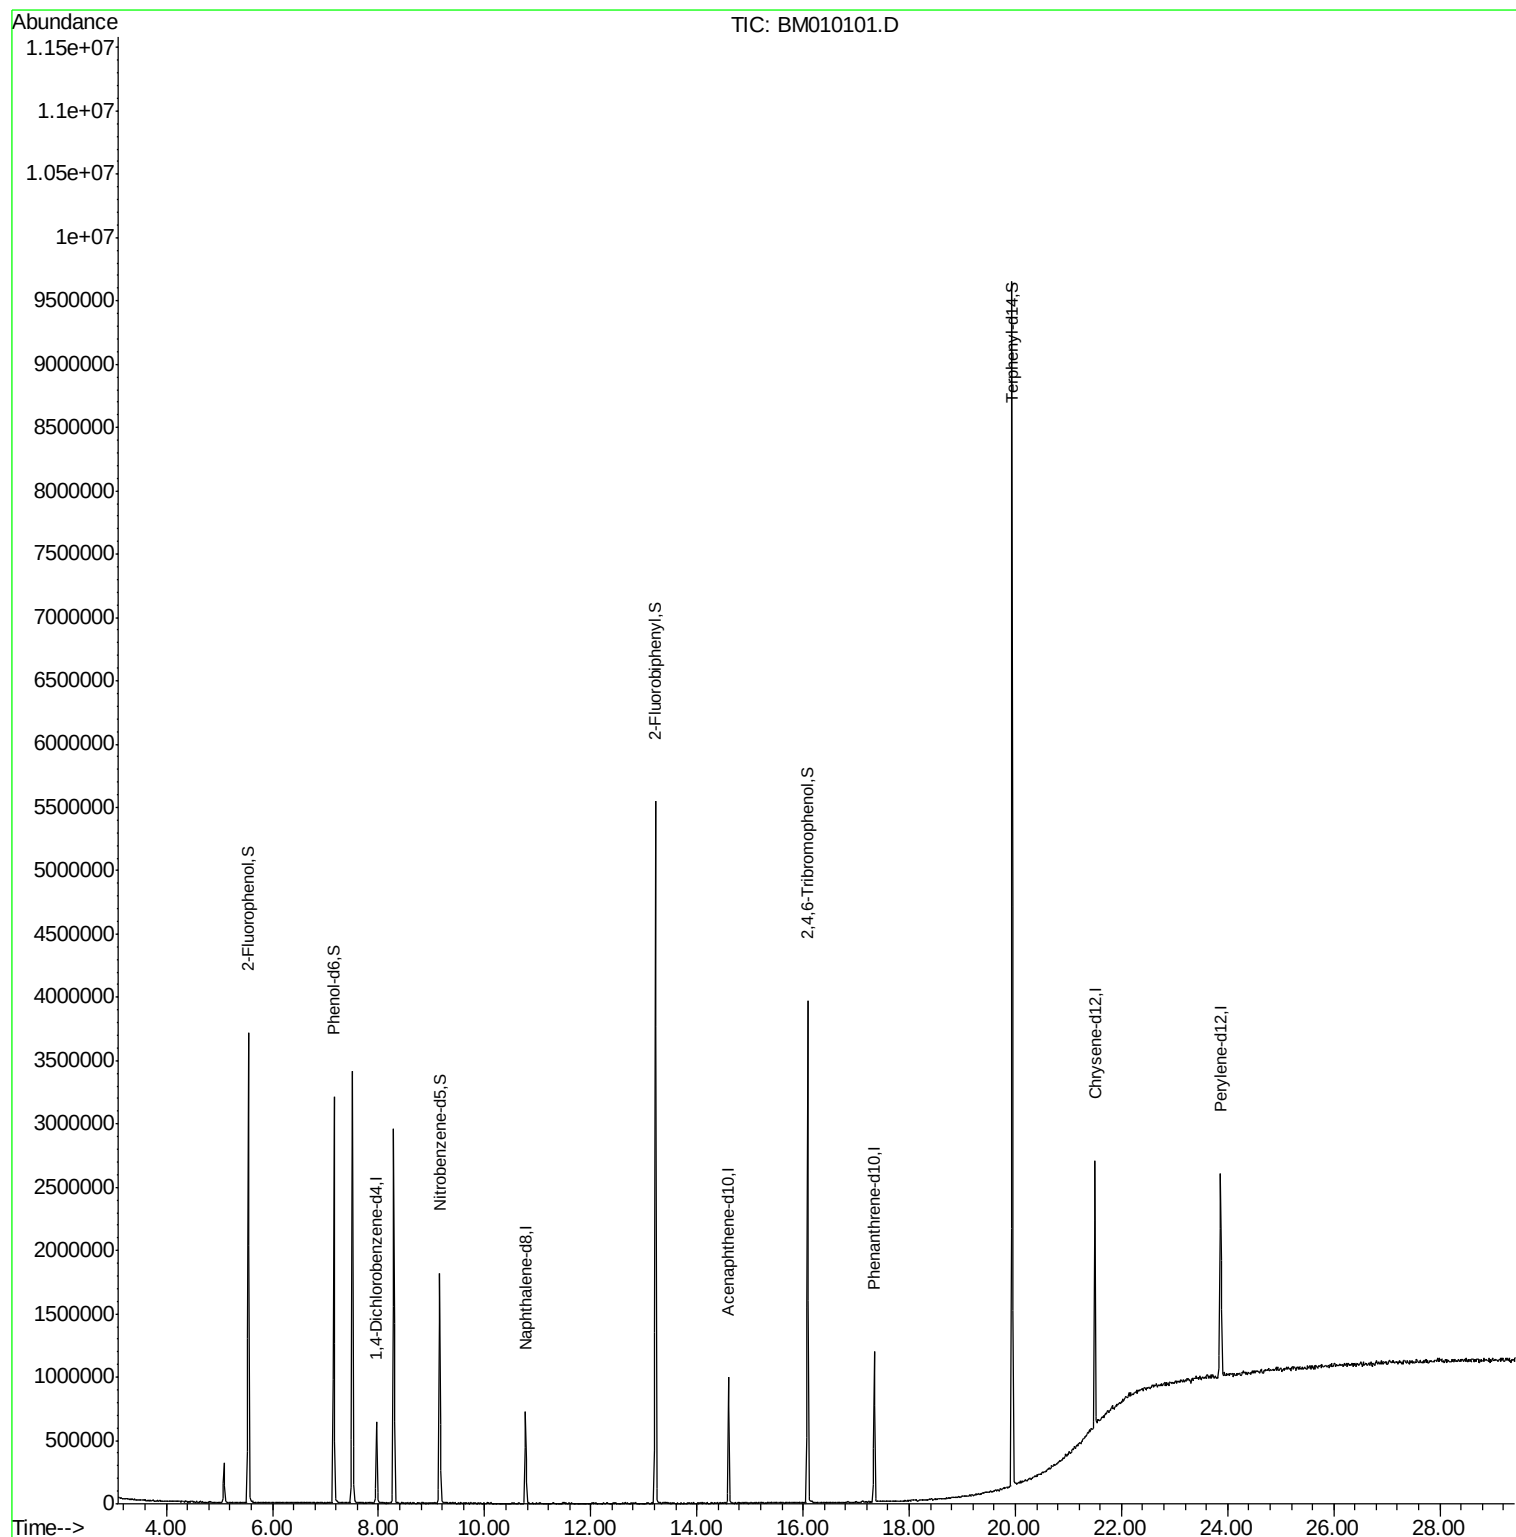

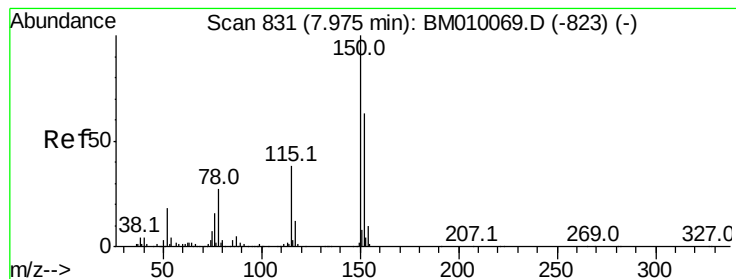


#1




1,4-Dichlorobenzene-d4
Concen: 20.00 ng
RT: 7.96 min Scan# 829
Delta R.T. -0.01 min
Lab File: BM010101.D
Acq: 22 May 2017 14:23

Instrument :
BNA_M
ClientSampleId :
PB99134BL

Tot Ion	152	Resp	158966
Ion	Ratio	Lower	Upper
152	100		
150	159.0	119.5	179.3
115	58.6	43.0	64.4

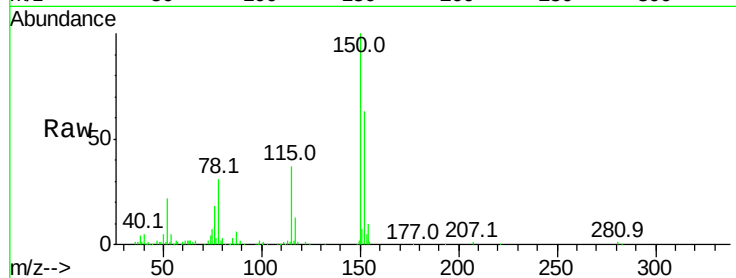


Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

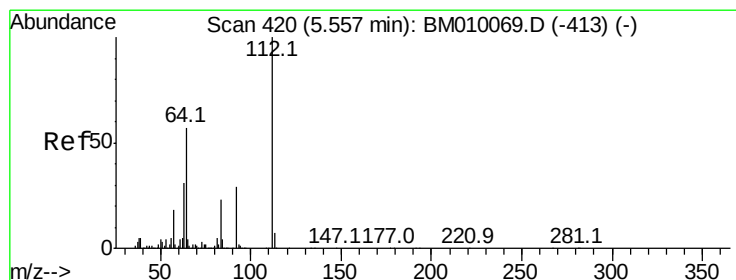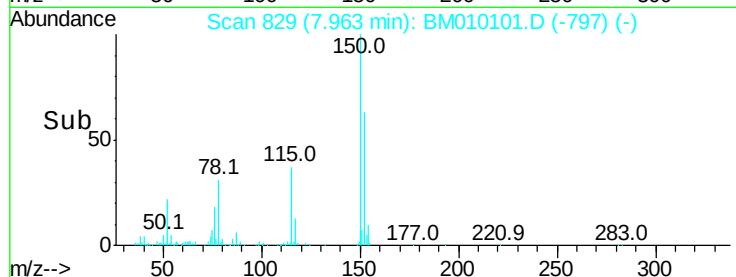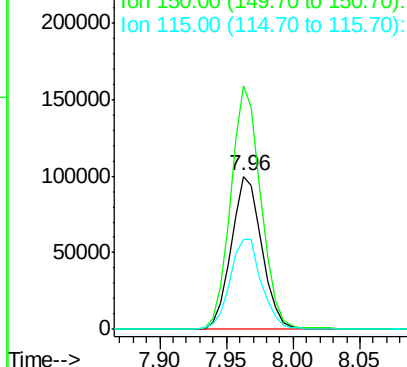



#5


2-Fluorophenol
Concen: 154.24 ng
RT: 5.55 min Scan# 418
Delta R.T. -0.01 min
Lab File: BM010101.D
Acq: 22 May 2017 14:23

Tgt Ion	112	Resp	1357793
Ion	Ratio	Lower	Upper
112	100		
64	63.1	38.6	57.8#
63	36.2	19.3	28.9#

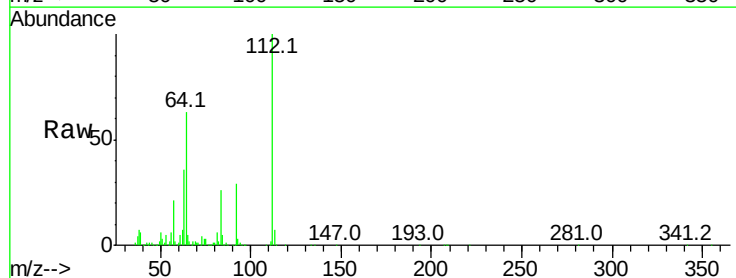

Abundance Ion 112.00 (111.70 to 112.70): E
Ion 64.00 (63.70 to 64.70): BM0
Ion 63.00 (62.70 to 63.70): BM0

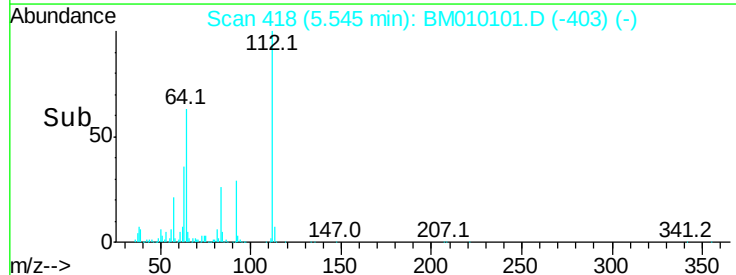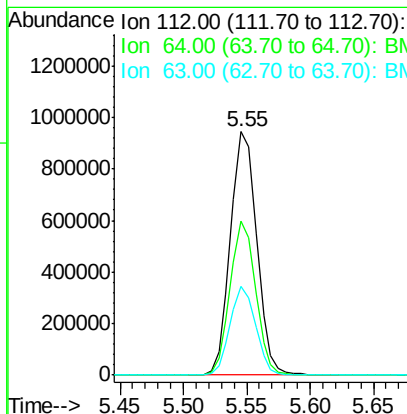

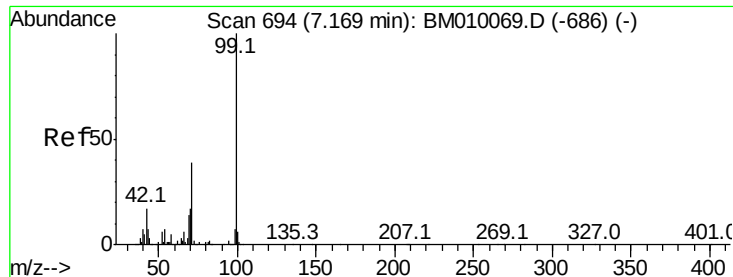

#7

Phenol-d6

Concen: 142.03 ng

RT: 7.16 min Scan# 692

Delta R.T. -0.01 min

Lab File: BM010101.D

Acq: 22 May 2017 14:23

Instrument :

BNA_M

ClientSampled :

PB99134BL


Tot Ion: 99 Resp: 1608754

Ion Ratio Lower Upper

99 100

42 18.5 11.0 16.4#




71 45.3 23.4 35.2#

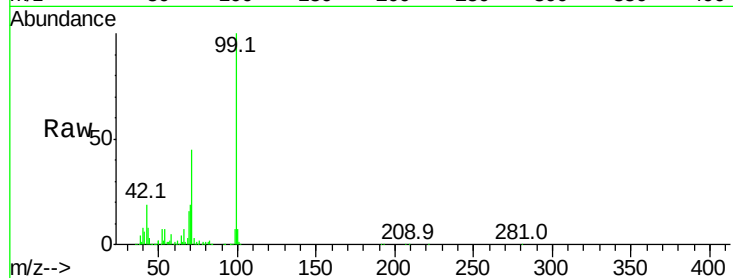

Abundance Ion 99.00 (98.70 to 99.70): BM010101.D (-677) (-)

Ion 42.00 (41.70 to 42.70): BM010101.D (-677) (-)

Ion 71.00 (70.70 to 71.70): BM010101.D (-677) (-)

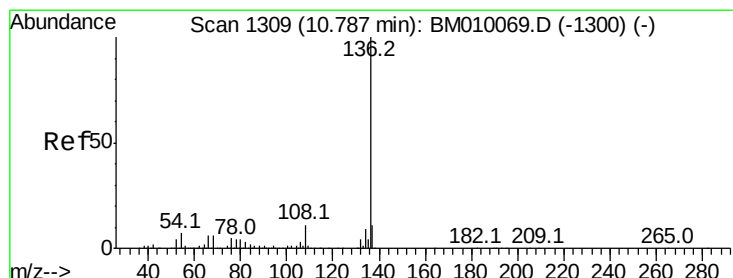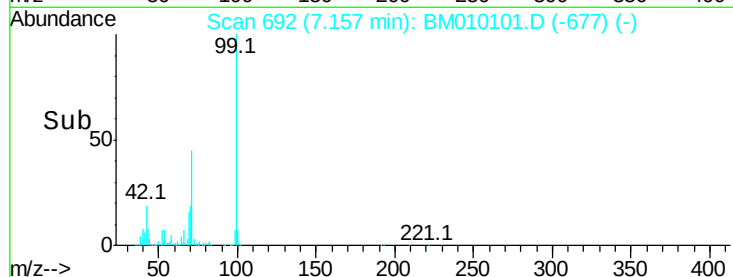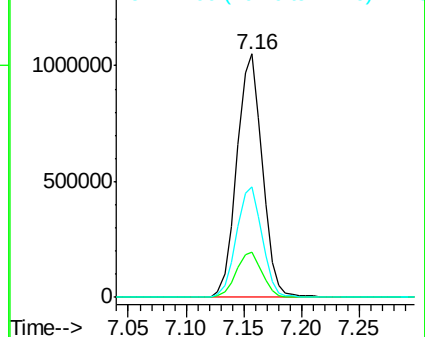

#21

Naphthalene-d8

Concen: 20.00 ng

RT: 10.77 min Scan# 1307

Delta R.T. -0.01 min

Lab File: BM010101.D

Acq: 22 May 2017 14:23

Tgt Ion: 136 Resp: 530668


Ion Ratio Lower Upper

136 100

137 11.9 8.7 13.1

54 6.4 4.6 6.8

68 5.3 3.7 5.5


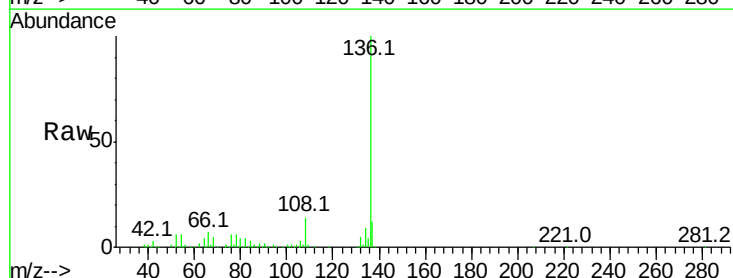



Abundance Ion 136.00 (135.70 to 136.70): BM010101.D (-1292) (-)

Ion 137.00 (136.70 to 137.70): BM010101.D (-1292) (-)

Ion 54.00 (53.70 to 54.70): BM010101.D (-1292) (-)

Ion 68.00 (67.70 to 68.70): BM010101.D (-1292) (-)

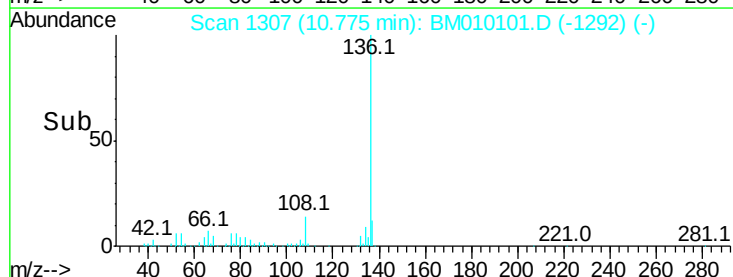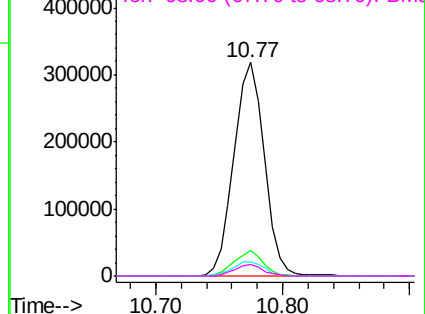




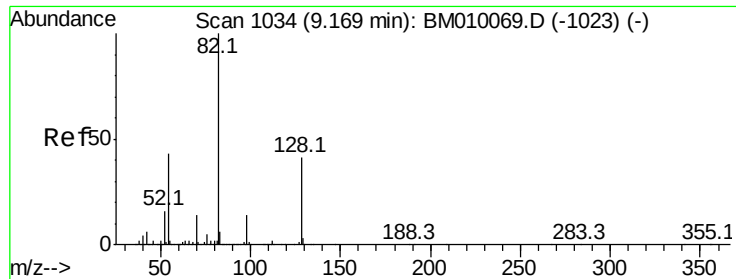


#23
 Nitrobenzene-d5
 Concen: 106.54 ng
 RT: 9.15 min Scan# 1031
 Delta R.T. -0.02 min
 Lab File: BM010101.D
 Acq: 22 May 2017 14:23

Instrument :
 BNA_M
 ClientSampleId :
 PB99134BL

Tot Ion: 82 Resp: 1047881




Ion	Ratio	Lower	Upper
82	100		
128	36.6	32.8	49.2
54	46.4	40.6	60.8

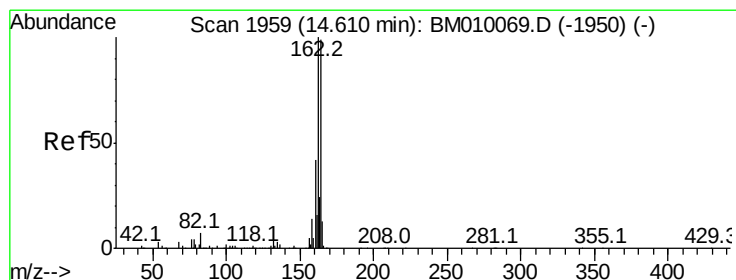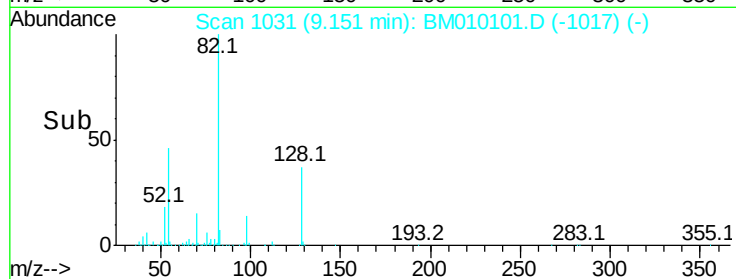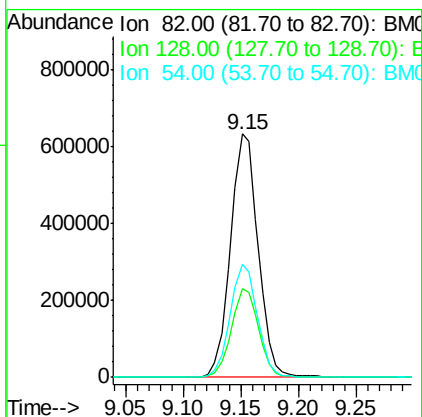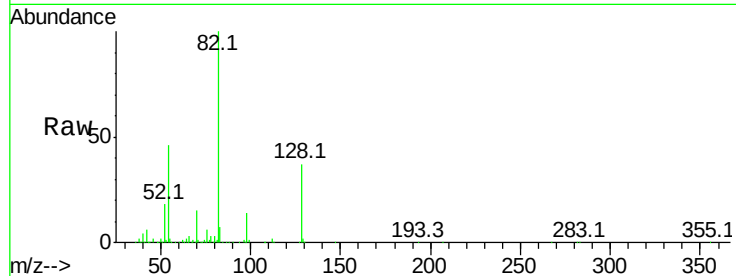


#38
 Acenaphthene-d10
 Concen: 20.00 ng
 RT: 14.60 min Scan# 1957
 Delta R.T. -0.01 min
 Lab File: BM010101.D
 Acq: 22 May 2017 14:23

Tgt Ion: 164 Resp: 317107

Ion	Ratio	Lower	Upper
164	100		
162	100.6	82.4	123.6
160	46.1	35.8	53.6


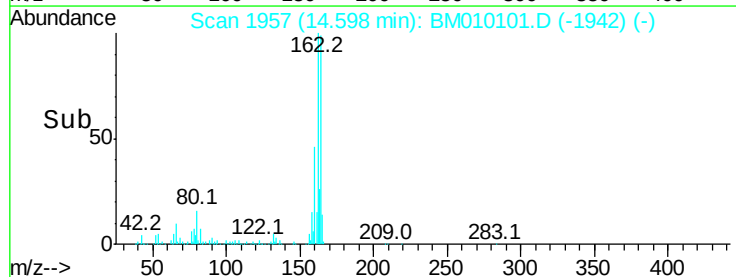
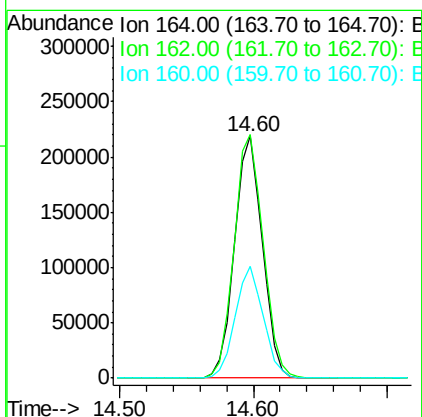
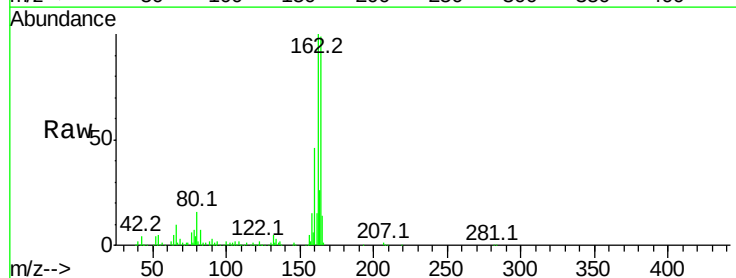


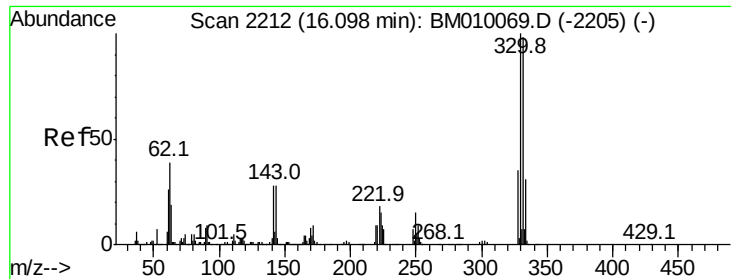

#41
 2,4,6-Tribromophenol
 Concen: 140.62 ng
 RT: 16.09 min Scan# 2210
 Delta R.T. -0.01 min
 Lab File: BM010101.D
 Acq: 22 May 2017 14:23




Instrument :
 BNA_M
 ClientSampleId :
 PB99134BL


Tot Ion	Ratio	Lower	Upper
330	100		
332	96.7	0.0	0.0#
141	31.0	0.0	0.0#

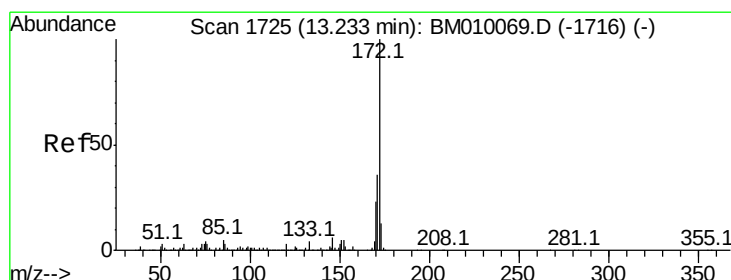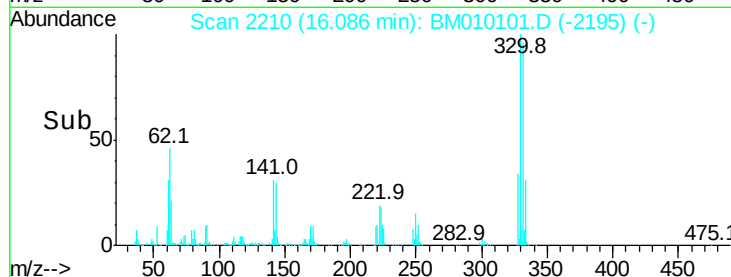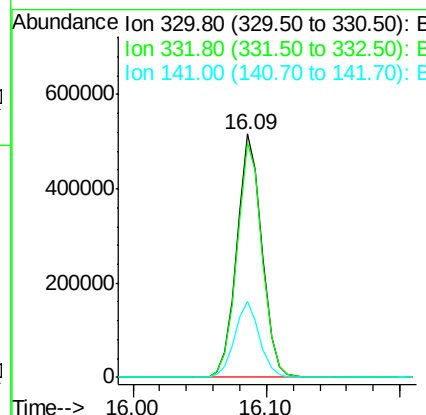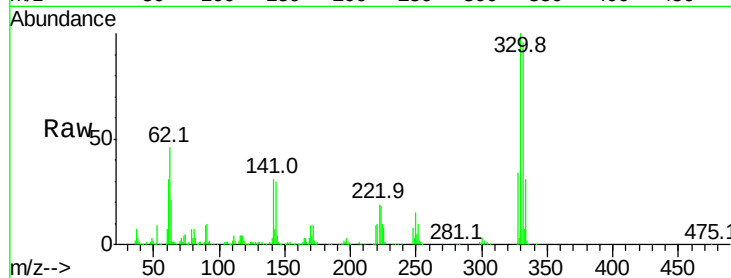

#44
 2-Fluorobiphenyl
 Concen: 106.82 ng
 RT: 13.22 min Scan# 1723
 Delta R.T. -0.01 min
 Lab File: BM010101.D
 Acq: 22 May 2017 14:23

Tgt Ion	Ratio	Lower	Upper
172	100		
171	35.6	28.5	42.7
170	22.9	18.8	28.2


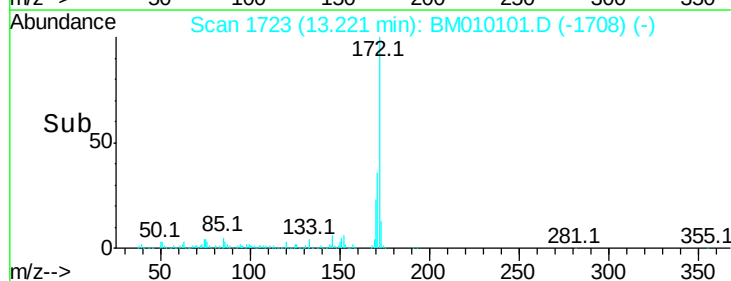
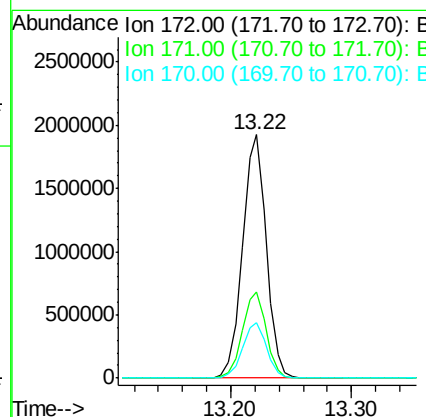
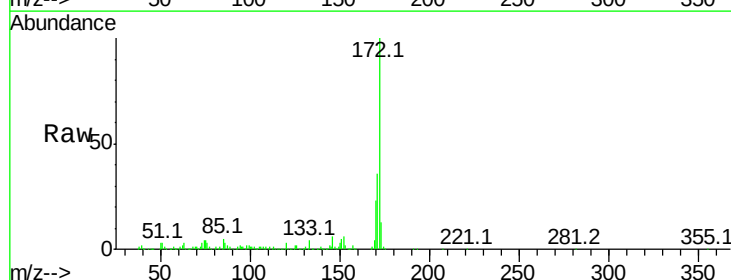


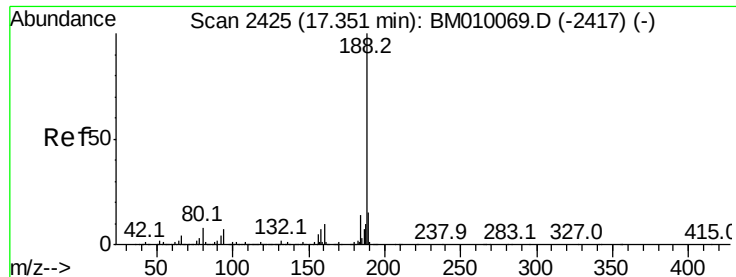

#63
Phenanthrene-d10
Concen: 20.00 ng
RT: 17.34 min Scan# 2423
Delta R.T. -0.01 min
Lab File: BM010101.D
Acq: 22 May 2017 14:23




Instrument :
BNA_M
ClientSampleId :
PB99134BL


Tot Ion	Ratio	Lower	Upper
188	100		
94	5.7	8.7	13.1#
80	7.0	9.3	13.9#

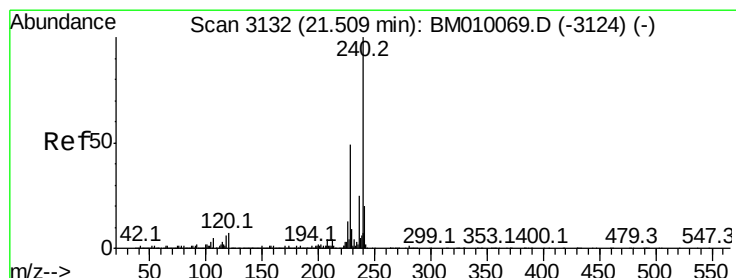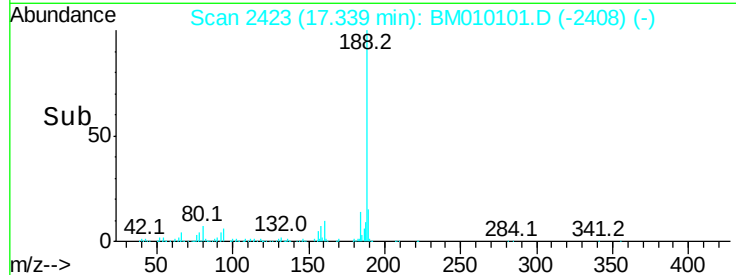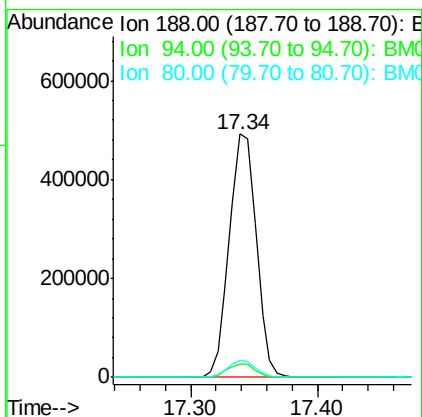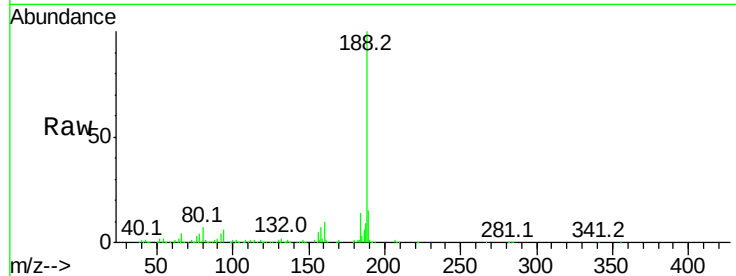

#75
Chrysene-d12
Concen: 20.00 ng
RT: 21.50 min Scan# 3130
Delta R.T. -0.01 min
Lab File: BM010101.D
Acq: 22 May 2017 14:23

Tgt Ion	Ratio	Lower	Upper
240	100		
120	5.9	8.2	12.2#
236	25.3	20.0	30.0

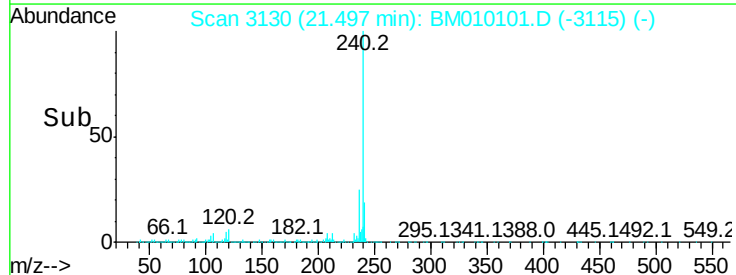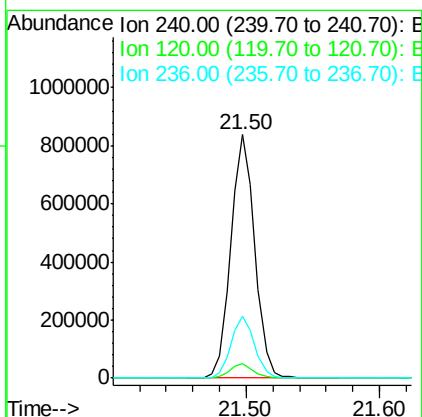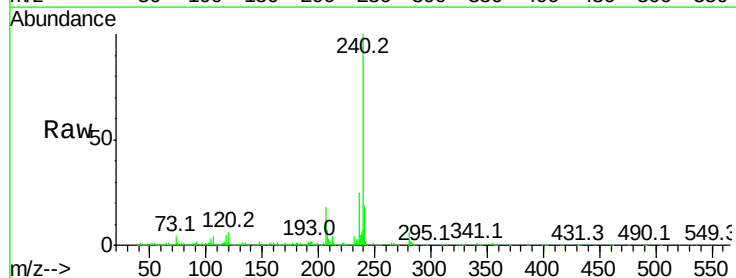

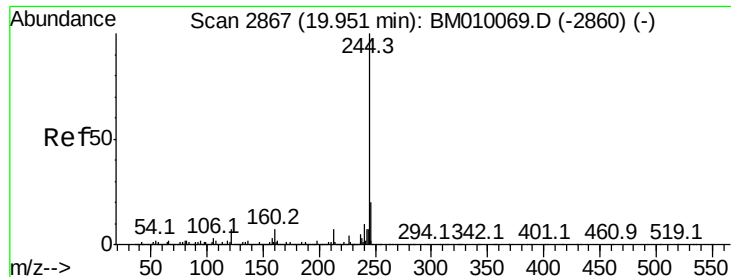

#78

Terphenyl-d14

Concen: 87.57 ng

RT: 19.94 min Scan# 2865

Delta R.T. -0.01 min

Lab File: BM010101.D

Acq: 22 May 2017 14:23

Instrument :

BNA_M

ClientSampleId :

PB99134BL


Tot Ion:244 Resp: 4042941

Ion	Ratio	Lower	Upper
244	100		
212	7.3	4.9	7.3
122	6.8	6.2	9.4

244 100

212 7.3 4.9 7.3




122 6.8 6.2 9.4

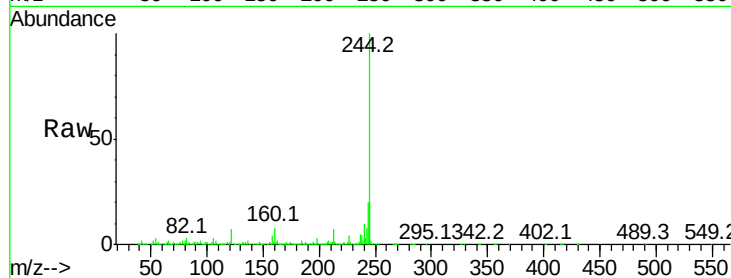

Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

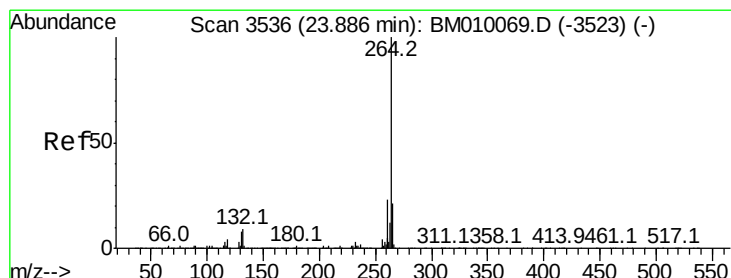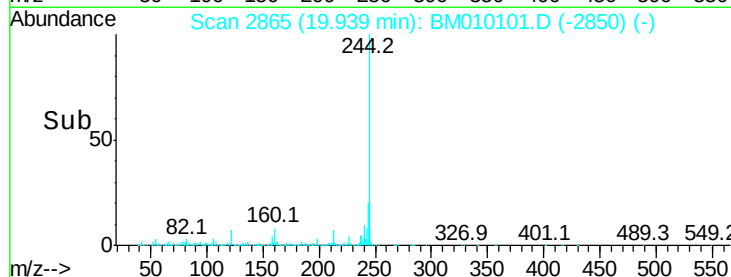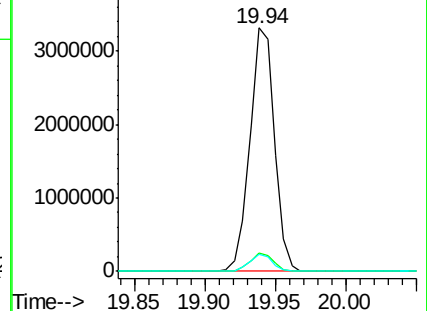

#86

Perylene-d12

Concen: 20.00 ng

RT: 23.87 min Scan# 3533

Delta R.T. -0.02 min

Lab File: BM010101.D

Acq: 22 May 2017 14:23


Tgt Ion:264 Resp: 1277896

Ion	Ratio	Lower	Upper
264	100		
260	24.1	18.6	27.8
265	22.9	17.3	25.9

264 100

260 24.1 18.6 27.8

265 22.9 17.3 25.9

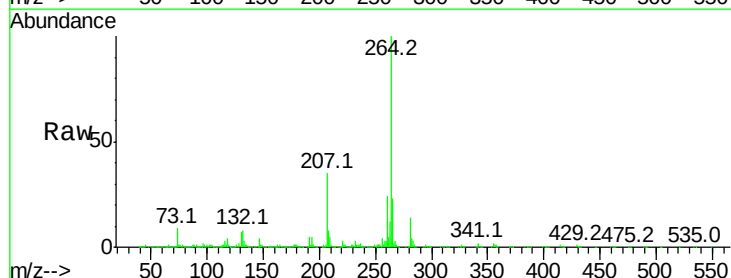

Abundance Ion 264.00 (263.70 to 264.70): E

Ion 260.00 (259.70 to 260.70): E

Ion 265.00 (264.70 to 265.70): E

