

Data Path : Z:\HPCHEM1\BNA M\DATA\BM052217\
 Data File : BM010111.D
 Acq On : 22 May 2017 20:22
 Operator : SJ/MA
 Sample : I3240-15
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 EP2-FB01

Quant Time: May 23 06:18:35 2017
 Quant Method : Z:\HPCHEM1\BNA M\METHODS\8270-BM051917.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat May 20 04:25:49 2017
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.96	152	158937	20.00	ng	-0.01
21) Naphthalene-d8	10.77	136	527438	20.00	ng	-0.02
38) Acenaphthene-d10	14.59	164	332255	20.00	ng	-0.02
63) Phenanthrene-d10	17.34	188	849316	20.00	ng	-0.01
75) Chrysene-d12	21.50	240	1257151	20.00	ng	-0.01
86) Perylene-d12	23.86	264	1284694	20.00	ng	-0.02
System Monitoring Compounds						
5) 2-Fluorophenol	5.55	112	514077	58.41	ng	-0.01
7) Phenol-d6	7.15	99	365477	32.27	ng	-0.02
23) Nitrobenzene-d5	9.15	82	978719	100.11	ng	-0.02
41) 2,4,6-Tribromophenol	16.09	330	739989	146.64	ng	-0.01
44) 2-Fluorobiphenyl	13.22	172	2500490	96.75	ng	-0.02
78) Terphenyl-d14	19.94	244	4987784	90.21	ng	-0.01


Target Compounds Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA M\DATA\BM052217\
Data File : BM010111.D
Acq On : 22 May 2017 20:22
Operator : SJ/MA
Sample : I3240-15
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
EP2-FB01

Quant Time: May 23 06:18:35 2017
Quant Method : Z:\HPCHEM1\BNA M\METHODS\8270-BM051917.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat May 20 04:25:49 2017
Response via : Initial Calibration

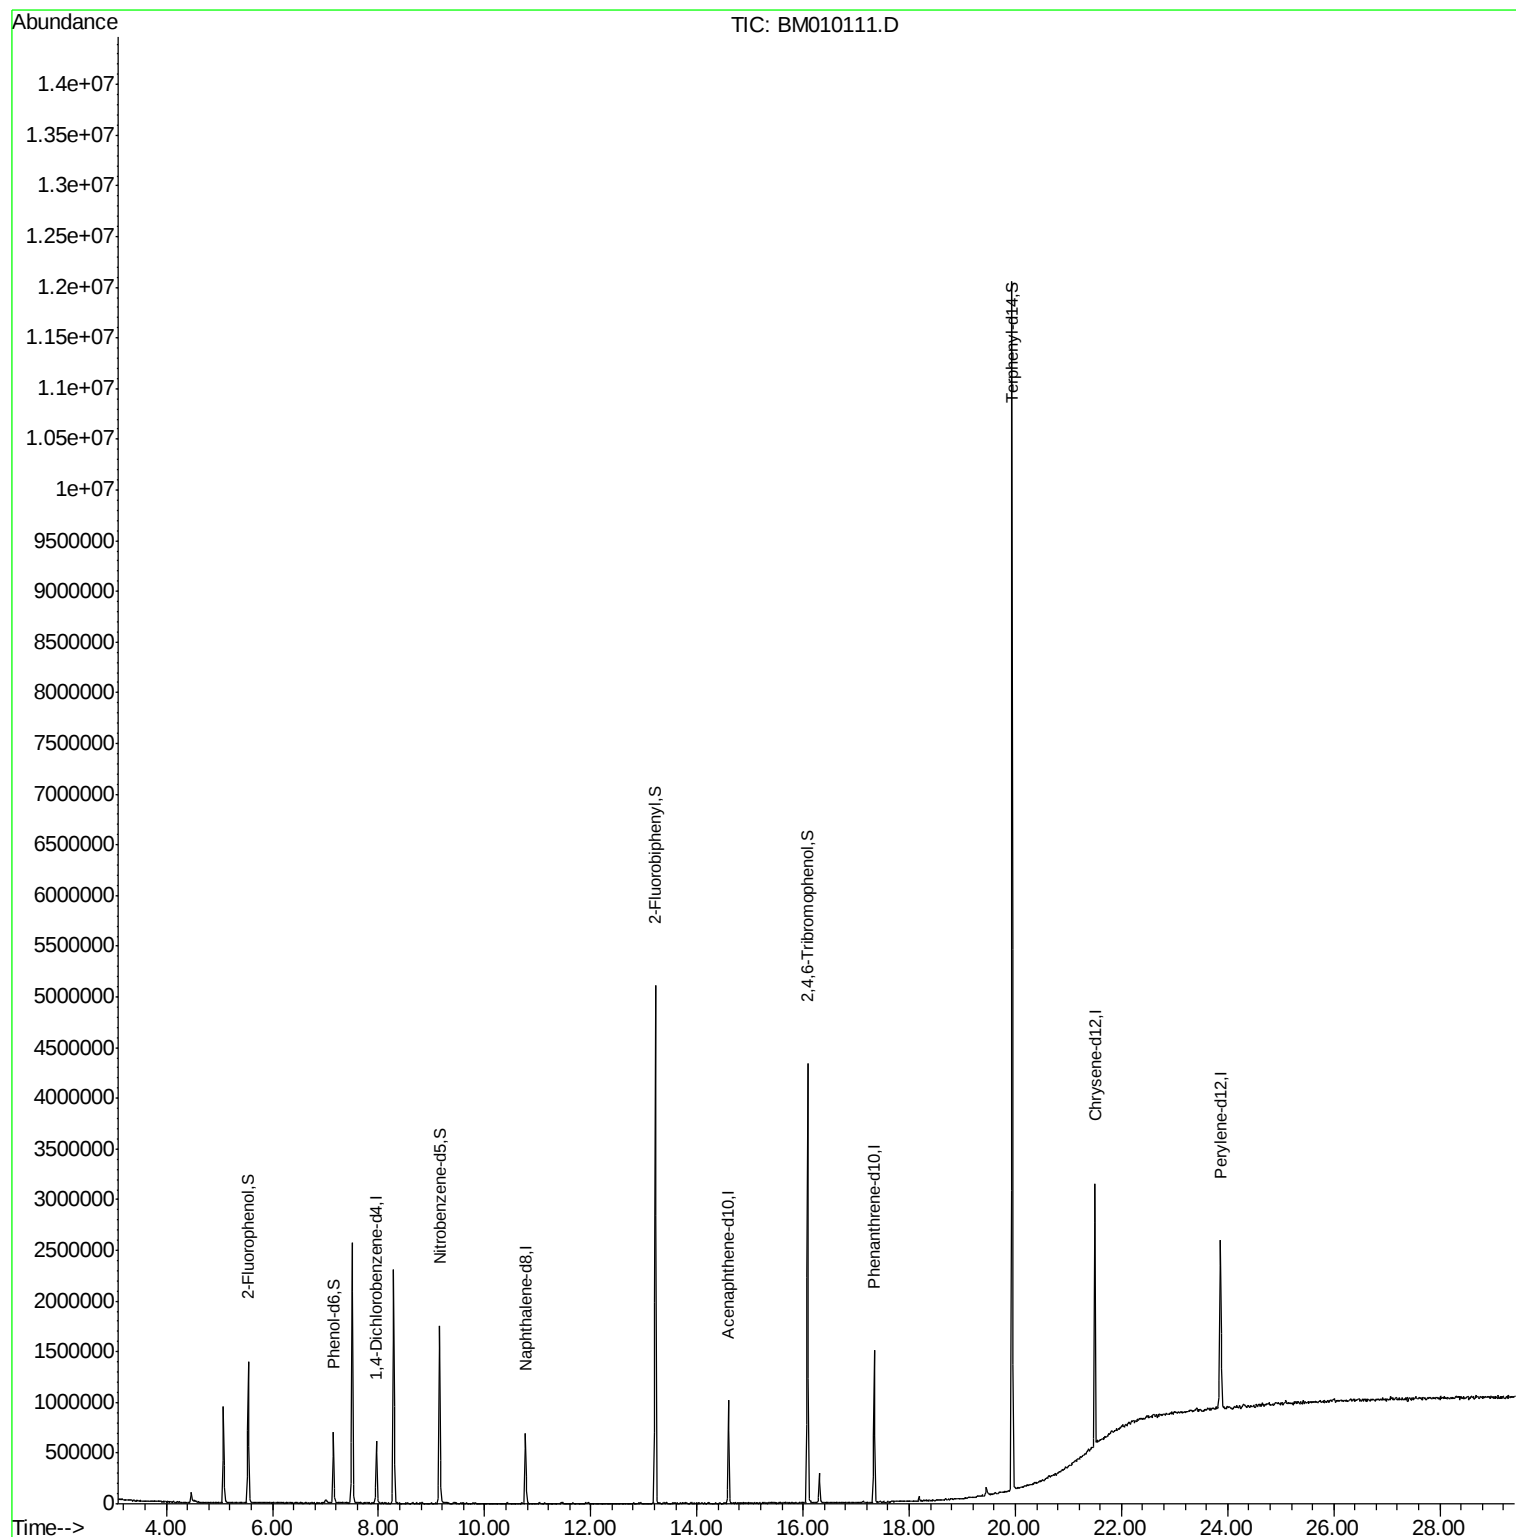




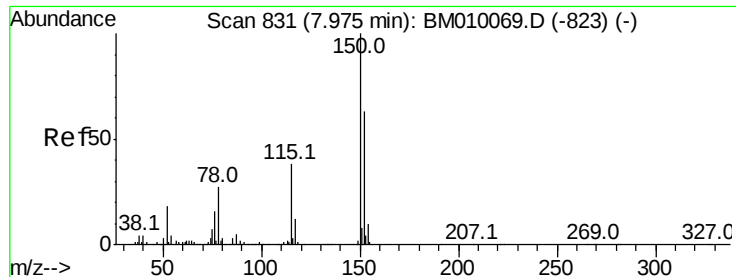


#1

1,4-Dichlorobenzene-d4
Concen: 20.00 ng
RT: 7.96 min Scan# 829
Delta R.T. -0.01 min
Lab File: BM010111.D
Acq: 22 May 2017 20:22

Instrument :
BNA_M
ClientSampleId :
EP2-FB01




Tot Ion	Ratio	Lower	Upper
152	100		
150	147.2	119.5	179.3
115	58.2	43.0	64.4

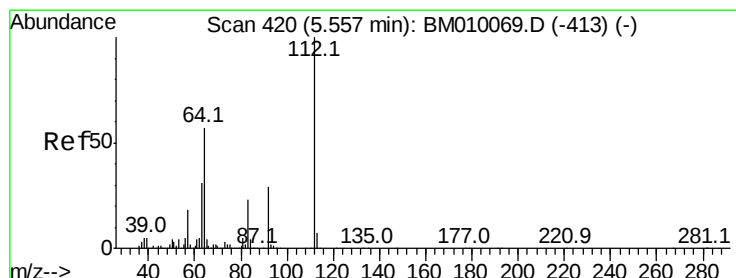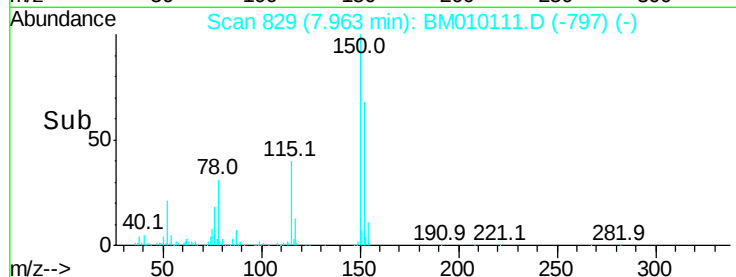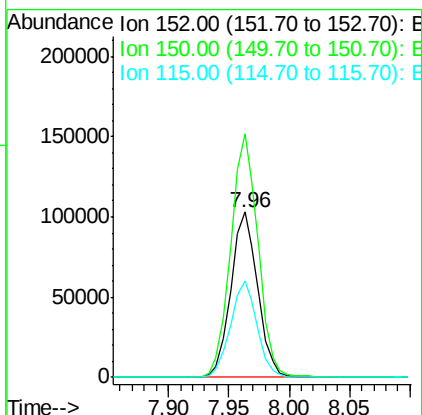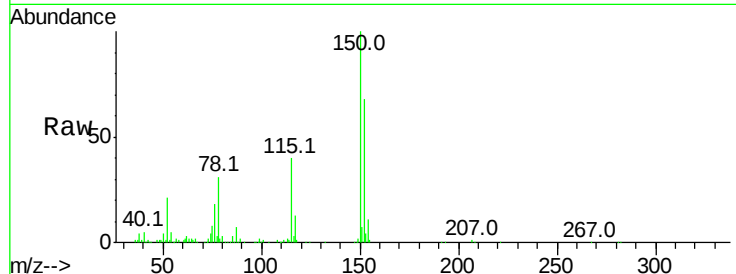


#5

2-Fluorophenol
Concen: 58.41 ng
RT: 5.55 min Scan# 418
Delta R.T. -0.01 min
Lab File: BM010111.D
Acq: 22 May 2017 20:22

Tgt Ion	Ratio	Lower	Upper
112	100		
64	60.9	38.6	57.8#
63	35.9	19.3	28.9#

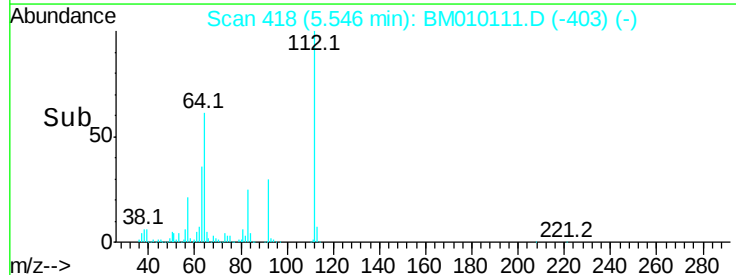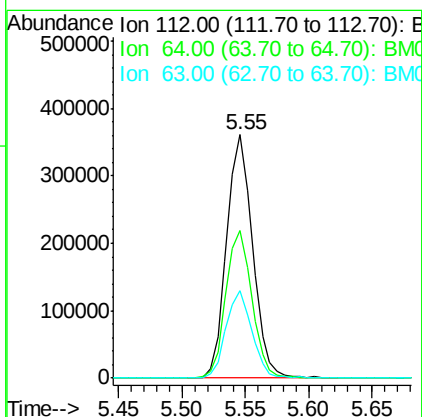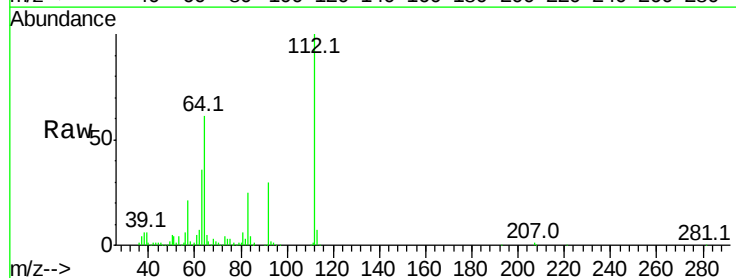

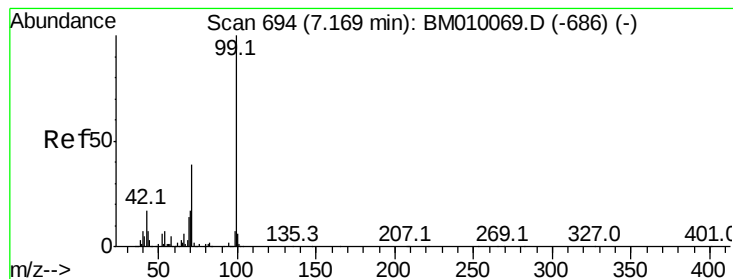

#7

Phenol-d6

Concen: 32.27 ng

RT: 7.15 min Scan# 691

Delta R.T. -0.02 min

Lab File: BM010111.D

Acq: 22 May 2017 20:22

Instrument :

BNA_M

ClientSampleId :

EP2-FB01


Tot Ion: 99 Resp: 365477

Ion Ratio Lower Upper

99 100

42 18.4 11.0 16.4#




71 43.7 23.4 35.2#

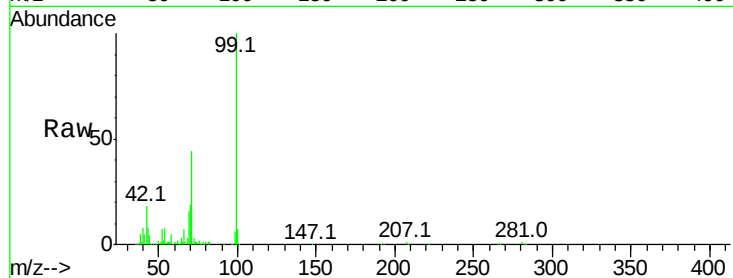

Abundance Ion 99.00 (98.70 to 99.70): BM010111.D (-677) (-)

Ion 42.00 (41.70 to 42.70): BM010111.D (-677) (-)

Ion 71.00 (70.70 to 71.70): BM010111.D (-677) (-)

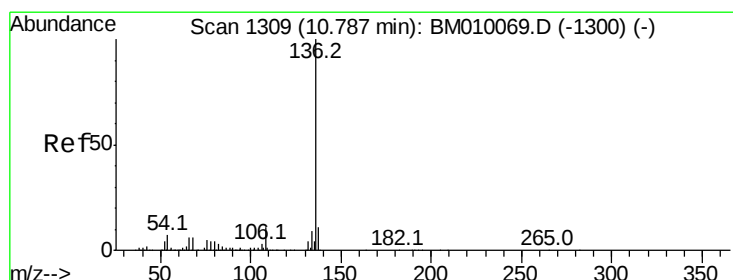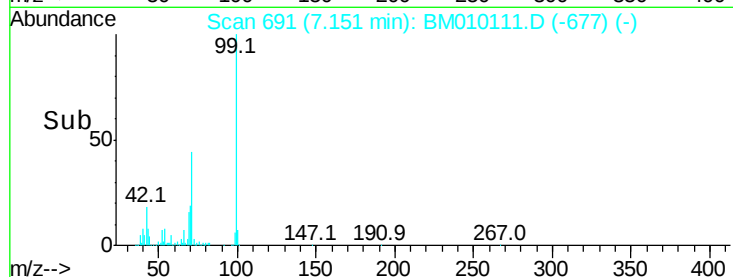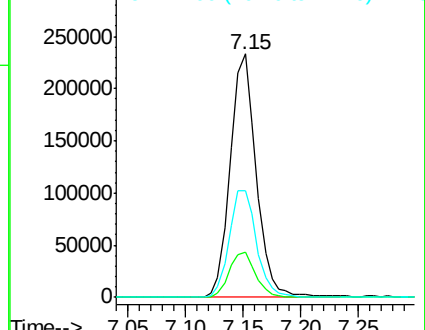

#21

Naphthalene-d8

Concen: 20.00 ng

RT: 10.77 min Scan# 1306

Delta R.T. -0.02 min

Lab File: BM010111.D

Acq: 22 May 2017 20:22

Tgt Ion: 136 Resp: 527438


Ion Ratio Lower Upper

136 100

137 11.2 8.7 13.1

54 6.6 4.6 6.8

68 5.6 3.7 5.5#


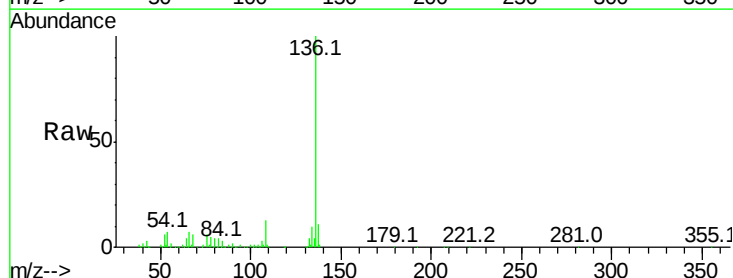



Abundance Ion 136.00 (135.70 to 136.70): BM010111.D (-1292) (-)

Ion 137.00 (136.70 to 137.70): BM010111.D (-1292) (-)

Ion 54.00 (53.70 to 54.70): BM010111.D (-1292) (-)

Ion 68.00 (67.70 to 68.70): BM010111.D (-1292) (-)



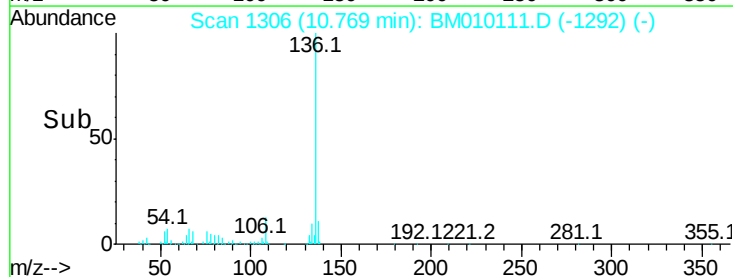
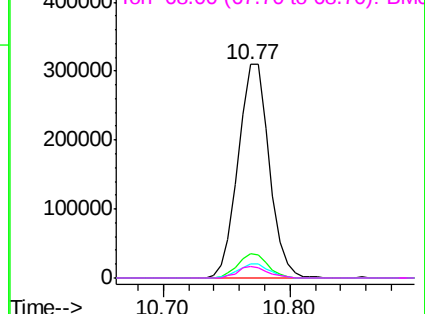


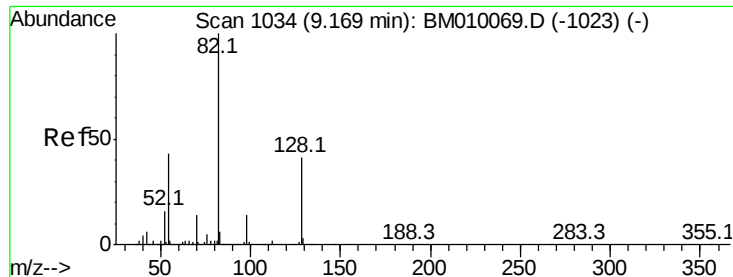

#23
 Nitrobenzene-d5
 Concen: 100.11 ng
 RT: 9.15 min Scan# 1031
 Delta R.T. -0.02 min
 Lab File: BM010111.D
 Acq: 22 May 2017 20:22




Instrument :
 BNA_M
 ClientSampleId :
 EP2-FB01


Tot Ion	Ratio	Lower	Upper
82	100		
128	36.0	32.8	49.2
54	44.8	40.6	60.8

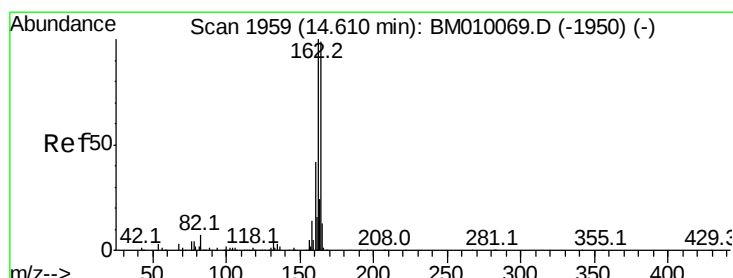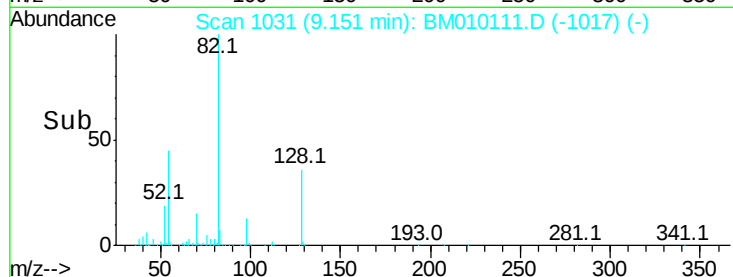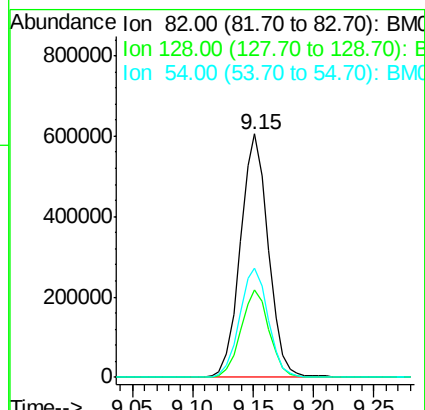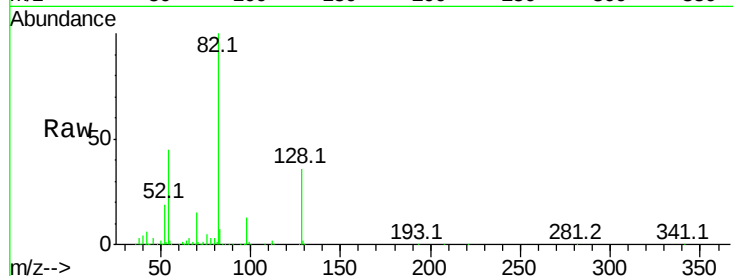

#38
 Acenaphthene-d10
 Concen: 20.00 ng
 RT: 14.59 min Scan# 1956
 Delta R.T. -0.02 min
 Lab File: BM010111.D
 Acq: 22 May 2017 20:22

Tgt Ion	Ratio	Lower	Upper
164	100		
162	104.5	82.4	123.6
160	45.4	35.8	53.6

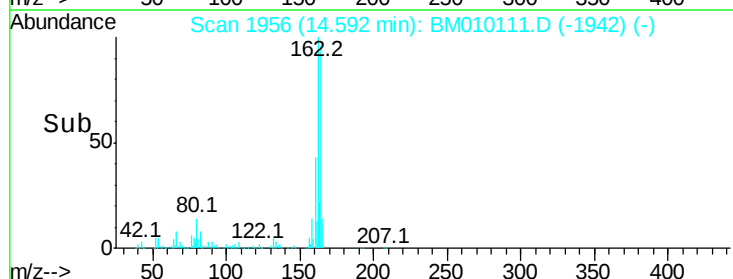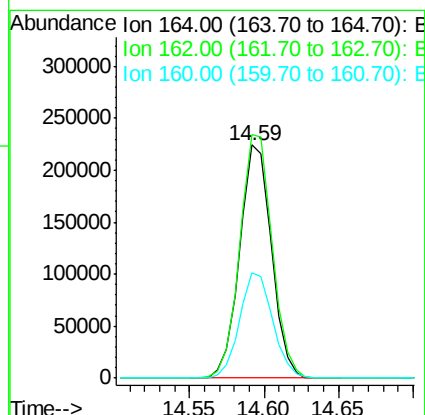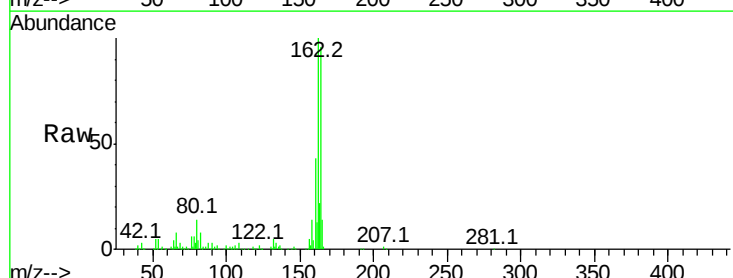

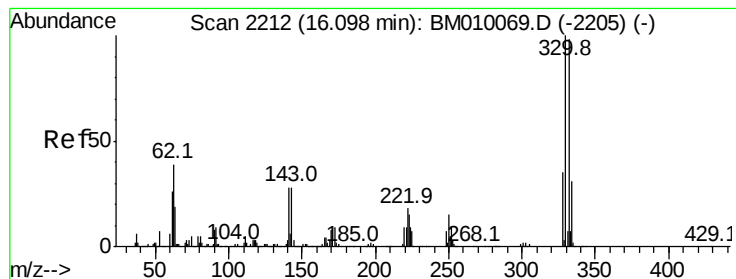

#41

2,4,6-Tribromophenol

Concen: 146.64 ng

RT: 16.09 min Scan# 2210

Delta R.T. -0.01 min

Lab File: BM010111.D

Acq: 22 May 2017 20:22

Instrument :

BNA_M

ClientSampleId :

EP2-FB01


Tot Ion:330 Resp: 739989

Ion Ratio Lower Upper




330 100

332 97.0 0.0 0.0#

141 31.8 0.0 0.0#

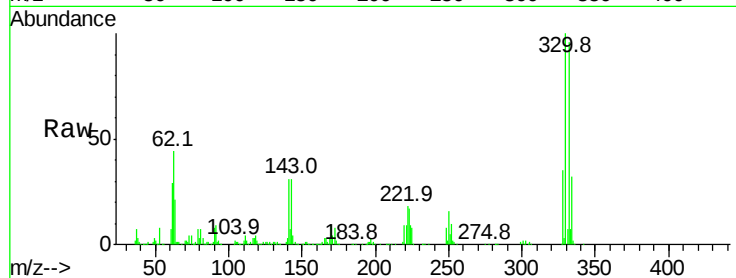

Abundance Ion 329.80 (329.50 to 330.50): E
Ion 331.80 (331.50 to 332.50): E
Ion 141.00 (140.70 to 141.70): E

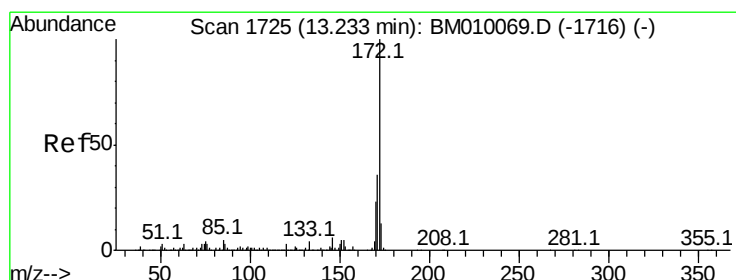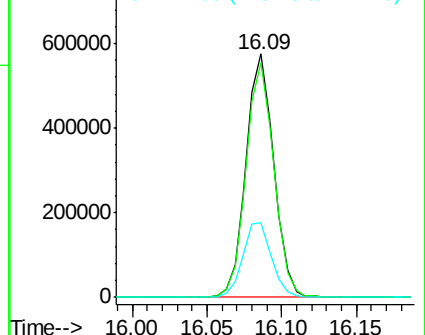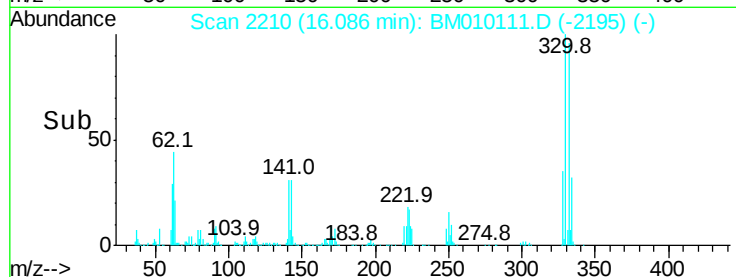

#44

2-Fluorobiphenyl

Concen: 96.75 ng

RT: 13.22 min Scan# 1722

Delta R.T. -0.02 min

Lab File: BM010111.D

Acq: 22 May 2017 20:22


Tgt Ion:172 Resp: 2500490

Ion Ratio Lower Upper



172 100


171 36.7 28.5 42.7

170 23.2 18.8 28.2

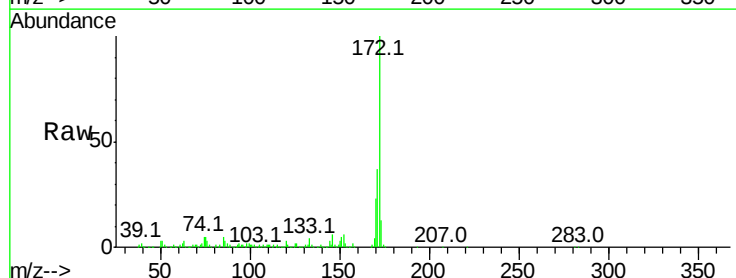

Abundance Ion 172.00 (171.70 to 172.70): E
Ion 171.00 (170.70 to 171.70): E
Ion 170.00 (169.70 to 170.70): E

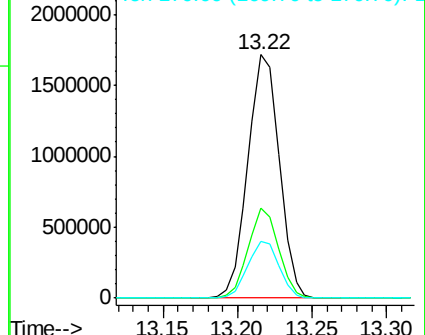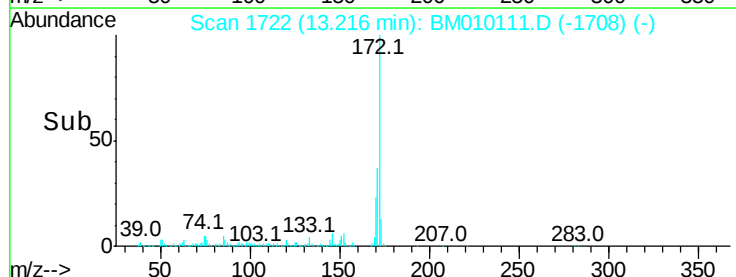


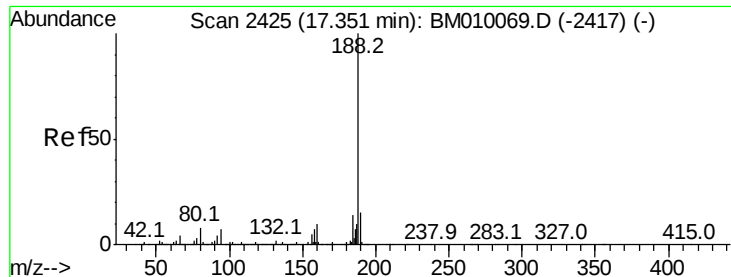




#63
Phenanthrene-d10
Concen: 20.00 ng
RT: 17.34 min Scan# 2423
Delta R.T. -0.01 min
Lab File: BM010111.D
Acq: 22 May 2017 20:22

Instrument :
BNA_M
ClientSampleId :
EP2-FB01

Tot Ion	Ratio	Lower	Upper
188	100		
94	6.1	8.7	13.1#
80	7.2	9.3	13.9#

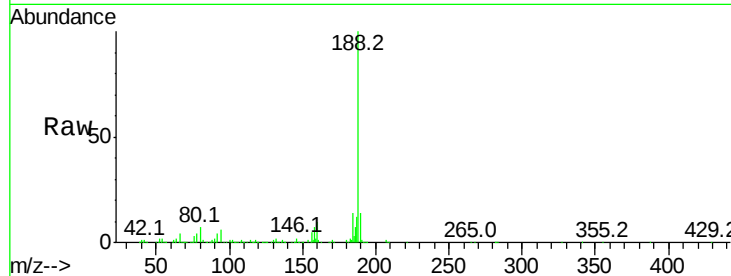


Abundance Ion 188.00 (187.70 to 188.70): E
Ion 94.00 (93.70 to 94.70): BM0
Ion 80.00 (79.70 to 80.70): BM0

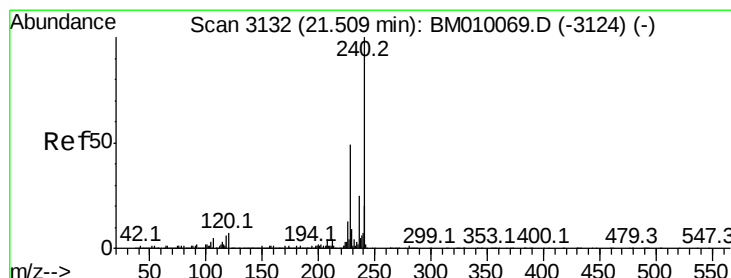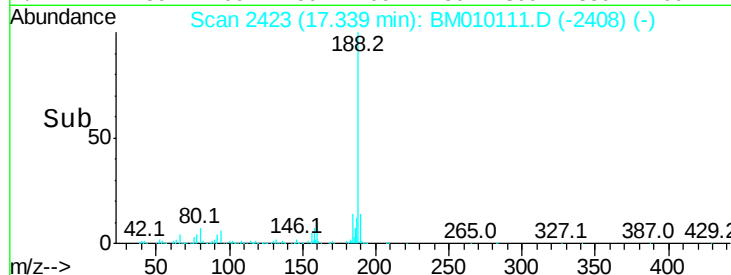
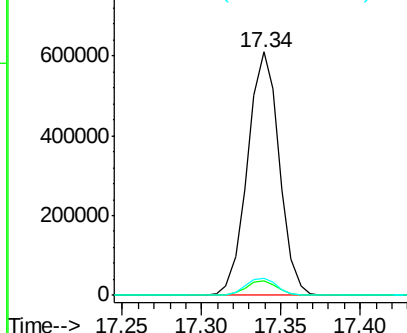



#75
Chrysene-d12
Concen: 20.00 ng
RT: 21.50 min Scan# 3130
Delta R.T. -0.01 min
Lab File: BM010111.D
Acq: 22 May 2017 20:22

Tgt Ion	Ratio	Lower	Upper
240	100		
120	5.8	8.2	12.2#
236	25.5	20.0	30.0

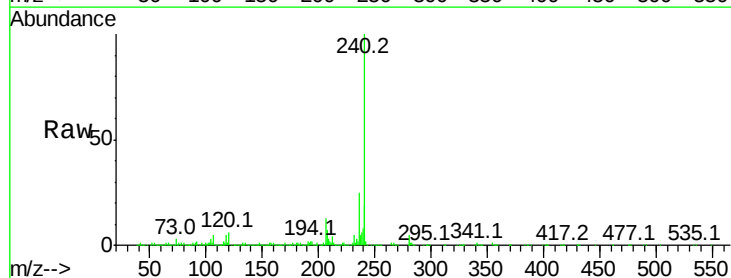

Abundance Ion 240.00 (239.70 to 240.70): E
Ion 120.00 (119.70 to 120.70): E
Ion 236.00 (235.70 to 236.70): E

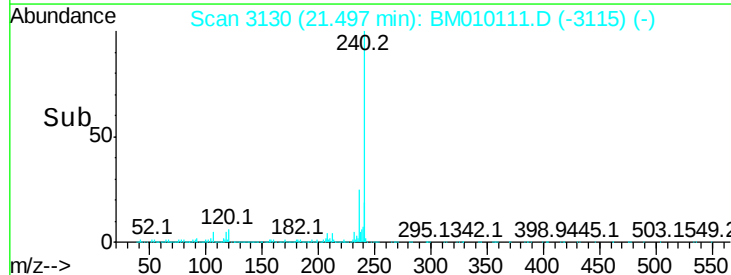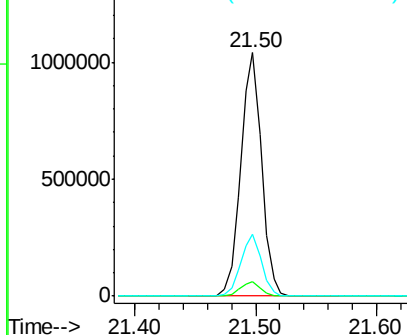

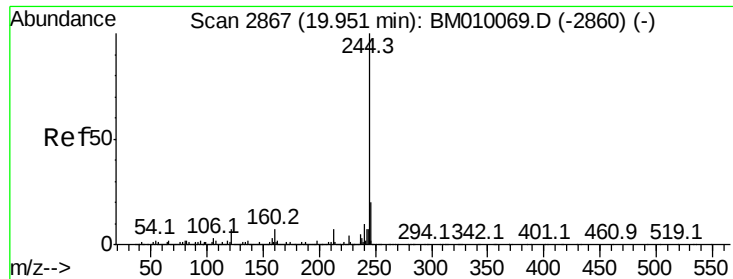

#78

Terphenyl-d14

Concen: 90.21 ng

RT: 19.94 min Scan# 2865

Delta R.T. -0.01 min

Lab File: BM010111.D

Acq: 22 May 2017 20:22

Instrument :

BNA_M

ClientSampled :

EP2-FB01


Tot Ion:244 Resp: 4987784

Ion Ratio Lower Upper

244 100

212 7.3 4.9 7.3#




122 6.8 6.2 9.4

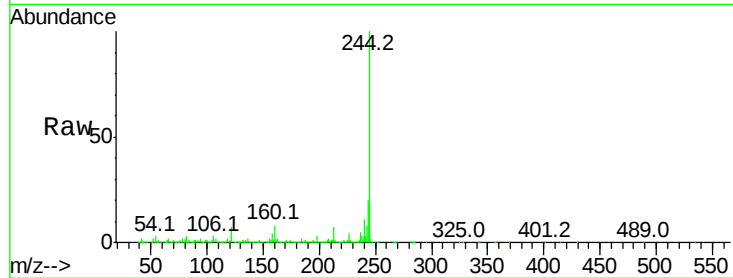

Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

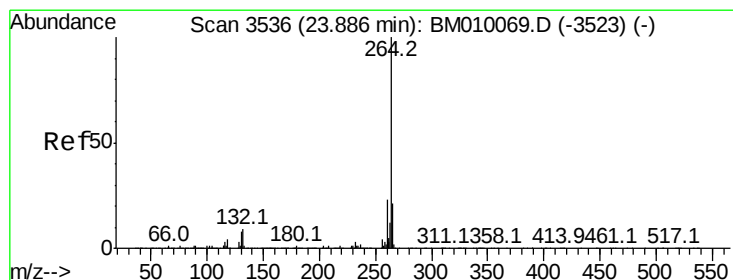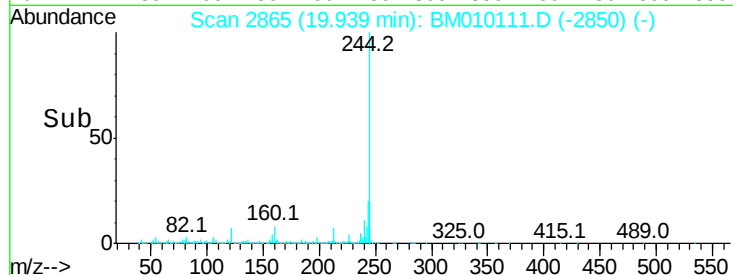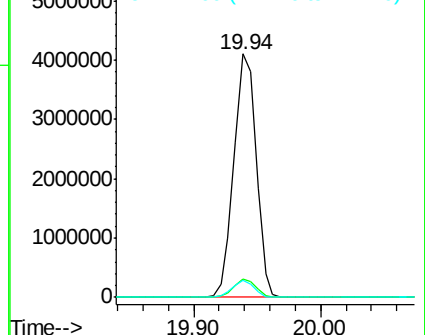

#86

Perylene-d12

Concen: 20.00 ng

RT: 23.86 min Scan# 3532

Delta R.T. -0.02 min

Lab File: BM010111.D

Acq: 22 May 2017 20:22


Tgt Ion:264 Resp: 1284694

Ion Ratio Lower Upper

264 100

260 24.3 18.6 27.8

265 23.5 17.3 25.9

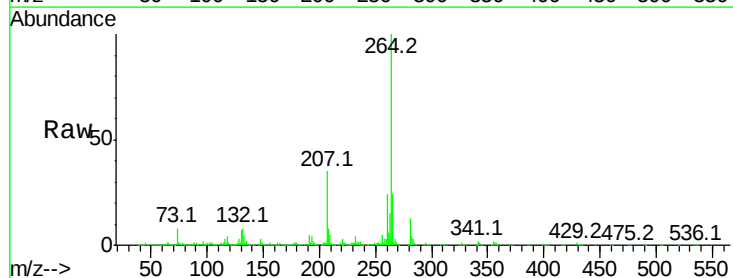

Abundance Ion 264.00 (263.70 to 264.70): E

Ion 260.00 (259.70 to 260.70): E

Ion 265.00 (264.70 to 265.70): E

